

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
 Data File : VX031530.D
 Acq On : 21 Sep 2022 17:27
 Operator : JC/MD
 Sample : N4614-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-10R

Quant Time: Sep 22 01:14:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	85476	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	138801	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	123909	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	57820	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	87454	55.811	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	111.620%
35) Dibromofluoromethane	5.391	113	74031	51.626	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.260%
50) Toluene-d8	8.653	98	279242	50.496	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.000%
62) 4-Bromofluorobenzene	11.079	95	89059	47.545	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.080%
Target Compounds						
					Qvalue	
6) Chloroethane	1.666	64	390	Below Cal	#	43
11) Tert butyl alcohol	2.995	59	20401	33.909	ug/l	97
13) Acrolein	2.197	56	53	Below Cal	#	1
15) Acrylonitrile	3.123	53	476	0.577	ug/l	# 35
16) Acetone	2.386	43	3776	Below Cal		99
18) Methyl Acetate	2.715	43	612	0.261	ug/l	# 52
19) Methyl tert-butyl Ether	3.117	73	38130	7.924	ug/l	97
20) Methylene Chloride	2.794	84	234	Below Cal	#	35
22) Diisopropyl ether	3.764	45	1919	0.408	ug/l	# 82
23) Vinyl Acetate	3.758	43	1162	0.289	ug/l	# 71
25) 2-Butanone	4.581	43	1444	1.193	ug/l	# 87
29) Tetrahydrofuran	5.032	42	731	0.926	ug/l	# 83
31) Cyclohexane	5.477	56	3310	1.424	ug/l	96
36) 1,1-Dichloropropene	5.556	75	6857	3.108	ug/l	# 49
38) Carbon Tetrachloride	5.550	117	8554	3.498	ug/l	# 16
39) Methylcyclohexane	7.379	83	1395	0.514	ug/l	91
40) Benzene	6.038	78	76782	11.665	ug/l	96
41) Methacrylonitrile	5.032	41	506	0.386	ug/l	# 42
52) Toluene	8.720	92	1386	0.323	ug/l	82
59) 2-Hexanone	9.452	43	958	0.490	ug/l	80
67) Ethyl Benzene	10.195	91	23953	3.550	ug/l	99
68) m/p-Xylenes	10.311	106	4974	1.835	ug/l	91
69) o-Xylene	10.647	106	609	0.235	ug/l	89
73) Isopropylbenzene	10.964	105	15682	3.632	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.244	83	20	Below Cal	#	25
76) 1,2,3-Trichloropropane	11.079	75	50339	39.008	ug/l	# 37
78) n-propylbenzene	11.305	91	29662	5.971	ug/l	97
79) 2-Chlorotoluene	11.305	91	29662	10.032	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.451	105	1162	0.317	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	50339	125.600	ug/l	# 11
82) 4-Chlorotoluene	11.305	91	29662	8.548	ug/l	# 44
84) 1,2,4-Trimethylbenzene	11.756	105	16212	4.492	ug/l	96
85) sec-Butylbenzene	11.890	105	2185	0.486	ug/l	97
89) n-Butylbenzene	12.335	91	1808	0.559	ug/l	# 61
90) Hexachloroethane	12.646	117	4156	6.373	ug/l	# 15
95) Naphthalene	13.780	128	28668	6.916	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031530.D
Acq On : 21 Sep 2022 17:27
Operator : JC/MD
Sample : N4614-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10R

Quant Time: Sep 22 01:14:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031530.D
Acq On : 21 Sep 2022 17:27
Operator : JC/MD
Sample : N4614-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-10R

Quant Time: Sep 22 01:14:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration




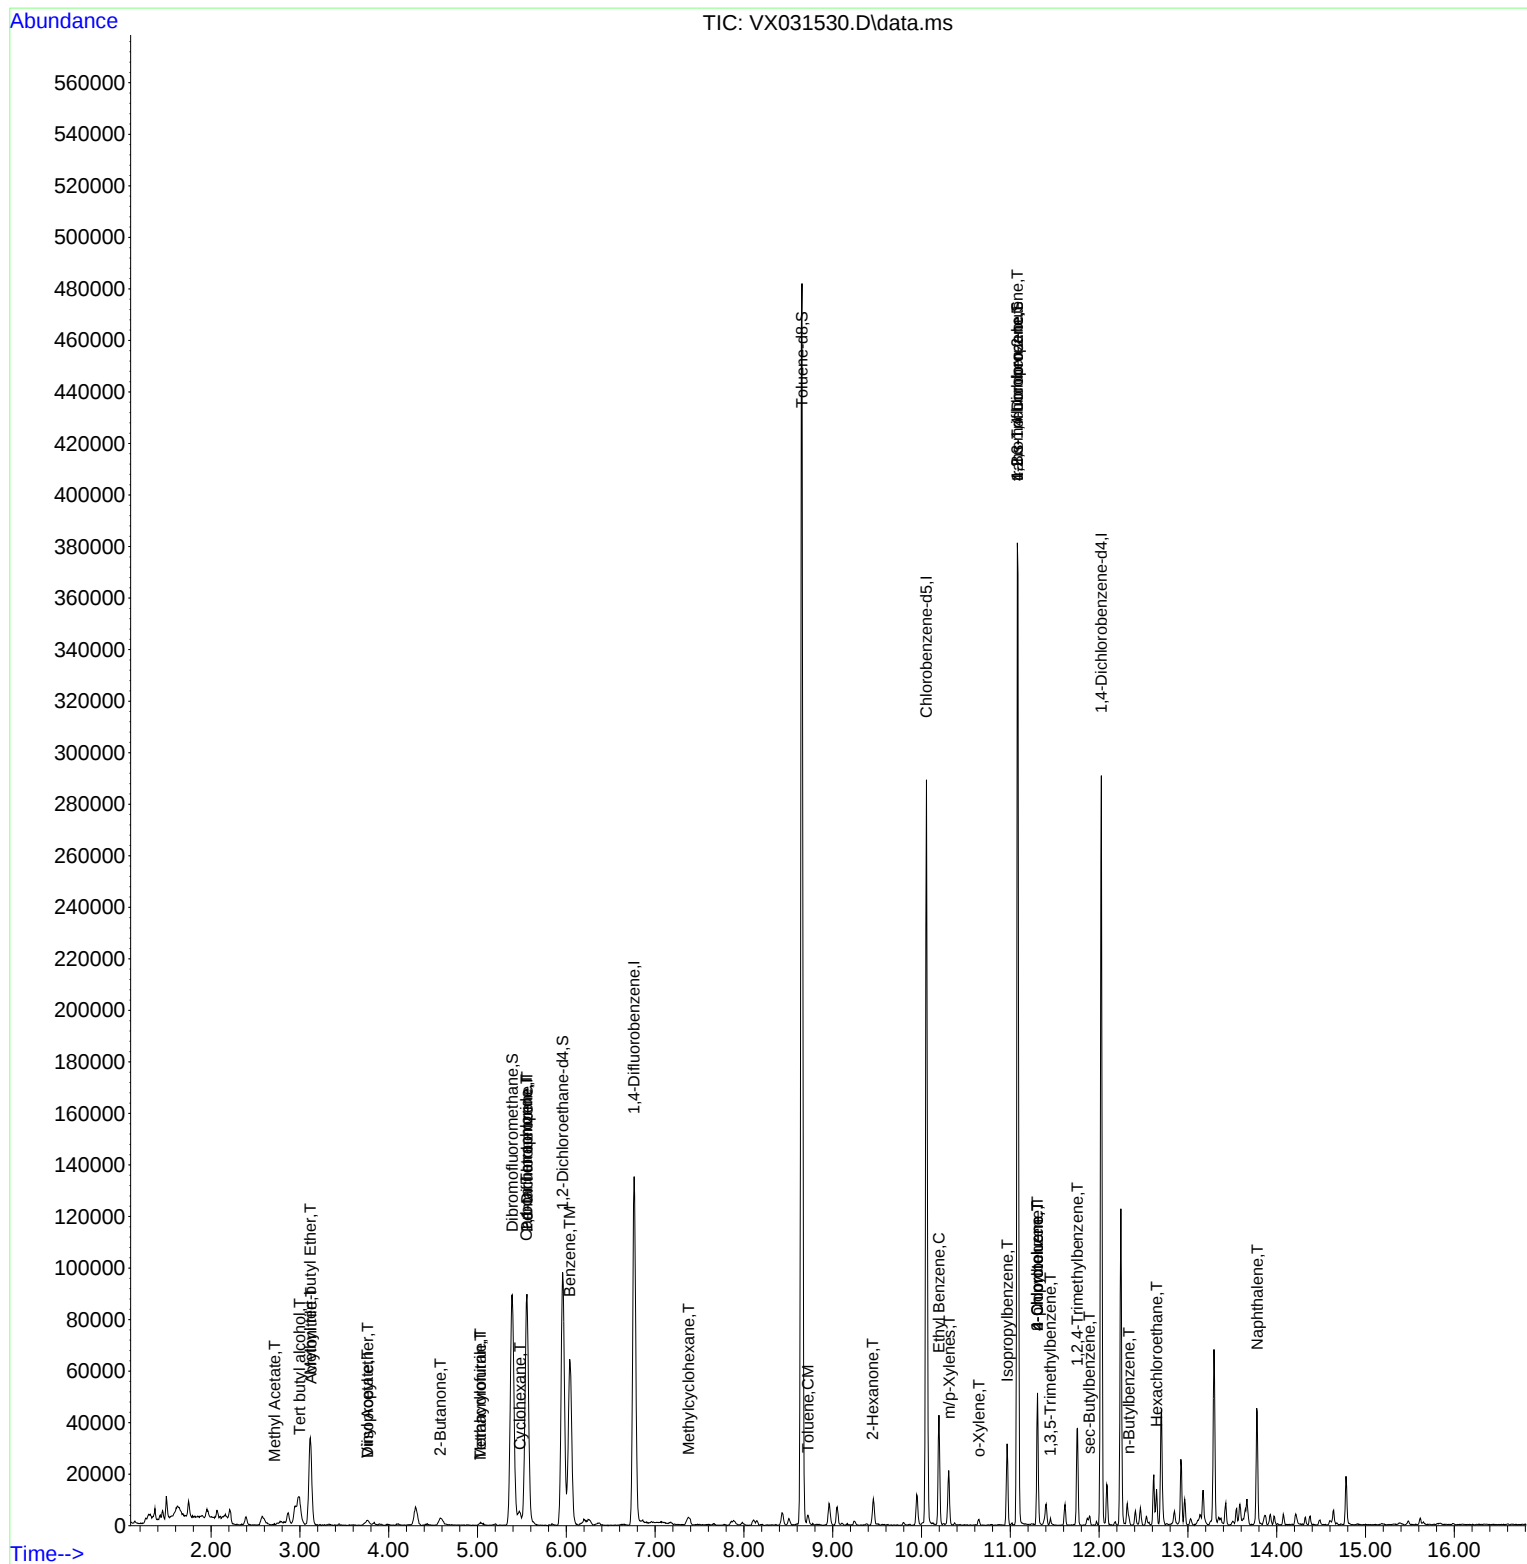




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:168 Resp: 85476
Ion Ratio Lower Upper
168 100
99 55.4 48.8 73.2



#6
Chloroethane
Concen: Below Cal
RT: 1.666 min Scan# 95
Delta R.T. -0.019 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 64 Resp: 390
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

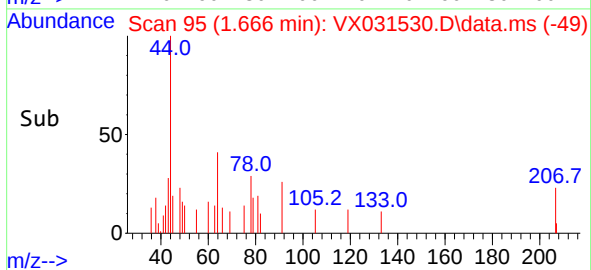



#11

Tert butyl alcohol

Concen: 33.909 ug/l

RT: 2.995 min Scan# 31

Delta R.T. 0.006 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27

Instrument :

MSVOA_X

ClientSampleId :





MW-10R

Tgt Ion: 59 Resp: 20401

Ion Ratio Lower Upper

59 100

57 9.1 8.2 12.2

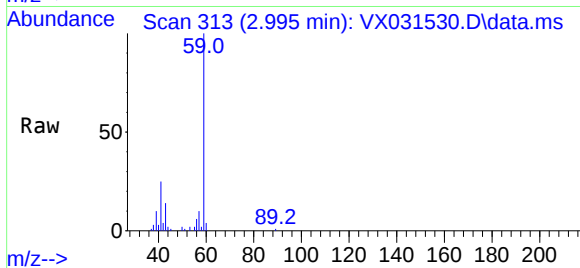

#13

Acrolein

Concen: Below Cal

RT: 2.197 min Scan# 182

Delta R.T. -0.042 min

Lab File: VX031530.D




Acq: 21 Sep 2022 17:27


Tgt Ion: 56 Resp: 53

Ion Ratio Lower Upper

56 100

55 3205.7 56.0 84.0#



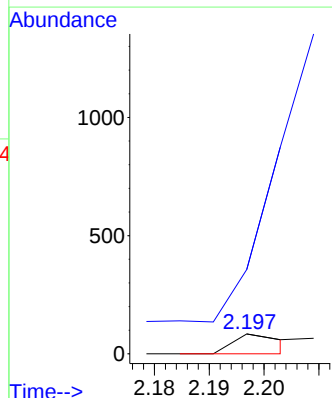
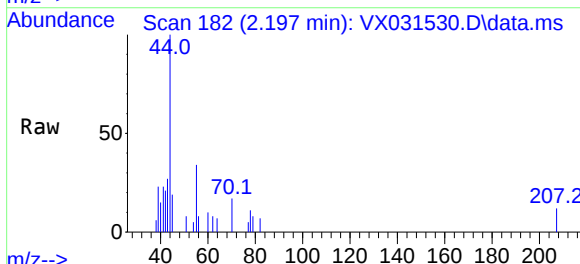




#15
Acrylonitrile
Concen: 0.577 ug/l
RT: 3.123 min Scan# 31
Delta R.T. 0.054 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 53 Resp: 476
Ion Ratio Lower Upper
53 100
52 0.0 66.9 100.3#
51 35.3 30.0 45.0



#16
Acetone
Concen: Below Cal
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 43 Resp: 3776
Ion Ratio Lower Upper
43 100
58 29.5 23.8 35.8


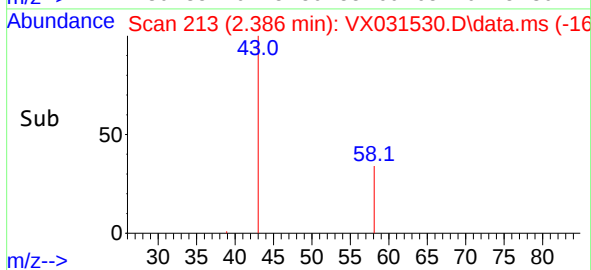






#18
Methyl Acetate
Concen: 0.261 ug/l
RT: 2.715 min Scan# 2
Delta R.T. 0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 43 Resp: 612
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#



#19
Methyl tert-butyl Ether
Concen: 7.924 ug/l
RT: 3.117 min Scan# 333
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 73 Resp: 38130
Ion Ratio Lower Upper
73 100
57 23.1 17.2 25.8

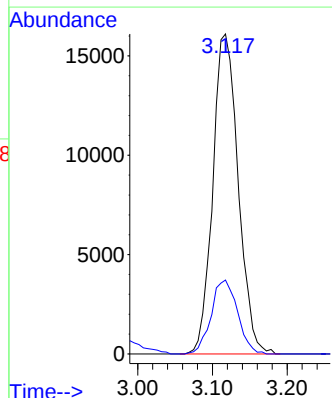



#20

Methylene Chloride

Concen: Below Cal

RT: 2.794 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27

Instrument :

MSVOA_X

ClientSampleId :

MW-10R

Tgt Ion: 84 Resp: 234





Ion Ratio Lower Upper

84 100

49 64.9 105.9 158.9#

51 0.0 32.2 48.2#

86 0.0 50.8 76.2#

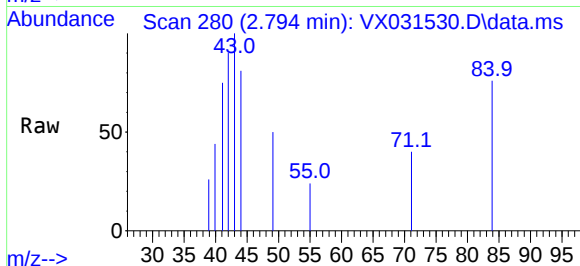

#22

Diisopropyl ether

Concen: 0.408 ug/l

RT: 3.764 min Scan# 439

Delta R.T. -0.000 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27

Tgt Ion: 45 Resp: 1919




Ion Ratio Lower Upper


45 100

43 51.5 59.0 88.6#

87 28.5 22.6 33.8

59 12.4 8.8 13.2

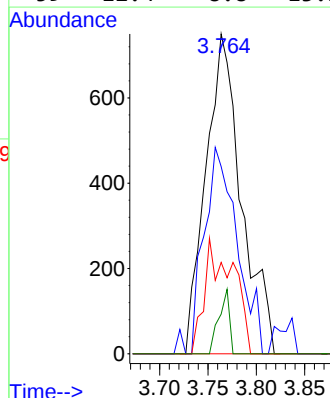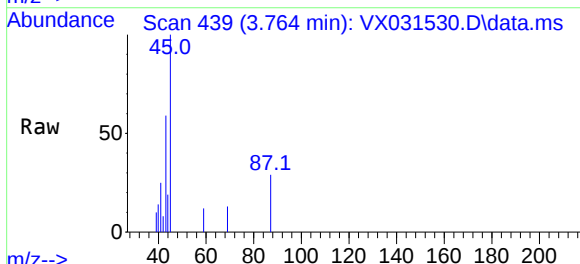



#23

Vinyl Acetate

Concen: 0.289 ug/l

RT: 3.758 min Scan# 41

Delta R.T. 0.031 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27

Instrument :

MSVOA_X

ClientSampleId :





MW-10R

Tgt Ion: 43 Resp: 1162

Ion Ratio Lower Upper

43 100

86 0.0 8.7 13.1#

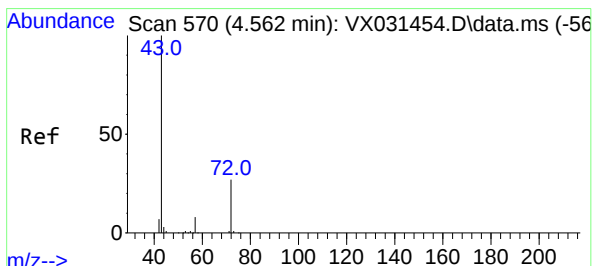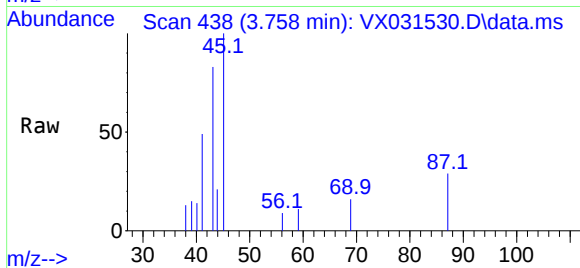

#25

2-Butanone

Concen: 1.193 ug/l

RT: 4.581 min Scan# 573

Delta R.T. 0.019 min

Lab File: VX031530.D




Acq: 21 Sep 2022 17:27


Tgt Ion: 43 Resp: 1444

Ion Ratio Lower Upper

43 100

72 19.7 21.1 31.7#


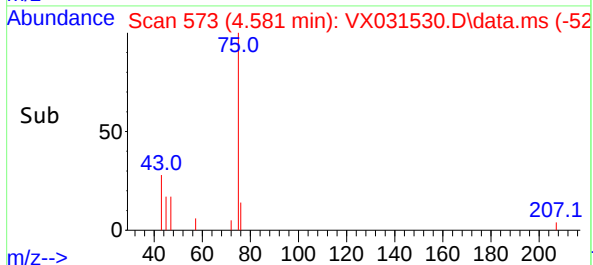
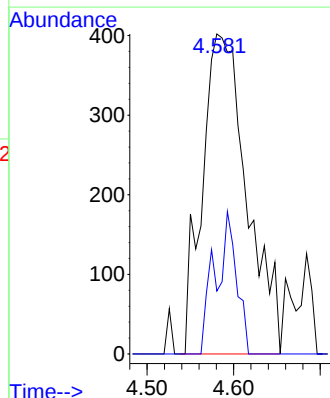
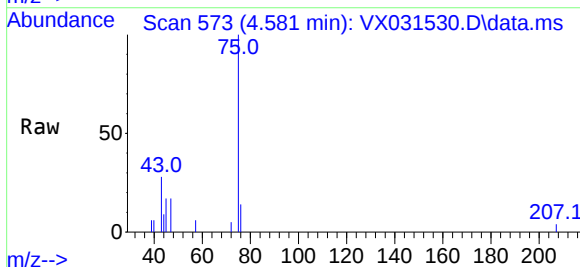




#29
Tetrahydrofuran
Concen: 0.926 ug/l
RT: 5.032 min Scan# 644
Delta R.T. 0.019 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 42 Resp: 731
Ion Ratio Lower Upper
42 100
72 27.9 36.4 54.6#
71 37.9 33.5 50.3

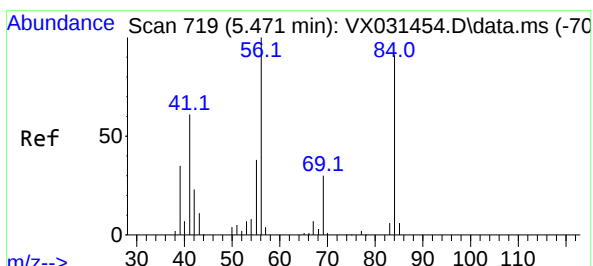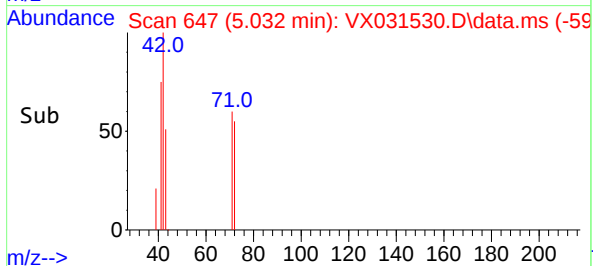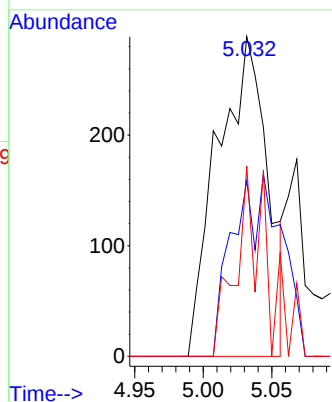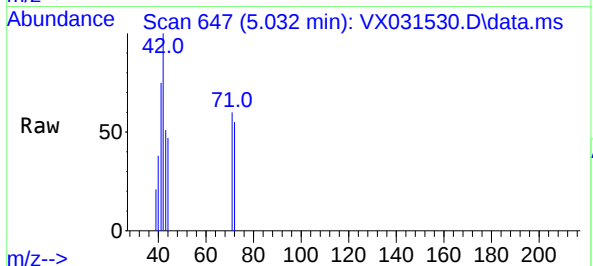

#31
Cyclohexane
Concen: 1.424 ug/l
RT: 5.477 min Scan# 720
Delta R.T. 0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 56 Resp: 3310
Ion Ratio Lower Upper
56 100
69 26.6 25.1 37.7
84 89.9 70.2 105.4


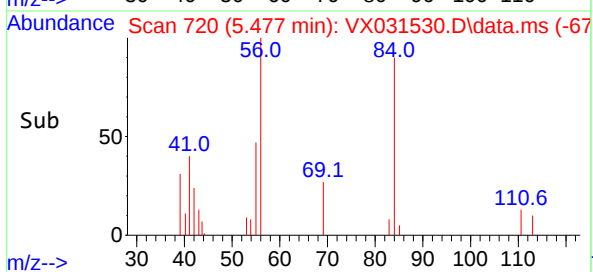
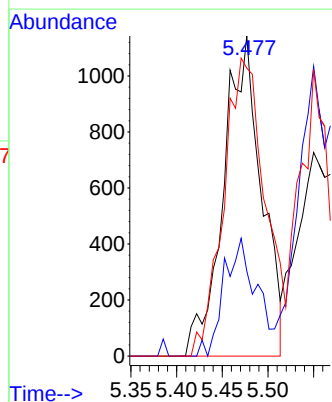





#33
1,2-Dichloroethane-d4
Concen: 55.811 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 65 Resp: 87454
Ion Ratio Lower Upper
65 100
67 51.4 0.0 102.4

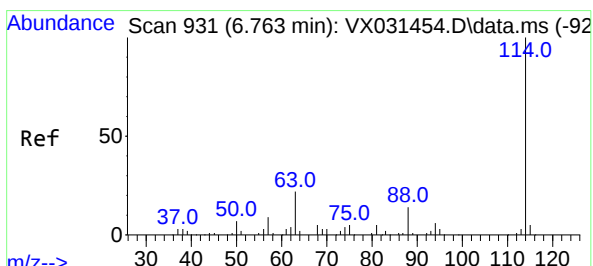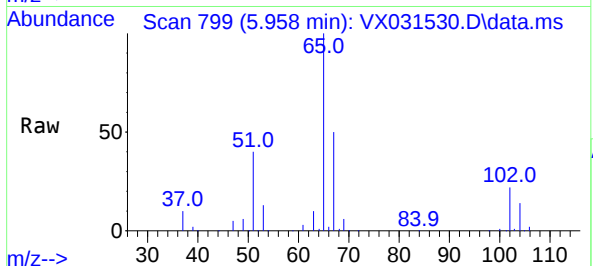

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 114 Resp: 138801
Ion Ratio Lower Upper
114 100
63 19.7 0.0 42.6
88 15.6 0.0 33.0


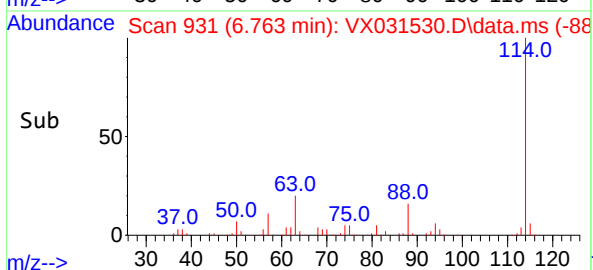




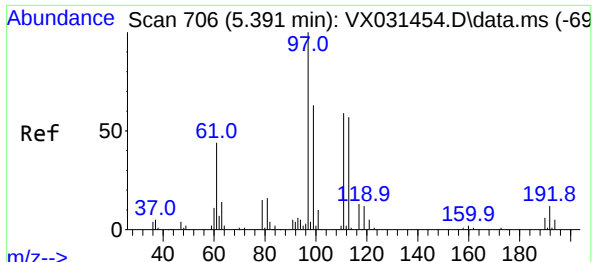

#35
Dibromofluoromethane
Concen: 51.626 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:	113	Resp:	74031
Ion	Ratio	Lower	Upper
113	100		
111	104.3	82.4	123.6
192	19.6	14.1	21.1

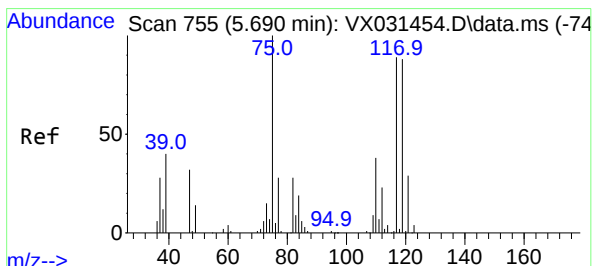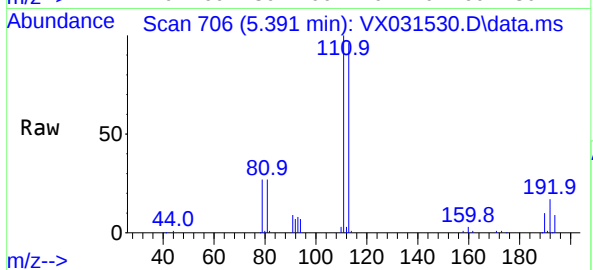

#36
1,1-Dichloropropene
Concen: 3.108 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion:	75	Resp:	6857
Ion	Ratio	Lower	Upper
75	100		
110	8.8	17.5	52.5#
77	0.0	24.9	37.3#


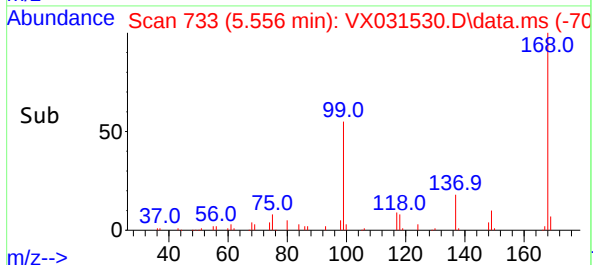
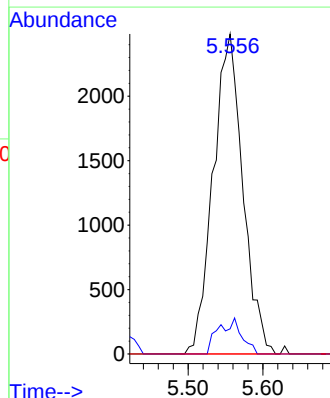
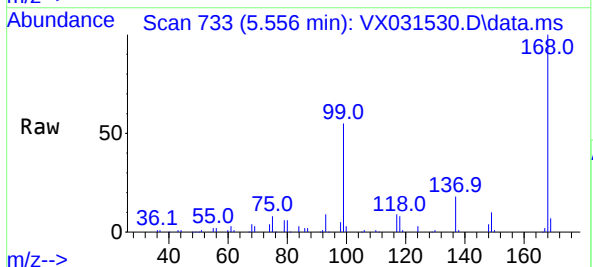




#38
Carbon Tetrachloride
Concen: 3.498 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:117 Resp: 8554
Ion Ratio Lower Upper
117 100
119 3.6 74.6 112.0#
121 0.0 25.3 37.9#



#39
Methylcyclohexane
Concen: 0.514 ug/l
RT: 7.379 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 83 Resp: 1395
Ion Ratio Lower Upper
83 100
55 86.0 61.0 91.4
98 50.0 37.7 56.5


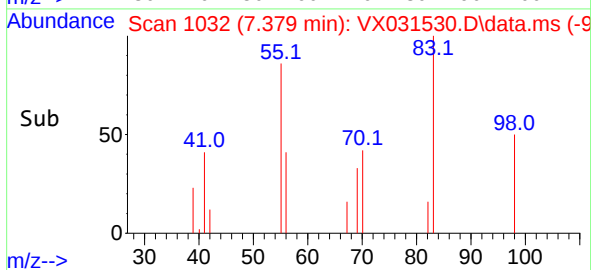






#40
Benzene
Concen: 11.665 ug/l
RT: 6.038 min Scan# 813
Delta R.T. -0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 78 Resp: 76782
Ion Ratio Lower Upper
78 100
77 25.3 18.7 28.1



#41
Methacrylonitrile
Concen: 0.386 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.104 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 41 Resp: 506
Ion Ratio Lower Upper
41 100
39 40.7 45.0 67.6#
67 0.0 58.2 87.4#
52 0.0 25.0 37.6#



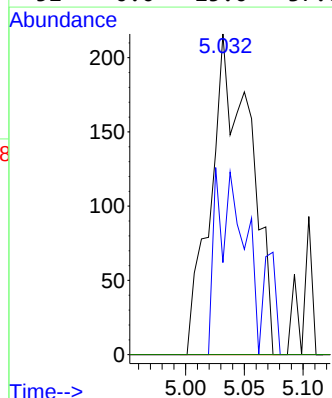



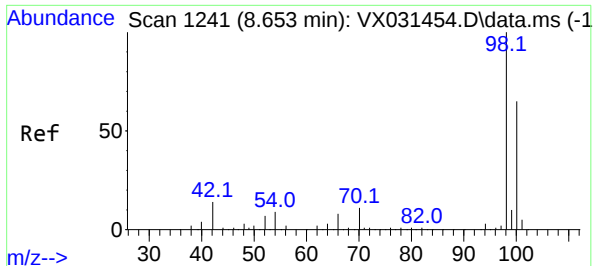

#50
Toluene-d8
Concen: 50.496 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 98 Resp: 279242
Ion Ratio Lower Upper
98 100
100 65.3 52.5 78.7

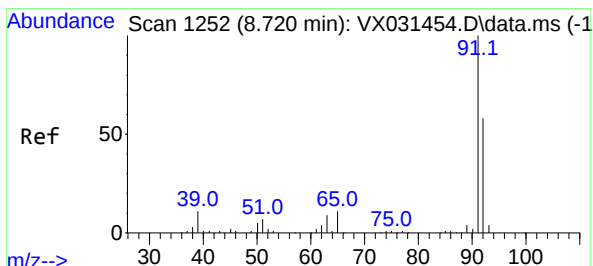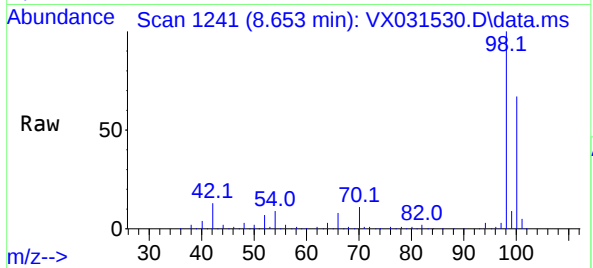

#52
Toluene
Concen: 0.323 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 92 Resp: 1386
Ion Ratio Lower Upper
92 100
91 195.7 137.1 205.7

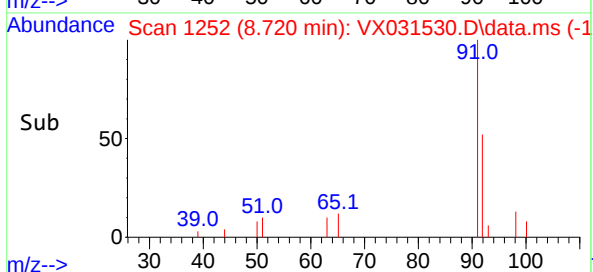



#59

2-Hexanone

Concen: 0.490 ug/l

RT: 9.452 min Scan# 11

Delta R.T. 0.019 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27

Instrument :

MSVOA_X

ClientSampleId :





MW-10R

Tgt Ion: 43 Resp: 958

Ion Ratio Lower Upper

43 100

58 39.2 26.7 80.0

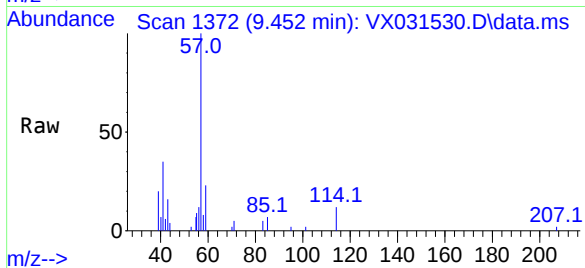

#62

4-Bromofluorobenzene

Concen: 47.545 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX031530.D

Acq: 21 Sep 2022 17:27




Tgt Ion: 95 Resp: 89059


Ion Ratio Lower Upper

95 100

174 89.9 0.0 153.2

176 87.9 0.0 144.0


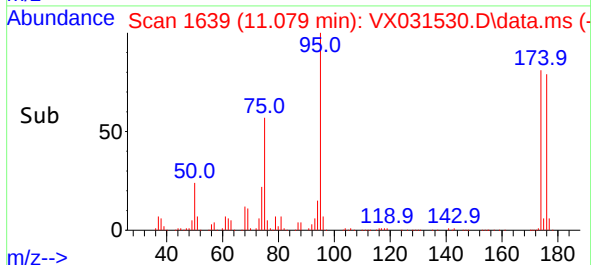
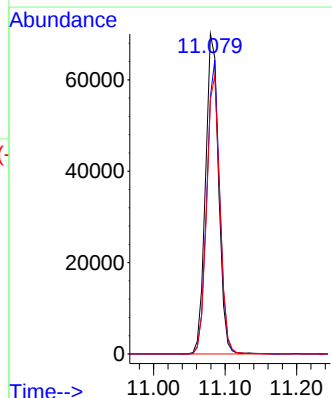
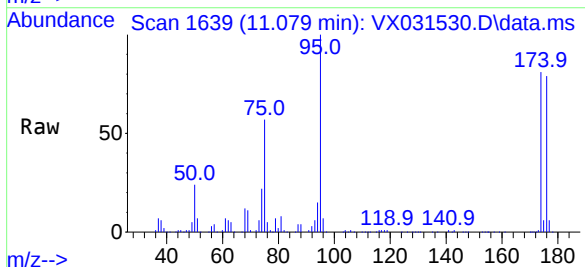




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:117 Resp: 123909
Ion Ratio Lower Upper
117 100
82 51.0 46.8 70.2
119 32.3 26.4 39.6

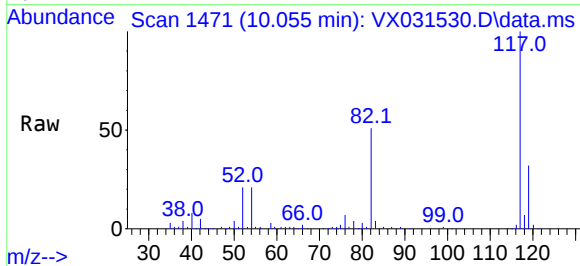

#67
Ethyl Benzene
Concen: 3.550 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 91 Resp: 23953
Ion Ratio Lower Upper
91 100
106 30.8 25.2 37.8



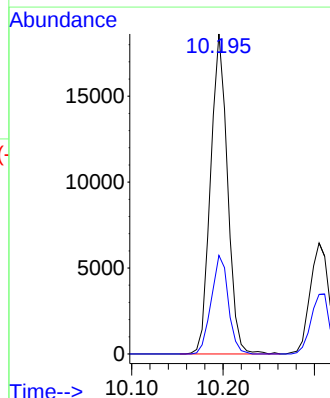
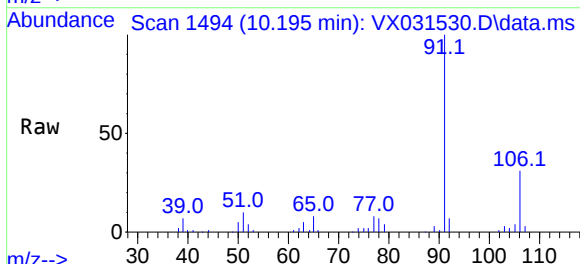




#68
m/p-Xylenes
Concen: 1.835 ug/l
RT: 10.311 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:106 Resp: 4974
Ion Ratio Lower Upper
106 100
91 187.3 161.0 241.4

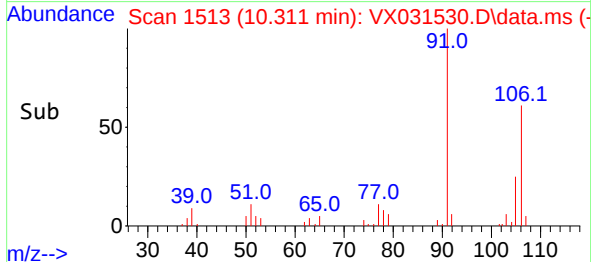

#69
o-Xylene
Concen: 0.235 ug/l
RT: 10.647 min Scan# 1568
Delta R.T. 0.001 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion:106 Resp: 609
Ion Ratio Lower Upper
106 100
91 231.0 107.2 321.6


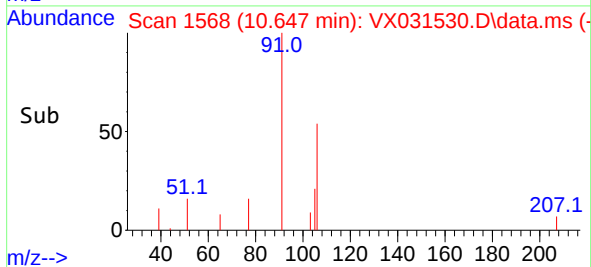

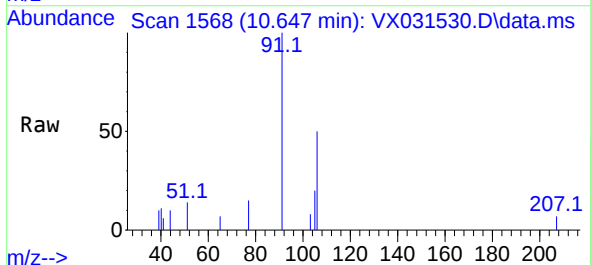




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:152 Resp: 57820
Ion Ratio Lower Upper
152 100
115 56.5 43.4 130.1
150 157.4 0.0 346.8

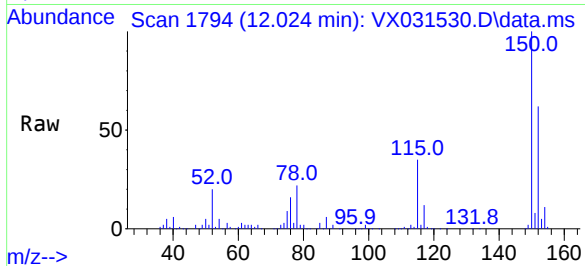

#73
Isopropylbenzene
Concen: 3.632 ug/l
RT: 10.964 min Scan# 1620
Delta R.T. 0.001 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion:105 Resp: 15682
Ion Ratio Lower Upper
105 100
120 26.2 13.7 41.0


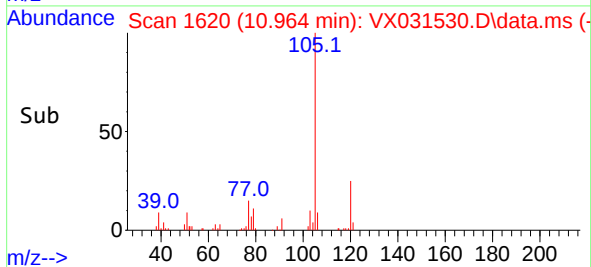

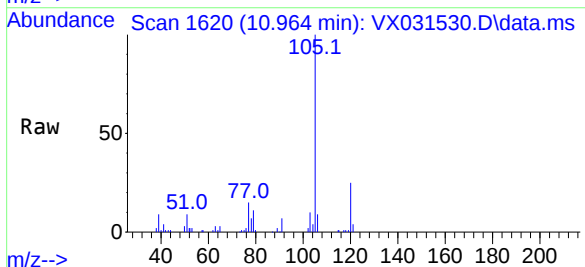




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.244 min Scan# 1666
Delta R.T. 0.031 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 83 Resp: 20
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.4#
85 0.0 32.6 97.8#

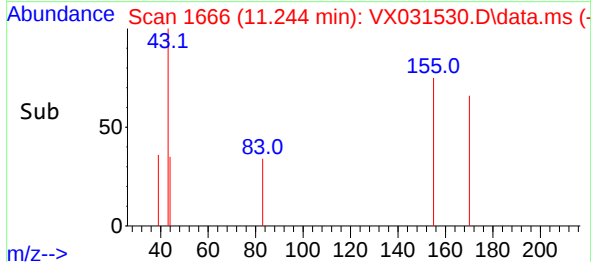

#76
1,2,3-Trichloropropane
Concen: 39.008 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 75 Resp: 50339
Ion Ratio Lower Upper
75 100
77 1.2 20.3 60.9#



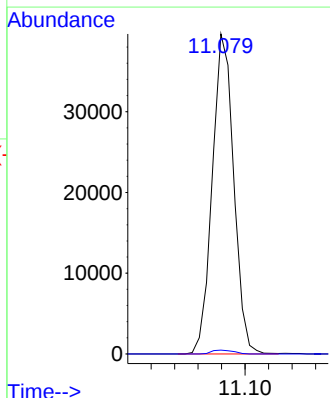





#78
n-propylbenzene
Concen: 5.971 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 91 Resp: 29662
Ion Ratio Lower Upper
91 100
120 22.3 11.8 35.4



#79
2-Chlorotoluene
Concen: 10.032 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 91 Resp: 29662
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#



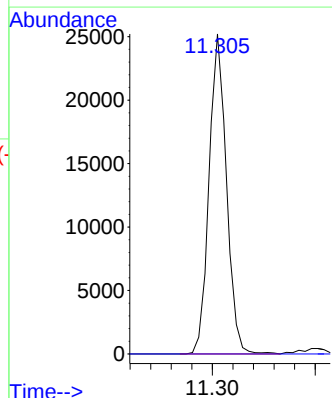





#80
1,3,5-Trimethylbenzene
Concen: 0.317 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion:105 Resp: 1162
Ion Ratio Lower Upper
105 100
120 51.2 24.5 73.5

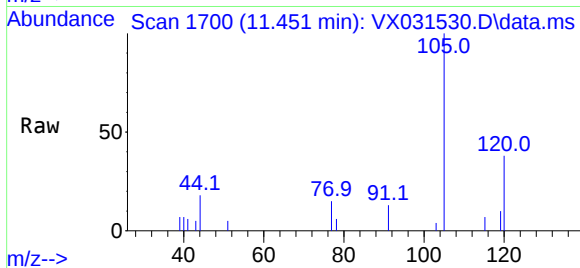

#81
trans-1,4-Dichloro-2-butene
Concen: 125.600 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 75 Resp: 50339
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


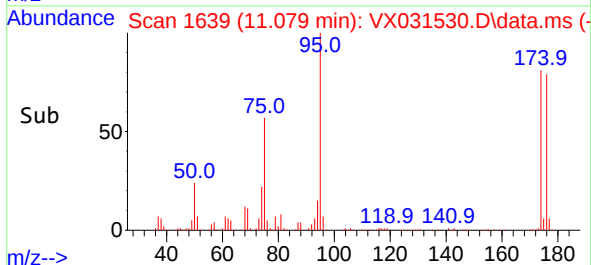
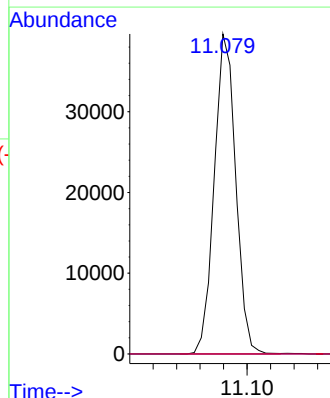
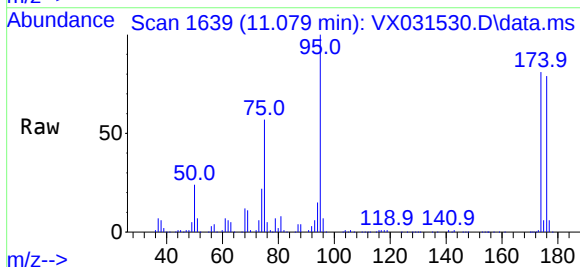




#82
4-Chlorotoluene
Concen: 8.548 ug/l
RT: 11.305 min Scan# 1701
Delta R.T. -0.152 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27




Instrument :
MSVOA_X
ClientSampleId :
MW-10R


Tgt Ion: 91 Resp: 29662
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

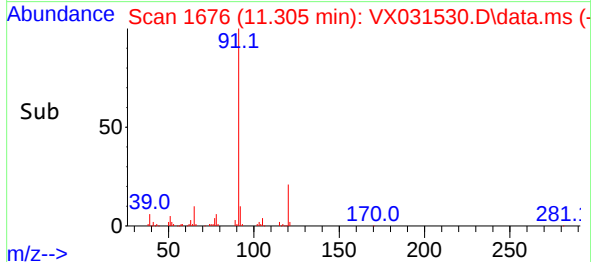

#84
1,2,4-Trimethylbenzene
Concen: 4.492 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.000 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion: 105 Resp: 16212
Ion Ratio Lower Upper
105 100
120 47.8 22.6 67.8


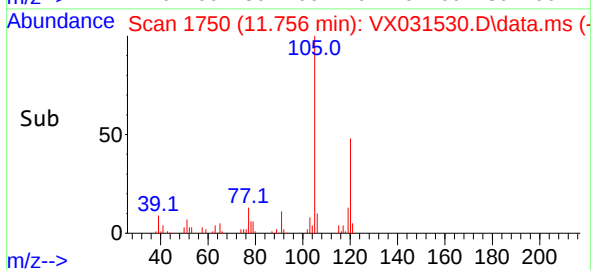






#85
 sec-Butylbenzene
 Concen: 0.486 ug/l
 RT: 11.890 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX031530.D
 Acq: 21 Sep 2022 17:27




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-10R


Tgt Ion:105 Resp: 2185
 Ion Ratio Lower Upper
 105 100
 134 19.1 10.4 31.1

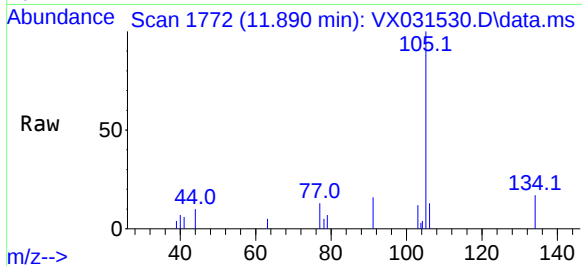

#89
 n-Butylbenzene
 Concen: 0.559 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX031530.D
 Acq: 21 Sep 2022 17:27

Tgt Ion: 91 Resp: 1808
 Ion Ratio Lower Upper
 91 100
 92 45.5 27.0 81.0
 134 75.5 13.3 39.9#


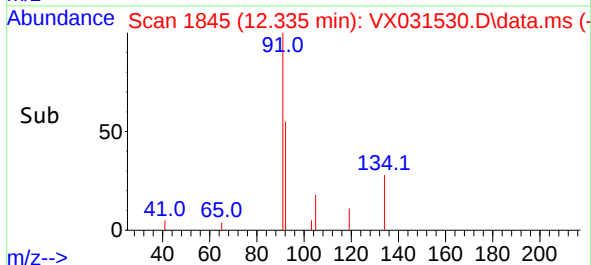
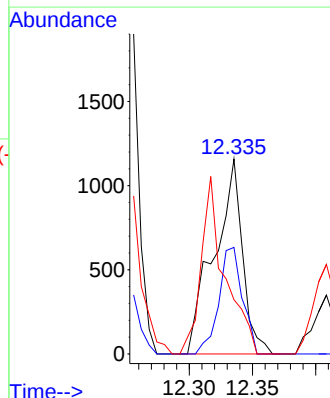
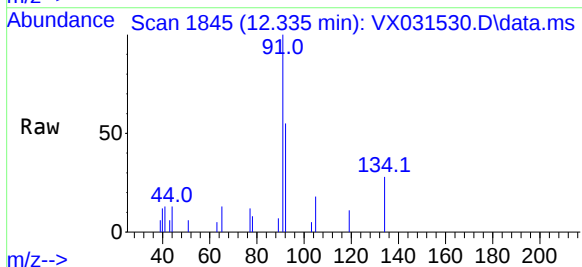




#90
Hexachloroethane
Concen: 6.373 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.104 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Instrument :
MSVOA_X
ClientSampleId :
MW-10R

Tgt Ion:117 Resp: 4156
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

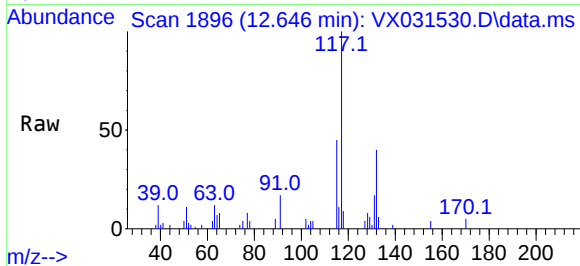

#95
Naphthalene
Concen: 6.916 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX031530.D
Acq: 21 Sep 2022 17:27

Tgt Ion:128 Resp: 28668
Ion Ratio Lower Upper
128 100
127 12.8 10.4 15.6
129 11.6 8.8 13.2

