

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
 Data File : VX031512.D
 Acq On : 21 Sep 2022 10:00
 Operator : JC/MD
 Sample : VX0921WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0921WBL01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Title : SW846 8260

Signal : TIC: VX031512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.624	83	88	91	rBV3	2690	5338	1.25%	0.269%
2	1.672	94	96	105	rVB7	2118	4636	1.09%	0.234%
3	2.940	298	304	312	rBV2	2553	5255	1.23%	0.265%
4	5.391	693	706	718	rBV	51613	150670	35.35%	7.590%
5	5.556	722	733	746	rVB	54341	152560	35.79%	7.685%
6	5.958	789	799	813	rBV2	58334	154026	36.13%	7.759%
7	6.763	921	931	947	rBV	79777	190313	44.65%	9.587%
8	8.647	1234	1240	1253	rBV	266668	426258	100.00%	21.472%
9	10.055	1465	1471	1484	rBV	202543	268737	63.05%	13.537%
10	11.079	1634	1639	1652	rVB	221711	279763	65.63%	14.092%
11	12.024	1788	1794	1802	rBV	276919	347653	81.56%	17.512%




Sum of corrected areas: 1985209

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031512.D
Acq On : 21 Sep 2022 10:00
Operator : JC/MD
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

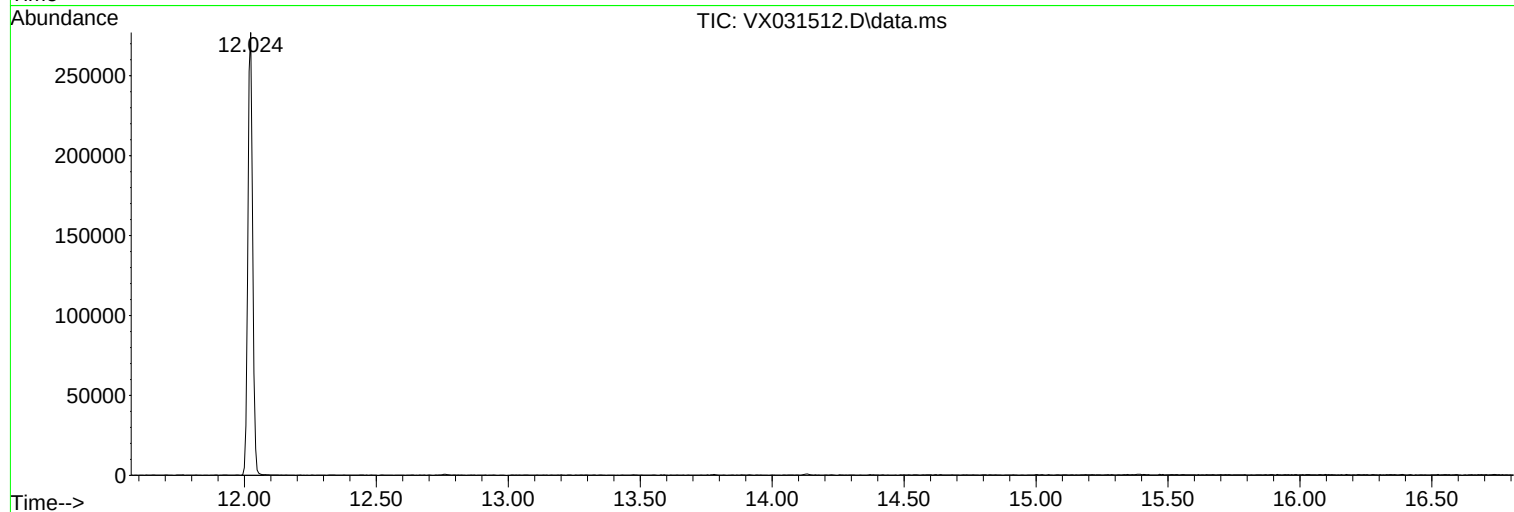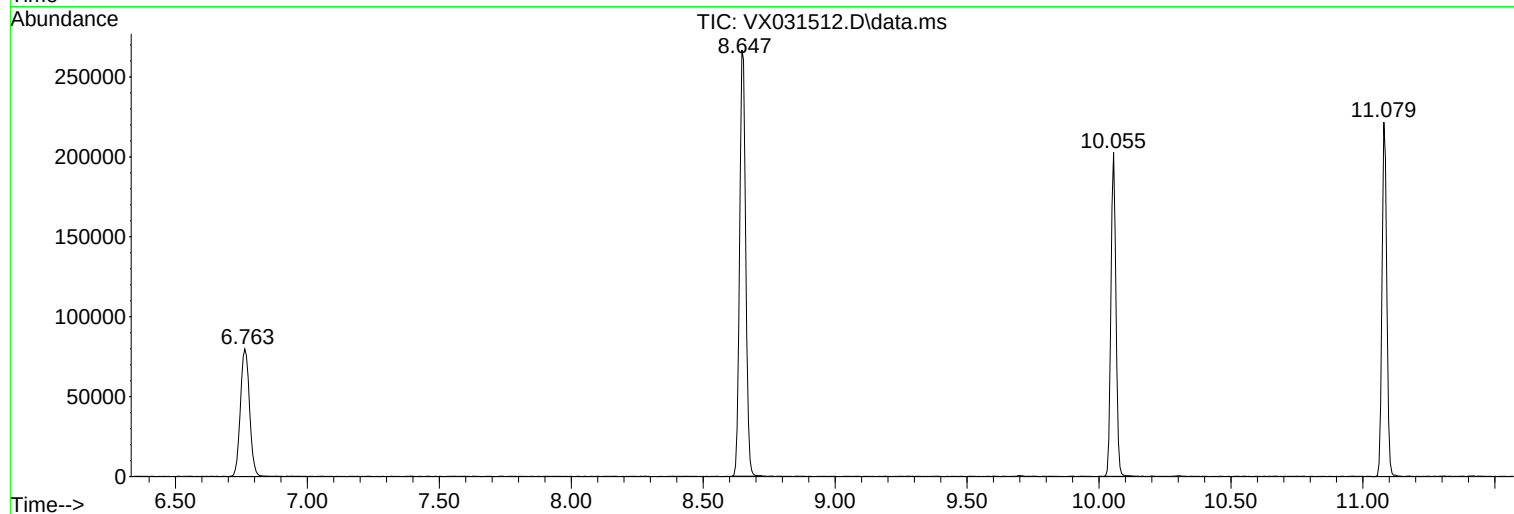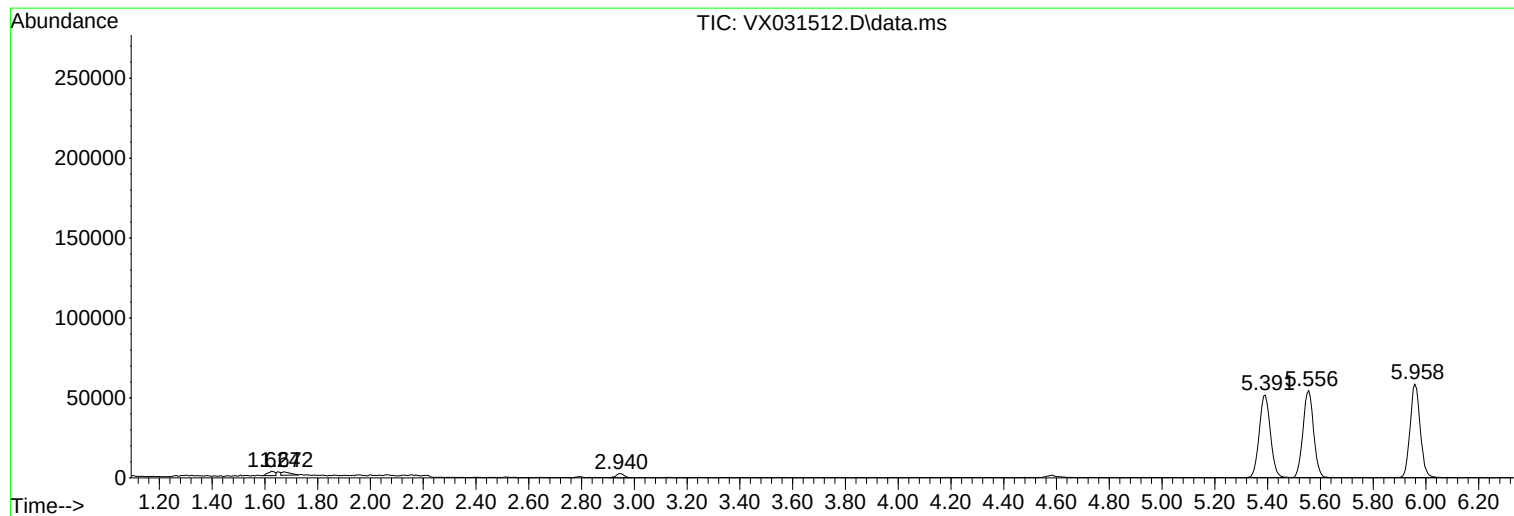

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031512.D
Acq On : 21 Sep 2022 10:00
Operator : JC/MD
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031512.D
Acq On : 21 Sep 2022 10:00
Operator : JC/MD
Sample : VX0921WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0921WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc