

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
 Data File : VX031527.D
 Acq On : 21 Sep 2022 16:16
 Operator : JC/MD
 Sample : N4509-16RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 S1-SO_UNK-20220902RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Title : SW846 8260

Signal : TIC: VX031527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	41	rBV2	9169	29926	3.03%	0.509%
2	1.605	72	85	96	rBV10	6314	25876	2.62%	0.440%
3	2.386	207	213	222	rBV2	8931	15570	1.58%	0.265%
4	2.788	273	279	288	rBV	9129	16347	1.66%	0.278%
5	2.947	297	305	314	rBV	5829	13895	1.41%	0.237%
6	4.721	587	596	608	rBV2	6345	19163	1.94%	0.326%
7	5.385	695	705	719	rBV	74728	213362	21.63%	3.632%
8	5.556	721	733	745	rVV	83496	233013	23.62%	3.966%
9	5.958	789	799	811	rBV	86582	224421	22.75%	3.820%
10	6.342	851	862	875	rBV2	37443	98976	10.03%	1.685%
11	6.763	920	931	941	rBV	136119	356673	36.16%	6.071%
12	7.641	1069	1075	1081	rBV	22059	41622	4.22%	0.708%
13	7.696	1081	1084	1092	rVB	7905	12590	1.28%	0.214%
14	7.799	1094	1101	1117	rBV	587188	986382	100.00%	16.789%
15	8.549	1215	1224	1234	rBV	113902	177400	17.98%	3.020%
16	8.653	1234	1241	1250	rBV	337023	541065	54.85%	9.210%
17	8.958	1285	1291	1306	rBV	153197	223162	22.62%	3.798%
18	9.244	1332	1338	1344	rBV	127952	183333	18.59%	3.121%
19	9.311	1344	1349	1352	rVV	15430	23766	2.41%	0.405%
20	9.348	1352	1355	1357	rVV	23377	33304	3.38%	0.567%
21	9.378	1357	1360	1369	rVV	63966	87570	8.88%	1.491%
22	9.482	1372	1377	1388	rVV	270264	353373	35.83%	6.015%
23	9.580	1388	1393	1406	rVB	193402	246483	24.99%	4.195%
24	9.915	1442	1448	1461	rBV	462583	563704	57.15%	9.595%
25	10.055	1461	1471	1478	rBV	304315	410987	41.67%	6.995%
26	10.640	1560	1567	1576	rBV	35039	45664	4.63%	0.777%
27	11.079	1634	1639	1648	rBV	268067	342978	34.77%	5.838%
28	12.024	1789	1794	1802	rVB	284968	354468	35.94%	6.033%




Sum of corrected areas: 5875073

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031527.D
Acq On : 21 Sep 2022 16:16
Operator : JC/MD
Sample : N4509-16RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S1-SO_UNK-20220902RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

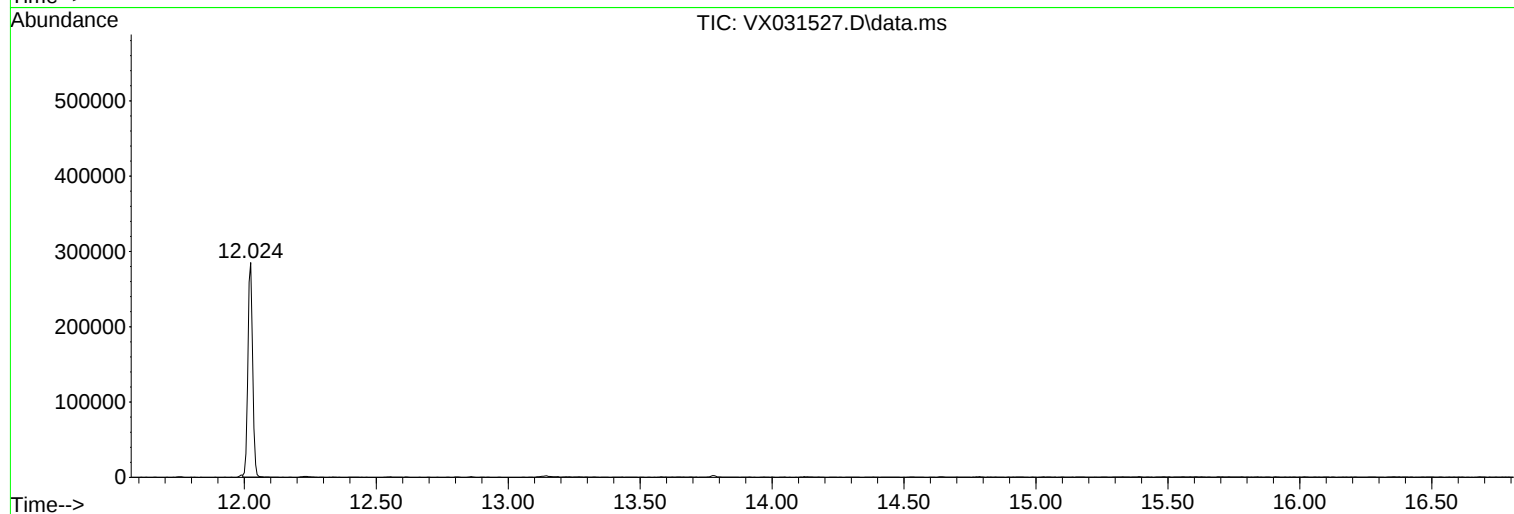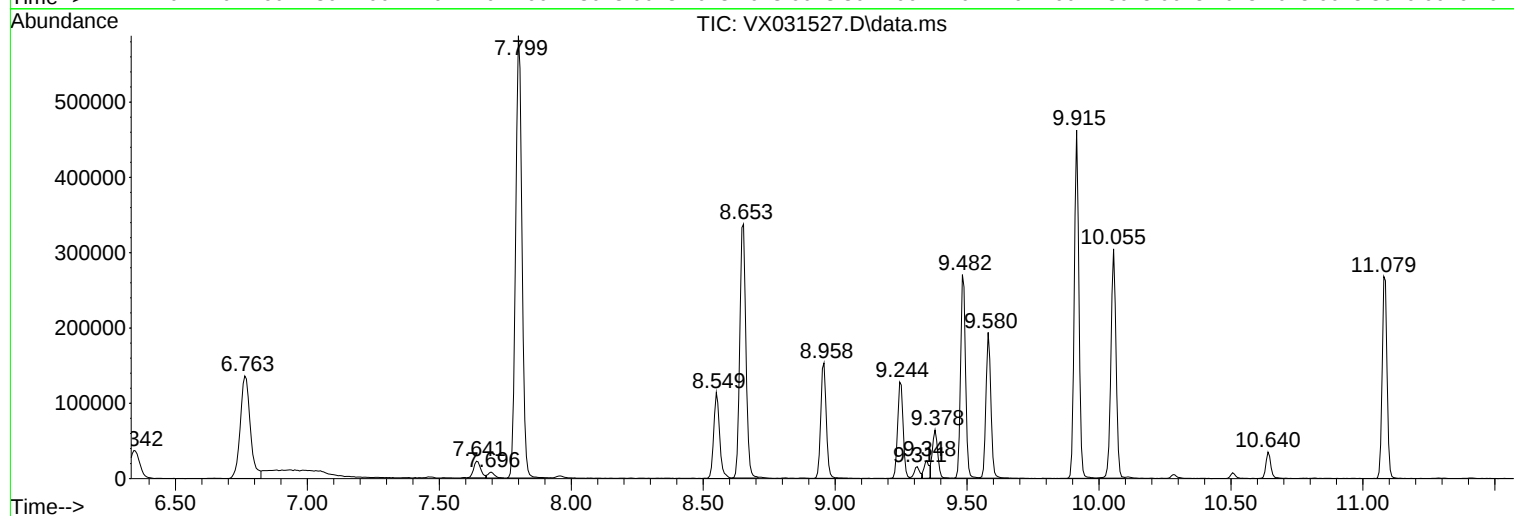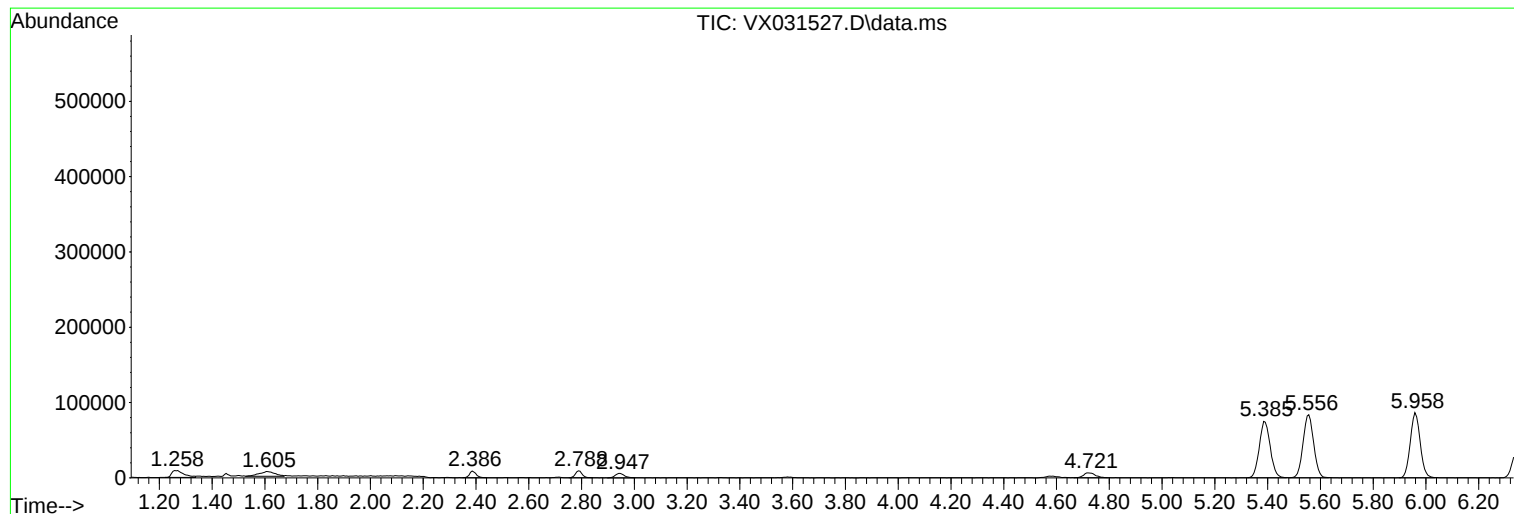

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031527.D
Acq On : 21 Sep 2022 16:16
Operator : JC/MD
Sample : N4509-16RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S1-SO_UNK-20220902RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031527.D
Acq On : 21 Sep 2022 16:16
Operator : JC/MD
Sample : N4509-16RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
S1-SO_UNK-20220902RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------