

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031546.D
Acq On : 22 Sep 2022 03:46
Operator : JC/MD
Sample : N4614-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-44

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M

Title : SW846 8260

Signal : TIC: VX031546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	722	rBV	79296	230049	33.97%	8.492%
2	5.556	722	733	743	rBV	75724	210896	31.14%	7.785%
3	5.958	789	799	814	rBV	87880	232945	34.40%	8.599%
4	6.763	922	931	945	rBV	116658	277406	40.97%	10.240%
5	8.653	1234	1241	1251	rBV	425418	677174	100.00%	24.998%
6	10.055	1465	1471	1483	rBV	252985	337419	49.83%	12.456%
7	11.079	1634	1639	1648	rBV	343849	437795	64.65%	16.161%
8	12.024	1788	1794	1803	rBV	242838	305274	45.08%	11.269%




Sum of corrected areas: 2708958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031546.D
Acq On : 22 Sep 2022 03:46
Operator : JC/MD
Sample : N4614-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

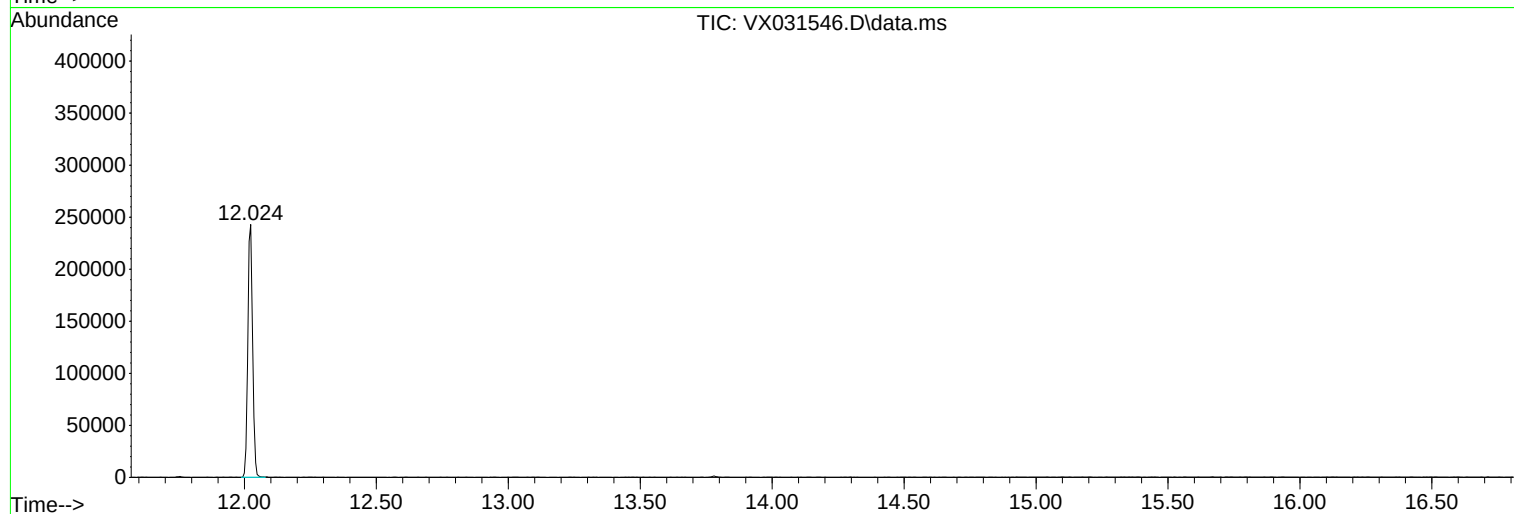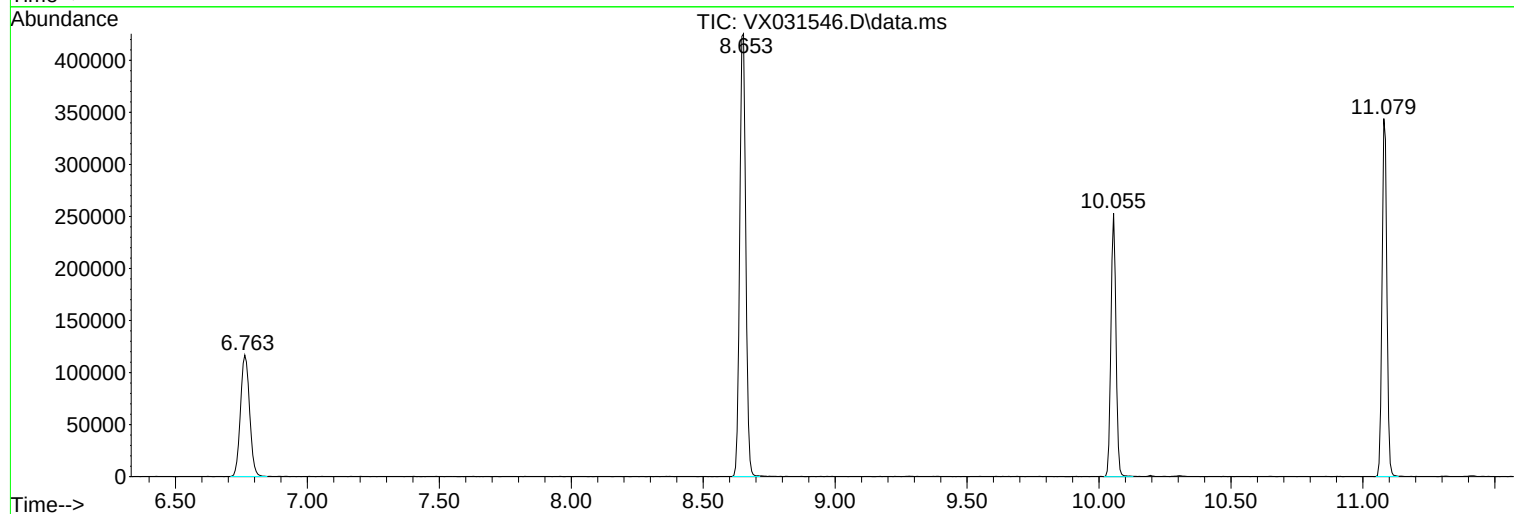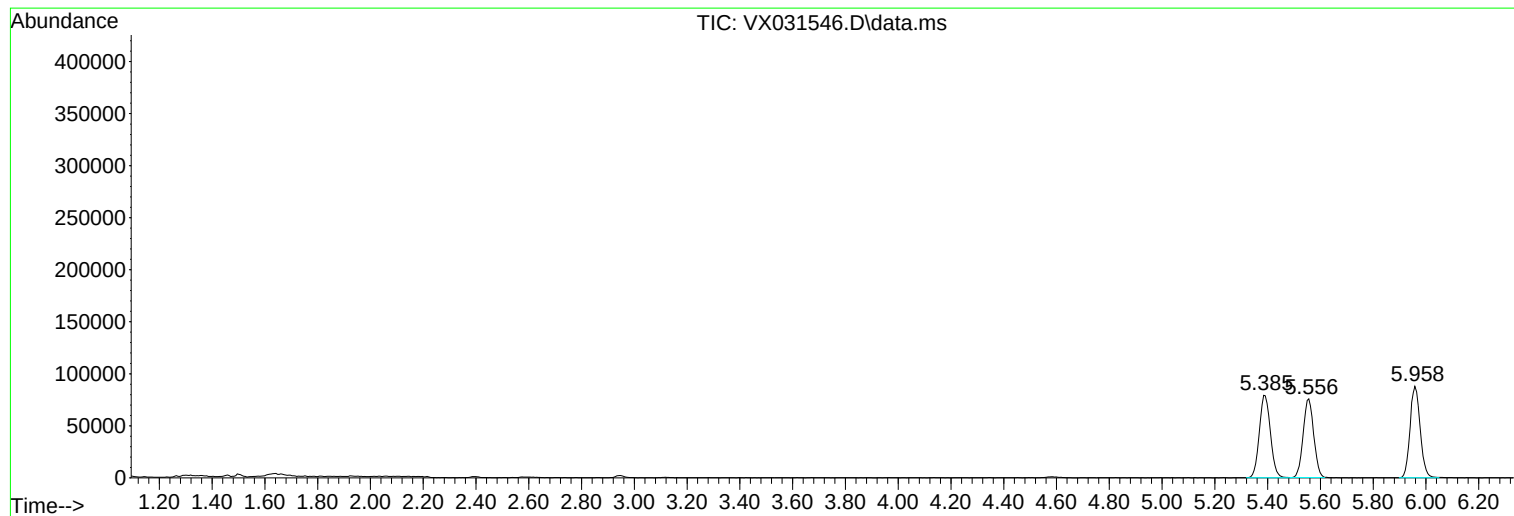

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031546.D
Acq On : 22 Sep 2022 03:46
Operator : JC/MD
Sample : N4614-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031546.D
Acq On : 22 Sep 2022 03:46
Operator : JC/MD
Sample : N4614-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-44

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------