
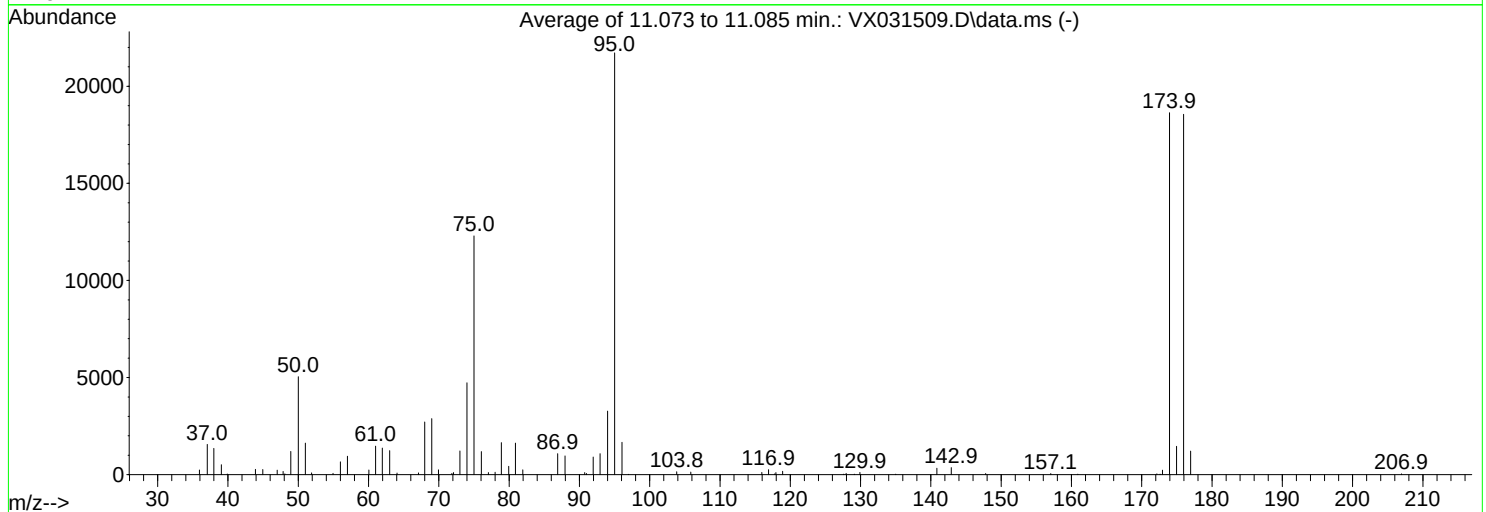


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092122\
Data File : VX031509.D
Acq On : 21 Sep 2022 07:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Title : SW846 8260
Last Update : Tue Sep 20 09:45:29 2022

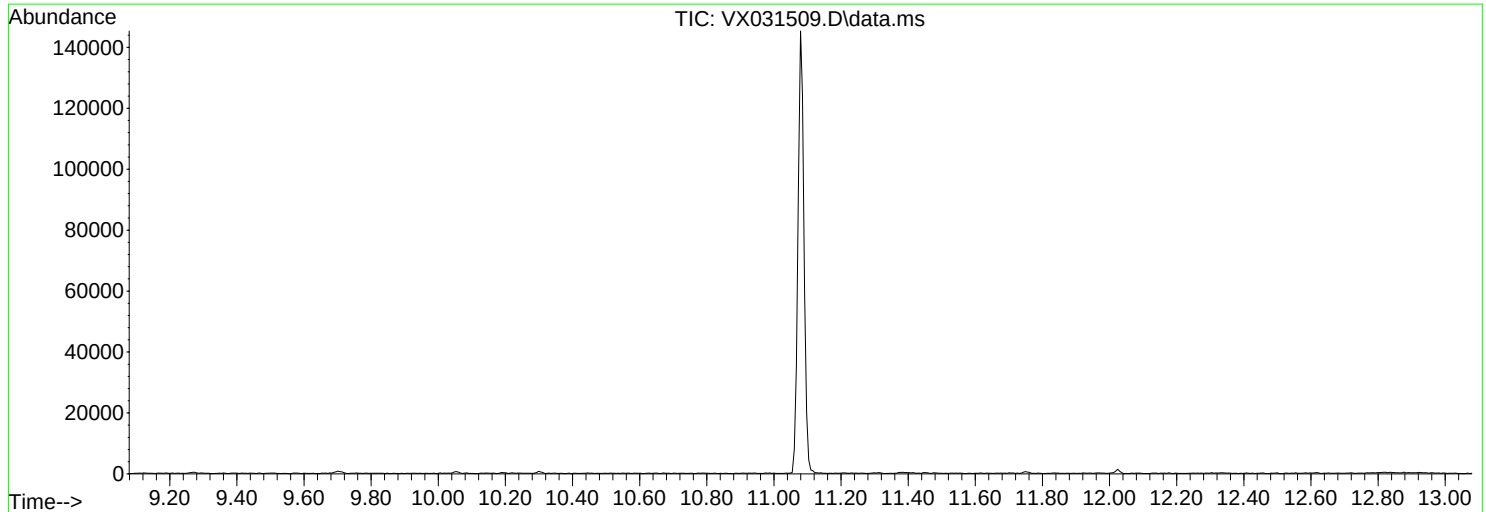

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	5041	PASS
75	95	30	60	56.6	12289	PASS
95	95	100	100	100.0	21720	PASS
96	95	5	9	7.7	1667	PASS
173	174	0.00	2	1.2	231	PASS
174	95	50	100	85.8	18634	PASS
175	174	5	9	7.8	1458	PASS
176	174	95	101	99.6	18556	PASS
177	176	5	9	6.5	1211	PASS