

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092123\
Data File : VX037851.D
Acq On : 21 Sep 2023 13:40
Operator : JC/MD
Sample : 04540-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRANSCO-M-R-HEATER

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M

Title : SW846 8260

Signal : TIC: VX037851.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	690	706	720	rBV	145344	425771	32.63%	5.913%
2	5.556	722	733	752	rVB	252480	720279	55.20%	10.003%
3	5.958	789	799	816	rBV2	155616	416819	31.95%	5.789%
4	6.763	922	931	953	rBV	393394	939763	72.03%	13.052%
5	8.647	1233	1240	1256	rBV	826225	1304744	100.00%	18.121%
6	10.055	1465	1471	1487	rBV	888436	1190374	91.23%	16.532%
7	11.079	1634	1639	1651	rBV	736907	940122	72.05%	13.057%
8	12.024	1788	1794	1804	rBV	984552	1262492	96.76%	17.534%




Sum of corrected areas: 7200364

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092123\
Data File : VX037851.D
Acq On : 21 Sep 2023 13:40
Operator : JC/MD
Sample : 04540-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRANSCO-M-R-HEATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

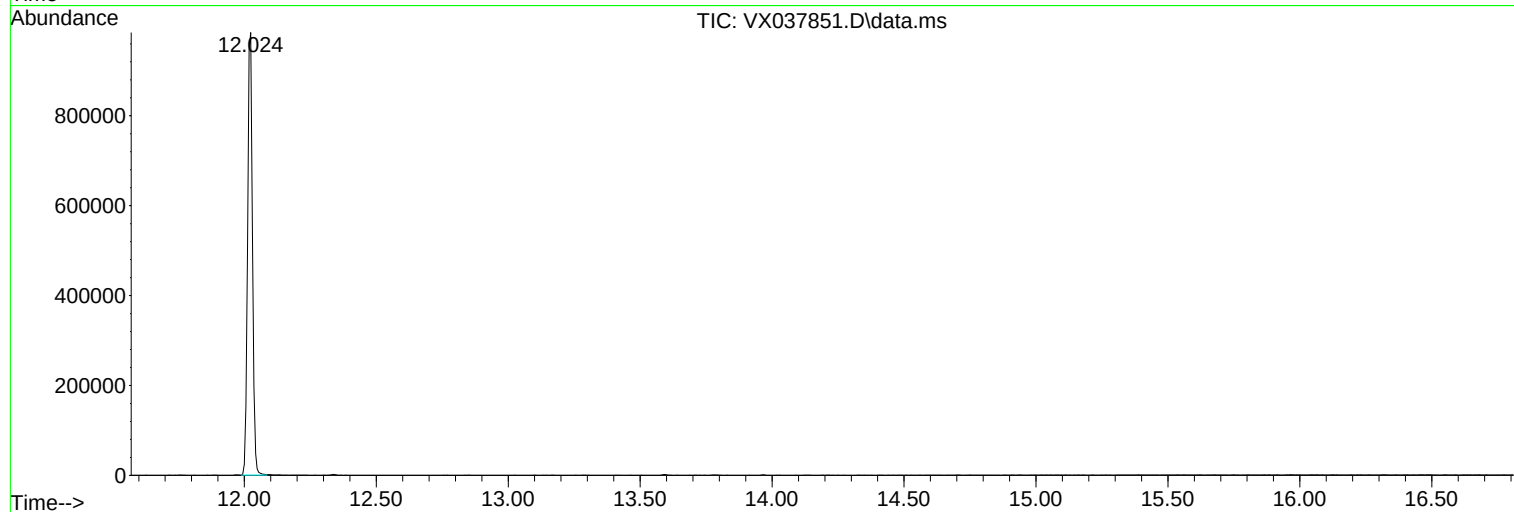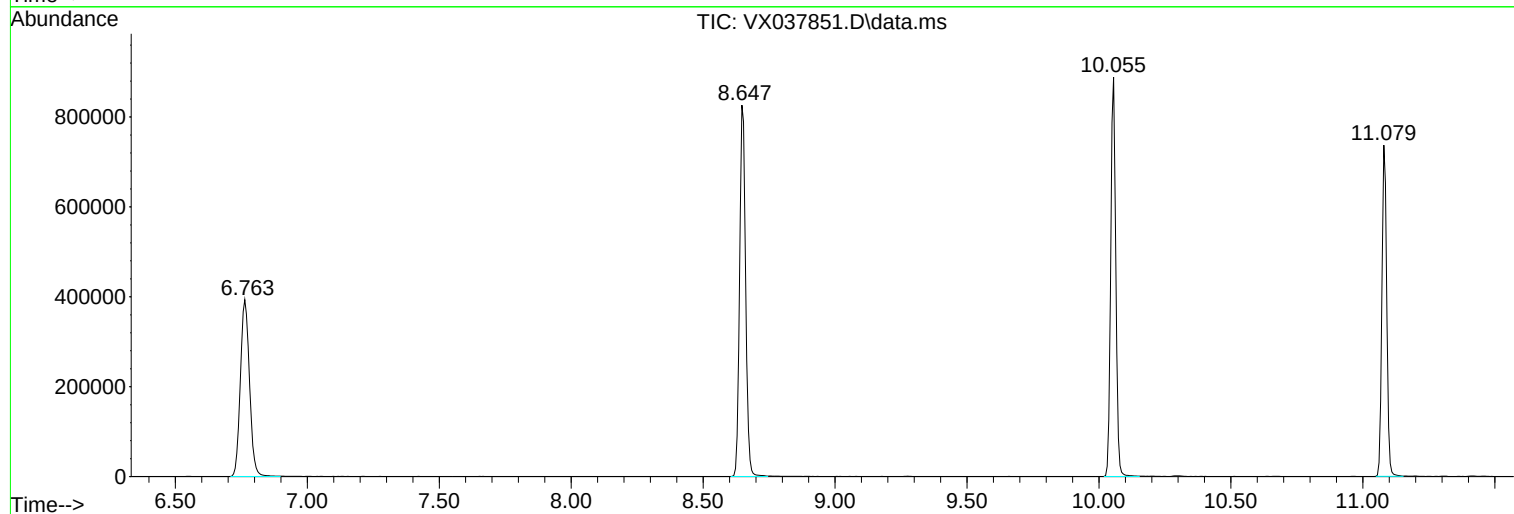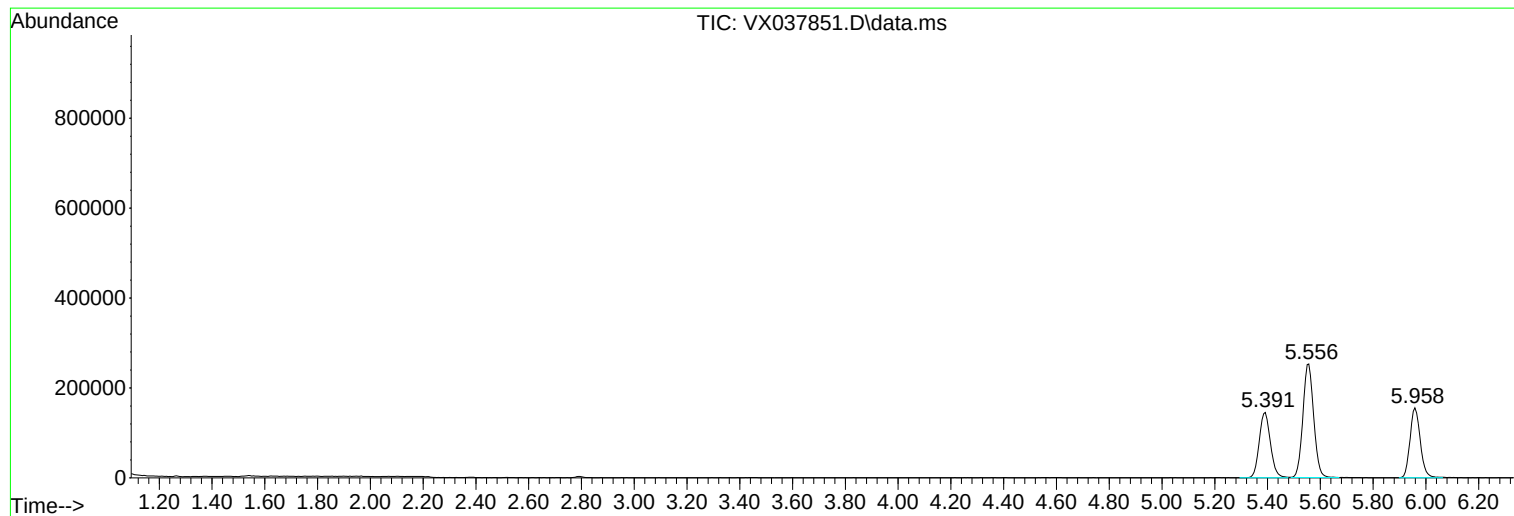

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092123\
Data File : VX037851.D
Acq On : 21 Sep 2023 13:40
Operator : JC/MD
Sample : 04540-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRANSCO-M-R-HEATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092123\
Data File : VX037851.D
Acq On : 21 Sep 2023 13:40
Operator : JC/MD
Sample : 04540-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TRANSCO-M-R-HEATER

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------