
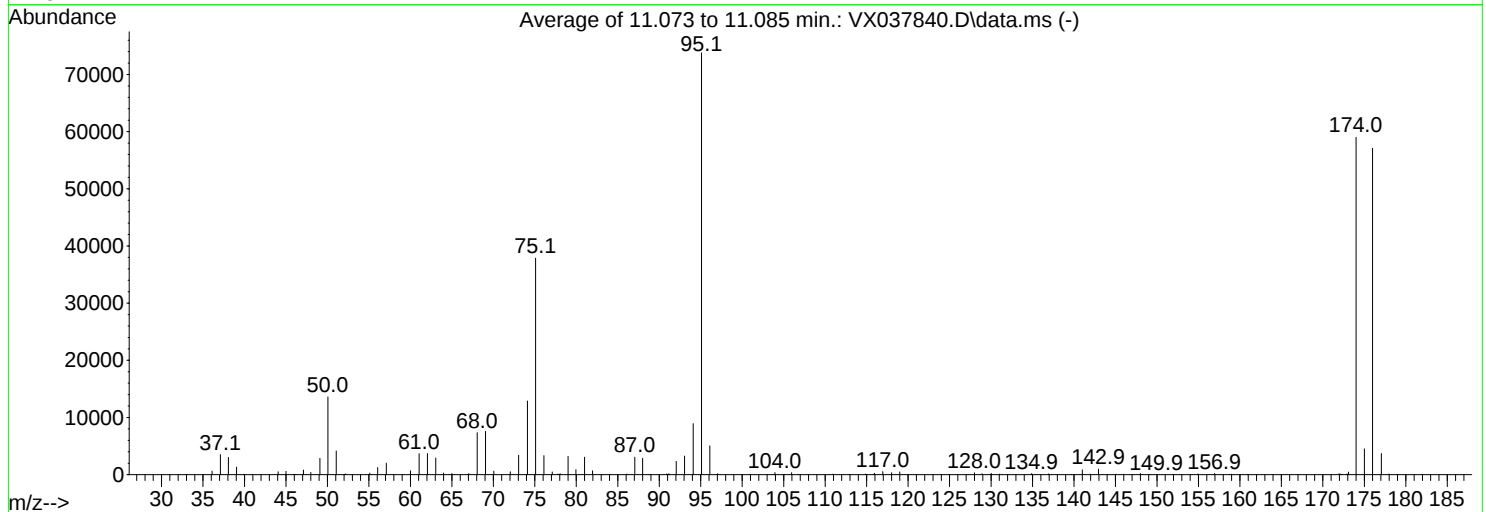


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092123\
 Data File : VX037840.D
 Acq On : 21 Sep 2023 08:07
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Title : SW846 8260
 Last Update : Sat Sep 16 04:55:44 2023

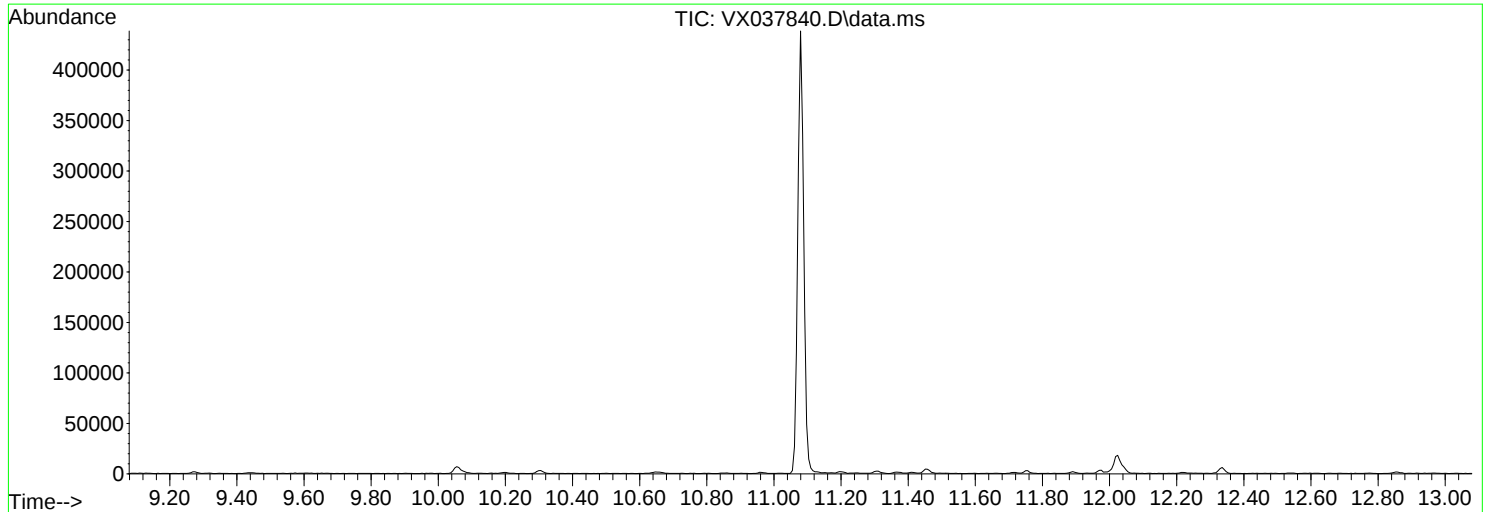

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	13598	PASS
75	95	30	60	51.3	37883	PASS
95	95	100	100	100.0	73789	PASS
96	95	5	9	6.8	5037	PASS
173	174	0.00	2	0.7	440	PASS
174	95	50	100	80.0	59005	PASS
175	174	5	9	7.6	4498	PASS
176	174	95	101	96.8	57112	PASS
177	176	5	9	6.5	3689	PASS