
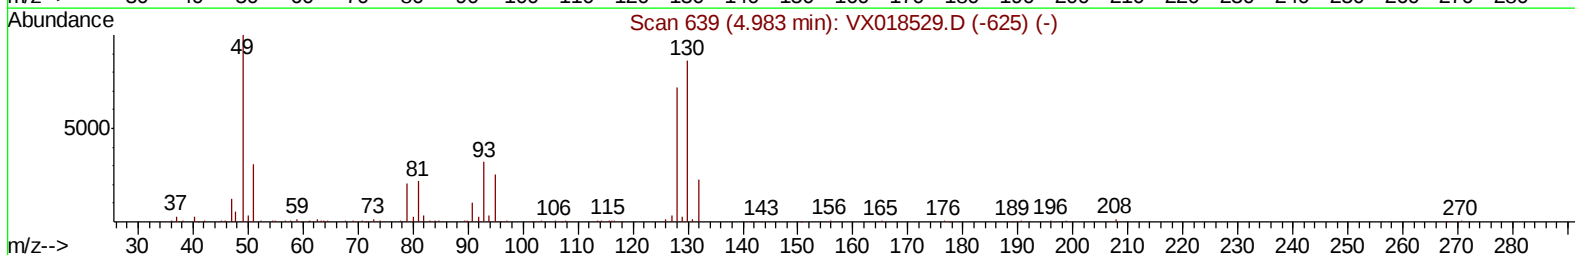
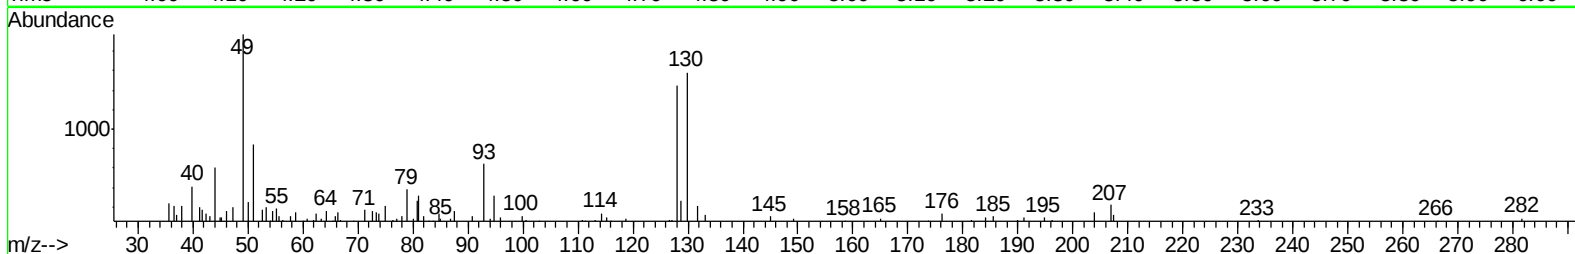


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092220\
Data File : VX018527.D
Acq On : 22 Sep 2020 17:54
Operator : JC/SP
Sample : VSTD0.561
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Sep 23 04:24:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR092220WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Sep 23 03:43:27 2020
Response via : Initial Calibration

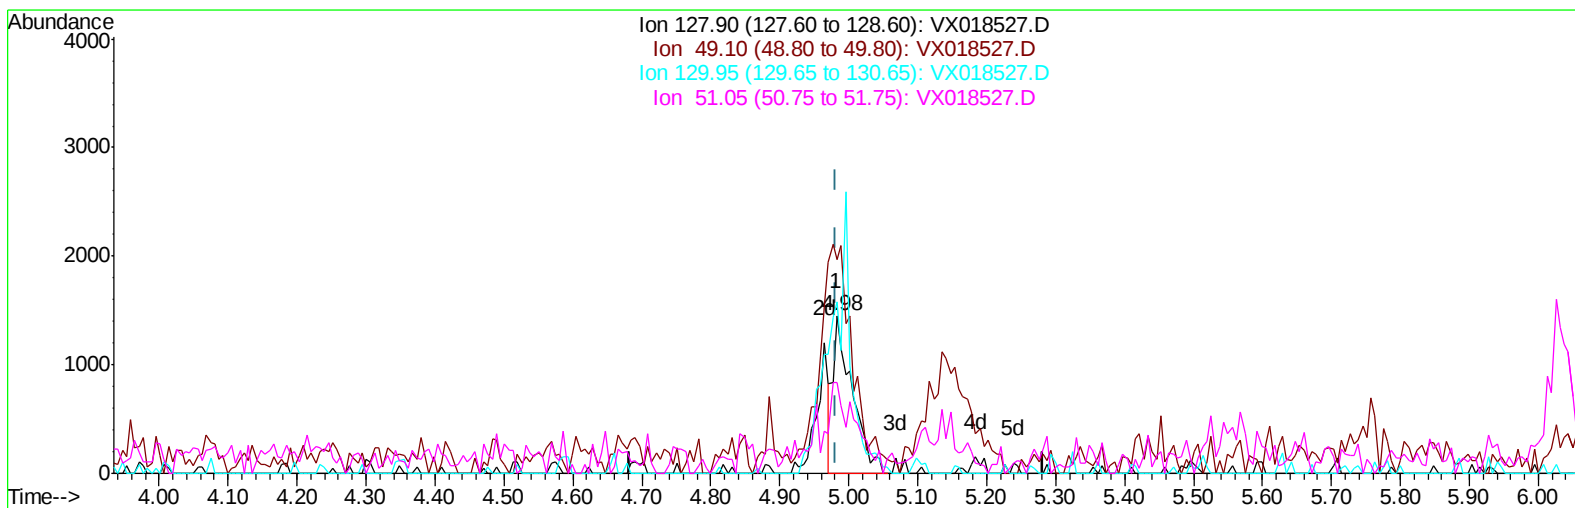

TIC: VX018527.D

(23) Bromochloromethane (T)

4.983min (+0.000) 0.30ug/L

response 2781

Ion	Exp%	Act%
127.90	100	100
49.10	142.30	136.00
129.95	119.40	109.24
51.05	44.00	57.79#