

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092220\
 Data File : VX018535.D
 Acq On : 23 Sep 2020 12:04
 Operator : JC/SP
 Sample : VX0922WBL01
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK301

Quant Time: Sep 24 00:59:52 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR092220WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 24 00:42:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	272883	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	264075	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	121175	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	70523	4.73	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.60%
7) Chloroethane-d5	1.70	69	57895	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.00%
11) 1,1-Dichloroethene-d2	2.34	63	122195	3.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.80%
20) 2-Butanone-d5	4.56	46	177059	50.68	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.36%
24) Chloroform-d	5.14	84	153210	4.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.20%
26) 1,2-Dichloroethane-d4	6.03	65	84689	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
32) Benzene-d6	6.04	84	289357	4.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.40%
36) 1,2-Dichloropropane-d6	7.37	67	88892	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	8.70	98	261622	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.40%
43) trans-1,3-Dichloropropene-	8.99	79	36455	4.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.20%
46) 2-Hexanone-d5	9.43	63	135649	47.68	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.36%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	61599	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
66) 1,2-Dichlorobenzene-d4	12.36	152	96288	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
16) Methylene chloride	2.84	84	12214	0.734 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092220\
Data File : VX018535.D
Acq On : 23 Sep 2020 12:04
Operator : JC/SP
Sample : VX0922WBL01
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK301

Quant Time: Sep 24 00:59:52 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR092220WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 24 00:42:13 2020
Response via : Initial Calibration

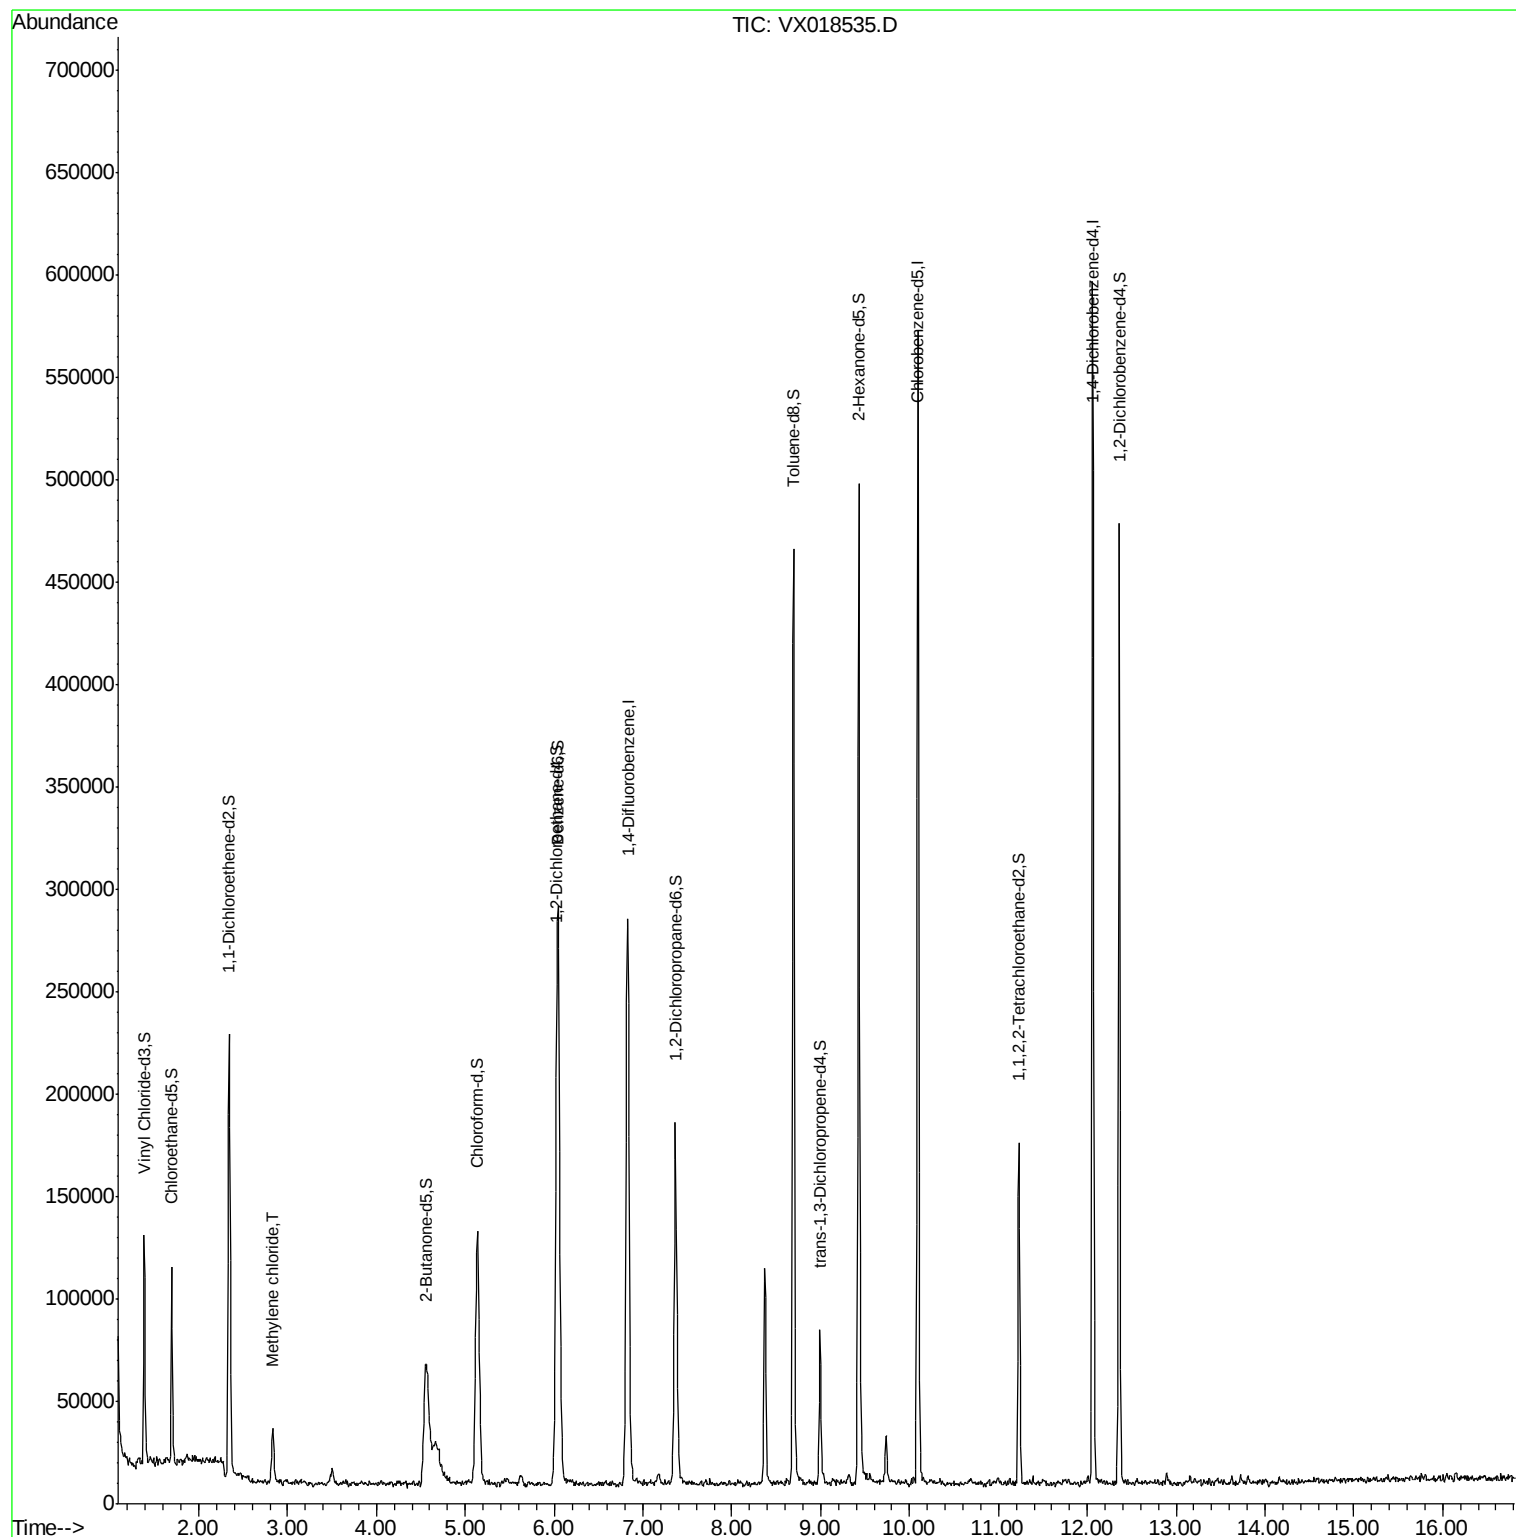

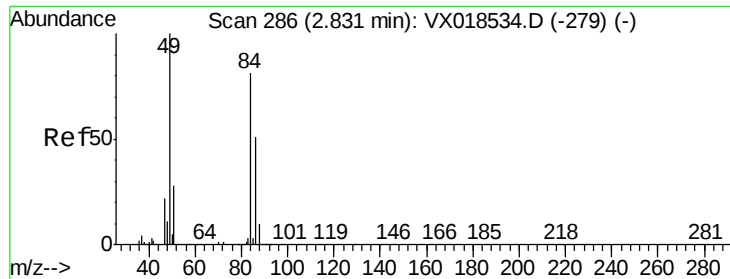

#16
 Methvlene chloride
 Concen: 0.734 ug/L
 RT: 2.84 min Scan# 287
 Delta R.T. 0.01 min
 Lab File: VX018535.D
 Acq: 23 Sep 2020 12:04

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK301

Tot Ion: 84 Resp: 12214
 Ion Ratio Lower Upper
 84 100
 86 66.7 39.8 74.0
 49 130.8 79.5 147.6

