

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX092220\
 Data File : VX018536.D
 Acq On : 23 Sep 2020 12:28
 Operator : JC/SP
 Sample : VX0922WBL02
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK302

Quant Time: Sep 24 01:08:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR092220WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 24 00:42:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	260530	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	253588	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.06	152	116527	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	74797	5.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	105.20%
7) Chloroethane-d5	1.70	69	62641	5.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.00%
11) 1,1-Dichloroethene-d2	2.34	63	136455	4.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	88.80%
20) 2-Butanone-d5	4.57	46	192187	57.62	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.24%
24) Chloroform-d	5.14	84	165376	5.49	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.80%
26) 1,2-Dichloroethane-d4	6.04	65	92597	5.35	ug/L	0.01
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.00%
32) Benzene-d6	6.05	84	320320	5.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.20%
36) 1,2-Dichloropropane-d6	7.37	67	98233	5.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	112.60%
41) Toluene-d8	8.70	98	288700	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%
43) trans-1,3-Dichloropropene-	8.99	79	40780	5.48	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	109.60%
46) 2-Hexanone-d5	9.43	63	152368	55.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.54%
56) 1,1,2,2-Tetrachloroethane-	11.23	84	68327	5.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.20%
66) 1,2-Dichlorobenzene-d4	12.36	152	103733	5.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.00%


Target Compounds					Ovalue
16) Methylene chloride	2.84	84	5620	0.354 ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092220\
Data File : VX018536.D
Acq On : 23 Sep 2020 12:28
Operator : JC/SP
Sample : VX0922WBL02
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK302

Quant Time: Sep 24 01:08:35 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXTR092220WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 24 00:42:13 2020
Response via : Initial Calibration

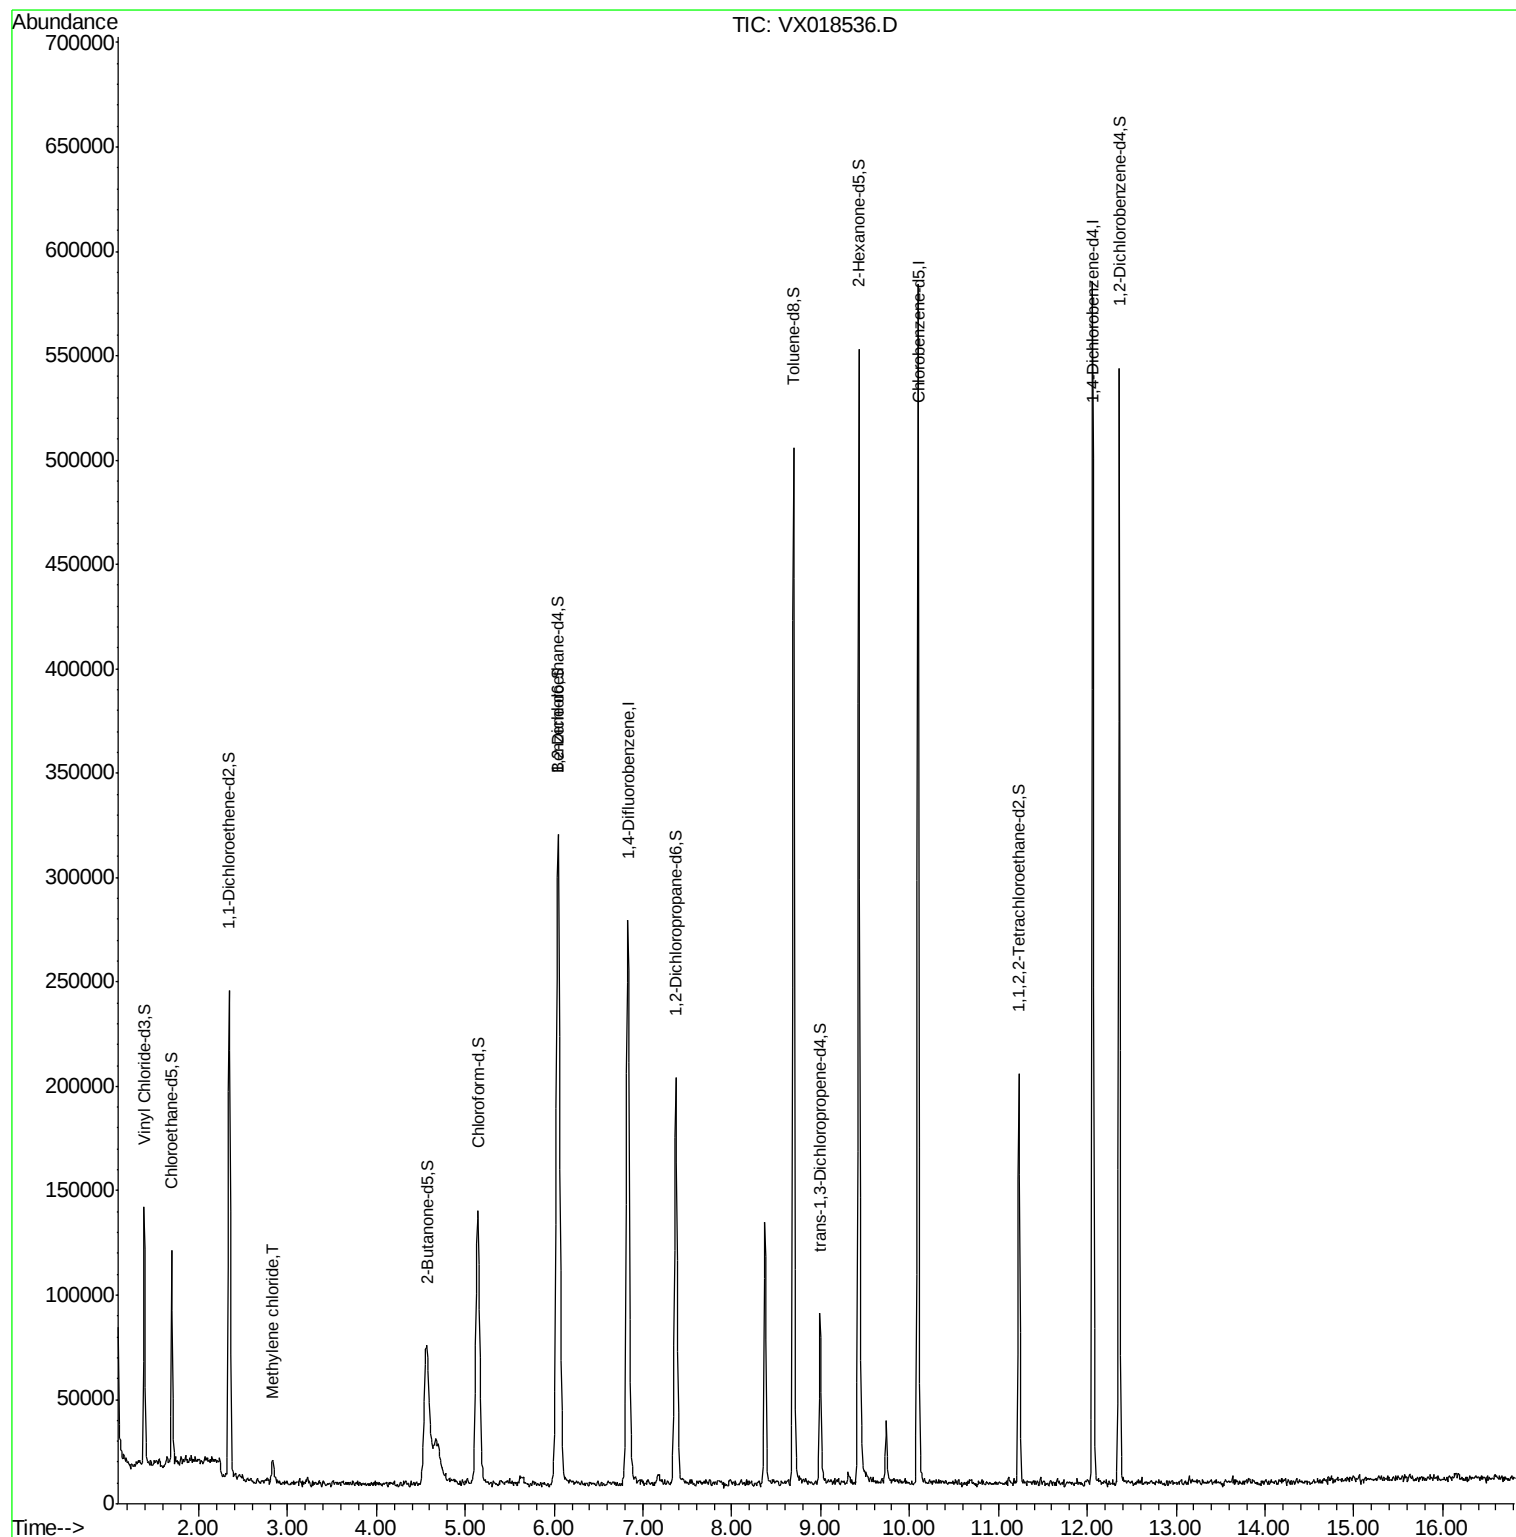

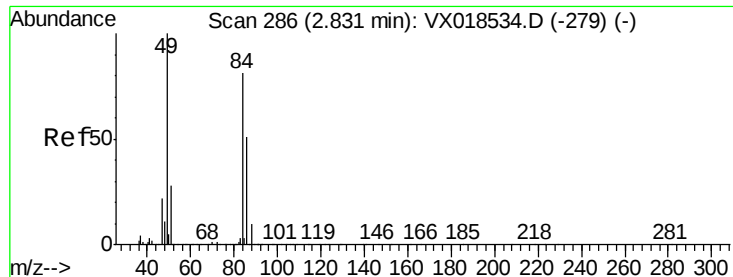

#16
 Methvlene chloride
 Concen: 0.354 ug/L
 RT: 2.84 min Scan# 287
 Delta R.T. 0.01 min
 Lab File: VX018536.D
 Acq: 23 Sep 2020 12:28

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK302

Tot Ion: 84 Resp: 5620
 Ion Ratio Lower Upper
 84 100
 86 62.4 39.8 74.0
 49 93.9 79.5 147.6

