

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031566.D
 Acq On : 22 Sep 2022 13:37
 Operator : JC/MD
 Sample : N4726-05DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CLI-0620DL

Quant Time: Sep 23 01:48:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	68408	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	114663	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	103625	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	48941	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	71803	57.284	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 114.560%	
35) Dibromofluoromethane	5.391	113	61529	51.944	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 103.880%	
50) Toluene-d8	8.653	98	235397	51.529	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 103.060%	
62) 4-Bromofluorobenzene	11.079	95	73818	47.704	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 95.400%	
Target Compounds						
						Qvalue
5) Bromomethane	1.618	94	799	0.377	ug/l	91
6) Chloroethane	1.709	64	107	Below Cal	#	43
10) Methyl Iodide	2.447	142	231	0.217	ug/l #	73
11) Tert butyl alcohol	2.940	59	3797	Below Cal	#	73
16) Acetone	2.386	43	13146	13.579	ug/l	95
19) Methyl tert-butyl Ether	3.123	73	1782	0.463	ug/l	92
20) Methylene Chloride	2.788	84	265	Below Cal	#	76
22) Diisopropyl ether	3.764	45	764	0.203	ug/l #	88
25) 2-Butanone	4.580	43	1055	1.089	ug/l #	49
36) 1,1-Dichloropropene	5.556	75	5631	3.090	ug/l #	49
38) Carbon Tetrachloride	5.550	117	7195	3.561	ug/l #	16
40) Benzene	6.044	78	19639	3.612	ug/l	94
52) Toluene	8.720	92	104723	29.531	ug/l	98
53) t-1,3-Dichloropropene	8.720	75	1271	0.621	ug/l #	1
67) Ethyl Benzene	10.195	91	32052	5.681	ug/l	99
68) m/p-Xylenes	10.299	106	65393	28.840	ug/l	96
69) o-Xylene	10.640	106	32677	15.099	ug/l	95
70) Styrene	10.640	104	2134	0.599	ug/l #	1
73) Isopropylbenzene	10.963	105	2069	0.566	ug/l	94
75) 1,1,2,2-Tetrachloroethane	11.085	83	112	Below Cal	#	1
76) 1,2,3-Trichloropropane	11.079	75	43397	39.730	ug/l #	37
78) n-propylbenzene	11.305	91	3661	0.871	ug/l	93
79) 2-Chlorotoluene	11.378	91	5019	2.005	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	12203	3.934	ug/l	100
81) trans-1,4-Dichloro-2-b...	11.079	75	43397	127.923	ug/l #	11
82) 4-Chlorotoluene	11.451	91	1650	0.562	ug/l #	51
83) tert-Butylbenzene	11.750	119	7049	2.345	ug/l #	57
84) 1,2,4-Trimethylbenzene	11.750	105	56383	18.459	ug/l	97
85) sec-Butylbenzene	11.750	105	56383	14.821	ug/l #	56
86) p-Isopropyltoluene	11.969	119	870	0.271	ug/l	97
89) n-Butylbenzene	12.323	91	1894	0.692	ug/l #	26
90) Hexachloroethane	12.530	117	436	0.790	ug/l #	15
94) Hexachlorobutadiene	13.719	225	211	Below Cal	#	59
95) Naphthalene	13.780	128	41094	11.713	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	237	0.240	ug/l	80

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031566.D
Acq On : 22 Sep 2022 13:37
Operator : JC/MD
Sample : N4726-05DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL

Quant Time: Sep 23 01:48:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031566.D
Acq On : 22 Sep 2022 13:37
Operator : JC/MD
Sample : N4726-05DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Quant Time: Sep 23 01:48:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration

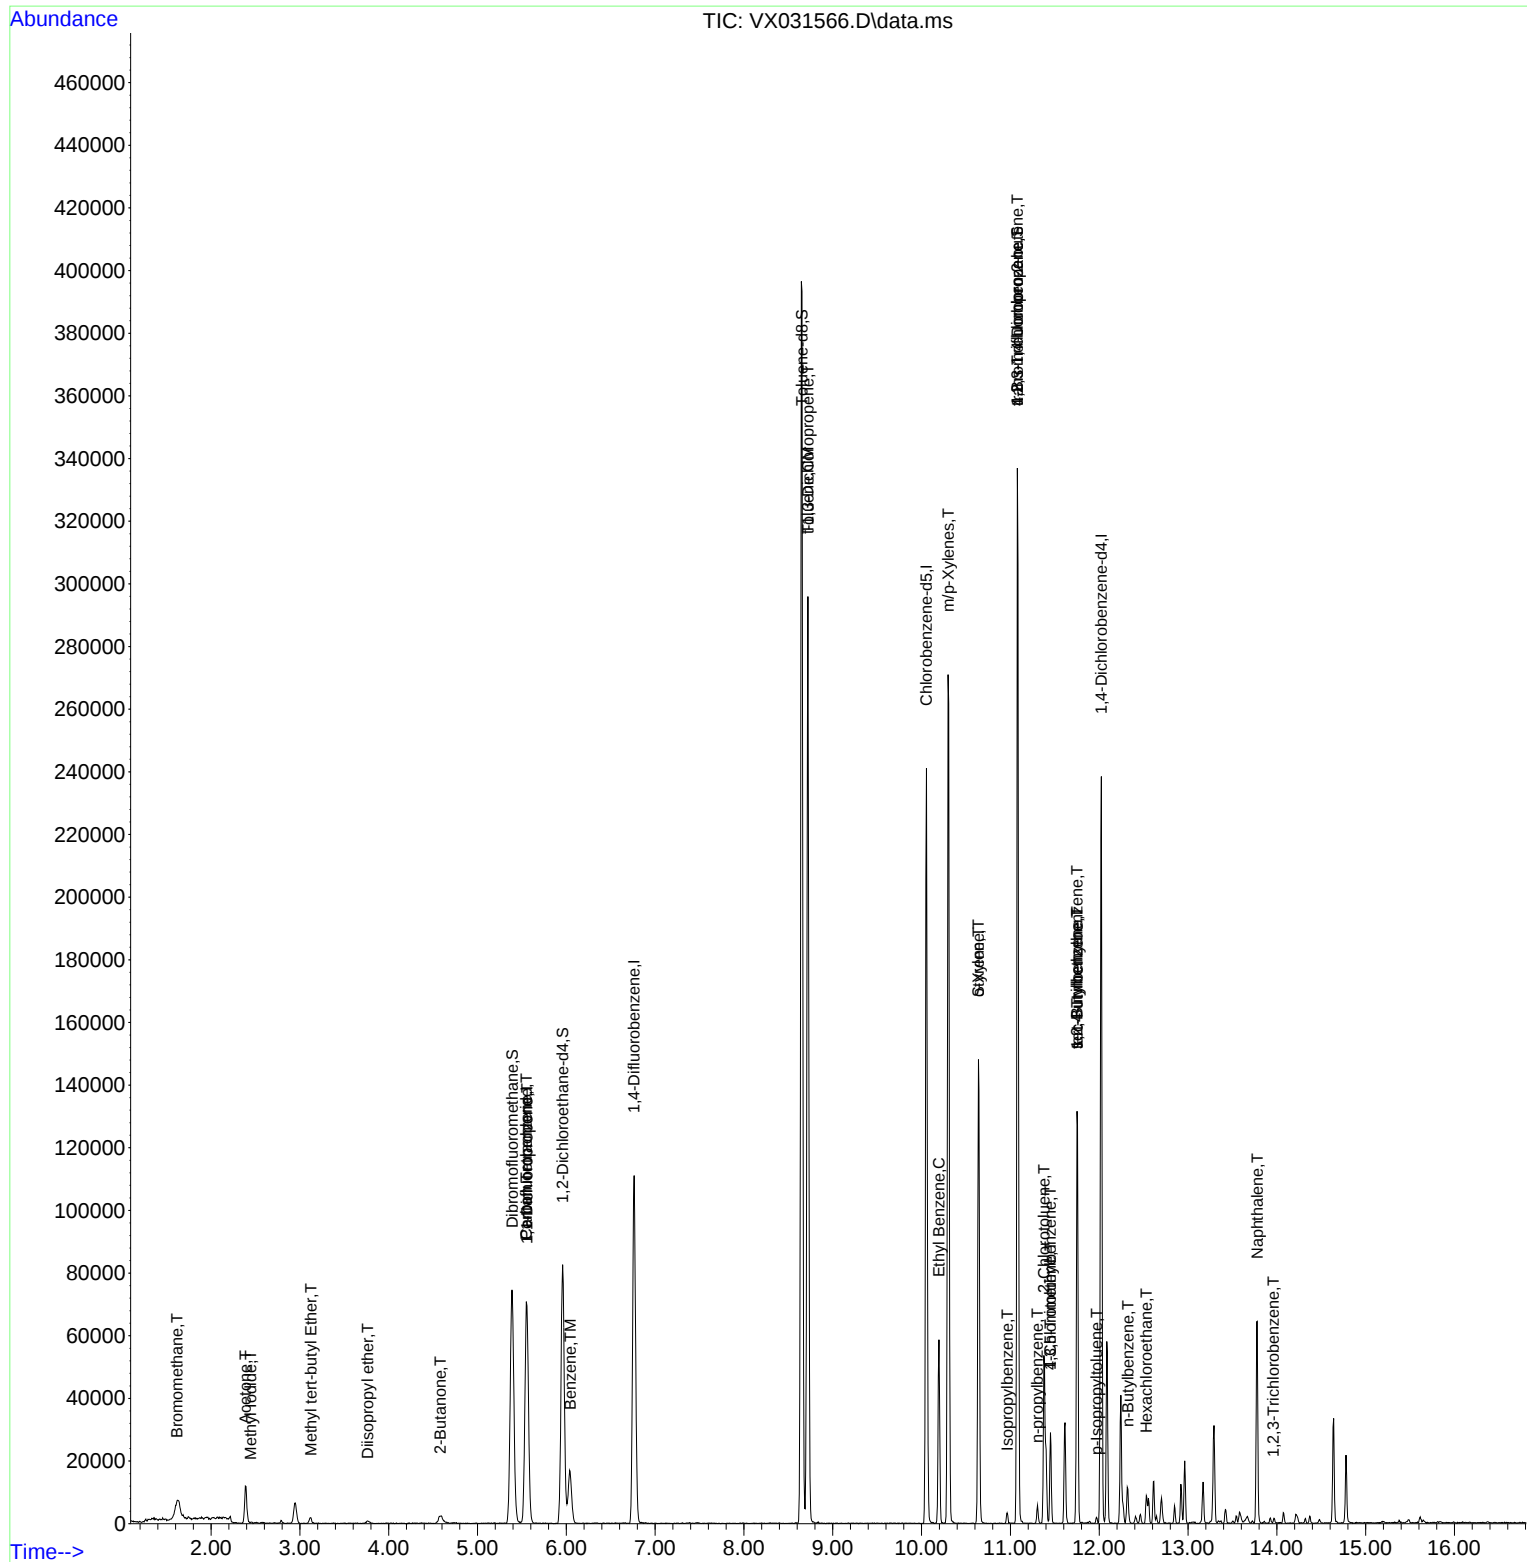






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL






Tgt Ion:168 Resp: 68408
Ion Ratio Lower Upper
168 100
99 52.7 48.8 73.2

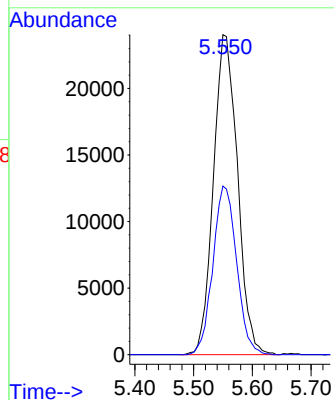


#5
Bromomethane
Concen: 0.377 ug/l
RT: 1.618 min Scan# 87
Delta R.T. 0.007 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 94 Resp: 799
Ion Ratio Lower Upper
94 100
96 84.7 74.4 111.6

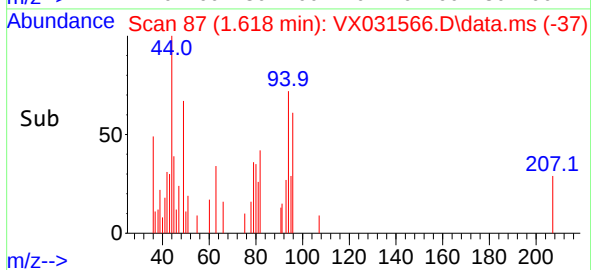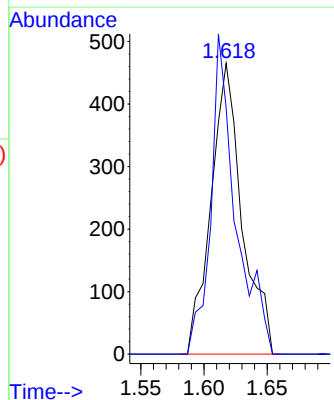


Abundance Scan 98 (1.685 min): VX031454.D\data.ms (-92)

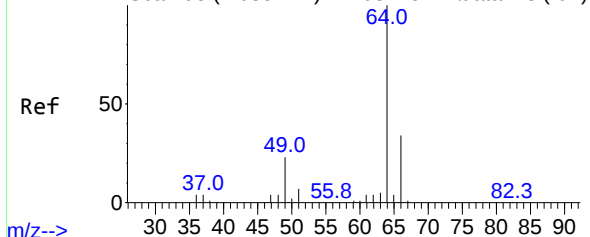


m/z-->

Abundance Scan 102 (1.709 min): VX031566.D\data.ms

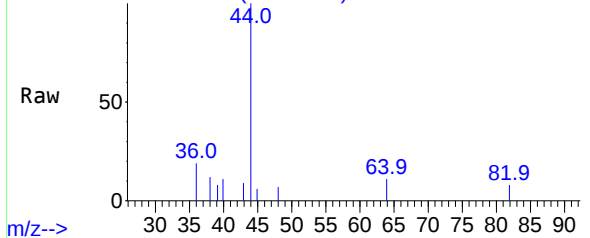


m/z-->

Abundance Scan 102 (1.709 min): VX031566.D\data.ms (-49)

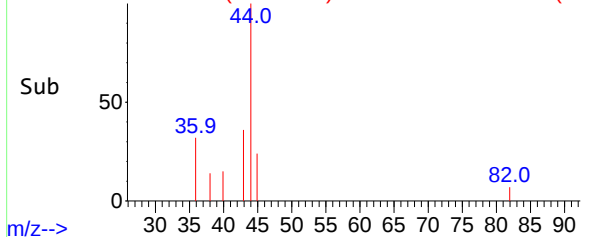


m/z-->

Abundance Scan 224 (2.453 min): VX031454.D\data.ms (-21)

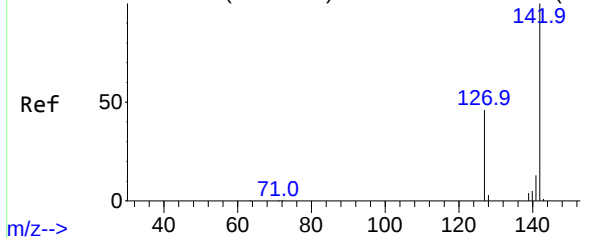


m/z-->

Abundance Scan 223 (2.447 min): VX031566.D\data.ms

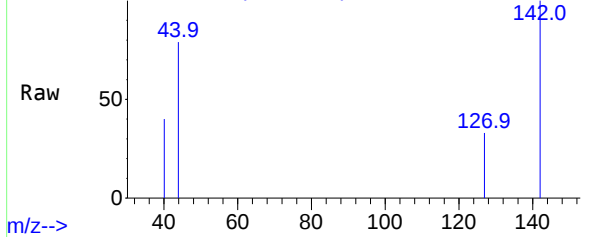

m/z-->

Abundance Scan 223 (2.447 min): VX031566.D\data.ms (-17)

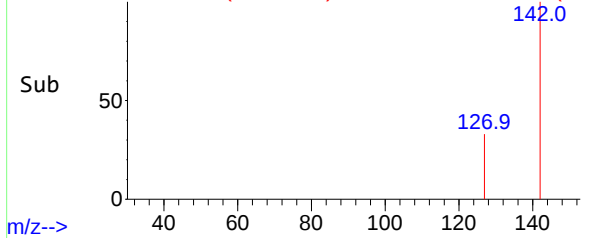

m/z-->

#6

Chloroethane

Concen: Below Cal

RT: 1.709 min Scan# 10

Delta R.T. 0.024 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37

Instrument :

MSVOA_X

ClientSampleId :

CLI-0620DL


Tgt Ion: 64 Resp: 107

Ion Ratio Lower Upper

64 100

66 0.0 25.0 37.4#

Abundance

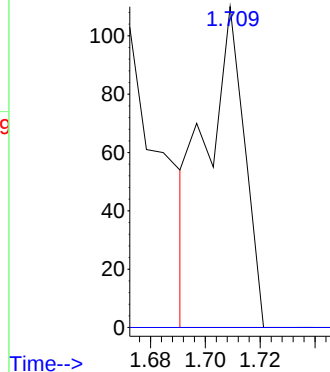

Time-->

#10

Methyl Iodide

Concen: 0.217 ug/l

RT: 2.447 min Scan# 223

Delta R.T. -0.006 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37

Tgt Ion:142 Resp: 231


Ion Ratio Lower Upper

142 100


127 30.3 37.4 56.0#

141 0.0 11.6 17.4#

Abundance

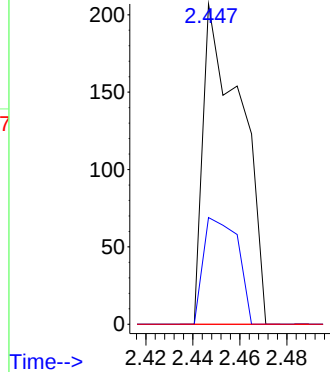

Time-->



#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.940 min Scan# 304

Delta R.T. -0.049 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37

Instrument :

MSVOA_X

ClientSampleId :





CLI-0620DL

Tgt Ion: 59 Resp: 3797

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

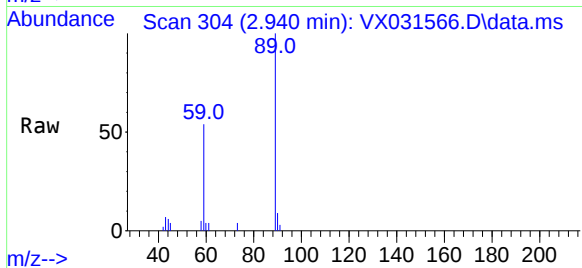

#16

Acetone

Concen: 13.579 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.000 min

Lab File: VX031566.D




Acq: 22 Sep 2022 13:37


Tgt Ion: 43 Resp: 13146

Ion Ratio Lower Upper

43 100

58 27.2 23.8 35.8



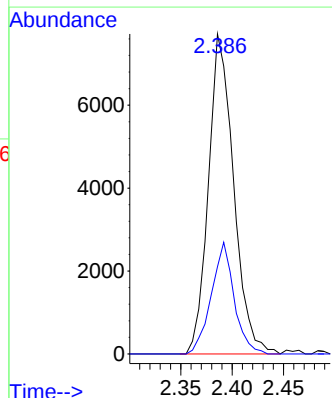
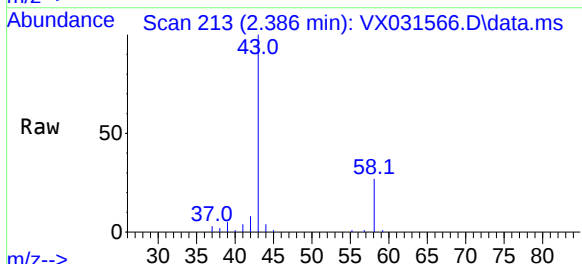




#19
Methyl tert-butyl Ether
Concen: 0.463 ug/l
RT: 3.123 min Scan# 31
Delta R.T. 0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 73 Resp: 1782
Ion Ratio Lower Upper
73 100
57 17.6 17.2 25.8

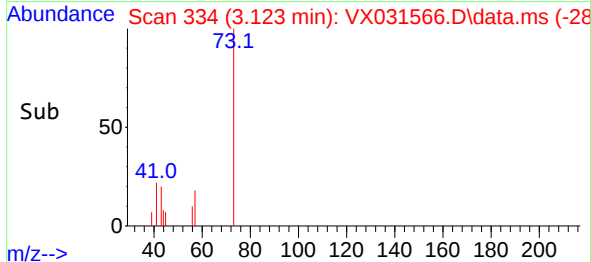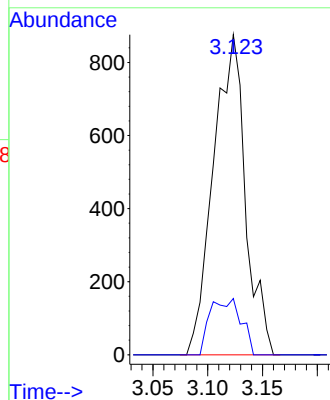

#20
Methylene Chloride
Concen: Below Cal
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37


Tgt Ion: 84 Resp: 265
Ion Ratio Lower Upper
84 100
49 102.4 105.9 158.9#
51 38.9 32.2 48.2
86 91.3 50.8 76.2#

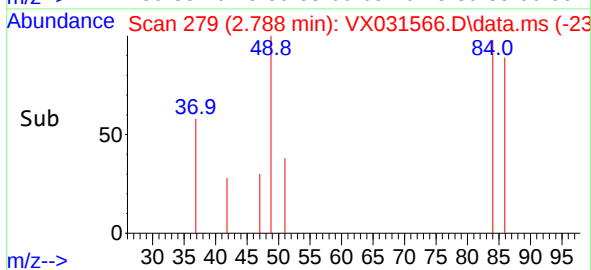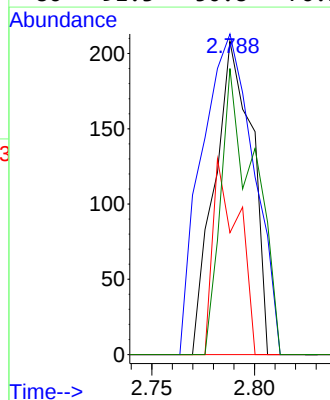






#22
Diisopropyl ether
Concen: 0.203 ug/l
RT: 3.764 min Scan# 41
Delta R.T. -0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL



Tgt Ion: 45 Resp: 764




Ion	Ratio	Lower	Upper
45	100		
43	64.0	59.0	88.6
87	25.1	22.6	33.8
59	0.0	8.8	13.2

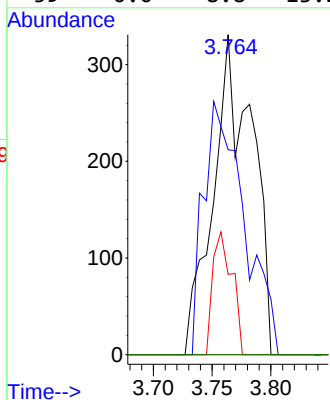


#25
2-Butanone
Concen: 1.089 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 43 Resp: 1055

Ion	Ratio	Lower	Upper
43	100		
72	0.0	21.1	31.7


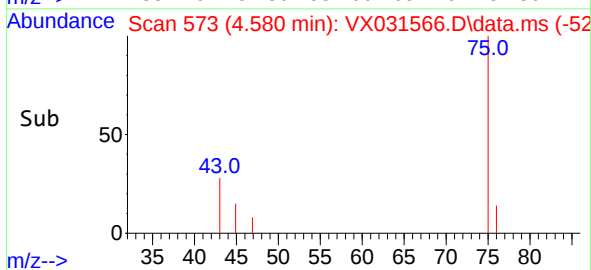
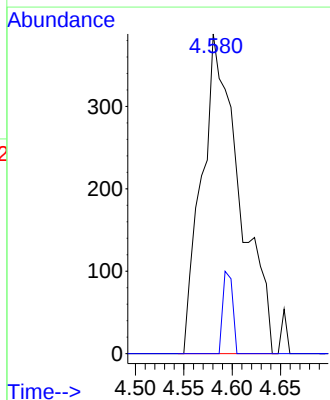



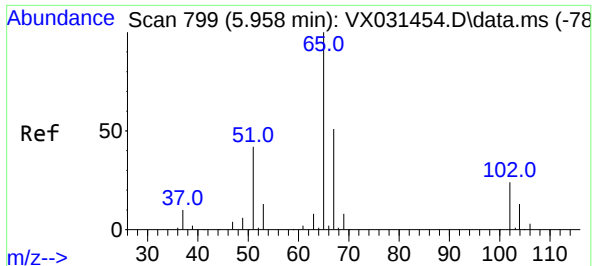

#33
1,2-Dichloroethane-d4
Concen: 57.284 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 65 Resp: 71803
Ion Ratio Lower Upper
65 100
67 52.3 0.0 102.4

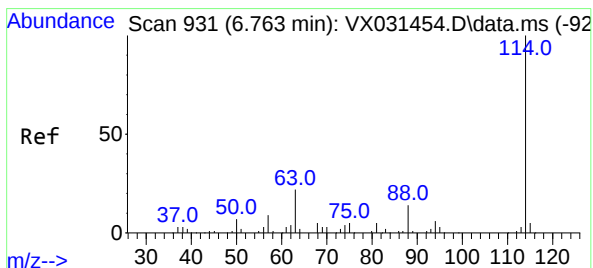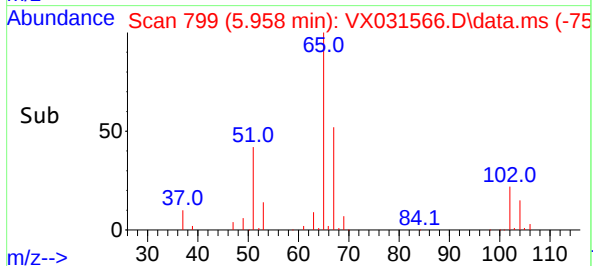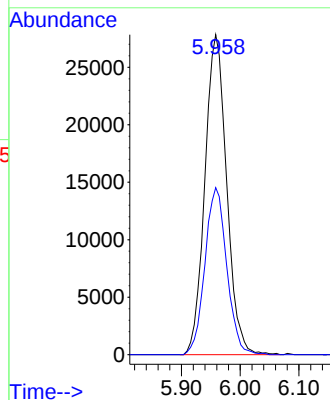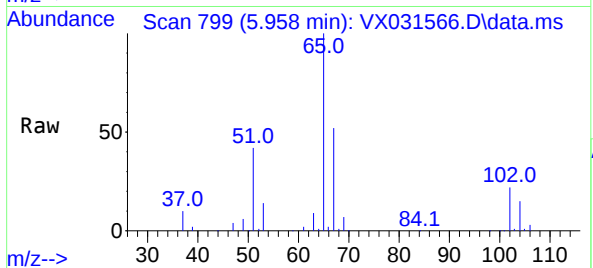

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37


Tgt Ion: 114 Resp: 114663
Ion Ratio Lower Upper
114 100
63 18.9 0.0 42.6
88 14.2 0.0 33.0

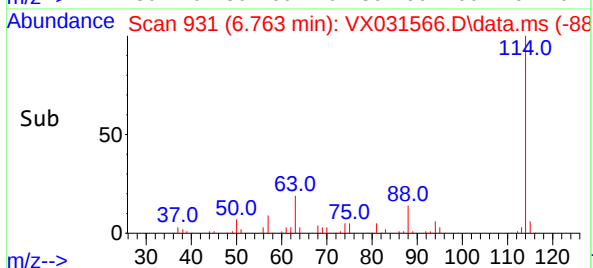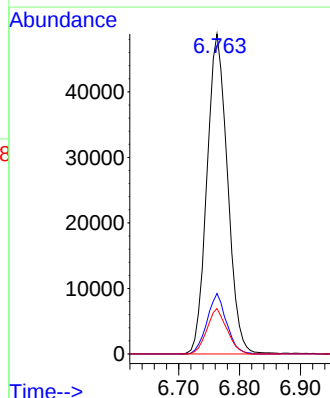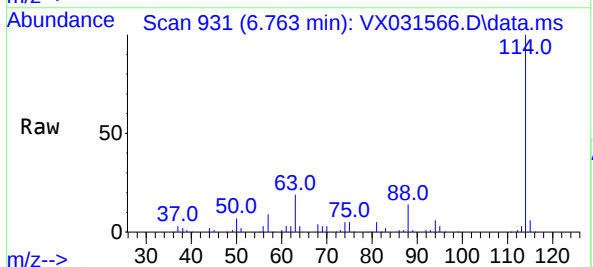



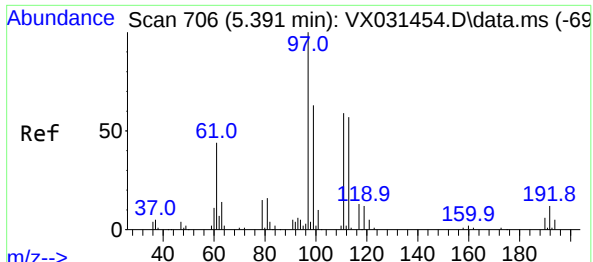


#35
Dibromofluoromethane
Concen: 51.944 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37


Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL

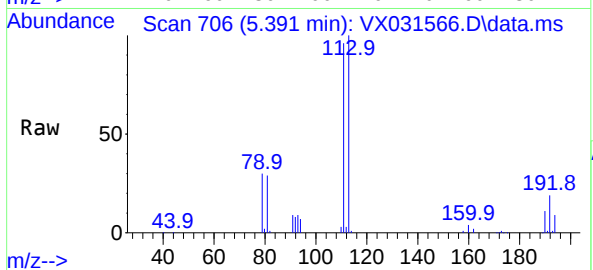



Tgt Ion:113 Resp: 61529
Ion Ratio Lower Upper
113 100
111 102.4 82.4 123.6
192 19.8 14.1 21.1

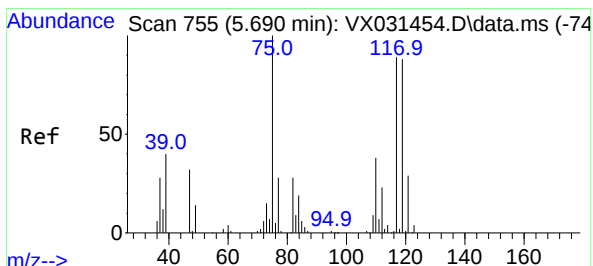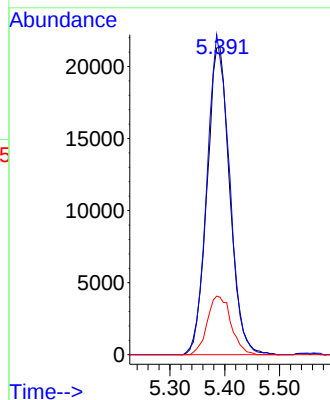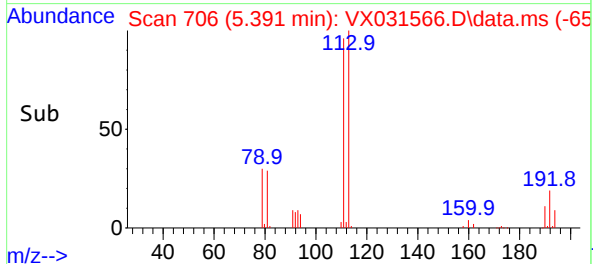


#36
1,1-Dichloropropene
Concen: 3.090 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

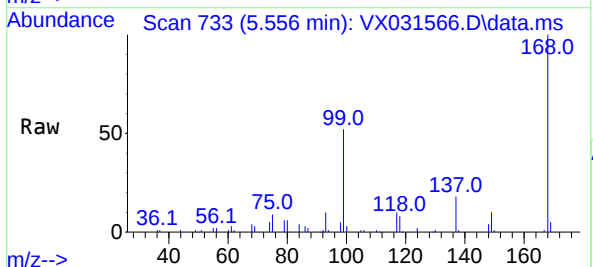


Tgt Ion: 75 Resp: 5631
Ion Ratio Lower Upper
75 100
110 8.8 17.5 52.5#
77 0.0 24.9 37.3#

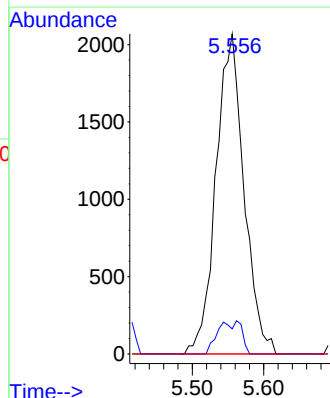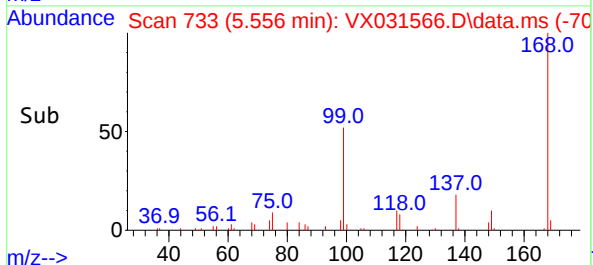






#38
Carbon Tetrachloride
Concen: 3.561 ug/l
RT: 5.550 min Scan# 7195
Delta R.T. -0.128 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL







Tgt Ion:117 Resp: 7195
Ion Ratio Lower Upper
117 100
119 3.4 74.6 112.0#
121 0.0 25.3 37.9#

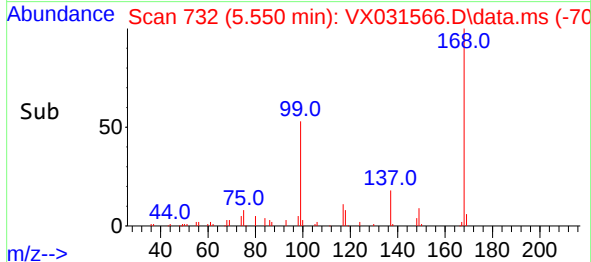

#40
Benzene
Concen: 3.612 ug/l
RT: 6.044 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 78 Resp: 19639
Ion Ratio Lower Upper
78 100
77 26.1 18.7 28.1

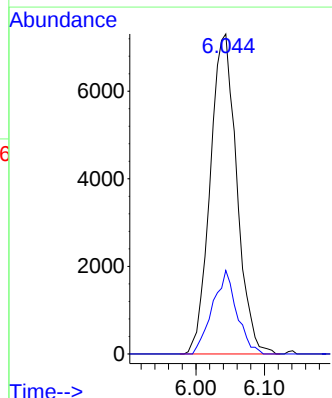

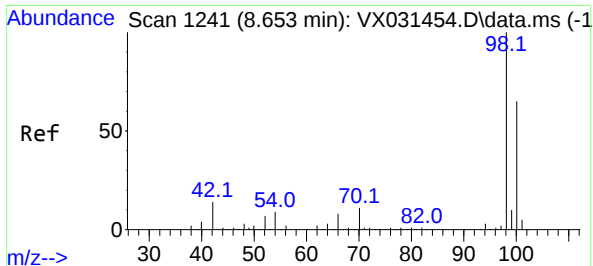

#50

Toluene-d8

Concen: 51.529 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37

Instrument :

MSVOA_X

ClientSampleId :





CLI-0620DL

Tgt Ion: 98 Resp: 235397

Ion Ratio Lower Upper

98 100

100 65.4 52.5 78.7

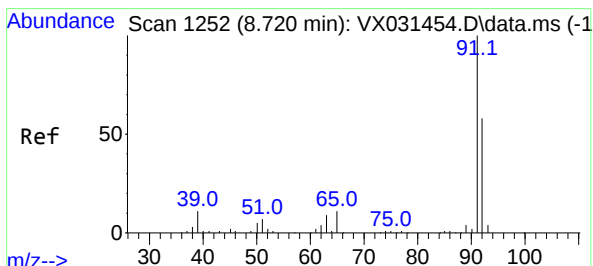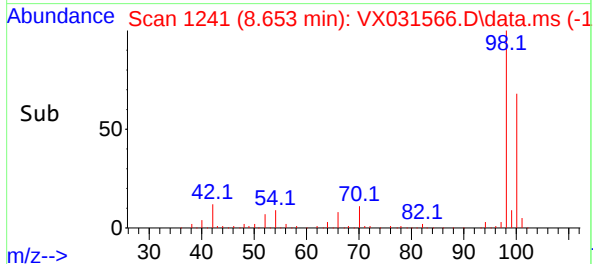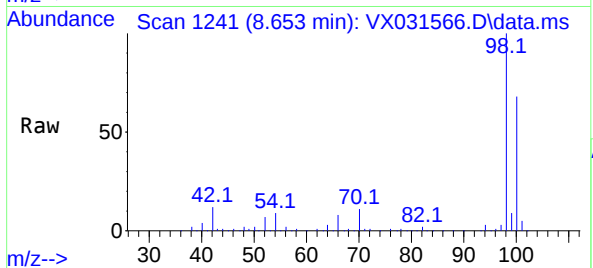

#52

Toluene

Concen: 29.531 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031566.D




Acq: 22 Sep 2022 13:37


Tgt Ion: 92 Resp: 104723

Ion Ratio Lower Upper

92 100

91 173.9 137.1 205.7

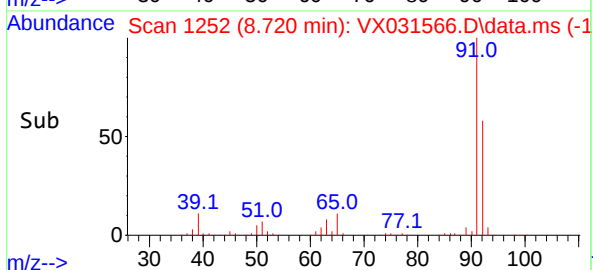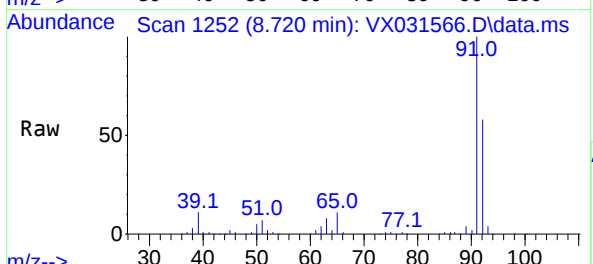



#53

t-1,3-Dichloropropene

Concen: 0.621 ug/l

RT: 8.720 min Scan# 11

Delta R.T. -0.262 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37

Instrument :

MSVOA_X

ClientSampleId :





CLI-0620DL

Tgt Ion: 75 Resp: 1271

Ion Ratio Lower Upper

75 100

77 177.5 24.8 37.2#

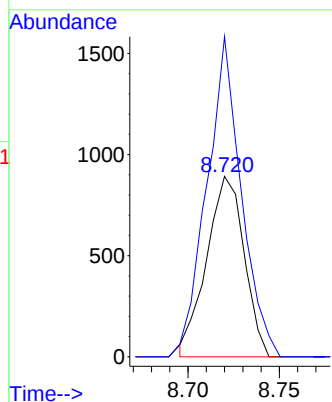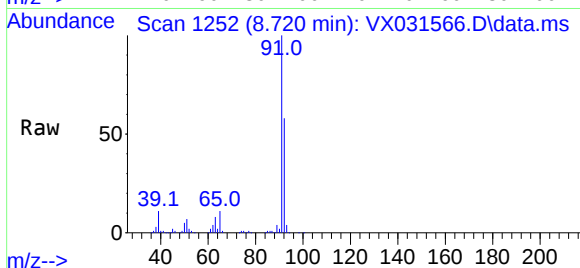

#62

4-Bromofluorobenzene

Concen: 47.704 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX031566.D

Acq: 22 Sep 2022 13:37




Tgt Ion: 95 Resp: 73818


Ion Ratio Lower Upper

95 100

174 93.0 0.0 153.2

176 89.1 0.0 144.0


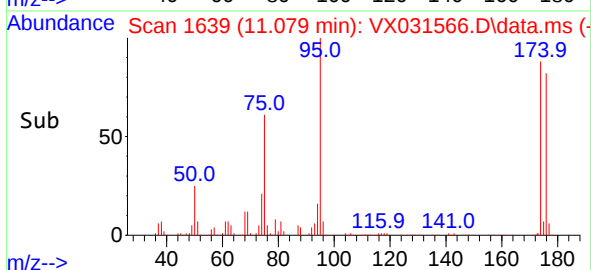

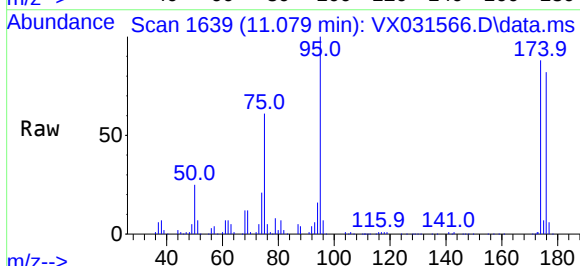




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:117 Resp: 103625
Ion Ratio Lower Upper
117 100
82 49.8 46.8 70.2
119 32.3 26.4 39.6



#67
Ethyl Benzene
Concen: 5.681 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 91 Resp: 32052
Ion Ratio Lower Upper
91 100
106 31.1 25.2 37.8



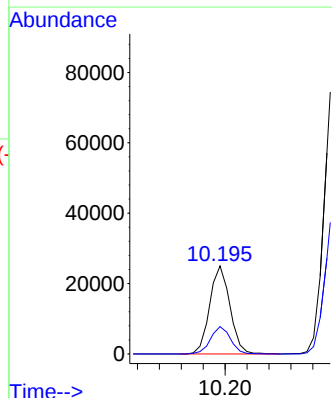
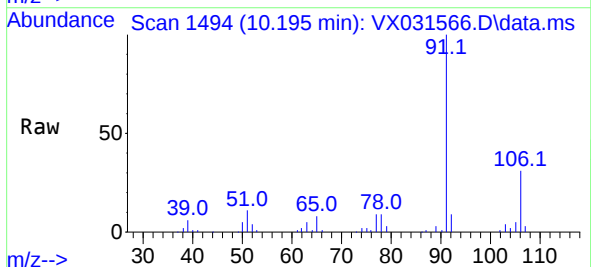




#68
m/p-Xylenes
Concen: 28.840 ug/l
RT: 10.299 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:106 Resp: 65393
Ion Ratio Lower Upper
106 100
91 195.4 161.0 241.4

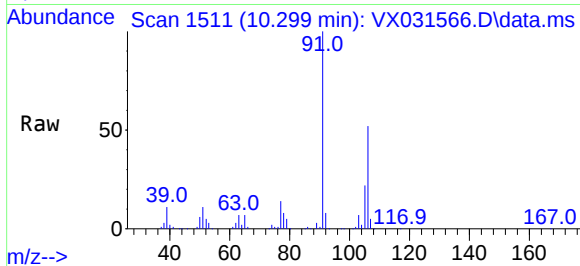

#69
o-Xylene
Concen: 15.099 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion:106 Resp: 32677
Ion Ratio Lower Upper
106 100
91 206.7 107.2 321.6


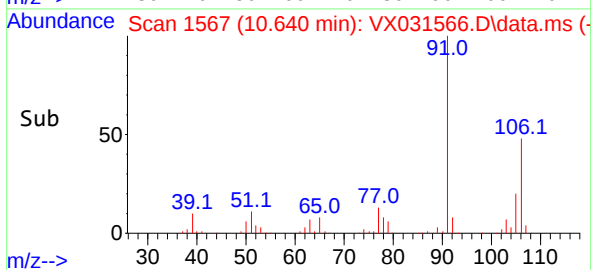

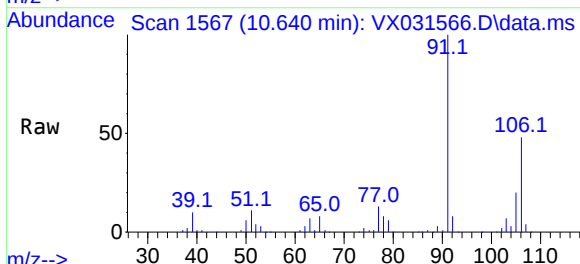




#70
Styrene
Concen: 0.599 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.019 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:104 Resp: 2134
Ion Ratio Lower Upper
104 100
78 249.6 41.4 62.2#
103 230.6 43.8 65.8#

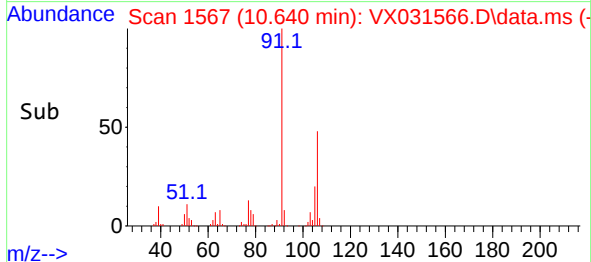

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion:152 Resp: 48941
Ion Ratio Lower Upper
152 100
115 54.2 43.4 130.1
150 154.2 0.0 346.8


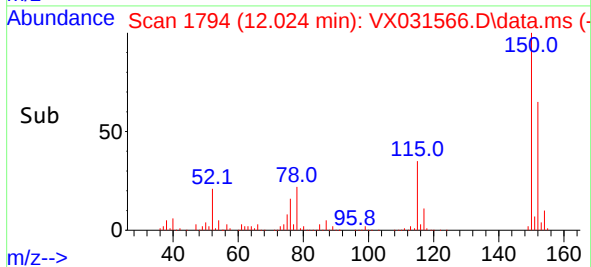

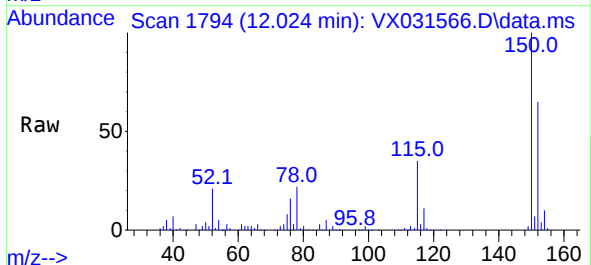




#73
Isopropylbenzene
Concen: 0.566 ug/l
RT: 10.963 min Scan# 1
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:105 Resp: 2069
Ion Ratio Lower Upper
105 100
120 23.9 13.7 41.0

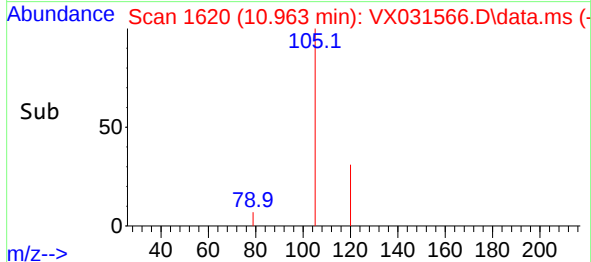

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.085 min Scan# 1640
Delta R.T. -0.128 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 83 Resp: 112
Ion Ratio Lower Upper
83 100
131 128.6 5.1 15.4#
85 0.0 32.6 97.8#


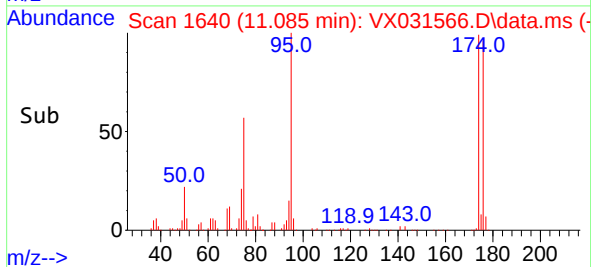

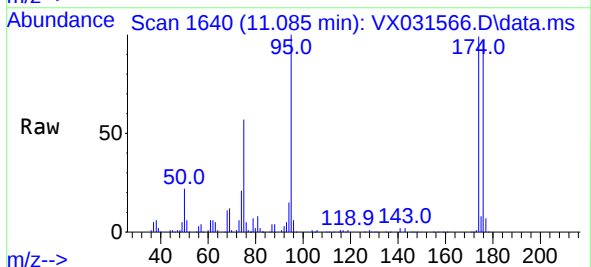




#76
1,2,3-Trichloropropane
Concen: 39.730 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 75 Resp: 43397
Ion Ratio Lower Upper
75 100
77 1.3 20.3 60.9#

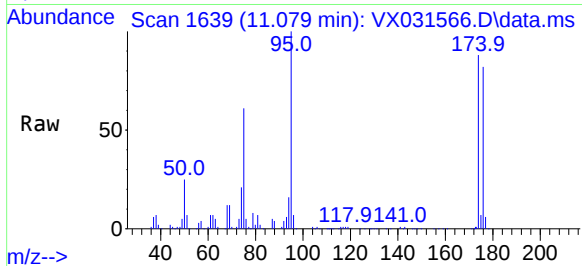

#78
n-propylbenzene
Concen: 0.871 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 91 Resp: 3661
Ion Ratio Lower Upper
91 100
120 20.0 11.8 35.4




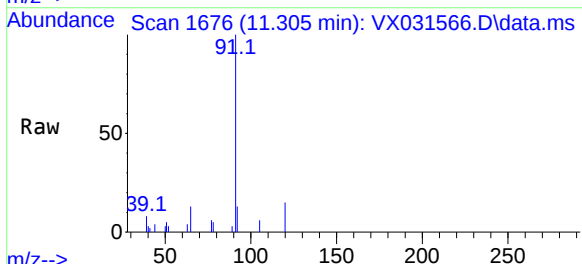




#79
2-Chlorotoluene
Concen: 2.005 ug/l
RT: 11.378 min Scan# 11
Delta R.T. 0.012 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 91 Resp: 5019
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#

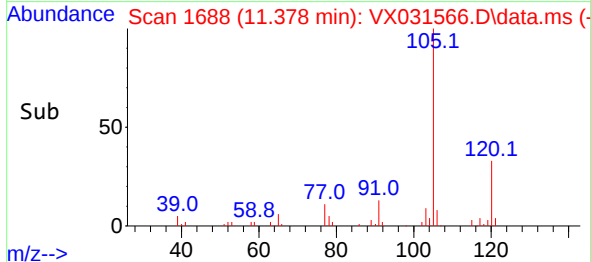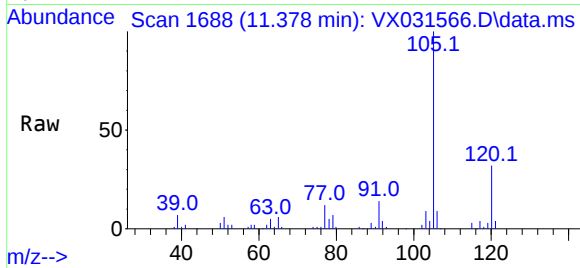

#80
1,3,5-Trimethylbenzene
Concen: 3.934 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 105 Resp: 12203
Ion Ratio Lower Upper
105 100
120 48.7 24.5 73.5


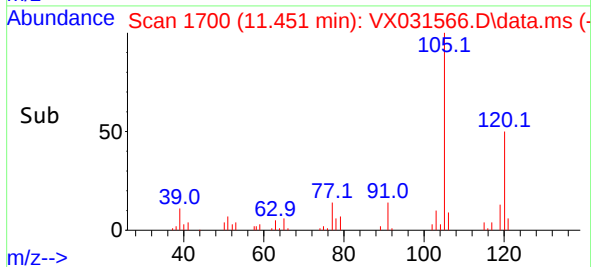

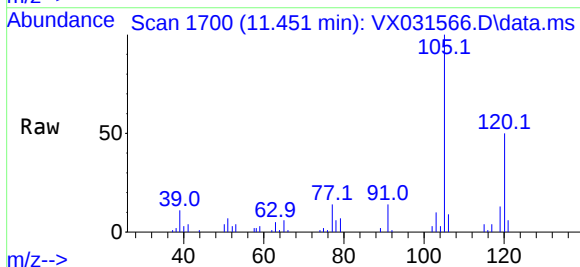




#81
trans-1,4-Dichloro-2-butene
Concen: 127.923 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 75 Resp: 43397
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

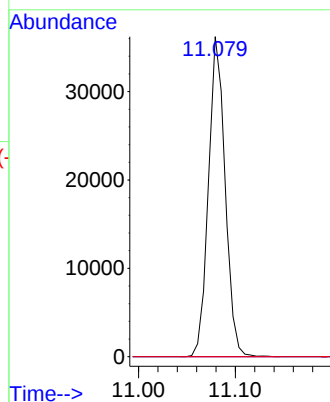

#82
4-Chlorotoluene
Concen: 0.562 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 91 Resp: 1650
Ion Ratio Lower Upper
91 100
126 3.4 15.1 45.3#


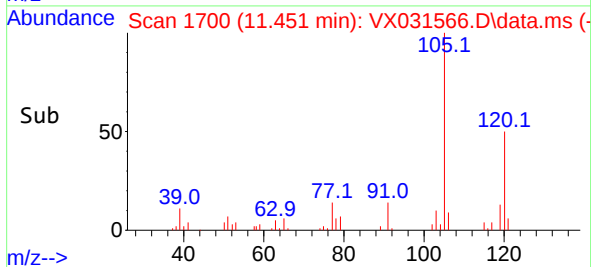
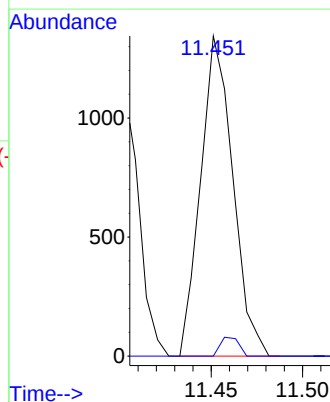
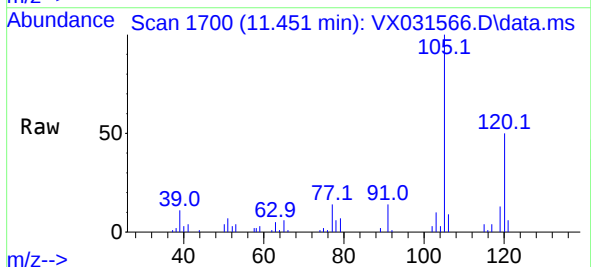




#83
tert-Butylbenzene
Concen: 2.345 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. 0.031 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:119 Resp: 7049
Ion Ratio Lower Upper
119 100
91 89.5 29.2 87.6#
134 0.0 11.6 34.8#

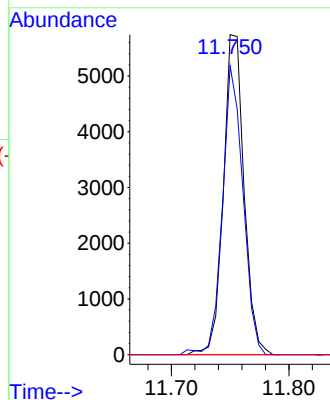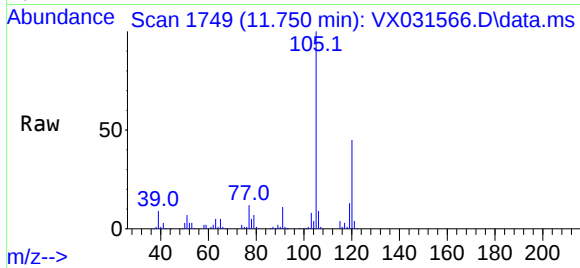

#84
1,2,4-Trimethylbenzene
Concen: 18.459 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion:105 Resp: 56383
Ion Ratio Lower Upper
105 100
120 46.9 22.6 67.8


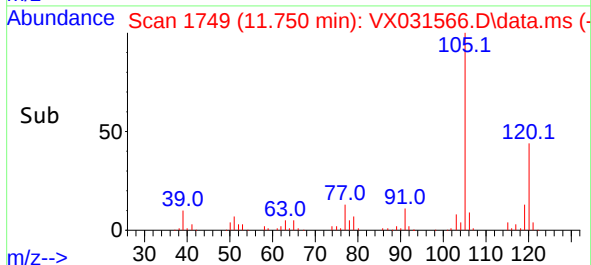
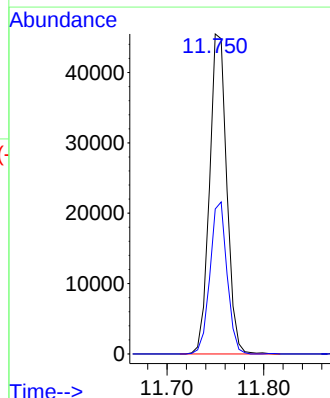
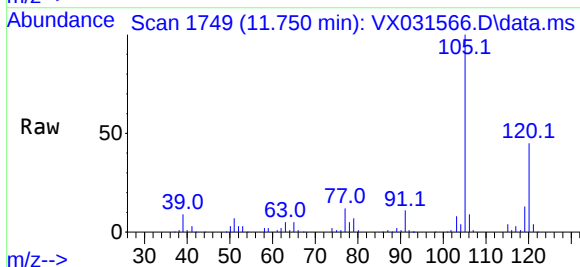




#85
 sec-Butylbenzene
 Concen: 14.821 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX031566.D
 Acq: 22 Sep 2022 13:37




Instrument :
 MSVOA_X
 ClientSampleId :
 CLI-0620DL


Tgt Ion:105 Resp: 56383
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

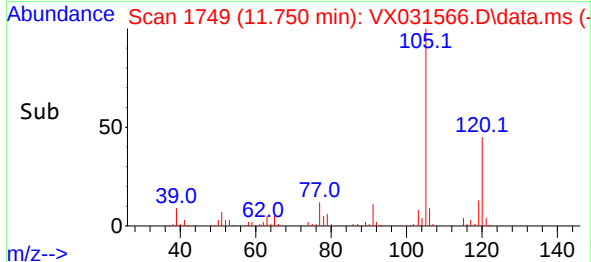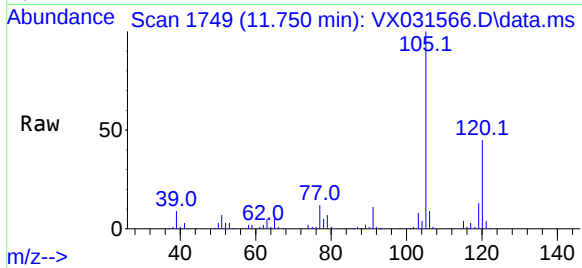

#86
 p-Isopropyltoluene
 Concen: 0.271 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. -0.043 min
 Lab File: VX031566.D
 Acq: 22 Sep 2022 13:37

Tgt Ion:119 Resp: 870
 Ion Ratio Lower Upper
 119 100
 134 26.2 13.4 40.2
 91 22.5 12.4 37.2


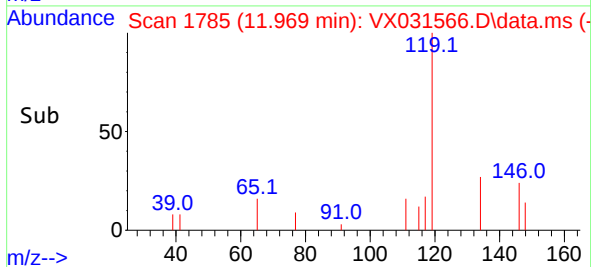

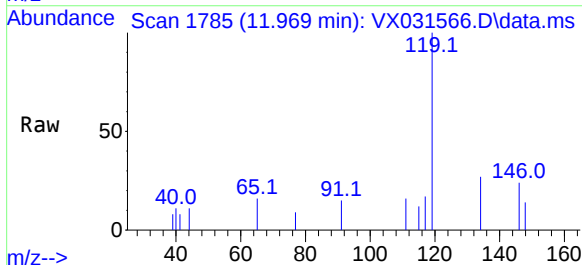




#89
n-Butylbenzene
Concen: 0.692 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion: 91 Resp: 1894
Ion Ratio Lower Upper
91 100
92 21.6 27.0 81.0#
134 95.3 13.3 39.9#

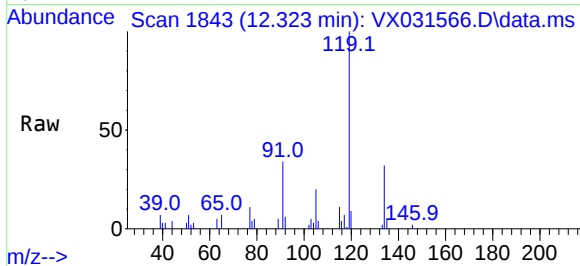

#90
Hexachloroethane
Concen: 0.790 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.012 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion: 117 Resp: 436
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#


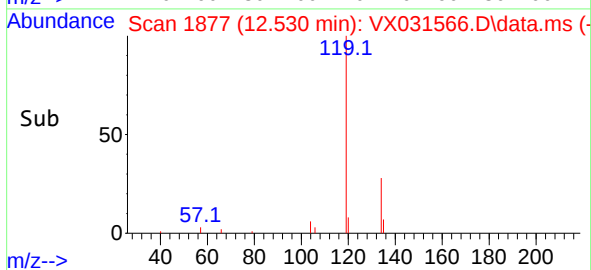

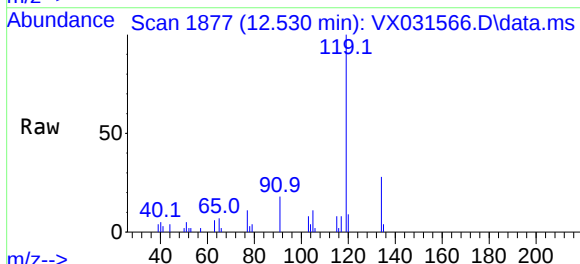




#94
Hexachlorobutadiene
Concen: Below Cal
RT: 13.719 min Scan# 2072
Delta R.T. -0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37




Instrument :
MSVOA_X
ClientSampleId :
CLI-0620DL


Tgt Ion:225 Resp: 211
Ion Ratio Lower Upper
225 100
223 34.6 30.8 92.4
227 28.0 32.3 96.9#

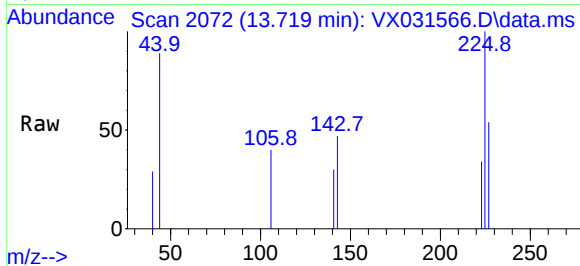

#95
Naphthalene
Concen: 11.713 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX031566.D
Acq: 22 Sep 2022 13:37

Tgt Ion:128 Resp: 41094
Ion Ratio Lower Upper
128 100
127 12.1 10.4 15.6
129 10.8 8.8 13.2

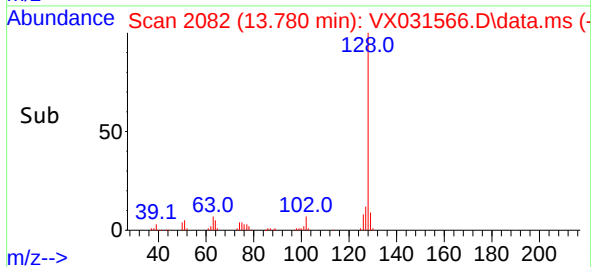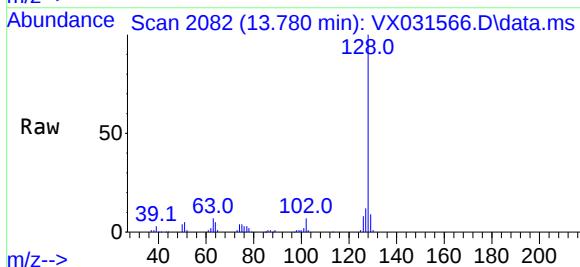



#96

1,2,3-Trichlorobenzene

Concen: 0.240 ug/l

RT: 13.963 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX031566.D


Acq: 22 Sep 2022 13:37

Instrument :

MSVOA_X

ClientSampleId :

CLI-0620DL

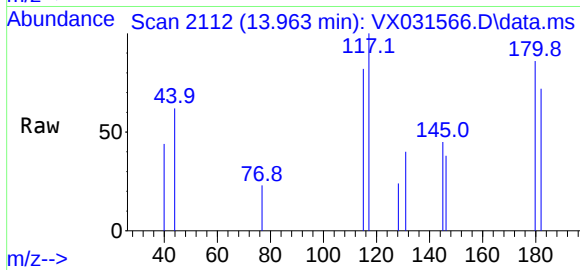

Tgt Ion:180 Resp: 237

Ion Ratio Lower Upper

180 100

182 73.8 47.9 143.8

145 43.5 17.6 52.8

