

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031570.D
 Acq On : 22 Sep 2022 15:11
 Operator : JC/MD
 Sample : N4642-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11R

Quant Time: Sep 23 01:49:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	70210	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	116715	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	108668	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	50949	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	71448	55.504	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery	=	111.000%	
35) Dibromofluoromethane	5.385	113	61232	50.768	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery	=	101.540%	
50) Toluene-d8	8.653	98	233967	50.315	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery	=	100.640%	
62) 4-Bromofluorobenzene	11.079	95	73464	46.641	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery	=	93.280%	
Target Compounds						Qvalue
5) Bromomethane	1.617	94	563	0.259	ug/l	83
6) Chloroethane	1.691	64	270	Below Cal	#	43
11) Tert butyl alcohol	2.989	59	1308	Below Cal	#	73
13) Acrolein	2.337	56	1339	Below Cal	#	70
14) Allyl chloride	2.776	41	2030	1.139	ug/l #	64
16) Acetone	2.392	43	479	Below Cal		99
18) Methyl Acetate	2.788	43	3850	2.001	ug/l #	52
20) Methylene Chloride	2.788	84	50	Below Cal	#	64
31) Cyclohexane	5.556	56	1802	0.944	ug/l #	40
36) 1,1-Dichloropropene	5.550	75	5752	3.100	ug/l #	49
38) Carbon Tetrachloride	5.556	117	6882	3.347	ug/l #	17
40) Benzene	6.031	78	3400	0.614	ug/l	92
43) Isopropyl Acetate	6.251	43	1231	0.362	ug/l #	61
48) Methyl methacrylate	7.769	41	389	0.250	ug/l #	73
51) 4-Methyl-2-Pentanone	8.653	43	1235	0.564	ug/l #	1
55) 1,1,2-Trichloroethane	9.104	97	1483	0.997	ug/l #	18
67) Ethyl Benzene	10.201	91	1553	0.262	ug/l #	83
73) Isopropylbenzene	10.963	105	8193	2.153	ug/l	98
75) 1,1,2,2-Tetrachloroethane	11.268	83	123	Below Cal	#	25
76) 1,2,3-Trichloropropane	11.079	75	42465	37.344	ug/l #	37
78) n-propylbenzene	11.305	91	3818	0.872	ug/l	96
79) 2-Chlorotoluene	11.305	91	3818	1.465	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.079	75	42465	120.243	ug/l #	11
82) 4-Chlorotoluene	11.305	91	3818	1.249	ug/l #	44
85) sec-Butylbenzene	11.890	105	3502	0.884	ug/l #	67
86) p-Isopropyltoluene	11.975	119	816	0.244	ug/l	97
89) n-Butylbenzene	12.311	91	1607	0.564	ug/l #	2
90) Hexachloroethane	12.646	117	3953	6.879	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	13.170	75	298	1.140	ug/l #	3
95) Naphthalene	13.780	128	1321	0.362	ug/l #	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Sep 23 01:49:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion:168 Resp: 70210
Ion Ratio Lower Upper
168 100
99 50.2 48.8 73.2





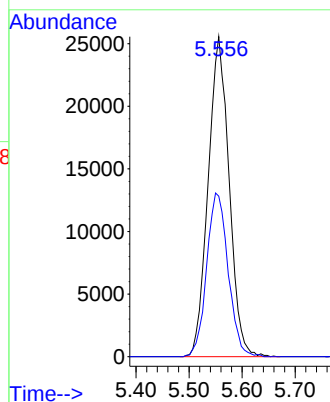
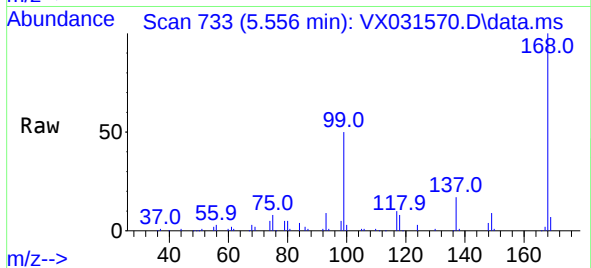


#5
Bromomethane
Concen: 0.259 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 94 Resp: 563
Ion Ratio Lower Upper
94 100
96 109.3 74.4 111.6

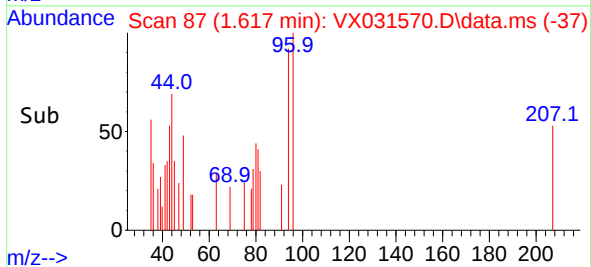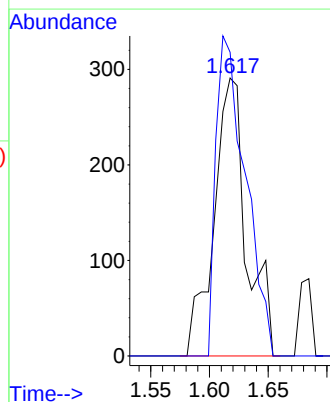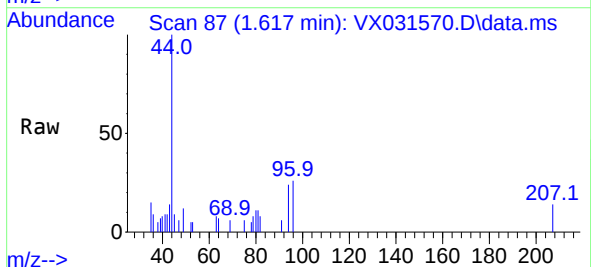


Abundance Scan 98 (1.685 min): VX031454.D\data.ms (-92)

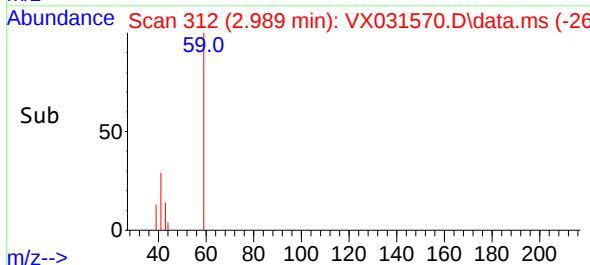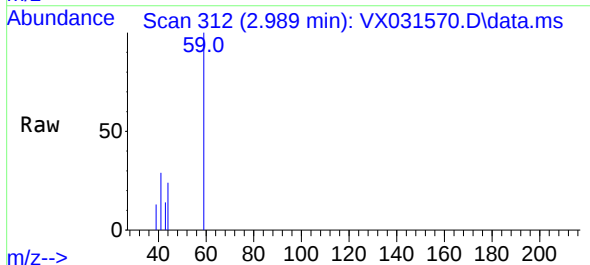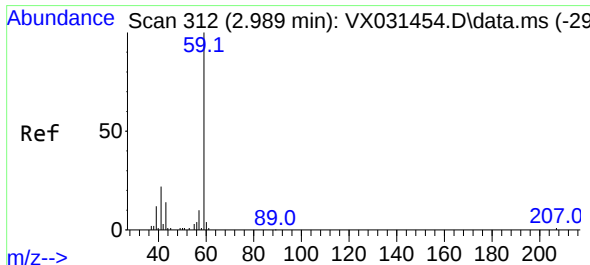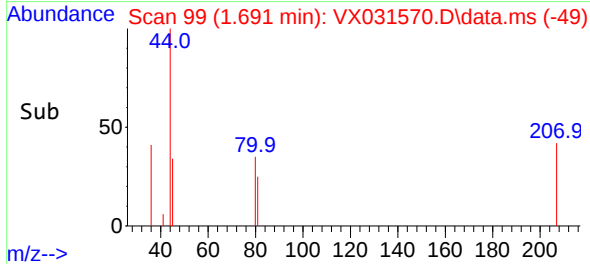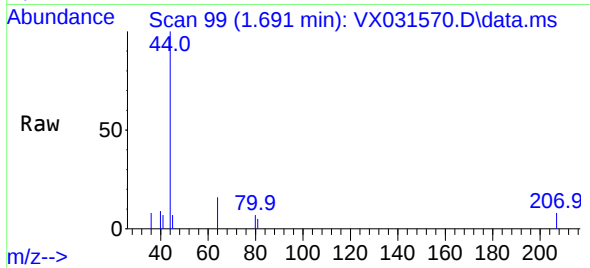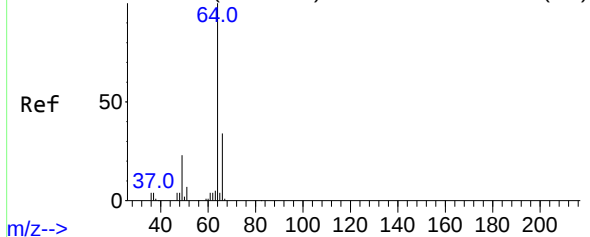

#6
Chloroethane
Concen: Below Cal
RT: 1.691 min Scan# 99
Delta R.T. 0.006 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11


Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 64 Resp: 270
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

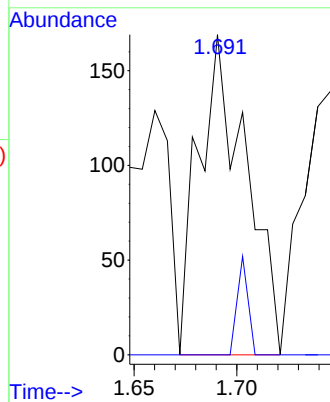

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.989 min Scan# 312
Delta R.T. 0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 59 Resp: 1308
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#




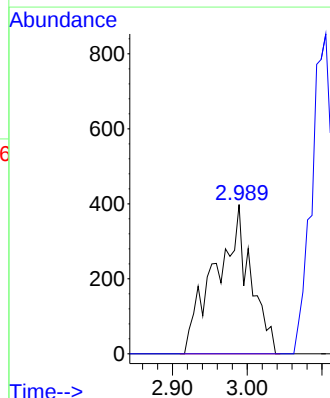




#13
Acrolein
Concen: Below Cal
RT: 2.337 min Scan# 205
Delta R.T. 0.098 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument : MSVOA_X
ClientSampleId : MW-11R


Tgt Ion: 56 Resp: 1339
Ion Ratio Lower Upper
56 100
55 45.0 56.0 84.0#

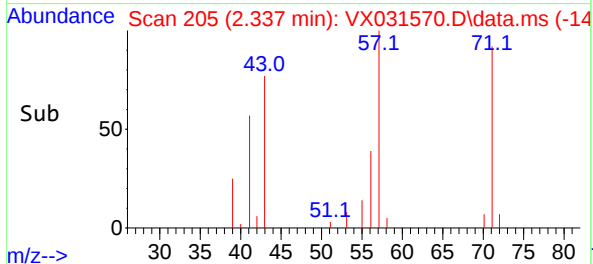

#14
Allyl chloride
Concen: 1.139 ug/l
RT: 2.776 min Scan# 277
Delta R.T. 0.110 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 41 Resp: 2030
Ion Ratio Lower Upper
41 100
39 51.9 58.2 87.4#
76 0.0 26.9 40.3#


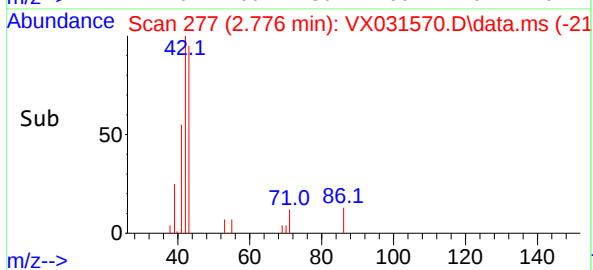

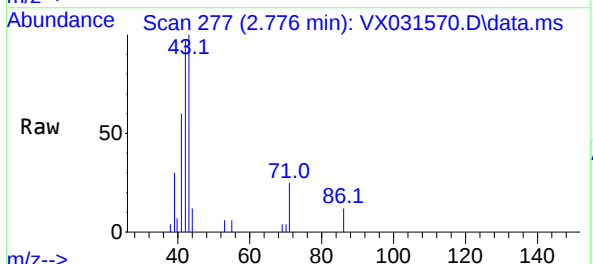




#16
Acetone
Concen: Below Cal
RT: 2.392 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 43 Resp: 479
Ion Ratio Lower Upper
43 100
58 29.3 23.8 35.8

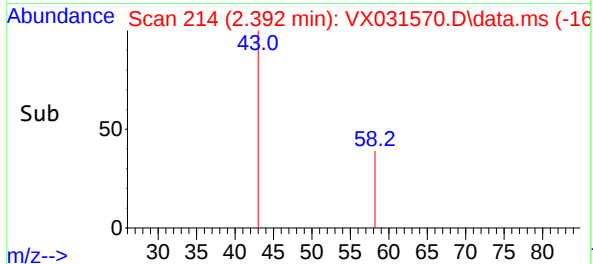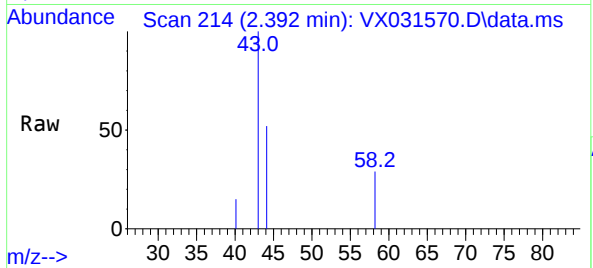

#18
Methyl Acetate
Concen: 2.001 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.079 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 43 Resp: 3850
Ion Ratio Lower Upper
43 100
74 0.0 18.6 27.8#

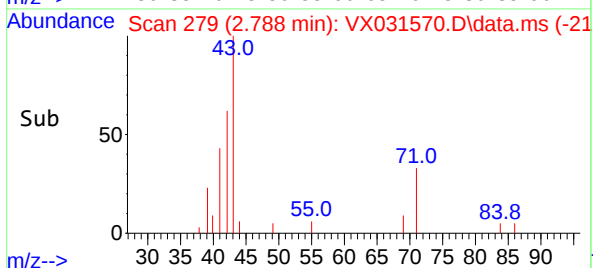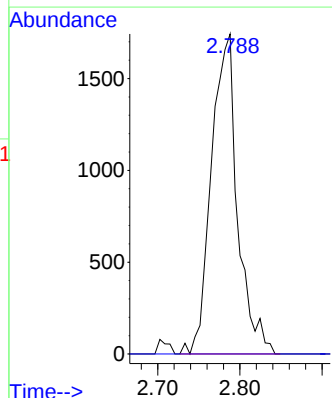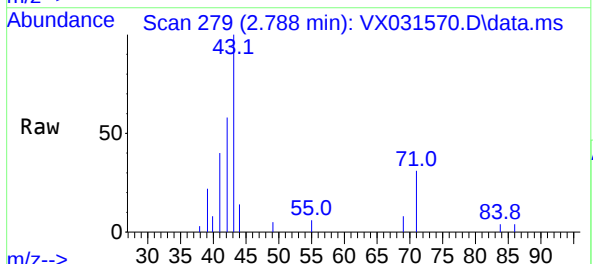



#20

Methylene Chloride

Concen: Below Cal

RT: 2.788 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11

Instrument :

MSVOA_X

ClientSampleId :

MW-11R

Tgt Ion: 84 Resp: 50





Ion Ratio Lower Upper

84 100

49 109.5 105.9 158.9

51 0.0 32.2 48.2#

86 105.4 50.8 76.2#

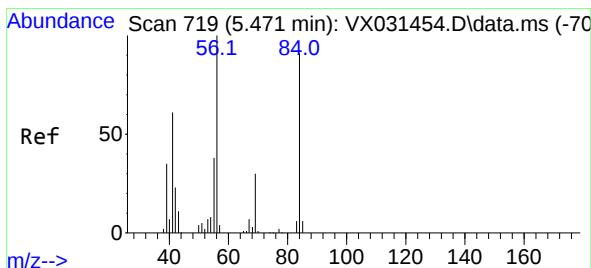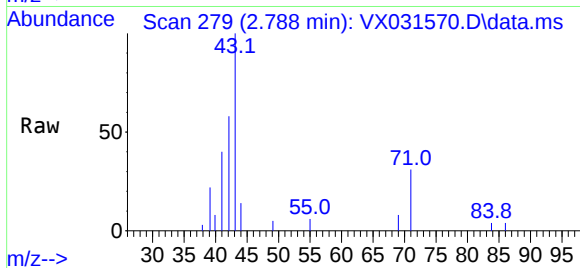

#31

Cyclohexane

Concen: 0.944 ug/l

RT: 5.556 min Scan# 733

Delta R.T. 0.085 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11




Tgt Ion: 56 Resp: 1802


Ion Ratio Lower Upper

56 100

69 79.7 25.1 37.7#

84 134.0 70.2 105.4#


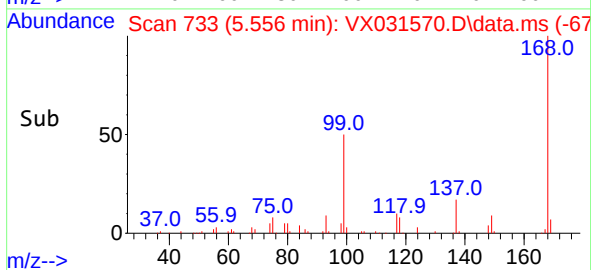

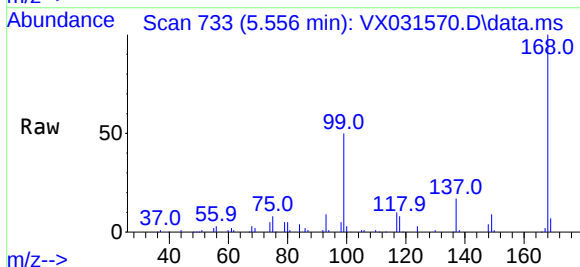




#33
1,2-Dichloroethane-d4
Concen: 55.504 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 65 Resp: 71448
Ion Ratio Lower Upper
65 100
67 51.6 0.0 102.4

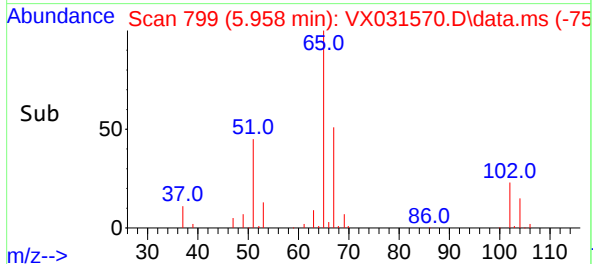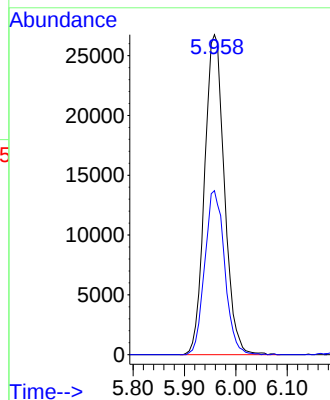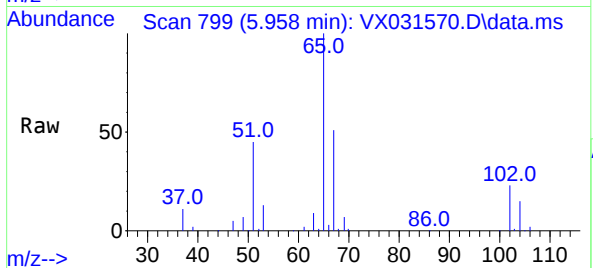

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. -0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 114 Resp: 116715
Ion Ratio Lower Upper
114 100
63 18.9 0.0 42.6
88 12.1 0.0 33.0

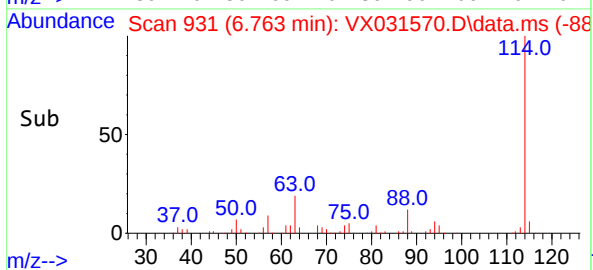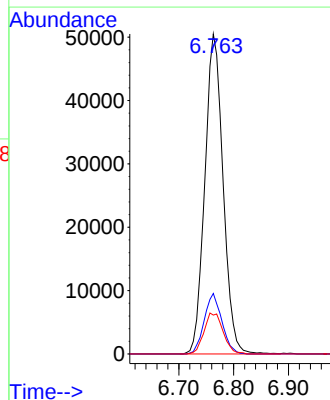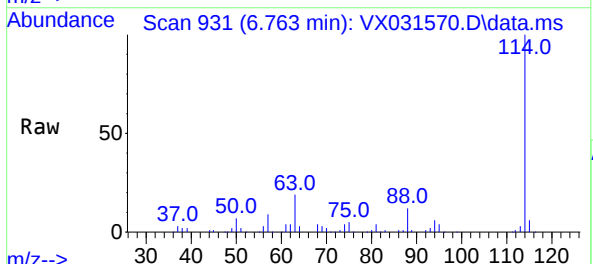

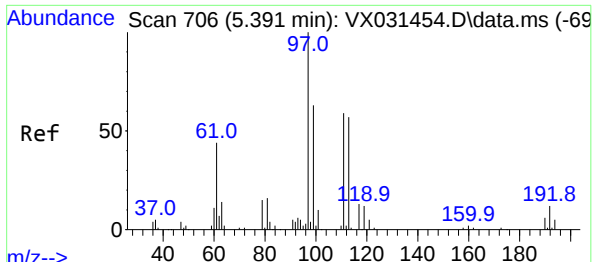

#35

Dibromofluoromethane

Concen: 50.768 ug/l

RT: 5.385 min Scan# 706

Delta R.T. -0.006 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11

Instrument :

MSVOA_X

ClientSampleId :

MW-11R





Tgt Ion:113 Resp: 61232

Ion Ratio Lower Upper

113 100

111 102.7 82.4 123.6

192 19.2 14.1 21.1

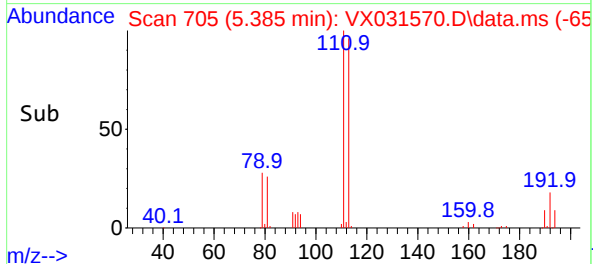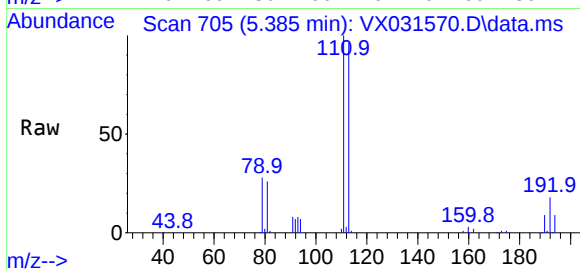

#36

1,1-Dichloropropene

Concen: 3.100 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.140 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11




Tgt Ion: 75 Resp: 5752


Ion Ratio Lower Upper

75 100

110 8.8 17.5 52.5#

77 0.0 24.9 37.3#


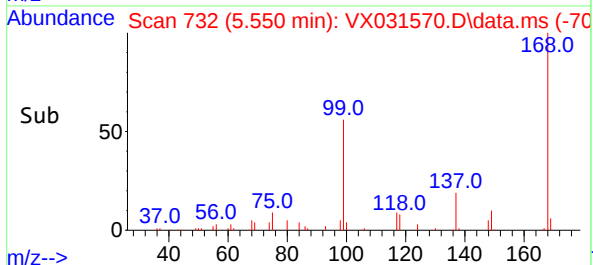
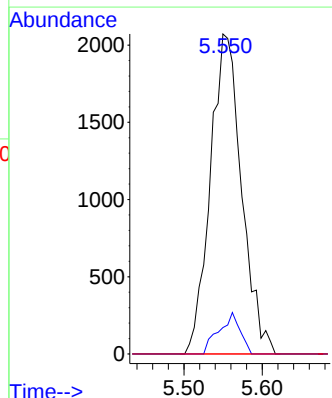
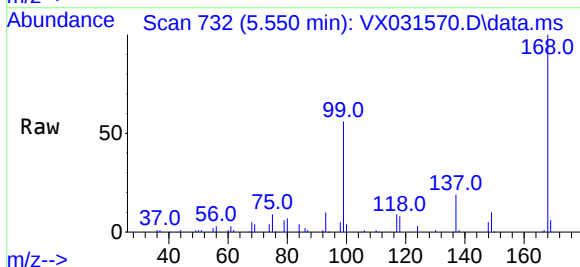




#38
Carbon Tetrachloride
Concen: 3.347 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:117 Resp: 6882
Ion Ratio Lower Upper
117 100
119 4.6 74.6 112.0#
121 0.0 25.3 37.9#

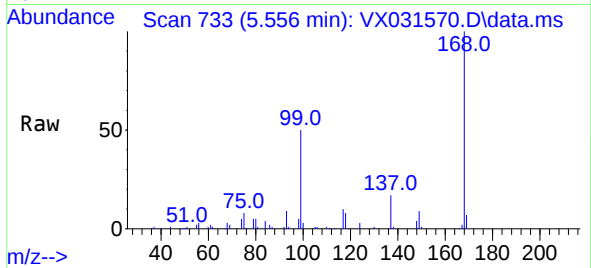

#40
Benzene
Concen: 0.614 ug/l
RT: 6.031 min Scan# 811
Delta R.T. -0.013 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 78 Resp: 3400
Ion Ratio Lower Upper
78 100
77 27.2 18.7 28.1


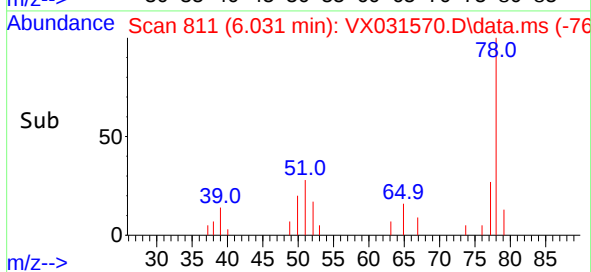






#43
Isopropyl Acetate
Concen: 0.362 ug/l
RT: 6.251 min Scan# 84
Delta R.T. -0.091 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 43 Resp: 1231
Ion Ratio Lower Upper
43 100
61 0.0 15.3 22.9#
87 0.0 10.6 15.8#

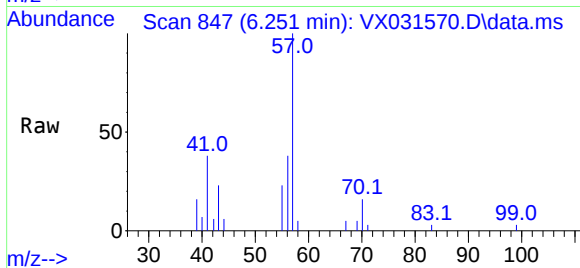

#48
Methyl methacrylate
Concen: 0.250 ug/l
RT: 7.769 min Scan# 1096
Delta R.T. 0.073 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 41 Resp: 389
Ion Ratio Lower Upper
41 100
69 51.9 64.6 96.8#
39 79.4 51.4 77.0#

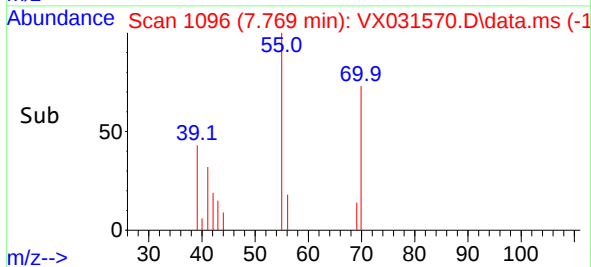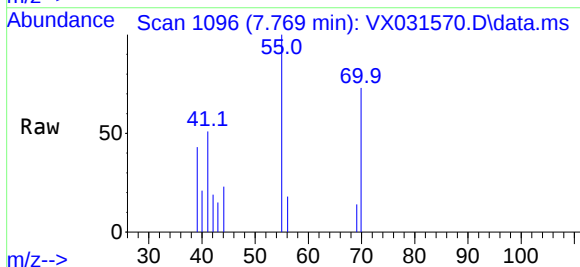



#50

Toluene-d8

Concen: 50.315 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11

Instrument :

MSVOA_X

ClientSampleId :





MW-11R

Tgt Ion: 98 Resp: 233967

Ion Ratio Lower Upper

98 100

100 65.1 52.5 78.7

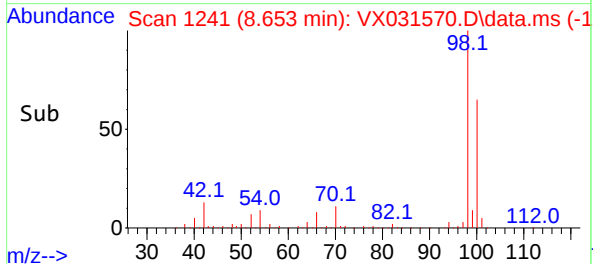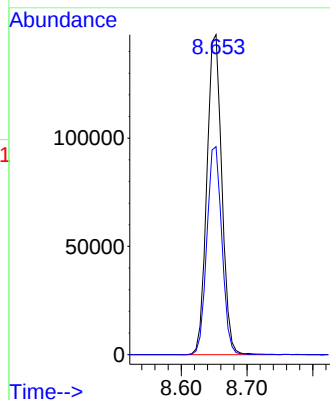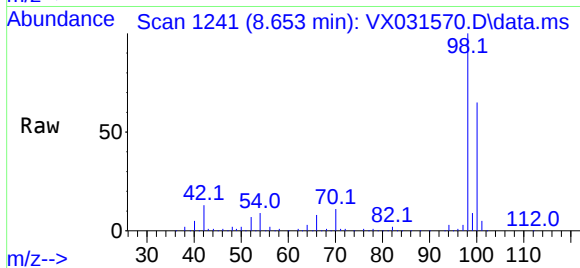

#51

4-Methyl-2-Pentanone

Concen: 0.564 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. 0.073 min

Lab File: VX031570.D




Acq: 22 Sep 2022 15:11


Tgt Ion: 43 Resp: 1235

Ion Ratio Lower Upper

43 100

58 153.3 30.6 46.0#

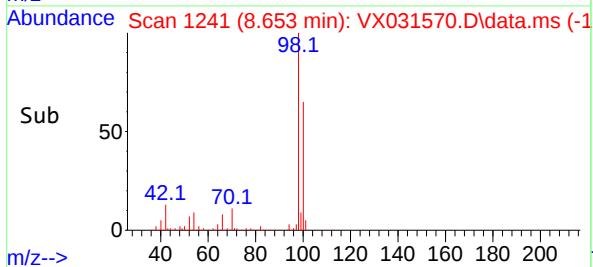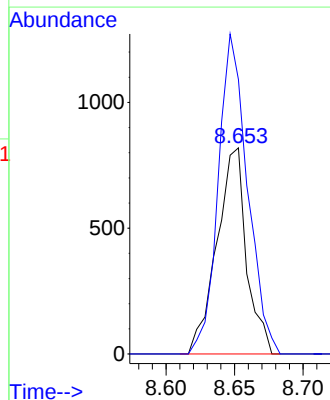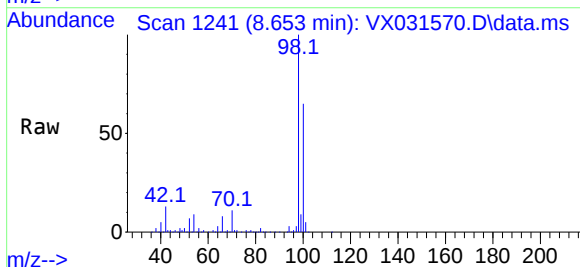







#55
1,1,2-Trichloroethane
Concen: 0.997 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion: 97 Resp: 1483




Ion	Ratio	Lower	Upper
97	100		
83	7.3	69.0	103.6#
85	0.0	44.1	66.1#
99	0.0	51.3	76.9#

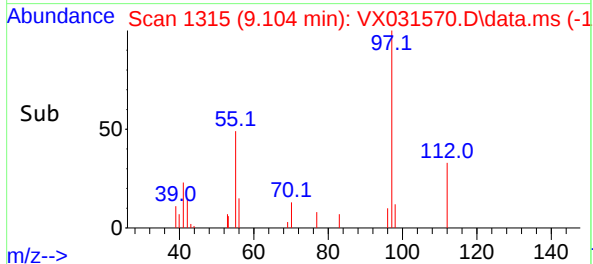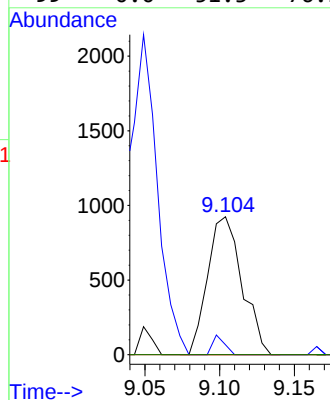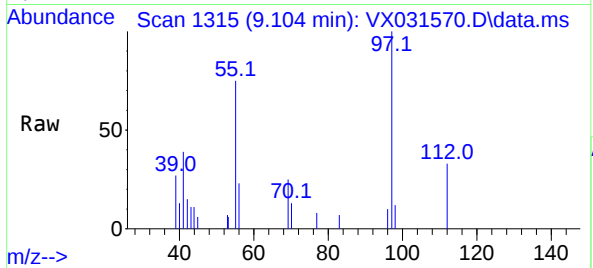


#62
4-Bromofluorobenzene
Concen: 46.641 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 95 Resp: 73464

Ion	Ratio	Lower	Upper
95	100		
174	92.7	0.0	153.2
176	89.6	0.0	144.0


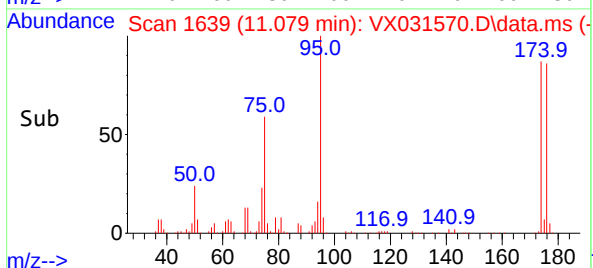
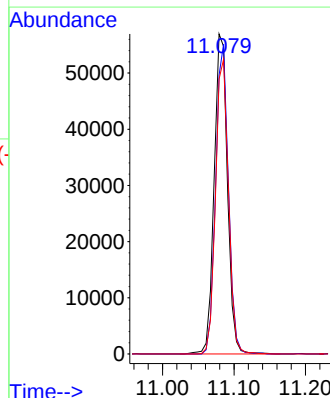
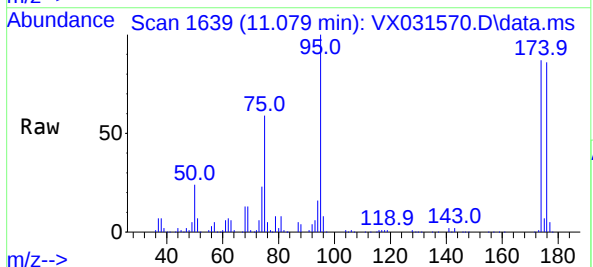




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:117 Resp: 108668
Ion Ratio Lower Upper
117 100
82 51.4 46.8 70.2
119 31.8 26.4 39.6

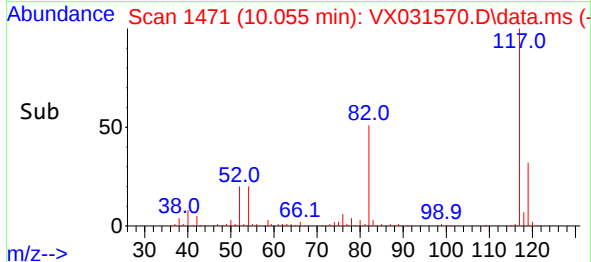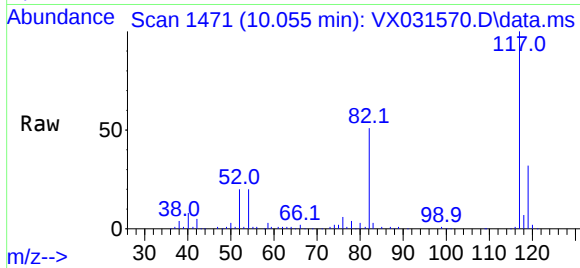

#67
Ethyl Benzene
Concen: 0.262 ug/l
RT: 10.201 min Scan# 1495
Delta R.T. 0.006 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 91 Resp: 1553
Ion Ratio Lower Upper
91 100
106 22.1 25.2 37.8#


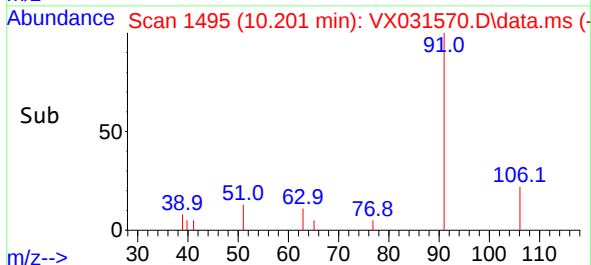
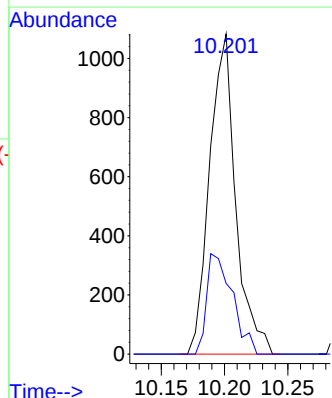
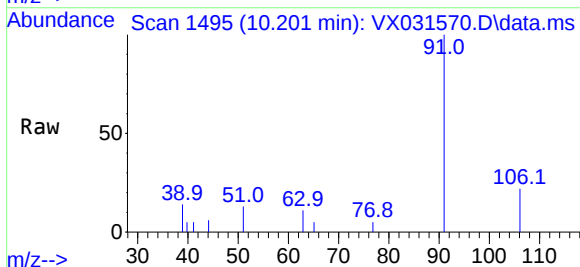




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion:152 Resp: 50949
Ion Ratio Lower Upper
152 100
115 55.3 43.4 130.1
150 156.2 0.0 346.8

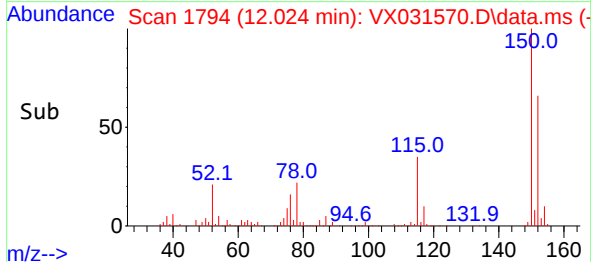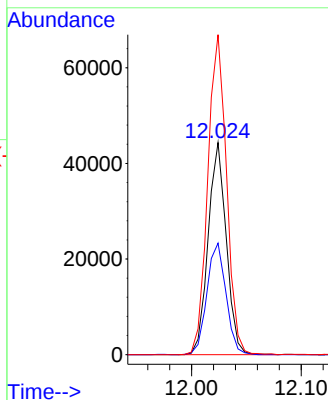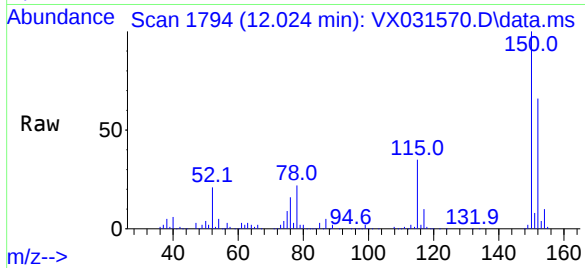

#73
Isopropylbenzene
Concen: 2.153 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion:105 Resp: 8193
Ion Ratio Lower Upper
105 100
120 28.4 13.7 41.0


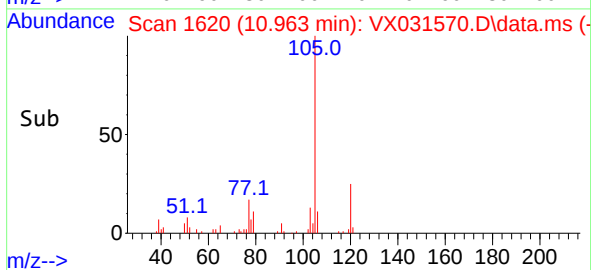
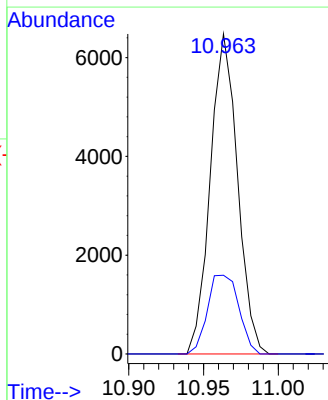
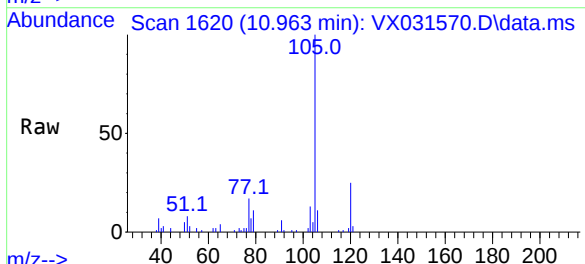




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.268 min Scan# 1639
Delta R.T. 0.055 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 83 Resp: 123
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.4#
85 0.0 32.6 97.8#



#76
1,2,3-Trichloropropane
Concen: 37.344 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 75 Resp: 42465
Ion Ratio Lower Upper
75 100
77 1.3 20.3 60.9#


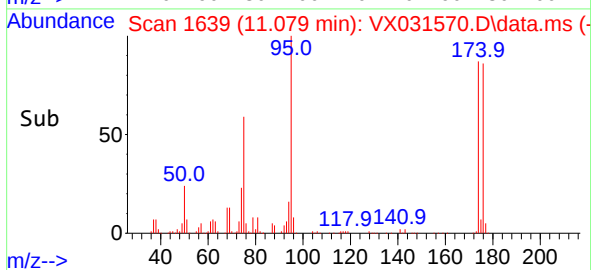






#78
n-propylbenzene
Concen: 0.872 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 91 Resp: 3818
Ion Ratio Lower Upper
91 100
120 21.7 11.8 35.4

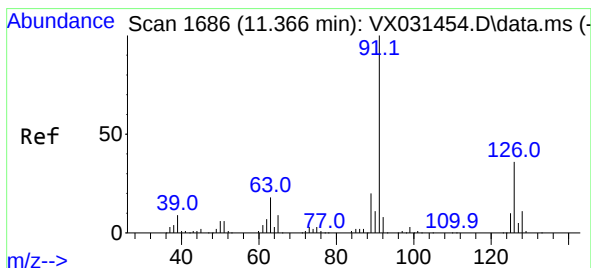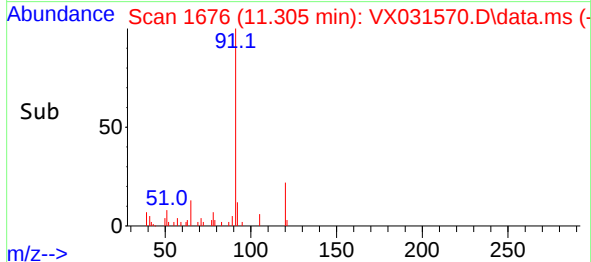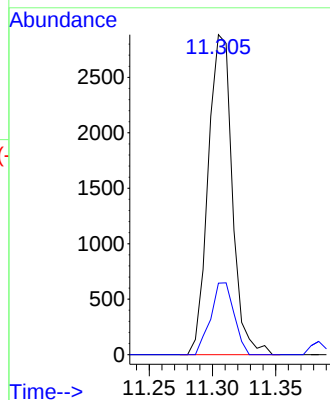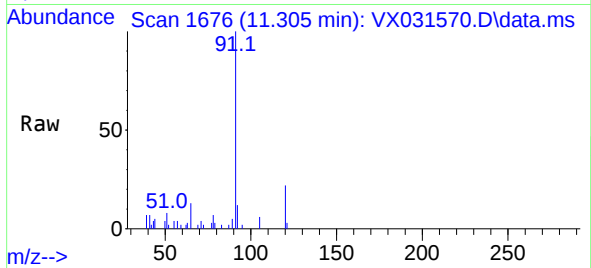

#79
2-Chlorotoluene
Concen: 1.465 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 91 Resp: 3818
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


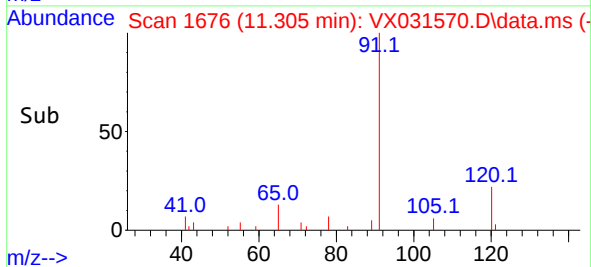
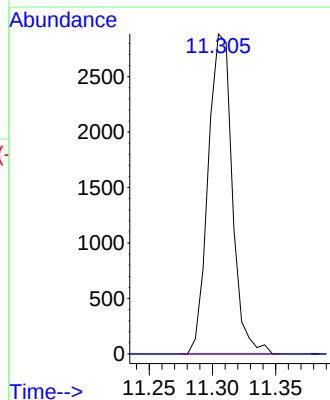
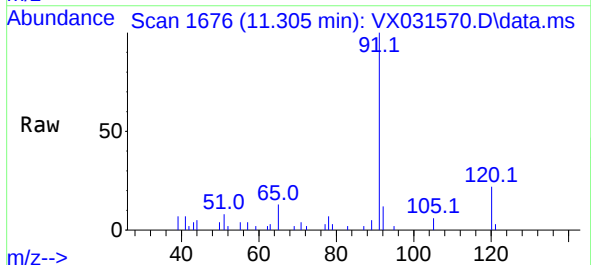




#81
trans-1,4-Dichloro-2-butene
Concen: 120.243 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11




Instrument :
MSVOA_X
ClientSampleId :
MW-11R


Tgt Ion: 75 Resp: 42465
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

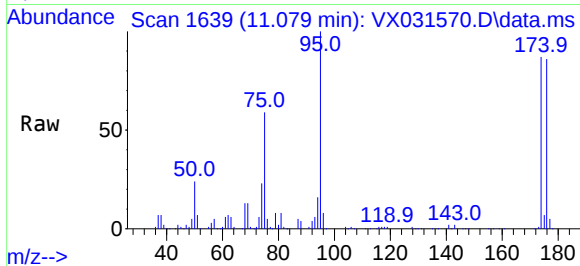

#82
4-Chlorotoluene
Concen: 1.249 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.152 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 91 Resp: 3818
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#


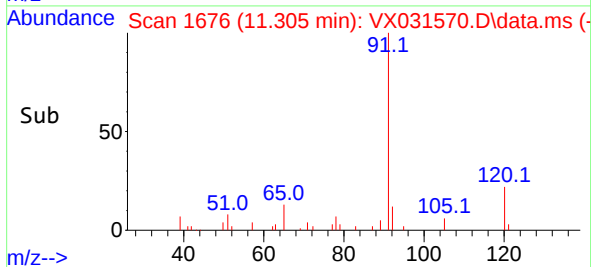

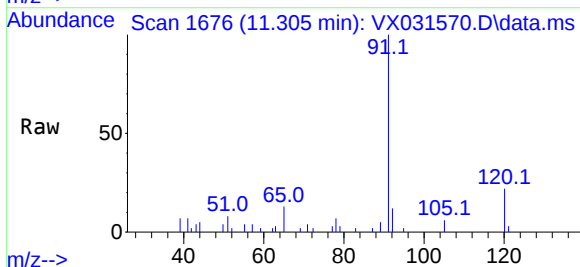




#85
 sec-Butylbenzene
 Concen: 0.884 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. -0.000 min
 Lab File: VX031570.D
 Acq: 22 Sep 2022 15:11




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-11R


Tgt Ion:105 Resp: 3502
 Ion Ratio Lower Upper
 105 100
 134 36.0 10.4 31.1#

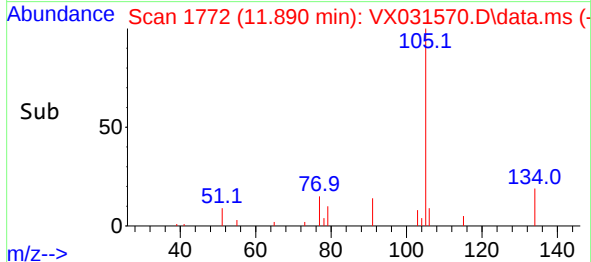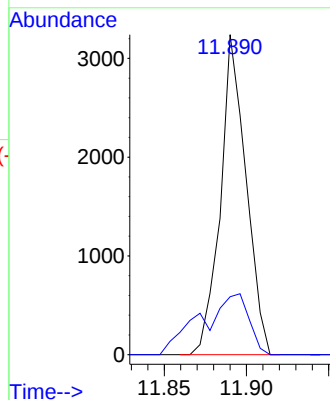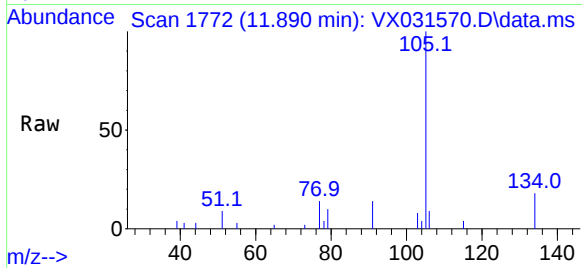

#86
 p-Isopropyltoluene
 Concen: 0.244 ug/l
 RT: 11.975 min Scan# 1786
 Delta R.T. -0.037 min
 Lab File: VX031570.D
 Acq: 22 Sep 2022 15:11

Tgt Ion:119 Resp: 816
 Ion Ratio Lower Upper
 119 100
 134 27.3 13.4 40.2
 91 27.7 12.4 37.2

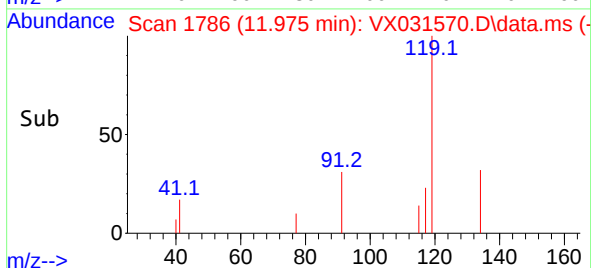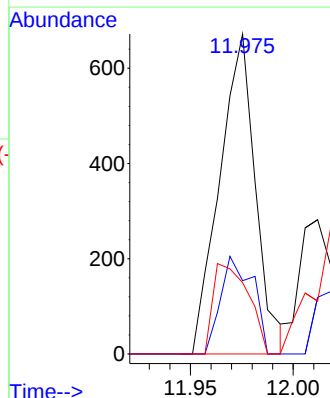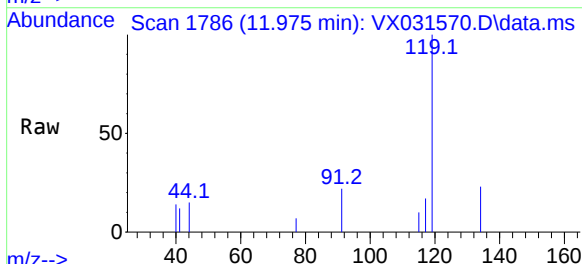



#89

n-Butylbenzene

Concen: 0.564 ug/l

RT: 12.311 min Scan# 1841

Delta R.T. -0.024 min

Lab File: VX031570.D

Acq: 22 Sep 2022 15:11

Instrument :

MSVOA_X

ClientSampleId :

MW-11R





Tgt Ion: 91 Resp: 1607

Ion Ratio Lower Upper

91 100

92 0.0 27.0 81.0#

134 101.2 13.3 39.9#

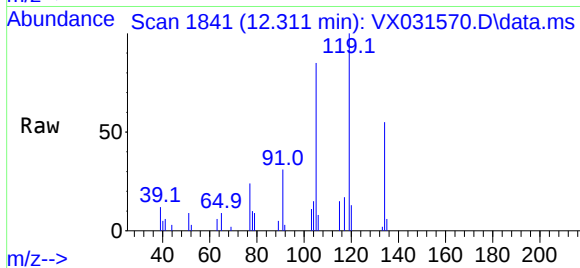

#90

Hexachloroethane

Concen: 6.879 ug/l

RT: 12.646 min Scan# 1896

Delta R.T. 0.104 min

Lab File: VX031570.D




Acq: 22 Sep 2022 15:11


Tgt Ion: 117 Resp: 3953

Ion Ratio Lower Upper

117 100

201 0.0 34.8 104.4#


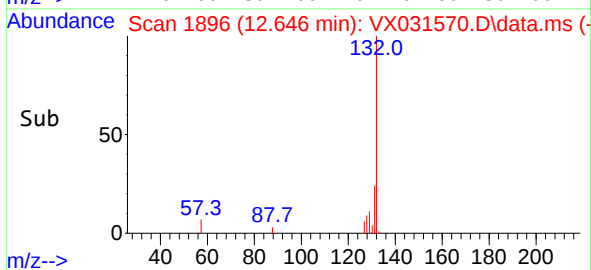

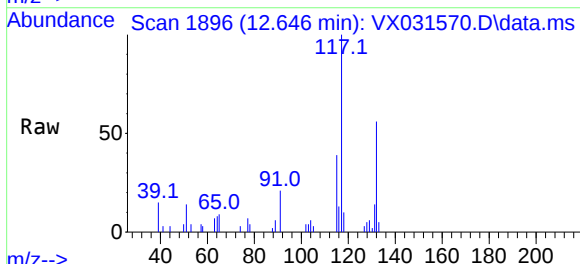




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.140 ug/l
RT: 13.170 min Scan# 1945
Delta R.T. 0.225 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Instrument :
MSVOA_X
ClientSampleId :
MW-11R

Tgt Ion: 75 Resp: 298
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.5 154.5#

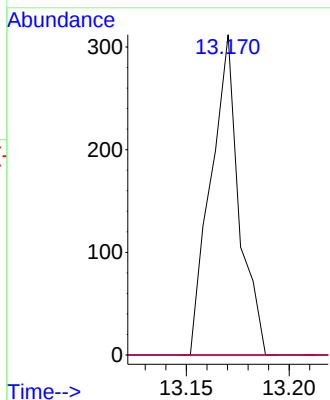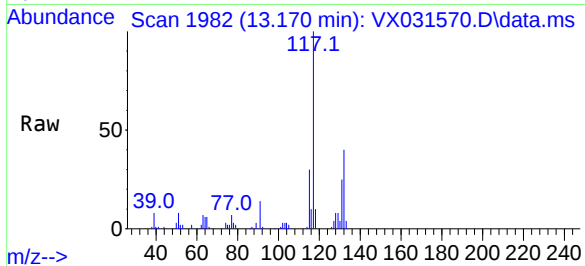

#95
Naphthalene
Concen: 0.362 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX031570.D
Acq: 22 Sep 2022 15:11

Tgt Ion: 128 Resp: 1321
Ion Ratio Lower Upper
128 100
127 7.3 10.4 15.6#
129 16.0 8.8 13.2#

