

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031596.D
 Acq On : 23 Sep 2022 02:34
 Operator : JC/MD
 Sample : N4614-06DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6RDL

Quant Time: Sep 23 04:47:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	76921	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	125903	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	112013	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	53853	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	75948	53.820	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 107.640%			
35) Dibromofluoromethane	5.385	113	64759	49.760	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.520%			
50) Toluene-d8	8.647	98	246448	49.131	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 98.260%			
62) 4-Bromofluorobenzene	11.079	95	76234	44.867	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 89.740%			
Target Compounds						Qvalue
5) Bromomethane	1.624	94	595	0.250	ug/l #	61
6) Chloroethane	1.685	64	263	Below Cal	#	43
11) Tert butyl alcohol	2.946	59	4422	Below Cal	#	73
13) Acrolein	2.215	56	132	Below Cal	#	1
14) Allyl chloride	2.788	41	1587	0.813	ug/l #	22
16) Acetone	2.392	43	608	Below Cal	#	79
19) Methyl tert-butyl Ether	3.111	73	2768	0.639	ug/l #	1
20) Methylene Chloride	2.794	84	553	Below Cal	#	70
25) 2-Butanone	4.580	43	746	0.685	ug/l #	49
31) Cyclohexane	5.470	56	4286	2.048	ug/l	98
36) 1,1-Dichloropropene	5.550	75	5903	2.950	ug/l #	52
38) Carbon Tetrachloride	5.562	117	7536	3.397	ug/l #	13
39) Methylcyclohexane	7.379	83	4448	1.806	ug/l	92
40) Benzene	6.037	78	243608	40.802	ug/l	97
42) 1,2-Dichloroethane	6.043	62	2404	1.092	ug/l #	75
48) Methyl methacrylate	7.659	41	577	0.344	ug/l #	50
52) Toluene	8.720	92	3661	0.940	ug/l	96
55) 1,1,2-Trichloroethane	9.104	97	491	0.306	ug/l #	15
67) Ethyl Benzene	10.195	91	131435	21.551	ug/l	100
68) m/p-Xylenes	10.305	106	8597	3.508	ug/l	97
69) o-Xylene	10.640	106	2273	0.972	ug/l	82
73) Isopropylbenzene	10.963	105	20746	5.159	ug/l	99
75) 1,1,2,2-Tetrachloroethane	11.280	83	28	Below Cal	#	25
76) 1,2,3-Trichloropropane	11.079	75	44347	36.896	ug/l #	37
78) n-propylbenzene	11.305	91	51624	11.158	ug/l	99
79) 2-Chlorotoluene	11.305	91	51624	18.746	ug/l #	40
80) 1,3,5-Trimethylbenzene	11.451	105	3336	0.977	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	44347	118.800	ug/l #	11
82) 4-Chlorotoluene	11.305	91	51624	15.973	ug/l #	44
84) 1,2,4-Trimethylbenzene	11.750	105	11556	3.438	ug/l	97
85) sec-Butylbenzene	11.890	105	2174	0.519	ug/l #	64
89) n-Butylbenzene	12.335	91	2619	0.870	ug/l #	68
90) Hexachloroethane	12.615	117	2132	3.510	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	13.170	75	149	0.539	ug/l #	3
95) Naphthalene	13.774	128	67442	17.469	ug/l	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031596.D
Acq On : 23 Sep 2022 02:34
Operator : JC/MD
Sample : N4614-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL

Quant Time: Sep 23 04:47:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031596.D
Acq On : 23 Sep 2022 02:34
Operator : JC/MD
Sample : N4614-06DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL

Quant Time: Sep 23 04:47:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration




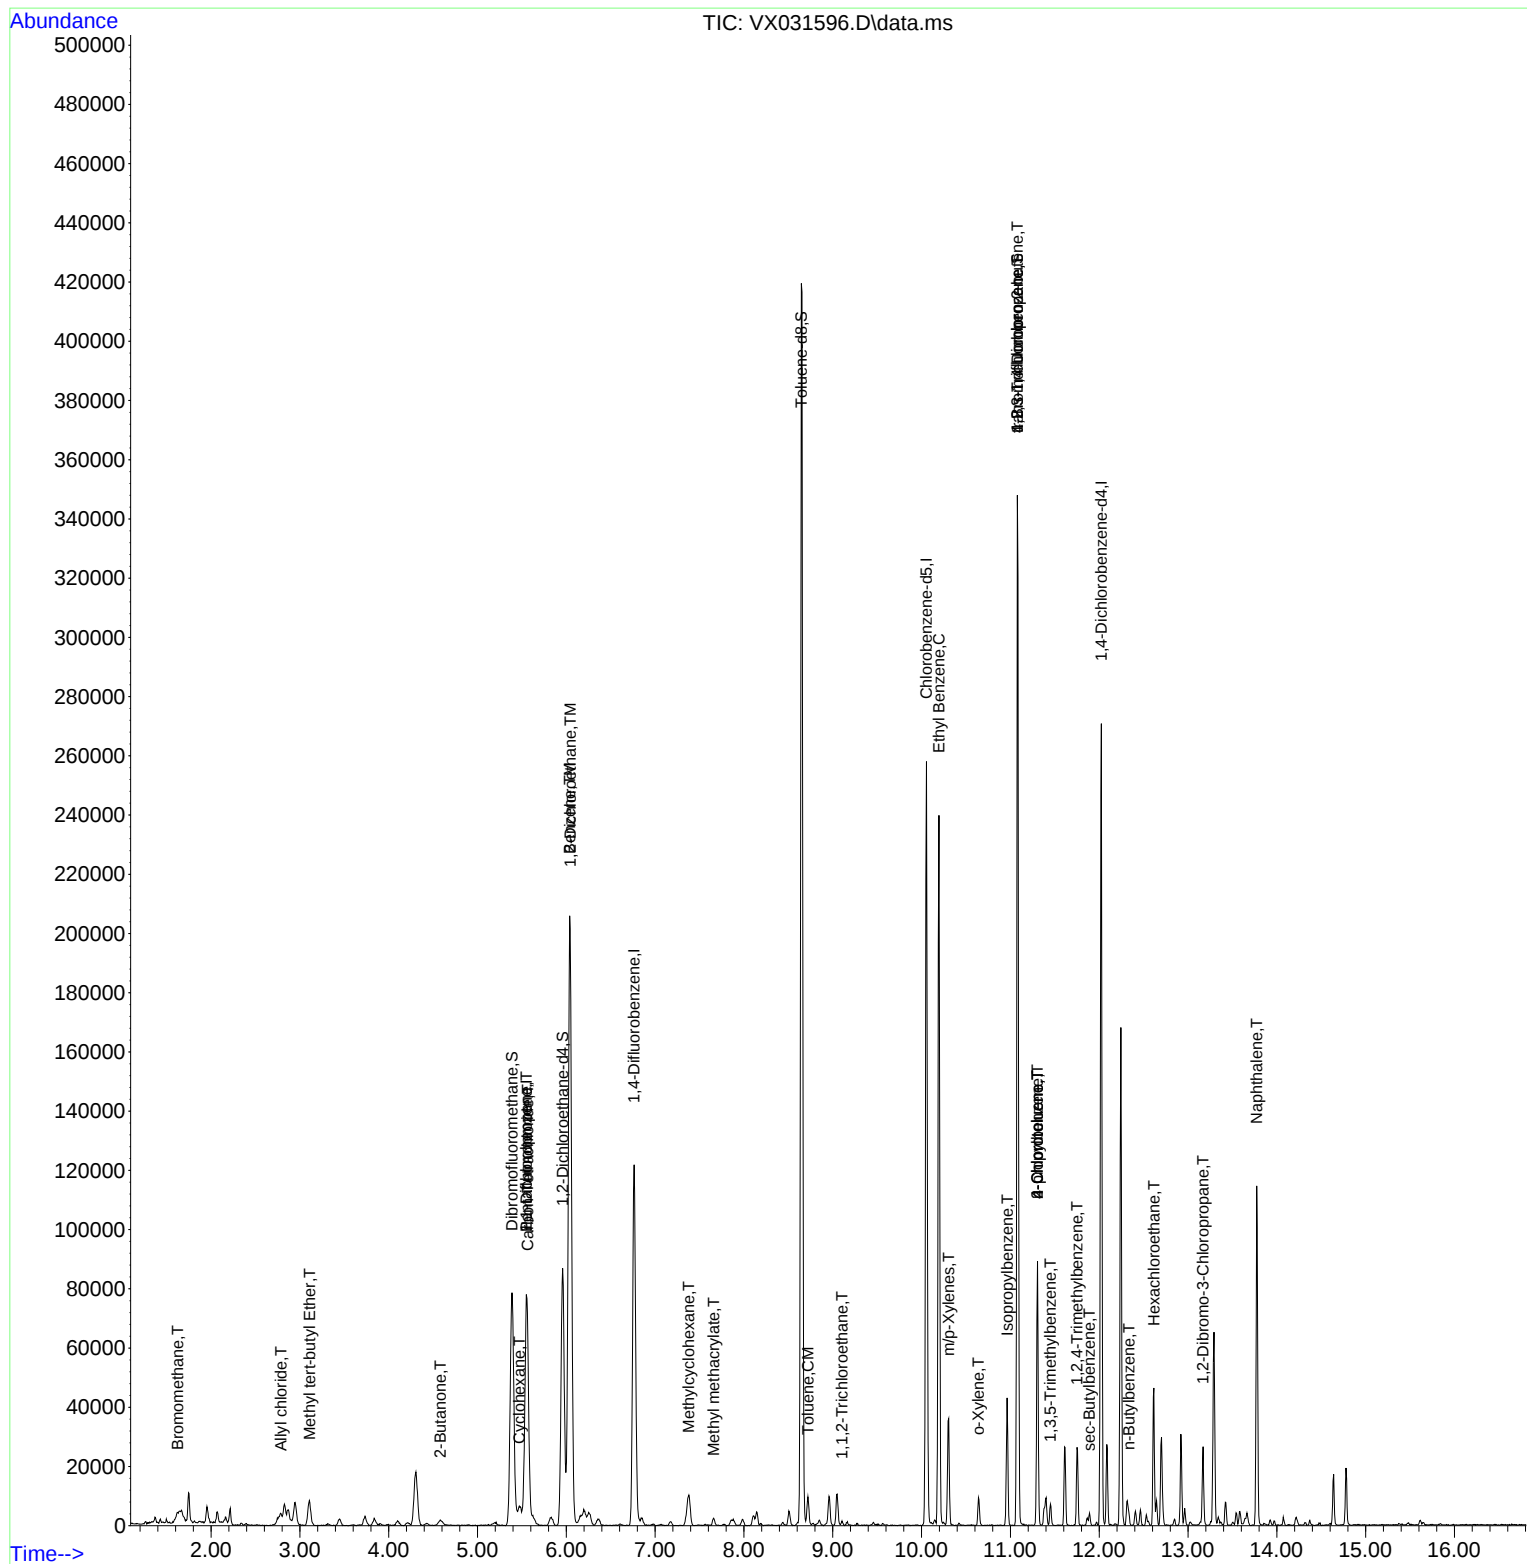




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL

Tgt Ion:168 Resp: 76921
Ion Ratio Lower Upper
168 100
99 52.5 48.8 73.2









#5
Bromomethane
Concen: 0.250 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.013 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 94 Resp: 595
Ion Ratio Lower Upper
94 100
96 56.0 74.4 111.6#

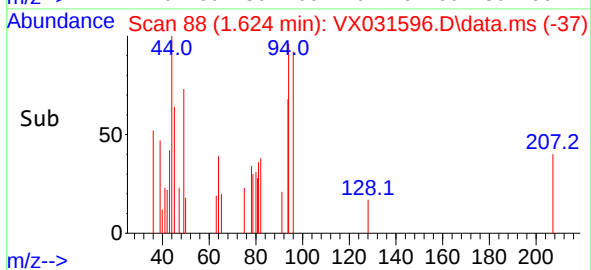


Abundance Scan 98 (1.685 min): VX031454.D\data.ms (-92)

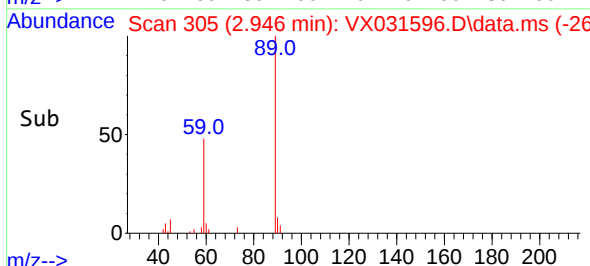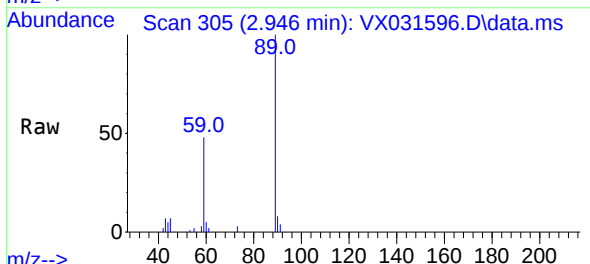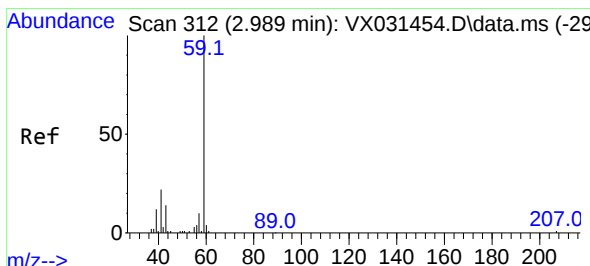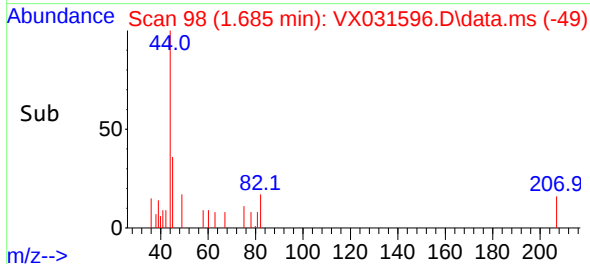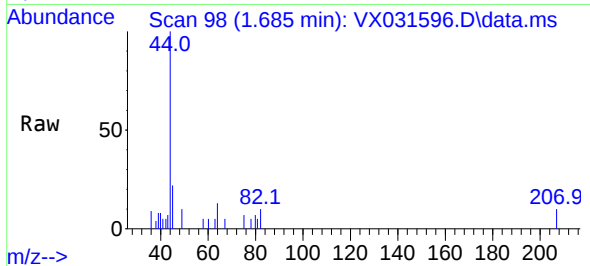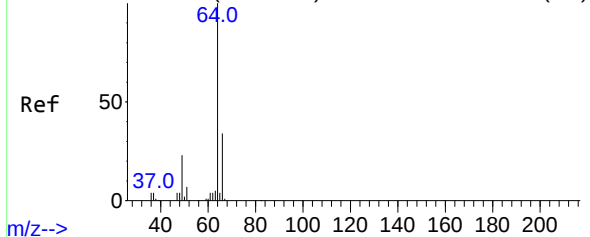

#6
Chloroethane
Concen: Below Cal
RT: 1.685 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34


Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 64 Resp: 263
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#



#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.946 min Scan# 305
Delta R.T. -0.043 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 59 Resp: 4422
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#




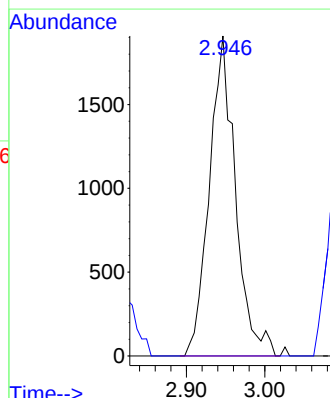




#13
Acrolein
Concen: Below Cal
RT: 2.215 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 56 Resp: 132
Ion Ratio Lower Upper
56 100
55 1672.7 56.0 84.0#

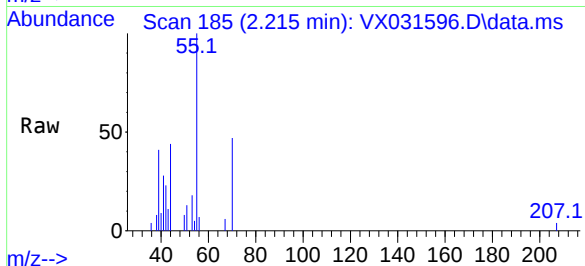

#14
Allyl chloride
Concen: 0.813 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.122 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 41 Resp: 1587
Ion Ratio Lower Upper
41 100
39 0.0 58.2 87.4#
76 0.0 26.9 40.3#


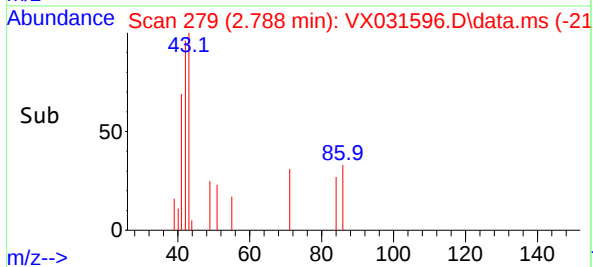

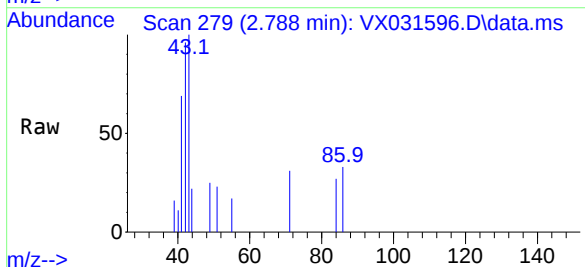




#16
Acetone
Concen: Below Cal
RT: 2.392 min Scan# 213
Delta R.T. 0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 43 Resp: 608
Ion Ratio Lower Upper
43 100
58 41.0 23.8 35.8#

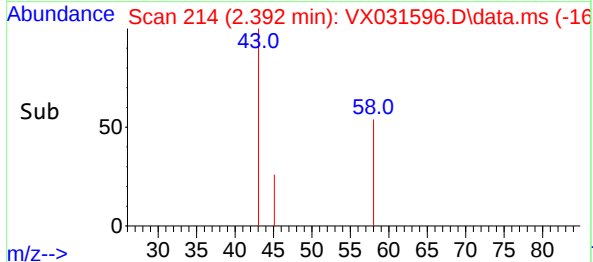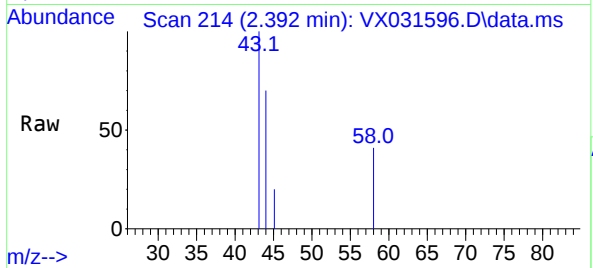

#19
Methyl tert-butyl Ether
Concen: 0.639 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 73 Resp: 2768
Ion Ratio Lower Upper
73 100
57 135.5 17.2 25.8#


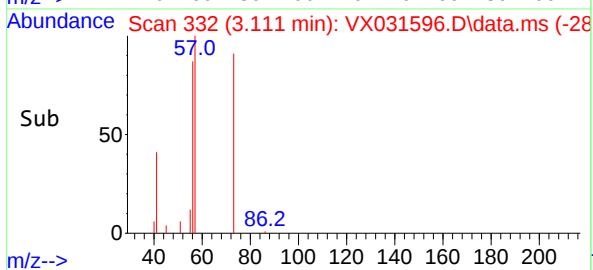






#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 84 Resp: 553
Ion Ratio Lower Upper
84 100
49 77.0 105.9 158.9#
51 47.4 32.2 48.2
86 60.2 50.8 76.2



#25
2-Butanone
Concen: 0.685 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 43 Resp: 746
Ion Ratio Lower Upper
43 100
72 0.0 21.1 31.7#


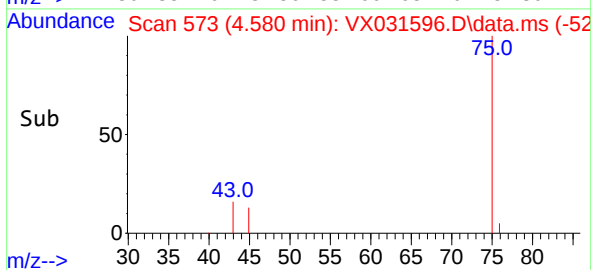






#31
Cyclohexane
Concen: 2.048 ug/l
RT: 5.470 min Scan# 719
Delta R.T. -0.001 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 56 Resp: 4286
Ion Ratio Lower Upper
56 100
69 29.5 25.1 37.7
84 88.9 70.2 105.4

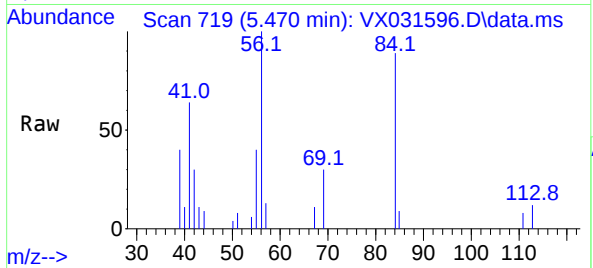

#33
1,2-Dichloroethane-d4
Concen: 53.820 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 65 Resp: 75948
Ion Ratio Lower Upper
65 100
67 52.4 0.0 102.4


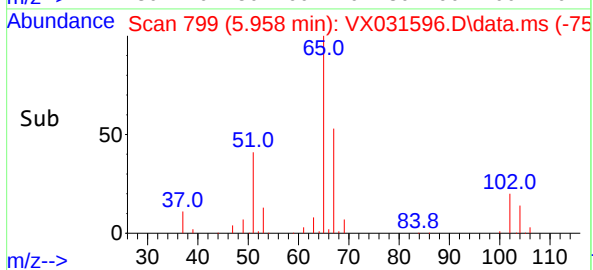






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:114 Resp: 125903
Ion Ratio Lower Upper
114 100
63 18.4 0.0 42.6
88 14.0 0.0 33.0

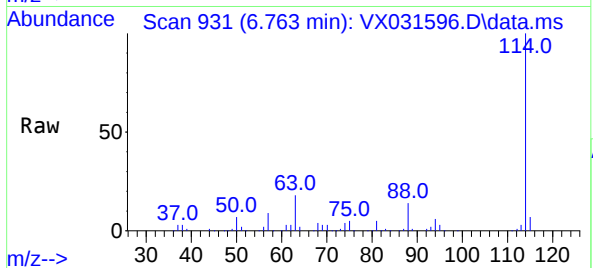

#35
Dibromofluoromethane
Concen: 49.760 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion:113 Resp: 64759
Ion Ratio Lower Upper
113 100
111 102.3 82.4 123.6
192 19.5 14.1 21.1

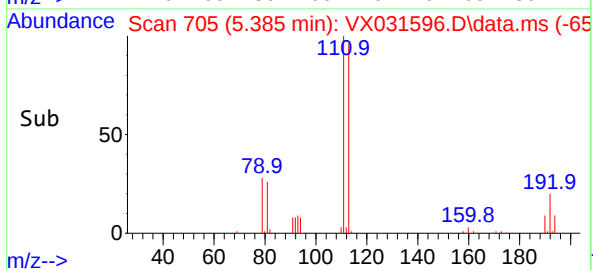



#36

1,1-Dichloropropene

Concen: 2.950 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.140 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34

Instrument :

MSVOA_X

ClientSampleId :

MW-6RDL





Tgt Ion: 75 Resp: 5903

Ion Ratio Lower Upper

75 100

110 11.3 17.5 52.5#

77 0.0 24.9 37.3#

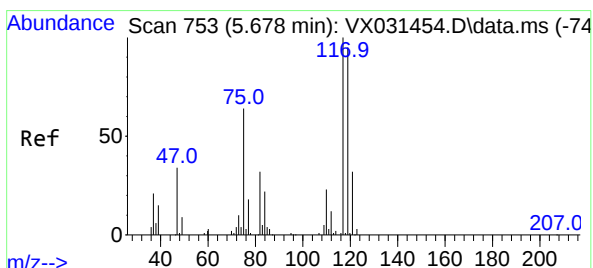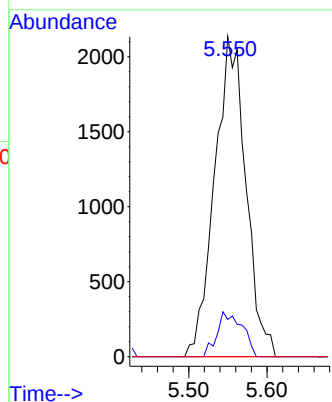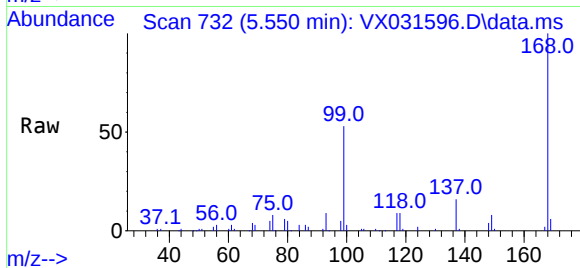

#38

Carbon Tetrachloride

Concen: 3.397 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.116 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34




Tgt Ion: 117 Resp: 7536


Ion Ratio Lower Upper

117 100

119 0.0 74.6 112.0#

121 0.0 25.3 37.9#

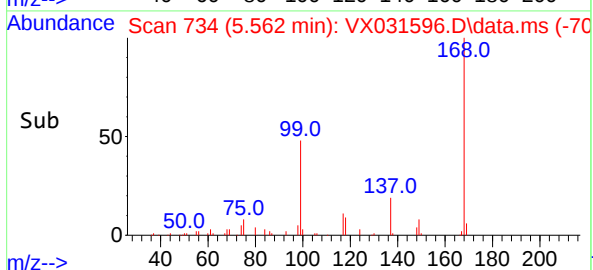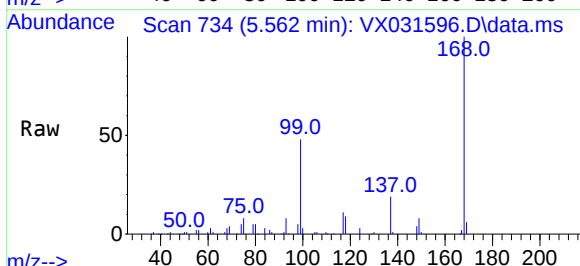



#39

Methylcyclohexane

Concen: 1.806 ug/l

RT: 7.379 min Scan# 10

Delta R.T. -0.006 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34

Instrument :

MSVOA_X

ClientSampleId :

MW-6RDL





Tgt Ion: 83 Resp: 4448

Ion Ratio Lower Upper

83 100

55 83.6 61.0 91.4

98 51.0 37.7 56.5

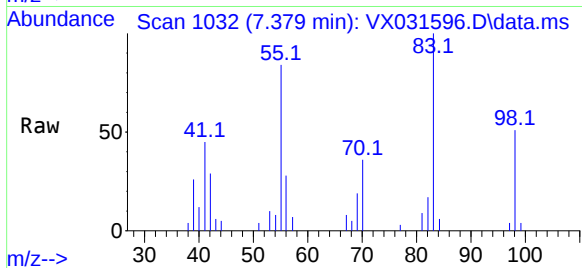

#40

Benzene

Concen: 40.802 ug/l

RT: 6.037 min Scan# 812

Delta R.T. -0.007 min

Lab File: VX031596.D




Acq: 23 Sep 2022 02:34


Tgt Ion: 78 Resp: 243608

Ion Ratio Lower Upper

78 100

77 24.9 18.7 28.1

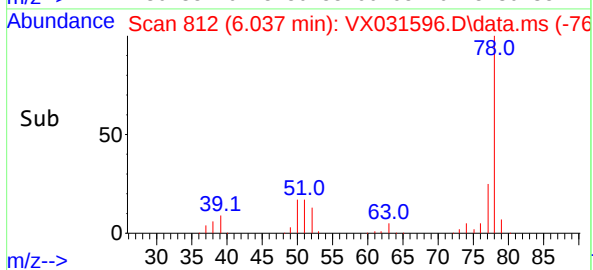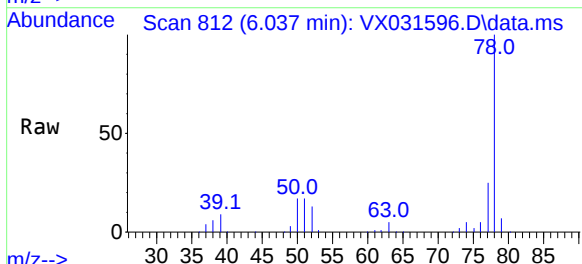



#42

1,2-Dichloroethane

Concen: 1.092 ug/l

RT: 6.043 min Scan# 81

Delta R.T. -0.049 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34

Instrument :

MSVOA_X

ClientSampleId :





MW-6RDL

Tgt Ion: 62 Resp: 2404

Ion Ratio Lower Upper

62 100

98 0.0 0.0 17.8

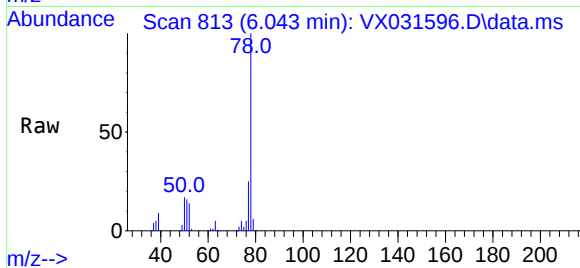

#48

Methyl methacrylate

Concen: 0.344 ug/l

RT: 7.659 min Scan# 1078

Delta R.T. -0.037 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34




Tgt Ion: 41 Resp: 577


Ion Ratio Lower Upper

41 100

69 139.9 64.6 96.8#

39 41.4 51.4 77.0#

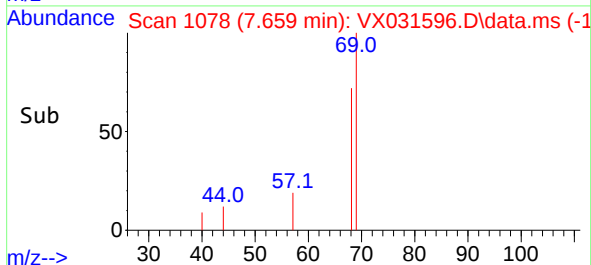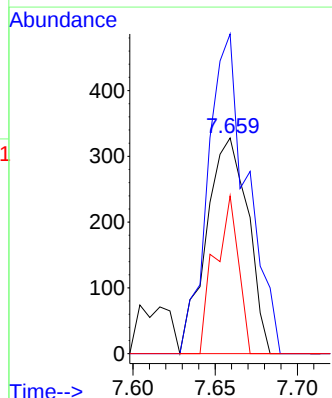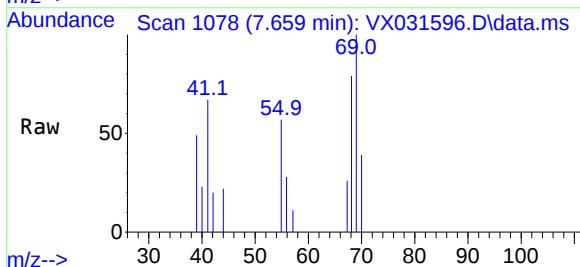



#50

Toluene-d8

Concen: 49.131 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX031596.D

Acq: 23 Sep 2022 02:34

Instrument :

MSVOA_X

ClientSampleId :





MW-6RDL

Tgt Ion: 98 Resp: 246448

Ion Ratio Lower Upper

98 100

100 64.8 52.5 78.7

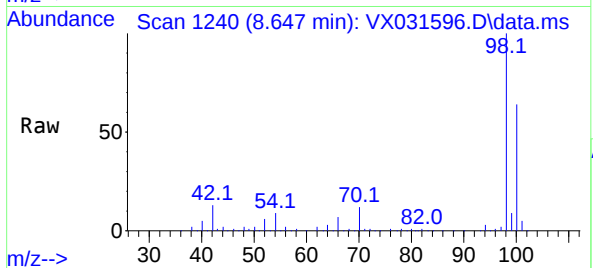

#52

Toluene

Concen: 0.940 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX031596.D




Acq: 23 Sep 2022 02:34


Tgt Ion: 92 Resp: 3661

Ion Ratio Lower Upper

92 100

91 165.5 137.1 205.7

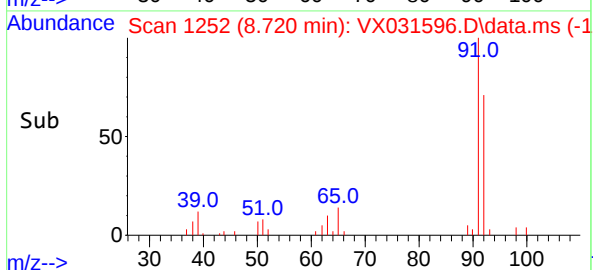







#55
1,1,2-Trichloroethane
Concen: 0.306 ug/l
RT: 9.104 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL

Tgt Ion: 97 Resp: 491




Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.0	103.6#
85	0.0	44.1	66.1#
99	0.0	51.3	76.9#

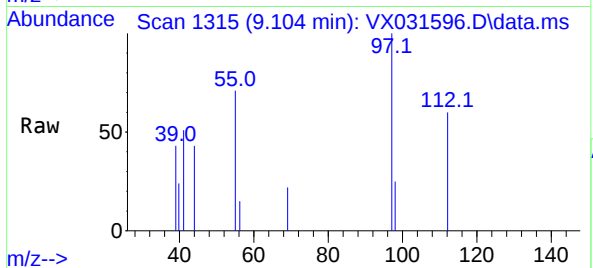


#62
4-Bromofluorobenzene
Concen: 44.867 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 95 Resp: 76234

Ion	Ratio	Lower	Upper
95	100		
174	92.7	0.0	153.2
176	90.7	0.0	144.0


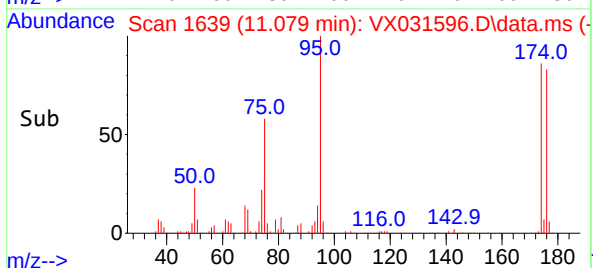
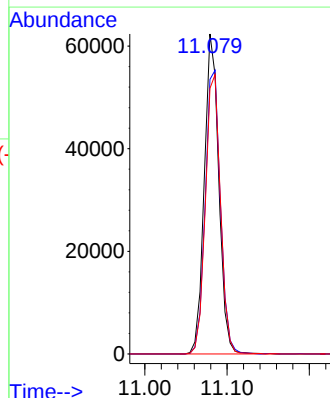





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:117 Resp: 112013
Ion Ratio Lower Upper
117 100
82 51.2 46.8 70.2
119 32.6 26.4 39.6

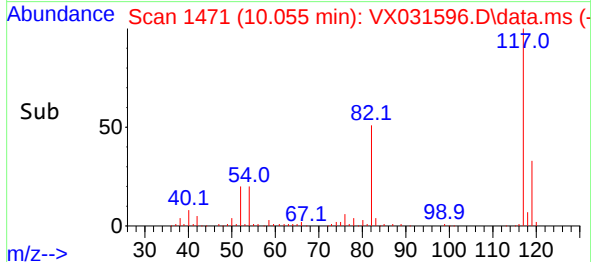

#67
Ethyl Benzene
Concen: 21.551 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 91 Resp: 131435
Ion Ratio Lower Upper
91 100
106 31.6 25.2 37.8


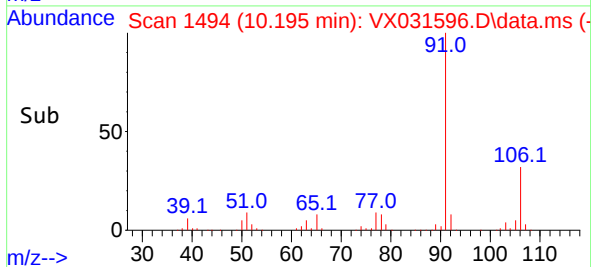

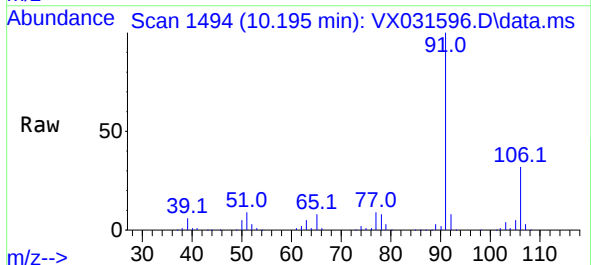




#68
m/p-Xylenes
Concen: 3.508 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:106 Resp: 8597
Ion Ratio Lower Upper
106 100
91 197.4 161.0 241.4

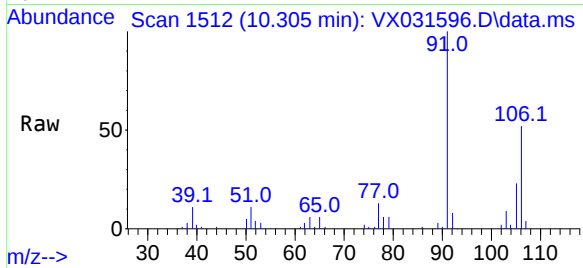

#69
o-Xylene
Concen: 0.972 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion:106 Resp: 2273
Ion Ratio Lower Upper
106 100
91 186.7 107.2 321.6


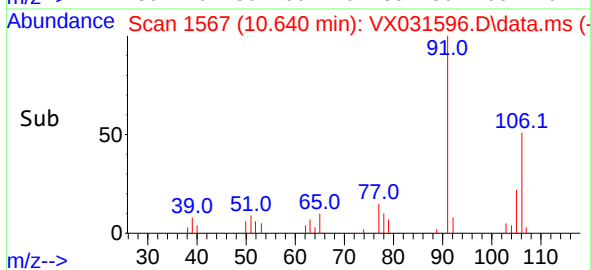

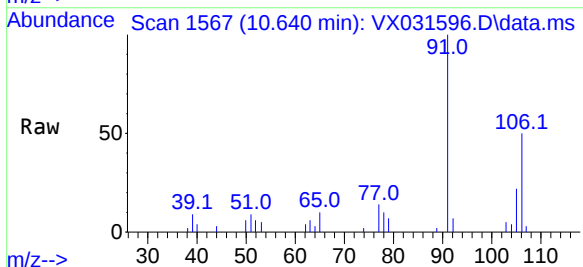




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:152 Resp: 53853
Ion Ratio Lower Upper
152 100
115 55.1 43.4 130.1
150 157.1 0.0 346.8

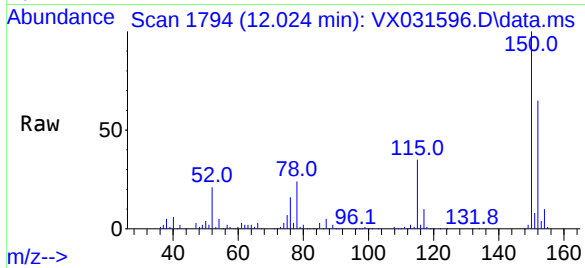

#73
Isopropylbenzene
Concen: 5.159 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion:105 Resp: 20746
Ion Ratio Lower Upper
105 100
120 27.7 13.7 41.0


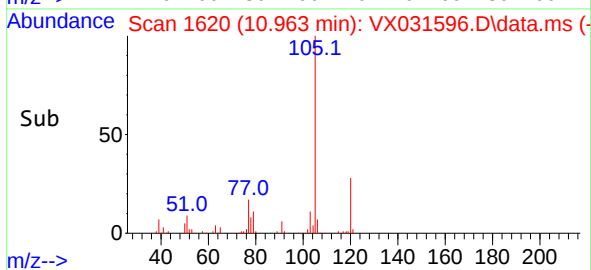

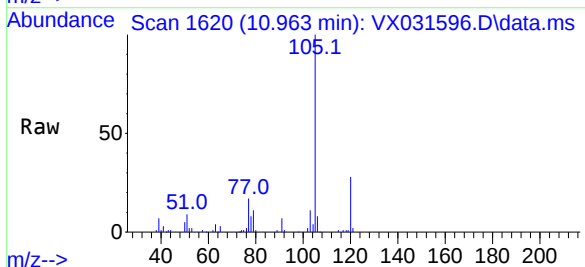




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.280 min Scan# 1639
Delta R.T. 0.067 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 83 Resp: 28
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.4#
85 0.0 32.6 97.8#

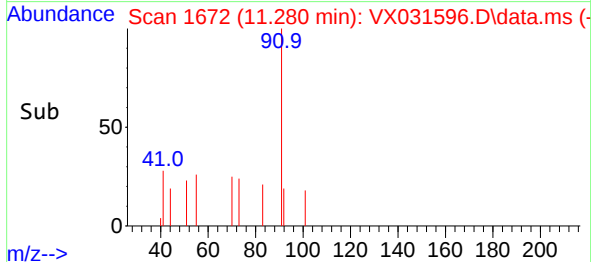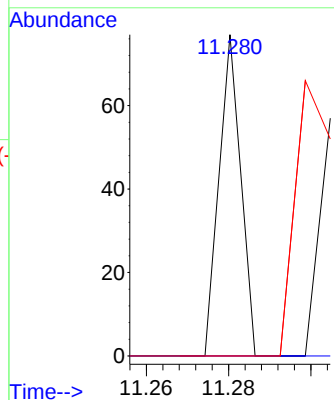

#76
1,2,3-Trichloropropane
Concen: 36.896 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 75 Resp: 44347
Ion Ratio Lower Upper
75 100
77 1.2 20.3 60.9#


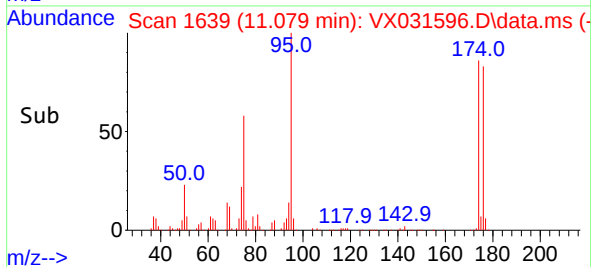
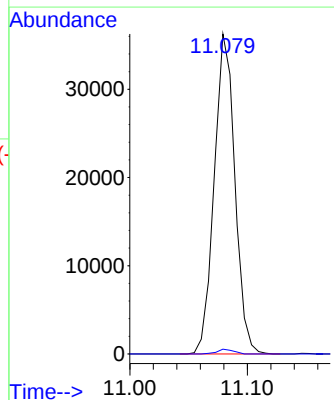
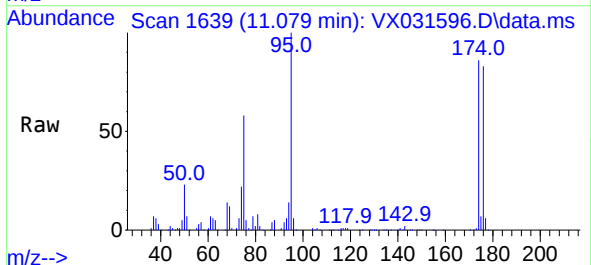




#78
n-propylbenzene
Concen: 11.158 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 91 Resp: 51624
Ion Ratio Lower Upper
91 100
120 23.0 11.8 35.4

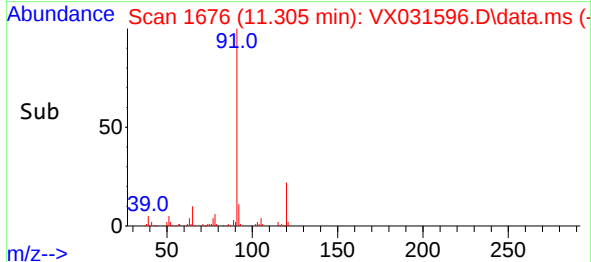

#79
2-Chlorotoluene
Concen: 18.746 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 91 Resp: 51624
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


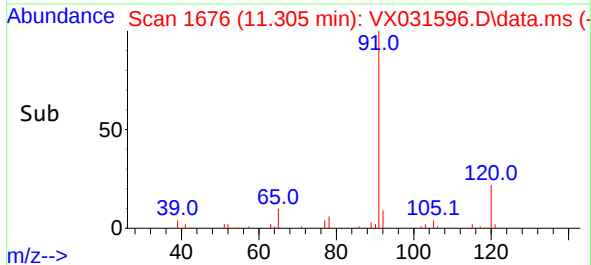

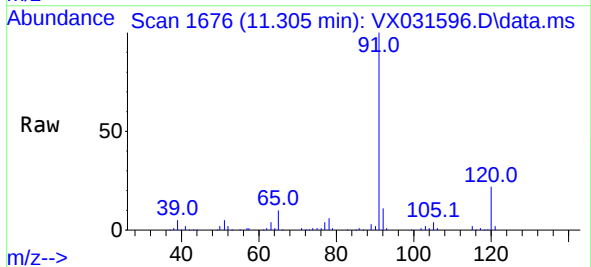




#80
1,3,5-Trimethylbenzene
Concen: 0.977 ug/l
RT: 11.451 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:105 Resp: 3336
Ion Ratio Lower Upper
105 100
120 51.2 24.5 73.5

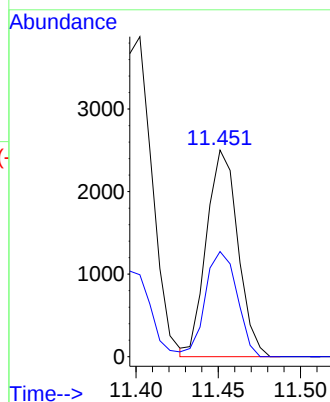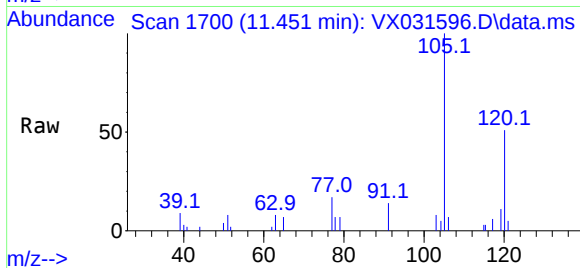

#81
trans-1,4-Dichloro-2-butene
Concen: 118.800 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 75 Resp: 44347
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


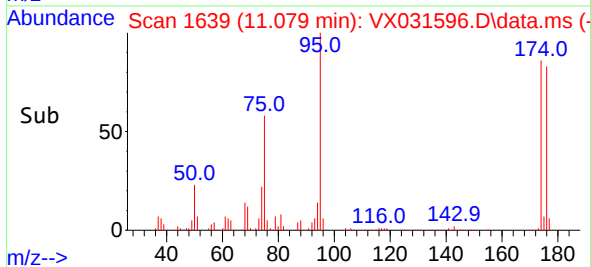

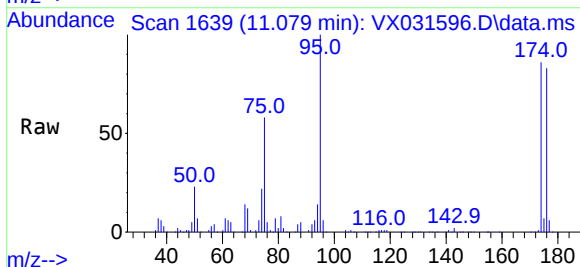




#82
4-Chlorotoluene
Concen: 15.973 ug/l
RT: 11.305 min Scan# 11
Delta R.T. -0.152 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion: 91 Resp: 51624
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

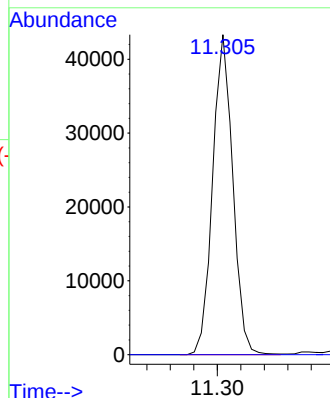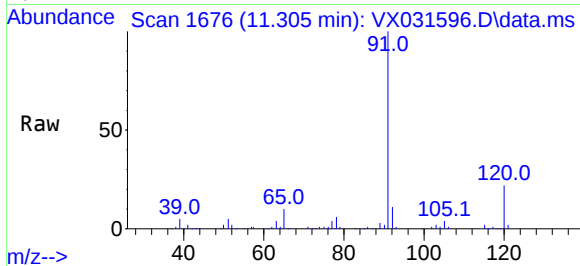

#84
1,2,4-Trimethylbenzene
Concen: 3.438 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.006 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 105 Resp: 11556
Ion Ratio Lower Upper
105 100
120 47.4 22.6 67.8


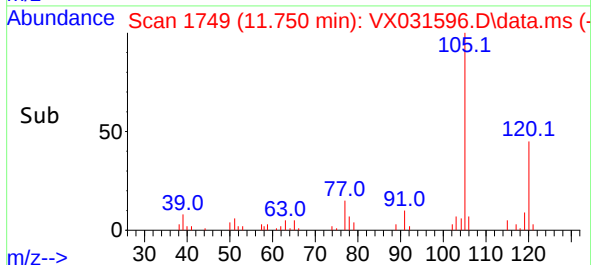

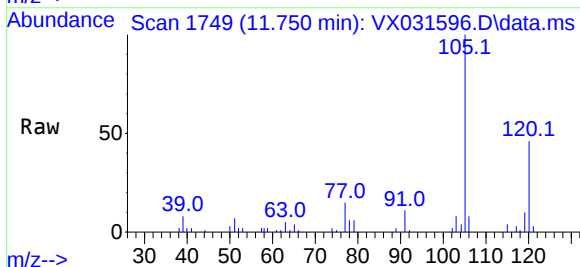




#85
 sec-Butylbenzene
 Concen: 0.519 ug/l
 RT: 11.890 min Scan# 1177
 Delta R.T. -0.000 min
 Lab File: VX031596.D
 Acq: 23 Sep 2022 02:34




Instrument :
 MSVOA_X
 ClientSampleId :
 MW-6RDL


Tgt Ion:105 Resp: 2174
 Ion Ratio Lower Upper
 105 100
 134 37.4 10.4 31.1#

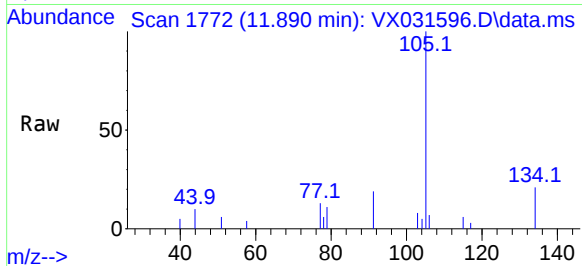

#89
 n-Butylbenzene
 Concen: 0.870 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.000 min
 Lab File: VX031596.D
 Acq: 23 Sep 2022 02:34

Tgt Ion: 91 Resp: 2619
 Ion Ratio Lower Upper
 91 100
 92 38.0 27.0 81.0
 134 0.0 13.3 39.9#


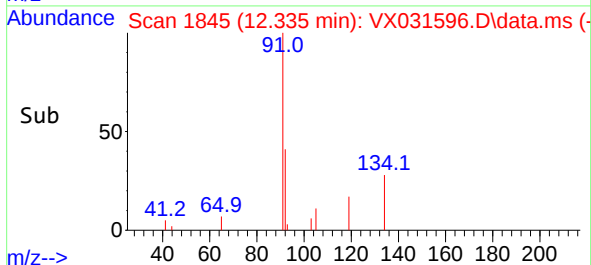
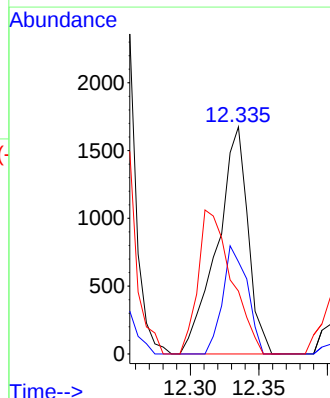
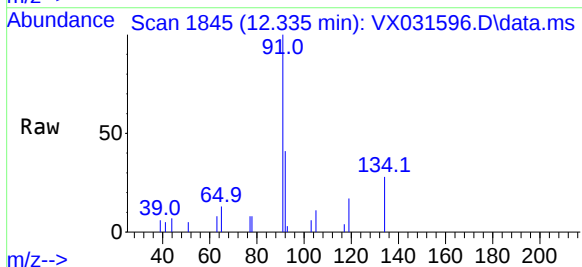




#90
Hexachloroethane
Concen: 3.510 ug/l
RT: 12.615 min Scan# 1879
Delta R.T. 0.073 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34




Instrument :
MSVOA_X
ClientSampleId :
MW-6RDL


Tgt Ion:117 Resp: 2132
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

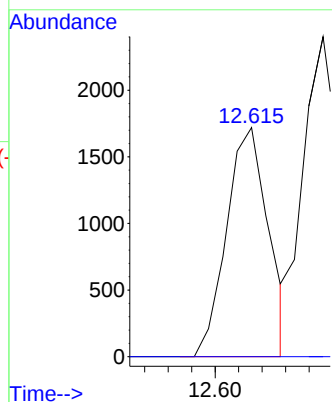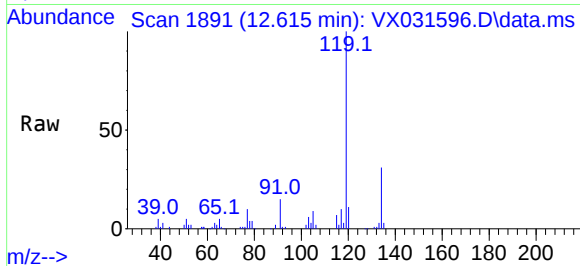

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.539 ug/l
RT: 13.170 min Scan# 1982
Delta R.T. 0.225 min
Lab File: VX031596.D
Acq: 23 Sep 2022 02:34

Tgt Ion: 75 Resp: 149
Ion Ratio Lower Upper
75 100
155 0.0 40.3 120.8#
157 0.0 51.5 154.5#

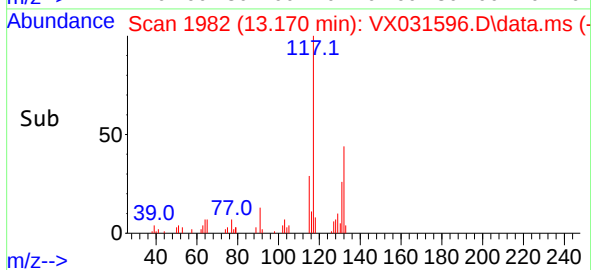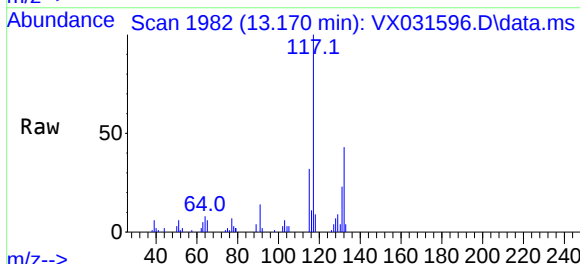



#95

Naphthalene

Concen: 17.469 ug/l

RT: 13.774 min Scan# 2081

Delta R.T. -0.000 min

Lab File: VX031596.D


Acq: 23 Sep 2022 02:34

Instrument :

MSVOA_X

ClientSampleId :

MW-6RDL



Tgt Ion:128 Resp: 67442

Ion Ratio Lower Upper

128 100

127 12.7 10.4 15.6

129 10.9 8.8 13.2

