

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031598.D
 Acq On : 23 Sep 2022 03:21
 Operator : JC/MD
 Sample : N4614-12DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-43DL

Quant Time: Sep 23 04:47:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	T.Q	Ion	Response	Conc	Units	Dev	(Min)


Internal Standards								
1) Pentafluorobenzene	5.555	168		73952	50.000	ug/l		0.00
34) 1,4-Difluorobenzene	6.763	114		120200	50.000	ug/l		0.00
63) Chlorobenzene-d5	10.055	117		109456	50.000	ug/l		0.00
72) 1,4-Dichlorobenzene-d4	12.024	152		53972	50.000	ug/l		0.00
System Monitoring Compounds								
33) 1,2-Dichloroethane-d4	5.958	65		74511	54.944	ug/l		0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.880%		
35) Dibromofluoromethane	5.385	113		62951	50.679	ug/l		0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.360%		
50) Toluene-d8	8.652	98		242708	50.682	ug/l		0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	101.360%		
62) 4-Bromofluorobenzene	11.079	95		76169	46.956	ug/l		0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.920%		
Target Compounds								
							Qvalue	
5) Bromomethane	1.617	94		541	0.236	ug/l	#	68
6) Chloroethane	1.648	64		33	Below Cal		#	43
11) Tert butyl alcohol	2.952	59		3044	Below Cal		#	73
16) Acetone	2.391	43		408	Below Cal		#	80
20) Methylene Chloride	2.794	84		425	Below Cal		#	76
25) 2-Butanone	4.592	43		334	0.319	ug/l	#	49
31) Cyclohexane	5.476	56		1344	0.668	ug/l	#	72
36) 1,1-Dichloropropene	5.555	75		5745	3.007	ug/l	#	50
38) Carbon Tetrachloride	5.543	117		7200	3.400	ug/l	#	16
39) Methylcyclohexane	7.384	83		1333	0.567	ug/l		86
40) Benzene	6.043	78		6996	1.227	ug/l	#	90
51) 4-Methyl-2-Pentanone	8.646	43		1159	0.514	ug/l	#	1
67) Ethyl Benzene	10.195	91		140536	23.581	ug/l		100
68) m/p-Xylenes	10.305	106		25862	10.798	ug/l		99
69) o-Xylene	10.646	106		7493	3.278	ug/l		97
73) Isopropylbenzene	10.963	105		8487	2.106	ug/l		97
75) 1,1,2,2-Tetrachloroethane	11.079	83		133	Below Cal		#	8
76) 1,2,3-Trichloropropane	11.079	75		44345	36.813	ug/l	#	37
78) n-propylbenzene	11.304	91		26353	5.683	ug/l		99
79) 2-Chlorotoluene	11.396	91		3860	1.399	ug/l	#	40
80) 1,3,5-Trimethylbenzene	11.451	105		7230	2.114	ug/l		98
81) trans-1,4-Dichloro-2-b...	11.079	75		44345	118.533	ug/l	#	11
82) 4-Chlorotoluene	11.457	91		1032	0.319	ug/l	#	44
83) tert-Butylbenzene	11.756	119		8331	2.513	ug/l	#	56
84) 1,2,4-Trimethylbenzene	11.756	105		67922	20.164	ug/l		97
85) sec-Butylbenzene	11.756	105		67922	16.190	ug/l	#	56
89) n-Butylbenzene	12.329	91		1656	0.549	ug/l	#	31
90) Hexachloroethane	12.530	117		688	1.130	ug/l	#	15
95) Naphthalene	13.774	128		49239	12.726	ug/l		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031598.D
Acq On : 23 Sep 2022 03:21
Operator : JC/MD
Sample : N4614-12DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-43DL

Quant Time: Sep 23 04:47:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration




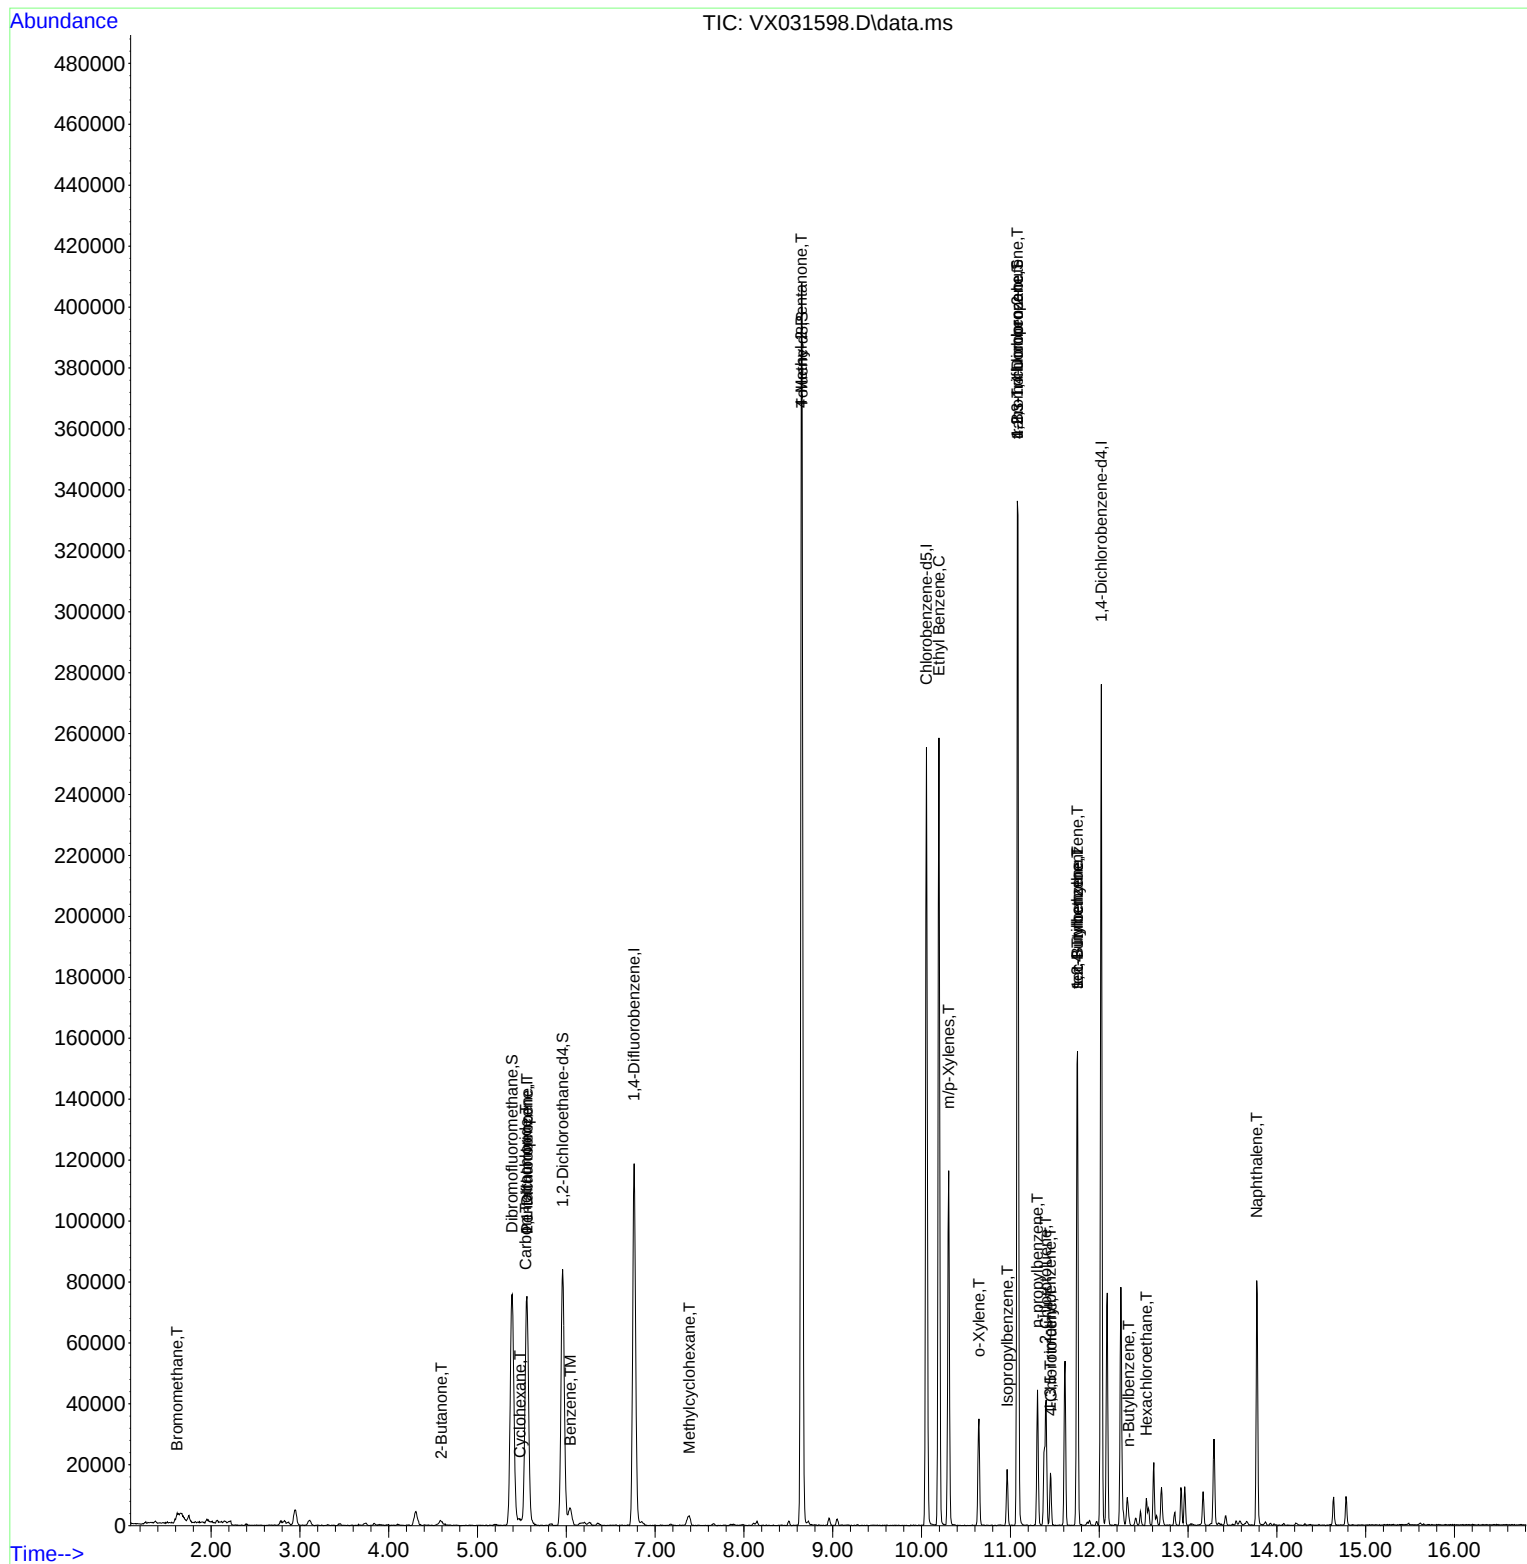




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.555 min Scan# 71
Delta R.T. -0.001 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
Client Sample Id :
MW-43DL

Tgt Ion: 168 Resp: 73952
Ion Ratio Lower Upper
168 100
99 51.7 48.8 73.2

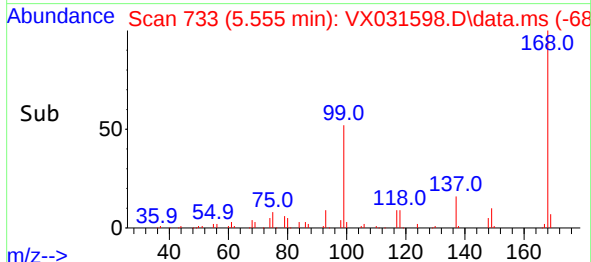


#5
Bromomethane
Concen: 0.236 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 94 Resp: 541
Ion Ratio Lower Upper
94 100
96 123.7 74.4 111.6#



Abundance Scan 98 (1.685 min): VX031454.D\data.ms (-92)

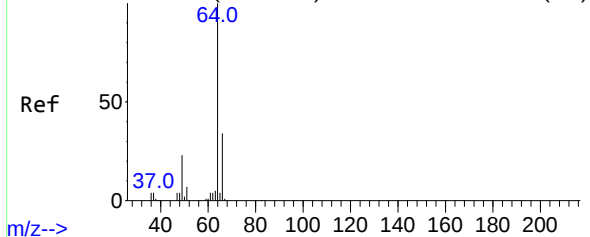

#6

Chloroethane

Concen: Below Cal

RT: 1.648 min Scan# 91

Delta R.T. -0.037 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21

Instrument :

MSVOA_X

ClientSampleId :

MW-43DL


Tgt Ion: 64 Resp: 33

Ion Ratio Lower Upper


64 100

66 0.0 25.0 37.4#


Abundance Scan 92 (1.648 min): VX031598.D\data.ms

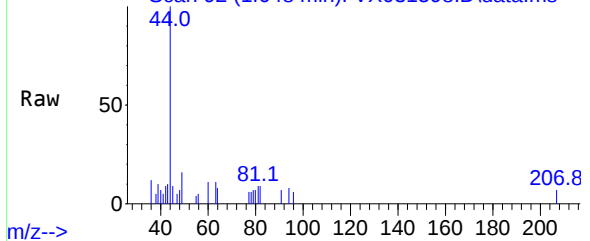


Abundance

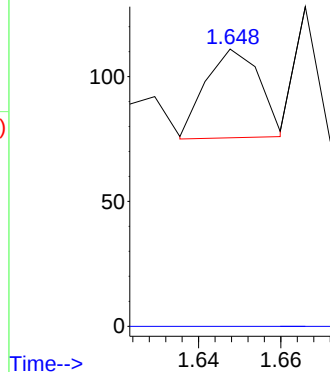

Abundance Scan 92 (1.648 min): VX031598.D\data.ms (-49)

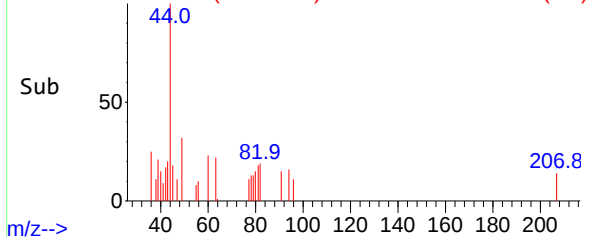

Abundance Scan 312 (2.989 min): VX031454.D\data.ms (-29)

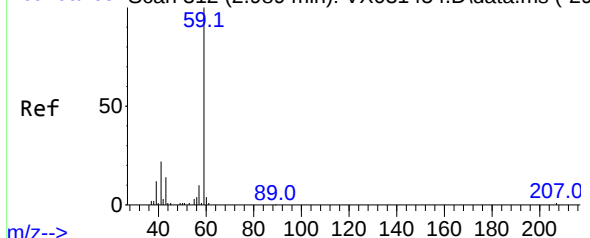

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.952 min Scan# 306

Delta R.T. -0.037 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21


Tgt Ion: 59 Resp: 3044

Ion Ratio Lower Upper


59 100

57 0.0 8.2 12.2#


Abundance Scan 306 (2.952 min): VX031598.D\data.ms

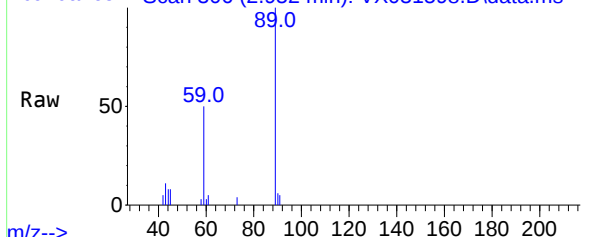


Abundance

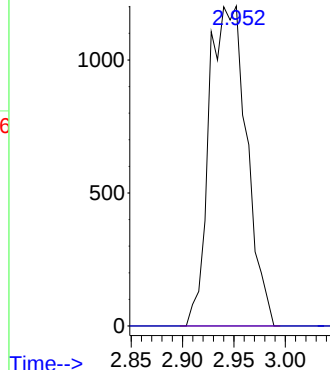

Abundance Scan 306 (2.952 min): VX031598.D\data.ms (-26)




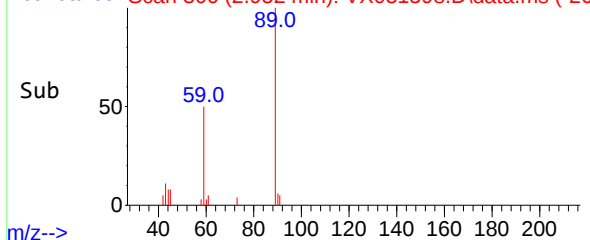




#16
Acetone
Concen: Below Cal
RT: 2.391 min Scan# 21
Delta R.T. 0.005 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 43 Resp: 408
Ion Ratio Lower Upper
43 100
58 40.6 23.8 35.8#



#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 84 Resp: 425
Ion Ratio Lower Upper
84 100
49 103.7 105.9 158.9#
51 21.6 32.2 48.2#
86 48.6 50.8 76.2#

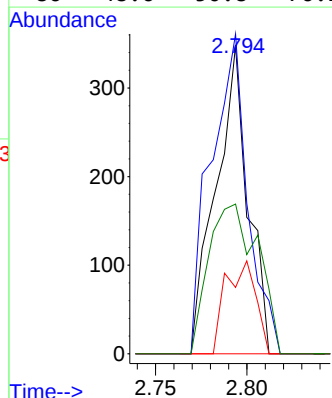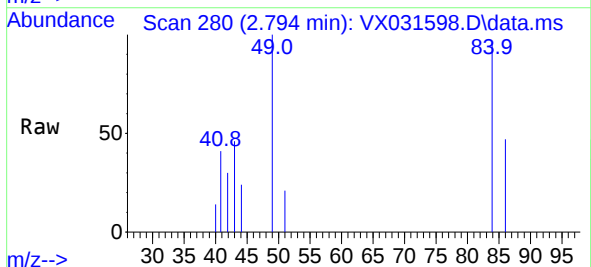

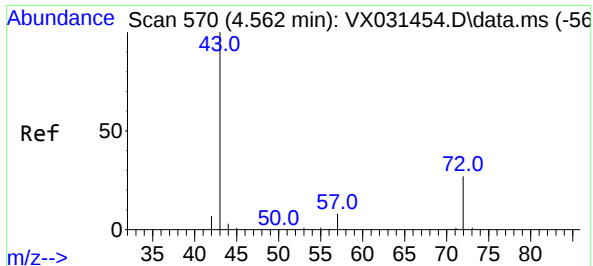

#25

2-Butanone

Concen: 0.319 ug/l

RT: 4.592 min Scan# 51

Delta R.T. 0.030 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21

Instrument :

MSVOA_X

ClientSampleId :





MW-43DL

Tgt Ion: 43 Resp: 334

Ion Ratio Lower Upper

43 100

72 0.0 21.1 31.7#

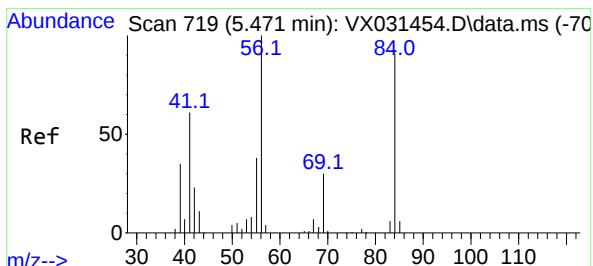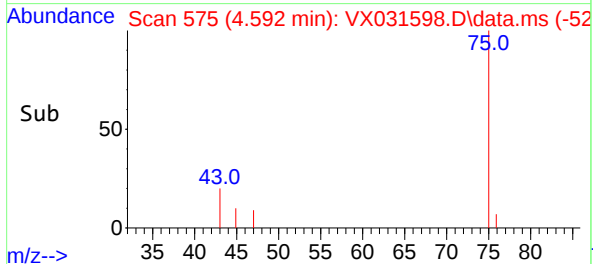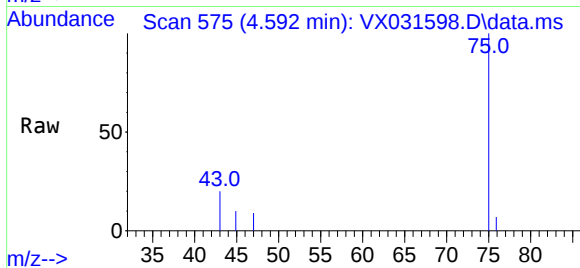

#31

Cyclohexane

Concen: 0.668 ug/l

RT: 5.476 min Scan# 720

Delta R.T. 0.005 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21




Tgt Ion: 56 Resp: 1344


Ion Ratio Lower Upper

56 100

69 19.2 25.1 37.7#

84 59.7 70.2 105.4#

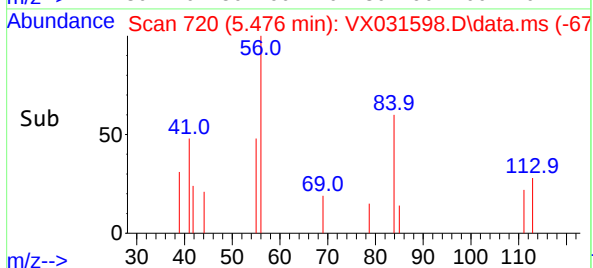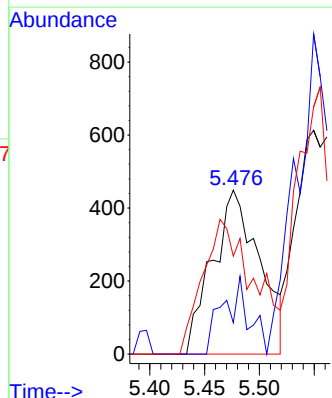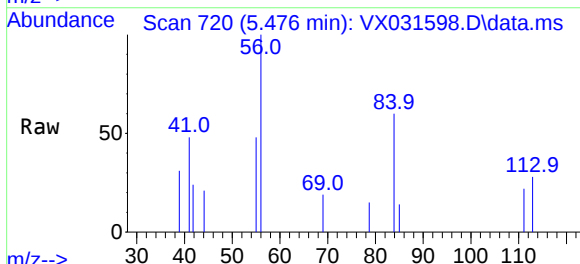



#33

1,2-Dichloroethane-d4

Concen: 54.944 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21

Instrument :

MSVOA_X

ClientSampleId :





MW-43DL

Tgt Ion: 65 Resp: 74511

Ion Ratio Lower Upper

65 100

67 51.6 0.0 102.4

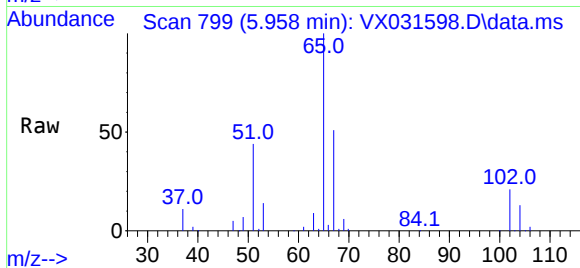

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21




Tgt Ion: 114 Resp: 120200


Ion Ratio Lower Upper

114 100

63 18.2 0.0 42.6

88 14.3 0.0 33.0




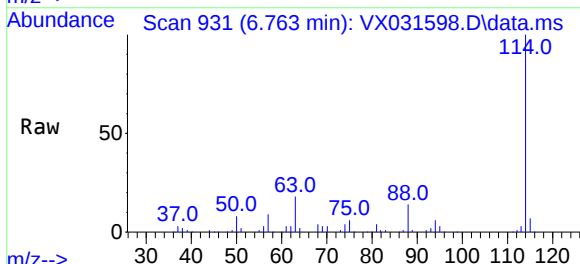


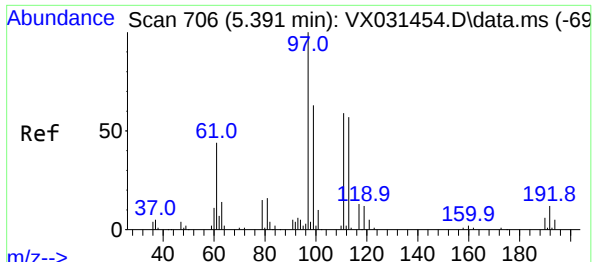

#35
Dibromofluoromethane
Concen: 50.679 ug/l
RT: 5.385 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:113 Resp: 62951
Ion Ratio Lower Upper
113 100
111 103.0 82.4 123.6
192 19.4 14.1 21.1

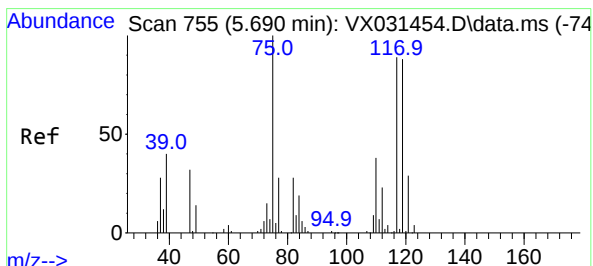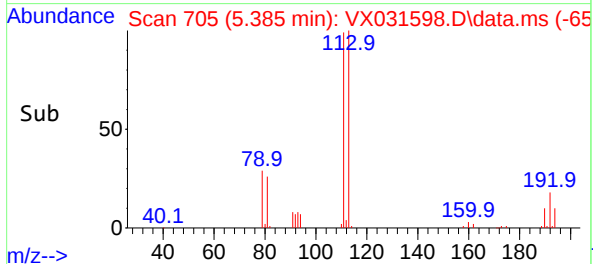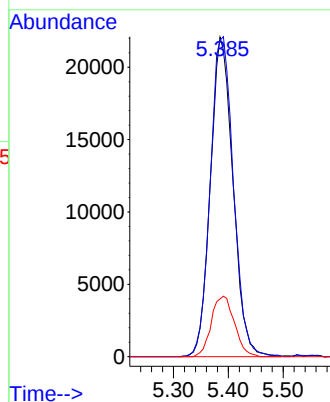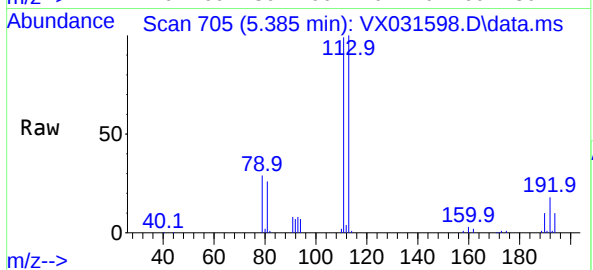

#36
1,1-Dichloropropene
Concen: 3.007 ug/l
RT: 5.555 min Scan# 733
Delta R.T. -0.135 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 75 Resp: 5745
Ion Ratio Lower Upper
75 100
110 9.4 17.5 52.5#
77 0.0 24.9 37.3#


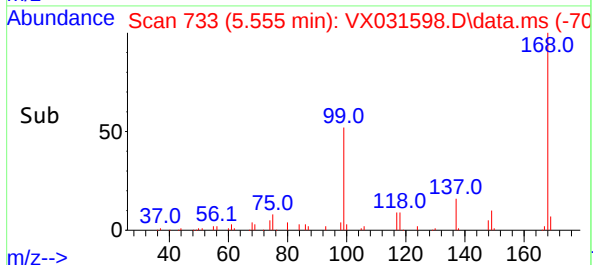

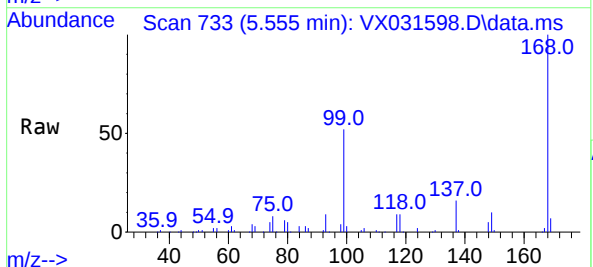




#38
Carbon Tetrachloride
Concen: 3.400 ug/l
RT: 5.543 min Scan# 71
Delta R.T. -0.135 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:117 Resp: 7200
Ion Ratio Lower Upper
117 100
119 4.3 74.6 112.0#
121 0.0 25.3 37.9#



#39
Methylcyclohexane
Concen: 0.567 ug/l
RT: 7.384 min Scan# 1033
Delta R.T. -0.001 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 83 Resp: 1333
Ion Ratio Lower Upper
83 100
55 63.4 61.0 91.4
98 55.5 37.7 56.5



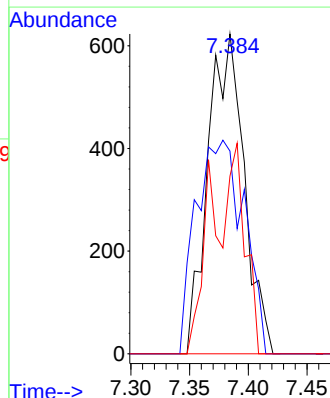





#40
Benzene
Concen: 1.227 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.001 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 78 Resp: 6996
Ion Ratio Lower Upper
78 100
77 18.4 18.7 28.1#



#50
Toluene-d8
Concen: 50.682 ug/l
RT: 8.652 min Scan# 1241
Delta R.T. -0.001 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 98 Resp: 242708
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7


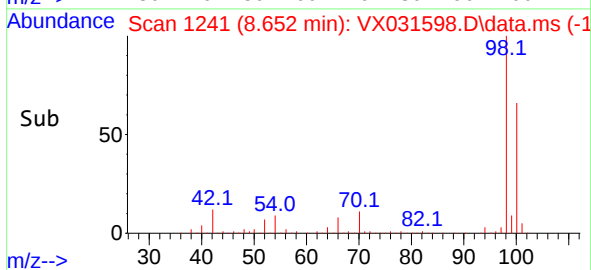






#51
4-Methyl-2-Pentanone
Concen: 0.514 ug/l
RT: 8.646 min Scan# 1159
Delta R.T. 0.066 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 43 Resp: 1159
Ion Ratio Lower Upper
43 100
58 169.9 30.6 46.0#



#62
4-Bromofluorobenzene
Concen: 46.956 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 95 Resp: 76169
Ion Ratio Lower Upper
95 100
174 92.5 0.0 153.2
176 89.5 0.0 144.0


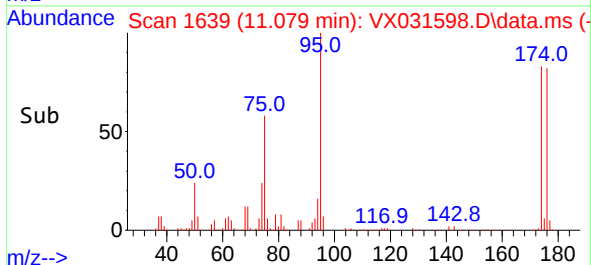
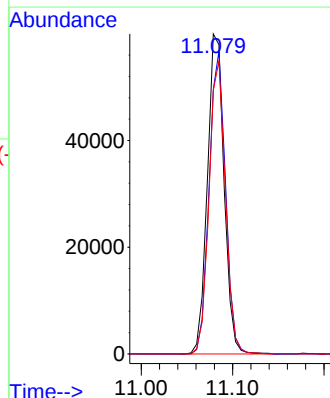
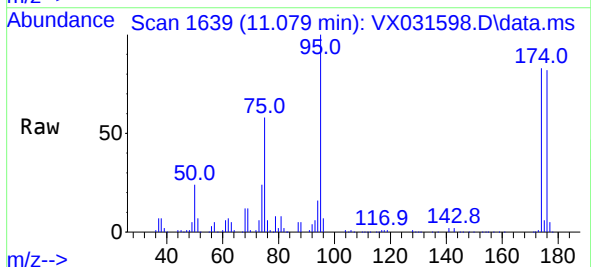




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:117 Resp: 109456
Ion Ratio Lower Upper
117 100
82 50.7 46.8 70.2
119 31.8 26.4 39.6

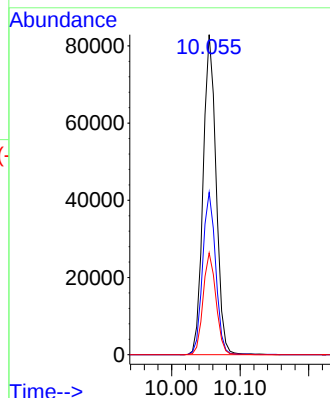

#67
Ethyl Benzene
Concen: 23.581 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 91 Resp: 140536
Ion Ratio Lower Upper
91 100
106 31.3 25.2 37.8



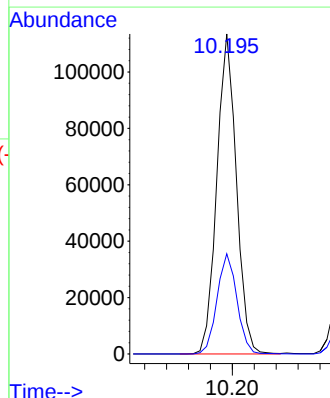





#68
m/p-Xylenes
Concen: 10.798 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:106 Resp: 25862
Ion Ratio Lower Upper
106 100
91 202.0 161.0 241.4

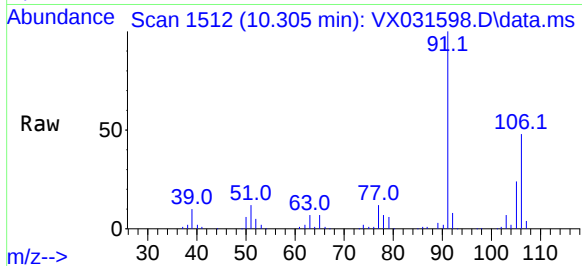

#69
o-Xylene
Concen: 3.278 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. 0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion:106 Resp: 7493
Ion Ratio Lower Upper
106 100
91 219.3 107.2 321.6


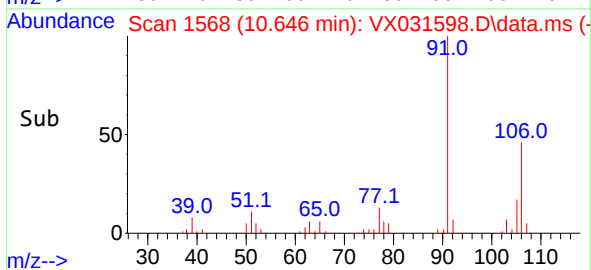

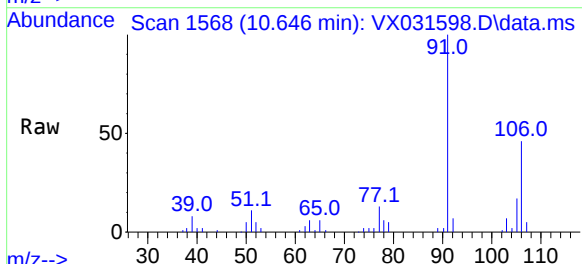




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:152 Resp: 53972
Ion Ratio Lower Upper
152 100
115 53.0 43.4 130.1
150 158.3 0.0 346.8

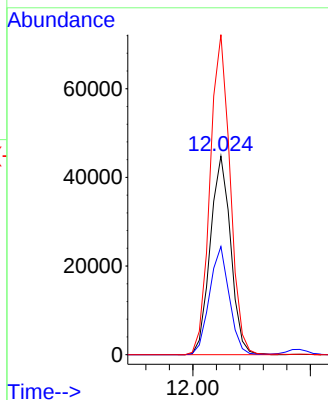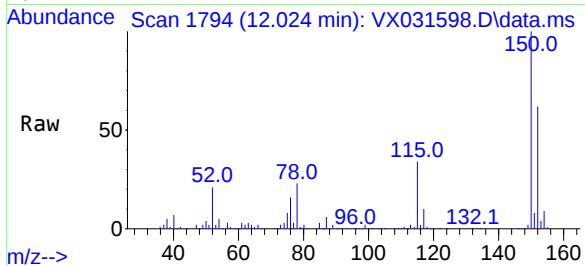

#73
Isopropylbenzene
Concen: 2.106 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion:105 Resp: 8487
Ion Ratio Lower Upper
105 100
120 25.8 13.7 41.0


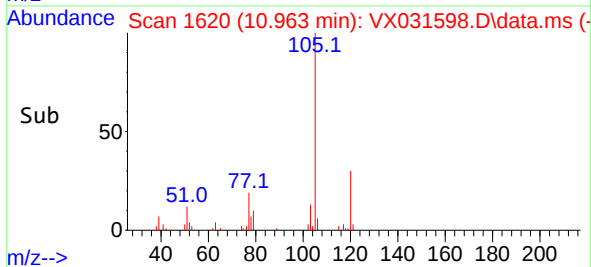
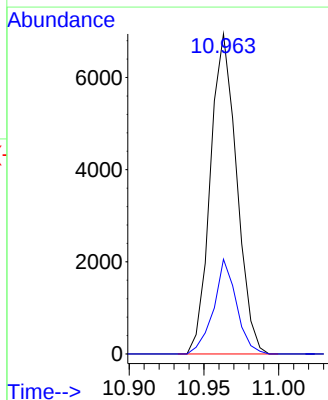
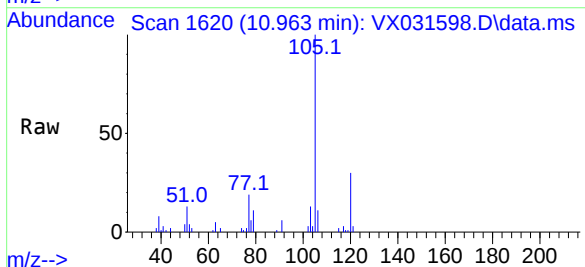




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.079 min Scan# 1639
Delta R.T. -0.134 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 83 Resp: 133
Ion Ratio Lower Upper
83 100
131 67.7 5.1 15.4#
85 0.0 32.6 97.8#

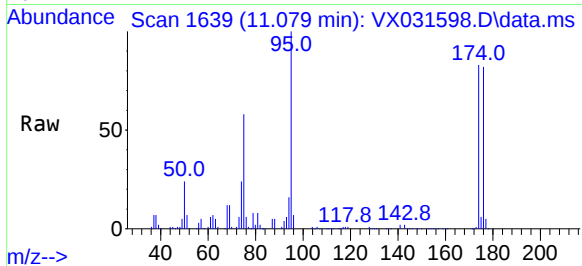

#76
1,2,3-Trichloropropane
Concen: 36.813 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 75 Resp: 44345
Ion Ratio Lower Upper
75 100
77 1.3 20.3 60.9#




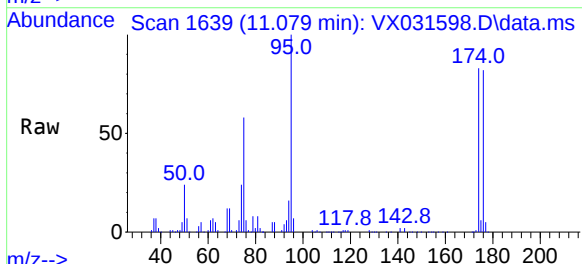




#78
n-propylbenzene
Concen: 5.683 ug/l
RT: 11.304 min Scan# 1690
Delta R.T. -0.001 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 91 Resp: 26353
Ion Ratio Lower Upper
91 100
120 24.1 11.8 35.4

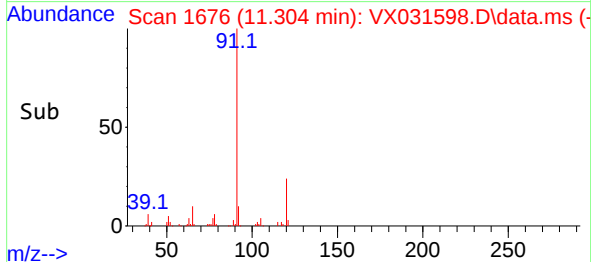

#79
2-Chlorotoluene
Concen: 1.399 ug/l
RT: 11.396 min Scan# 1691
Delta R.T. 0.030 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 91 Resp: 3860
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#


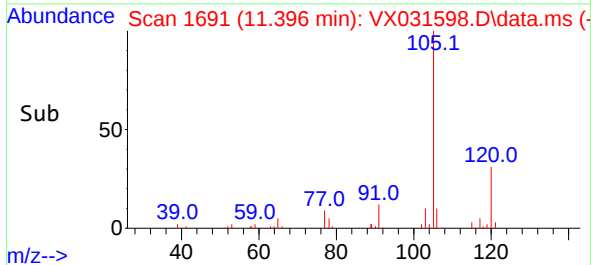

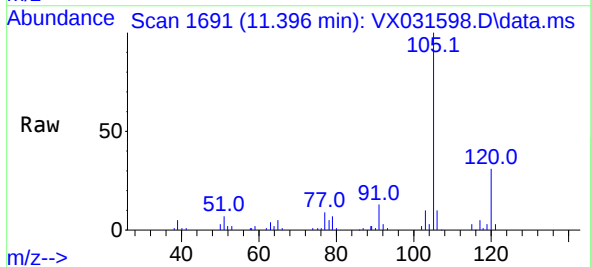




#80
1,3,5-Trimethylbenzene
Concen: 2.114 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:105 Resp: 7230
Ion Ratio Lower Upper
105 100
120 50.3 24.5 73.5

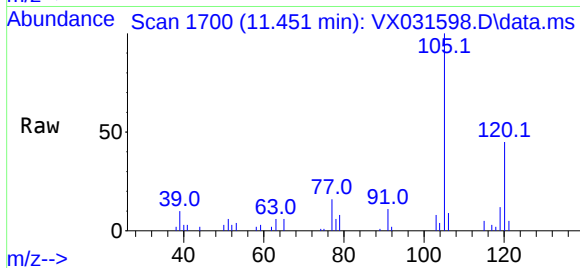

#81
trans-1,4-Dichloro-2-butene
Concen: 118.533 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 75 Resp: 44345
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#


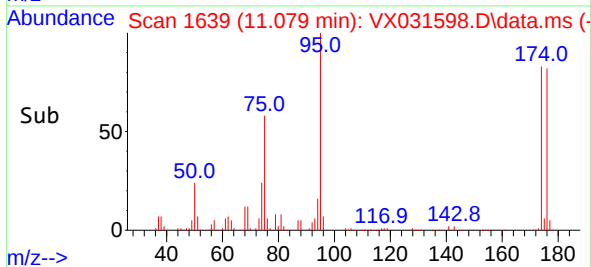

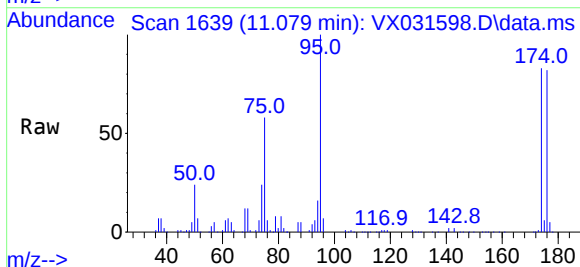




#82
4-Chlorotoluene
Concen: 0.319 ug/l
RT: 11.457 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion: 91 Resp: 1032
Ion Ratio Lower Upper
91 100
126 0.0 15.1 45.3#

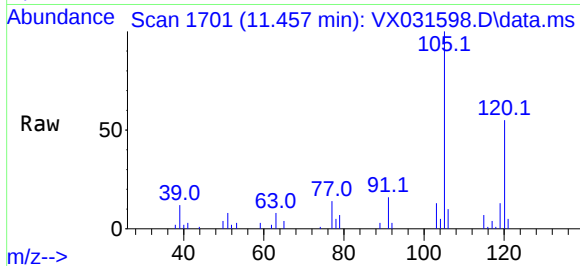

#83
tert-Butylbenzene
Concen: 2.513 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.037 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion: 119 Resp: 8331
Ion Ratio Lower Upper
119 100
91 90.0 29.2 87.6#
134 0.0 11.6 34.8#


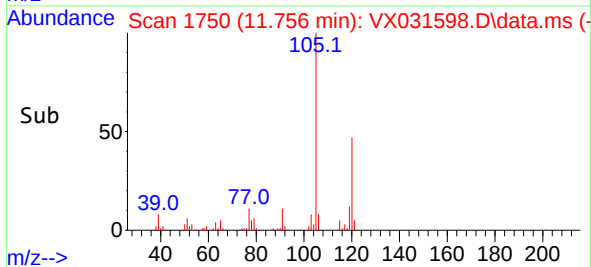

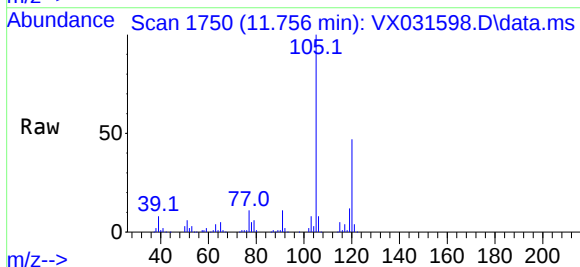




#84
1,2,4-Trimethylbenzene
Concen: 20.164 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21




Instrument :
MSVOA_X
ClientSampleId :
MW-43DL


Tgt Ion:105 Resp: 67922
Ion Ratio Lower Upper
105 100
120 47.1 22.6 67.8

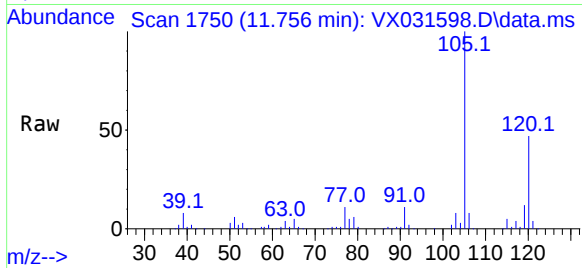

#85
sec-Butylbenzene
Concen: 16.190 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.134 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Tgt Ion:105 Resp: 67922
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

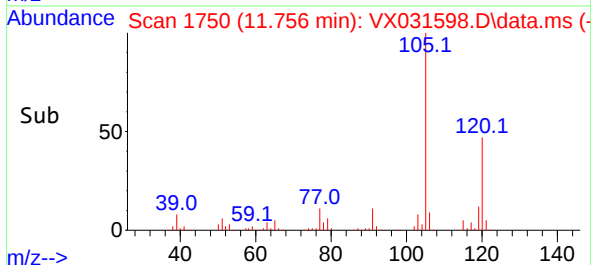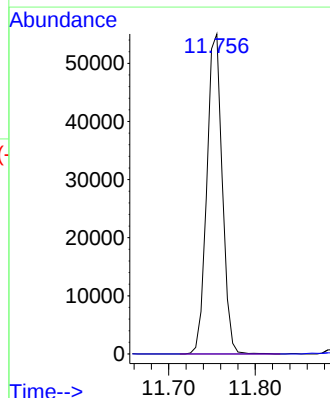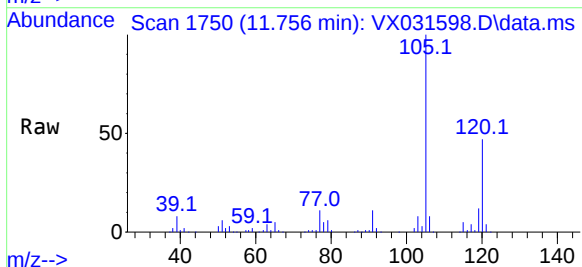



#89

n-Butylbenzene

Concen: 0.549 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX031598.D

Acq: 23 Sep 2022 03:21

Instrument :

MSVOA_X

ClientSampleId :

MW-43DL





Tgt Ion: 91 Resp: 1656

Ion Ratio Lower Upper

91 100

92 35.4 27.0 81.0

134 106.5 13.3 39.9#

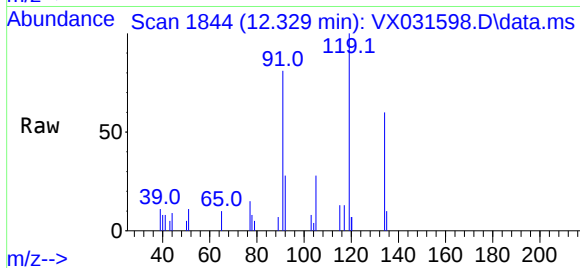

#90

Hexachloroethane

Concen: 1.130 ug/l

RT: 12.530 min Scan# 1877

Delta R.T. -0.012 min

Lab File: VX031598.D




Acq: 23 Sep 2022 03:21


Tgt Ion: 117 Resp: 688

Ion Ratio Lower Upper

117 100


201 0.0 34.8 104.4#

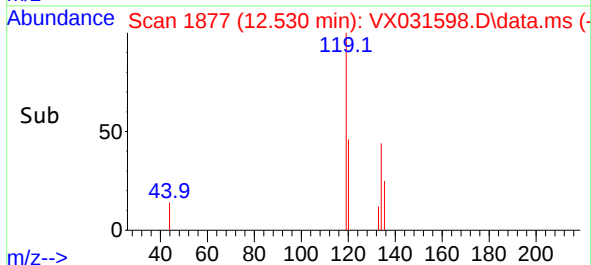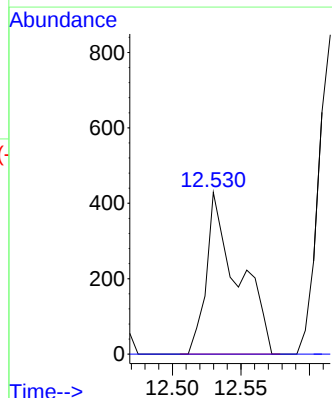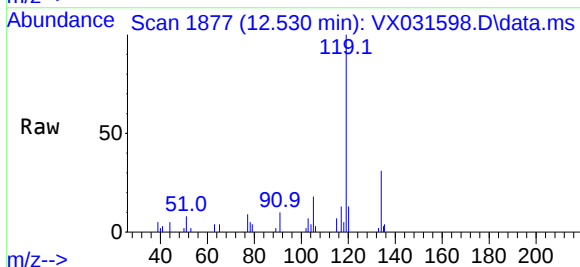



#95
Naphthalene
Concen: 12.726 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX031598.D
Acq: 23 Sep 2022 03:21

Instrument :
MSVOA_X
ClientSampleId :
MW-43DL

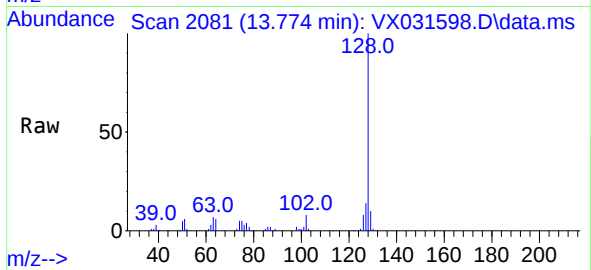

Tgt Ion:	128	Resp:	49239
Ion	Ratio	Lower	Upper
128	100		
127	13.7	10.4	15.6
129	10.9	8.8	13.2

