

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031604.D
 Acq On : 23 Sep 2022 05:40
 Operator : JC/MD
 Sample : N4750-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SB-16

Quant Time: Sep 23 09:18:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Sep 20 09:45:29 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	77915	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	129566	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	126198	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	57690	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	78789	55.148	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 110.300%			
35) Dibromofluoromethane	5.391	113	67730	50.583	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.160%			
50) Toluene-d8	8.653	98	265476	51.429	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 102.860%			
62) 4-Bromofluorobenzene	11.079	95	85718	49.023	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 98.040%			
Target Compounds						Qvalue
5) Bromomethane	1.617	94	541	0.224	ug/l	100
6) Chloroethane	1.727	64	106	Below Cal	#	43
11) Tert butyl alcohol	2.946	59	1158	Below Cal	#	73
13) Acrolein	2.239	56	138	Below Cal		86
16) Acetone	2.392	43	19865	22.736	ug/l	89
17) Carbon Disulfide	2.514	76	758	0.232	ug/l	# 90
18) Methyl Acetate	2.709	43	1648	0.772	ug/l	94
20) Methylene Chloride	2.788	84	8674	4.675	ug/l	88
25) 2-Butanone	4.580	43	4463	4.046	ug/l	92
29) Tetrahydrofuran	5.031	42	310	0.431	ug/l	# 53
36) 1,1-Dichloropropene	5.556	75	5834	2.833	ug/l	# 50
37) Ethyl Acetate	4.721	43	10846	4.414	ug/l	99
38) Carbon Tetrachloride	5.556	117	7746	3.393	ug/l	# 15
40) Benzene	6.043	78	123824	20.153	ug/l	96
43) Isopropyl Acetate	6.342	43	47688	12.629	ug/l	99
48) Methyl methacrylate	7.799	41	46350	26.867	ug/l	# 46
51) 4-Methyl-2-Pentanone	8.549	43	38853	15.996	ug/l	# 46
52) Toluene	8.720	92	82843	20.674	ug/l	97
54) cis-1,3-Dichloropropene	8.549	75	16840	6.657	ug/l	# 66
57) 1,3-Dichloropropane	9.482	76	2357	0.870	ug/l	# 43
59) 2-Hexanone	9.482	43	29904	16.394	ug/l	89
67) Ethyl Benzene	10.195	91	9360	1.362	ug/l	96
68) m/p-Xylenes	10.299	106	15175	5.496	ug/l	96
69) o-Xylene	10.640	106	6673	2.532	ug/l	93
70) Styrene	10.659	104	5285	1.218	ug/l	91
74) N-amyl acetate	10.774	43	1702	0.975	ug/l	# 48
75) 1,1,2,2-Tetrachloroethane	11.079	83	180	Below Cal	#	1
76) 1,2,3-Trichloropropane	11.079	75	49755	38.642	ug/l	# 37
78) n-propylbenzene	11.305	91	1040	0.210	ug/l	89
80) 1,3,5-Trimethylbenzene	11.451	105	1875	0.513	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.079	75	49755	124.423	ug/l	# 11
84) 1,2,4-Trimethylbenzene	11.756	105	7601	2.111	ug/l	74
85) sec-Butylbenzene	11.756	105	7601	1.695	ug/l	# 56
90) Hexachloroethane	12.414	117	2654	4.079	ug/l	# 15
95) Naphthalene	13.774	128	76362	18.464	ug/l	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031604.D
Acq On : 23 Sep 2022 05:40
Operator : JC/MD
Sample : N4750-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-16

Quant Time: Sep 23 09:18:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031604.D
Acq On : 23 Sep 2022 05:40
Operator : JC/MD
Sample : N4750-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SB-16


Quant Time: Sep 23 09:18:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260
QLast Update : Tue Sep 20 09:45:29 2022
Response via : Initial Calibration

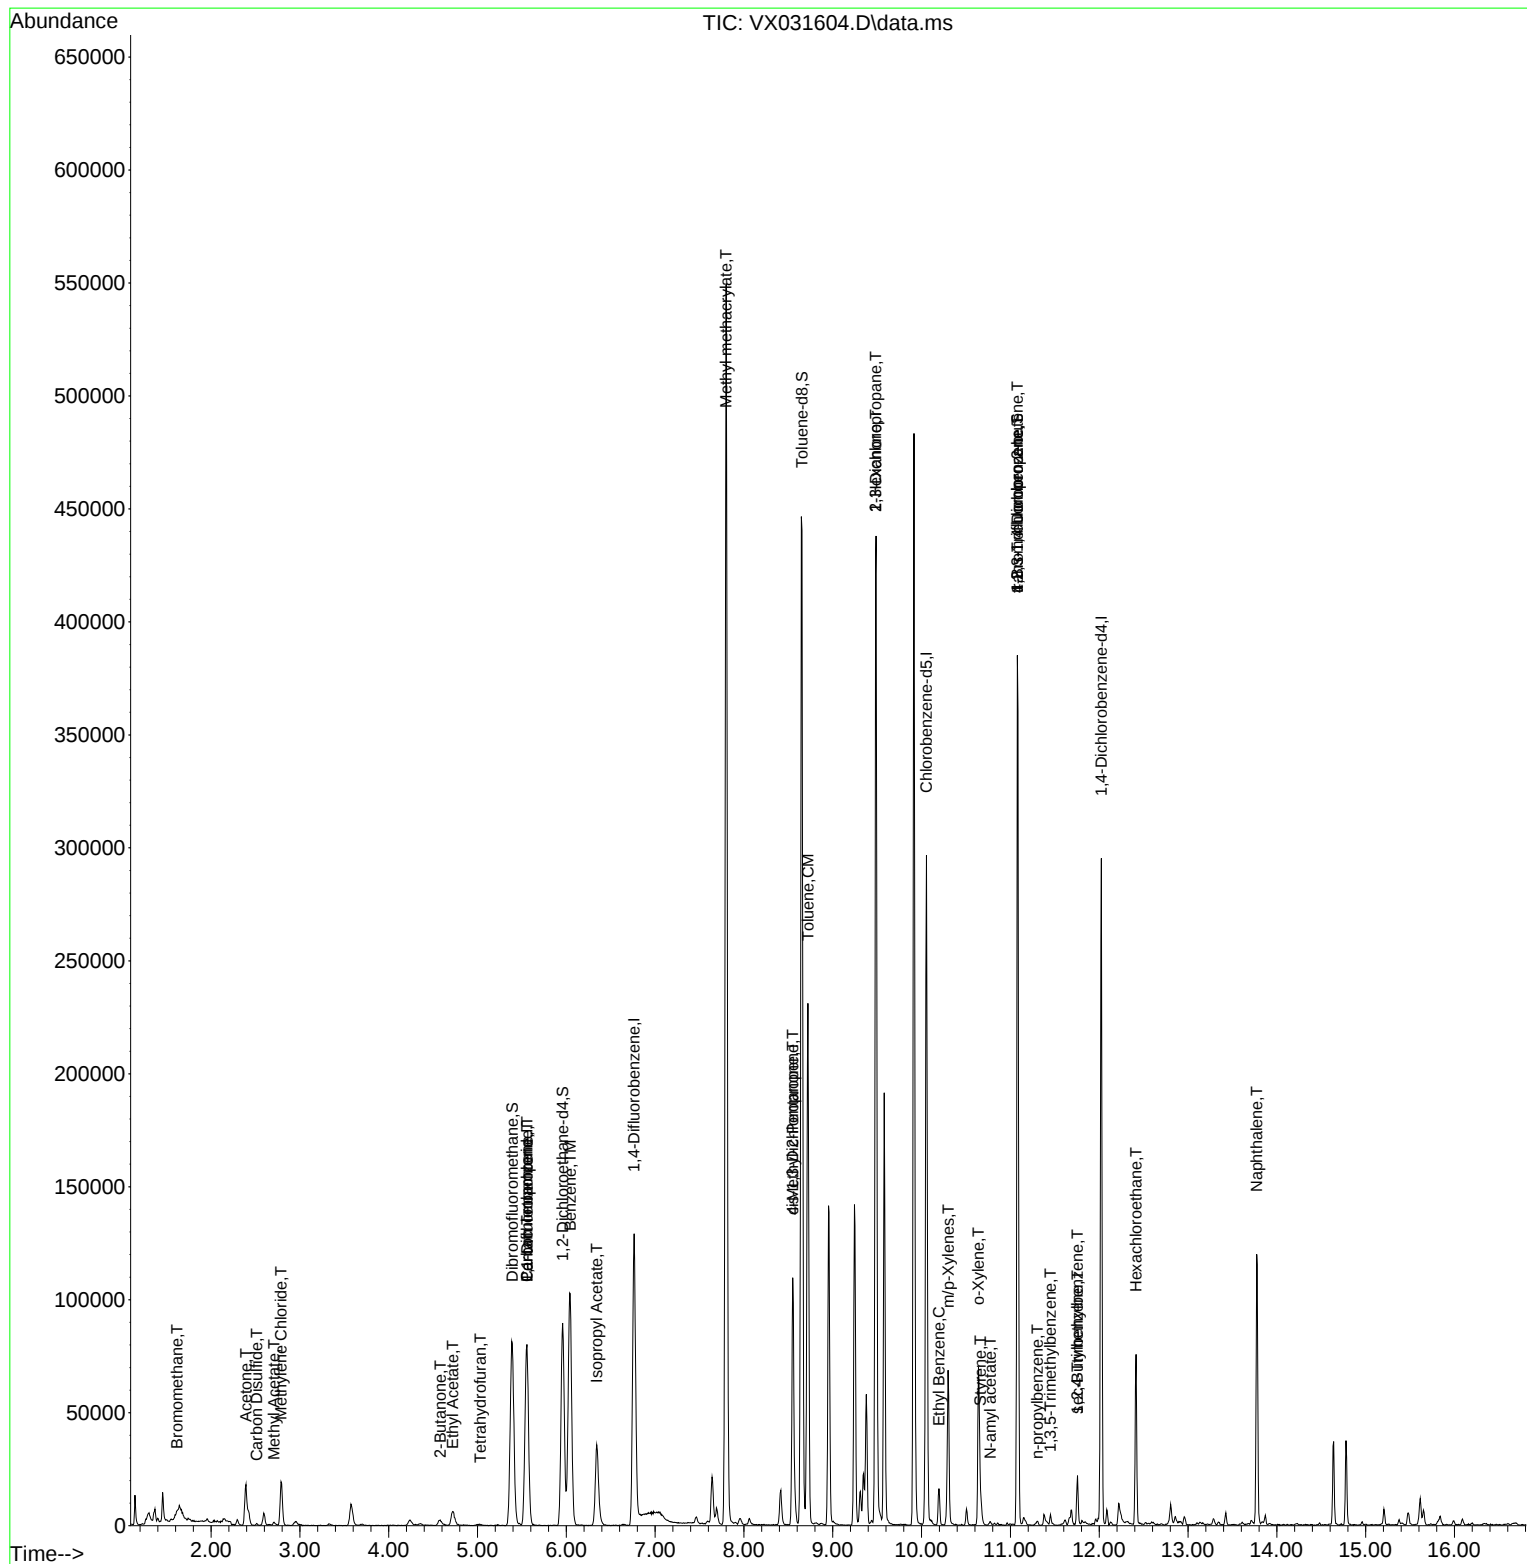






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Instrument :
MSVOA_X
ClientSampleId :
SB-16







Tgt Ion:168 Resp: 77915
Ion Ratio Lower Upper
168 100
99 51.7 48.8 73.2



#5
Bromomethane
Concen: 0.224 ug/l
RT: 1.617 min Scan# 87
Delta R.T. 0.006 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 94 Resp: 541
Ion Ratio Lower Upper
94 100
96 93.0 74.4 111.6







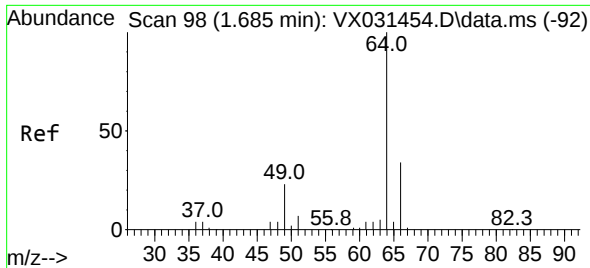

#6
Chloroethane
Concen: Below Cal
RT: 1.727 min Scan# 106
Delta R.T. 0.042 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 64 Resp: 106
Ion Ratio Lower Upper
64 100
66 0.0 25.0 37.4#

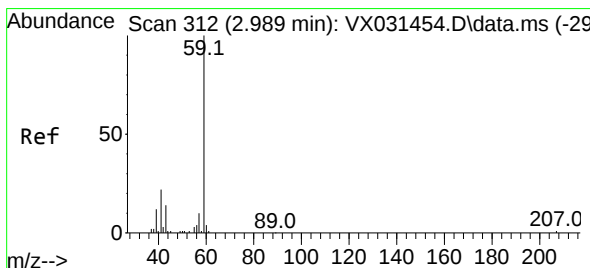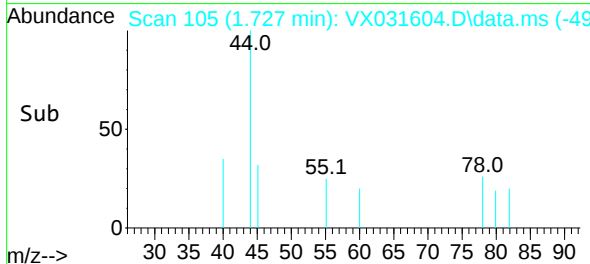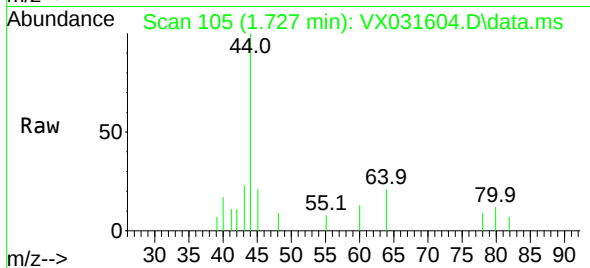

#11
Tert butyl alcohol
Concen: Below Cal
RT: 2.946 min Scan# 305
Delta R.T. -0.042 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 59 Resp: 1158
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.2#


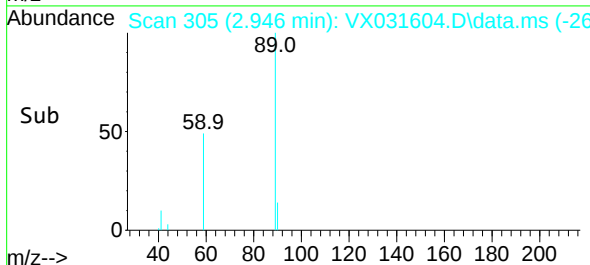

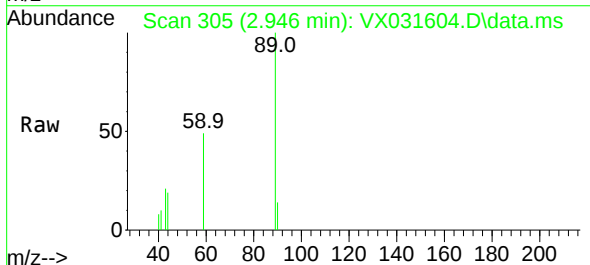


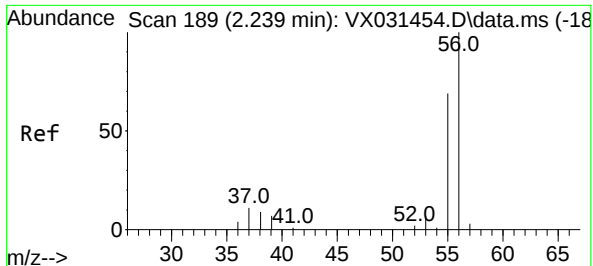

#13
Acrolein
Concen: Below Cal
RT: 2.239 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 56 Resp: 138
Ion Ratio Lower Upper
56 100
55 58.7 56.0 84.0

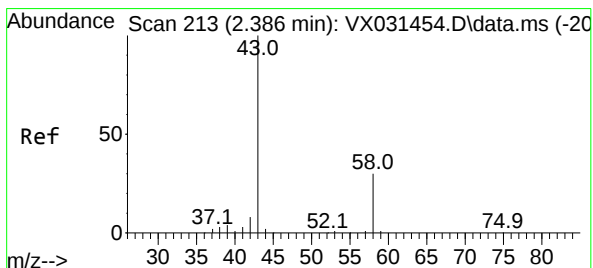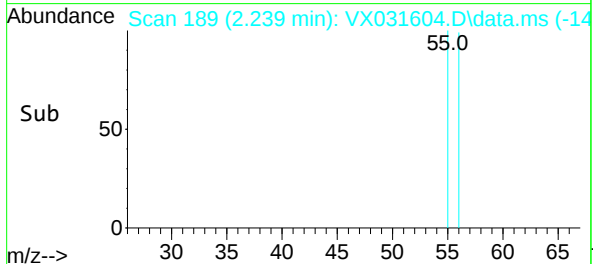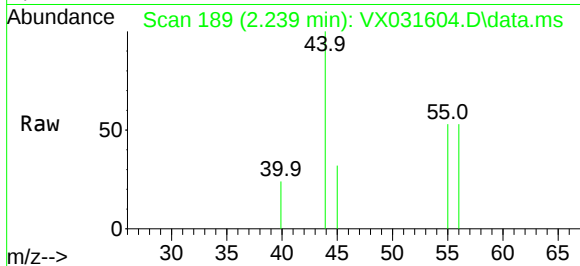

#16
Acetone
Concen: 22.736 ug/l
RT: 2.392 min Scan# 214
Delta R.T. 0.006 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 43 Resp: 19865
Ion Ratio Lower Upper
43 100
58 35.7 23.8 35.8


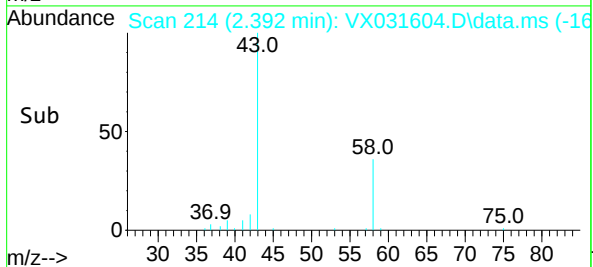

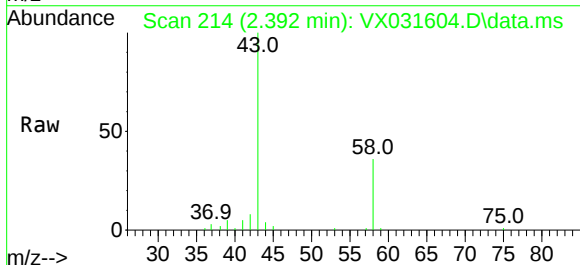




#17
Carbon Disulfide
Concen: 0.232 ug/l
RT: 2.514 min Scan# 217
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 76 Resp: 758
Ion Ratio Lower Upper
76 100
78 12.7 7.2 10.8#



#18
Methyl Acetate
Concen: 0.772 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 43 Resp: 1648
Ion Ratio Lower Upper
43 100
74 26.2 18.6 27.8


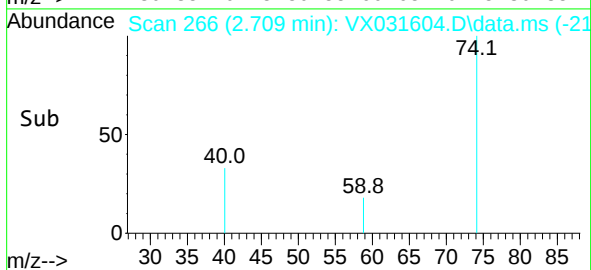






#20
Methylene Chloride
Concen: 4.675 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion:	84	Resp:	8674
Ion	Ratio	Lower	Upper
84	100		
49	113.3	105.9	158.9
51	35.6	32.2	48.2
86	67.2	50.8	76.2



#25
2-Butanone
Concen: 4.046 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.018 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion:	43	Resp:	4463
Ion	Ratio	Lower	Upper
43	100		
72	30.4	21.1	31.7

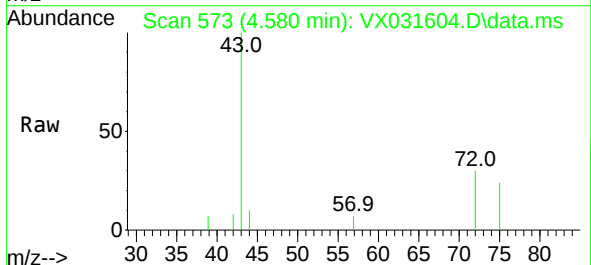



#29

Tetrahydrofuran

Concen: 0.431 ug/l

RT: 5.031 min Scan# 64

Delta R.T. 0.018 min

Lab File: VX031604.D

Acq: 23 Sep 2022 05:40

Instrument :

MSVOA_X

ClientSampleId :

SB-16





Tgt Ion: 42 Resp: 310

Ion Ratio Lower Upper

42 100

72 13.2 36.4 54.6#

71 13.5 33.5 50.3#

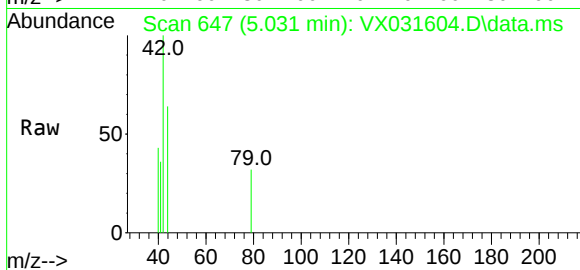

#33

1,2-Dichloroethane-d4

Concen: 55.148 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX031604.D




Acq: 23 Sep 2022 05:40


Tgt Ion: 65 Resp: 78789

Ion Ratio Lower Upper

65 100

67 51.7 0.0 102.4


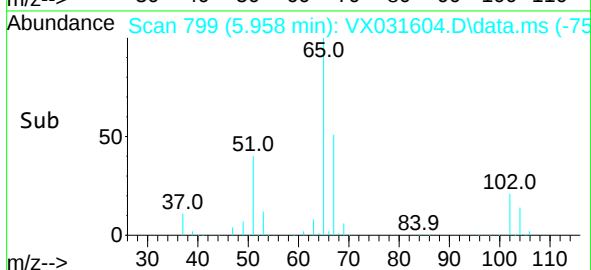

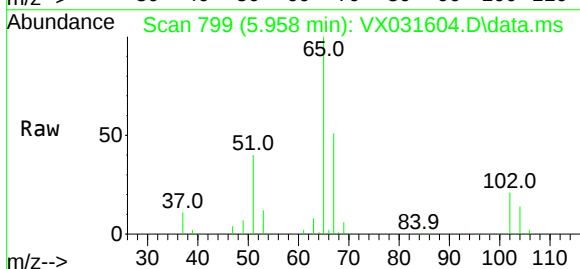




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion:114 Resp: 129566
Ion Ratio Lower Upper
114 100
63 20.2 0.0 42.6
88 13.6 0.0 33.0



#35
Dibromofluoromethane
Concen: 50.583 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion:113 Resp: 67730
Ion Ratio Lower Upper
113 100
111 102.1 82.4 123.6
192 19.3 14.1 21.1

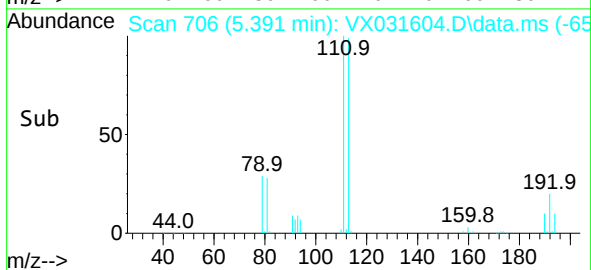

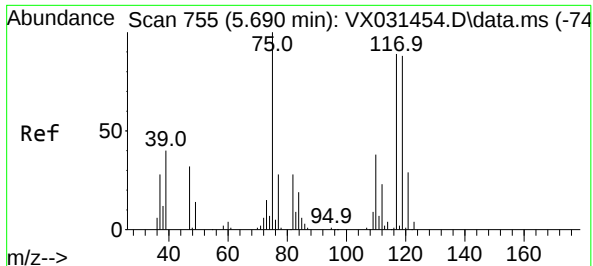

#36

1,1-Dichloropropene

Concen: 2.833 ug/l

RT: 5.556 min Scan# 755

Delta R.T. -0.134 min

Lab File: VX031604.D

Acq: 23 Sep 2022 05:40

Instrument :

MSVOA_X

ClientSampleId :

SB-16





Tgt Ion: 75 Resp: 5834

Ion Ratio Lower Upper

75 100

110 9.5 17.5 52.5#

77 0.0 24.9 37.3#

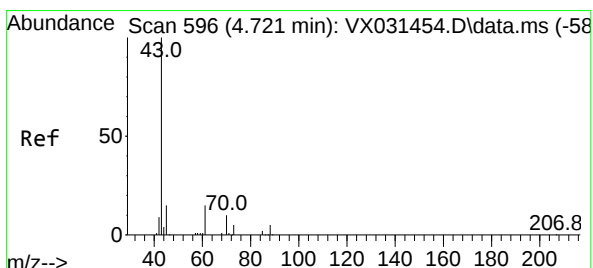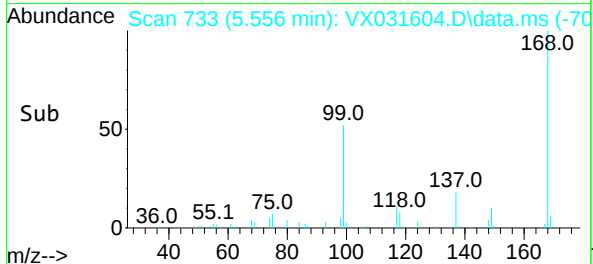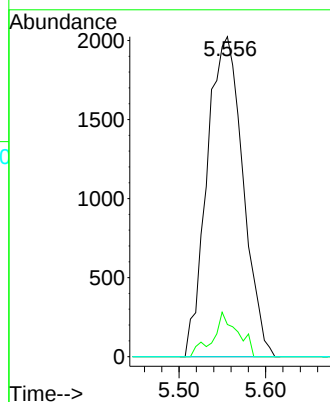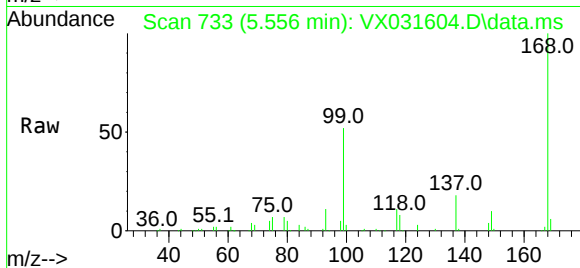

#37

Ethyl Acetate

Concen: 4.414 ug/l

RT: 4.721 min Scan# 596

Delta R.T. -0.000 min

Lab File: VX031604.D

Acq: 23 Sep 2022 05:40




Tgt Ion: 43 Resp: 10846


Ion Ratio Lower Upper

43 100

61 14.2 11.1 16.7

70 10.1 8.6 13.0


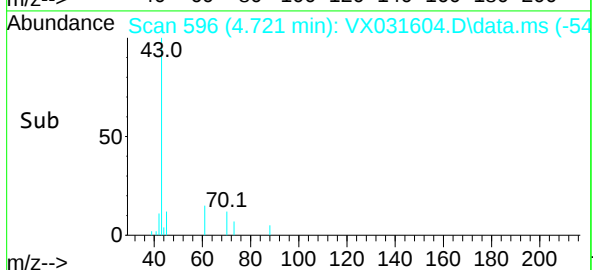

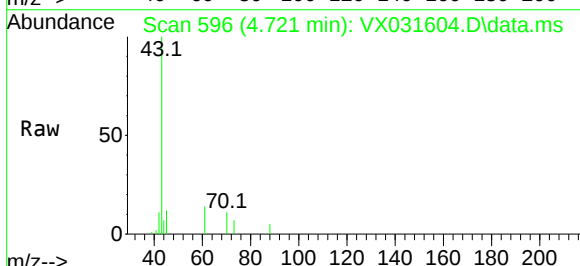




#38
Carbon Tetrachloride
Concen: 3.393 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion:117 Resp: 7746
Ion Ratio Lower Upper
117 100
119 3.0 74.6 112.0#
121 0.0 25.3 37.9#

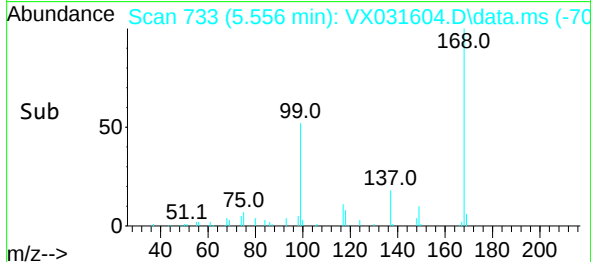

#40
Benzene
Concen: 20.153 ug/l
RT: 6.043 min Scan# 813
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 78 Resp: 123824
Ion Ratio Lower Upper
78 100
77 25.2 18.7 28.1




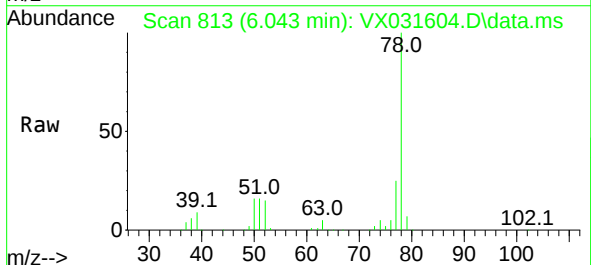




#43
Isopropyl Acetate
Concen: 12.629 ug/l
RT: 6.342 min Scan# 81
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 43 Resp: 47688
Ion Ratio Lower Upper
43 100
61 19.3 15.3 22.9
87 13.9 10.6 15.8

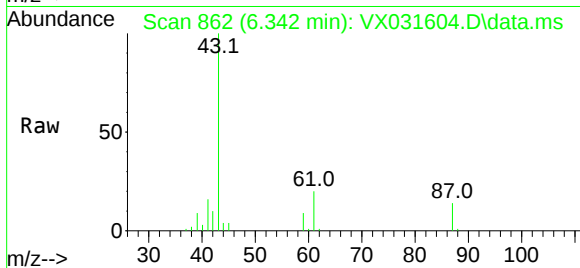

#48
Methyl methacrylate
Concen: 26.867 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.103 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 41 Resp: 46350
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 58.8 51.4 77.0

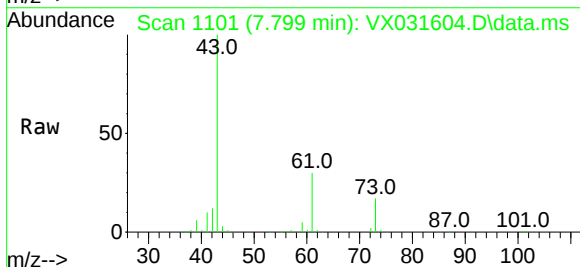

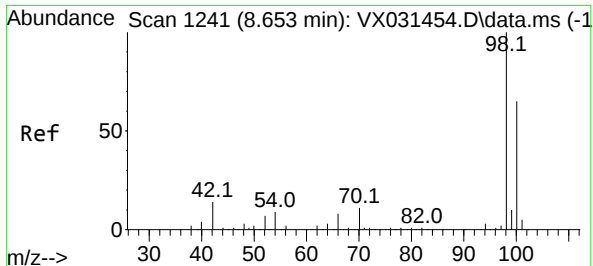

#50

Toluene-d8

Concen: 51.429 ug/l

RT: 8.653 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX031604.D

Acq: 23 Sep 2022 05:40

Instrument :

MSVOA_X

ClientSampleId :





SB-16

Tgt Ion: 98 Resp: 265476

Ion Ratio Lower Upper

98 100

100 64.5 52.5 78.7

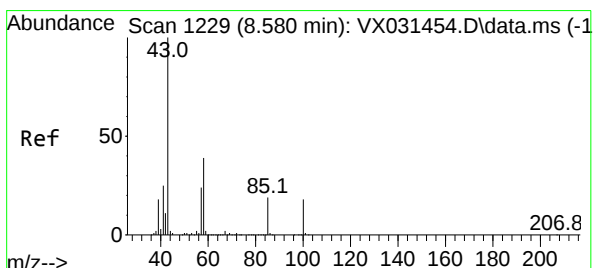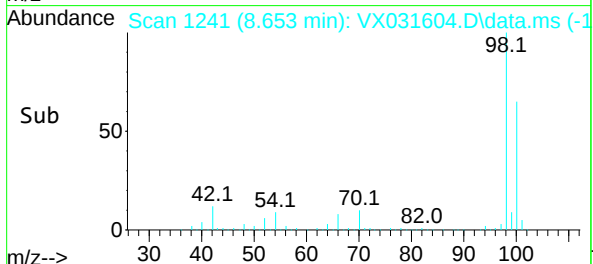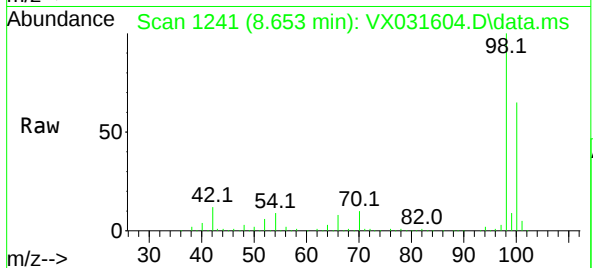

#51

4-Methyl-2-Pentanone

Concen: 15.996 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.031 min

Lab File: VX031604.D




Acq: 23 Sep 2022 05:40


Tgt Ion: 43 Resp: 38853

Ion Ratio Lower Upper

43 100

58 5.3 30.6 46.0#


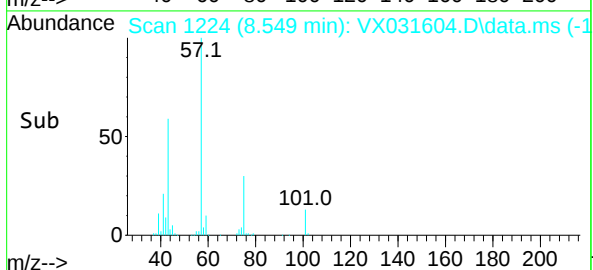

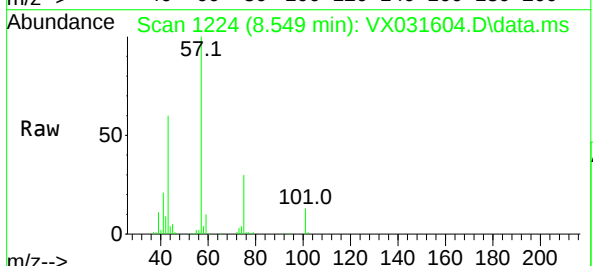




#52
Toluene
Concen: 20.674 ug/l
RT: 8.720 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 92 Resp: 82843
Ion Ratio Lower Upper
92 100
91 176.0 137.1 205.7



#54
cis-1,3-Dichloropropene
Concen: 6.657 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. 0.183 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 75 Resp: 16840
Ion Ratio Lower Upper
75 100
77 2.3 24.4 36.6#
39 37.3 43.7 65.5#

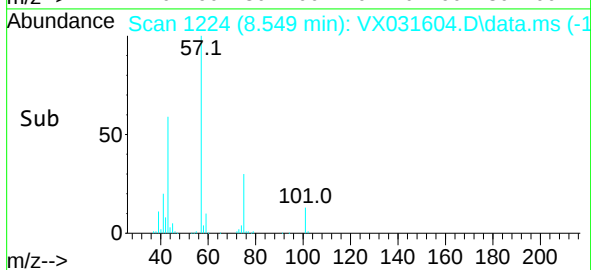

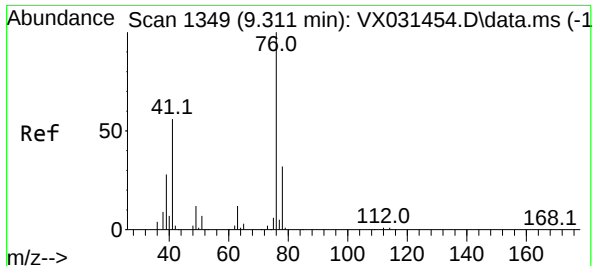

#57

1,3-Dichloropropane

Concen: 0.870 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.171 min

Lab File: VX031604.D

Acq: 23 Sep 2022 05:40

Instrument :

MSVOA_X

ClientSampleId :





SB-16

Tgt Ion: 76 Resp: 2357

Ion Ratio Lower Upper

76 100

78 0.0 25.5 38.3#

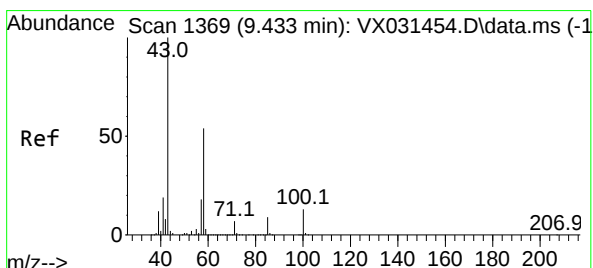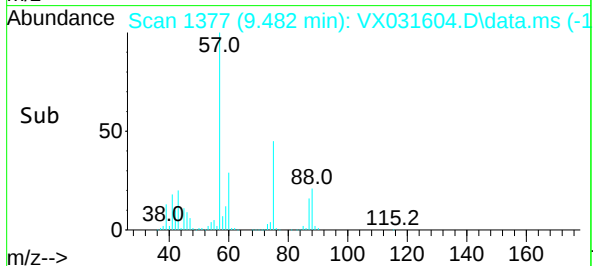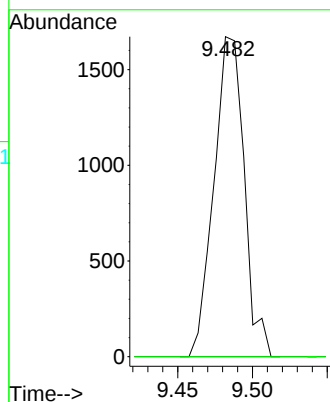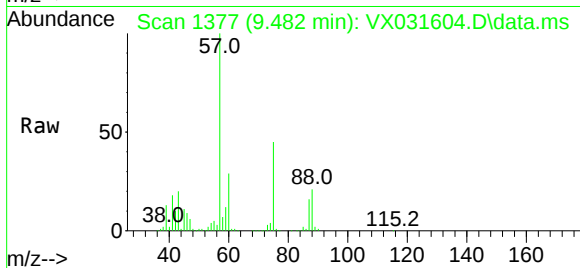

#59

2-Hexanone

Concen: 16.394 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX031604.D




Acq: 23 Sep 2022 05:40


Tgt Ion: 43 Resp: 29904

Ion Ratio Lower Upper

43 100

58 45.2 26.7 80.0


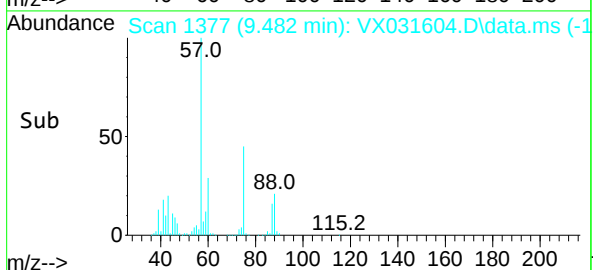

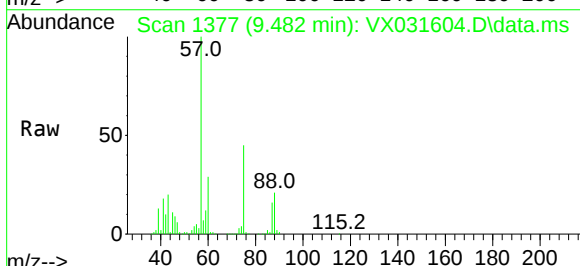




#62
4-Bromofluorobenzene
Concen: 49.023 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 95 Resp: 85718
Ion Ratio Lower Upper
95 100
174 91.6 0.0 153.2
176 89.2 0.0 144.0

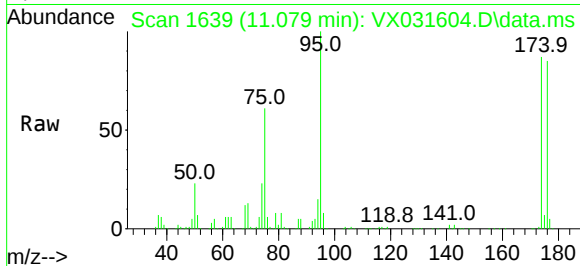

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 117 Resp: 126198
Ion Ratio Lower Upper
117 100
82 52.8 46.8 70.2
119 32.3 26.4 39.6




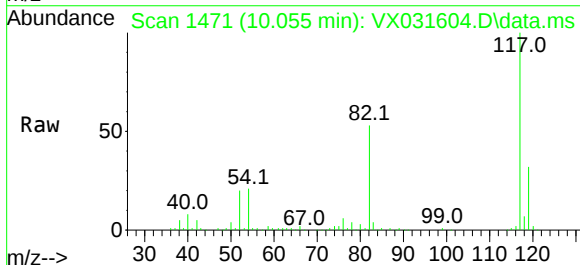




#67
Ethyl Benzene
Concen: 1.362 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 91 Resp: 9360
Ion Ratio Lower Upper
91 100
106 29.1 25.2 37.8

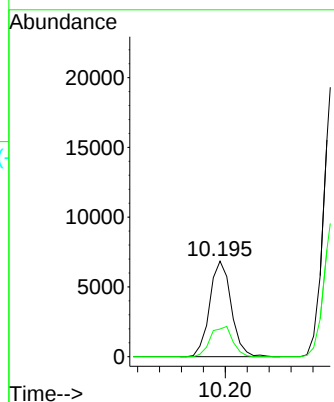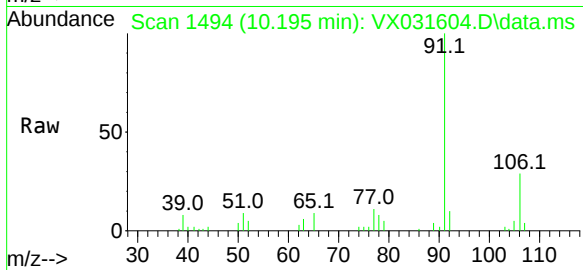

#68
m/p-Xylenes
Concen: 5.496 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.006 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 106 Resp: 15175
Ion Ratio Lower Upper
106 100
91 195.2 161.0 241.4


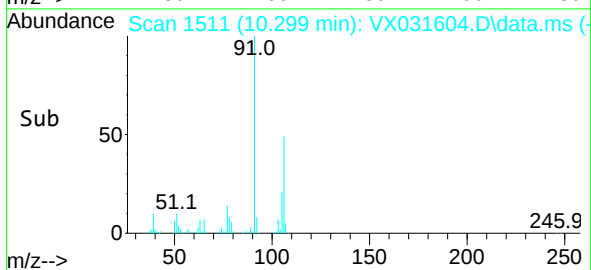
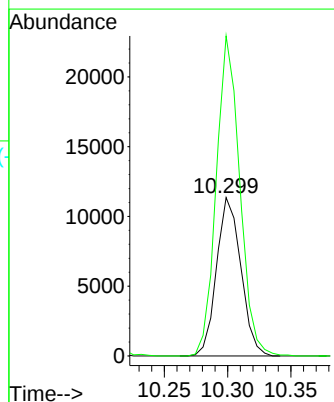





#69
o-Xylene
Concen: 2.532 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion:106 Resp: 6673
Ion Ratio Lower Upper
106 100
91 204.0 107.2 321.6

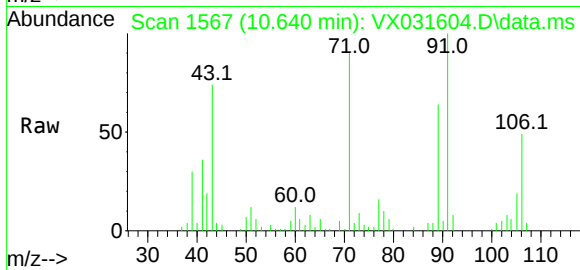

#70
Styrene
Concen: 1.218 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion:104 Resp: 5285
Ion Ratio Lower Upper
104 100
78 57.0 41.4 62.2
103 62.5 43.8 65.8




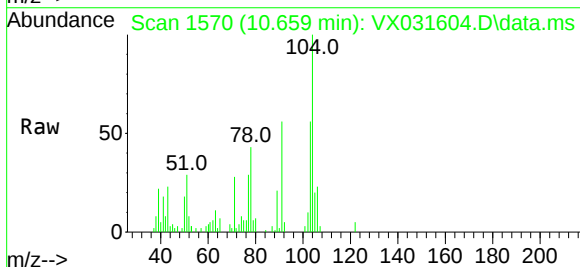




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX031604.D
 Acq: 23 Sep 2022 05:40




Instrument :
 MSVOA_X
 ClientSampleId :
 SB-16


Tgt Ion:152 Resp: 57690
 Ion Ratio Lower Upper
 152 100
 115 55.7 43.4 130.1
 150 156.2 0.0 346.8

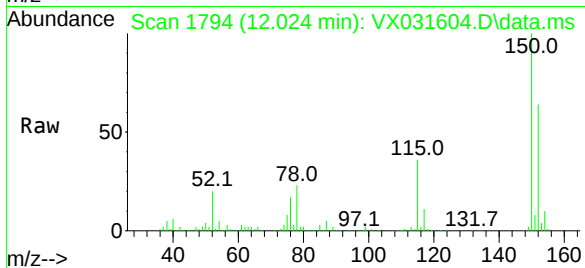

#74
 N-ethyl acetate
 Concen: 0.975 ug/l
 RT: 10.774 min Scan# 1589
 Delta R.T. -0.068 min
 Lab File: VX031604.D
 Acq: 23 Sep 2022 05:40

Tgt Ion: 43 Resp: 1702
 Ion Ratio Lower Upper
 43 100
 70 0.0 33.4 50.2#
 55 9.0 18.2 27.2#
 61 0.0 19.3 28.9#




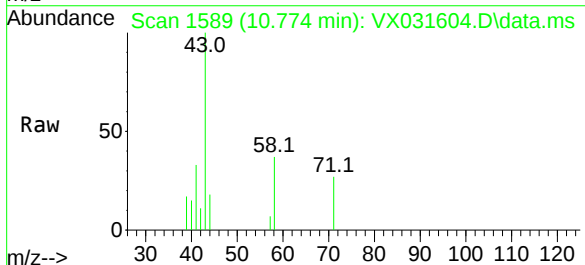




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 11.079 min Scan# 1639
Delta R.T. -0.134 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 83 Resp: 180
Ion Ratio Lower Upper
83 100
131 117.8 5.1 15.4#
85 0.0 32.6 97.8#

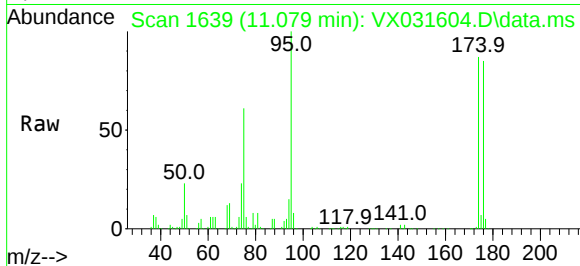

#76
1,2,3-Trichloropropane
Concen: 38.642 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 75 Resp: 49755
Ion Ratio Lower Upper
75 100
77 1.2 20.3 60.9#


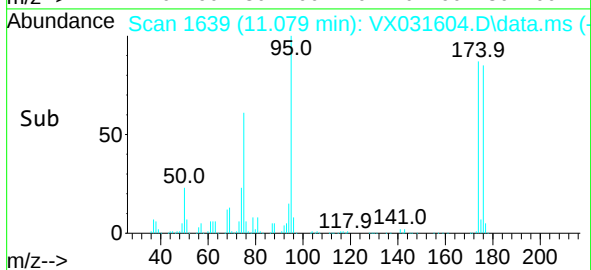

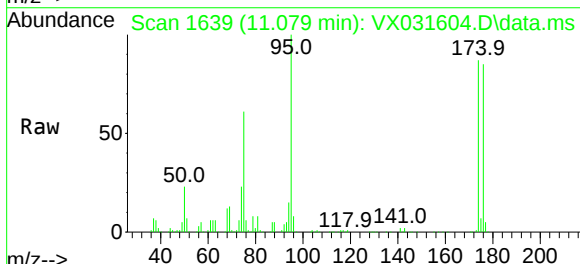


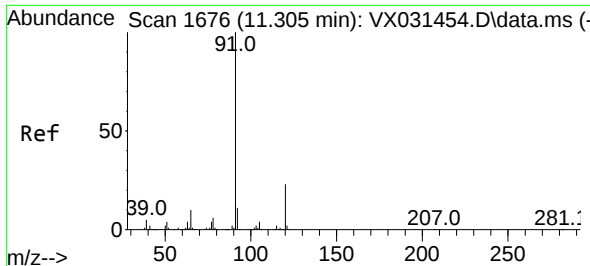

#78
n-propylbenzene
Concen: 0.210 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 91 Resp: 1040
Ion Ratio Lower Upper
91 100
120 18.4 11.8 35.4

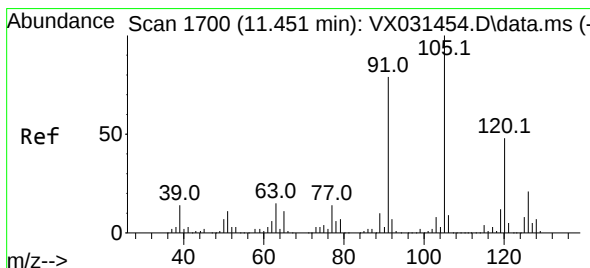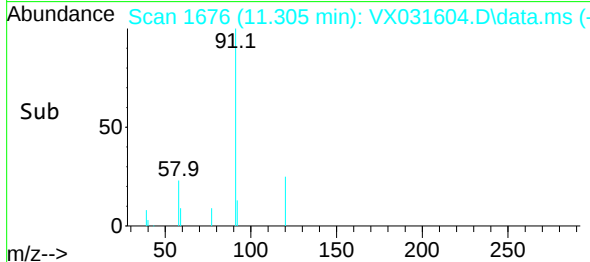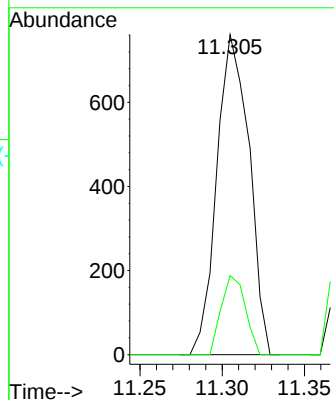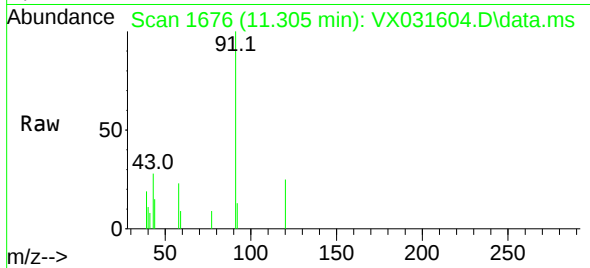

#80
1,3,5-Trimethylbenzene
Concen: 0.513 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. 0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 105 Resp: 1875
Ion Ratio Lower Upper
105 100
120 53.3 24.5 73.5


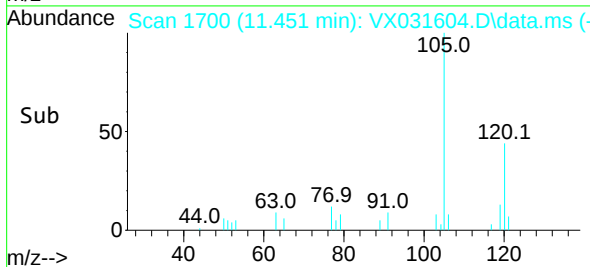
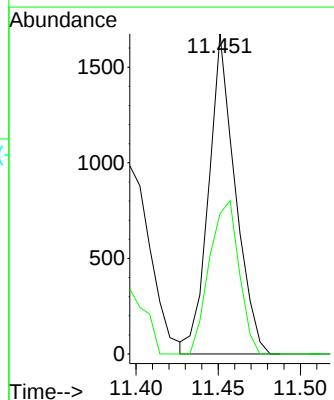
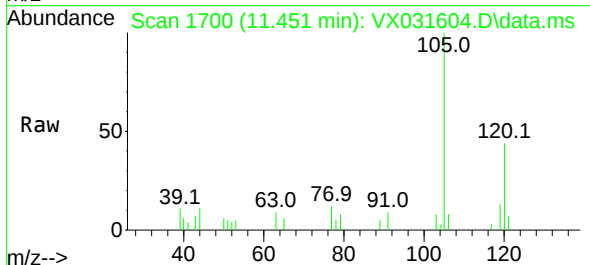




#81
trans-1,4-Dichloro-2-butene
Concen: 124.423 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion: 75 Resp: 49755
Ion Ratio Lower Upper
75 100
53 0.0 77.6 116.4#
89 0.0 37.4 56.0#

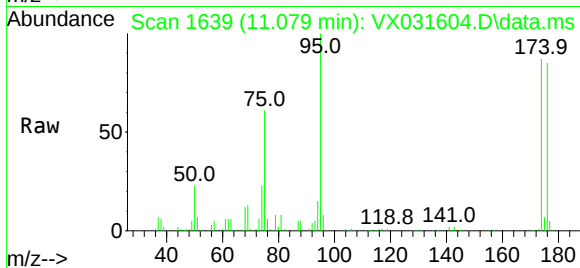

#84
1,2,4-Trimethylbenzene
Concen: 2.111 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Tgt Ion: 105 Resp: 7601
Ion Ratio Lower Upper
105 100
120 28.1 22.6 67.8


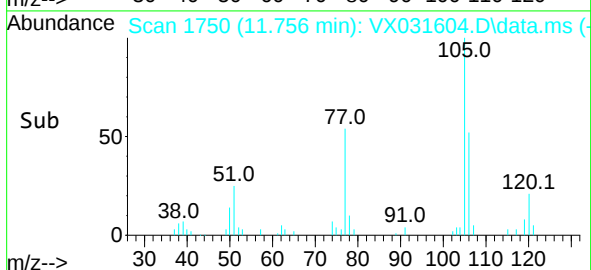

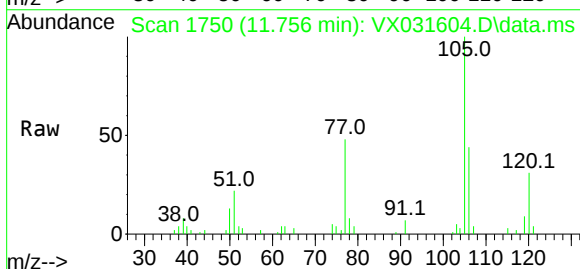


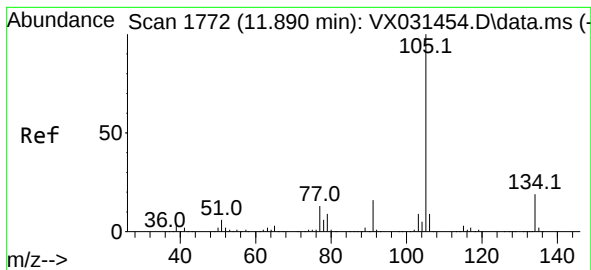

#85
sec-Butylbenzene
Concen: 1.695 ug/l
RT: 11.756 min Scan# 11
Delta R.T. -0.134 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40




Instrument :
MSVOA_X
ClientSampleId :
SB-16


Tgt Ion:105 Resp: 7601
Ion Ratio Lower Upper
105 100
134 0.0 10.4 31.1#

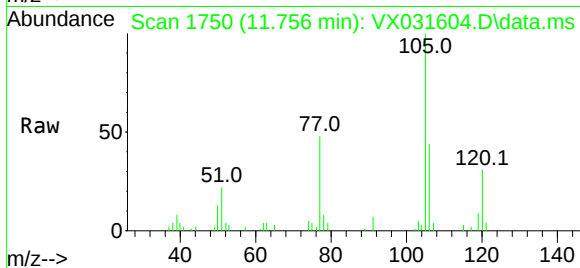

#90
Hexachloroethane
Concen: 4.079 ug/l
RT: 12.414 min Scan# 1858
Delta R.T. -0.128 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40


Tgt Ion:117 Resp: 2654
Ion Ratio Lower Upper
117 100
201 0.0 34.8 104.4#

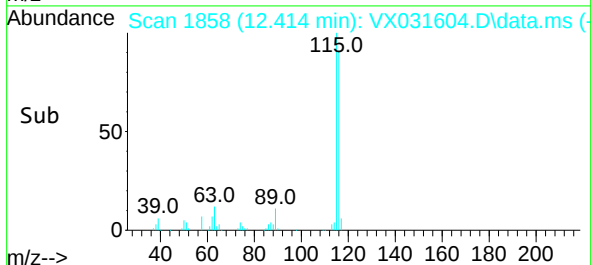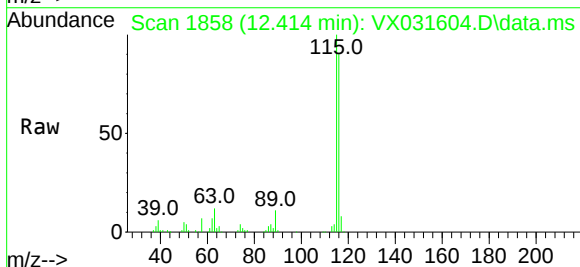



#95
Naphthalene
Concen: 18.464 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX031604.D
Acq: 23 Sep 2022 05:40

Instrument :
MSVOA_X
ClientSampleId :
SB-16

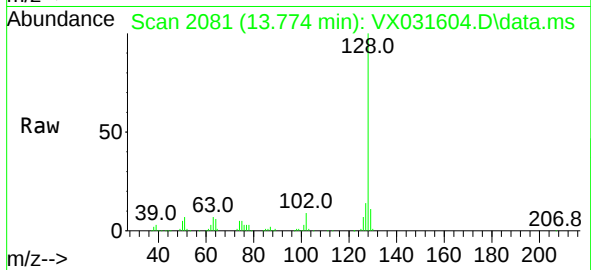

Tgt Ion:128 Resp: 76362
Ion Ratio Lower Upper
128 100
127 13.0 10.4 15.6
129 10.7 8.8 13.2

