

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
 Data File : VX031581.D
 Acq On : 22 Sep 2022 19:28
 Operator : JC/MD
 Sample : N4614-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-23R

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
 Title : SW846 8260

Signal : TIC: VX031581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.337	199	205	211	rBV3	3919	7803	1.24%	0.279%
2	2.782	268	278	285	rBV2	7037	15200	2.41%	0.543%
3	5.385	695	705	722	rBV2	74336	214928	34.03%	7.680%
4	5.550	722	732	754	rVB	73234	215452	34.11%	7.699%
5	5.958	787	799	808	rBV	87397	215524	34.12%	7.702%
6	6.044	808	813	824	rVB4	6731	17997	2.85%	0.643%
7	6.251	833	847	858	rBV7	8670	29401	4.65%	1.051%
8	6.763	922	931	941	rBV2	112729	266906	42.25%	9.538%
9	8.110	1146	1152	1156	rBV3	4751	9114	1.44%	0.326%
10	8.507	1213	1217	1225	rVB3	5810	9872	1.56%	0.353%
11	8.653	1230	1241	1258	rVB	398056	631657	100.00%	22.572%
12	8.842	1265	1272	1281	rVB4	5178	9050	1.43%	0.323%
13	8.958	1287	1291	1300	rVB3	7922	13089	2.07%	0.468%
14	9.049	1300	1306	1312	rBV	8651	13173	2.09%	0.471%
15	10.055	1462	1471	1478	rBV	248746	333017	52.72%	11.900%
16	10.964	1616	1620	1625	rBV	7931	8881	1.41%	0.317%
17	11.079	1634	1639	1649	rVB	324964	409509	64.83%	14.633%
18	12.024	1788	1794	1802	rBV	248172	308512	48.84%	11.024%
19	12.250	1826	1831	1837	rBV	7571	10026	1.59%	0.358%
20	12.646	1893	1896	1901	rVB2	6932	8361	1.32%	0.299%
21	13.170	1979	1982	1993	rVB2	8155	11068	1.75%	0.396%
22	13.292	1998	2002	2008	rVB	12517	15666	2.48%	0.560%
23	13.640	2053	2059	2060	rVV2	5361	8111	1.28%	0.290%
24	13.664	2060	2063	2072	rVB	13169	16124	2.55%	0.576%




Sum of corrected areas: 2798441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031581.D
Acq On : 22 Sep 2022 19:28
Operator : JC/MD
Sample : N4614-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

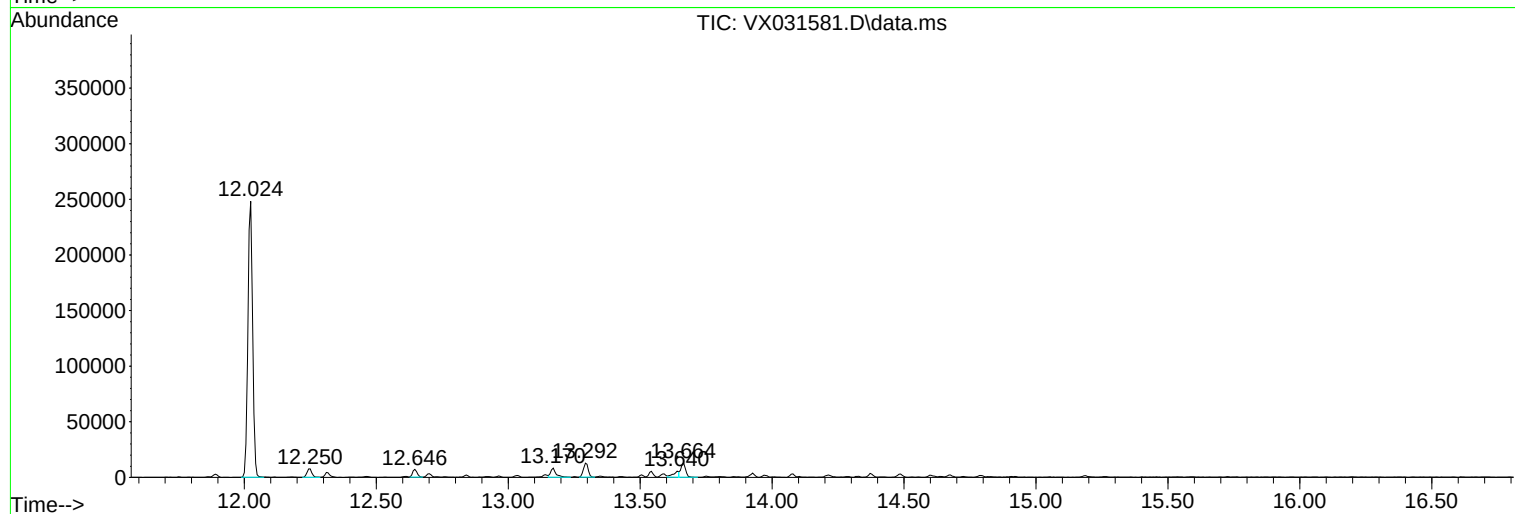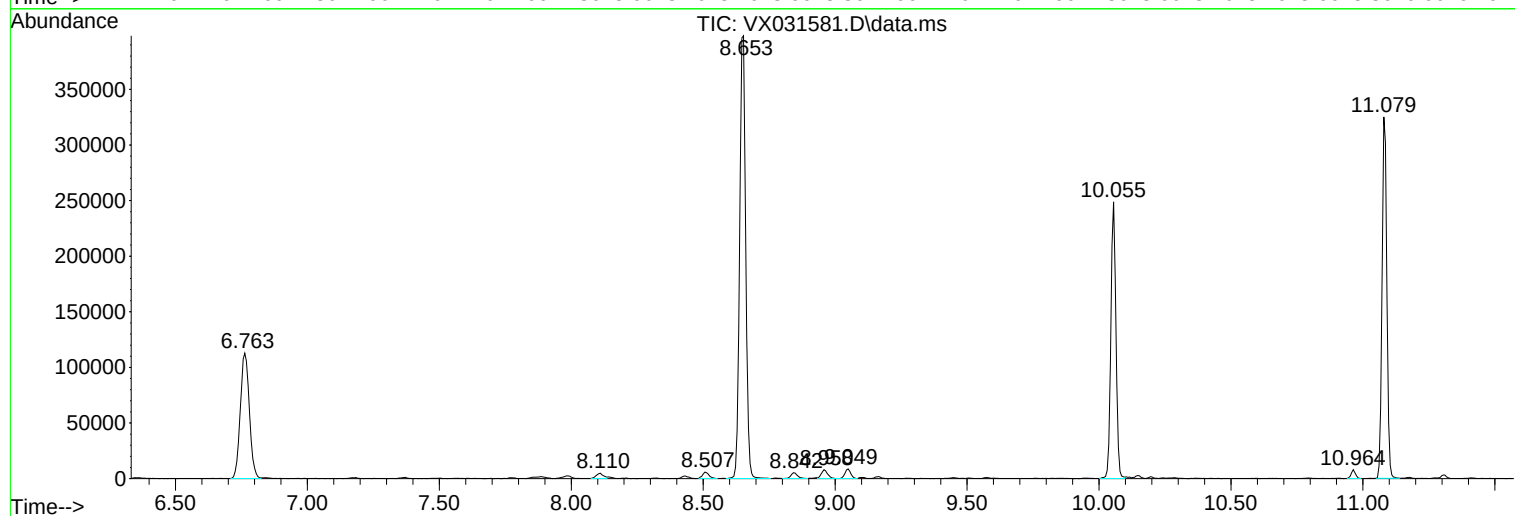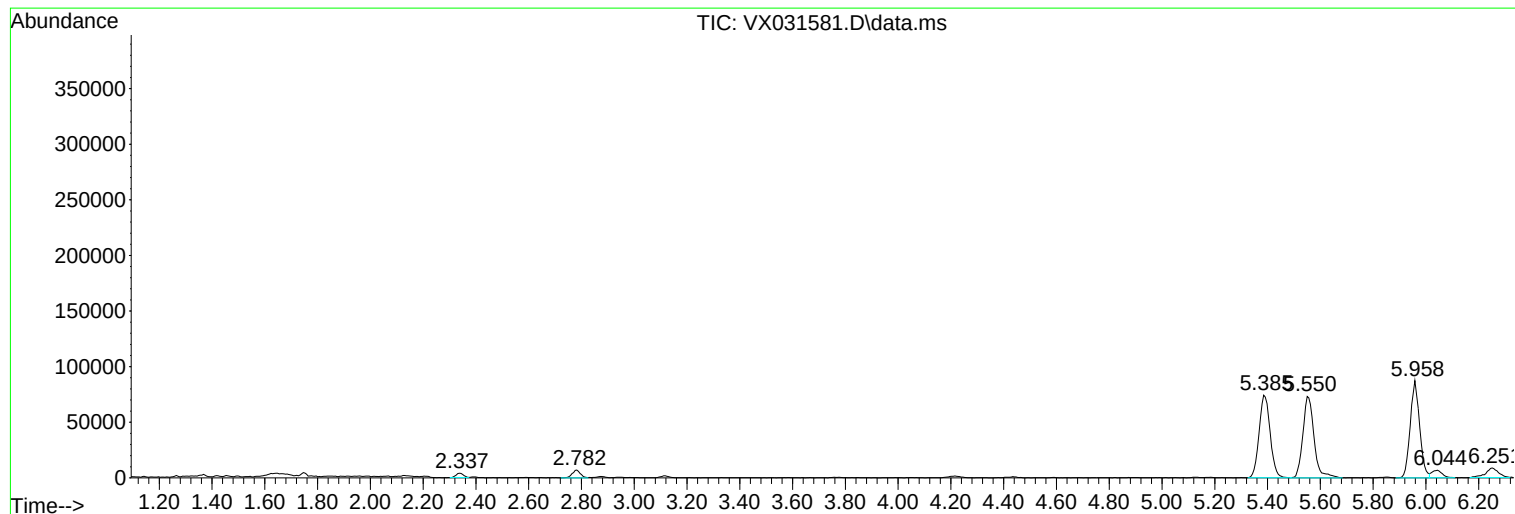

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031581.D
Acq On : 22 Sep 2022 19:28
Operator : JC/MD
Sample : N4614-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.251 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.251	5.51 ug/l	29401	1,4-Difluorobenzene	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2(3H)-Furanone, dihydro-5,5-dime...	114	C6H10O2	003123-97-5	38		
2	Pentane, 1-ethoxy-	116	C7H16O	017952-11-3	35		
3	Cyclopropane, 1,1-dimethyl-	70	C5H10	001630-94-0	27		
4	Carbamic acid, (cyanomethyl)-, 1...	156	C7H12N2O2	085363-04-8	23		
5	1-Butene, 3-methyl-	70	C5H10	000563-45-1	16		

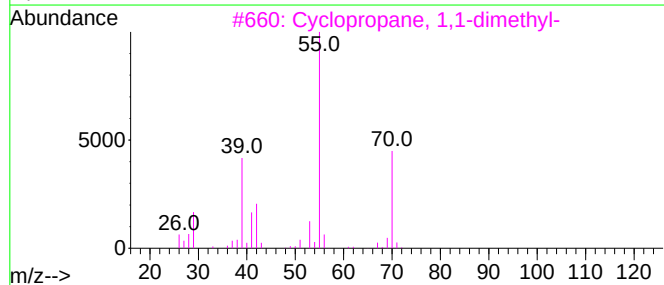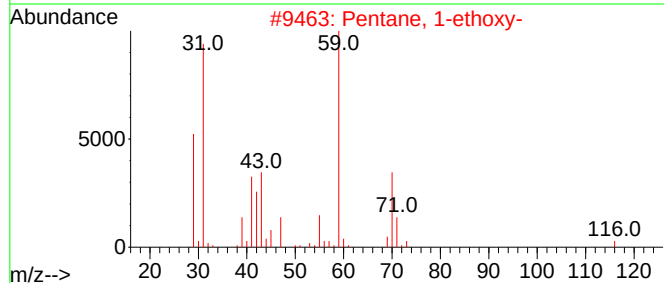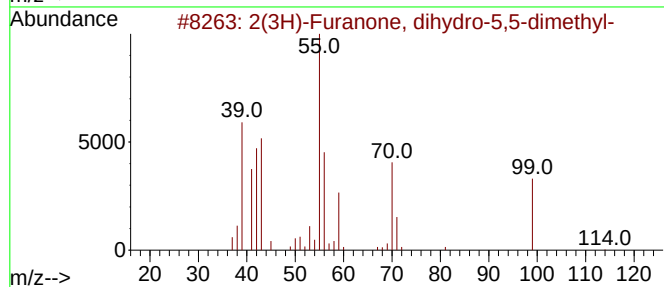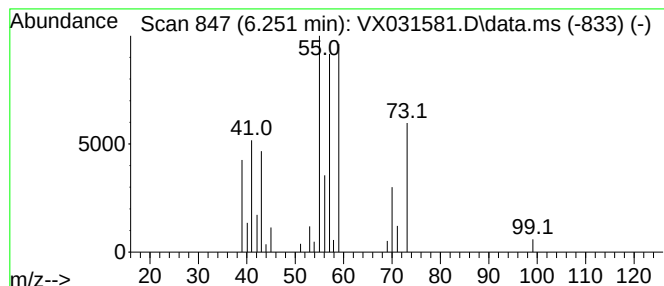

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092222\
Data File : VX031581.D
Acq On : 22 Sep 2022 19:28
Operator : JC/MD
Sample : N4614-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-23R

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091922W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.251	6.251	5.5	ug/l	29401	2	6.763	266906	50.0