

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092223\
 Data File : VX037874.D
 Acq On : 22 Sep 2023 13:27
 Operator : JC/MD
 Sample : 04578-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 23 01:24:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	215003	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	371187	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	357267	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	185990	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	137226	48.579	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.160%
35) Dibromofluoromethane	5.391	113	115466	46.491	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.980%
50) Toluene-d8	8.653	98	449593	48.719	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.440%
62) 4-Bromofluorobenzene	11.079	95	168578	50.271	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	100.540%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092223\
Data File : VX037874.D
Acq On : 22 Sep 2023 13:27
Operator : JC/MD
Sample : 04578-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Sep 23 01:24:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




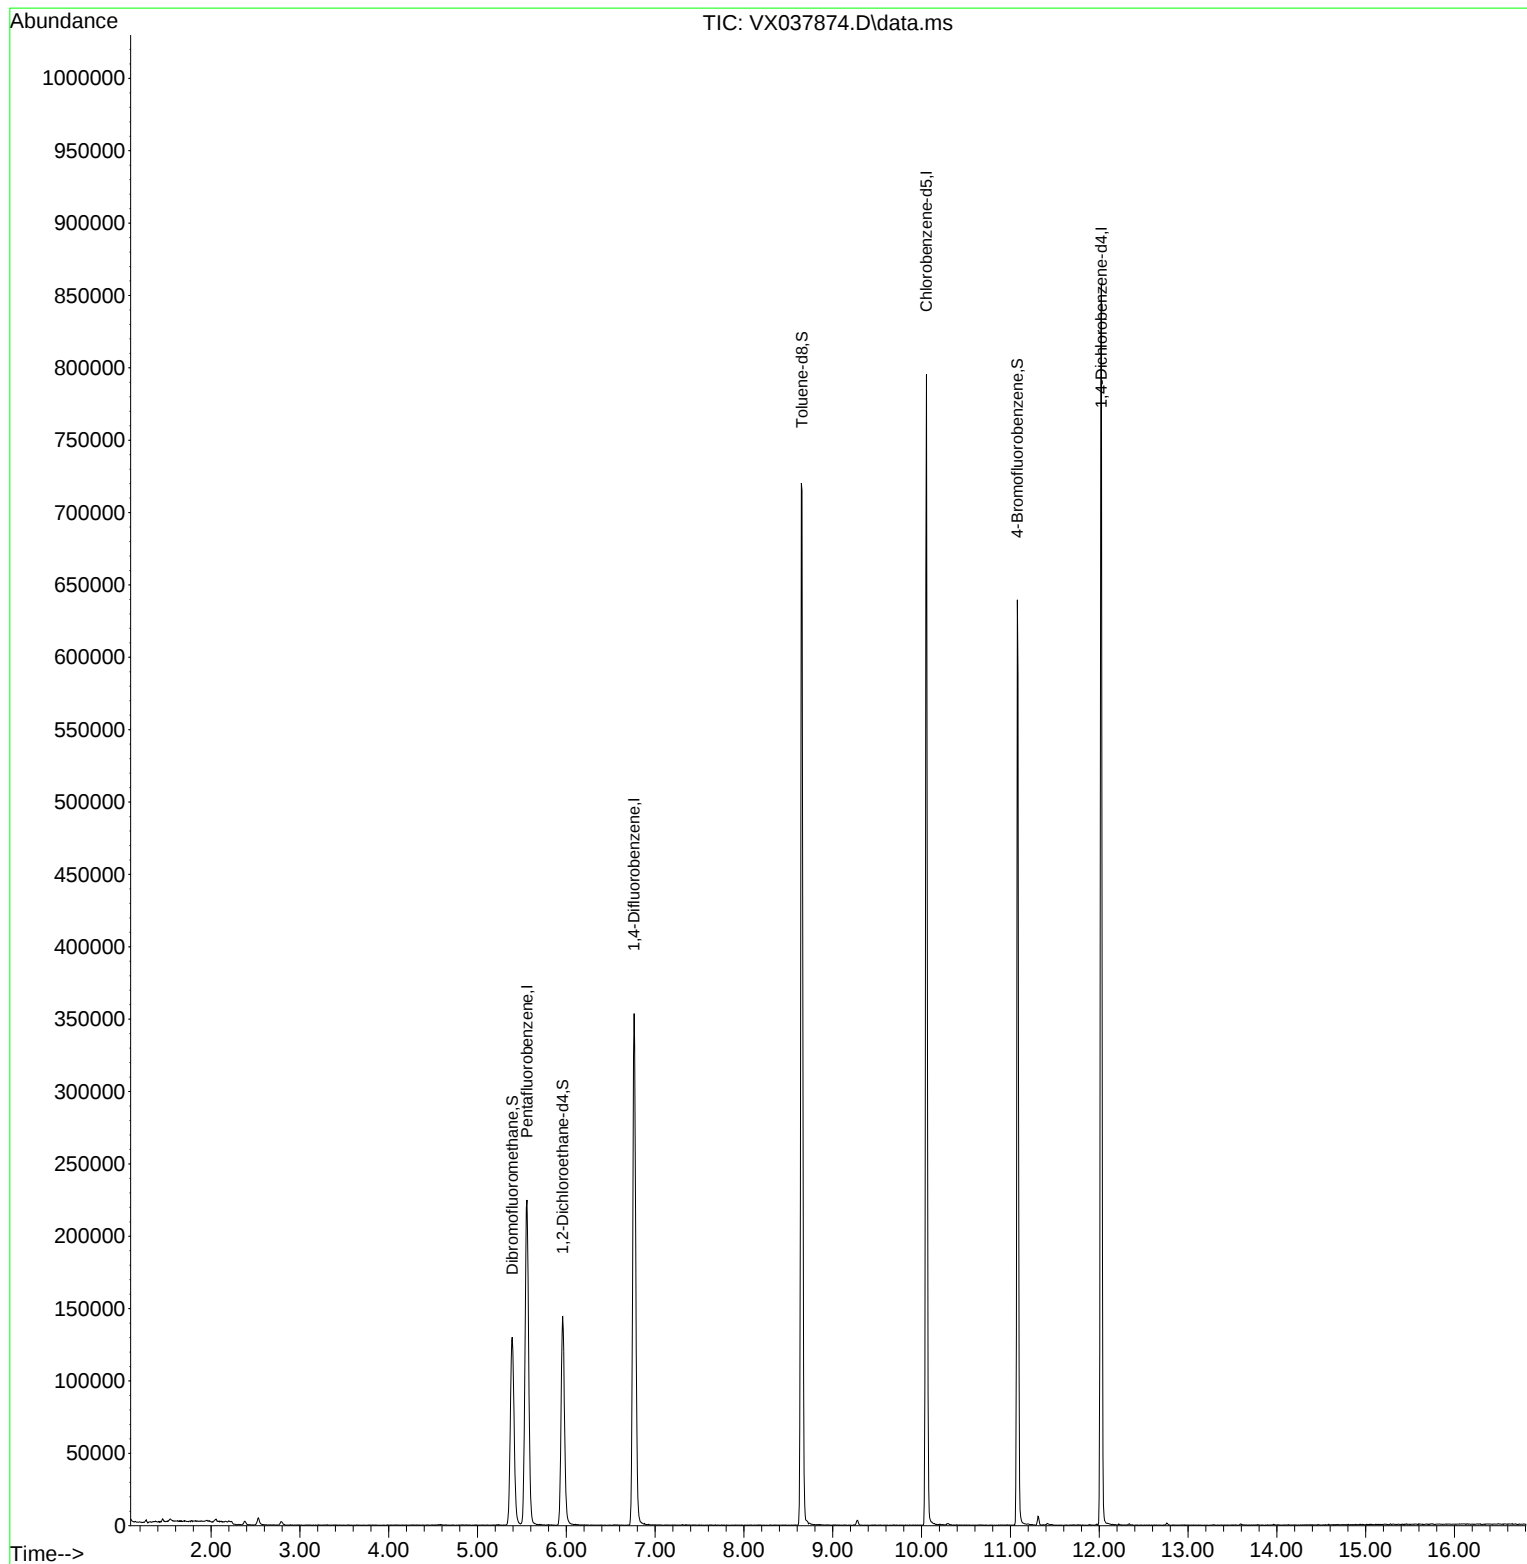




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX037874.D
Acq: 22 Sep 2023 13:27




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:168 Resp: 215003
Ion Ratio Lower Upper
168 100
99 55.2 56.6 85.0#

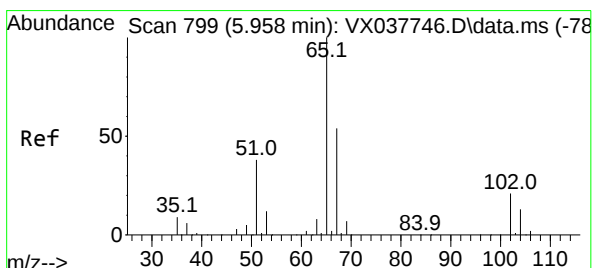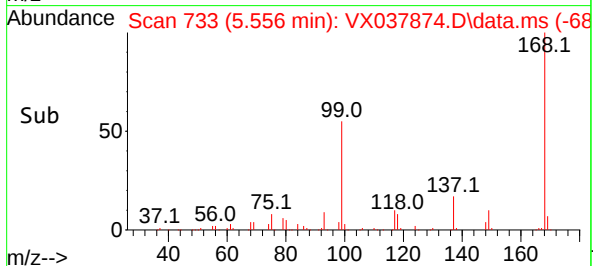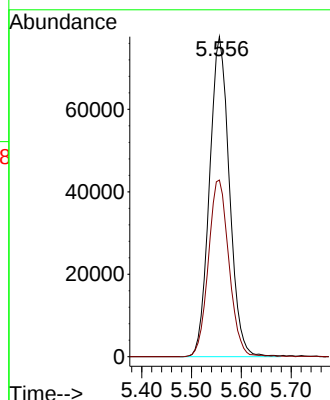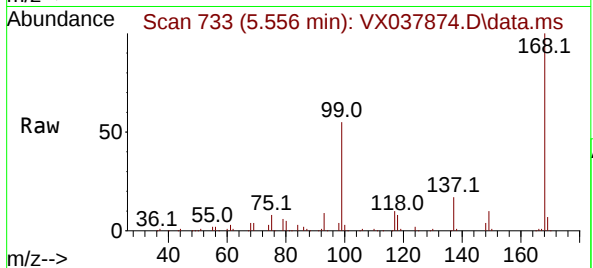

#33
1,2-Dichloroethane-d4
Concen: 48.579 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037874.D
Acq: 22 Sep 2023 13:27

Tgt Ion: 65 Resp: 137226
Ion Ratio Lower Upper
65 100
67 52.8 0.0 100.2

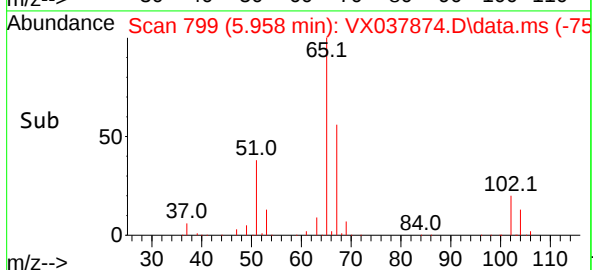
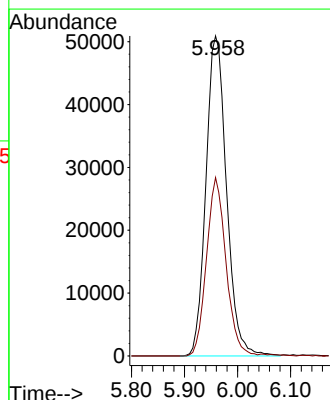
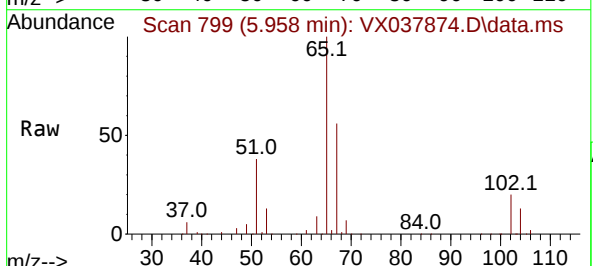




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX037874.D
Acq: 22 Sep 2023 13:27




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 371187
Ion Ratio Lower Upper
114 100
63 19.3 0.0 45.0
88 15.5 0.0 36.6

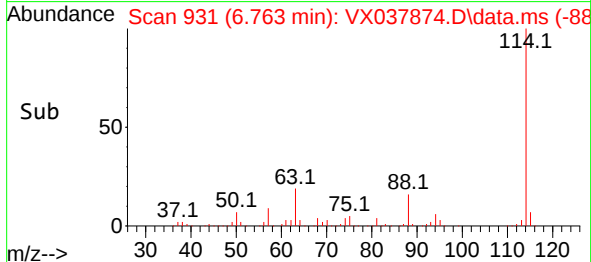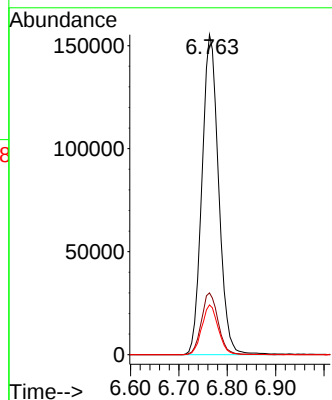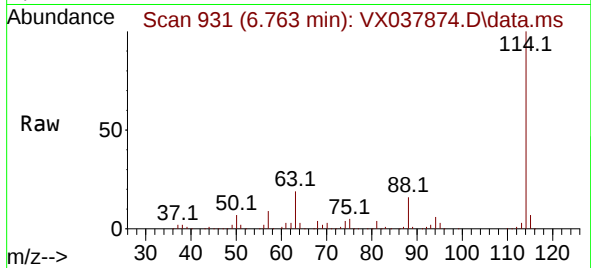

#35
Dibromofluoromethane
Concen: 46.491 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX037874.D
Acq: 22 Sep 2023 13:27

Tgt Ion:113 Resp: 115466
Ion Ratio Lower Upper
113 100
111 103.5 82.9 124.3
192 19.4 13.3 19.9

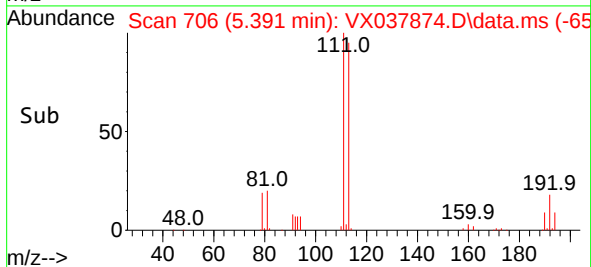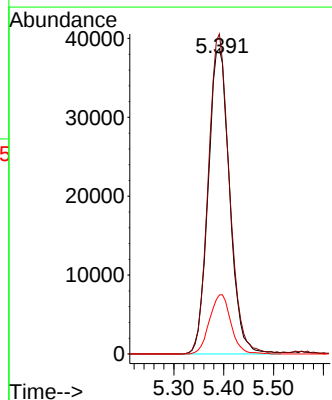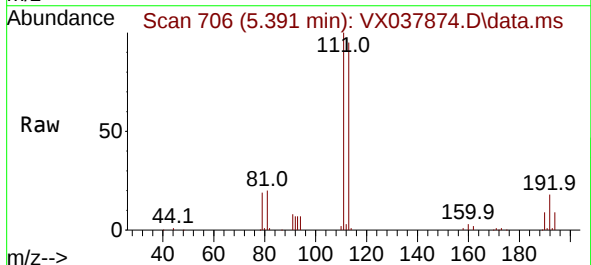

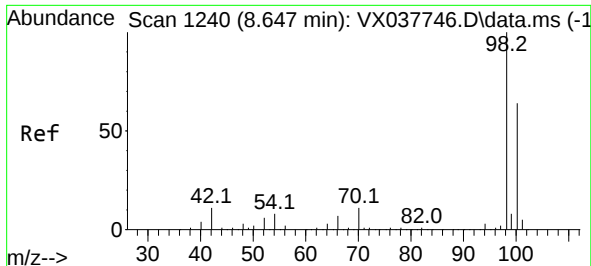

#50

Toluene-d8

Concen: 48.719 ug/l

RT: 8.653 min Scan# 11

Delta R.T. 0.006 min

Lab File: VX037874.D

Acq: 22 Sep 2023 13:27

Instrument :

MSVOA_X

ClientSampleId :





STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion: 98 Resp: 449593

Ion Ratio Lower Upper

98 100

100 64.3 53.1 79.7

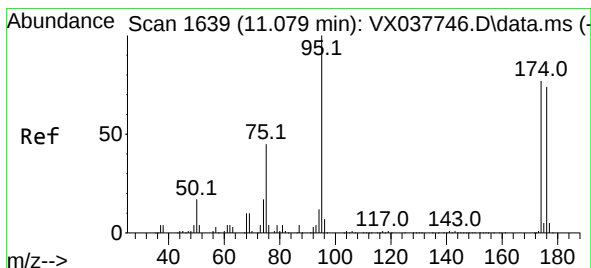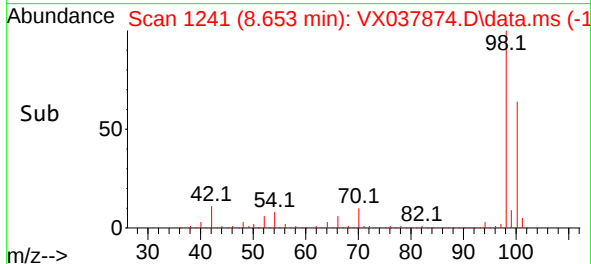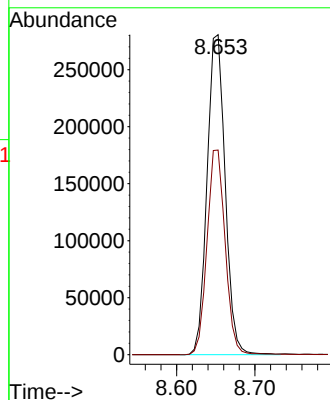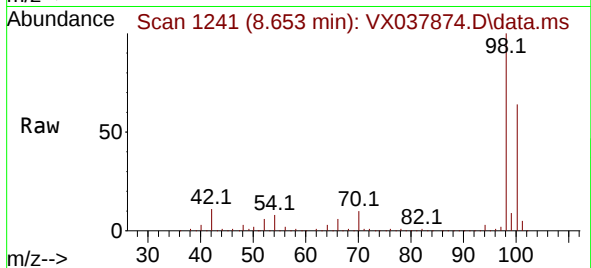

#62

4-Bromofluorobenzene

Concen: 50.271 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX037874.D

Acq: 22 Sep 2023 13:27




Tgt Ion: 95 Resp: 168578

Ion Ratio Lower Upper

95 100

174 80.6 0.0 135.6

176 77.4 0.0 131.0

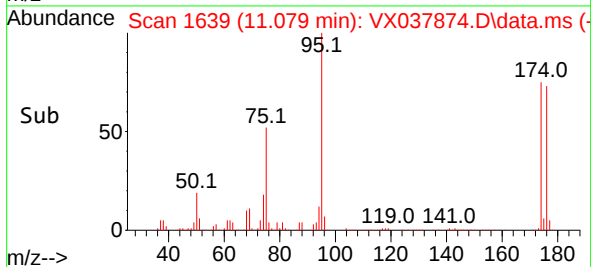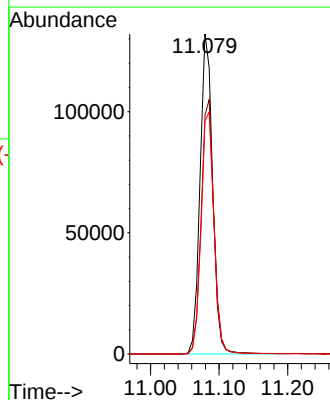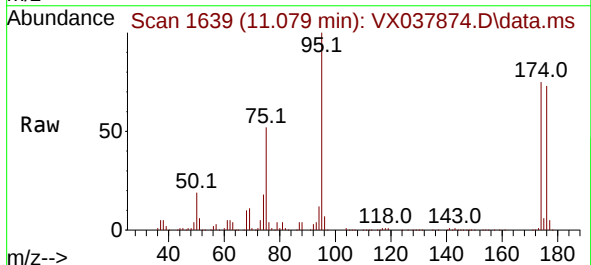



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. -0.000 min

Lab File: VX037874.D

Acq: 22 Sep 2023 13:27

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANAG





Tgt Ion:117 Resp: 357267

Ion Ratio Lower Upper

117 100

82 54.1 46.2 69.4

119 31.8 25.5 38.3

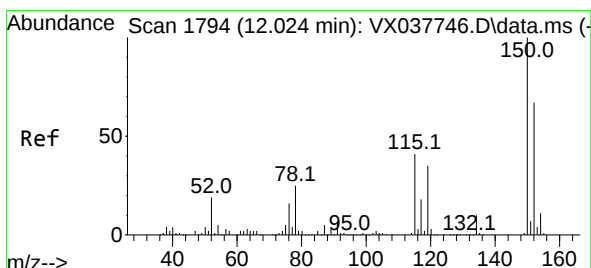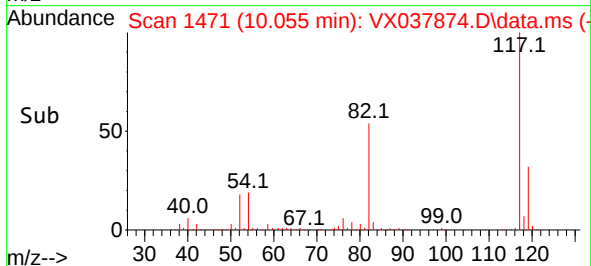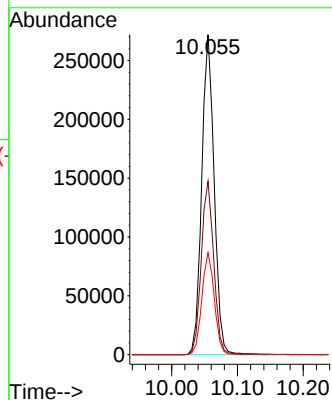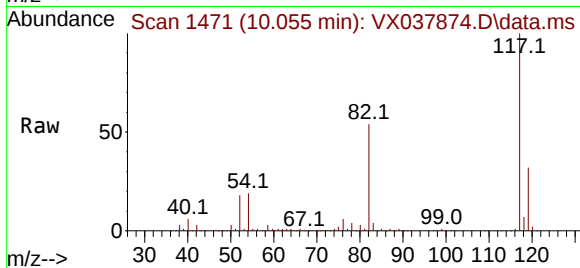

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. -0.000 min

Lab File: VX037874.D

Acq: 22 Sep 2023 13:27

Tgt Ion:152 Resp: 185990

Ion Ratio Lower Upper

152 100

115 59.4 43.3 129.9

150 155.5 0.0 345.0

