

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092223\  
Data File : VX037873.D  
Acq On : 22 Sep 2023 13:04  
Operator : JC/MD  
Sample : 04578-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M

Title : SW846 8260

Signal : TIC: VX037873.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.385       | 693           | 705         | 722          | rBV2     | 130327         | 384583        | 32.79%          | 5.990%        |
| 2         | 5.556       | 722           | 733         | 750          | rVB      | 223440         | 636036        | 54.23%          | 9.907%        |
| 3         | 5.958       | 790           | 799         | 815          | rBV      | 142062         | 383470        | 32.70%          | 5.973%        |
| 4         | 6.763       | 921           | 931         | 950          | rBV      | 352310         | 846693        | 72.19%          | 13.188%       |
| 5         | 8.653       | 1234          | 1241        | 1256         | rBV      | 733716         | 1172826       | 100.00%         | 18.268%       |
| 6         | 10.055      | 1465          | 1471        | 1481         | rBV      | 801713         | 1064254       | 90.74%          | 16.577%       |
| 7         | 11.079      | 1634          | 1639        | 1654         | rBV      | 644989         | 825151        | 70.36%          | 12.853%       |
| 8         | 12.024      | 1788          | 1794        | 1805         | rBV      | 862077         | 1107101       | 94.40%          | 17.244%       |




Sum of corrected areas: 6420114

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092223\  
Data File : VX037873.D  
Acq On : 22 Sep 2023 13:04  
Operator : JC/MD  
Sample : 04578-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

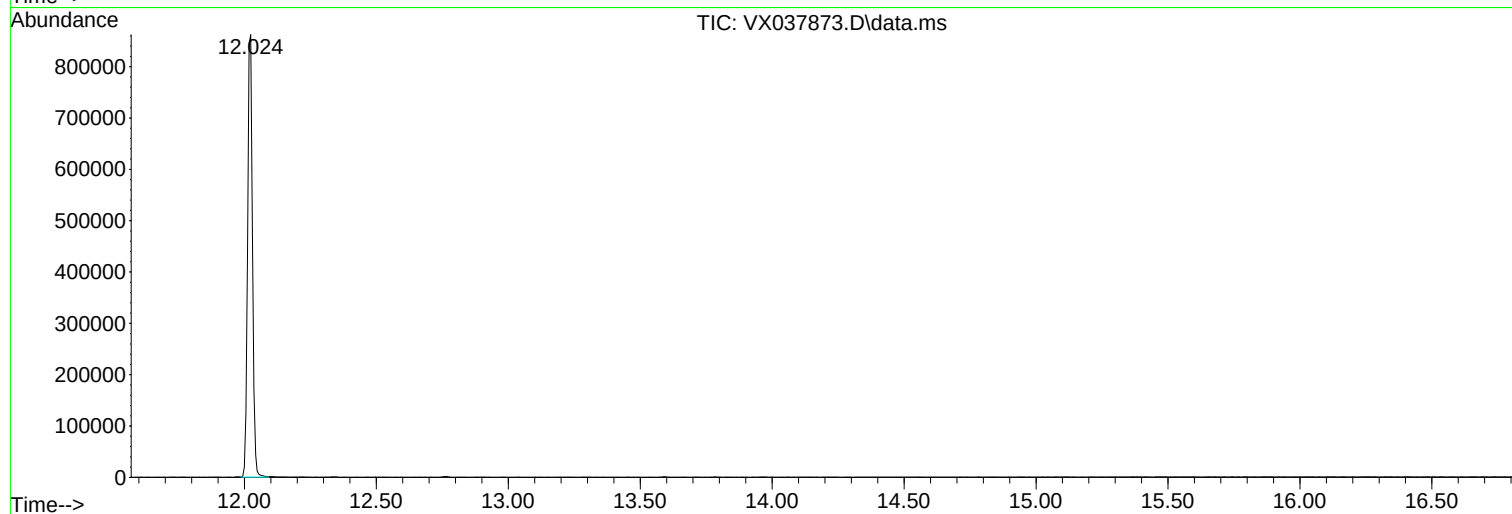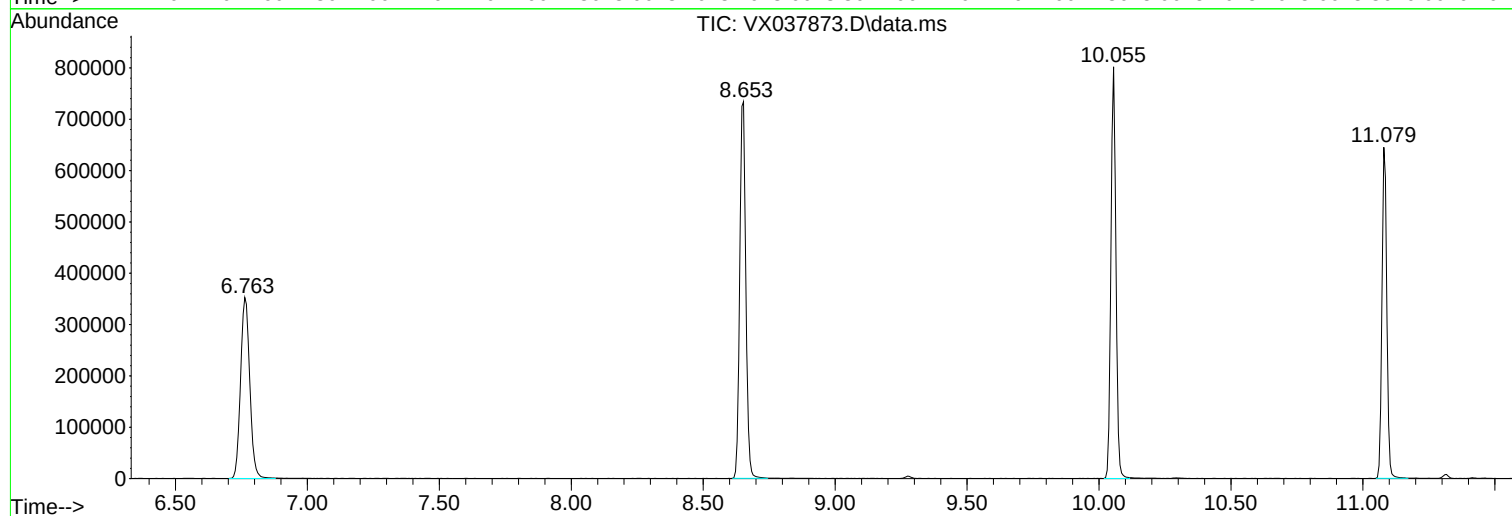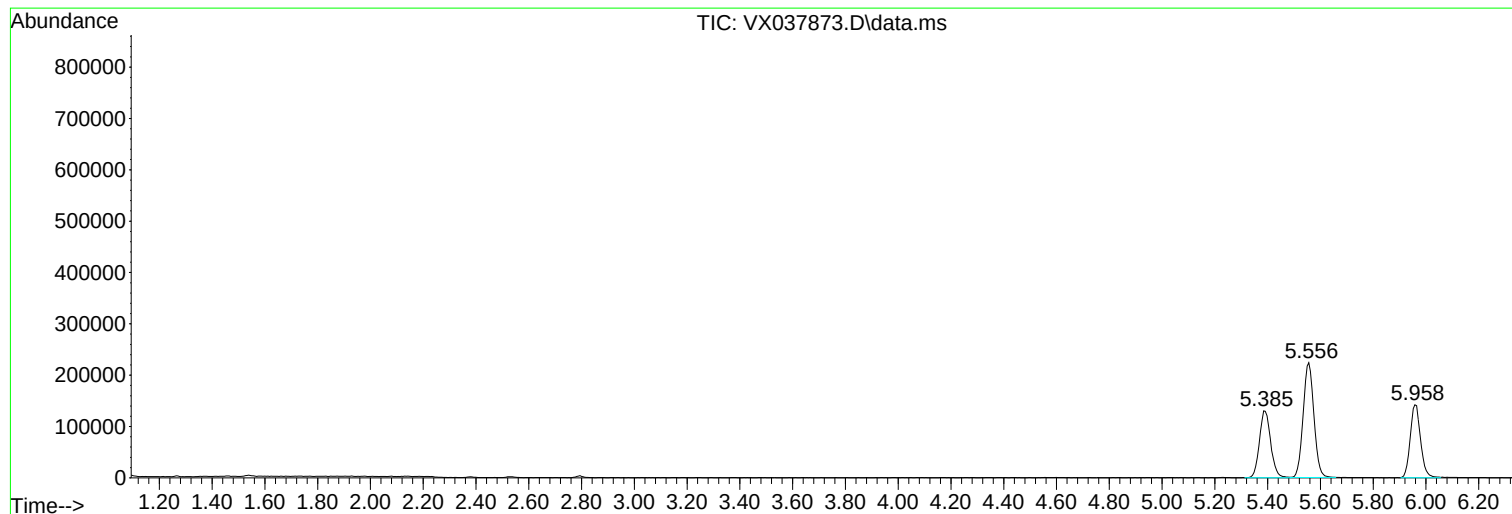

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092223\  
Data File : VX037873.D  
Acq On : 22 Sep 2023 13:04  
Operator : JC/MD  
Sample : 04578-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX092223\  
Data File : VX037873.D  
Acq On : 22 Sep 2023 13:04  
Operator : JC/MD  
Sample : 04578-03  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X091523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |