

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092319\
 Data File : VX012606.D
 Acq On : 23 Sep 2019 15:57
 Operator : JC/SP
 Sample : K5000-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.070	26	30	42	rBV	349766	431978	44.85%	7.986%
2	1.265	58	62	69	rBV	26630	34032	3.53%	0.629%
3	2.436	247	254	261	rVB	8597	15188	1.58%	0.281%
4	2.594	275	280	290	rVB	30276	55395	5.75%	1.024%
5	5.490	744	755	769	rBV	104630	298124	30.95%	5.511%
6	5.654	770	782	795	rVV	200521	567479	58.92%	10.491%
7	6.051	838	847	862	rBV	128934	338491	35.14%	6.257%
8	6.849	968	978	992	rBV	301846	724157	75.19%	13.387%
9	8.709	1276	1283	1301	rBV	616383	963152	100.00%	17.805%
10	10.111	1506	1513	1522	rBV	570313	793016	82.34%	14.660%
11	11.135	1675	1681	1690	rBV	428961	558264	57.96%	10.320%
12	12.074	1830	1835	1844	rBV	524943	630157	65.43%	11.649%


Sum of corrected areas: 5409433

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092319\
Data File : VX012606.D
Acq On : 23 Sep 2019 15:57
Operator : JC/SP
Sample : K5000-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

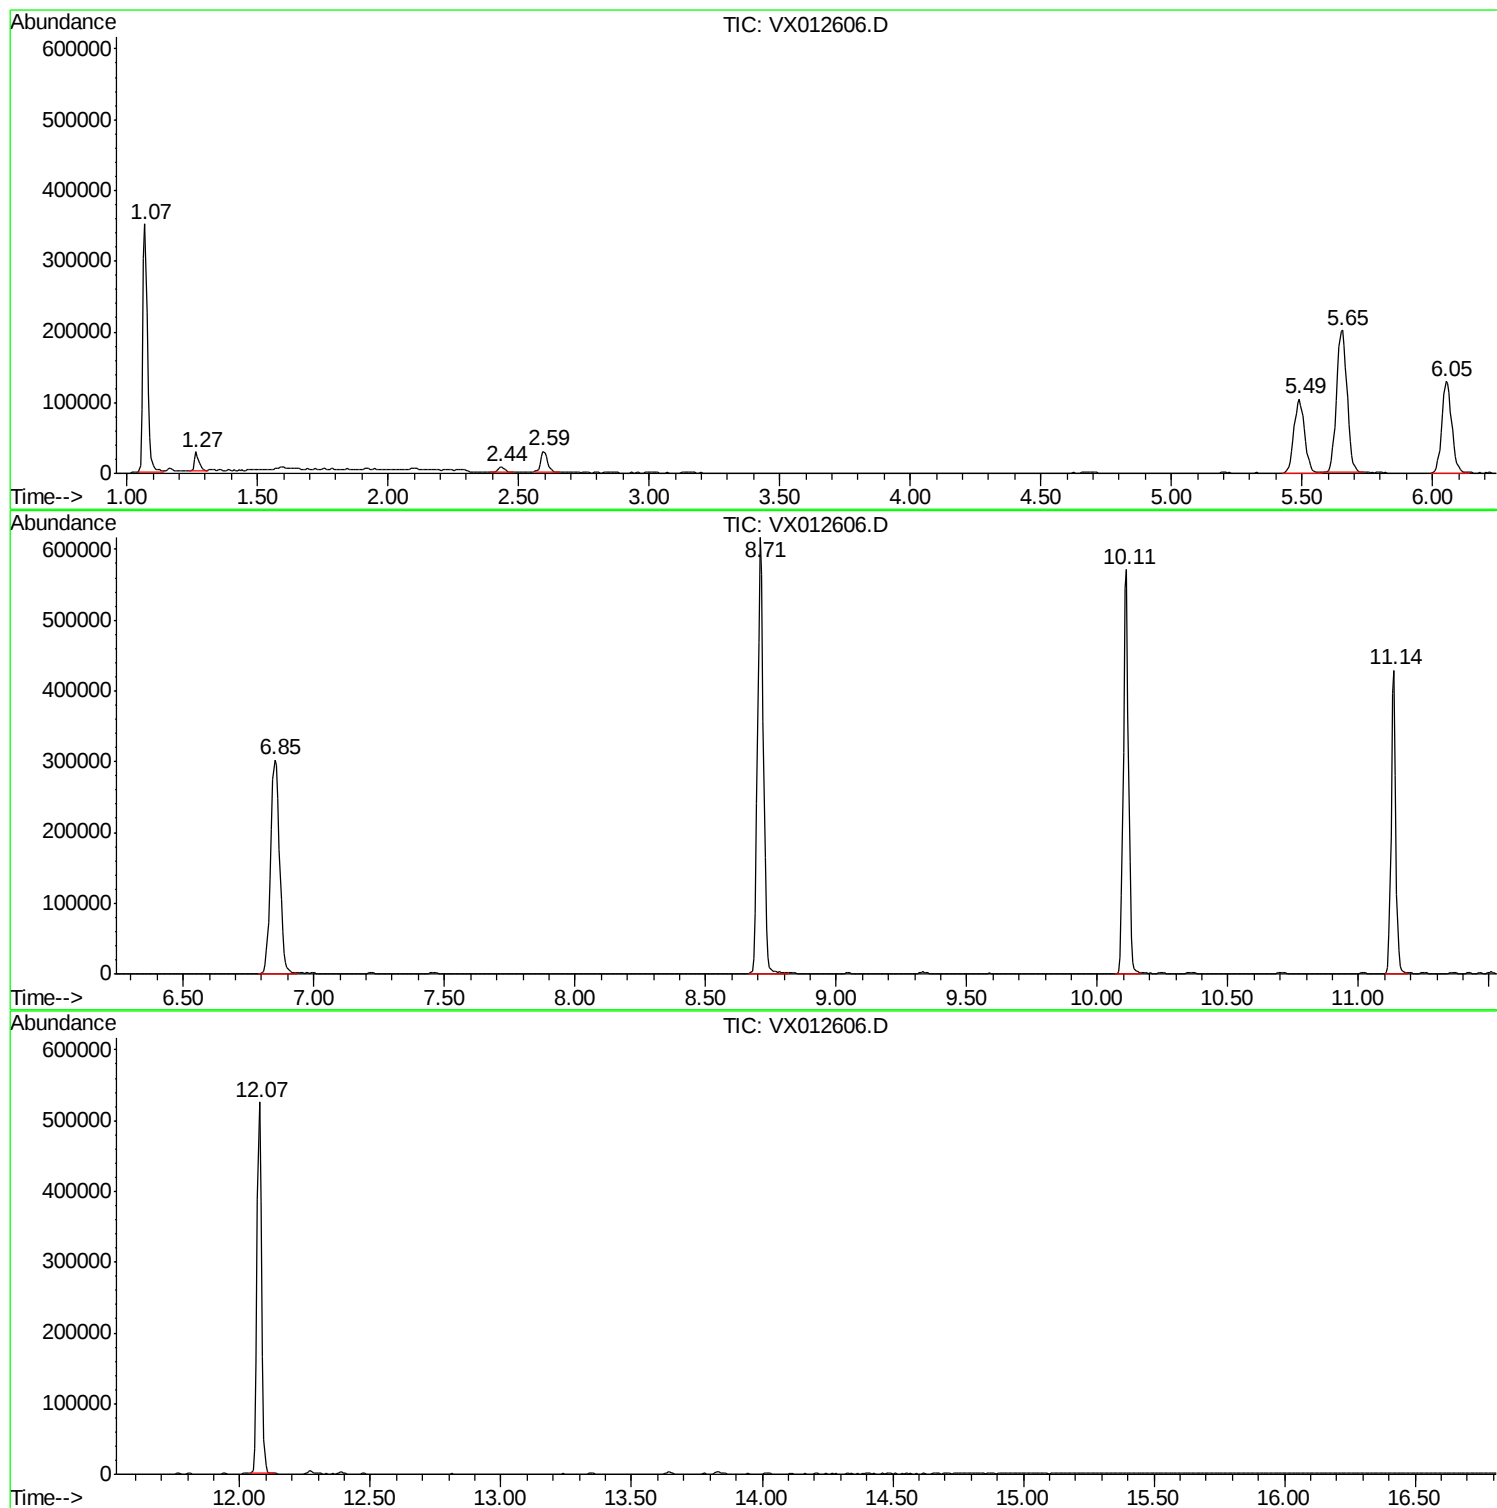

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092319\
Data File : VX012606.D
Acq On : 23 Sep 2019 15:57
Operator : JC/SP
Sample : K5000-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092319\
Data File : VX012606.D
Acq On : 23 Sep 2019 15:57
Operator : JC/SP
Sample : K5000-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
