

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092320\
Data File : VX018547.D
Acq On : 23 Sep 2020 20:15
Operator : JC/SP
Sample : L4120-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMPACTOR-ELECTRICAL-SERVI

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X091720W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	30	33	37	rBV2	34162	32393	1.32%	0.234%
2	2.624	243	252	253	rBV	21016	42816	1.75%	0.309%
3	4.648	579	584	594	rVB	12234	28554	1.16%	0.206%
4	5.471	706	719	730	rBV	305418	883850	36.04%	6.388%
5	5.635	734	746	759	rVV	511839	1444232	58.89%	10.439%
6	6.032	799	811	825	rBV	333342	883497	36.03%	6.386%
7	6.830	930	942	956	rBV	769055	1827039	74.50%	13.206%
8	8.696	1239	1248	1256	rBV	1576627	2452317	100.00%	17.725%
9	10.098	1469	1478	1492	rBV	1655042	2207461	90.02%	15.955%
10	11.000	1620	1626	1632	rVB	71978	94095	3.84%	0.680%
11	11.122	1639	1646	1658	rBV	1392814	1741930	71.03%	12.591%
12	12.061	1795	1800	1810	rVB	1765736	2197061	89.59%	15.880%


Sum of corrected areas: 13835245

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092320\
Data File : VX018547.D
Acq On : 23 Sep 2020 20:15
Operator : JC/SP
Sample : L4120-05
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMPACTOR-ELECTRICAL-SERVI

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

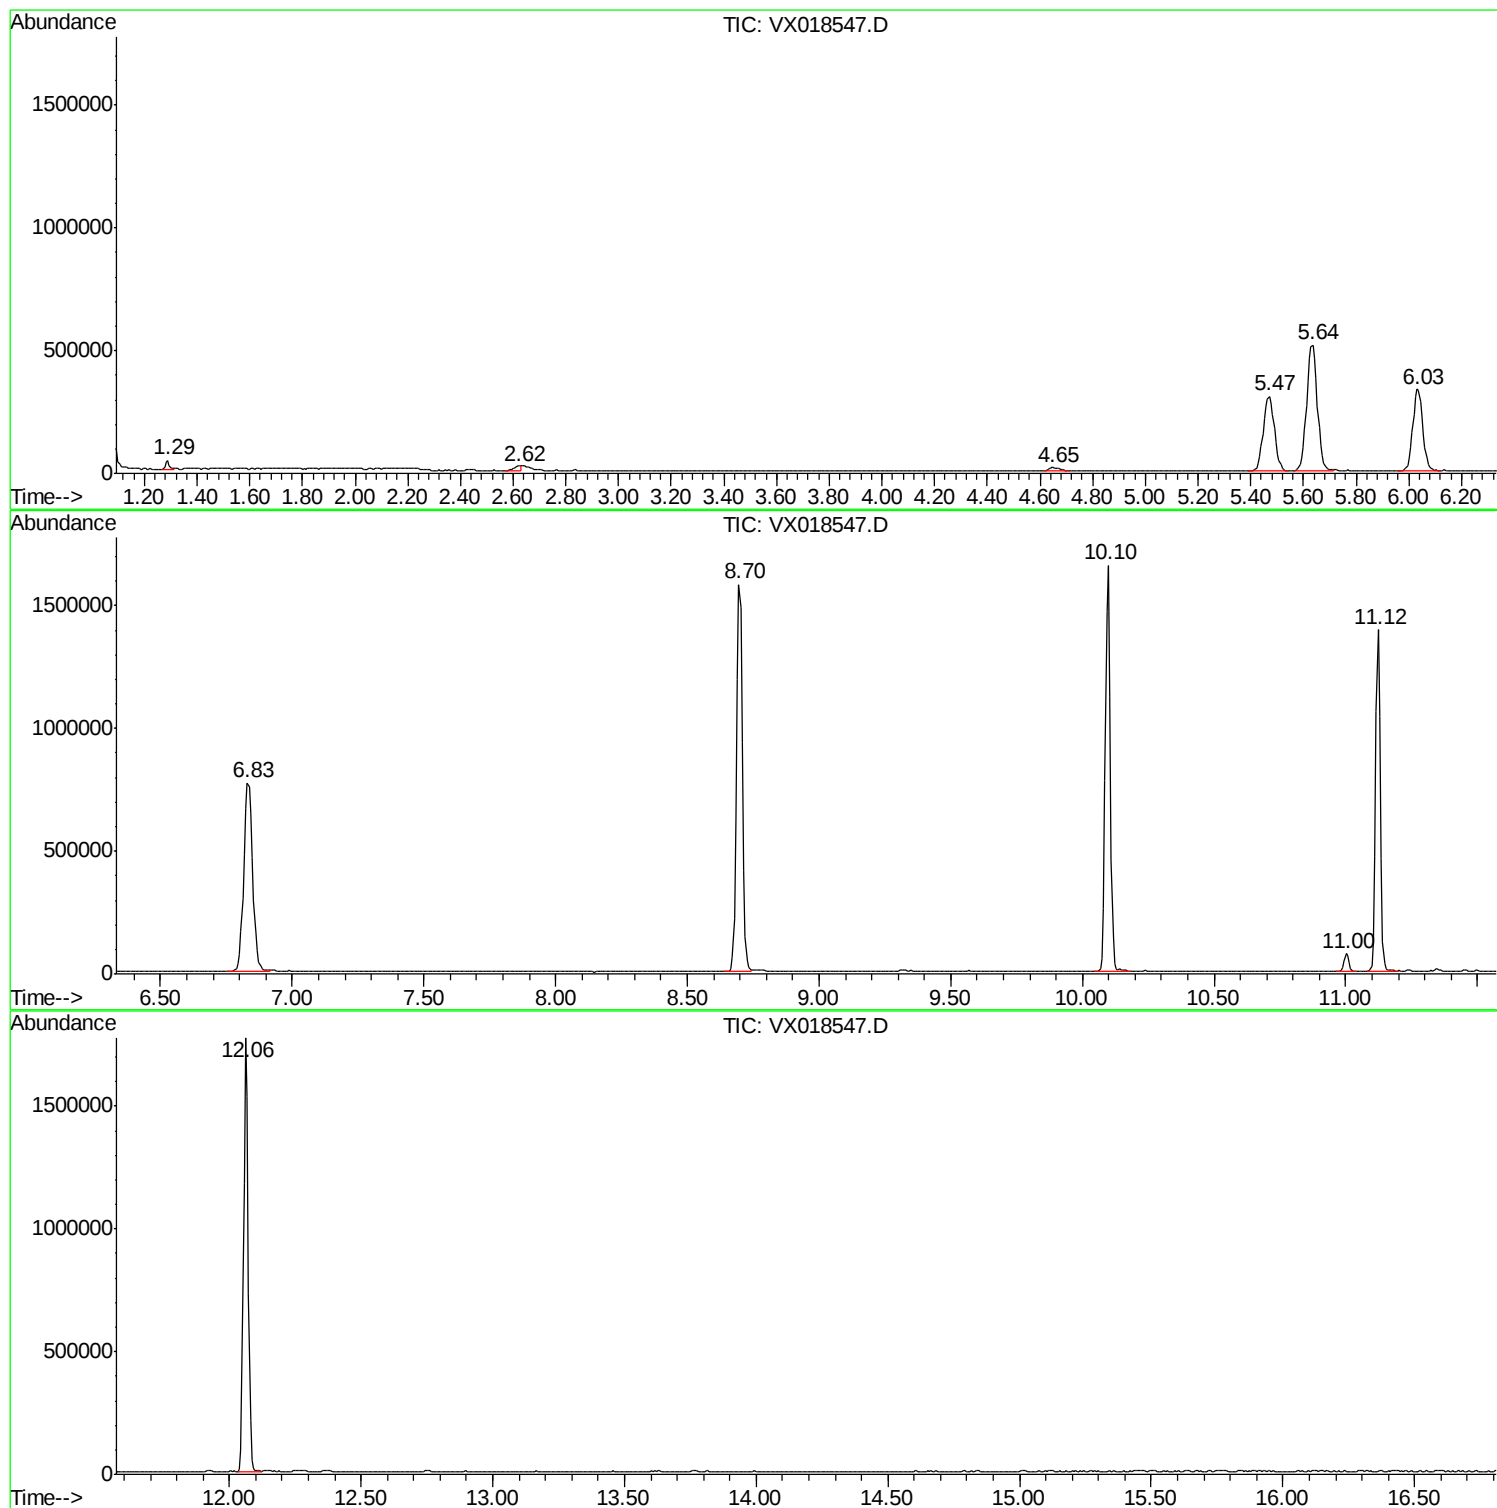

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_X\DATA\VX092320\
Data File : VX018547.D
Acq On : 23 Sep 2020 20:15
Operator : JC/SP
Sample : L4120-05
Misc : 5.0mL/MSV0A_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSV0A_X
ClientSampleId :
COMPACTOR-ELECTRICAL-SERVI

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_X\METHOD\82X091720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX092320\
Data File : VX018547.D
Acq On : 23 Sep 2020 20:15
Operator : JC/SP
Sample : L4120-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMPACTOR-ELECTRICAL-SERVI

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X091720W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc