



Chloroethane

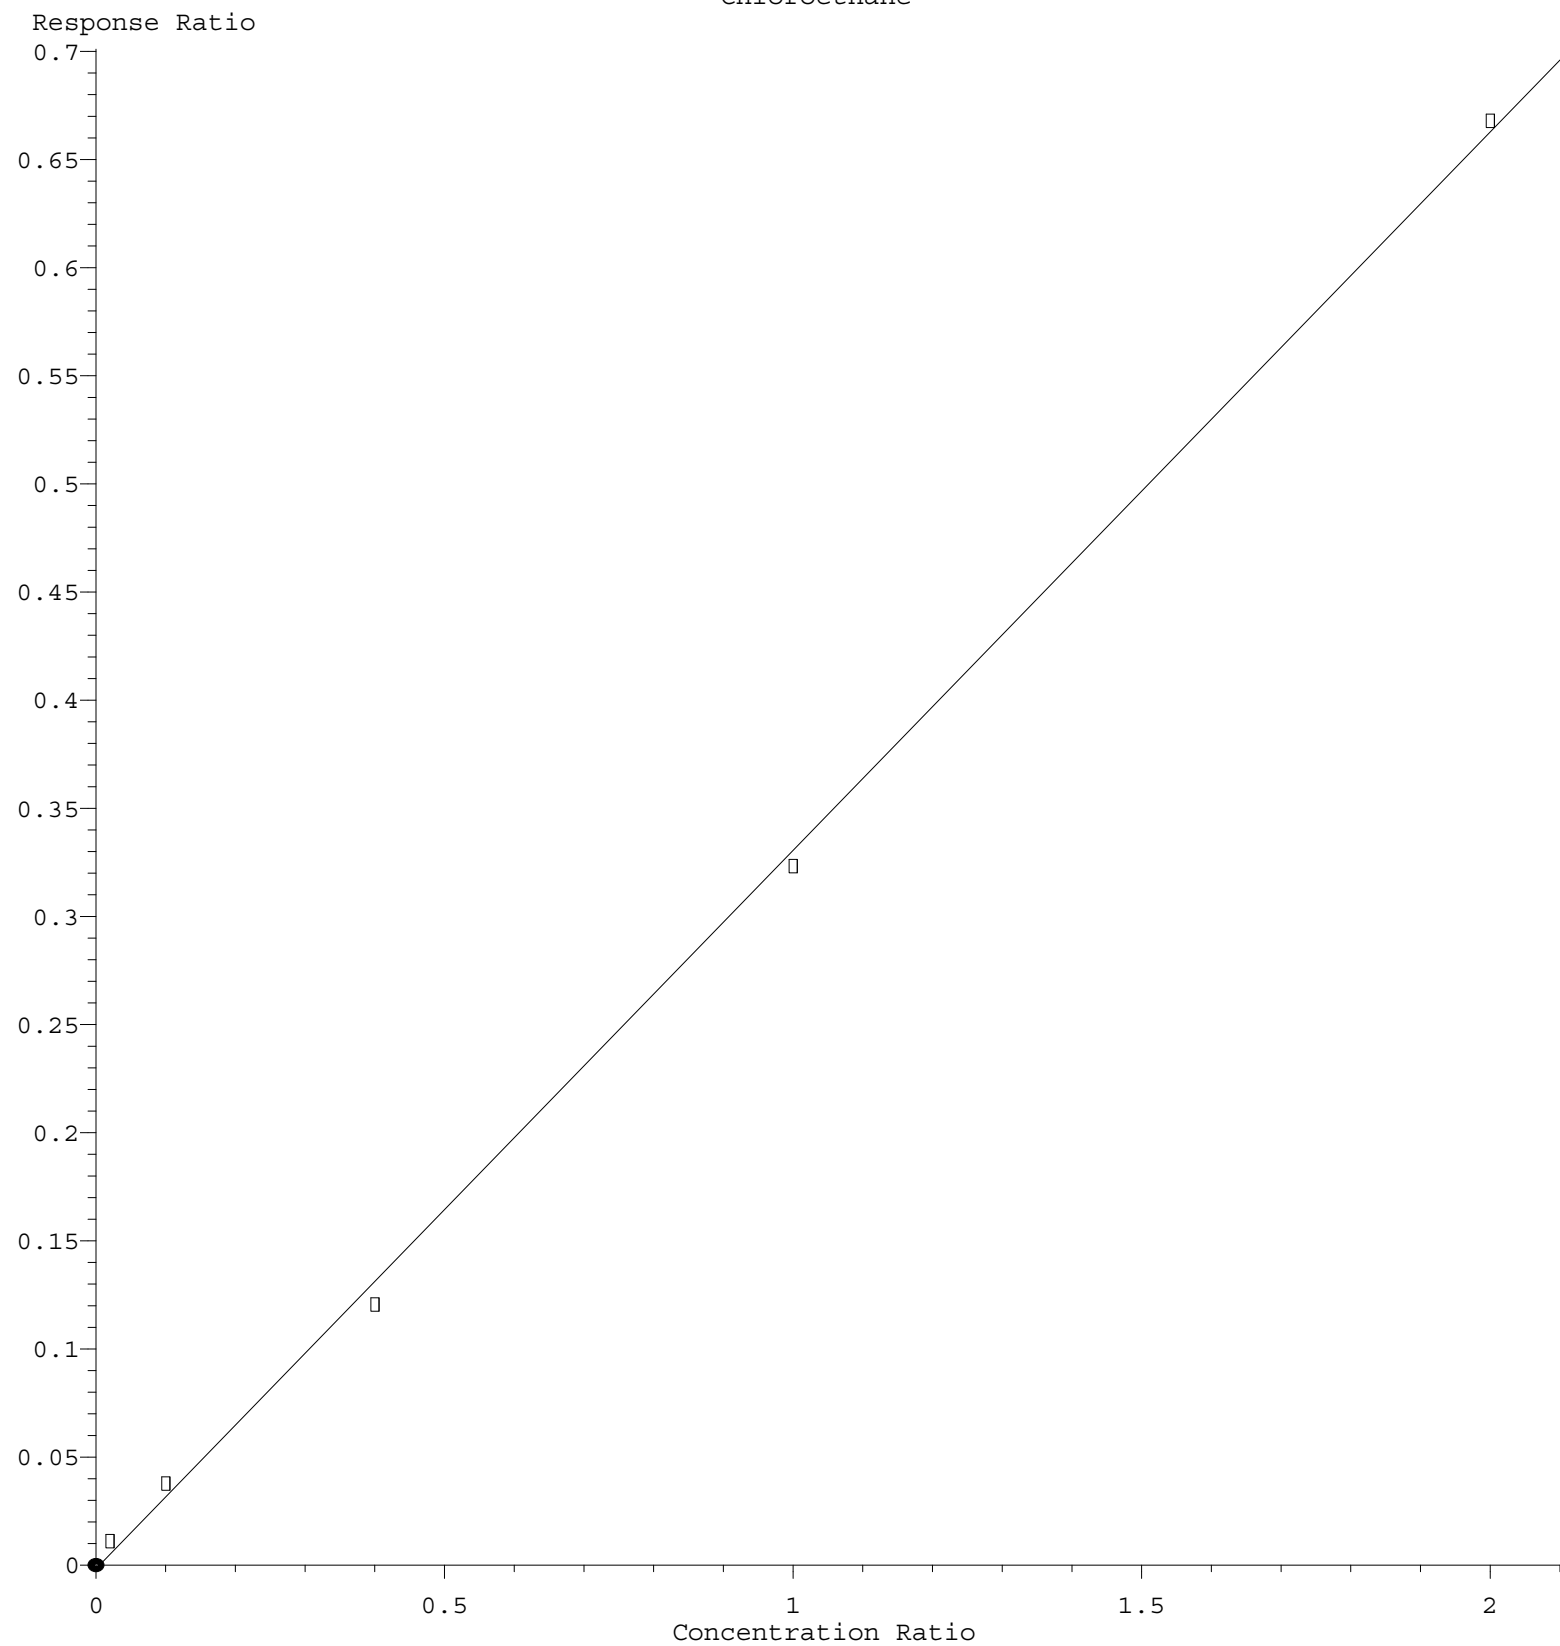

Response = $3.321e-001 * \text{Amt} - 1.716e-003$
 Coef of Det (r^2) = 0.999091 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M
 Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Tert butyl alcohol

Response Ratio

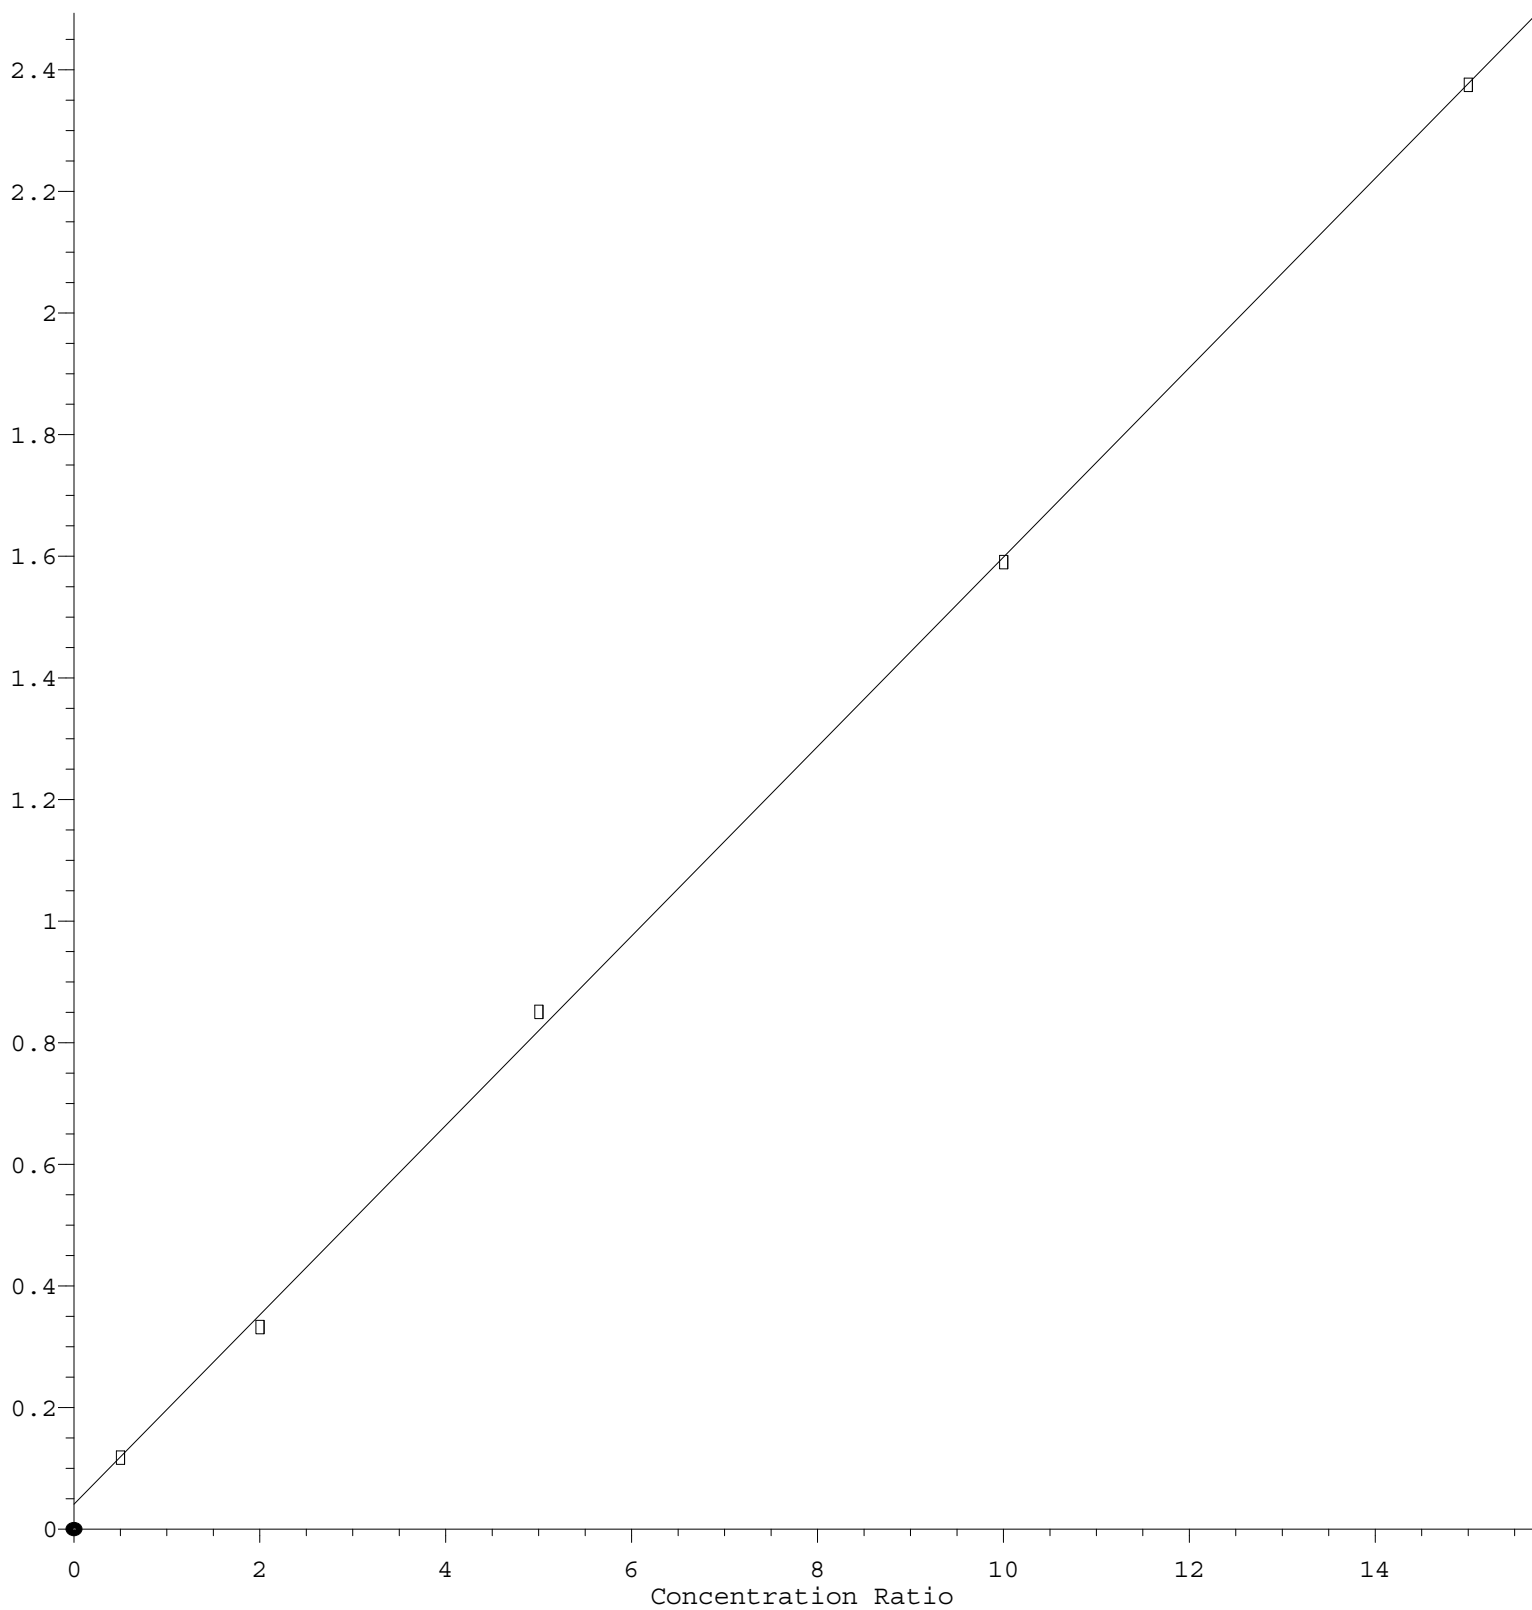


$$\text{Response} = 1.558\text{e-}001 * \text{Amt} + 4.054\text{e-}002$$

Coef of Det (r^2) = 0.999590 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M

Calibration Table Last Updated: Thu Sep 23 18:24:34 2021


Acrolein

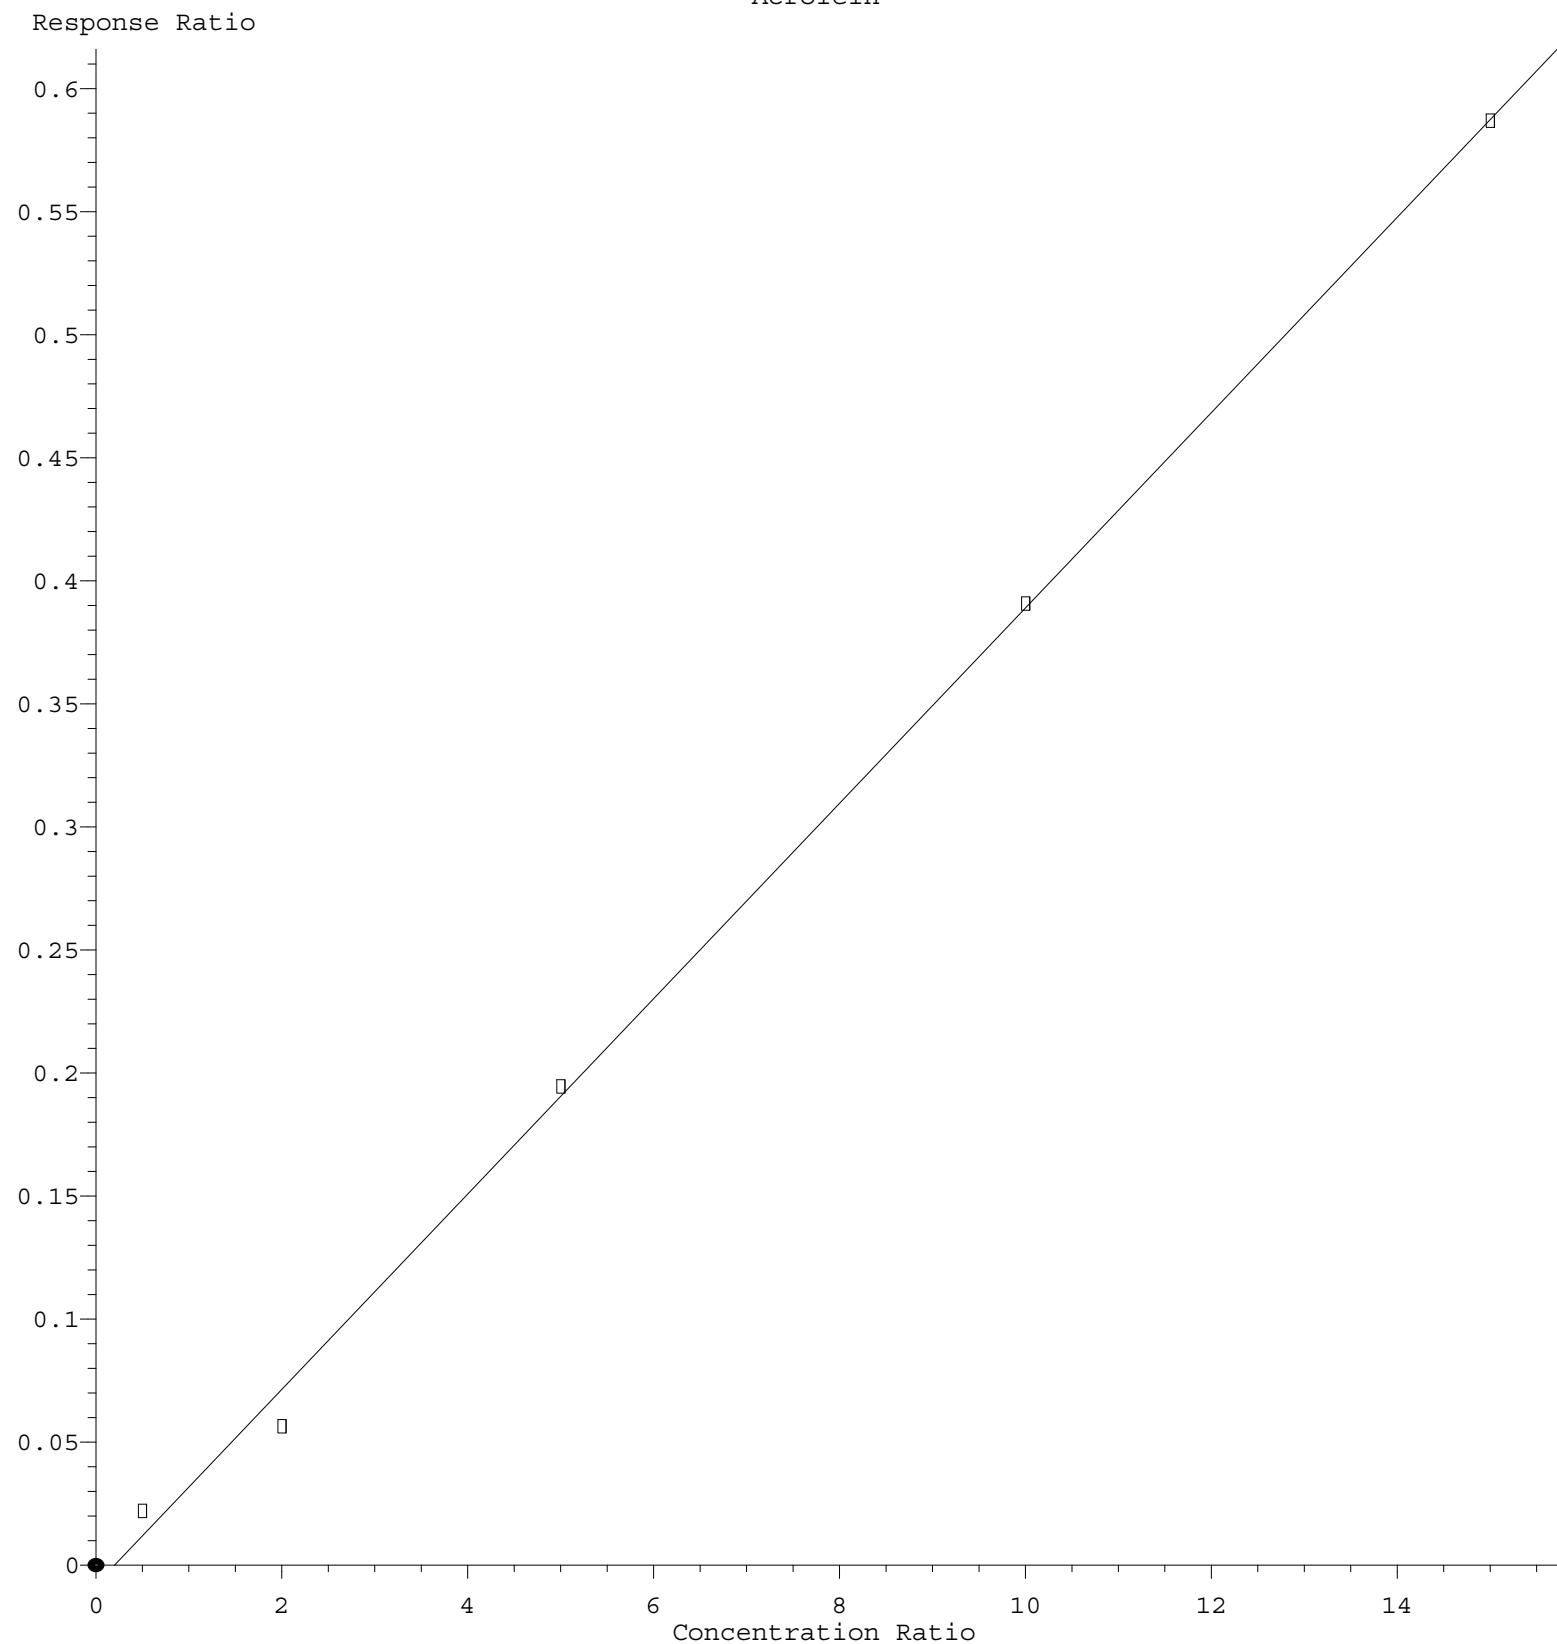

Response = $3.971 \times 10^{-2} \times \text{Amt} - 7.988 \times 10^{-3}$
 Coef of Det (r^2) = 0.998462 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M
 Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Acetone


Response Ratio

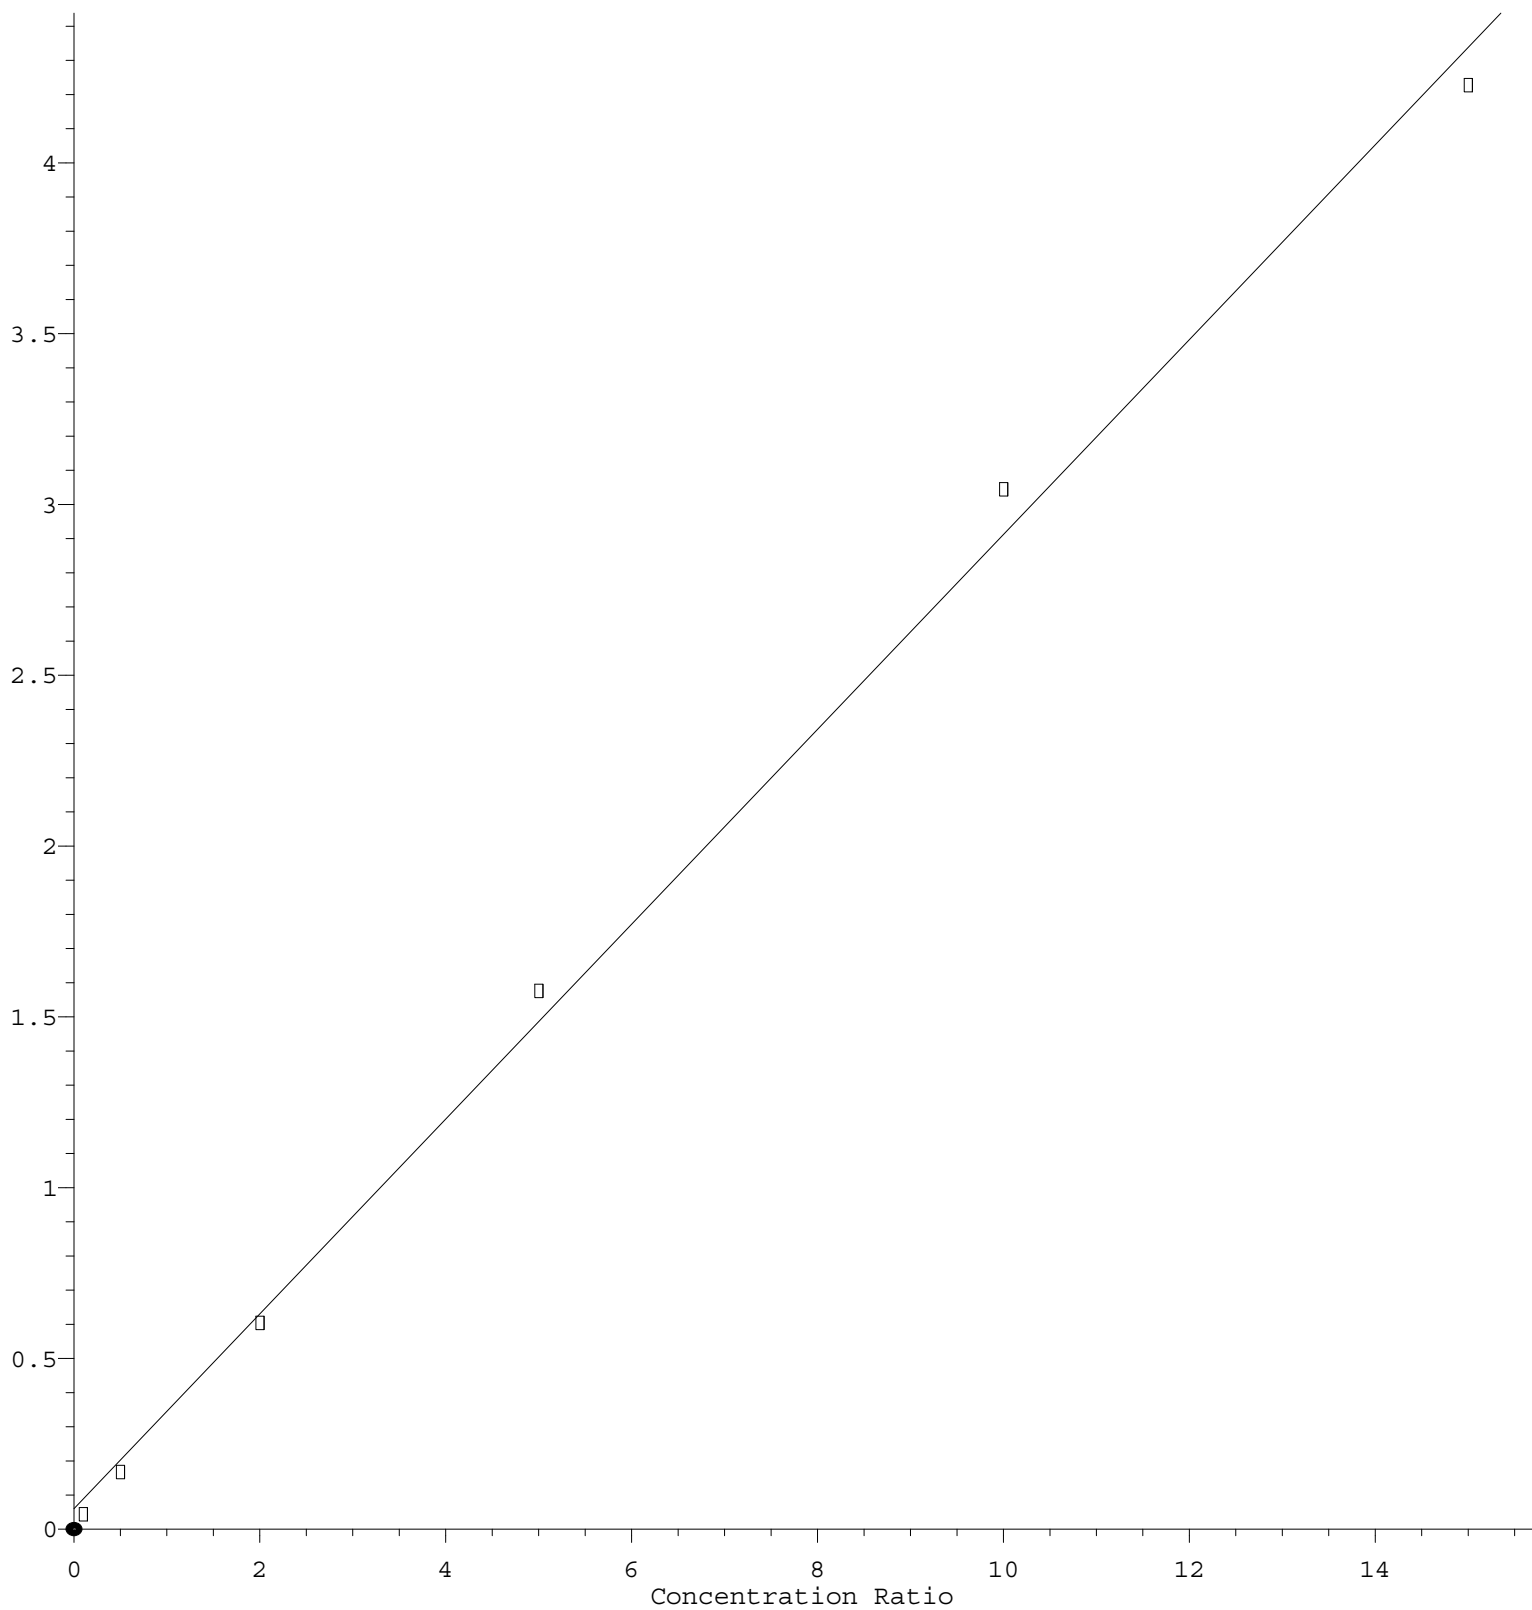

Response = 2.853e-001 * Amt + 6.031e-002
Coef of Det (r^2) = 0.997115 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M
Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Carbon Disulfide

Response Ratio

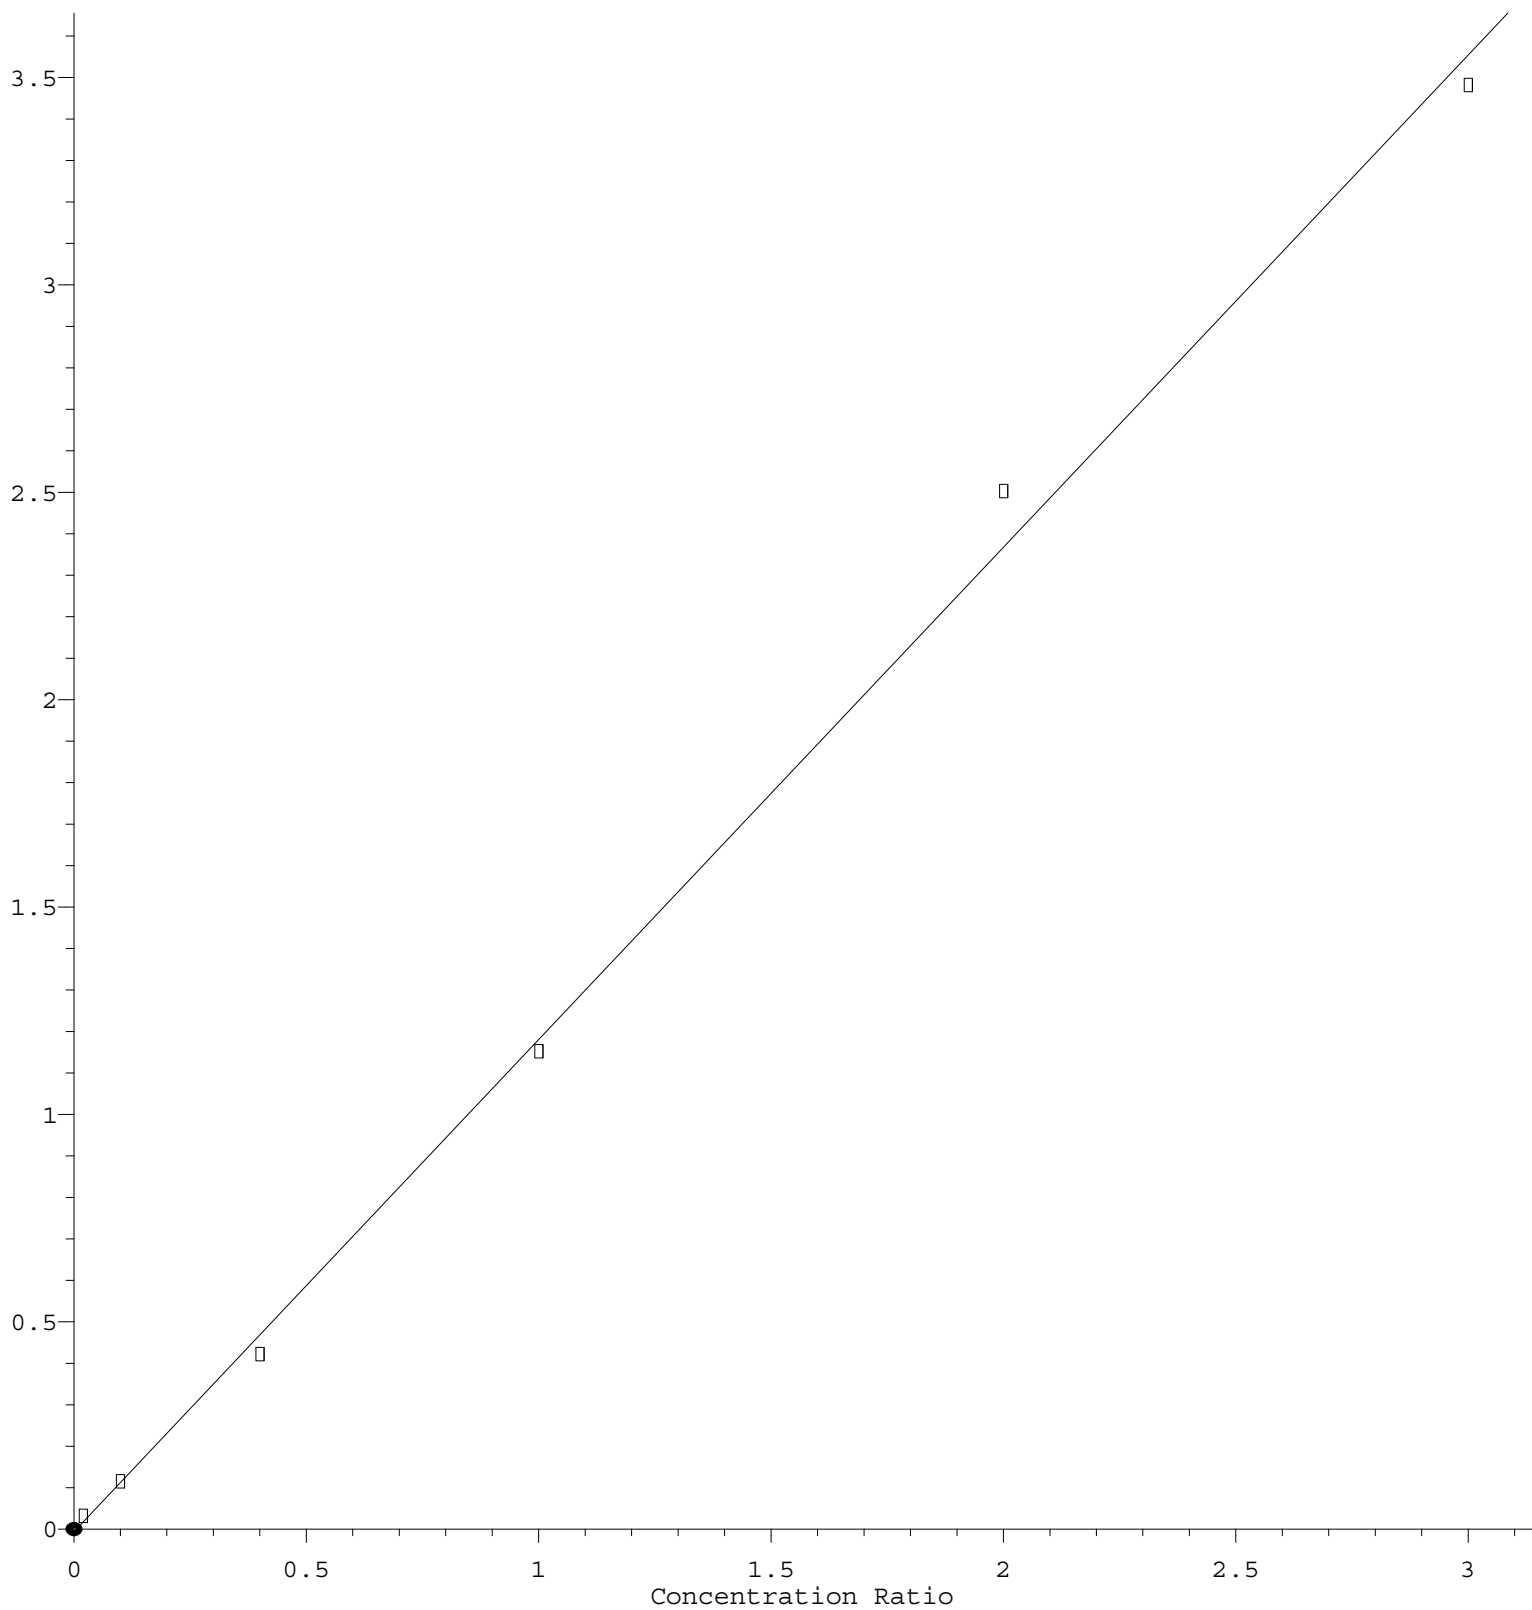

$$\text{Response} = 1.187\text{e}+000 * \text{Amt} - 5.405\text{e}-003$$


Coef of Det (r^2) = 0.997327 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M

Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Methylene Chloride


Response Ratio

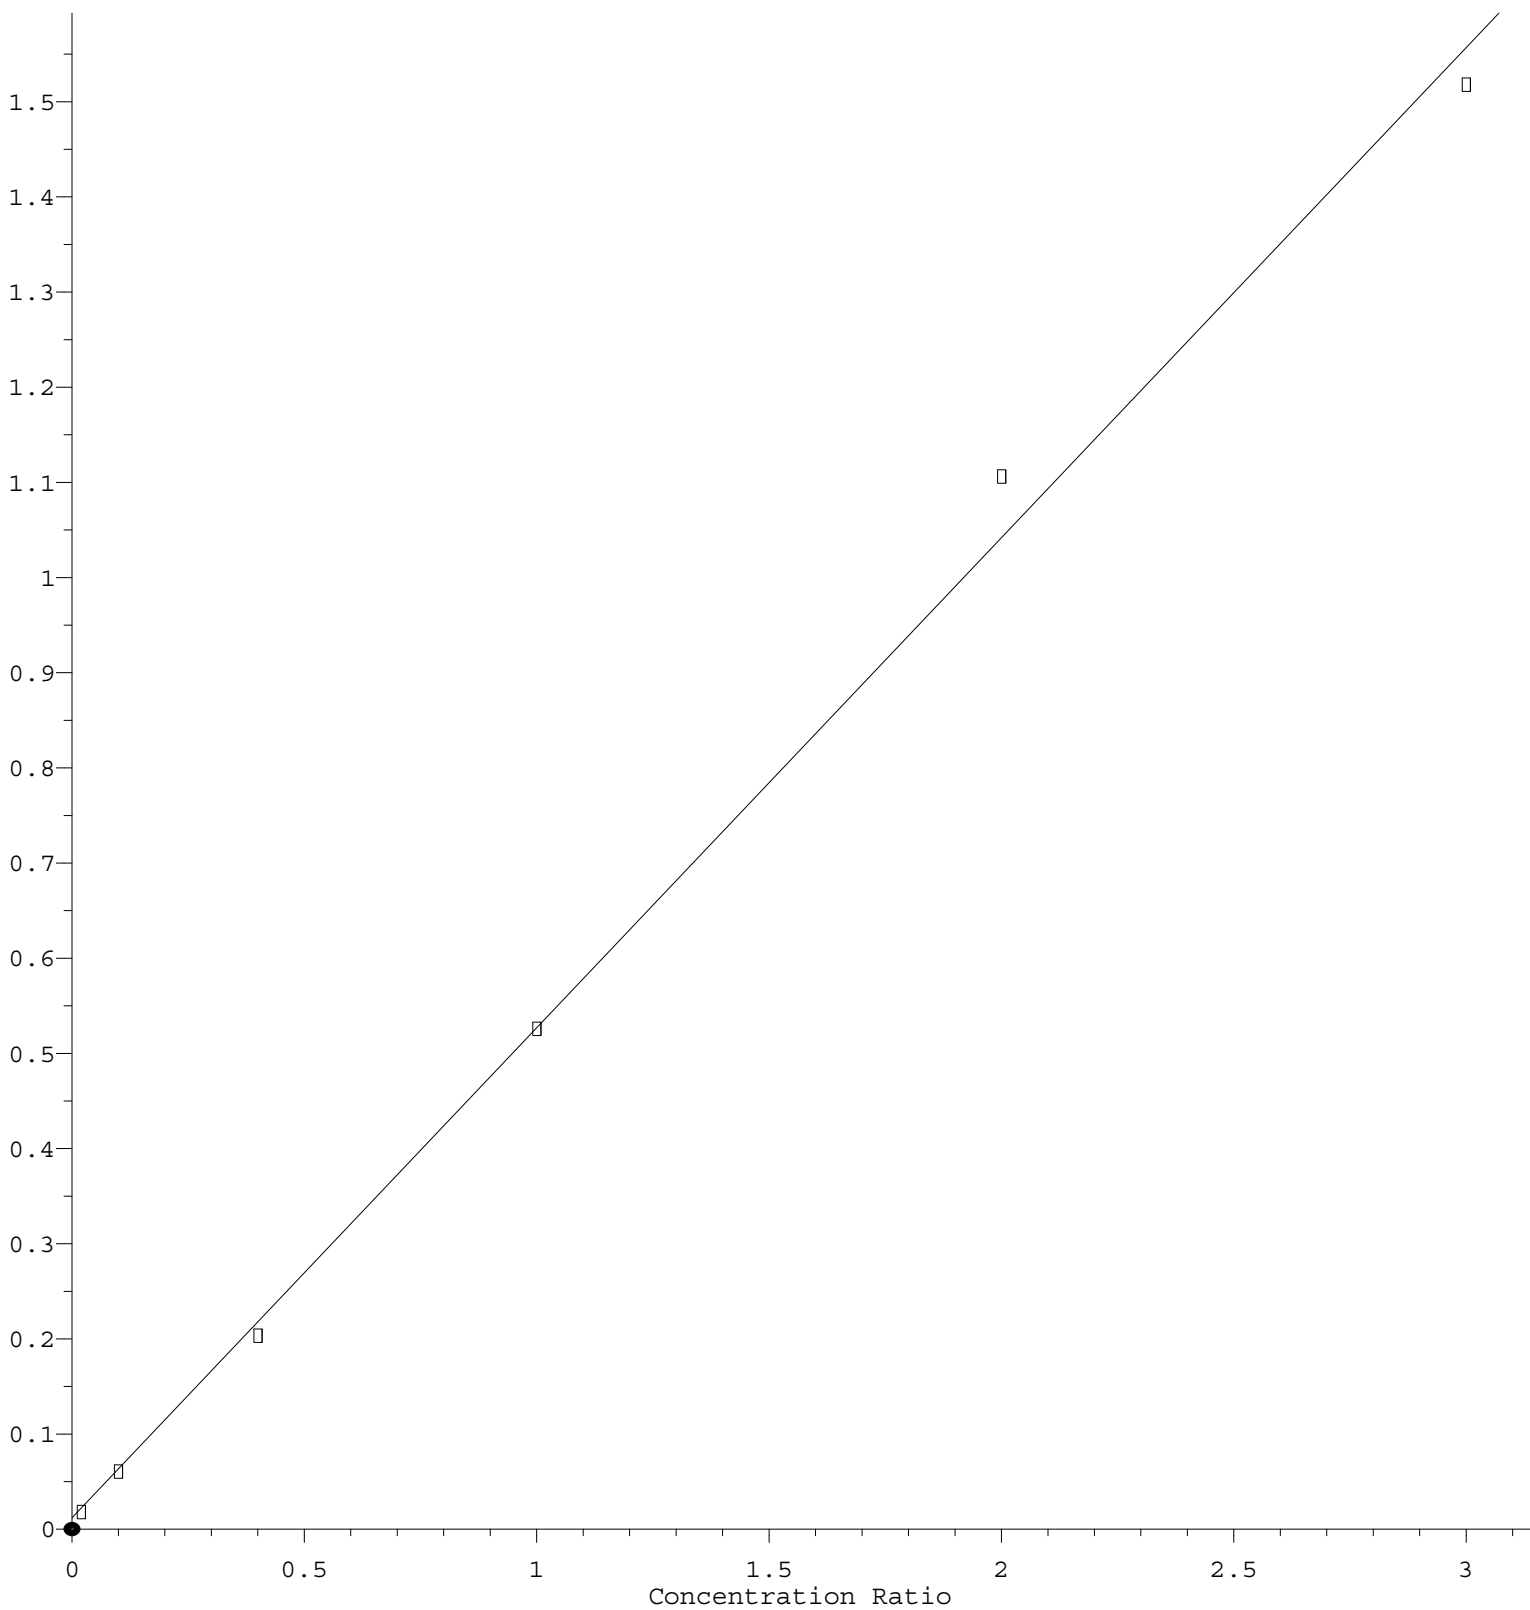

$\text{Response} = 5.152\text{e-}001 * \text{Amt} + 1.207\text{e-}002$
 Coef of Det (r^2) = 0.996877 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M
 Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Dibromochloromethane

Response Ratio

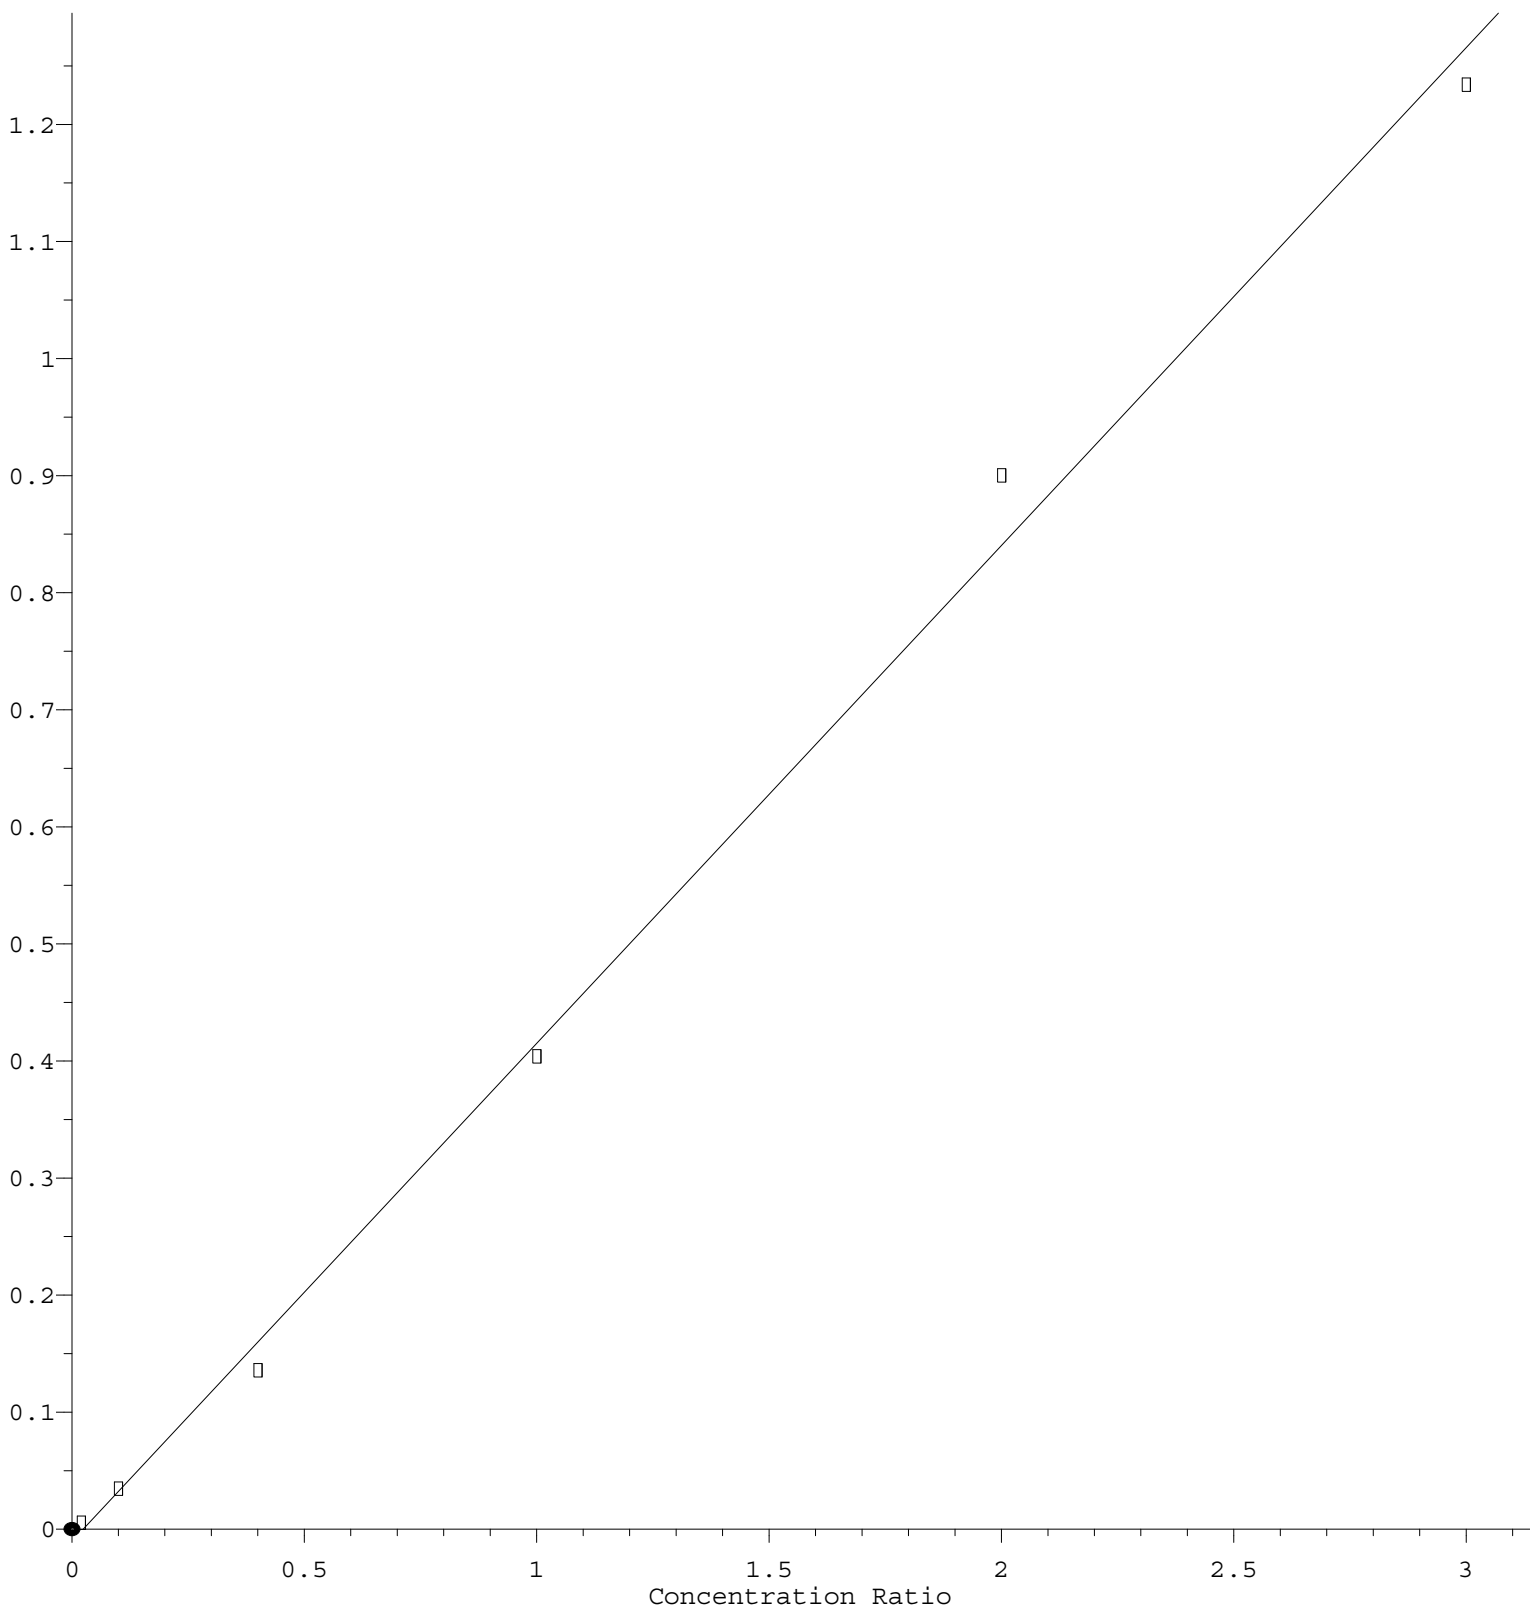

$$\text{Response} = 4.255\text{e-}001 * \text{Amt} - 1.010\text{e-}002$$


Coef of Det (r^2) = 0.995845 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M

Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

Bromoform

Response Ratio

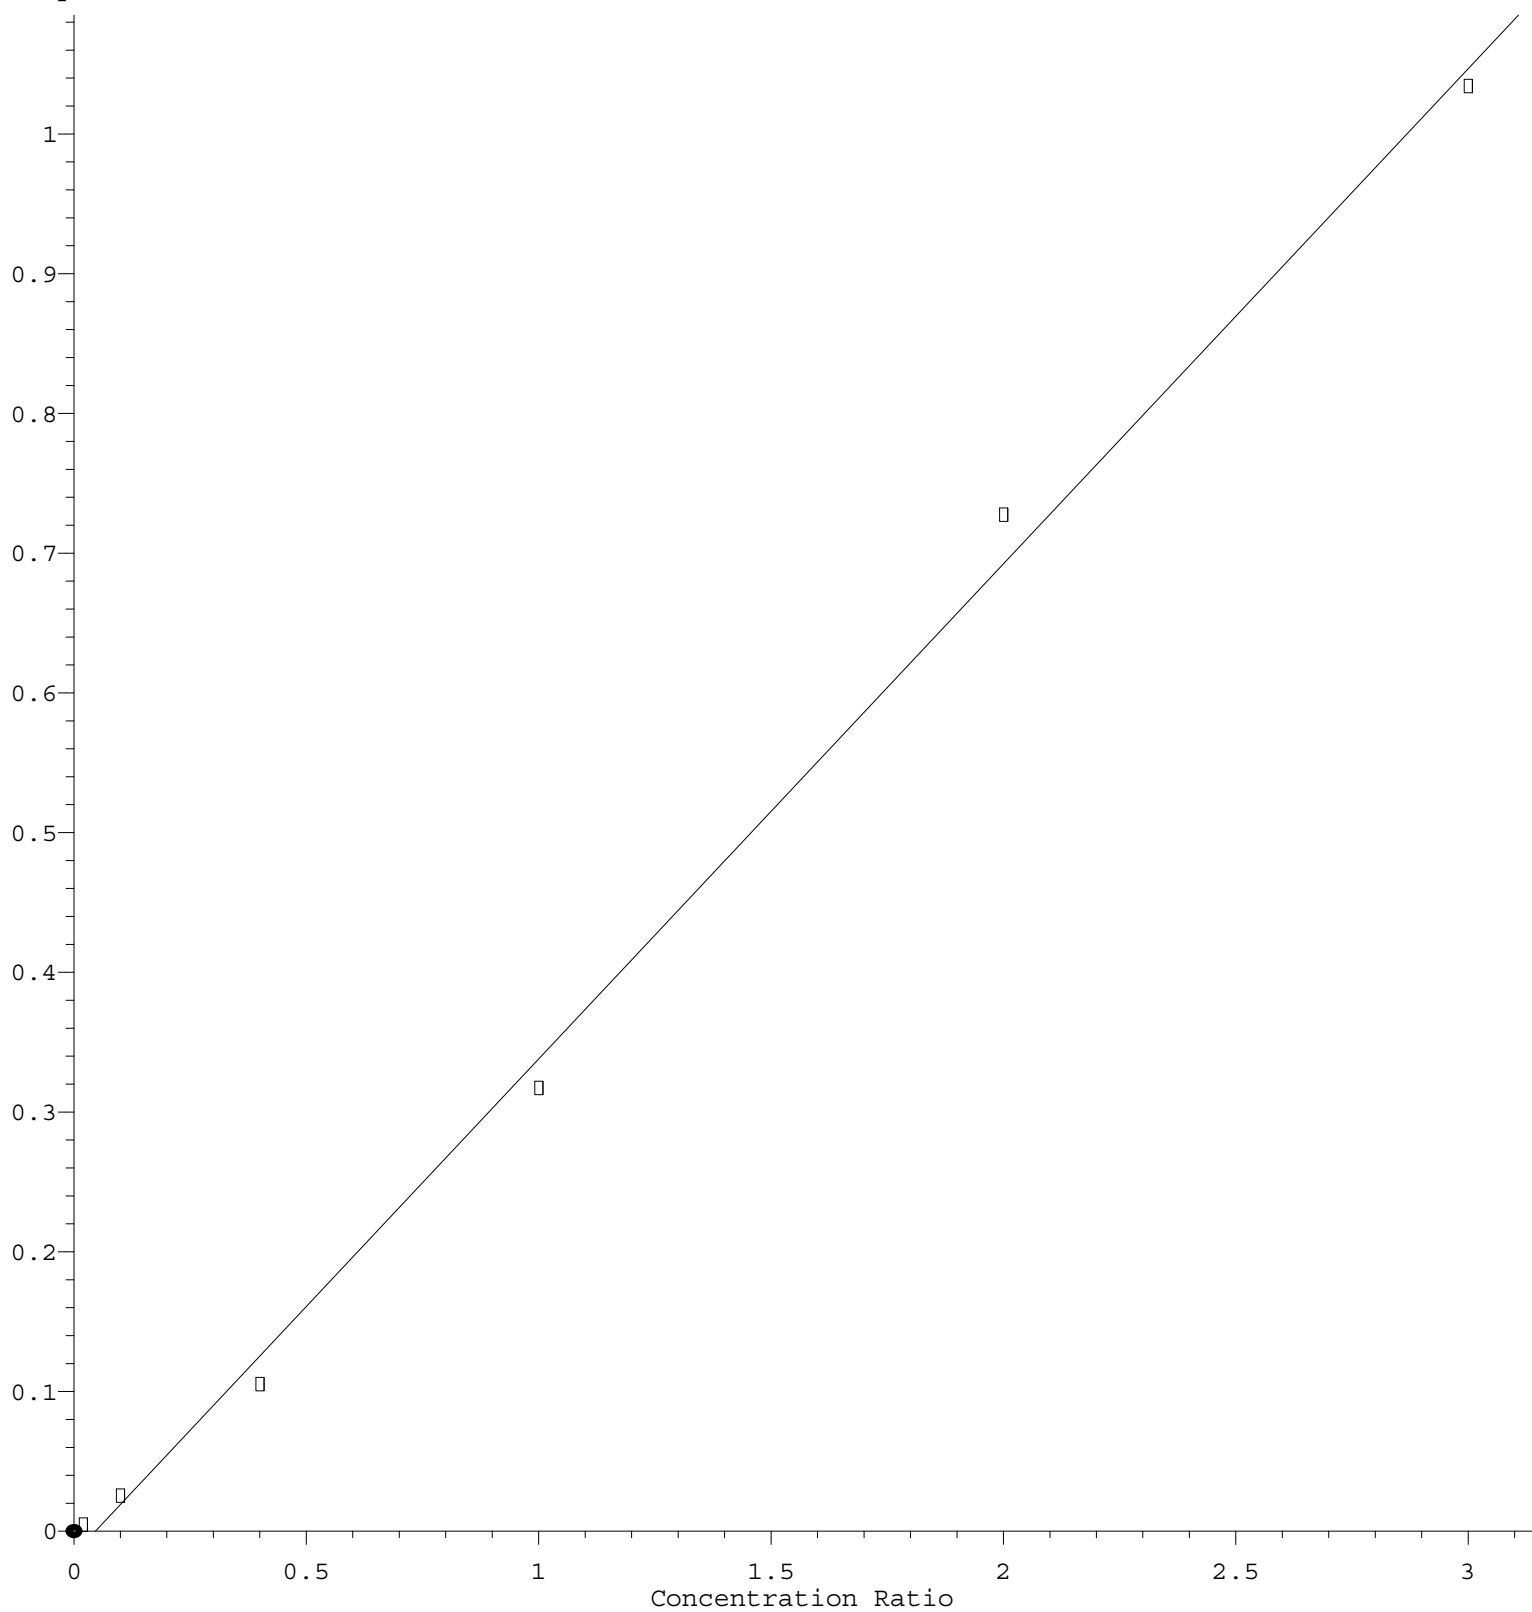

$$\text{Response} = 3.547\text{e-}001 * \text{Amt} - 1.645\text{e-}002$$


Coef of Det (r^2) = 0.997244 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M

Calibration Table Last Updated: Thu Sep 23 18:24:34 2021

trans-1,4-Dichloro-2-butene

Response Ratio

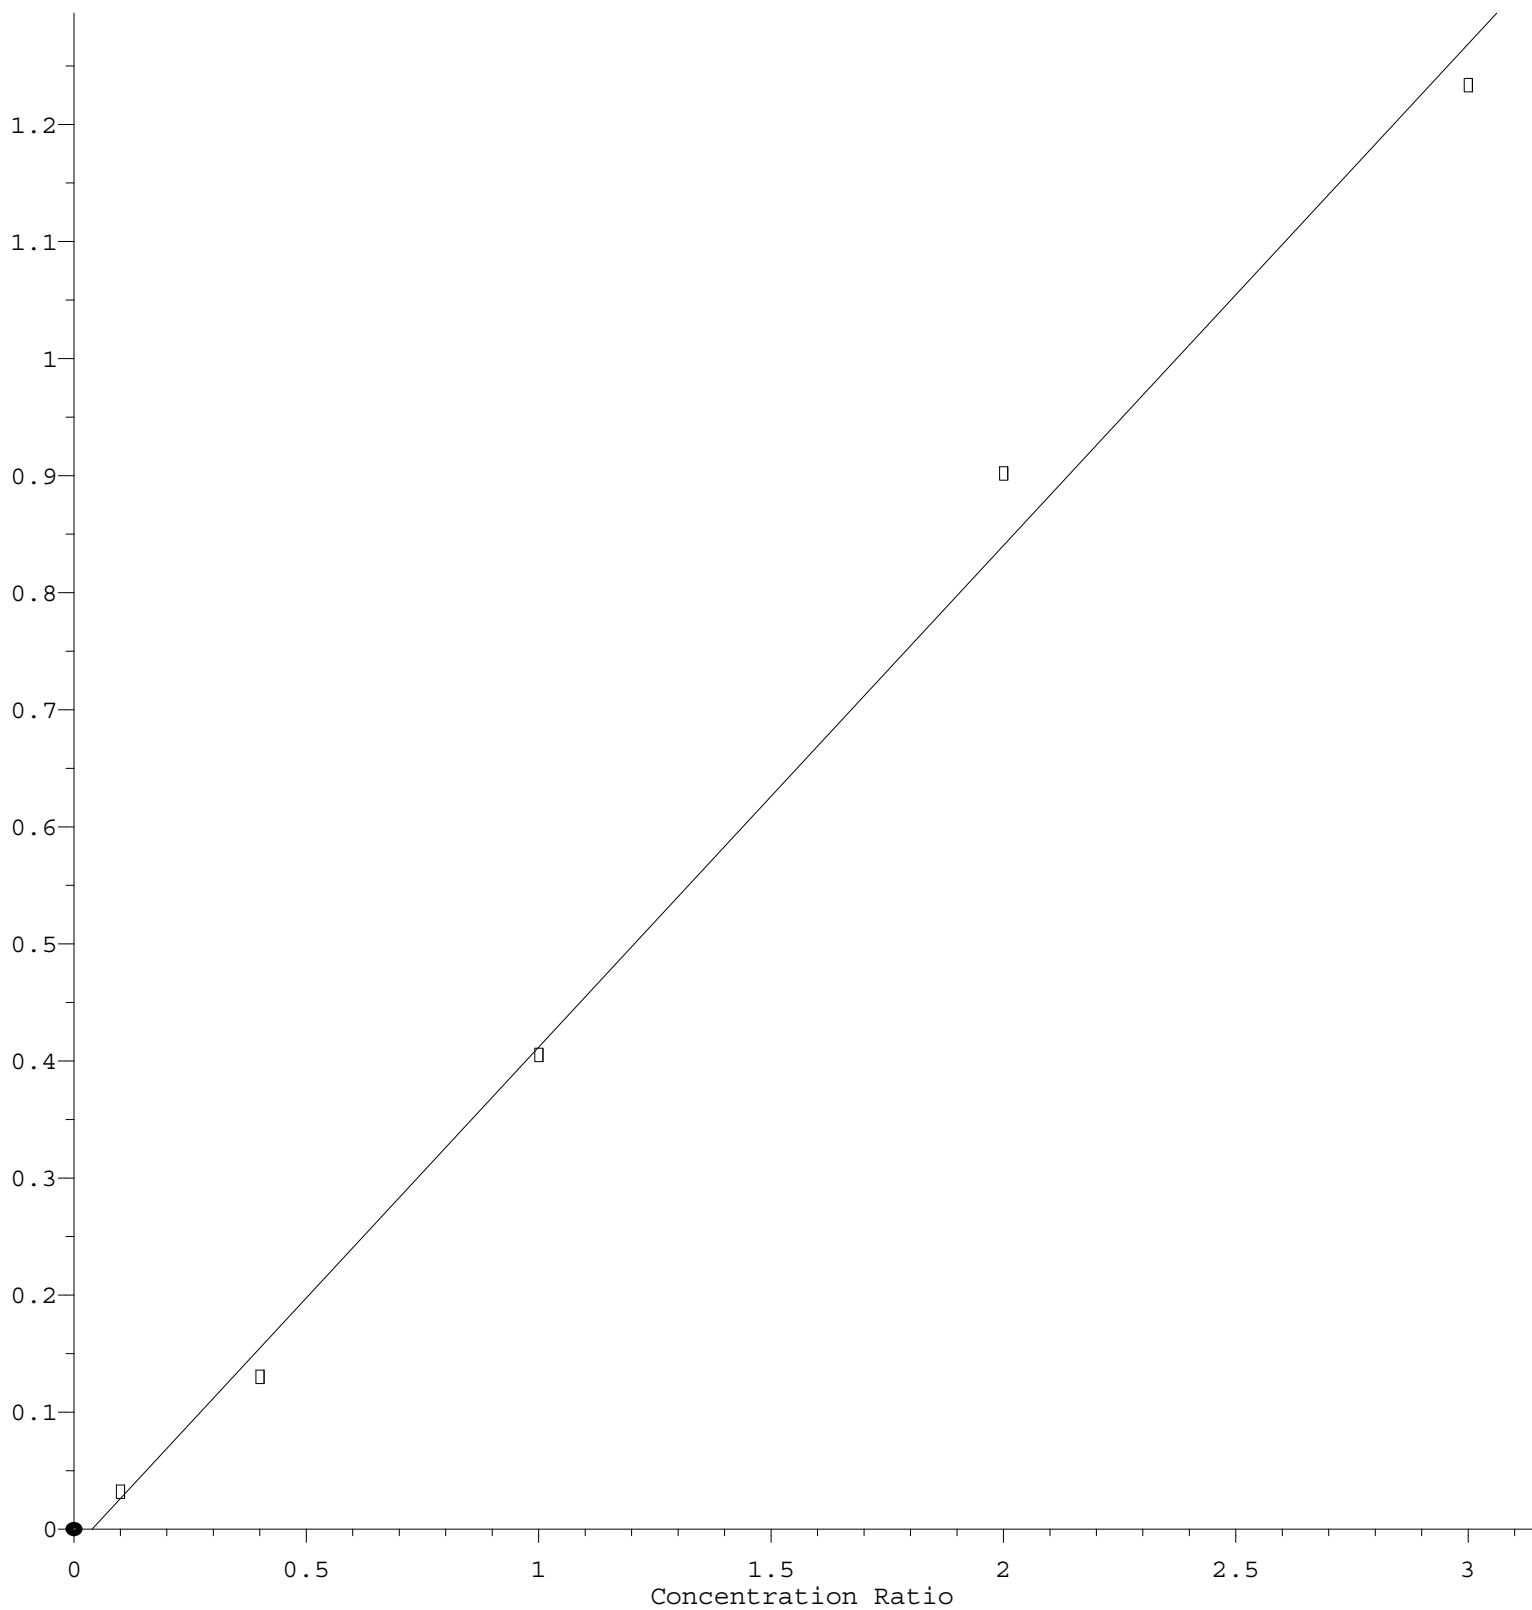

$$\text{Response} = 4.286\text{e-}001 * \text{Amt} - 1.659\text{e-}002$$

Coef of Det (r^2) = 0.994592 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA X\Method\82X092321W.M

Calibration Table Last Updated: Thu Sep 23 18:24:34 2021