

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024458.D
 Acq On : 23 Sep 2021 18:51
 Operator : JC/MD
 Sample : VX0923WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0923WBL01

Quant Time: Sep 24 07:37:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Quant Title : SW846 8260
 QLast Update : Thu Sep 23 18:24:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	134884	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	230356	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	220523	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	94549	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	99680	52.435	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 104.860%	
35) Dibromofluoromethane	5.397	113	77041	50.343	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.680%	
50) Toluene-d8	8.653	98	285313	50.656	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.320%	
62) 4-Bromofluorobenzene	11.085	95	103884	46.910	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 93.820%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024458.D
Acq On : 23 Sep 2021 18:51
Operator : JC/MD
Sample : VX0923WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0923WBL01

Quant Time: Sep 24 07:37:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260
QLast Update : Thu Sep 23 18:24:34 2021
Response via : Initial Calibration




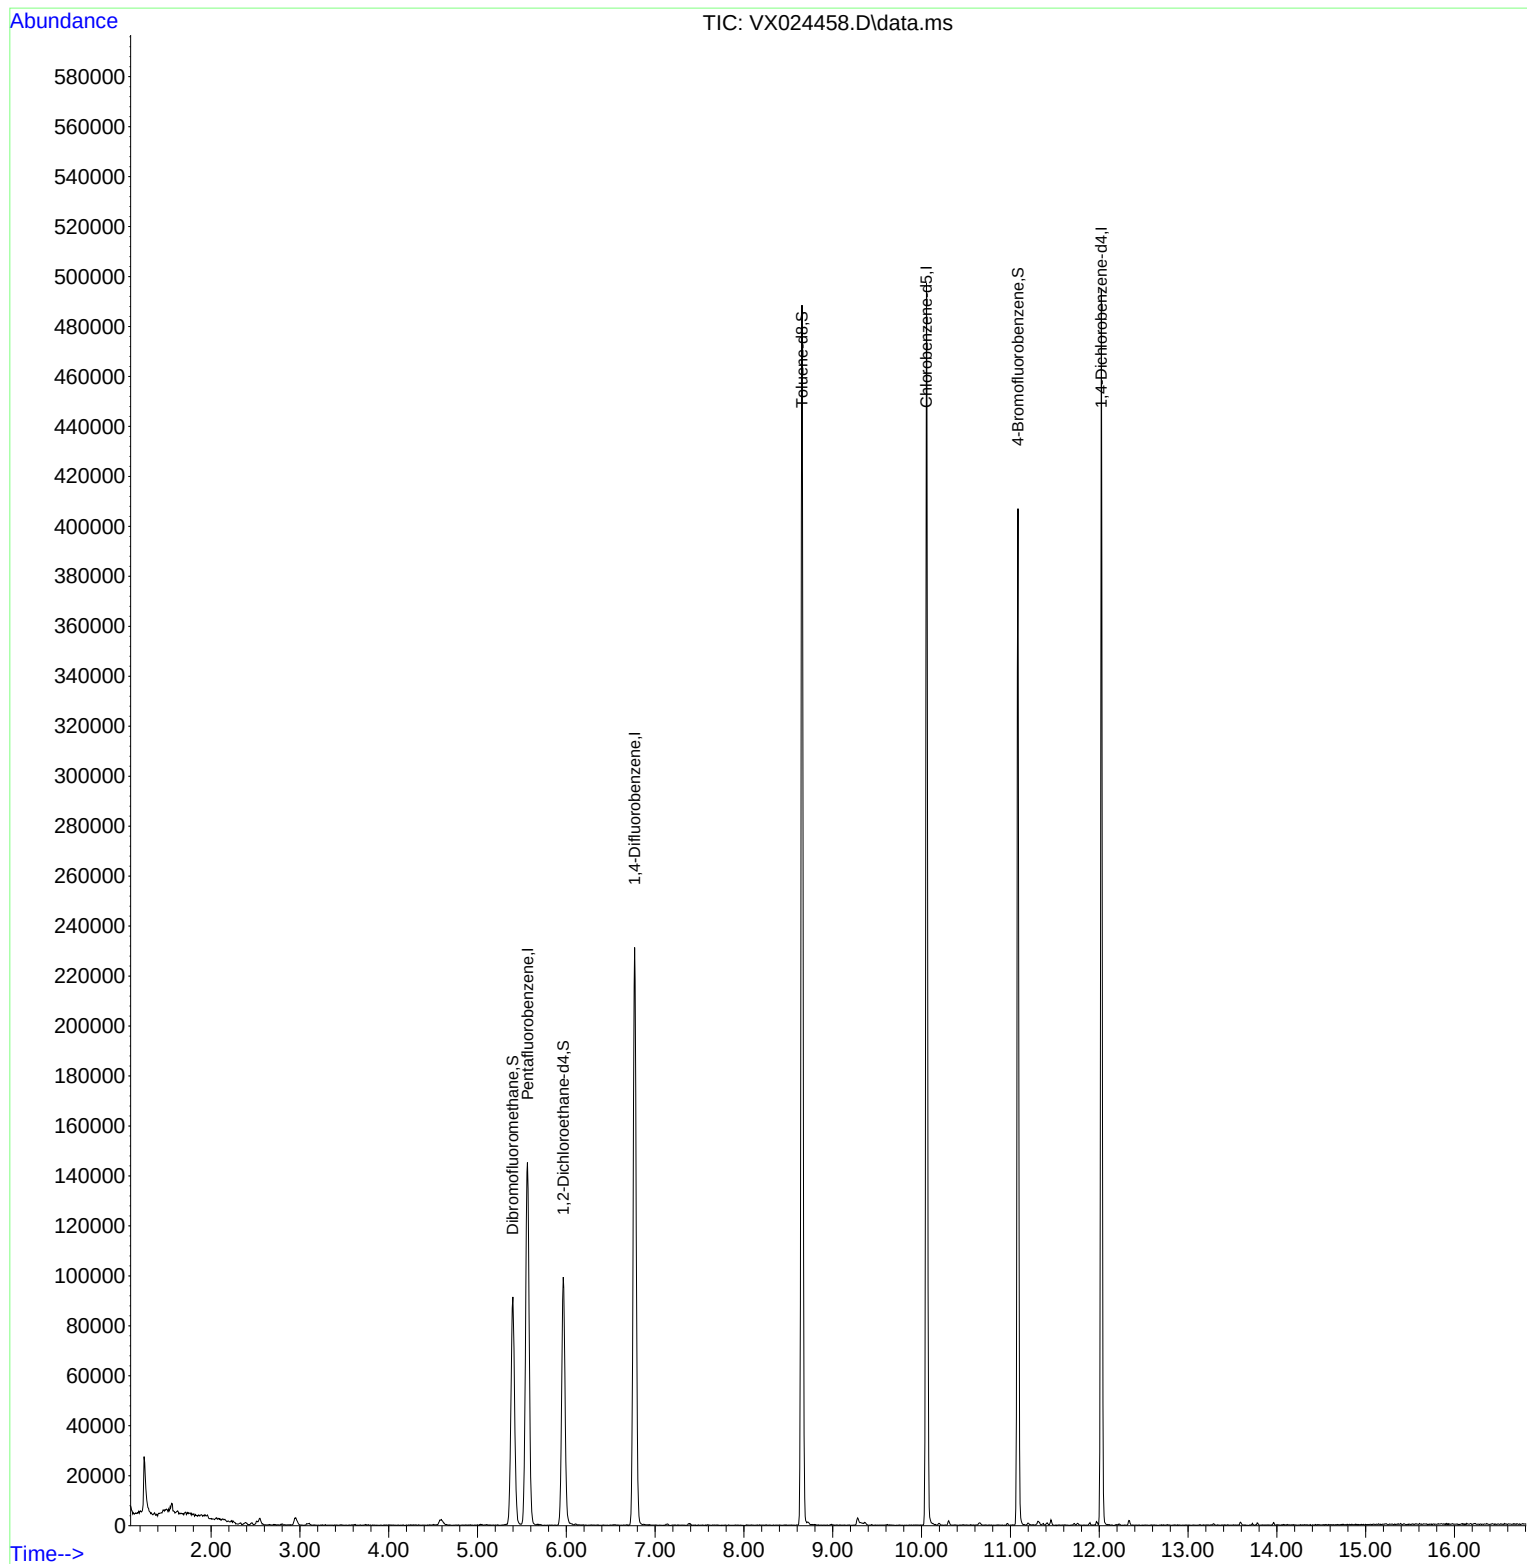


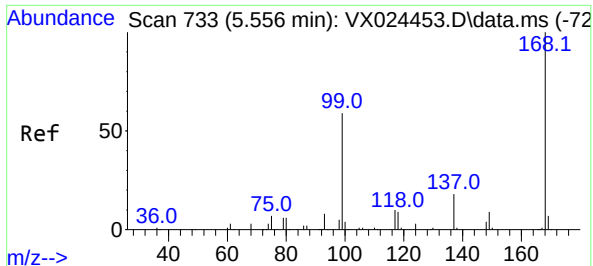

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.006 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51




Instrument :
MSVOA_X
ClientSampleId :
VX0923WBL01


Tgt Ion:168 Resp: 134884
Ion Ratio Lower Upper
168 100
99 58.0 45.8 68.6

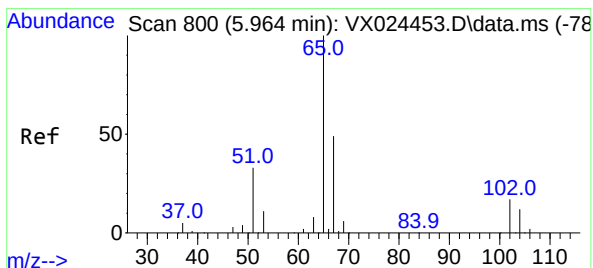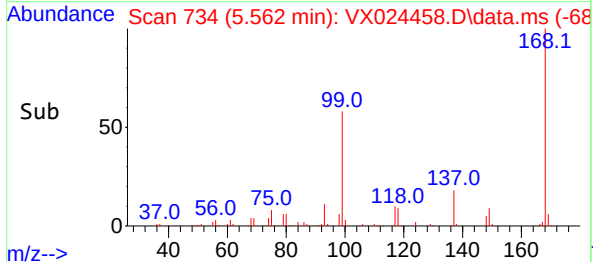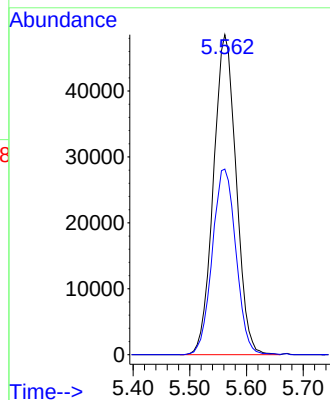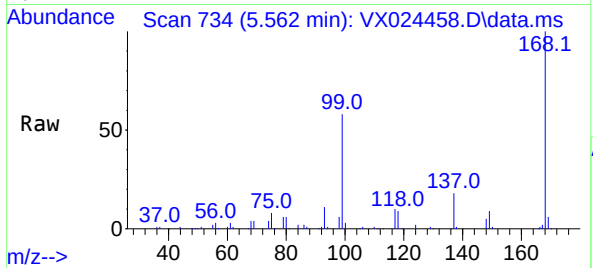

#33
1,2-Dichloroethane-d4
Concen: 52.435 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51

Tgt Ion: 65 Resp: 99680
Ion Ratio Lower Upper
65 100
67 50.0 0.0 105.4


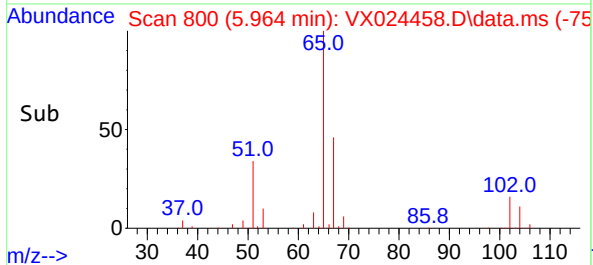
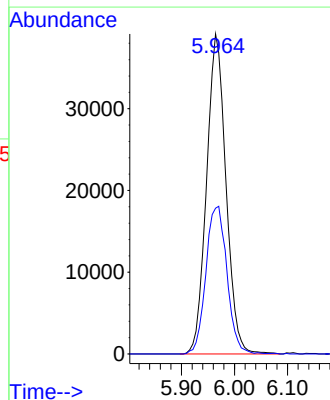
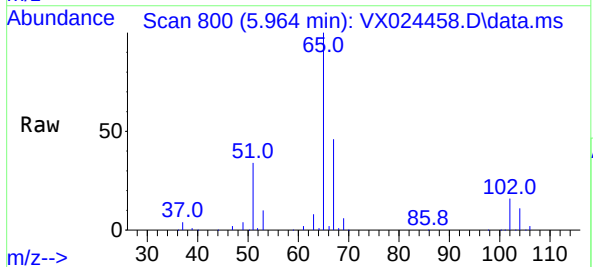


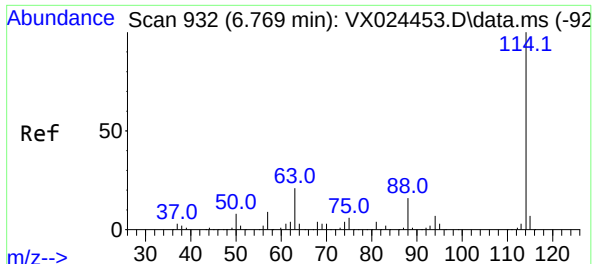

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51




Instrument :
MSVOA_X
ClientSampleId :
VX0923WBL01


Tgt Ion:114 Resp: 230356
Ion Ratio Lower Upper
114 100
63 21.3 0.0 40.8
88 16.7 0.0 32.8

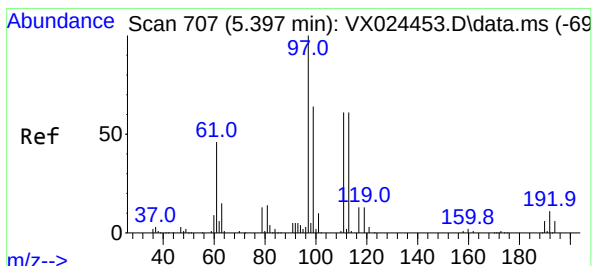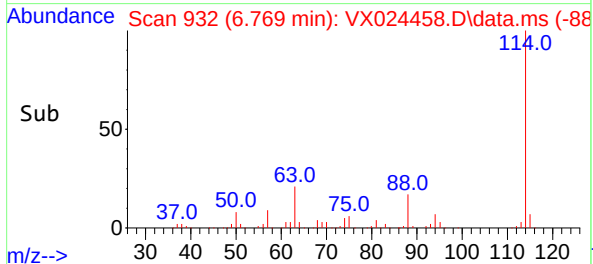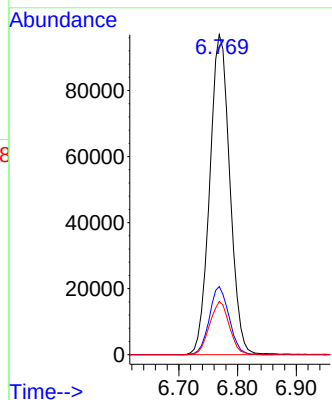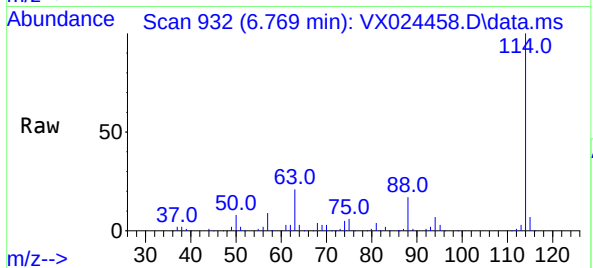

#35
Dibromofluoromethane
Concen: 50.343 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51

Tgt Ion:113 Resp: 77041
Ion Ratio Lower Upper
113 100
111 102.6 81.9 122.9
192 19.0 16.7 25.1

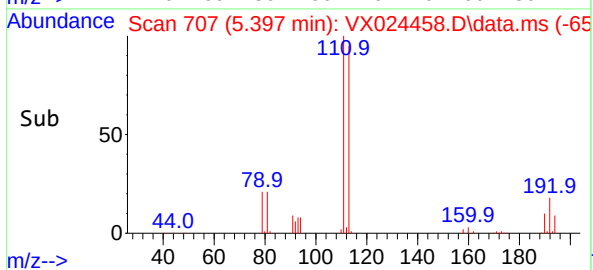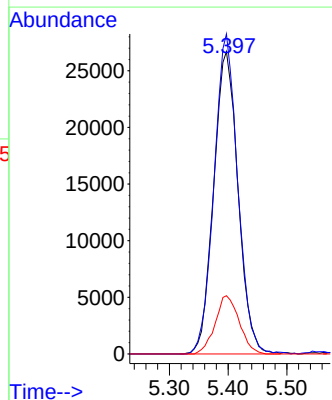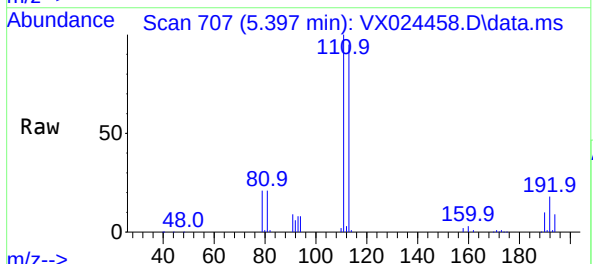

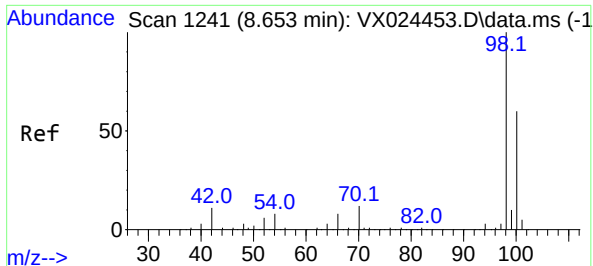

#50

Toluene-d8

Concen: 50.656 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX024458.D





Acq: 23 Sep 2021 18:51

Tgt Ion: 98 Resp: 285313

Ion Ratio Lower Upper

98 100

100 63.6 51.9 77.9

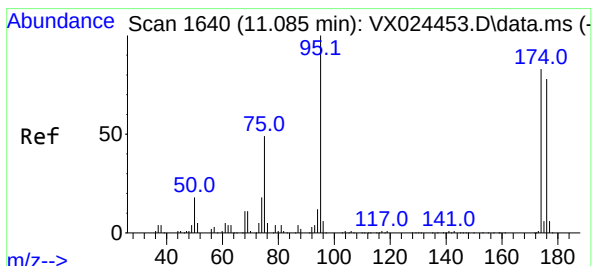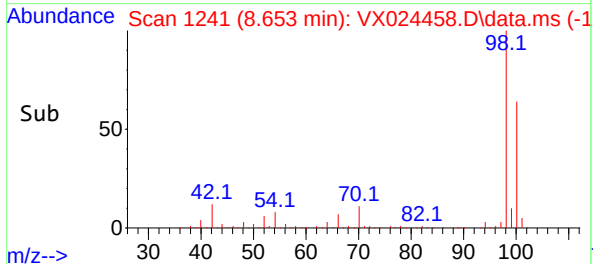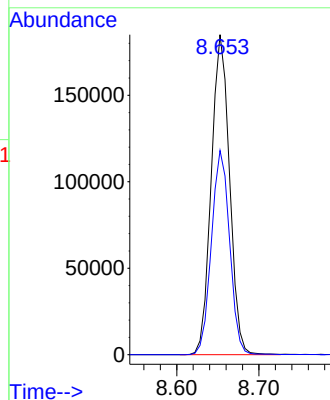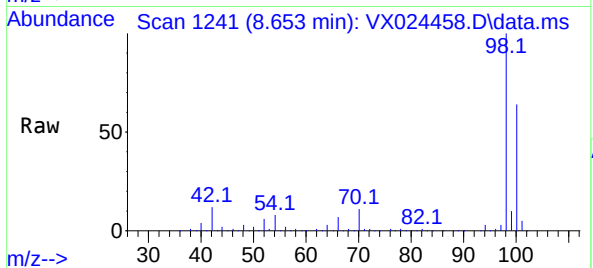

#62

4-Bromofluorobenzene

Concen: 46.910 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.000 min

Lab File: VX024458.D

Acq: 23 Sep 2021 18:51




Tgt Ion: 95 Resp: 103884


Ion Ratio Lower Upper

95 100

174 79.9 0.0 154.6

176 77.7 0.0 155.8


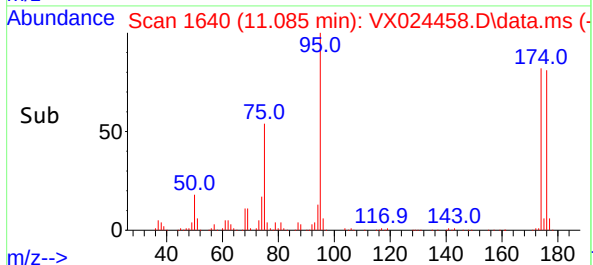
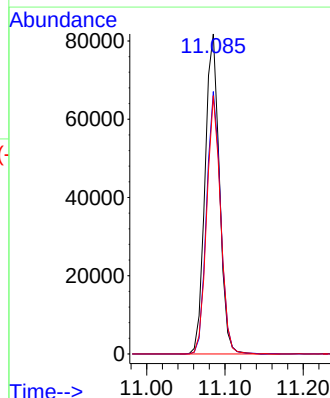
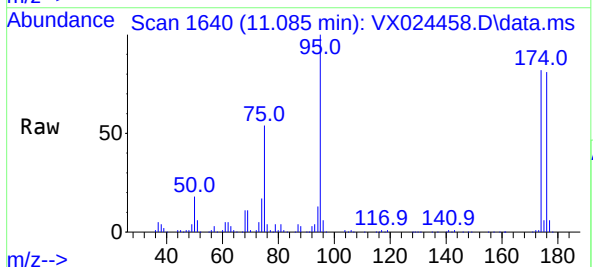


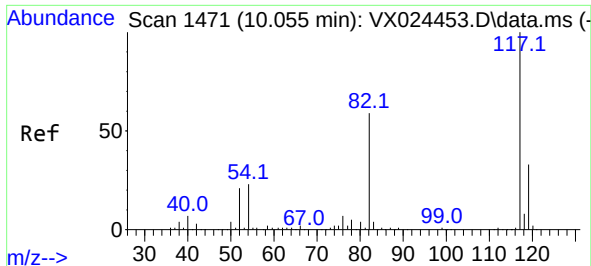

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51

Instrument :
MSVOA_X
ClientSampleId :
VX0923WBL01

Tgt Ion:117 Resp: 220523
Ion Ratio Lower Upper
117 100
82 57.6 47.4 71.2
119 32.2 26.6 39.8

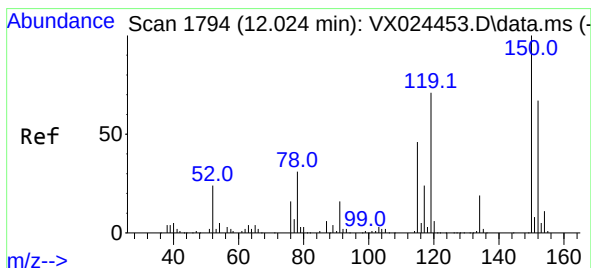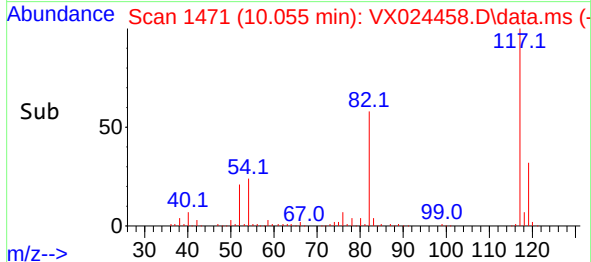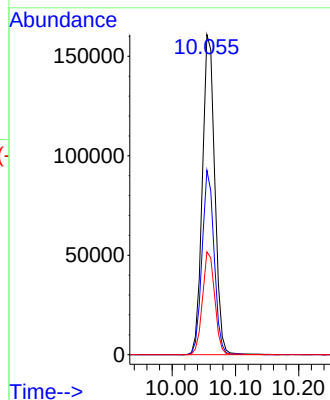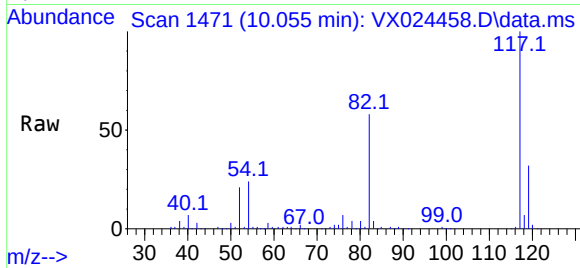

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX024458.D
Acq: 23 Sep 2021 18:51

Tgt Ion:152 Resp: 94549
Ion Ratio Lower Upper
152 100
115 61.5 41.1 123.3
150 159.3 0.0 349.0

