

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024464.D
 Acq On : 23 Sep 2021 21:12
 Operator : JC/MD
 Sample : M3833-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP08-20210919

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024464.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	42	rBV	25346	47562	5.81%	1.101%
2	2.544	231	239	247	rVB2	4495	8348	1.02%	0.193%
3	5.397	696	707	722	rBV2	96582	278060	33.99%	6.437%
4	5.562	722	734	752	rVB	146880	411562	50.30%	9.528%
5	5.964	788	800	814	rBV	106506	277537	33.92%	6.425%
6	6.763	922	931	945	rBV	233624	564118	68.95%	13.059%
7	7.129	986	991	999	rBV2	4964	10878	1.33%	0.252%
8	8.653	1234	1241	1252	rBV	527003	818169	100.00%	18.940%
9	9.281	1338	1344	1349	rBV5	5775	10239	1.25%	0.237%
10	10.055	1465	1471	1479	rBV	530922	737529	90.14%	17.074%
11	11.085	1634	1640	1651	rBV	433623	538680	65.84%	12.470%
12	12.024	1789	1794	1802	rBV	495823	617028	75.42%	14.284%




Sum of corrected areas: 4319710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024464.D
Acq On : 23 Sep 2021 21:12
Operator : JC/MD
Sample : M3833-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

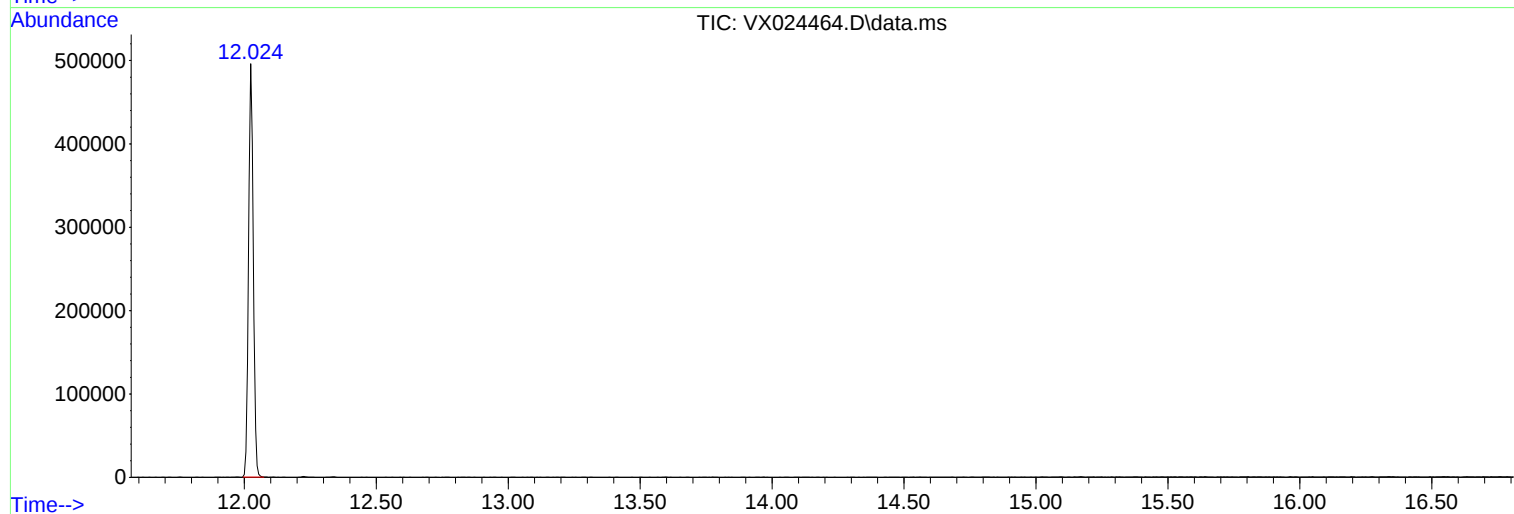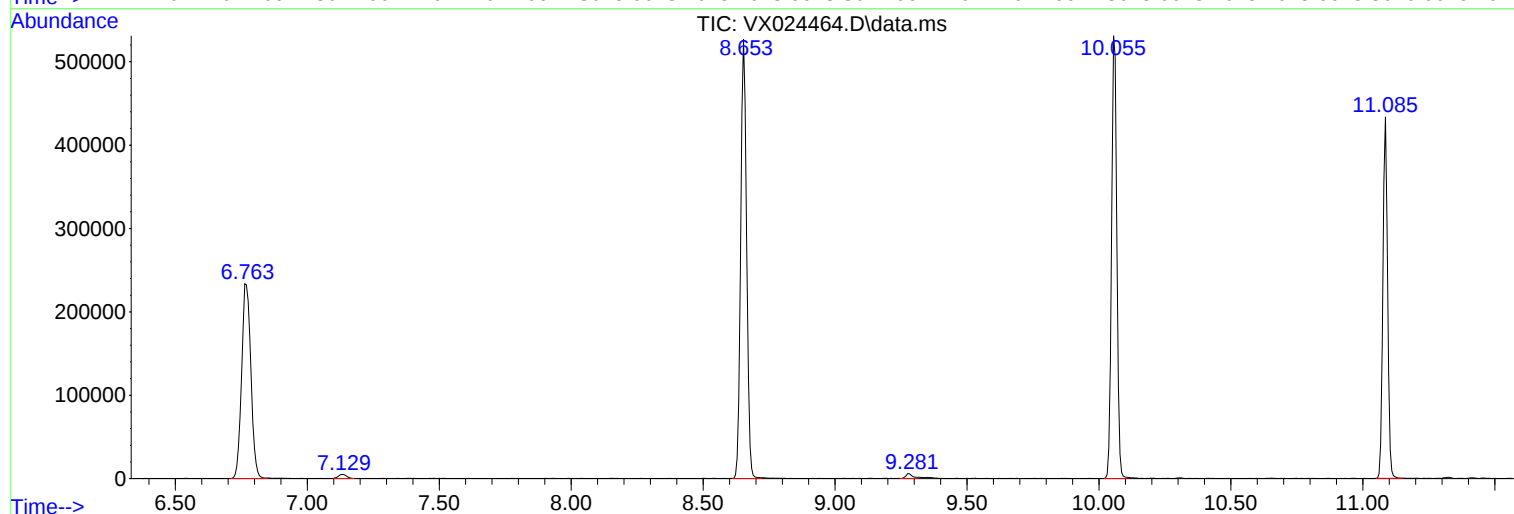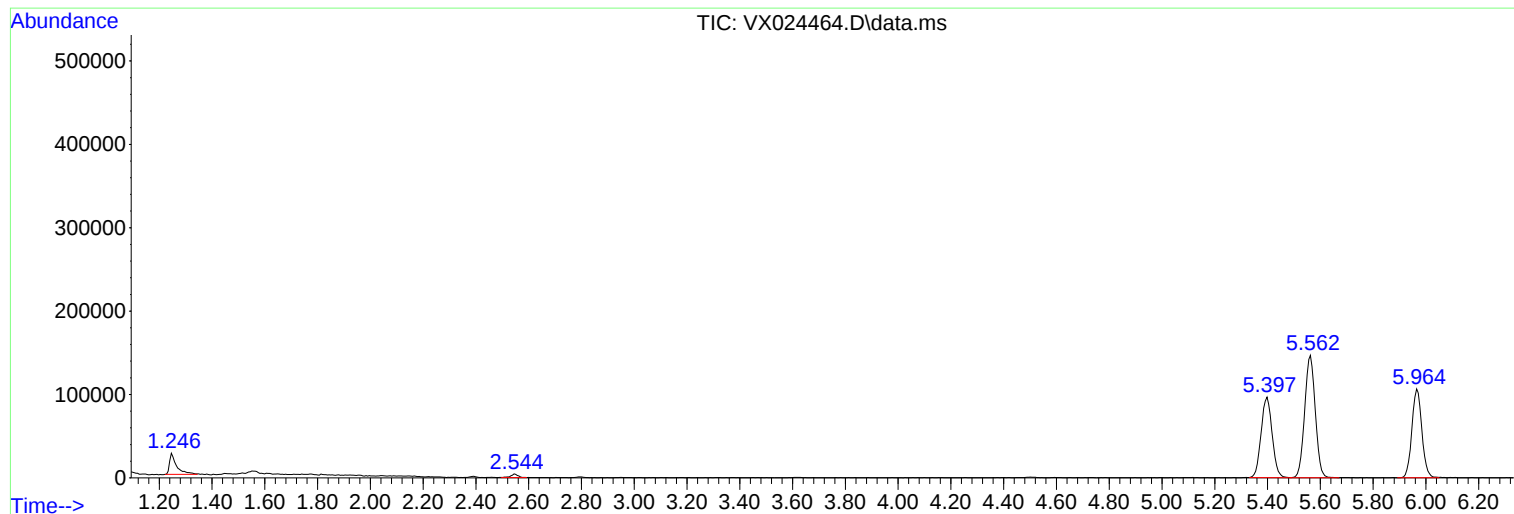

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024464.D
Acq On : 23 Sep 2021 21:12
Operator : JC/MD
Sample : M3833-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024464.D
Acq On : 23 Sep 2021 21:12
Operator : JC/MD
Sample : M3833-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP08-20210919

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------