

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024467.D
 Acq On : 23 Sep 2021 22:23
 Operator : JC/MD
 Sample : M3833-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE126D3-20210920

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rVB	20502	37834	4.99%	0.967%
2	2.544	235	239	249	rVB	6407	11951	1.58%	0.305%
3	5.397	693	707	721	rBV	86948	251031	33.09%	6.415%
4	5.556	723	733	750	rVB	142959	394314	51.97%	10.077%
5	5.964	787	800	812	rBV	97764	253255	33.38%	6.472%
6	6.769	920	932	948	rBV	224755	531933	70.11%	13.594%
7	7.135	985	992	1001	rVB	9397	18846	2.48%	0.482%
8	8.653	1233	1241	1250	rBV	499498	758738	100.00%	19.390%
9	9.275	1338	1343	1349	rBV3	10095	16571	2.18%	0.423%
10	10.055	1465	1471	1482	rBV	453229	616539	81.26%	15.756%
11	11.085	1634	1640	1651	rBV	384274	485007	63.92%	12.395%
12	12.024	1789	1794	1802	rBV	436397	536999	70.78%	13.723%


Sum of corrected areas: 3913018

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024467.D
Acq On : 23 Sep 2021 22:23
Operator : JC/MD
Sample : M3833-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

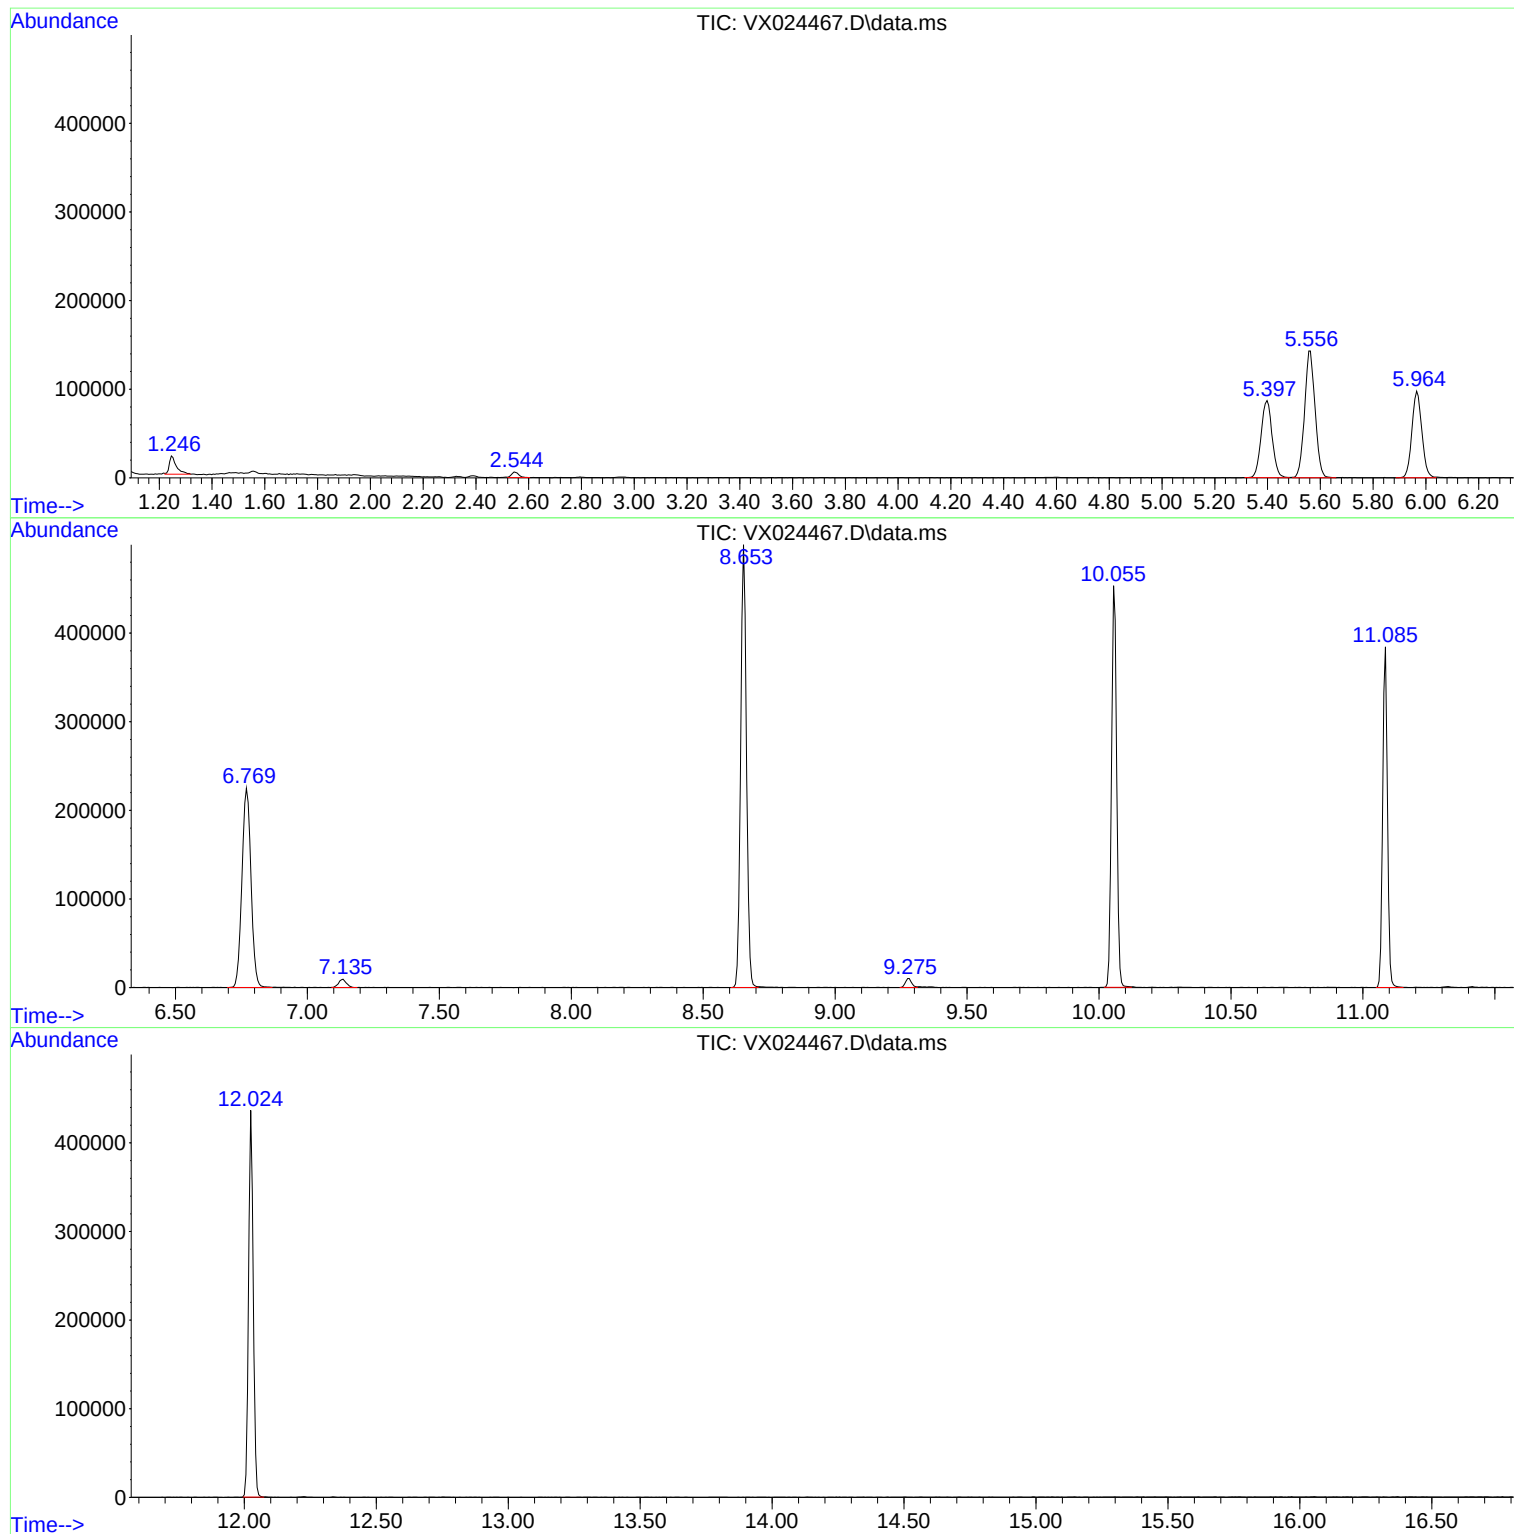

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024467.D
Acq On : 23 Sep 2021 22:23
Operator : JC/MD
Sample : M3833-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024467.D
Acq On : 23 Sep 2021 22:23
Operator : JC/MD
Sample : M3833-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE126D3-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
