

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024471.D
 Acq On : 23 Sep 2021 23:57
 Operator : JC/MD
 Sample : M3833-13 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE122D2-20210920

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	40	rBV2	15144	32217	3.55%	0.680%
2	5.397	696	707	719	rBV2	89721	254355	28.06%	5.372%
3	5.562	723	734	746	rBV	139948	396515	43.74%	8.375%
4	5.964	789	800	819	rBV	92547	251369	27.73%	5.309%
5	6.769	922	932	945	rBV	222341	529343	58.40%	11.180%
6	7.129	982	991	1005	rBV	419852	906455	100.00%	19.145%
7	8.653	1234	1241	1250	rBV	453878	690667	76.19%	14.588%
8	10.055	1465	1471	1485	rBV	452962	618578	68.24%	13.065%
9	11.085	1634	1640	1654	rBV	383917	483855	53.38%	10.220%
10	12.024	1789	1794	1807	rBV	472093	571262	63.02%	12.066%




Sum of corrected areas: 4734616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024471.D
Acq On : 23 Sep 2021 23:57
Operator : JC/MD
Sample : M3833-13 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

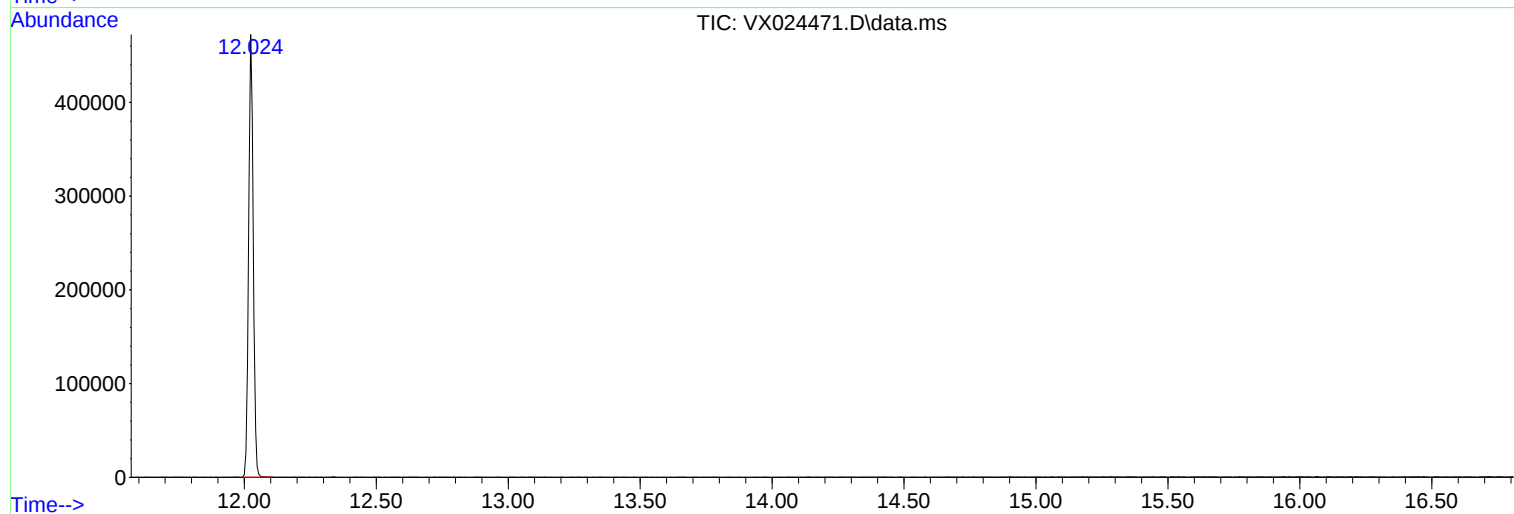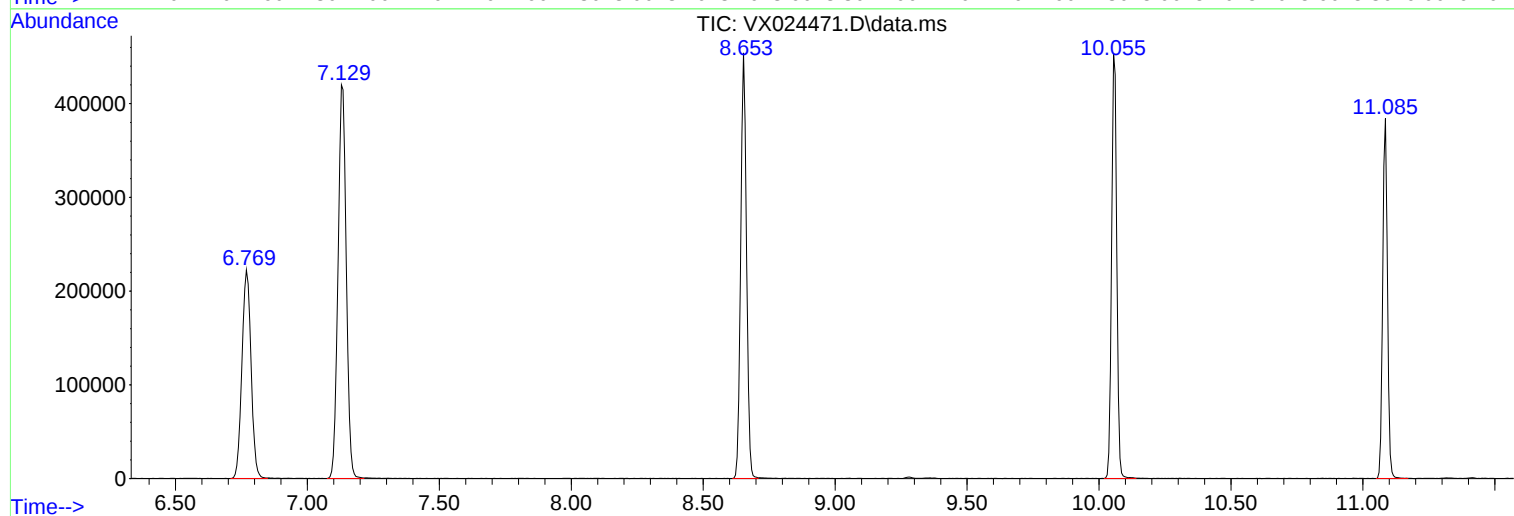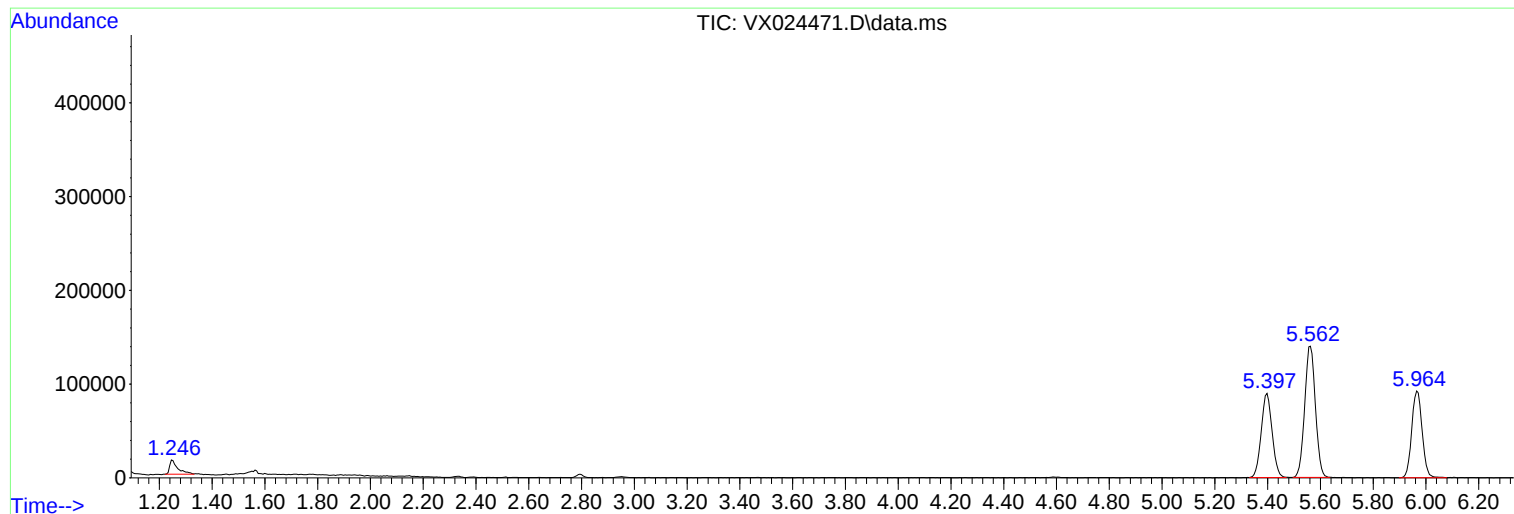

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024471.D
Acq On : 23 Sep 2021 23:57
Operator : JC/MD
Sample : M3833-13 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024471.D
Acq On : 23 Sep 2021 23:57
Operator : JC/MD
Sample : M3833-13 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE122D2-20210920

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
