

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024487.D
 Acq On : 24 Sep 2021 06:59
 Operator : JC/MD
 Sample : M3829-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE108D1-20210917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	21	26	41	rBV2	13849	30016	4.07%	0.653%
2	2.544	231	239	248	rBV	5911	11552	1.57%	0.251%
3	5.397	695	707	722	rBV2	97734	281319	38.18%	6.118%
4	5.562	722	734	747	rVV	160343	444832	60.36%	9.674%
5	5.964	787	800	814	rBV	96077	250582	34.00%	5.450%
6	6.769	922	932	945	rBV	235964	556720	75.55%	12.108%
7	7.129	982	991	1001	rBV	176814	386333	52.43%	8.402%
8	8.653	1234	1241	1254	rBV	486650	736908	100.00%	16.026%
9	9.275	1339	1343	1349	rBV	15584	22477	3.05%	0.489%
10	10.055	1465	1471	1483	rBV	545897	710528	96.42%	15.453%
11	11.085	1634	1640	1650	rBV	418193	542007	73.55%	11.788%
12	12.024	1789	1794	1809	rVB	519444	624852	84.79%	13.589%


Sum of corrected areas: 4598126

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024487.D
Acq On : 24 Sep 2021 06:59
Operator : JC/MD
Sample : M3829-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

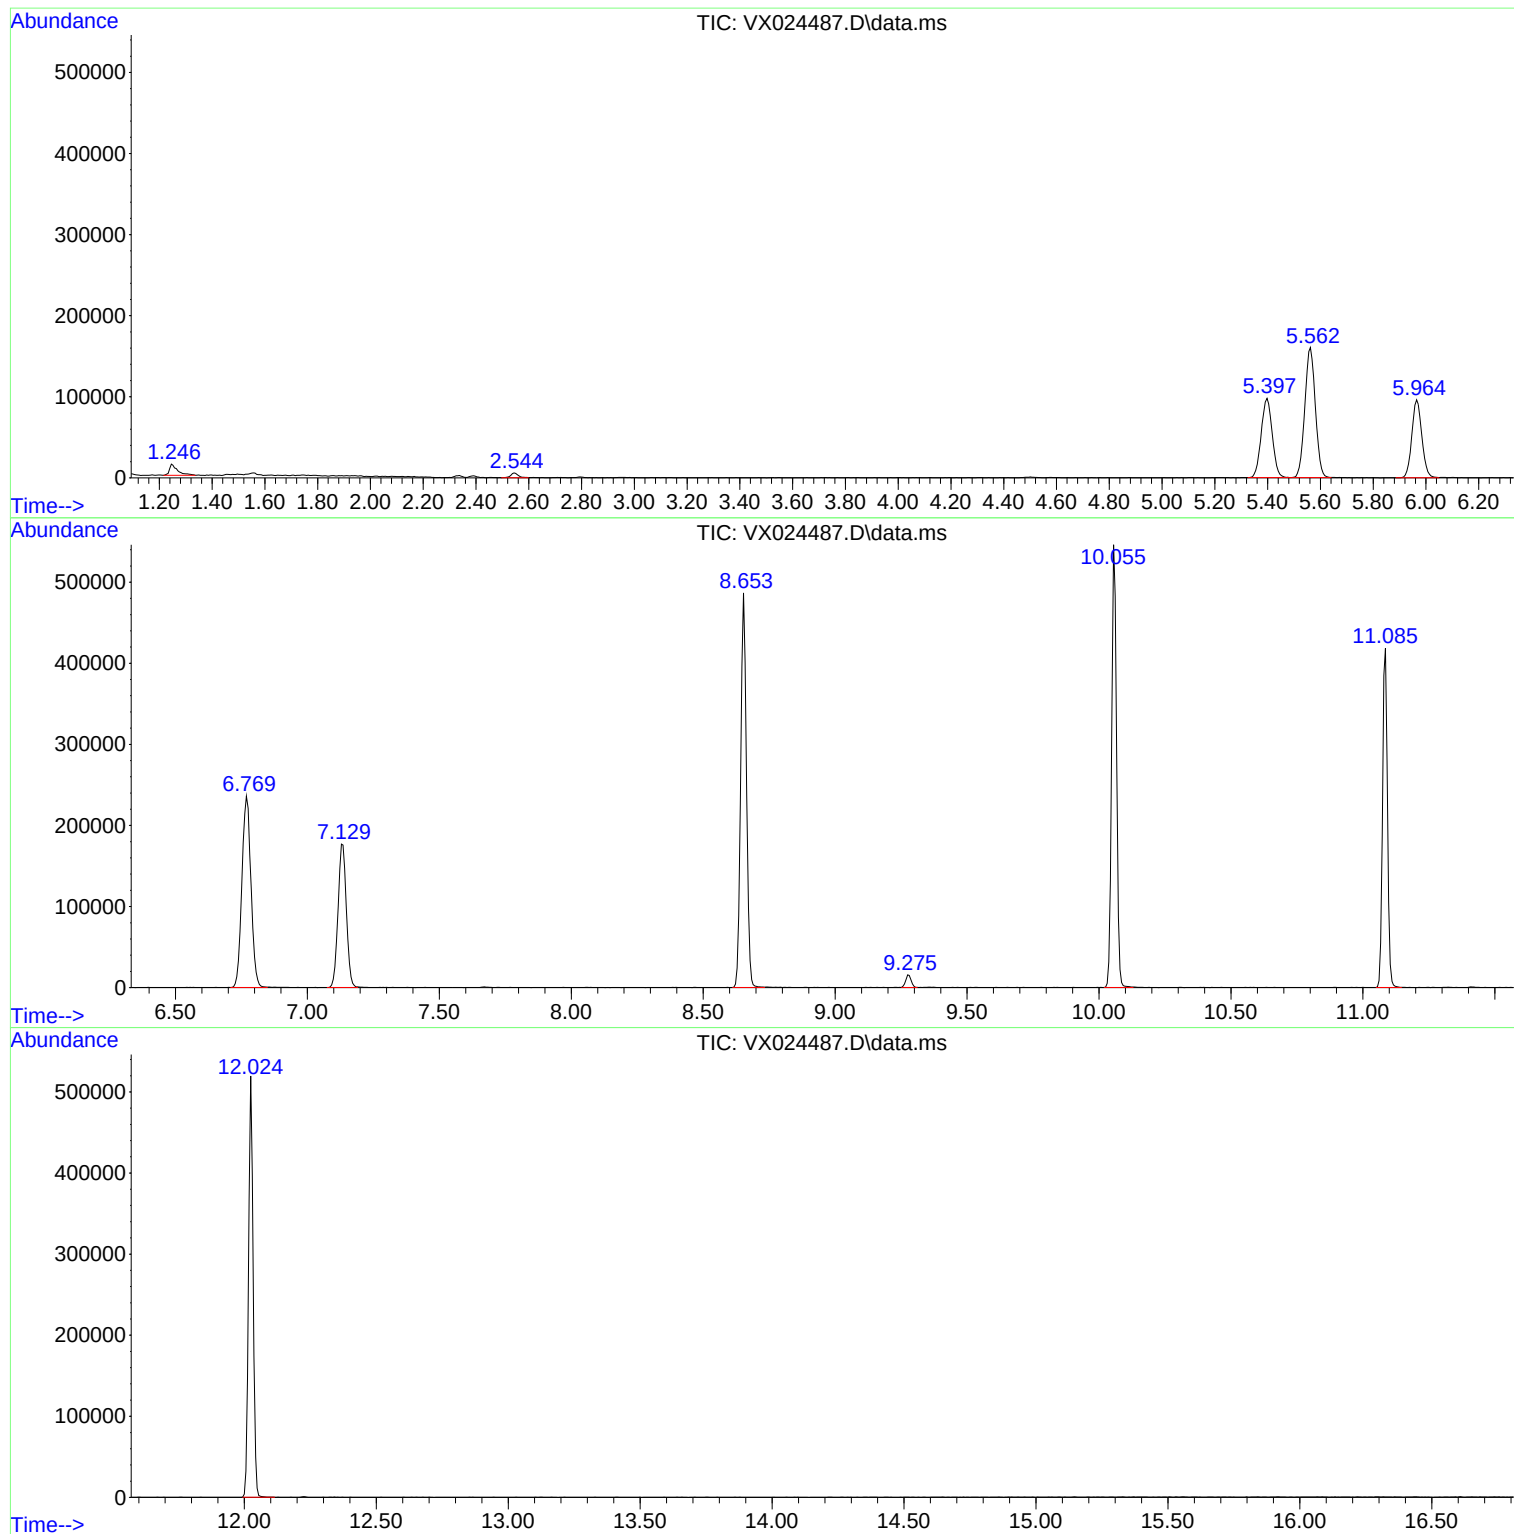

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024487.D
Acq On : 24 Sep 2021 06:59
Operator : JC/MD
Sample : M3829-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024487.D
Acq On : 24 Sep 2021 06:59
Operator : JC/MD
Sample : M3829-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE108D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
