

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024491.D
 Acq On : 24 Sep 2021 08:33
 Operator : JC/MD
 Sample : M3829-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D1-20210917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rBV	12871	29145	1.23%	0.454%
2	2.331	197	204	211	rBV2	35364	67862	2.87%	1.058%
3	4.495	550	559	570	rBV2	11601	31873	1.35%	0.497%
4	5.397	696	707	721	rBV	93555	264703	11.19%	4.127%
5	5.562	722	734	749	rVB	146639	402966	17.03%	6.283%
6	5.964	787	800	818	rBV	98846	253184	10.70%	3.948%
7	6.769	922	932	946	rBV	203807	484136	20.46%	7.549%
8	7.135	980	992	1013	rBV	1113401	2365679	100.00%	36.886%
9	8.653	1234	1241	1252	rBV	461900	727678	30.76%	11.346%
10	9.275	1337	1343	1350	rBV	87013	126586	5.35%	1.974%
11	10.055	1466	1471	1485	rBV	471345	658466	27.83%	10.267%
12	11.085	1634	1640	1653	rBV	369049	462246	19.54%	7.207%
13	12.024	1789	1794	1804	rVB	452243	538948	22.78%	8.403%




Sum of corrected areas: 6413472

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024491.D
Acq On : 24 Sep 2021 08:33
Operator : JC/MD
Sample : M3829-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

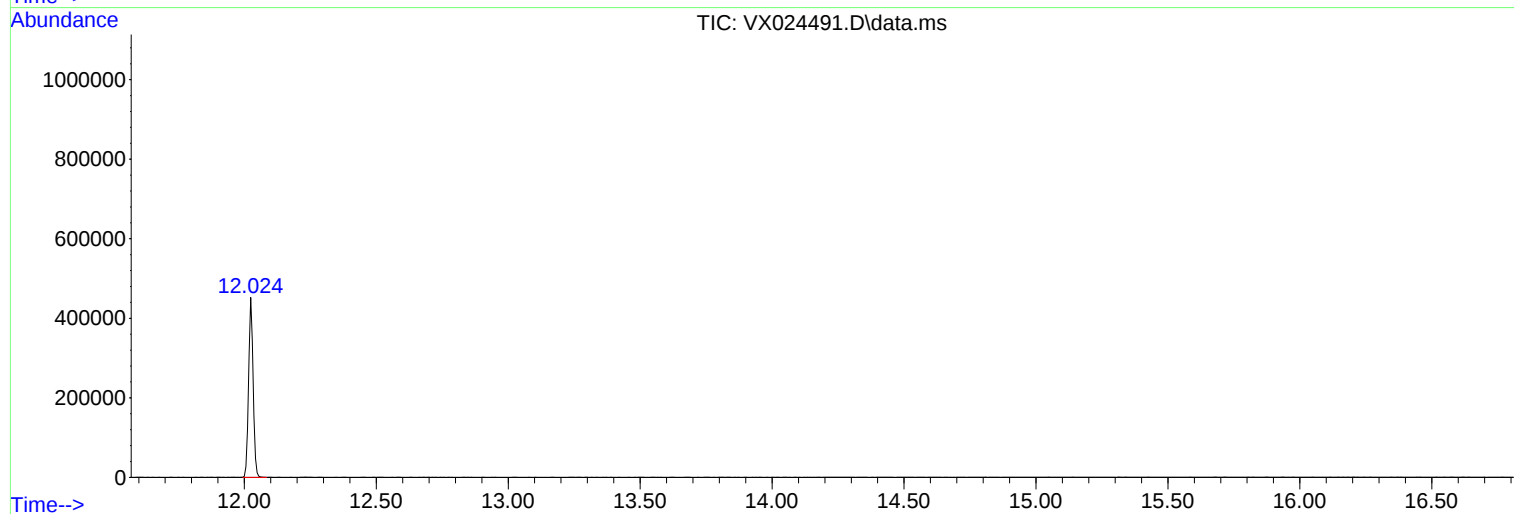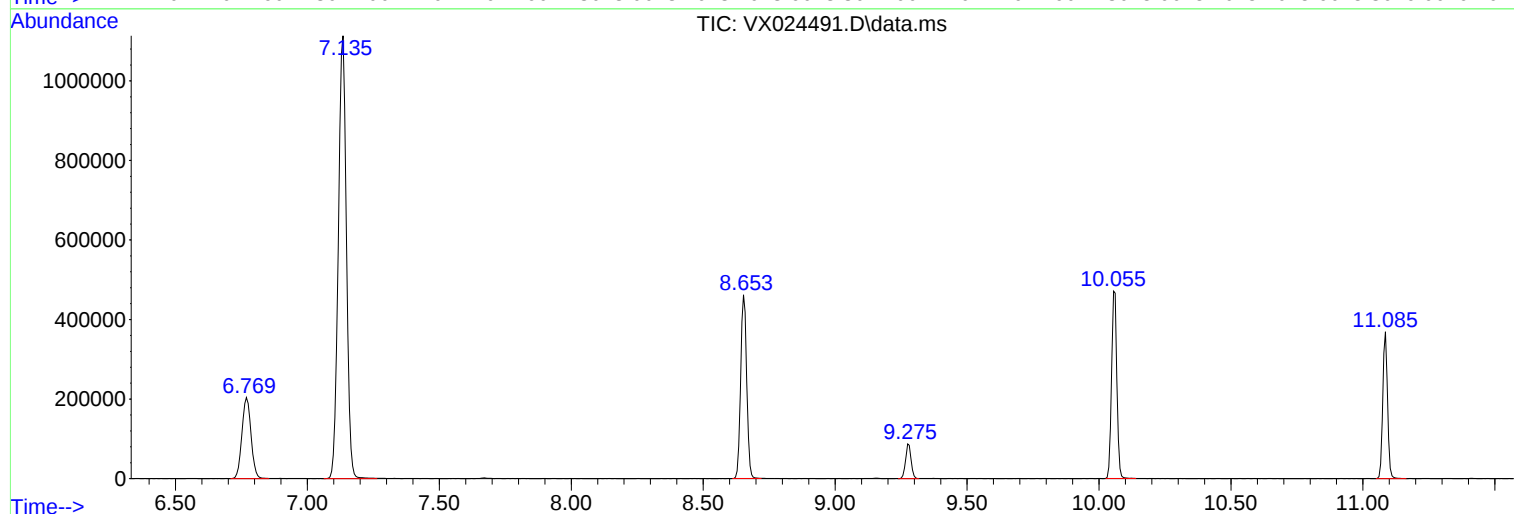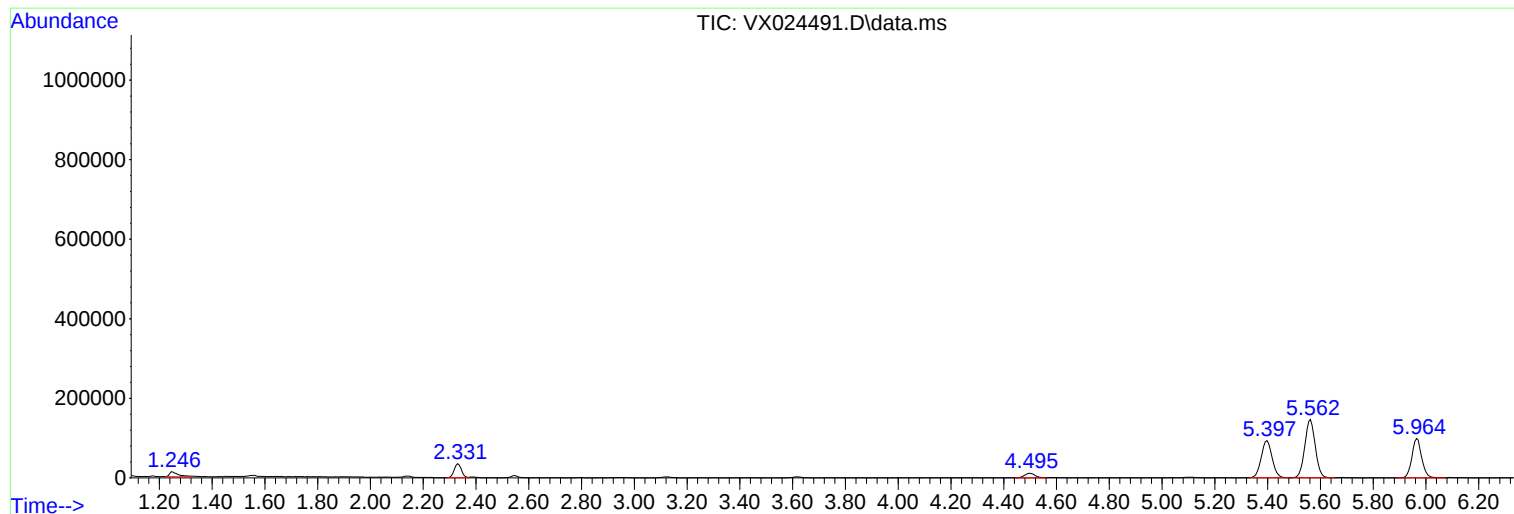

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024491.D
Acq On : 24 Sep 2021 08:33
Operator : JC/MD
Sample : M3829-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024491.D
Acq On : 24 Sep 2021 08:33
Operator : JC/MD
Sample : M3829-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D1-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
