

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024492.D
 Acq On : 24 Sep 2021 08:57
 Operator : JC/MD
 Sample : M3829-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D3-20210917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
 Title : SW846 8260

Signal : TIC: VX024492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	39	rVB2	9132	19576	1.06%	0.324%
2	2.331	195	204	220	rVB	267848	508446	27.51%	8.414%
3	2.538	233	238	246	rBV	10138	18495	1.00%	0.306%
4	5.397	695	707	720	rBV	81071	232472	12.58%	3.847%
5	5.562	723	734	748	rVB	125040	353468	19.13%	5.849%
6	5.964	790	800	815	rBV	86690	231269	12.51%	3.827%
7	6.769	921	932	947	rBV	203591	478133	25.87%	7.912%
8	7.135	982	992	1006	rBV	849015	1848067	100.00%	30.582%
9	8.653	1234	1241	1254	rBV	434011	665745	36.02%	11.017%
10	9.275	1338	1343	1351	rBV	55374	80758	4.37%	1.336%
11	10.055	1465	1471	1487	rBV	454283	602143	32.58%	9.964%
12	11.085	1634	1640	1650	rBV	367564	463870	25.10%	7.676%
13	12.024	1789	1794	1805	rBV	447773	540481	29.25%	8.944%




Sum of corrected areas: 6042923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024492.D
Acq On : 24 Sep 2021 08:57
Operator : JC/MD
Sample : M3829-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

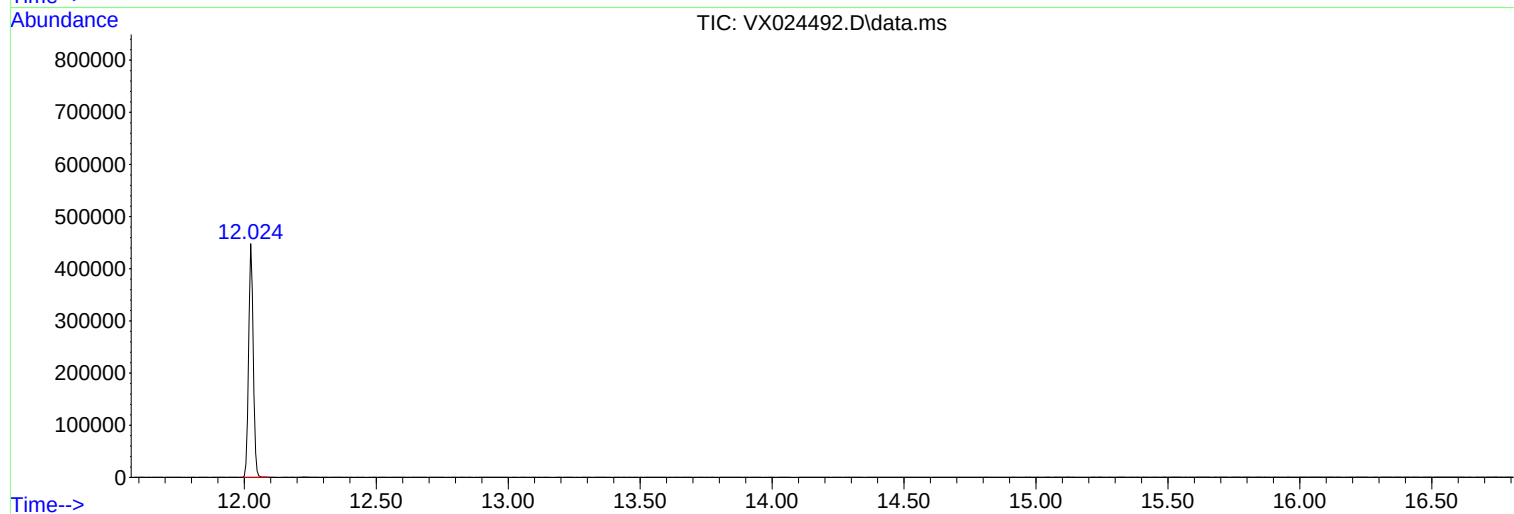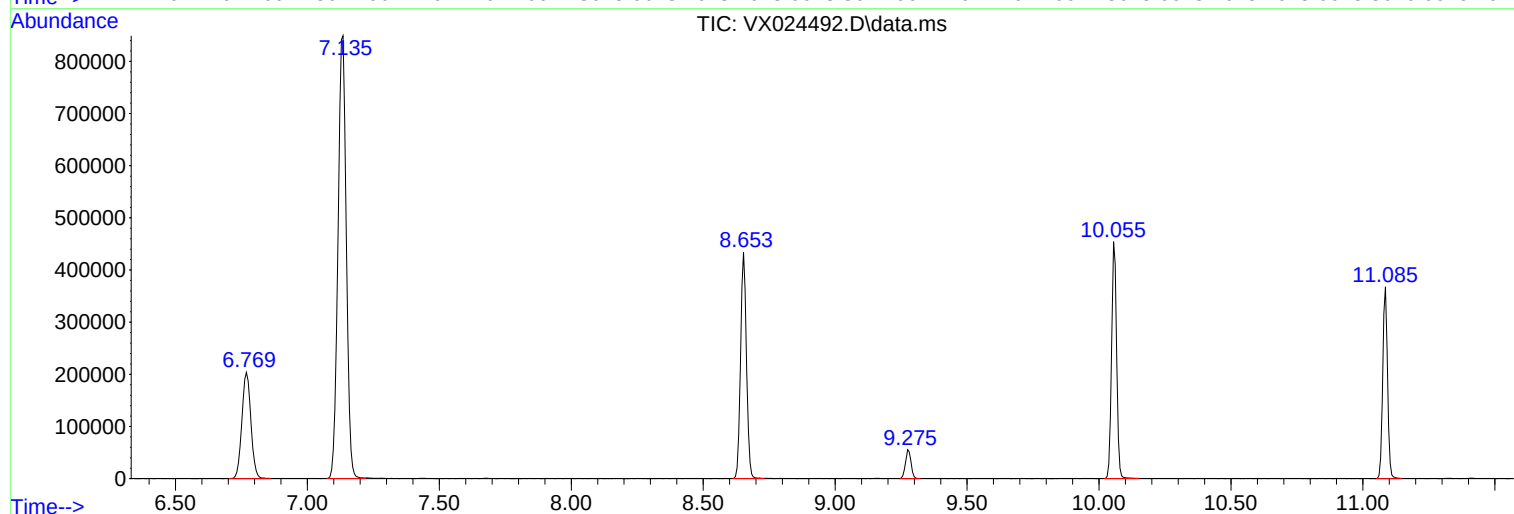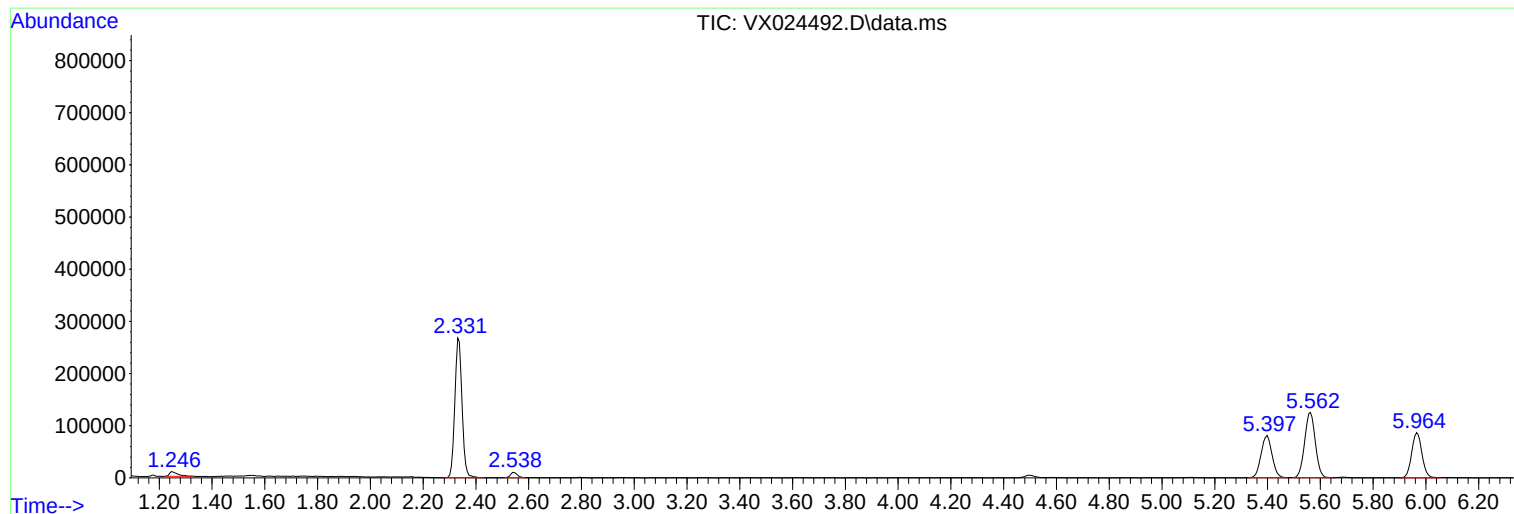

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024492.D
Acq On : 24 Sep 2021 08:57
Operator : JC/MD
Sample : M3829-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024492.D
Acq On : 24 Sep 2021 08:57
Operator : JC/MD
Sample : M3829-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
