

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
 Data File : VX024493.D
 Acq On : 24 Sep 2021 09:20
 Operator : JC/MD
 Sample : M3829-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE120D3-20210917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M

Title : SW846 8260

Signal : TIC: VX024493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	33	rBV	9952	15811	2.30%	0.403%
2	2.538	232	238	245	rBV	6486	11788	1.71%	0.301%
3	5.397	691	707	722	rBV	83224	240006	34.86%	6.120%
4	5.562	722	734	750	rVB2	131046	368579	53.54%	9.399%
5	5.964	790	800	813	rBV	91164	240501	34.94%	6.133%
6	6.769	922	932	944	rBV	208793	494160	71.78%	12.601%
7	7.129	983	991	1006	rVB	112551	245360	35.64%	6.257%
8	8.653	1234	1241	1253	rBV	450905	688402	100.00%	17.555%
9	10.055	1466	1471	1487	rVB	458079	617420	89.69%	15.745%
10	11.085	1634	1640	1649	rBV	376543	467544	67.92%	11.923%
11	12.024	1789	1794	1804	rVB	435282	531874	77.26%	13.563%




Sum of corrected areas: 3921445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024493.D
Acq On : 24 Sep 2021 09:20
Operator : JC/MD
Sample : M3829-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

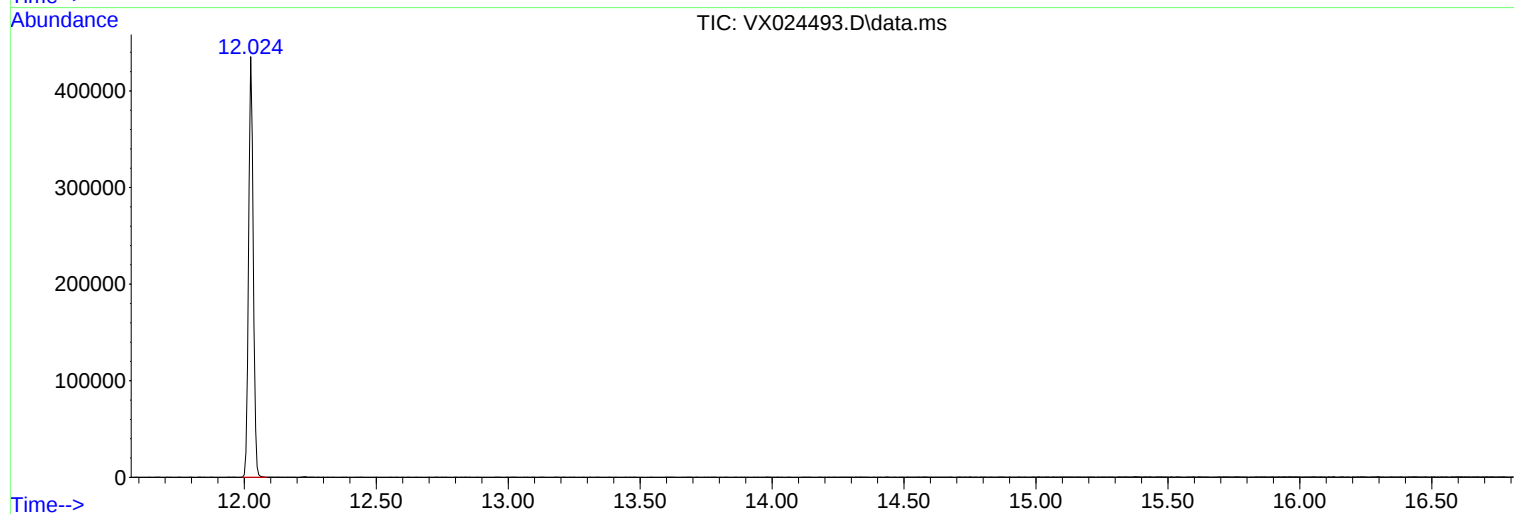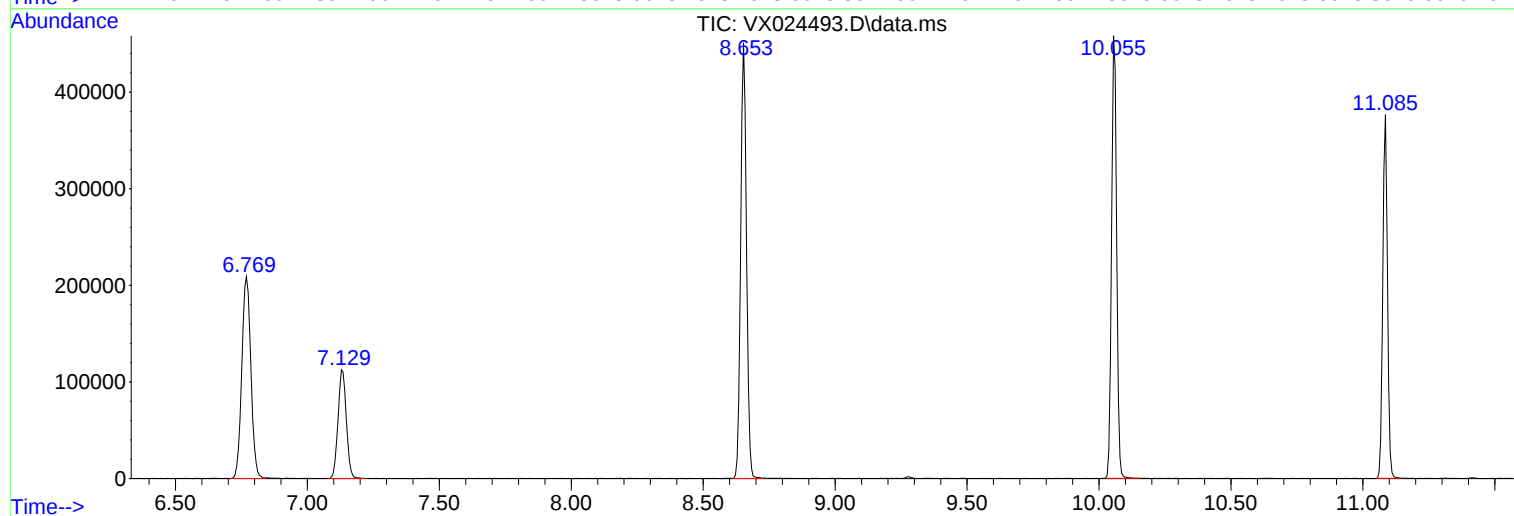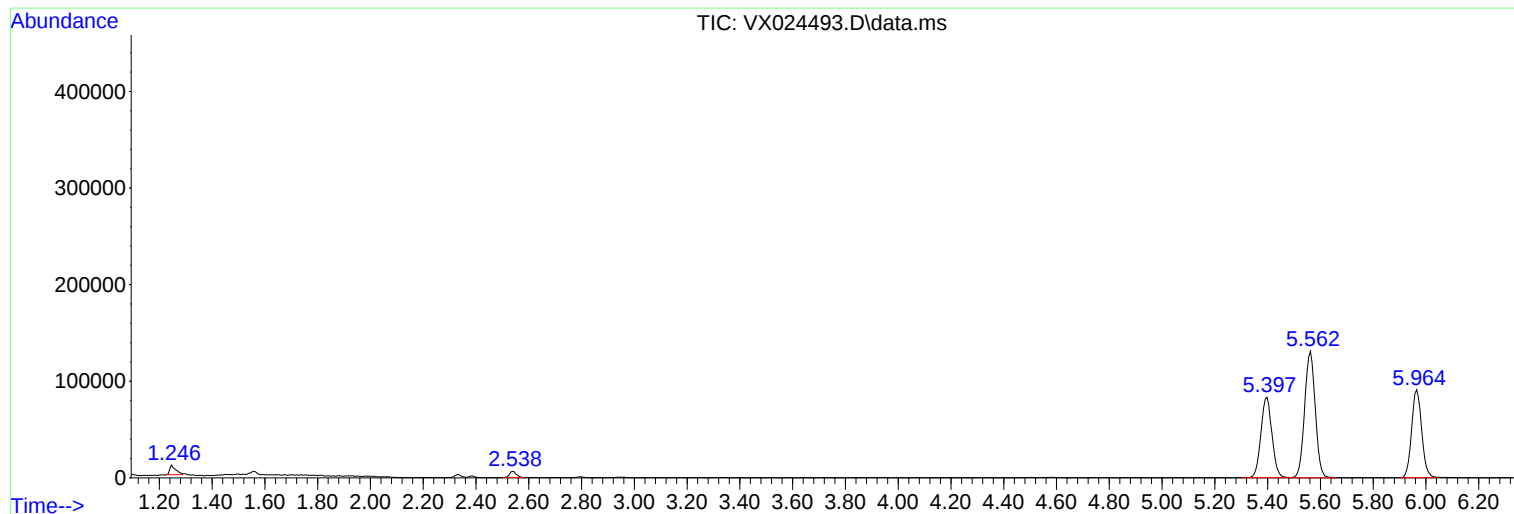

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024493.D
Acq On : 24 Sep 2021 09:20
Operator : JC/MD
Sample : M3829-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092321\
Data File : VX024493.D
Acq On : 24 Sep 2021 09:20
Operator : JC/MD
Sample : M3829-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D3-20210917

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092321W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
