



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092324\
Data File : VX043099.D
Acq On : 23 Sep 2024 07:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X092324W.M
Title : SW846 8260
Last Update : Tue Sep 24 03:13:52 2024

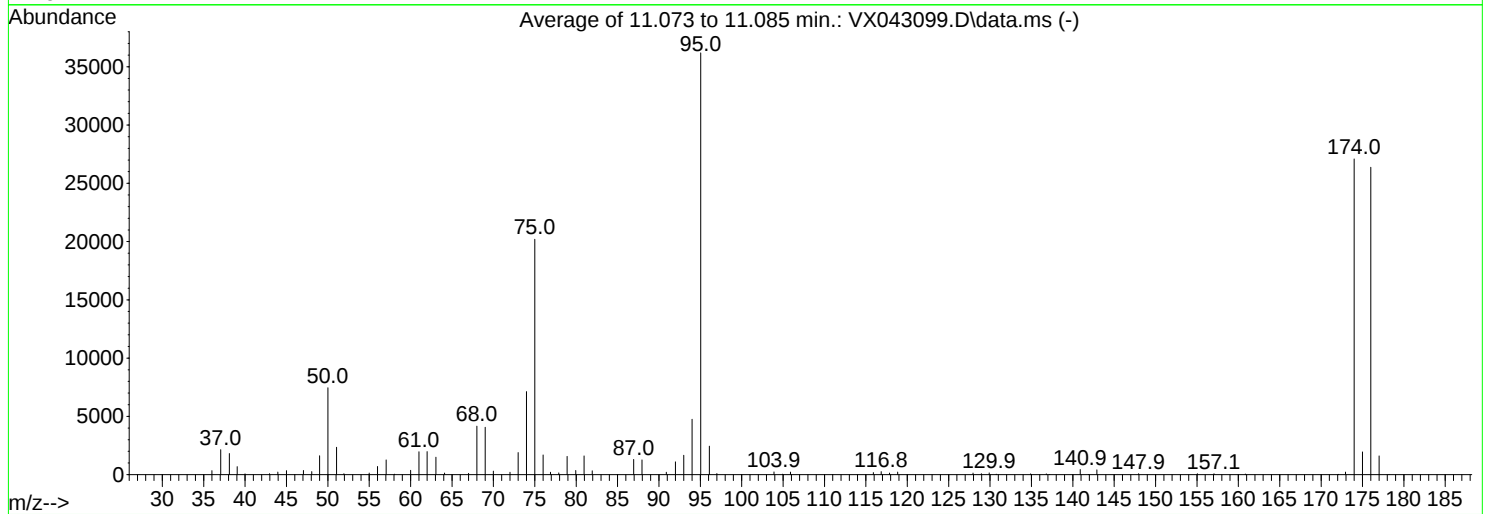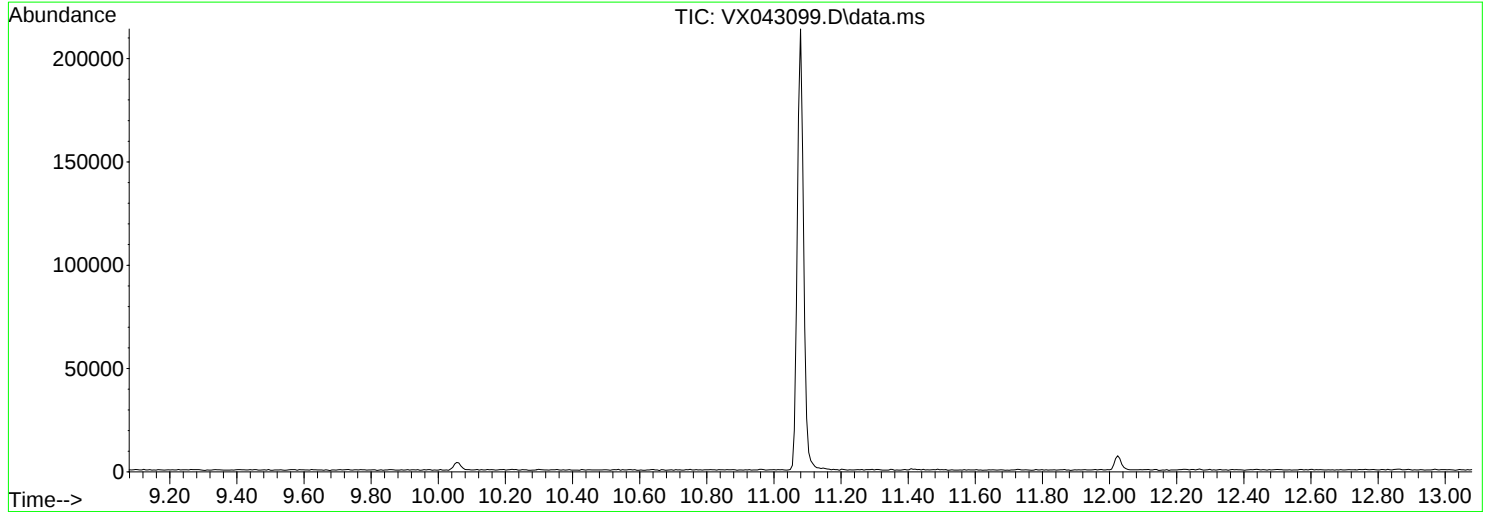

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	7456	PASS
75	95	30	60	55.8	20198	PASS
95	95	100	100	100.0	36195	PASS
96	95	5	9	6.8	2447	PASS
173	174	0.00	2	0.8	226	PASS
174	95	50	100	74.9	27096	PASS
175	174	5	9	7.2	1954	PASS
176	174	95	101	97.4	26381	PASS
177	176	5	9	6.1	1608	PASS