

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047739.D
Acq On : 23 Sep 2025 17:16
Operator : JC/MD
Sample : Q3097-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20250912

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M

Title : SW846 8260

Signal : TIC: VX047739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.337	197	205	231	rBV	287714	630418	15.44%	6.709%
2	5.373	691	703	720	rBV3	85380	277386	6.79%	2.952%
3	5.544	720	731	749	rVB	122572	381989	9.36%	4.065%
4	5.946	785	797	817	rBV	92667	274337	6.72%	2.920%
5	6.751	917	929	944	rBV	242602	631971	15.48%	6.726%
6	7.110	975	988	1013	rBV	1755117	4083176	100.00%	43.456%
7	8.635	1231	1238	1253	rBV	487653	790214	19.35%	8.410%
8	9.256	1335	1340	1353	rVB2	69575	109347	2.68%	1.164%
9	10.037	1462	1468	1487	rBV	579774	816076	19.99%	8.685%
10	11.067	1631	1637	1647	rBV	417720	574810	14.08%	6.118%
11	12.006	1785	1791	1803	rBV	626225	826355	20.24%	8.795%




Sum of corrected areas: 9396079

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047739.D
Acq On : 23 Sep 2025 17:16
Operator : JC/MD
Sample : Q3097-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20250912

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

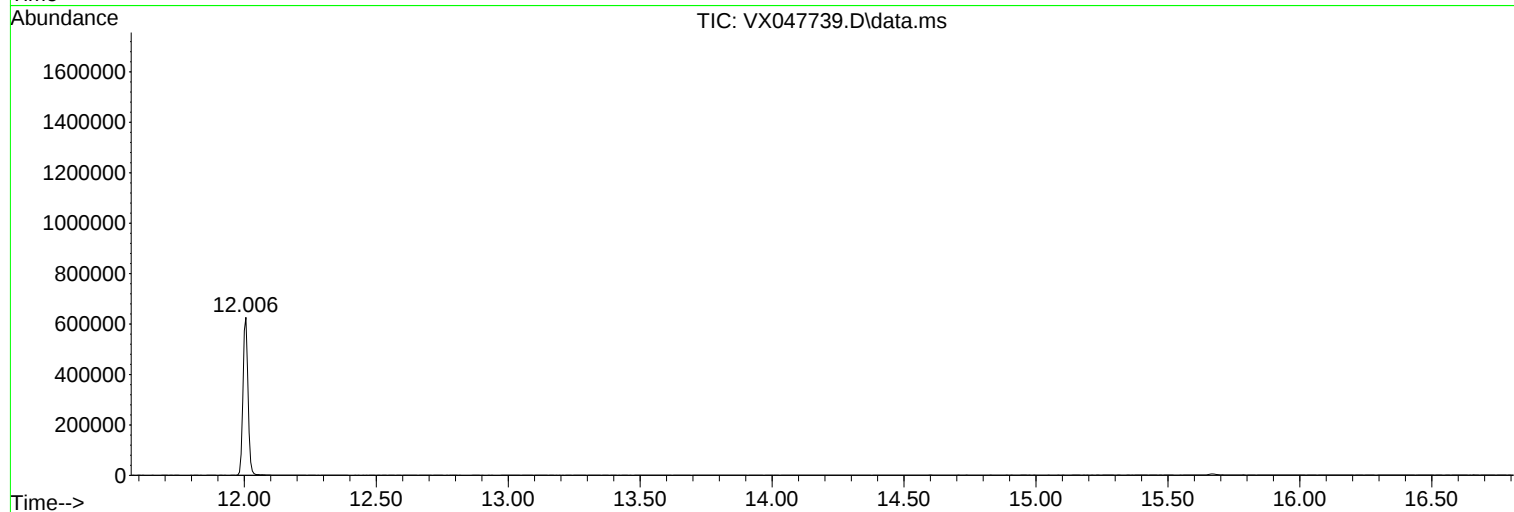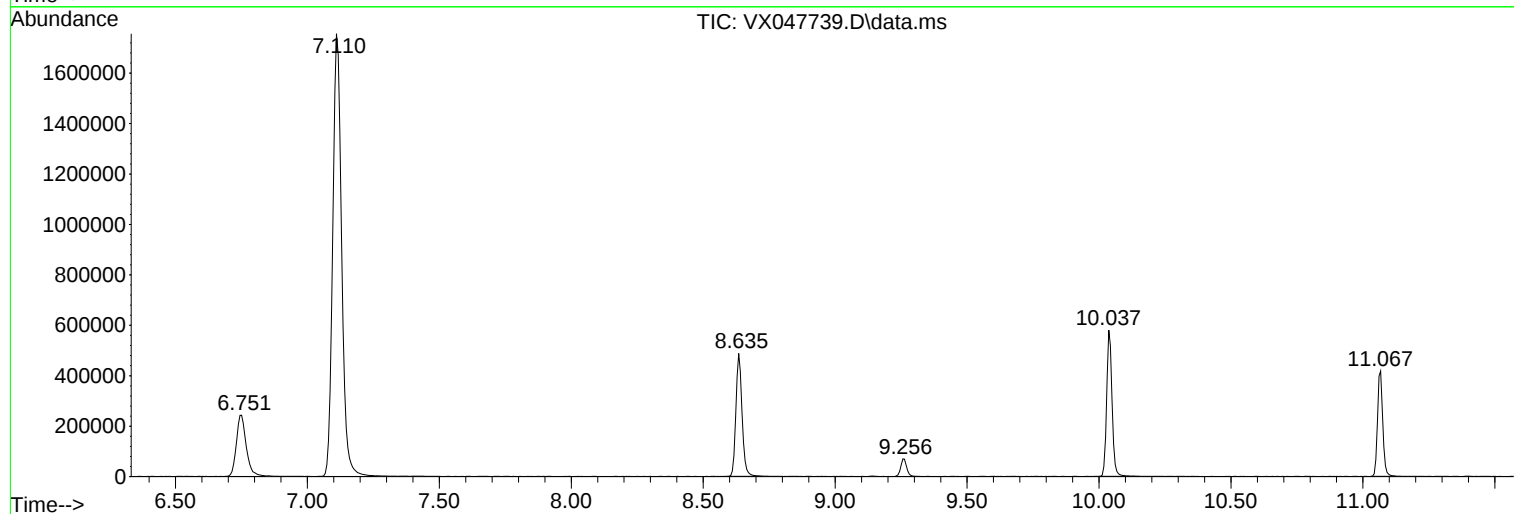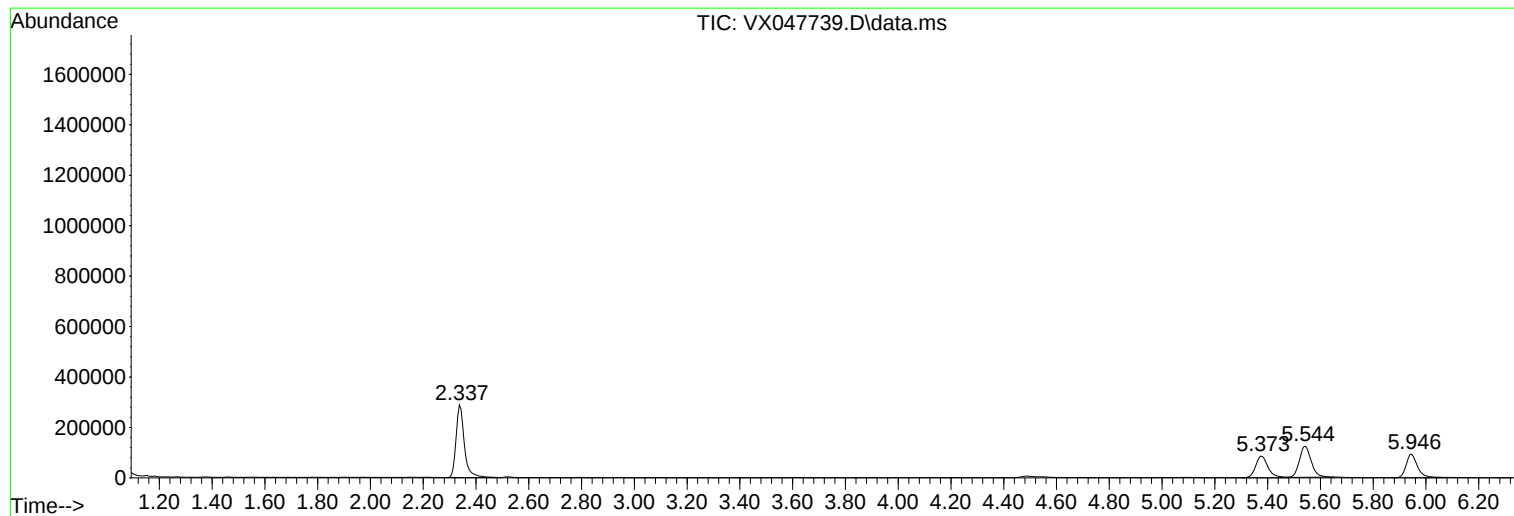

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047739.D
Acq On : 23 Sep 2025 17:16
Operator : JC/MD
Sample : Q3097-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20250912

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047739.D
Acq On : 23 Sep 2025 17:16
Operator : JC/MD
Sample : Q3097-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE120D2-20250912

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc