

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
 Data File : VX047762.D
 Acq On : 24 Sep 2025 09:04
 Operator : JC/MD
 Sample : Q3127-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP07-20250915

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M

Title : SW846 8260

Signal : TIC: VX047762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.483	549	557	571	rBV4	8756	29744	1.41%	0.440%
2	5.379	689	704	720	rBV3	82526	272541	12.89%	4.034%
3	5.538	720	730	753	rVB	117821	375400	17.75%	5.557%
4	5.946	786	797	818	rBV	89720	269118	12.73%	3.984%
5	6.751	918	929	945	rBV	233844	610855	28.89%	9.043%
6	7.110	978	988	1013	rBV	916632	2114394	100.00%	31.299%
7	8.635	1231	1238	1257	rBV	470313	775712	36.69%	11.483%
8	9.256	1334	1340	1351	rBV2	114458	180679	8.55%	2.675%
9	10.037	1462	1468	1485	rBV	545305	790072	37.37%	11.695%
10	11.067	1631	1637	1652	rBV	408483	560315	26.50%	8.294%
11	12.006	1785	1791	1801	rBV	583533	776545	36.73%	11.495%




Sum of corrected areas: 6755375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047762.D
Acq On : 24 Sep 2025 09:04
Operator : JC/MD
Sample : Q3127-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20250915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

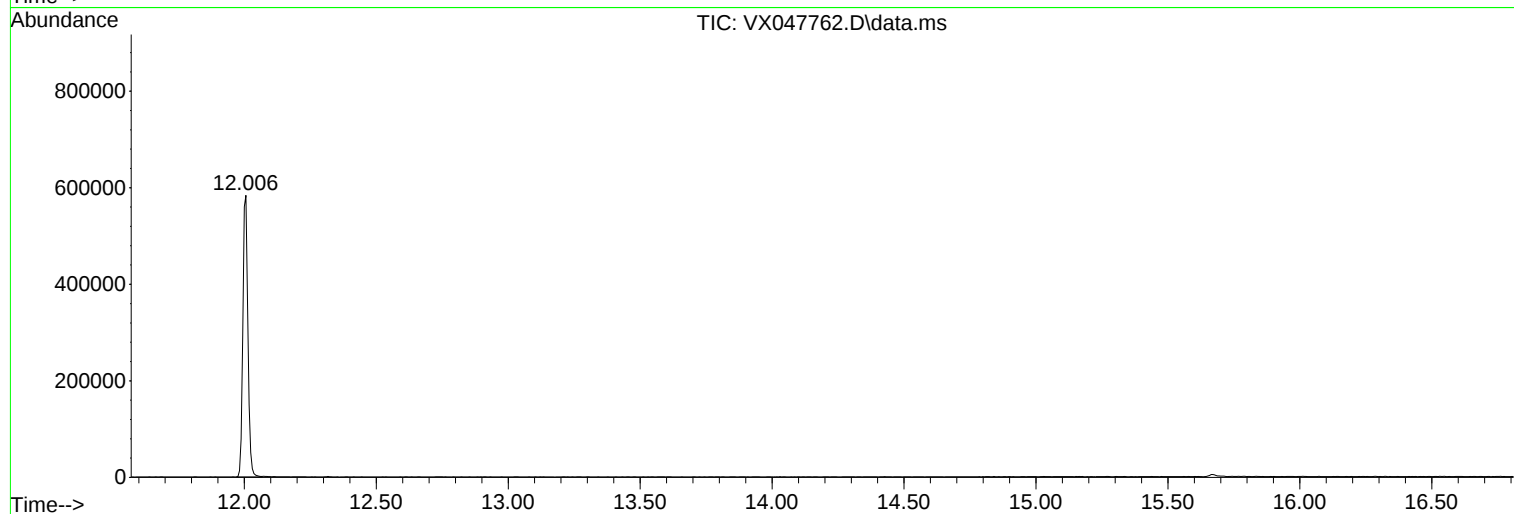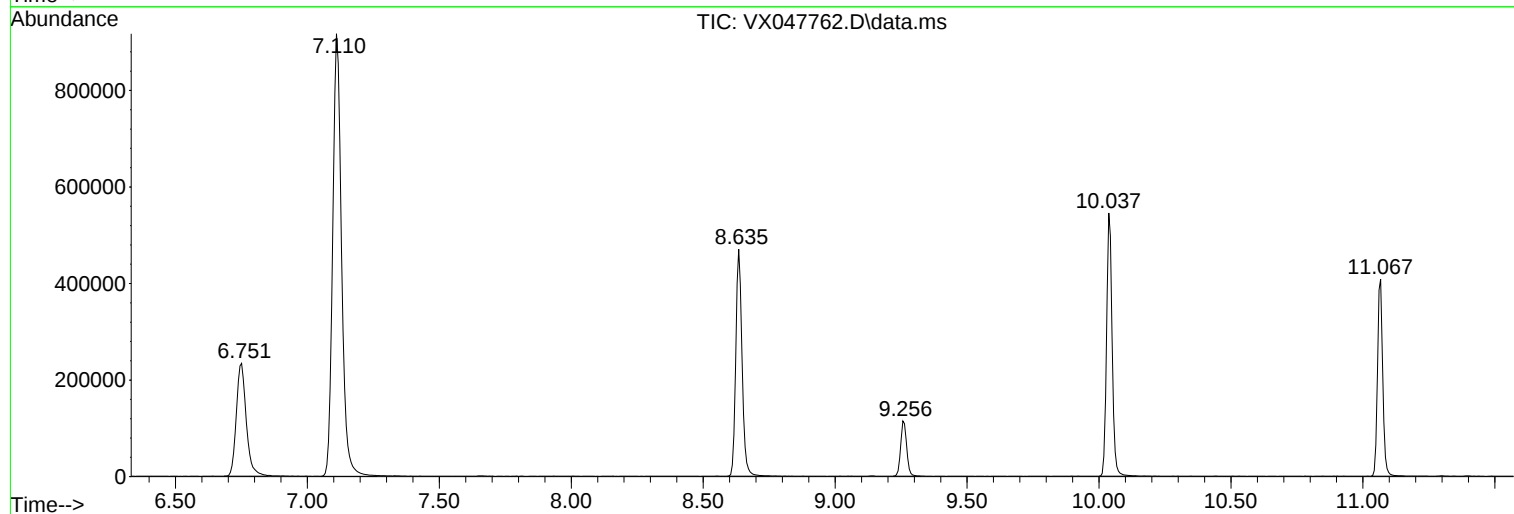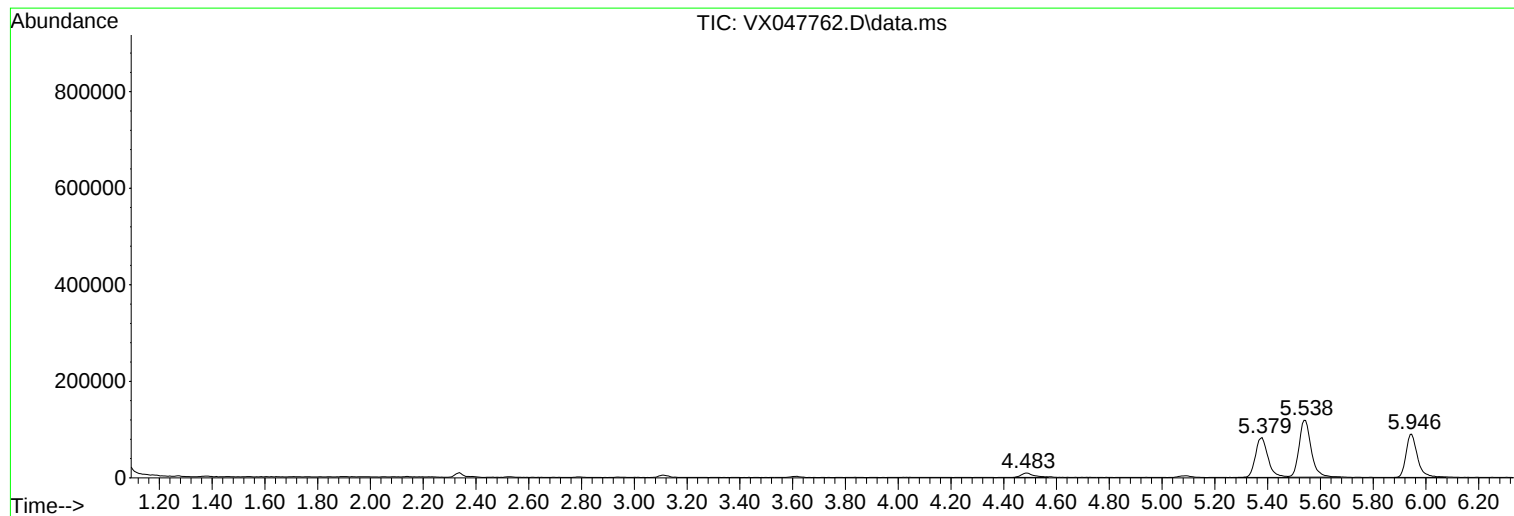

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047762.D
Acq On : 24 Sep 2025 09:04
Operator : JC/MD
Sample : Q3127-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20250915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092325\
Data File : VX047762.D
Acq On : 24 Sep 2025 09:04
Operator : JC/MD
Sample : Q3127-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP07-20250915

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc