

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092420\  
 Data File : VX018563.D  
 Acq On : 24 Sep 2020 11:47  
 Operator : JC/SP  
 Sample : L4083-17  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 FB01-20200917

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X091720W.M

Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.434       | 215           | 221         | 230          | rVB      | 16023          | 31024         | 1.26%           | 0.220%        |
| 2         | 2.629       | 245           | 253         | 259          | rBV3     | 12206          | 43237         | 1.76%           | 0.307%        |
| 3         | 5.470       | 706           | 719         | 734          | rBV      | 311085         | 907424        | 36.98%          | 6.449%        |
| 4         | 5.629       | 734           | 745         | 758          | rBV2     | 513593         | 1435284       | 58.49%          | 10.200%       |
| 5         | 6.031       | 799           | 811         | 822          | rBV      | 336605         | 876365        | 35.71%          | 6.228%        |
| 6         | 6.830       | 932           | 942         | 955          | rBV      | 767902         | 1807212       | 73.65%          | 12.843%       |
| 7         | 8.695       | 1241          | 1248        | 1255         | rVV      | 1600749        | 2453838       | 100.00%         | 17.439%       |
| 8         | 8.763       | 1255          | 1259        | 1268         | rVB      | 265004         | 421908        | 17.19%          | 2.998%        |
| 9         | 10.098      | 1472          | 1478        | 1488         | rBV      | 1621794        | 2195872       | 89.49%          | 15.606%       |
| 10        | 11.122      | 1640          | 1646        | 1656         | rBV      | 1376627        | 1723812       | 70.25%          | 12.251%       |
| 11        | 12.061      | 1795          | 1800        | 1808         | rBV      | 1765090        | 2175157       | 88.64%          | 15.458%       |


Sum of corrected areas: 14071133

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092420\  
Data File : VX018563.D  
Acq On : 24 Sep 2020 11:47  
Operator : JC/SP  
Sample : L4083-17  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20200917

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

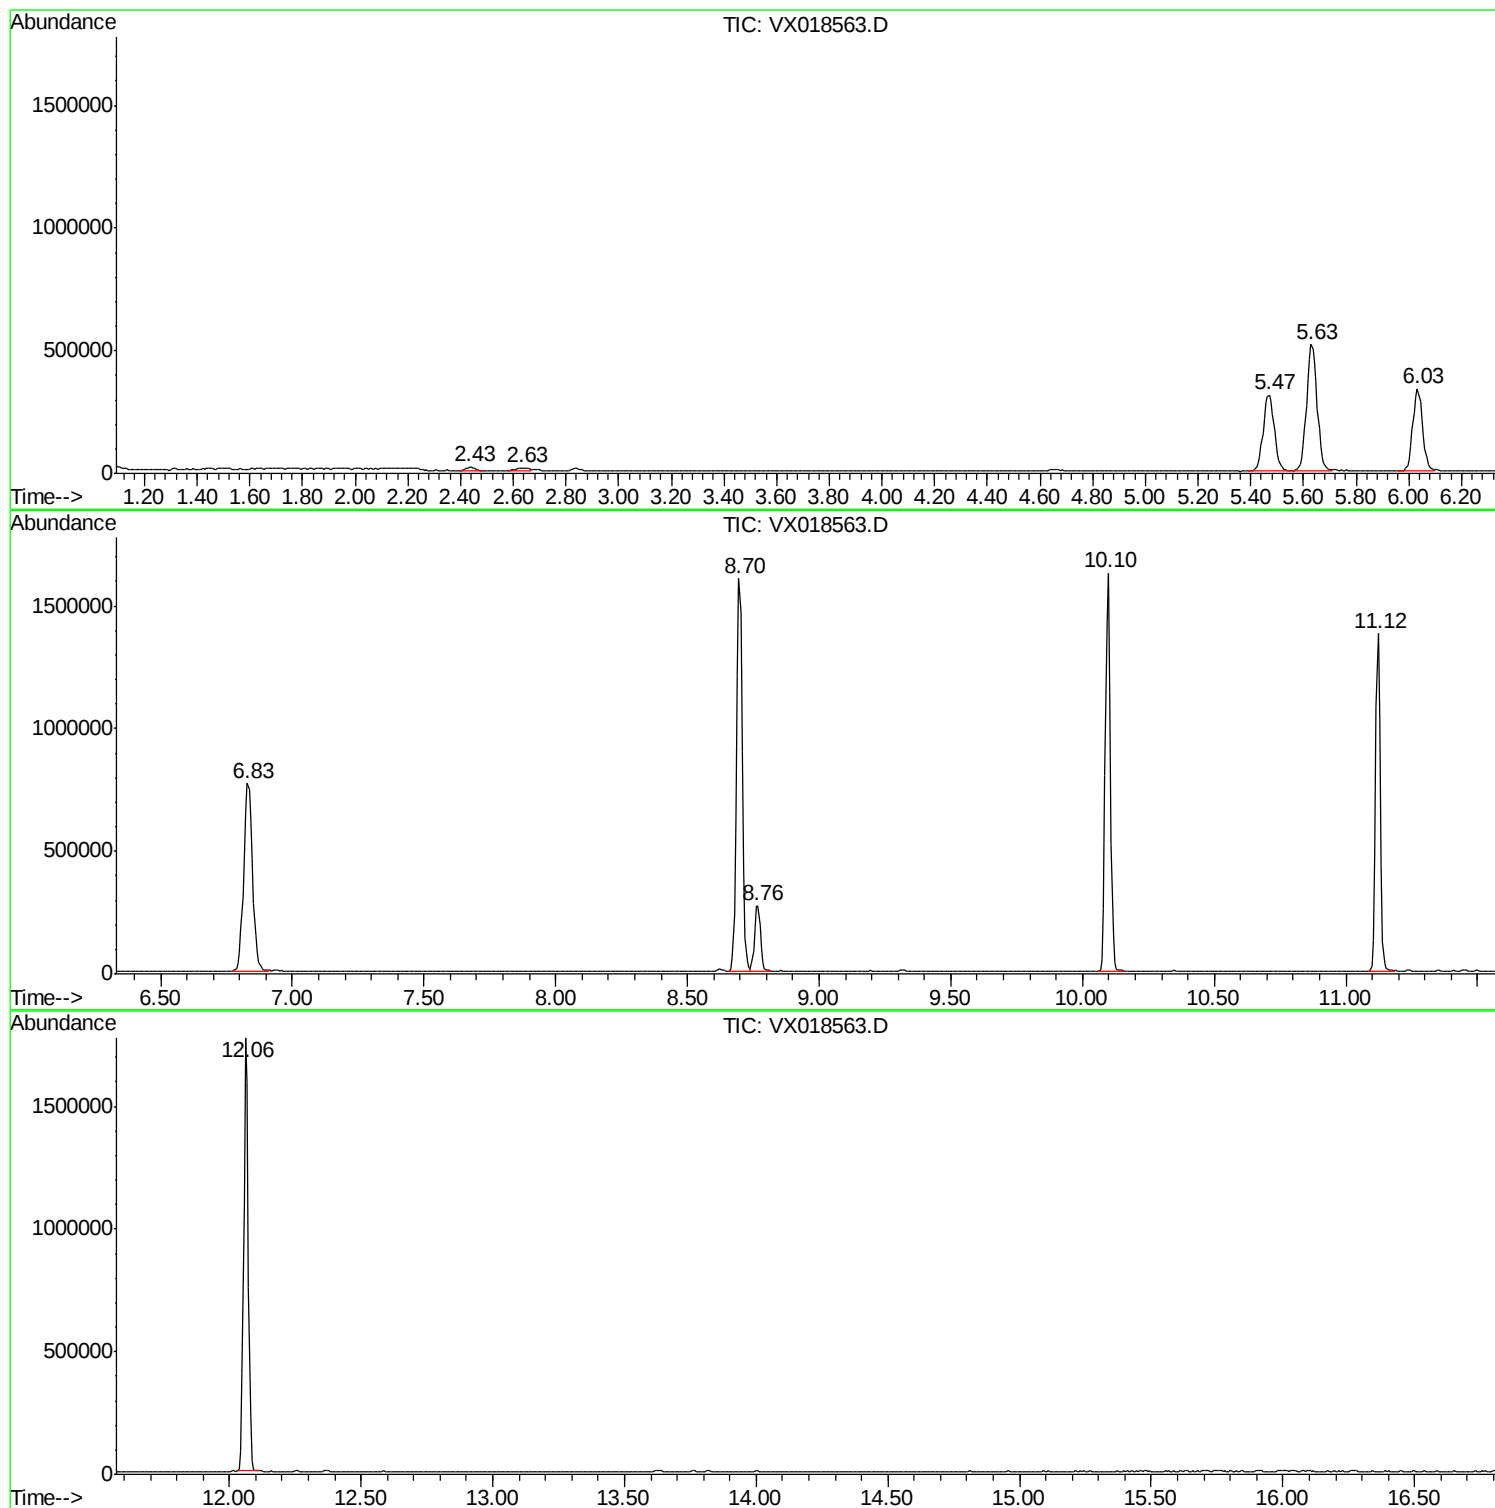

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX092420\  
Data File : VX018563.D  
Acq On : 24 Sep 2020 11:47  
Operator : JC/SP  
Sample : L4083-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20200917

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX092420\  
Data File : VX018563.D  
Acq On : 24 Sep 2020 11:47  
Operator : JC/SP  
Sample : L4083-17  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
FB01-20200917

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X091720W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |