

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092519\
 Data File : VX012650.D
 Acq On : 25 Sep 2019 10:48
 Operator : JC/SP
 Sample : VX0925WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0925WBL01

Quant Time: Sep 25 23:26:02 2019
 Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
 Quant Title : SW846 8260
 QLast Update : Mon Sep 23 12:27:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	178871	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	310345	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	255462	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	96369	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.05	65	131883	50.63	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.26%	
35) Dibromofluoromethane	5.48	113	93643	50.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.34%	
50) Toluene-d8	8.71	98	361985	50.86	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.72%	
62) 4-Bromofluorobenzene	11.14	95	123143	44.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092519\
Data File : VX012650.D
Acq On : 25 Sep 2019 10:48
Operator : JC/SP
Sample : VX0925WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0925WBL01

Quant Time: Sep 25 23:26:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Quant Title : SW846 8260
QLast Update : Mon Sep 23 12:27:01 2019
Response via : Initial Calibration

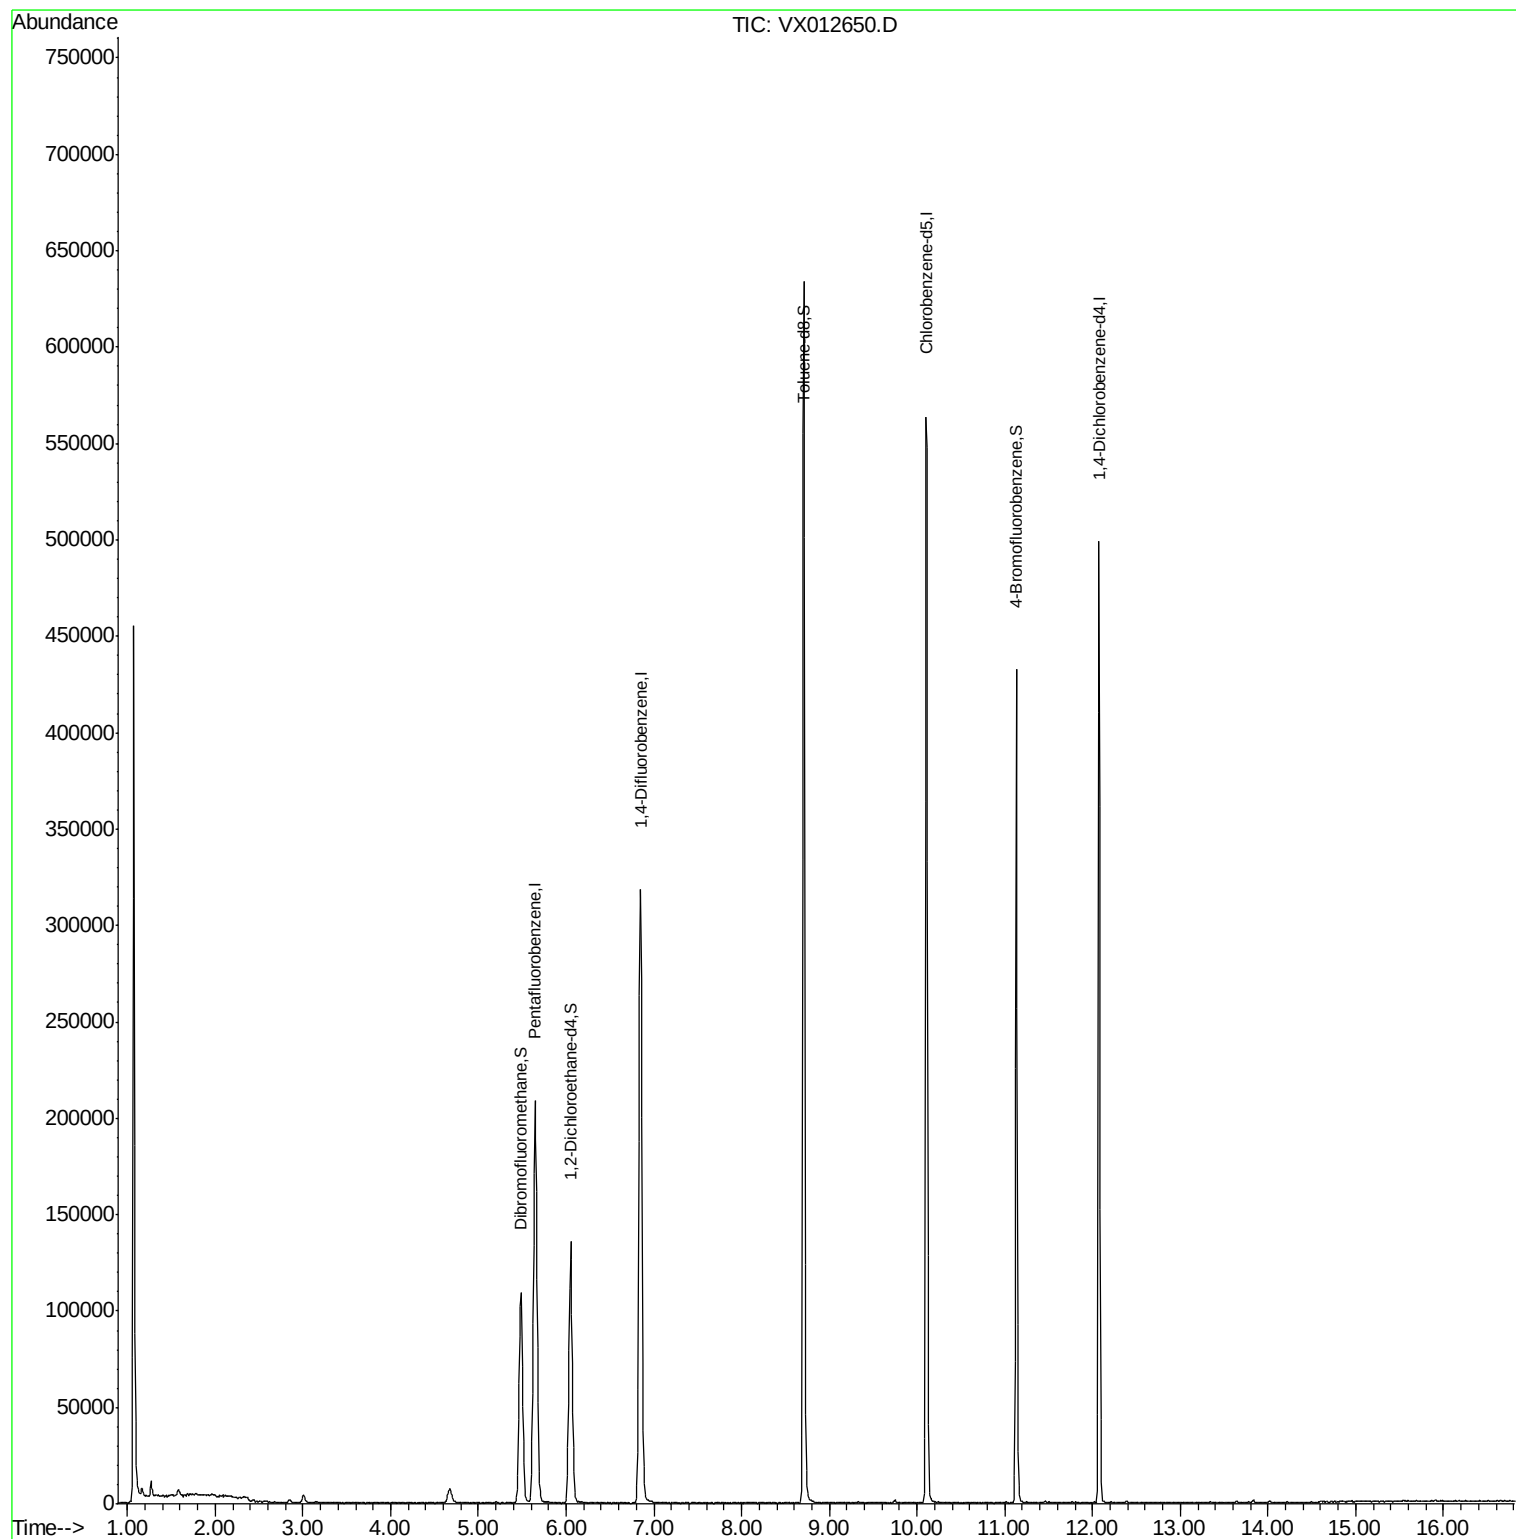

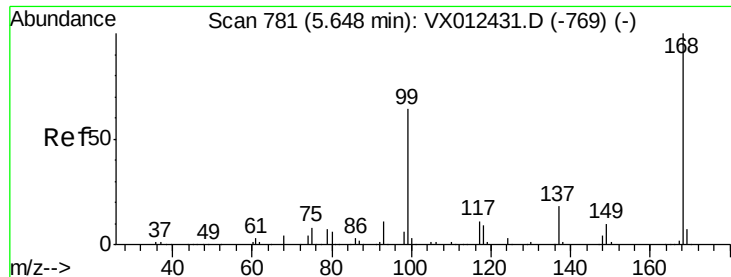

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 781

Delta R.T. 0.00 min

Lab File: VX012650.D

Acq: 25 Sep 2019 10:48

Instrument :

MSVOA_X

ClientSampleId :


VX0925WBL01

Tot Ion:168 Resp: 178871

Ion Ratio Lower Upper




168 100

99 70.4 51.4 77.2

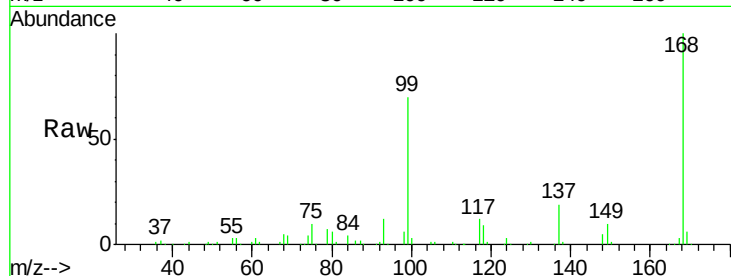

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

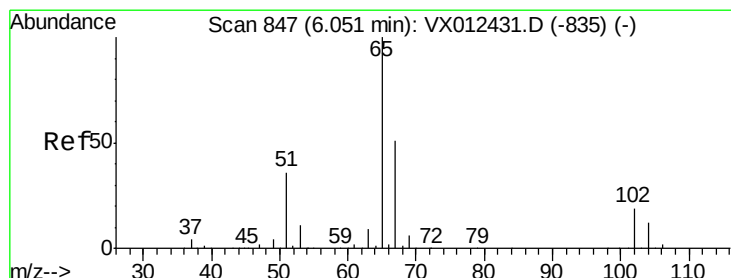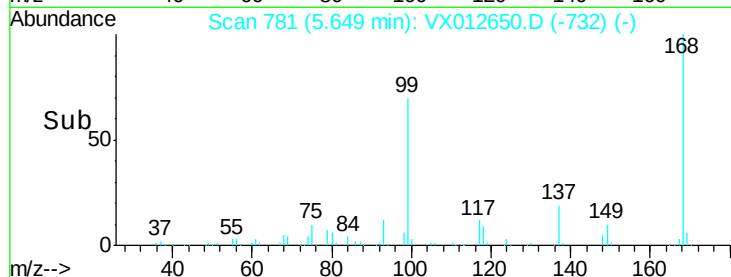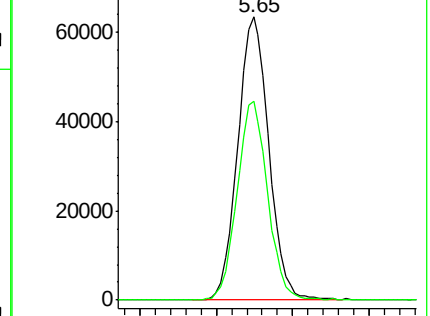

#33

1,2-Dichloroethane-d4

Concen: 50.633 ug/l

RT: 6.05 min Scan# 847

Delta R.T. 0.00 min

Lab File: VX012650.D


Acq: 25 Sep 2019 10:48

Tgt Ion: 65 Resp: 131883

Ion Ratio Lower Upper



65 100


67 50.6 0.0 101.2

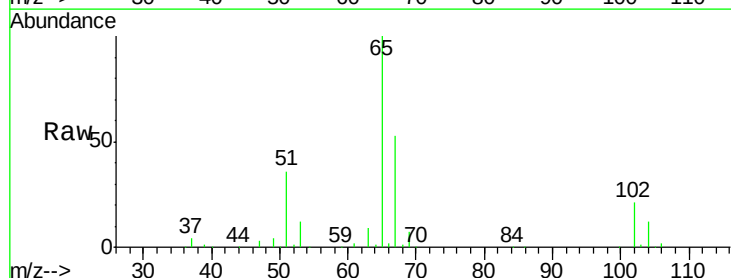

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0



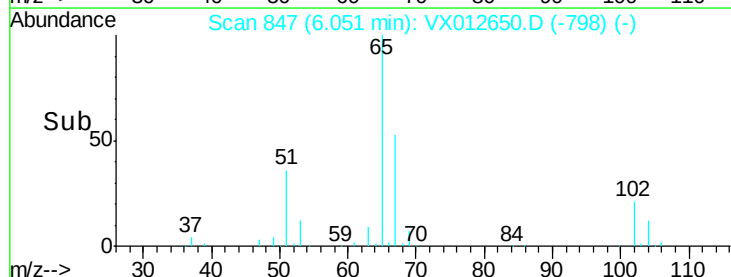
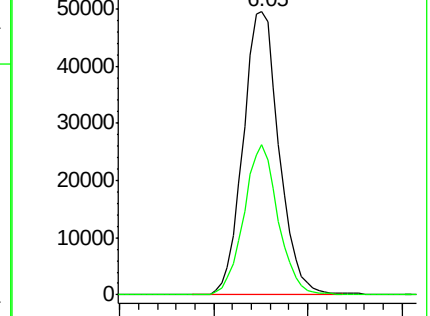


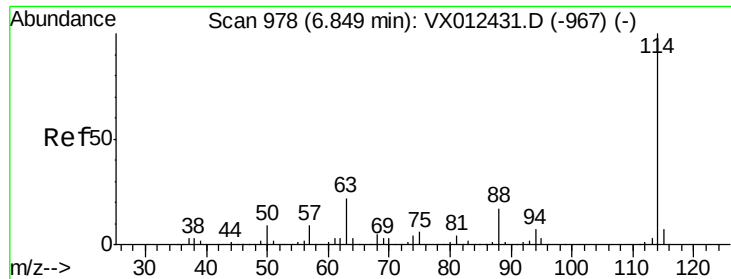

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 978
 Delta R.T. 0.00 min
 Lab File: VX012650.D
 Acq: 25 Sep 2019 10:48




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0925WBL01


Tot Ion	Ratio	Lower	Upper
114	100		
63	21.5	0.0	43.2
88	17.3	0.0	33.2

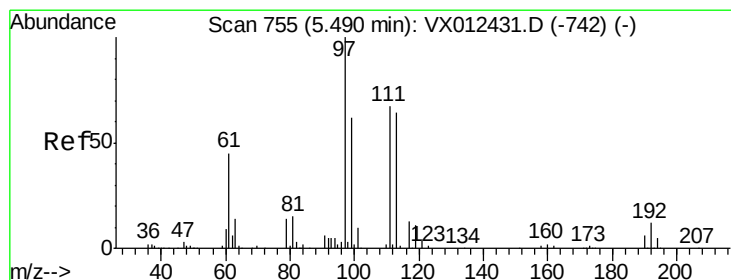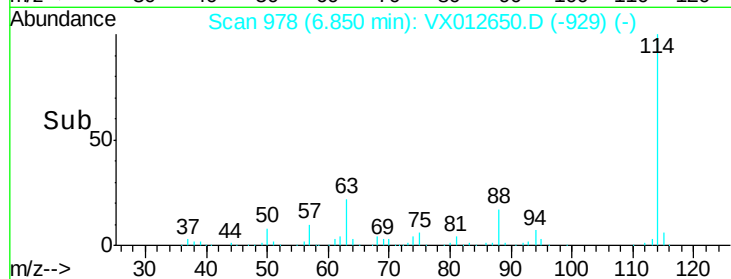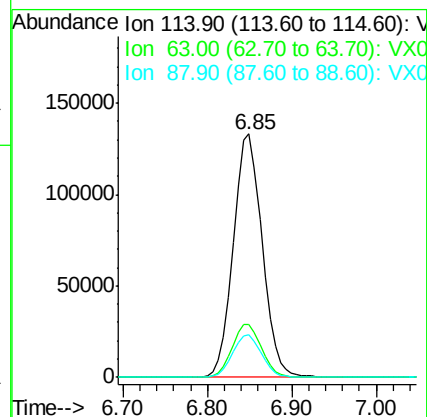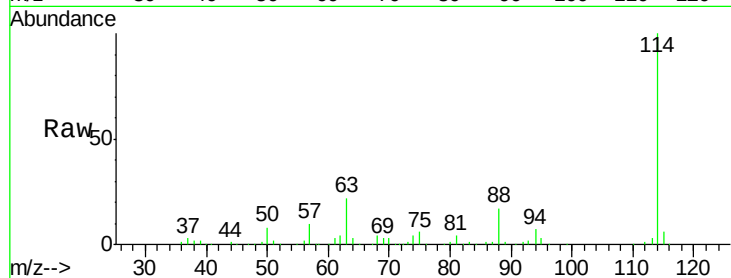

#35
 Dibromofluoromethane
 Concen: 50.666 ug/l
 RT: 5.48 min Scan# 754
 Delta R.T. -0.01 min
 Lab File: VX012650.D
 Acq: 25 Sep 2019 10:48

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.3	83.4	125.2
192	17.2	14.4	21.6

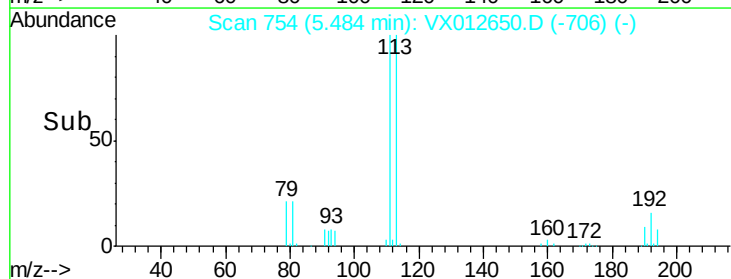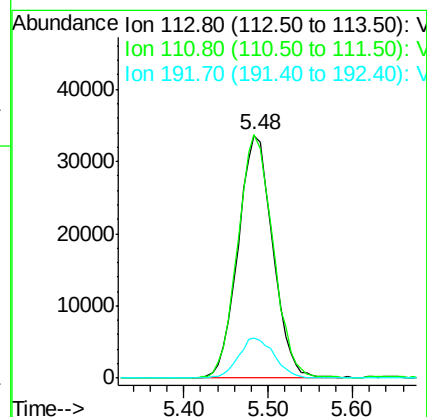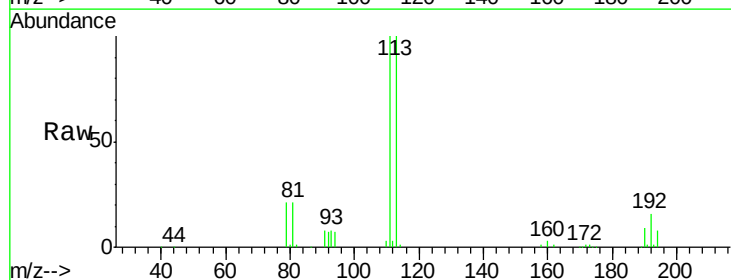

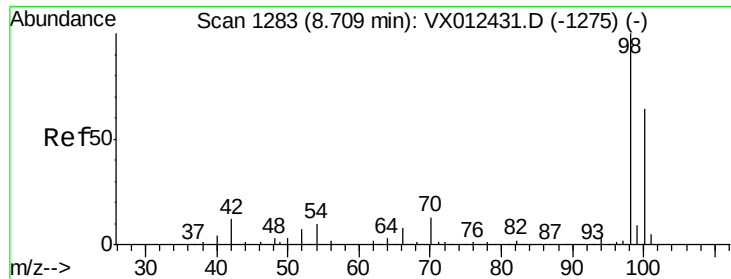

#50

Toluene-d8

Concen: 50.857 ug/l

RT: 8.71 min Scan# 1283

Delta R.T. 0.00 min

Lab File: VX012650.D

Acq: 25 Sep 2019 10:48

Instrument :

MSVOA_X

ClientSampled :


VX0925WBL01

Tot Ion: 98 Resp: 361985

Ion Ratio Lower Upper

98 100

100 66.5 53.4 80.2

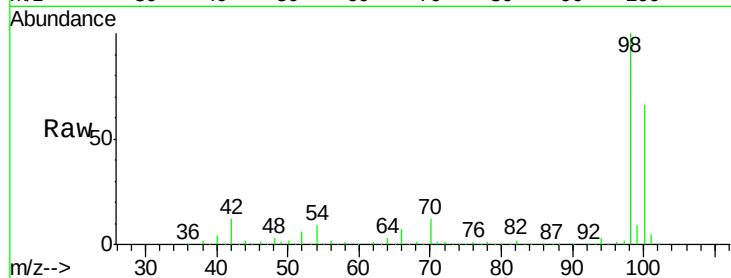

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.71

250000

200000



150000

100000

50000

0

Time--> 8.60 8.70 8.80

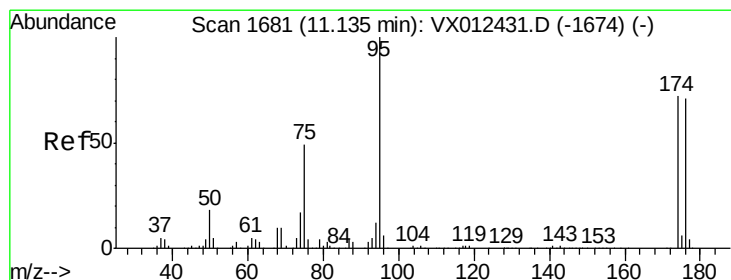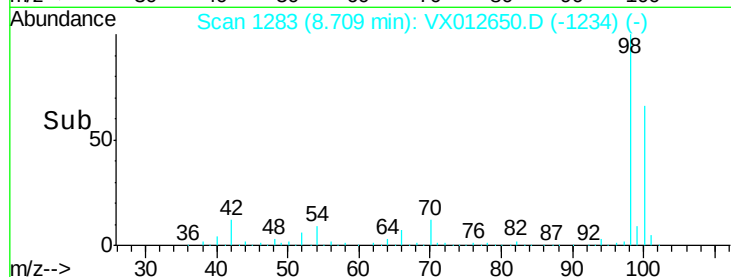

#62

4-Bromofluorobenzene

Concen: 44.000 ug/l

RT: 11.14 min Scan# 1681

Delta R.T. 0.00 min

Lab File: VX012650.D

Acq: 25 Sep 2019 10:48


Tgt Ion: 95 Resp: 123143

Ion Ratio Lower Upper

95 100

174 66.8 0.0 140.0

176 64.0 0.0 135.4

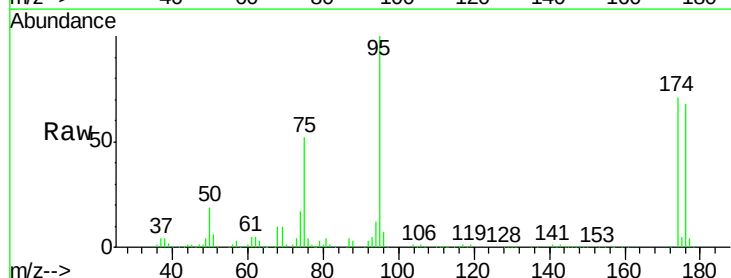

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

120000

100000

80000


60000


40000

20000

0

Time--> 11.10 11.20

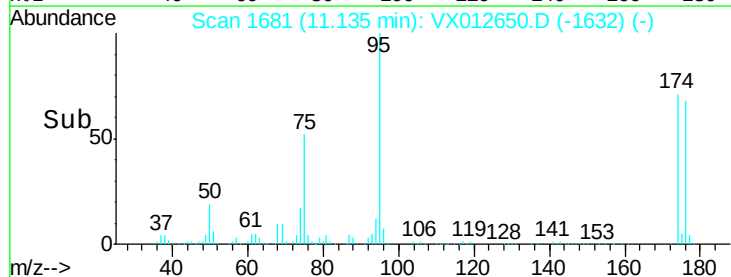


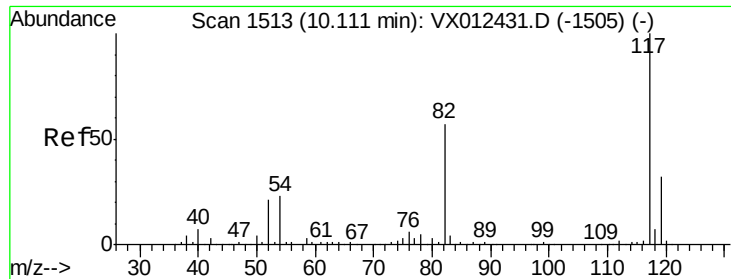




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1513
Delta R.T. 0.00 min
Lab File: VX012650.D
Acq: 25 Sep 2019 10:48

Instrument :
MSVOA_X
ClientSampleId :
VX0925WBL01

Tot Ion:117 Resp: 255462
Ion Ratio Lower Upper
117 100
82 57.9 45.9 68.9
119 32.0 25.3 37.9

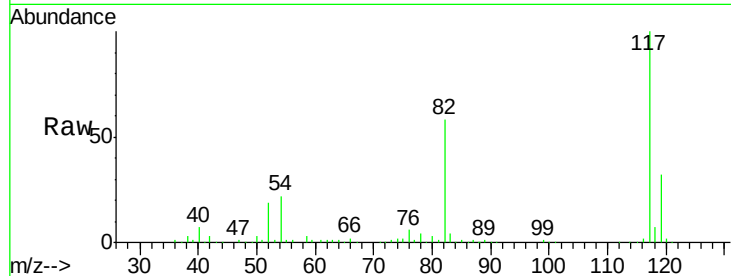


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

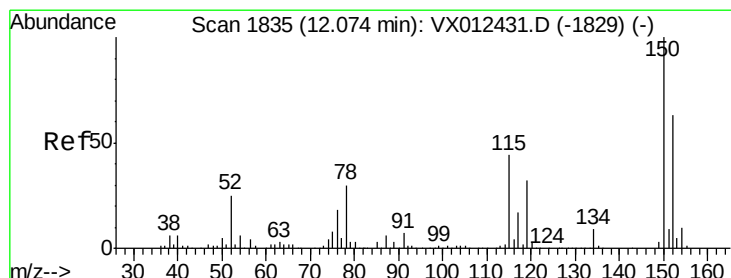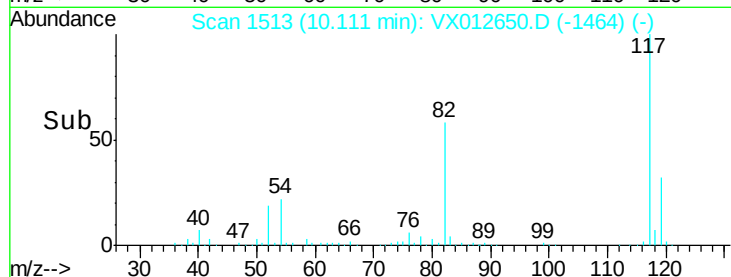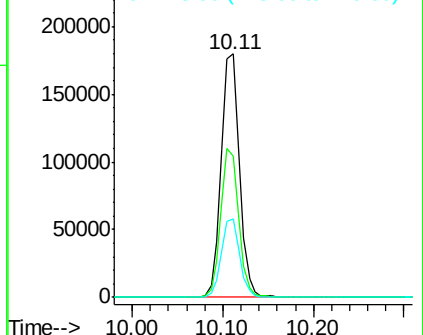

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.07 min Scan# 1835
Delta R.T. 0.00 min
Lab File: VX012650.D
Acq: 25 Sep 2019 10:48

Tgt Ion:152 Resp: 96369
Ion Ratio Lower Upper
152 100
115 64.6 44.1 132.3
150 154.2 0.0 343.8

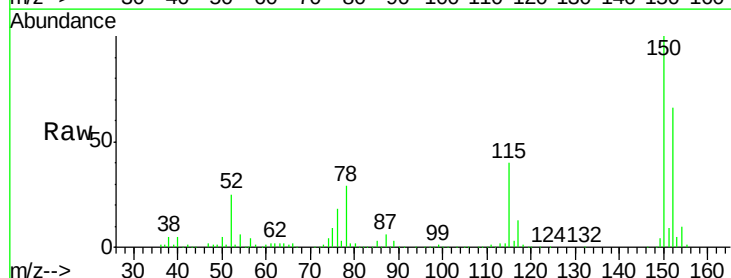

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

