


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092519\
Data File : VX012648.D
Acq On : 25 Sep 2019 09:33
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260
Last Update : Mon Sep 23 12:27:01 2019

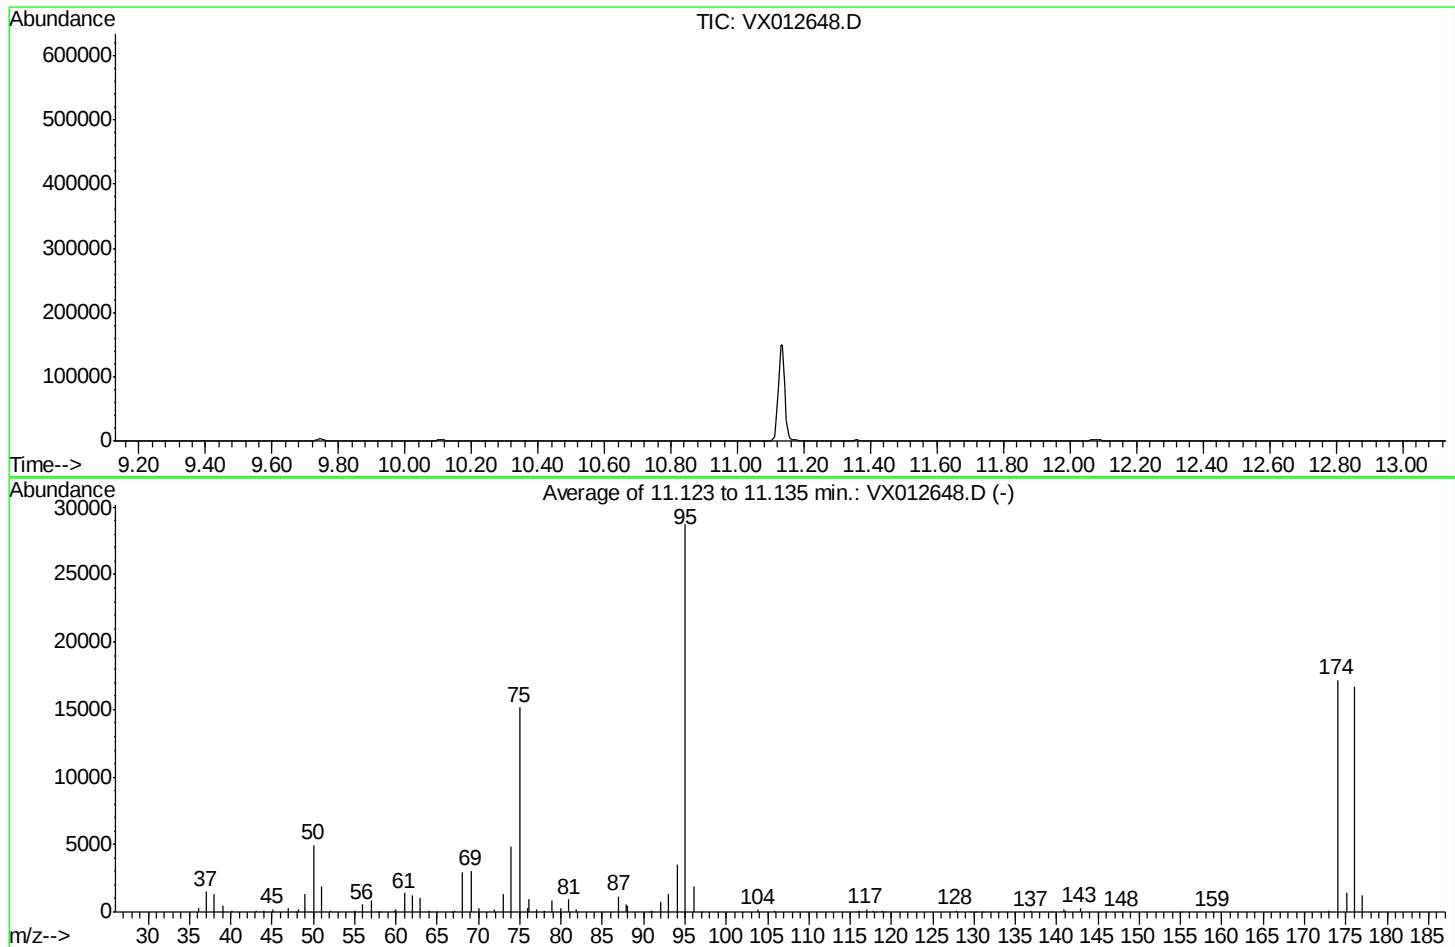

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4952	PASS
75	95	30	60	52.7	15141	PASS
95	95	100	100	100.0	28728	PASS
96	95	5	9	6.6	1899	PASS
173	174	0.00	2	0.3	59	PASS
174	95	50	100	59.9	17197	PASS
175	174	5	9	8.0	1381	PASS
176	174	95	101	96.9	16662	PASS
177	176	5	9	7.2	1198	PASS