

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092523\
 Data File : VX037891.D
 Acq On : 25 Sep 2023 12:56
 Operator : JC/MD
 Sample : 04595-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW10A-GW-440-442

Quant Time: Sep 26 06:57:31 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
 Quant Title : SW846 8260
 QLast Update : Sat Sep 16 04:55:44 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	262601	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	443545	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	426376	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	221963	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	162759	47.174	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	94.340%		
35) Dibromofluoromethane	5.391	113	142754	48.101	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.200%		
50) Toluene-d8	8.647	98	526640	47.759	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.520%		
62) 4-Bromofluorobenzene	11.079	95	206256	51.473	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	102.940%		
Target Compounds						
16) Acetone	2.374	43	4553	2.743	ug/l	Qvalue 94
25) 2-Butanone	4.587	43	3243	1.385	ug/l	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092523\
Data File : VX037891.D
Acq On : 25 Sep 2023 12:56
Operator : JC/MD
Sample : 04595-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-440-442

Quant Time: Sep 26 06:57:31 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Quant Title : SW846 8260
QLast Update : Sat Sep 16 04:55:44 2023
Response via : Initial Calibration




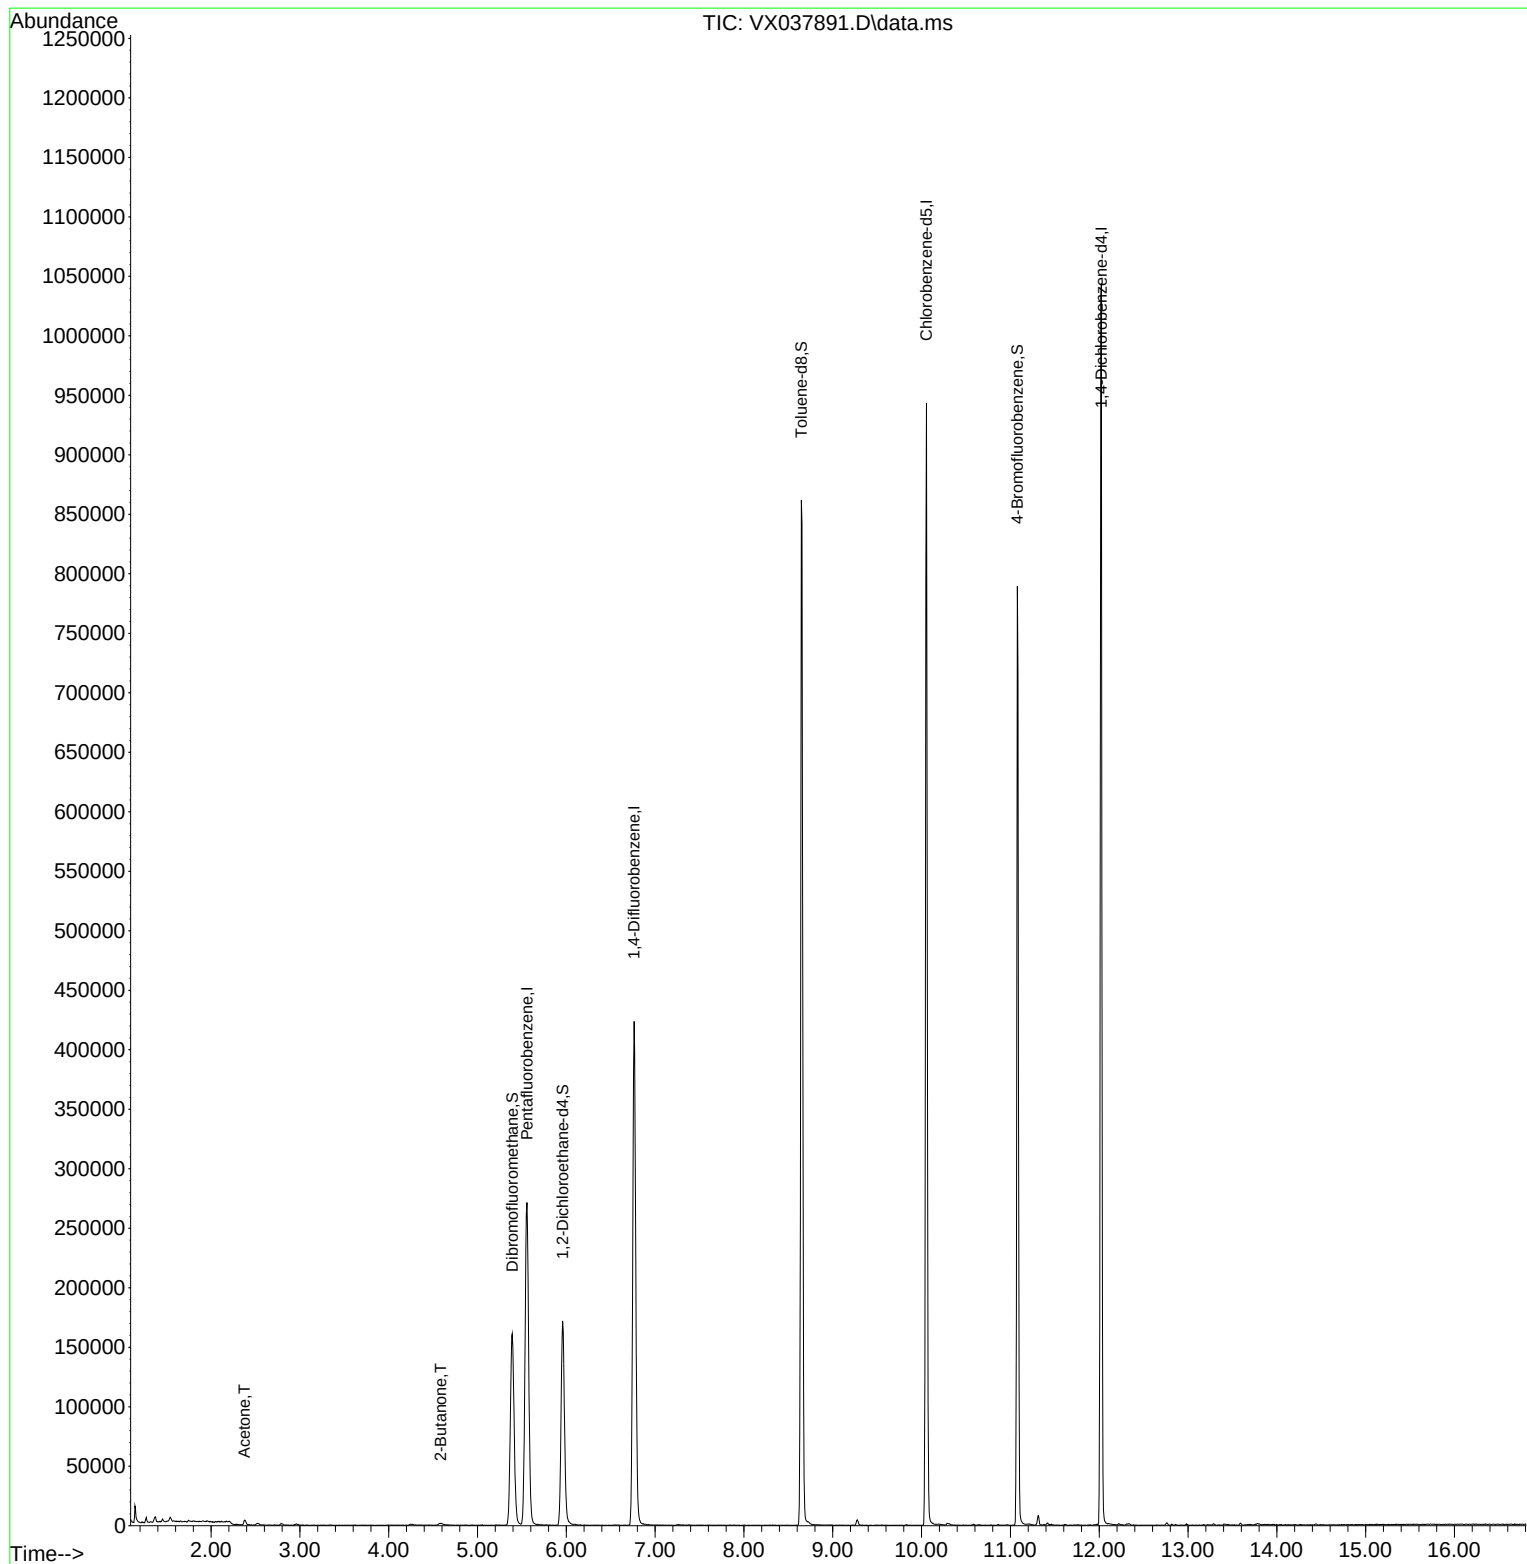


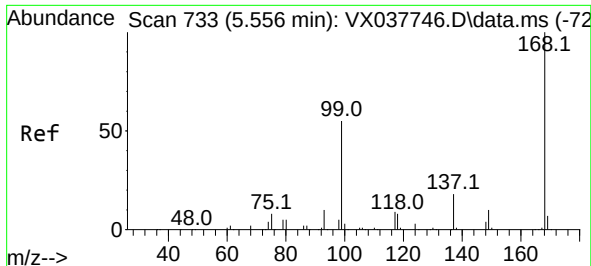

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-440-442


Tgt Ion:168 Resp: 262601
Ion Ratio Lower Upper
168 100
99 54.2 56.6 85.0#

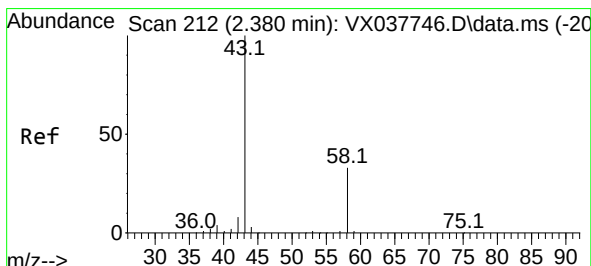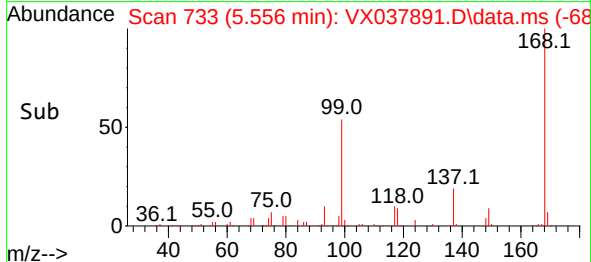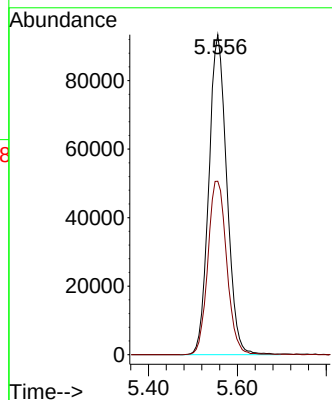

#16
Acetone
Concen: 2.743 ug/l
RT: 2.374 min Scan# 211
Delta R.T. -0.006 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56

Tgt Ion: 43 Resp: 4553
Ion Ratio Lower Upper
43 100
58 30.6 21.9 32.9


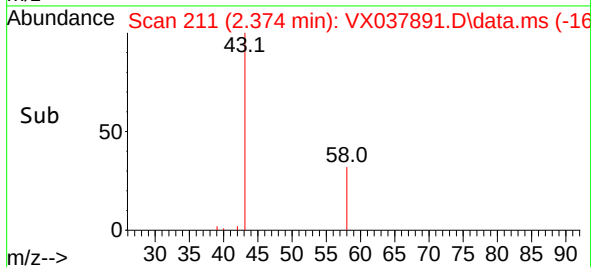
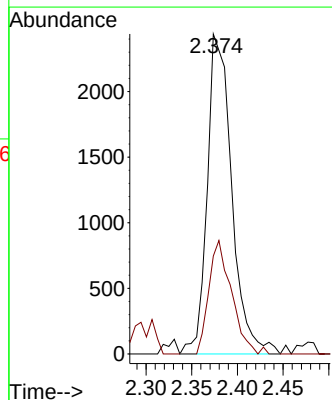
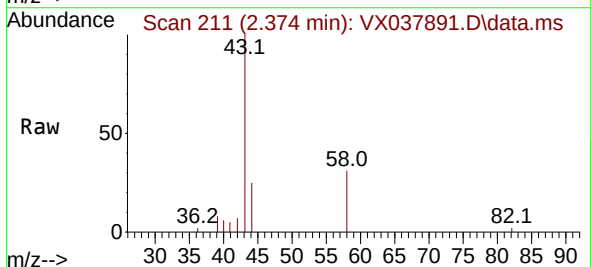




#25
2-Butanone
Concen: 1.385 ug/l
RT: 4.587 min Scan# 51
Delta R.T. 0.018 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-440-442


Tgt Ion: 43 Resp: 3243
Ion Ratio Lower Upper
43 100
72 34.0 19.4 29.2#

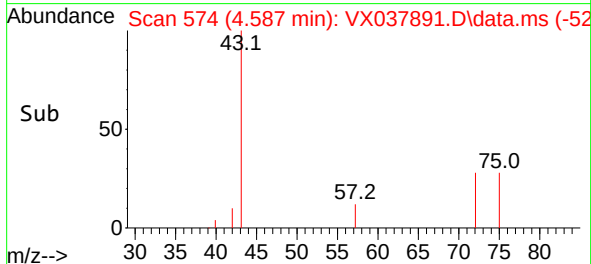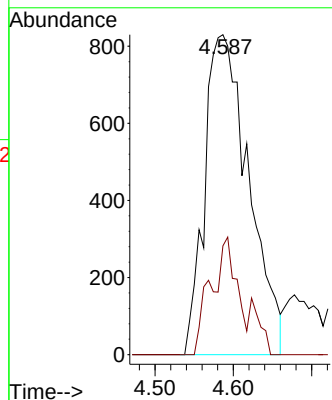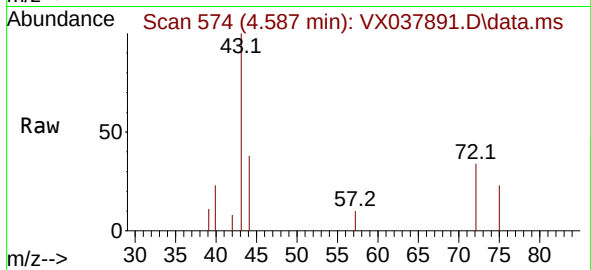

#33
1,2-Dichloroethane-d4
Concen: 47.174 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56

Tgt Ion: 65 Resp: 162759
Ion Ratio Lower Upper
65 100
67 53.5 0.0 100.2



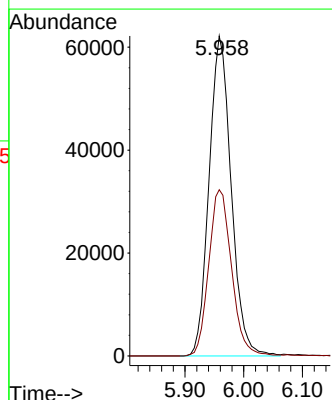
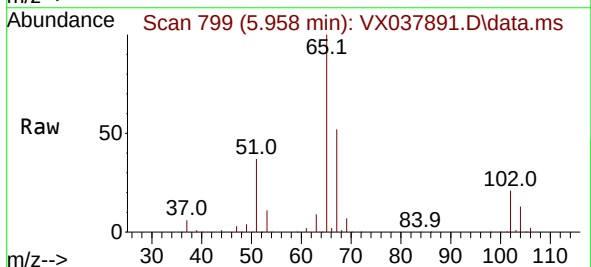


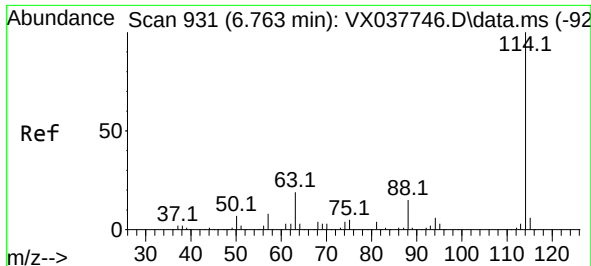

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-440-442


Tgt Ion:114 Resp: 443545
Ion Ratio Lower Upper
114 100
63 19.2 0.0 45.0
88 16.1 0.0 36.6

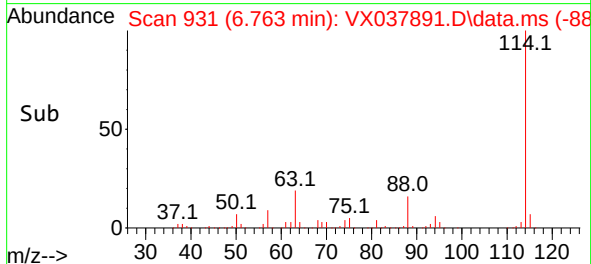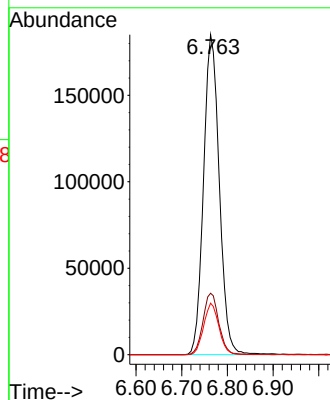

#35
Dibromofluoromethane
Concen: 48.101 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56

Tgt Ion:113 Resp: 142754
Ion Ratio Lower Upper
113 100
111 101.9 82.9 124.3
192 19.6 13.3 19.9


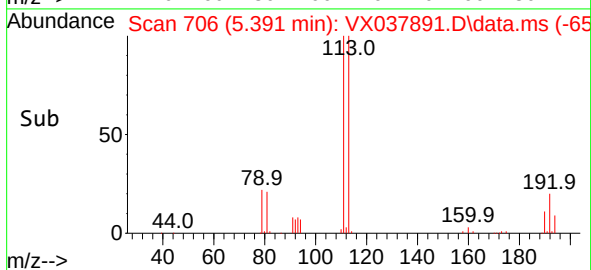
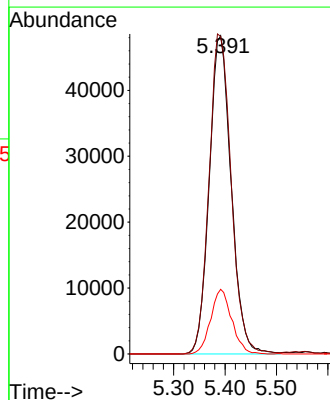
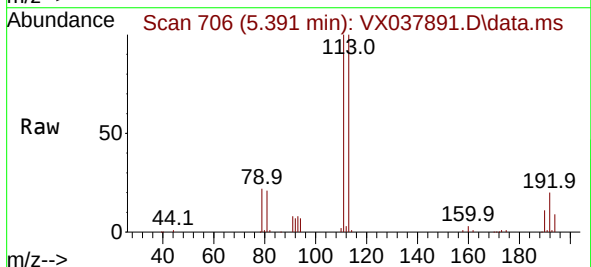


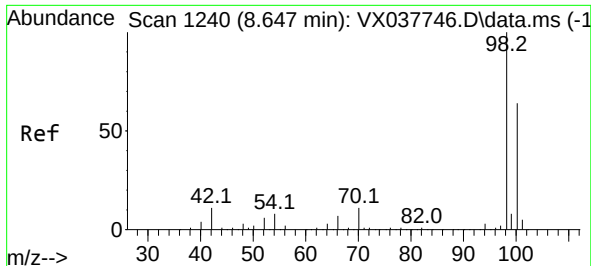

#50
Toluene-d8
Concen: 47.759 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56




Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW10A-GW-440-442


Tgt Ion: 98 Resp: 526640
Ion Ratio Lower Upper
98 100
100 64.4 53.1 79.7

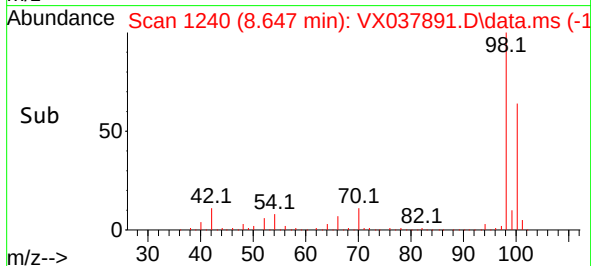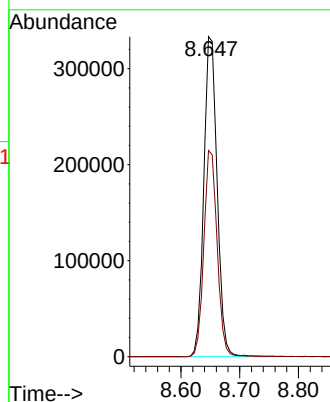

#62
4-Bromofluorobenzene
Concen: 51.473 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX037891.D
Acq: 25 Sep 2023 12:56

Tgt Ion: 95 Resp: 206256
Ion Ratio Lower Upper
95 100
174 81.8 0.0 135.6
176 78.8 0.0 131.0

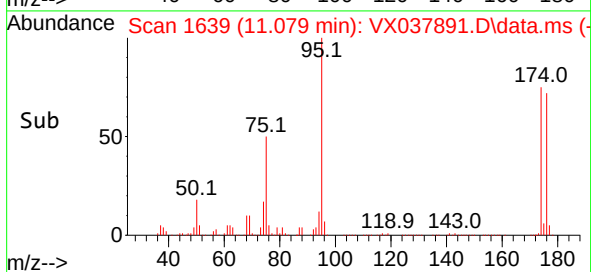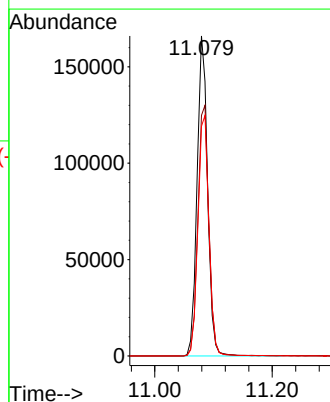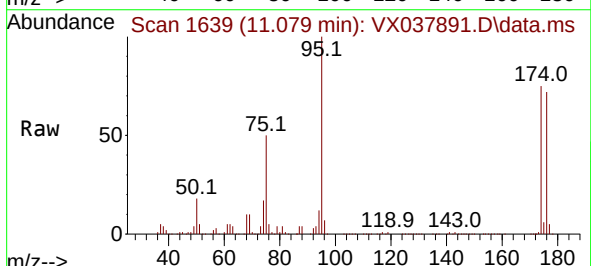



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX037891.D

Acq: 25 Sep 2023 12:56

Instrument :

MSVOA_X

ClientSampleId :

BP-VPB-RW10A-GW-440-442





Tgt Ion:117 Resp: 426376

Ion Ratio Lower Upper

117 100

82 55.6 46.2 69.4

119 32.1 25.5 38.3

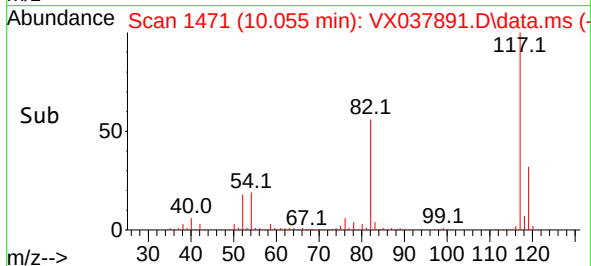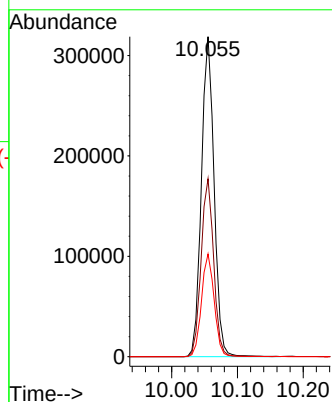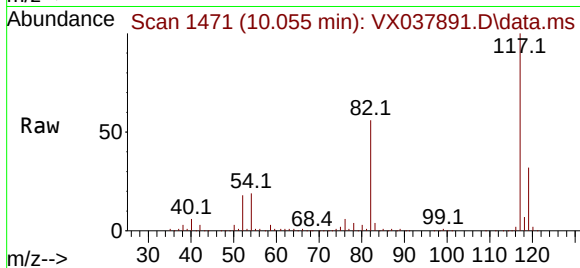

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX037891.D

Acq: 25 Sep 2023 12:56

Tgt Ion:152 Resp: 221963

Ion Ratio Lower Upper

152 100

115 60.1 43.3 129.9

150 158.0 0.0 345.0

