



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092523\
Data File : VX037881.D
Acq On : 25 Sep 2023 08:49
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091523W.M
Title : SW846 8260
Last Update : Sat Sep 16 04:55:44 2023

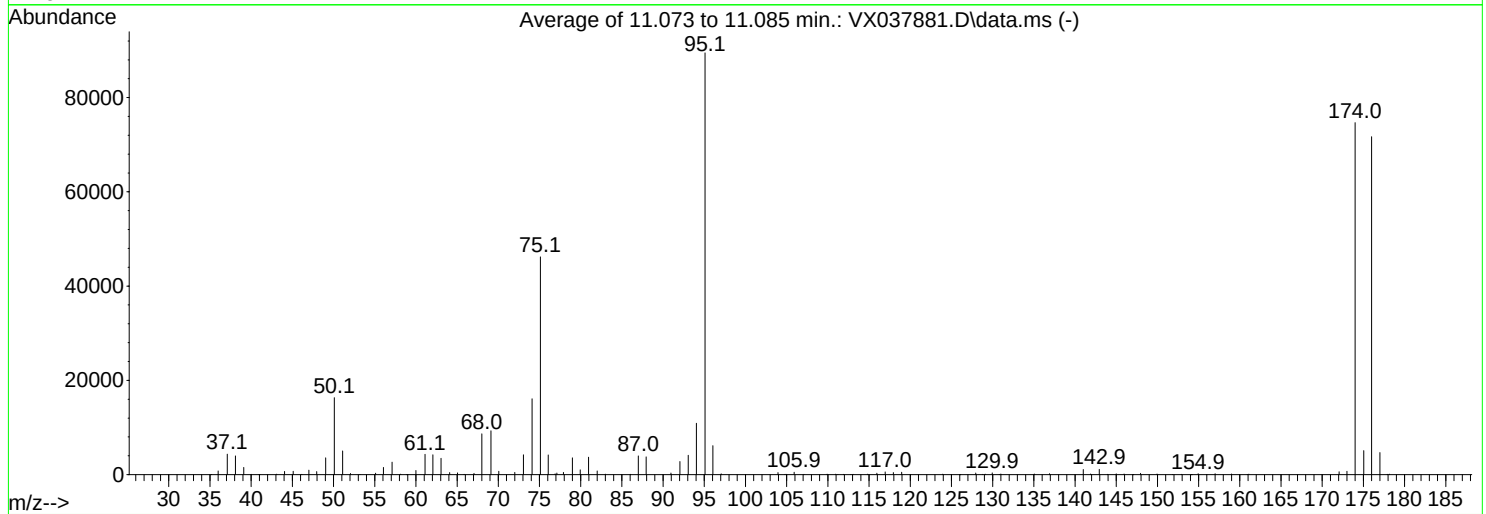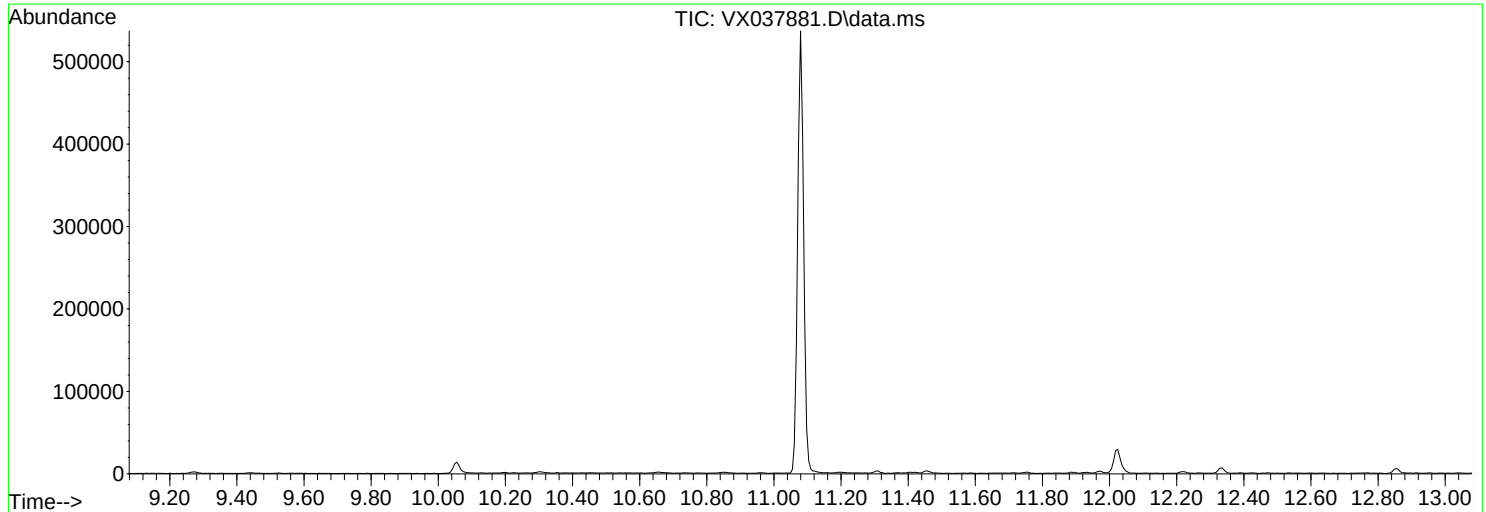

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	16312	PASS
75	95	30	60	51.6	46189	PASS
95	95	100	100	100.0	89488	PASS
96	95	5	9	6.9	6150	PASS
173	174	0.00	2	1.0	720	PASS
174	95	50	100	83.4	74672	PASS
175	174	5	9	6.8	5083	PASS
176	174	95	101	96.0	71685	PASS
177	176	5	9	6.6	4697	PASS