

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092525\
 Data File : VX047829.D
 Acq On : 26 Sep 2025 03:31
 Operator : JC/MD
 Sample : Q3156-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE10-MW01S-20250918

Quant Time: Sep 26 06:52:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.532	168	123505	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	6.739	114	257582	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	255230	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	123234	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.934	65	96094	48.881	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.760%
35) Dibromofluoromethane	5.367	113	83114	48.113	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.220%
50) Toluene-d8	8.629	98	285991	47.845	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.700%
62) 4-Bromofluorobenzene	11.061	95	117321	51.716	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.440%

Target Compounds			Qvalue			
9) 1,1,2-Trichlorotrifluo...	2.337	101	659	0.461	ug/l #	77
10) Methyl Iodide	2.465	142	1386	0.622	ug/l #	96
11) Tert butyl alcohol	2.941	59	249	1.137	ug/l #	72
13) Acrolein	2.227	56	91	0.451	ug/l #	21
15) Acrylonitrile	3.075	53	331	0.408	ug/l #	49
16) Acetone	2.374	43	1853	2.168	ug/l	97
17) Carbon Disulfide	2.520	76	1734	0.432	ug/l #	76
18) Methyl Acetate	2.703	43	391	0.206	ug/l #	87
19) Methyl tert-butyl Ether	3.105	73	5250	0.980	ug/l #	90
20) Methylene Chloride	2.782	84	544	0.301	ug/l #	88
24) 1,1-Dichloroethane	3.599	63	853	0.273	ug/l #	81
27) cis-1,2-Dichloroethene	4.471	96	620	0.320	ug/l #	1
29) Tetrahydrofuran	5.020	42	161	0.251	ug/l #	34
30) Chloroform	5.087	83	809	0.257	ug/l #	58
38) Carbon Tetrachloride	5.532	117	12900	4.703	ug/l #	18
39) Methylcyclohexane	7.354	83	617	0.215	ug/l #	33
44) Trichloroethene	7.111	130	1671	0.902	ug/l	98
52) Toluene	8.696	92	1122	0.238	ug/l	99
60) Dibromochloromethane	9.257	129	9494	4.524	ug/l #	11
64) Tetrachloroethene	9.257	164	9922	5.963	ug/l	96
76) 1,2,3-Trichloropropane	11.061	75	60443	24.225	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.061	75	60443	61.776	ug/l #	8
85) sec-Butylbenzene	11.872	105	2247	0.240	ug/l	94
86) p-Isopropyltoluene	11.994	119	2060	0.260	ug/l #	82
87) 1,3-Dichlorobenzene	11.951	146	919	0.214	ug/l	99
88) 1,4-Dichlorobenzene	11.951	146	919	0.209	ug/l	98
89) n-Butylbenzene	12.317	91	3029	0.413	ug/l	95
90) Hexachloroethane	12.518	117	326	0.234	ug/l	91
93) 1,2,4-Trichlorobenzene	13.567	180	1541	0.581	ug/l	98
94) Hexachlorobutadiene	13.707	225	1261	1.399	ug/l	93
95) Naphthalene	13.762	128	3030	0.375	ug/l	95
96) 1,2,3-Trichlorobenzene	13.945	180	1192	0.483	ug/l	91





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.532 min Scan# 71
Delta R.T. -0.012 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:168 Resp: 123505
Ion Ratio Lower Upper
168 100
99 68.3 48.8 73.2

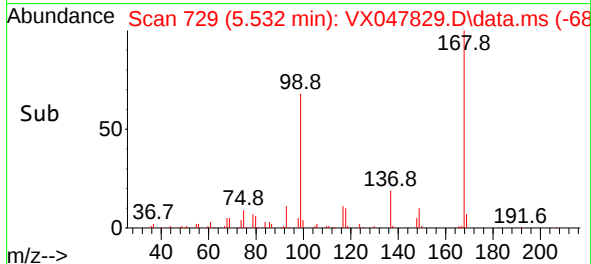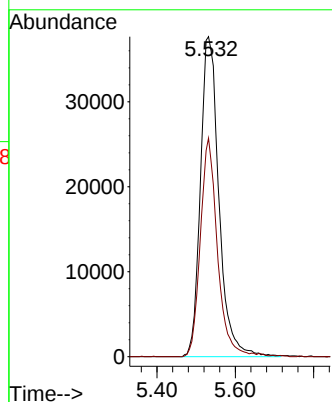

#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.461 ug/l
RT: 2.337 min Scan# 205
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31


Tgt Ion:101 Resp: 659
Ion Ratio Lower Upper
101 100
85 18.8 35.5 53.3#
151 85.1 59.4 89.0








#10
Methyl Iodide
Concen: 0.622 ug/l
RT: 2.465 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918







Tgt Ion:142 Resp: 1386
Ion Ratio Lower Upper
142 100
127 46.4 37.2 55.8
141 7.8 11.4 17.0#

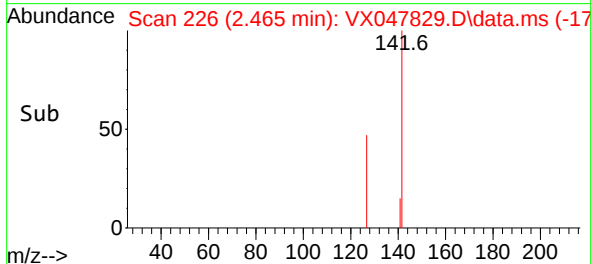

#11
Tert butyl alcohol
Concen: 1.137 ug/l
RT: 2.941 min Scan# 304
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 59 Resp: 249
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#









#13
Acrolein
Concen: 0.451 ug/l
RT: 2.227 min Scan# 11
Delta R.T. -0.012 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 56 Resp: 91
Ion Ratio Lower Upper
56 100
55 137.4 57.2 85.8#

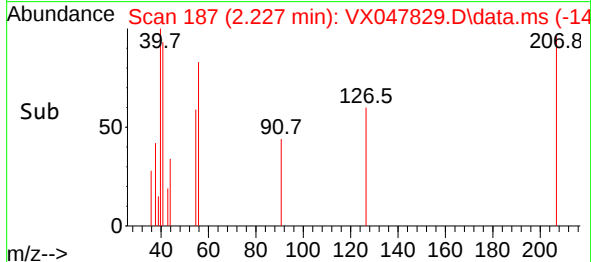

#15
Acrylonitrile
Concen: 0.408 ug/l
RT: 3.075 min Scan# 326
Delta R.T. 0.012 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 53 Resp: 331
Ion Ratio Lower Upper
53 100
52 18.4 66.4 99.6#
51 33.5 29.5 44.3









#16
Acetone
Concen: 2.168 ug/l
RT: 2.374 min Scan# 211
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 43 Resp: 1853
Ion Ratio Lower Upper
43 100
58 30.6 23.4 35.0

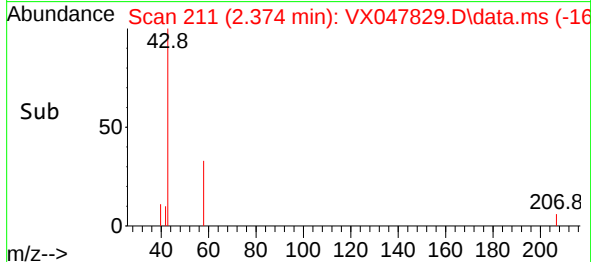

#17
Carbon Disulfide
Concen: 0.432 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 76 Resp: 1734
Ion Ratio Lower Upper
76 100
78 0.0 6.8 10.2#





#18

Methyl Acetate

Concen: 0.206 ug/l

RT: 2.703 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31

Instrument :

MSVOA_X

ClientSampleId :





RE10-MW01S-20250918

Tgt Ion: 43 Resp: 391

Ion Ratio Lower Upper

43 100

74 15.9 17.4 26.2#

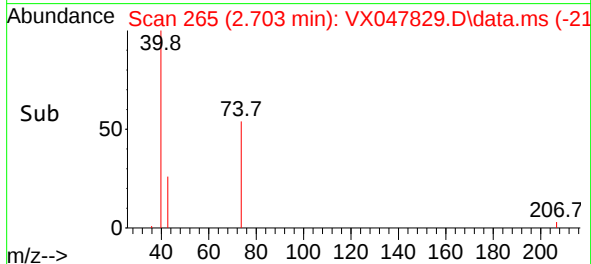

#19

Methyl tert-butyl Ether

Concen: 0.980 ug/l

RT: 3.105 min Scan# 331

Delta R.T. -0.006 min

Lab File: VX047829.D




Acq: 26 Sep 2025 03:31


Tgt Ion: 73 Resp: 5250

Ion Ratio Lower Upper

73 100

57 16.9 17.4 26.2#







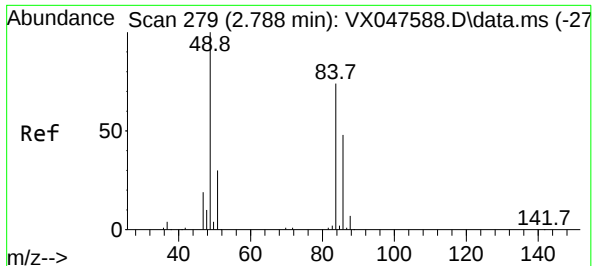

#20
Methylene Chloride
Concen: 0.301 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:	84	Resp:	544
Ion	Ratio	Lower	Upper
84	100		
49	124.2	108.6	162.8
51	52.0	32.6	48.8#
86	53.8	52.0	78.0

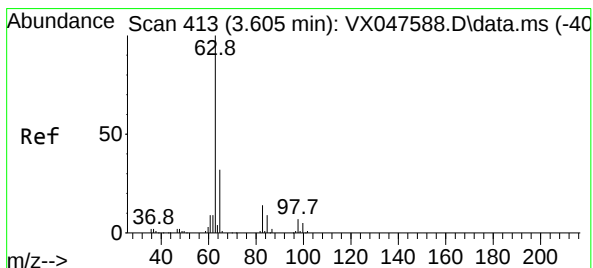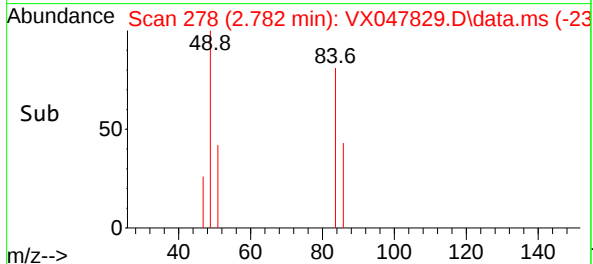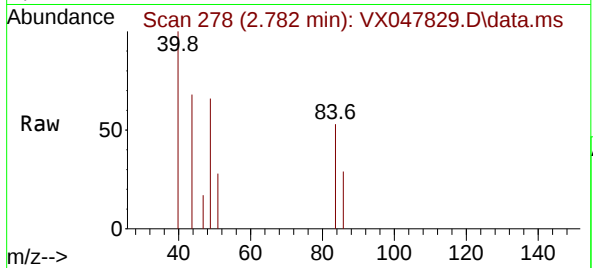

#24
1,1-Dichloroethane
Concen: 0.273 ug/l
RT: 3.599 min Scan# 412
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion:	63	Resp:	853
Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.8	11.2#
100	0.0	2.3	6.9#

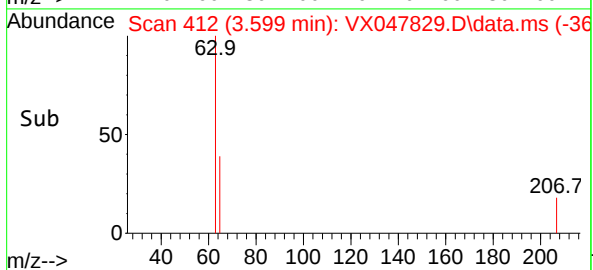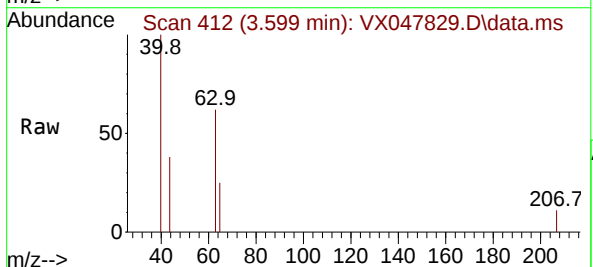



#27

cis-1,2-Dichloroethene

Concen: 0.320 ug/l

RT: 4.471 min Scan# 51

Delta R.T. -0.012 min

Lab File: VX047829.D


Acq: 26 Sep 2025 03:31

Instrument :




MSVOA_X

ClientSampleId :

RE10-MW01S-20250918

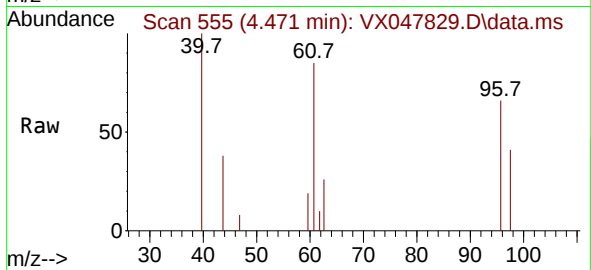

Tgt Ion:	96	Resp:	620
Ion	Ratio	Lower	Upper
96	100		
61	321.8	0.0	303.2#
98	133.9	0.0	127.8#

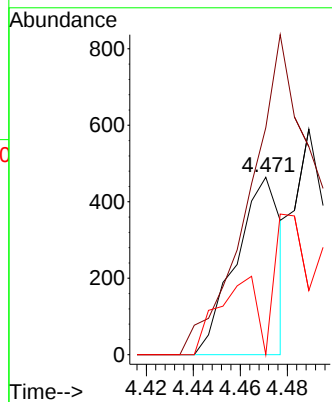

#29

Tetrahydrofuran

Concen: 0.251 ug/l




RT: 5.020 min Scan# 645


Delta R.T. 0.031 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31

Tgt Ion:	42	Resp:	161
Ion	Ratio	Lower	Upper
42	100		
72	0.0	34.2	51.2#
71	0.0	31.9	47.9#

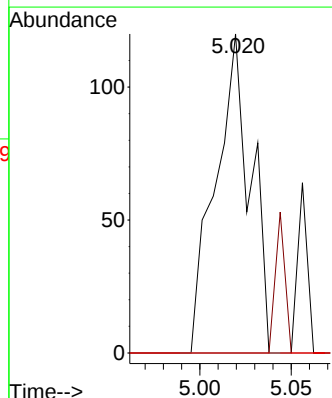



#30

Chloroform

Concen: 0.257 ug/l

RT: 5.087 min Scan# 61

Delta R.T. 0.006 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31

Instrument :

MSVOA_X

ClientSampleId :





RE10-MW01S-20250918

Tgt Ion: 83 Resp: 809

Ion Ratio Lower Upper

83 100

85 31.6 51.8 77.6#

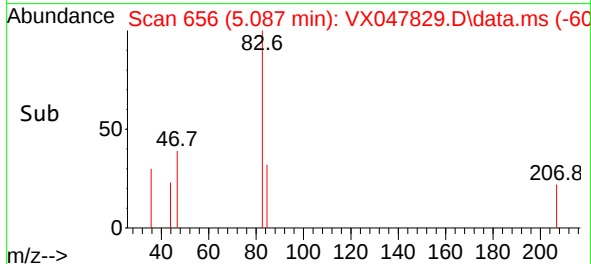

#33

1,2-Dichloroethane-d4

Concen: 48.881 ug/l

RT: 5.934 min Scan# 795

Delta R.T. -0.006 min

Lab File: VX047829.D




Acq: 26 Sep 2025 03:31


Tgt Ion: 65 Resp: 96094

Ion Ratio Lower Upper

65 100

67 52.4 0.0 103.0









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.739 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:114 Resp: 257582
Ion Ratio Lower Upper
114 100
63 22.0 0.0 44.0
88 16.7 0.0 34.2

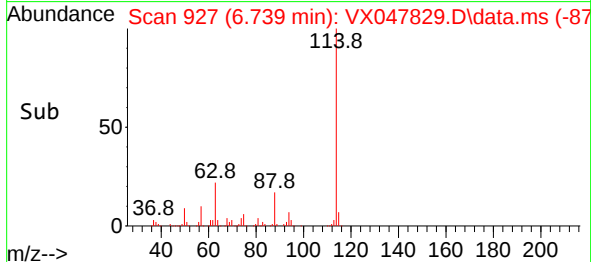

#35
Dibromofluoromethane
Concen: 48.113 ug/l
RT: 5.367 min Scan# 702
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion:113 Resp: 83114
Ion Ratio Lower Upper
113 100
111 104.0 80.9 121.3
192 18.4 14.2 21.4









#38
Carbon Tetrachloride
Concen: 4.703 ug/l
RT: 5.532 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 117 Resp: 12900
Ion Ratio Lower Upper
117 100
119 5.0 73.4 110.2#
121 0.0 23.8 35.6#

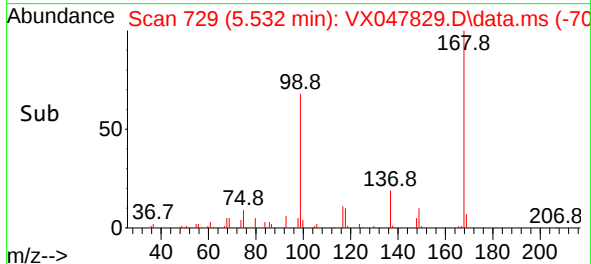

#39
Methylcyclohexane
Concen: 0.215 ug/l
RT: 7.354 min Scan# 1028
Delta R.T. -0.012 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 83 Resp: 617
Ion Ratio Lower Upper
83 100
55 0.0 66.4 99.6#
98 32.0 38.1 57.1#


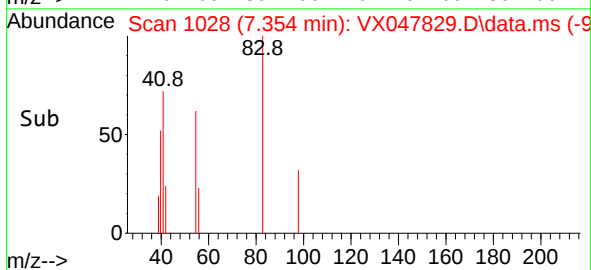






#44
Trichloroethene
Concen: 0.902 ug/l
RT: 7.111 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:130 Resp: 1671
Ion Ratio Lower Upper
130 100
95 108.0 0.0 210.8

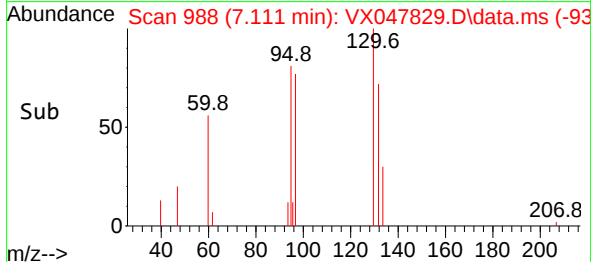

#50
Toluene-d8
Concen: 47.845 ug/l
RT: 8.629 min Scan# 1237
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 98 Resp: 285991
Ion Ratio Lower Upper
98 100
100 66.8 53.0 79.4









#52
Toluene
Concen: 0.238 ug/l
RT: 8.696 min Scan# 1122
Delta R.T. -0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 92 Resp: 1122
Ion Ratio Lower Upper
92 100
91 169.5 137.1 205.7

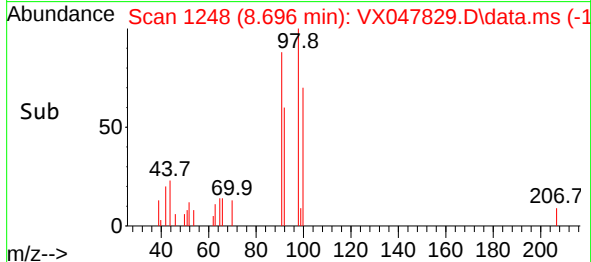

#60
Dibromochloromethane
Concen: 4.524 ug/l
RT: 9.257 min Scan# 1340
Delta R.T. -0.250 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 129 Resp: 9494
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#







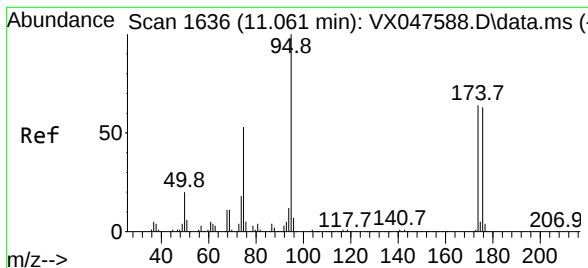

#62
4-Bromofluorobenzene
Concen: 51.716 ug/l
RT: 11.061 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 95 Resp: 117321
Ion Ratio Lower Upper
95 100
174 73.2 0.0 141.6
176 70.7 0.0 138.4

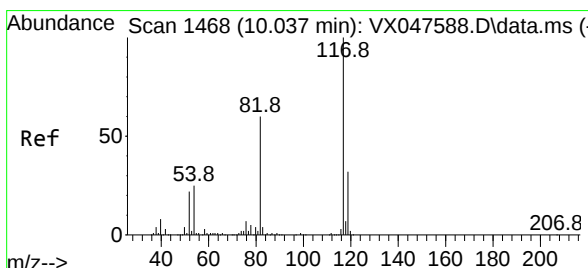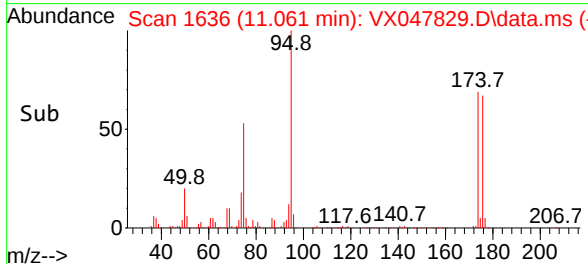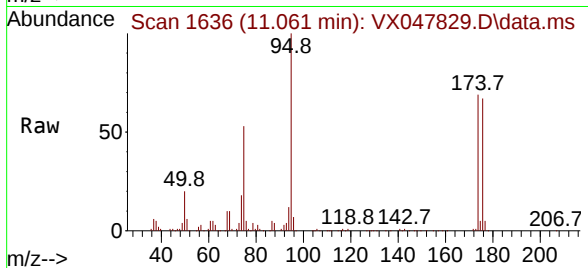

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 117 Resp: 255230
Ion Ratio Lower Upper
117 100
82 57.4 47.8 71.6
119 32.5 25.2 37.8


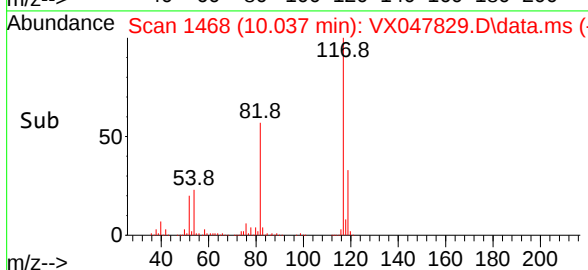

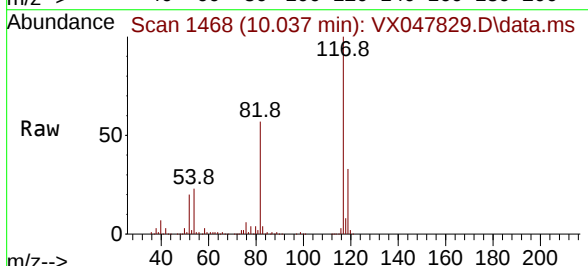




#64
Tetrachloroethene
Concen: 5.963 ug/l
RT: 9.257 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:164	Resp:	9922
Ion	Ratio	Lower Upper
164	100	
166	130.5	100.2 150.2
129	100.2	81.8 122.6
131	92.5	78.6 118.0

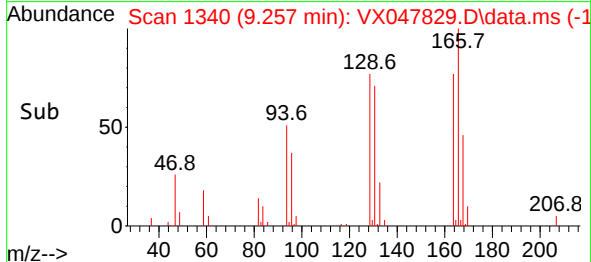

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion:152	Resp:	123234
Ion	Ratio	Lower Upper
152	100	
115	62.0	44.9 134.5
150	157.4	0.0 352.0









#76
1,2,3-Trichloropropane
Concen: 24.225 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.158 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion: 75 Resp: 60443
Ion Ratio Lower Upper
75 100
77 1.7 18.8 56.4#

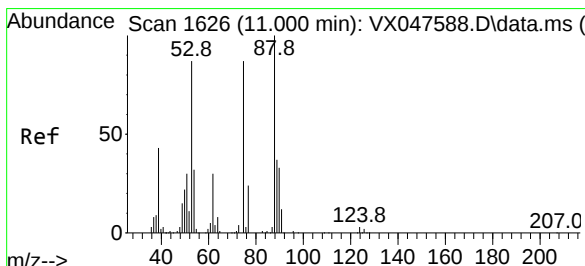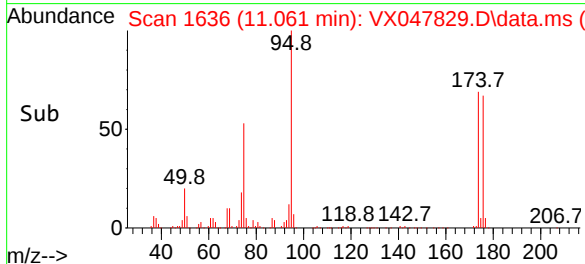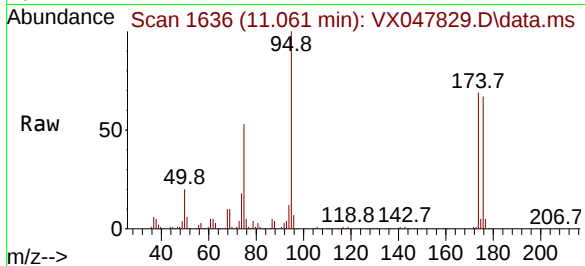

#81
trans-1,4-Dichloro-2-butene
Concen: 61.776 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion: 75 Resp: 60443
Ion Ratio Lower Upper
75 100
53 0.0 83.4 125.2#
89 0.0 36.3 54.5#


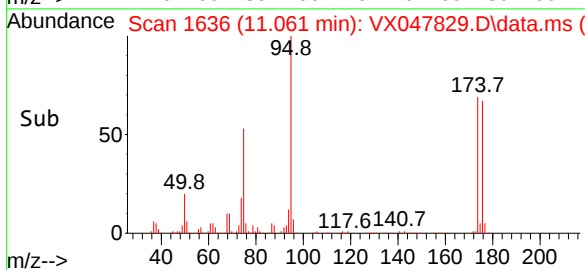

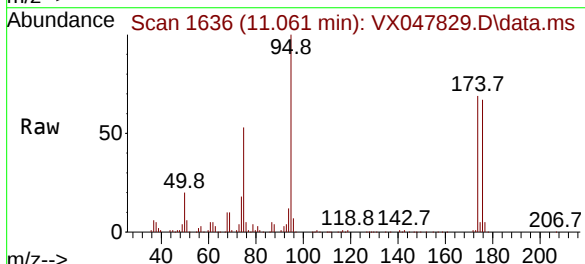




#85
 sec-Butylbenzene
 Concen: 0.240 ug/l
 RT: 11.872 min Scan# 1769
 Delta R.T. 0.000 min
 Lab File: VX047829.D
 Acq: 26 Sep 2025 03:31




Instrument :
 MSVOA_X
 ClientSampleId :
 RE10-MW01S-20250918


Tgt Ion:105 Resp: 2247
 Ion Ratio Lower Upper
 105 100
 134 17.1 9.8 29.5

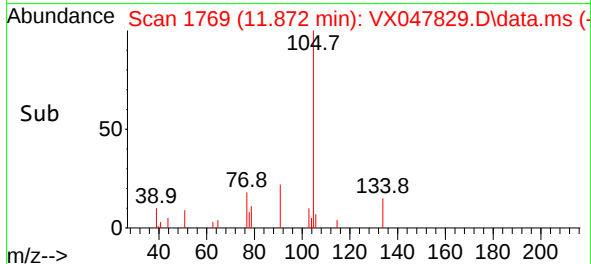

#86
 p-Isopropyltoluene
 Concen: 0.260 ug/l
 RT: 11.994 min Scan# 1789
 Delta R.T. 0.000 min
 Lab File: VX047829.D
 Acq: 26 Sep 2025 03:31

Tgt Ion:119 Resp: 2060
 Ion Ratio Lower Upper
 119 100
 134 24.6 12.6 37.8
 91 42.2 12.6 37.6#


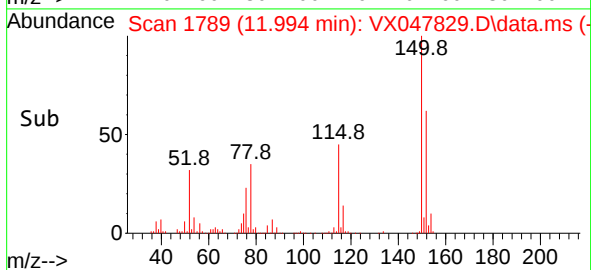






#87
1,3-Dichlorobenzene
Concen: 0.214 ug/l
RT: 11.951 min Scan# 1782
Delta R.T. 0.000 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31




Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918


Tgt Ion:	146	Resp:	919
Ion	Ratio	Lower	Upper
146	100		
111	42.1	21.5	64.5
148	65.1	32.0	96.0

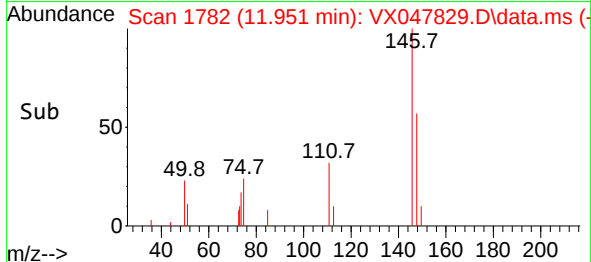

#88
1,4-Dichlorobenzene
Concen: 0.209 ug/l
RT: 11.951 min Scan# 1782
Delta R.T. -0.073 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion:	146	Resp:	919
Ion	Ratio	Lower	Upper
146	100		
111	42.1	20.8	62.4
148	65.1	31.7	95.1





#89

n-Butylbenzene

Concen: 0.413 ug/l

RT: 12.317 min Scan# 1841

Delta R.T. 0.006 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31

Instrument :

MSVOA_X

ClientSampleId :

RE10-MW01S-20250918





Tgt Ion: 91 Resp: 3029

Ion Ratio Lower Upper

91 100

92 51.3 27.6 82.7

134 22.3 12.6 37.8

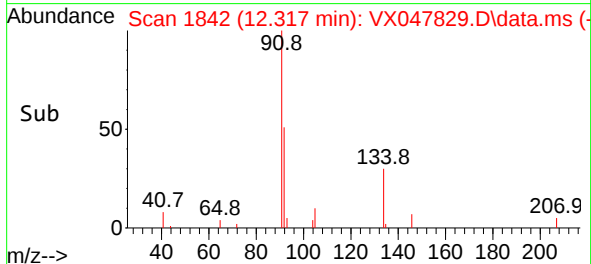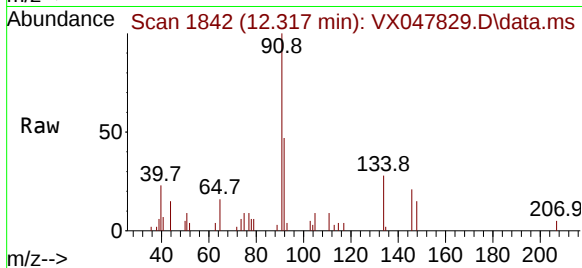

#90

Hexachloroethane

Concen: 0.234 ug/l

RT: 12.518 min Scan# 1875

Delta R.T. 0.000 min

Lab File: VX047829.D




Acq: 26 Sep 2025 03:31


Tgt Ion: 117 Resp: 326

Ion Ratio Lower Upper

117 100

201 61.0 34.2 102.5

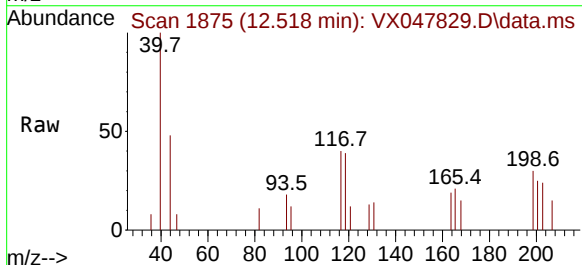



#93

1,2,4-Trichlorobenzene

Concen: 0.581 ug/l

RT: 13.567 min Scan# 2047

Delta R.T. 0.000 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31

Instrument :

MSVOA_X

ClientSampleId :

RE10-MW01S-20250918





Tgt Ion:180 Resp: 1541

Ion Ratio Lower Upper

180 100

182 93.8 46.6 139.8

145 30.2 16.4 49.1

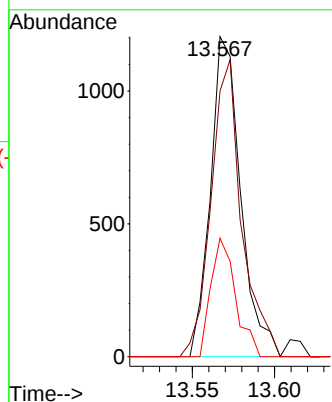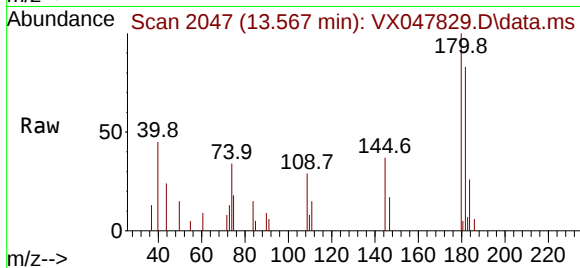

#94

Hexachlorobutadiene

Concen: 1.399 ug/l

RT: 13.707 min Scan# 2070

Delta R.T. 0.000 min

Lab File: VX047829.D

Acq: 26 Sep 2025 03:31




Tgt Ion:225 Resp: 1261


Ion Ratio Lower Upper

225 100

223 73.8 31.7 95.1

227 63.2 32.0 96.0


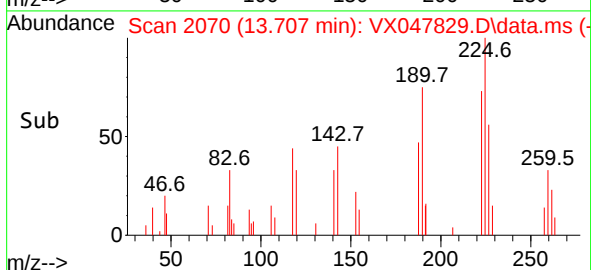

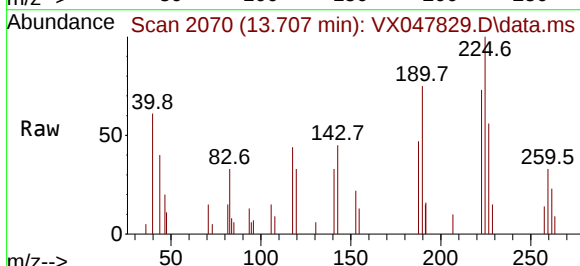




#95
Naphthalene
Concen: 0.375 ug/l
RT: 13.762 min Scan# 2078
Delta R.T. 0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Instrument :
MSVOA_X
ClientSampleId :
RE10-MW01S-20250918

Tgt Ion:	128	Resp:	3030
Ion Ratio	Lower	Upper	
128	100		
127	10.7	10.2	15.2
129	9.5	8.8	13.2

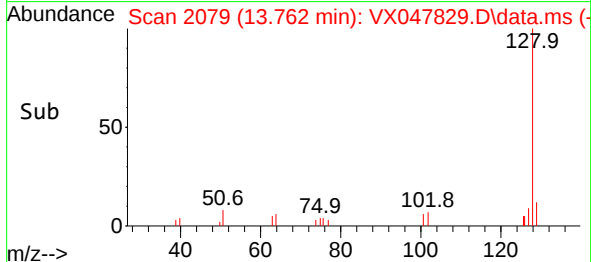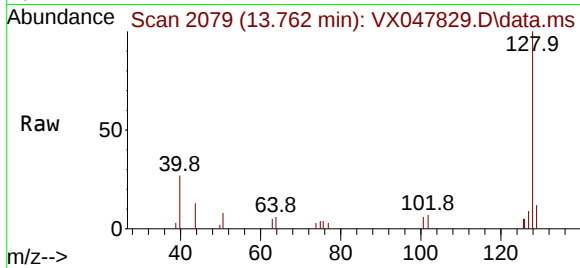

#96
1,2,3-Trichlorobenzene
Concen: 0.483 ug/l
RT: 13.945 min Scan# 2109
Delta R.T. 0.006 min
Lab File: VX047829.D
Acq: 26 Sep 2025 03:31

Tgt Ion:	180	Resp:	1192
Ion Ratio	Lower	Upper	
180	100		
182	103.4	47.6	142.8
145	41.0	17.9	53.7

