

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092618\
 Data File : VX004727.D
 Acq On : 26 Sep 2018 14:16
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 ICVVX092618

Quant Time: Sep 27 01:10:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	306506	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	394137	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	363426	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	223846	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	188466	43.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	86.08%	
35) Dibromofluoromethane	5.50	113	166608	49.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.76%	
50) Toluene-d8	8.71	98	557533	50.21	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.42%	
62) 4-Bromofluorobenzene	11.14	95	208629	52.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.30%	

Target Compounds

						Qvalue
2) Dichlorodifluoromethane	1.20	85	221684	53.046	ug/l	99
3) Chloromethane	1.32	50	259009	51.084	ug/l	99
4) Vinyl Chloride	1.40	62	239614	50.387	ug/l	97
5) Bromomethane	1.64	94	150020	53.200	ug/l	97
6) Chloroethane	1.71	64	141015	54.628	ug/l	98
7) Trichlorofluoromethane	1.92	101	314007	53.337	ug/l	97
8) Diethyl Ether	2.19	74	122820	48.022	ug/l	94
9) 1,1,2-Trichlorotrifluoroet	2.38	101	174826	52.132	ug/l	97
10) Methyl Iodide	2.51	142	219572	48.930	ug/l	99
11) Tert butyl alcohol	3.08	59	298160	243.544	ug/l	99
12) 1,1-Dichloroethene	2.37	96	168416	50.711	ug/l	97
13) Acrolein	2.29	56	212619	244.095	ug/l	98
14) Allyl chloride	2.73	41	379739	52.404	ug/l	93
15) Acrylonitrile	3.15	53	629028	233.401	ug/l	95
16) Acetone	2.45	43	663990	259.755	ug/l	91
17) Carbon Disulfide	2.56	76	502528	50.356	ug/l	100
18) Methyl Acetate	2.78	43	300049	46.329	ug/l	95
19) Methyl tert-butyl Ether	3.20	73	592292	51.703	ug/l	93
20) Methylene Chloride	2.85	84	179966	48.395	ug/l	93
21) trans-1,2-Dichloroethene	3.16	96	170291	46.841	ug/l	88
22) Diisopropyl ether	3.87	45	641986	52.612	ug/l	96
23) Vinyl Acetate	3.82	43	2906455	260.216	ug/l	97
24) 1,1-Dichloroethane	3.69	63	334308	45.929	ug/l	99
25) 2-Butanone	4.70	43	990160	262.785	ug/l #	88
26) 2,2-Dichloropropane	4.58	77	277195	54.688	ug/l	97
27) cis-1,2-Dichloroethene	4.60	96	205506	50.600	ug/l	99
28) Bromochloromethane	5.01	49	164534	48.002	ug/l	90
29) Tetrahydrofuran	5.15	42	595191	254.148	ug/l	92
30) Chloroform	5.21	83	315385	45.847	ug/l	97
31) Cyclohexane	5.57	56	302783	54.350	ug/l	86
32) 1,1,1-Trichloroethane	5.49	97	270473	48.144	ug/l	100
36) 1,1-Dichloropropene	5.79	75	246609	54.111	ug/l	99
37) Ethyl Acetate	4.87	43	326125	53.908	ug/l	98
38) Carbon Tetrachloride	5.78	117	237565	49.588	ug/l	96

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092618\
 Data File : VX004727.D
 Acq On : 26 Sep 2018 14:16
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618

Quant Time: Sep 27 01:10:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
39) Methylcyclohexane	7.46	83	280046	60.177	ug/l	# 84
40) Benzene	6.14	78	754845	52.904	ug/l	97
41) Methacrylonitrile	5.06	41	180791	53.887	ug/l	96
42) 1,2-Dichloroethane	6.20	62	255608	50.676	ug/l	97
43) Isopropyl Acetate	6.46	43	458566	52.517	ug/l	98
44) Trichloroethene	7.21	130	177551	50.620	ug/l	92
45) 1,2-Dichloropropane	7.52	63	179312	51.247	ug/l	98
46) Dibromomethane	7.66	93	113329	51.537	ug/l	99
47) Bromodichloromethane	7.90	83	216632	52.618	ug/l	100
48) Methyl methacrylate	7.78	41	226631	57.184	ug/l	95
49) 1,4-Dioxane	7.76	88	106468	1081.318	ug/l	96
51) 4-Methyl-2-Pentanone	8.65	43	1523520	277.110	ug/l	96
52) Toluene	8.79	92	414999	52.933	ug/l	96
53) t-1,3-Dichloropropene	9.04	75	251702	54.101	ug/l	99
54) cis-1,3-Dichloropropene	8.44	75	272299	55.878	ug/l	99
55) 1,1,2-Trichloroethane	9.22	97	170783	49.730	ug/l	97
56) Ethyl methacrylate	9.18	69	272184	48.908	ug/l	94
57) 1,3-Dichloropropane	9.37	76	290208	50.774	ug/l	100
58) 2-Chloroethyl Vinyl ether	8.32	63	761232	256.841	ug/l	95
59) 2-Hexanone	9.50	43	1225954	267.588	ug/l	94
60) Dibromochloromethane	9.59	129	177369	51.644	ug/l	100
61) 1,2-Dibromoethane	9.68	107	177398	48.234	ug/l	99
64) Tetrachloroethene	9.34	164	172874	48.331	ug/l	97
65) Chlorobenzene	10.14	112	465053	49.902	ug/l	96
66) 1,1,1,2-Tetrachloroethane	10.23	131	165567	50.535	ug/l	99
67) Ethyl Benzene	10.26	91	793533	53.633	ug/l	97
68) m/p-Xylenes	10.36	106	626451	108.351	ug/l	95
69) o-Xylene	10.70	106	298519	56.214	ug/l	97
70) Styrene	10.71	104	505796	50.886	ug/l	97
71) Bromoform	10.86	173	144095	51.373	ug/l	100
73) Isopropylbenzene	11.02	105	793472	56.237	ug/l	100
74) N-amyl acetate	10.90	43	391119	50.419	ug/l	93
75) 1,1,2,2-Tetrachloroethane	11.27	83	280478	48.835	ug/l	100
76) 1,2,3-Trichloropropane	11.30	75	327423	65.260	ug/l	89
77) Bromobenzene	11.26	156	212891	51.948	ug/l	98
78) n-propylbenzene	11.36	91	928111	57.331	ug/l	100
79) 2-Chlorotoluene	11.42	91	554405	54.942	ug/l	98
80) 1,3,5-Trimethylbenzene	11.51	105	690112	53.379	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.08	75	86463	47.121	ug/l	98
82) 4-Chlorotoluene	11.51	91	664380	55.937	ug/l	99
83) tert-Butylbenzene	11.77	119	664895	57.236	ug/l	99
84) 1,2,4-Trimethylbenzene	11.81	105	711624	53.374	ug/l	98
85) sec-Butylbenzene	11.94	105	812118	57.396	ug/l	98
86) p-Isopropyltoluene	12.07	119	737210	57.507	ug/l	98
87) 1,3-Dichlorobenzene	12.03	146	399470	52.202	ug/l	99
88) 1,4-Dichlorobenzene	12.10	146	408703	51.737	ug/l	99
89) n-Butylbenzene	12.39	91	678112	58.244	ug/l	98
90) Hexachloroethane	12.60	117	111602	52.287	ug/l	99
91) 1,2-Dichlorobenzene	12.40	146	400041	50.023	ug/l	98
92) 1,2-Dibromo-3-Chloropropan	13.00	75	63310	50.203	ug/l	96

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092618\
Data File : VX004727.D
Acq On : 26 Sep 2018 14:16
Operator : JC/MD
Sample : VSTDICV050
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
ICVVX092618

Quant Time: Sep 27 01:10:01 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 26 14:17:02 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	13.65	180	311506	55.528	ug/l	99
94) Hexachlorobutadiene	13.79	225	152114	52.290	ug/l	96
95) Naphthalene	13.83	128	968467	51.985	ug/l	99
96) 1,2,3-Trichlorobenzene	14.02	180	313631	54.120	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092618\
 Data File : VX004727.D
 Acq On : 26 Sep 2018 14:16
 Operator : JC/MD
 Sample : VSTDICV050
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 Client Sampled :
 ICVVX092618

Quant Time: Sep 27 01:10:01 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration









#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.67 min Scan# 740
 Delta R.T. 0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618


Tgt Ion: 168 Resp: 306506
 Ion Ratio Lower Upper
 168 100
 99 49.0 39.9 59.9



#2
 Dichlorodifluoromethane
 Concen: 53.046 ug/l
 RT: 1.20 min Scan# 7
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 85 Resp: 221684
 Ion Ratio Lower Upper
 85 100
 87 34.2 17.0 50.9








#3
 Chloromethane
 Concen: 51.084 ug/l
 RT: 1.32 min Scan# 28
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16





Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion: 50 Resp: 259009
 Ion Ratio Lower Upper
 50 100
 52 33.0 26.2 39.2



#4
 Vinyl Chloride
 Concen: 50.387 ug/l
 RT: 1.40 min Scan# 41
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 62 Resp: 239614
 Ion Ratio Lower Upper
 62 100
 64 30.4 25.8 38.8









#5
 Bromomethane
 Concen: 53.200 ug/l
 RT: 1.64 min Scan# 79
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
94	150020		
96	96.4	74.5	111.7



#6
 Chloroethane
 Concen: 54.628 ug/l
 RT: 1.71 min Scan# 92
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
64	141015		
66	31.9	24.6	36.8









#7
 Trichlorofluoromethane
 Concen: 53.337 ug/l
 RT: 1.92 min Scan# 126
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
101	314007		
103	58.9	48.9	73.3



#8
 Diethyl Ether
 Concen: 48.022 ug/l
 RT: 2.19 min Scan# 170
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
74	122820		
45	102.6	48.3	144.8









#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 52.132 ug/l
 RT: 2.38 min Scan# 201
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
101	174826		
101	100		
85	40.4	34.2	51.4
151	83.0	65.0	97.6



#10
 Methyl Iodide
 Concen: 48.930 ug/l
 RT: 2.51 min Scan# 222
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
142	219572		
142	100		
127	42.7	33.8	50.6
141	13.7	11.4	17.0









#11
 Tert butyl alcohol
 Concen: 243.544 ug/l
 RT: 3.08 min Scan# 316
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
59	100		
57	9.8	8.2	12.4

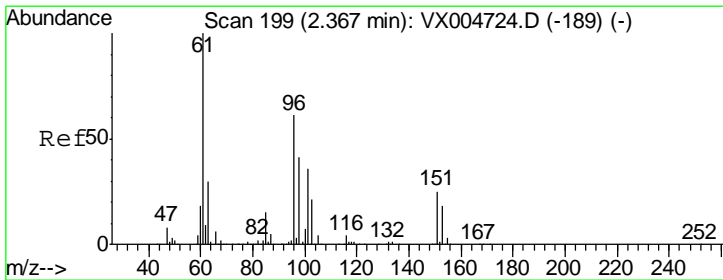

#12
 1,1-Dichloroethene
 Concen: 50.711 ug/l
 RT: 2.37 min Scan# 199
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
96	100		
61	157.6	128.8	193.2
98	62.1	52.2	78.2








#13
 Acrolein
 Concen: 244.095 ug/l
 RT: 2.29 min Scan# 187
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
56	100		
55	69.7	54.7	82.1



#14
 Allyl chloride
 Concen: 52.404 ug/l
 RT: 2.73 min Scan# 258
 Delta R.T. 0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
41	100		
39	58.0	48.9	73.3
76	27.0	26.7	40.1









#15
 Acrylonitrile
 Concen: 233.401 ug/l
 RT: 3.15 min Scan# 327
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
53	100		
52	86.8	65.2	97.8
51	36.1	28.2	42.2

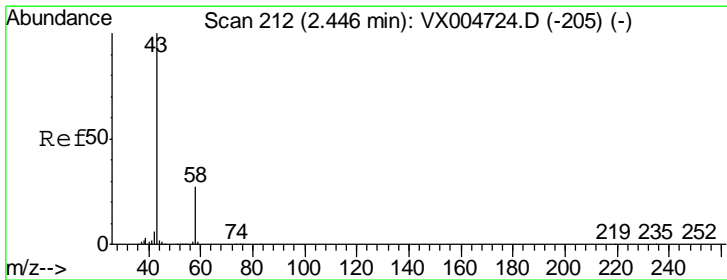

#16
 Acetone
 Concen: 259.755 ug/l
 RT: 2.45 min Scan# 212
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
43	100		
58	27.8	26.2	39.4









#17
 Carbon Disulfide
 Concen: 50.356 ug/l
 RT: 2.56 min Scan# 231
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618


Tgt Ion: 76 Resp: 502528
 Ion Ratio Lower Upper
 76 100
 78 8.7 7.0 10.6



#18
 Methyl Acetate
 Concen: 46.329 ug/l
 RT: 2.78 min Scan# 266
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 43 Resp: 300049
 Ion Ratio Lower Upper
 43 100
 74 21.6 19.4 29.2









#19
 Methyl tert-butyl Ether
 Concen: 51.703 ug/l
 RT: 3.20 min Scan# 336
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion	Resp	Lower	Upper
73	100		
57	24.9	17.1	25.7



#20
 Methylene Chloride
 Concen: 48.395 ug/l
 RT: 2.85 min Scan# 279
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
84	100		
49	133.1	101.2	151.8
51	40.4	29.5	44.3
86	74.7	52.3	78.5









#21
 trans-1,2-Dichloroethene
 Concen: 46.841 ug/l
 RT: 3.16 min Scan# 329
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
96	170291		
96	100		
61	163.7	113.8	170.6
98	63.6	51.8	77.8



#22
 Diisopropyl ether
 Concen: 52.612 ug/l
 RT: 3.87 min Scan# 446
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
45	641986		
45	100		
43	50.8	42.8	64.2
87	24.6	22.6	34.0
59	11.9	9.6	14.4









#23
 Vinyl Acetate
 Concen: 260.216 ug/l
 RT: 3.82 min Scan# 438
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleID : ICVVX092618


Tgt Ion	Resp	Lower	Upper
43	100		
86	9.8	8.9	13.3



#24
 1,1-Dichloroethane
 Concen: 45.929 ug/l
 RT: 3.69 min Scan# 416
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
63	100		
98	6.8	3.5	10.4
100	4.2	2.4	7.1









#25
 2-Butanone
 Concen: 262.785 ug/l
 RT: 4.70 min Scan# 582
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
43	990160		
72	21.1	22.0	33.0#



#26
 2,2-Dichloropropane
 Concen: 54.688 ug/l
 RT: 4.58 min Scan# 562
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
77	277195		
97	21.9	11.7	35.0









#27
 cis-1,2-Dichloroethene
 Concen: 50.600 ug/l
 RT: 4.60 min Scan# 565
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
96	205506		
61	141.8	0.0	282.6
98	67.8	0.0	130.2



#28
 Bromochloromethane
 Concen: 48.002 ug/l
 RT: 5.01 min Scan# 633
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
49	164534		
129	1.9	0.0	4.2
130	75.6	67.5	101.3









#29
 Tetrahydrofuran
 Concen: 254.148 ug/l
 RT: 5.15 min Scan# 656
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
42	100		
72	41.6	37.4	56.0
71	38.1	34.5	51.7



#30
 Chloroform
 Concen: 45.847 ug/l
 RT: 5.21 min Scan# 666
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
83	100		
85	63.2	52.6	79.0









#31
 Cyclohexane
 Concen: 54.350 ug/l
 RT: 5.57 min Scan# 724
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
56	100		
69	27.8	25.4	38.2
84	74.2	71.4	107.2



#32
 1,1,1-Trichloroethane
 Concen: 48.144 ug/l
 RT: 5.49 min Scan# 712
 Delta R.T. 0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
97	100		
99	65.2	52.0	78.0
61	43.5	34.9	52.3









#33
 1,2-Dichloroethane-d4
 Concen: 43.044 ug/l
 RT: 6.07 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleID : ICVVX092618




Tgt Ion	Resp	Lower	Upper
65	188466		
67	58.2	0.0	106.8



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
114	394137		
63	20.3	0.0	39.0
88	14.8	0.0	30.4









#35
 Dibromofluoromethane
 Concen: 49.877 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16


Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion	Resp	Lower	Upper
113	166608		
111	100.4	82.4	123.6
192	22.8	19.4	29.2



#36
 1,1-Dichloropropene
 Concen: 54.111 ug/l
 RT: 5.79 min Scan# 761
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
75	246609		
110	37.1	18.0	54.0
77	30.7	24.6	36.8









#37
Ethyl Acetate
Concen: 53.908 ug/l
RT: 4.87 min Scan# 609
Delta R.T. 0.01 min
Lab File: VX004727.D
Acq: 26 Sep 2018 14:16




Instrument :
MSVOA_X
ClientSampled :
ICVVX092618


Tgt Ion	Resp	Lower	Upper
43	100		
61	14.1	11.5	17.3
70	10.1	9.0	13.6



#38
Carbon Tetrachloride
Concen: 49.588 ug/l
RT: 5.78 min Scan# 759
Delta R.T. 0.00 min
Lab File: VX004727.D
Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
117	100		
119	103.2	78.8	118.2
121	32.9	24.9	37.3









#39
 Methylcyclohexane
 Concen: 60.177 ug/l
 RT: 7.46 min Scan# 1035
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
83	100		
55	64.1	61.0	91.4
98	36.1	39.6	59.4#



#40
 Benzene
 Concen: 52.904 ug/l
 RT: 6.14 min Scan# 818
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
78	100		
77	22.2	19.0	28.4









#41
 Methacrylonitrile
 Concen: 53.887 ug/l
 RT: 5.06 min Scan# 641
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Instrument : MSVOA_X
 ClientSampled : ICVVX092618

Tgt Ion	Resp	Lower	Upper
41	100		
39	53.5	42.4	63.6
67	68.0	59.2	88.8
52	27.3	23.0	34.4




Abundance Ion 41.00 (40.70 to 41.70): VX0
 Ion 39.00 (38.70 to 39.70): VX0
 Ion 67.00 (66.70 to 67.70): VX0
 Ion 52.00 (51.70 to 52.70): VX0






#42
 1,2-Dichloroethane
 Concen: 50.676 ug/l
 RT: 6.20 min Scan# 827
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
62	100		
98	9.4	0.0	20.6



Abundance Ion 61.90 (61.60 to 62.60): VX0
 Ion 97.90 (97.60 to 98.60): VX0









#43
 Isopropyl Acetate
 Concen: 52.517 ug/l
 RT: 6.46 min Scan# 871
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
43	100		
61	20.9	17.0	25.4
87	13.1	11.4	17.2



#44
 Trichloroethene
 Concen: 50.620 ug/l
 RT: 7.21 min Scan# 994
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
130	100		
95	97.9	0.0	181.6









#45
 1,2-Dichloropropane
 Concen: 51.247 ug/l
 RT: 7.52 min Scan# 1044
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion	Resp	Lower	Upper
63	179312		
65	31.4	24.3	36.5



#46
 Dibromomethane
 Concen: 51.537 ug/l
 RT: 7.66 min Scan# 1068
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
93	113329		
95	84.1	65.5	98.3
174	118.3	94.2	141.4








#47
 Bromodichloromethane
 Concen: 52.618 ug/l
 RT: 7.90 min Scan# 1106
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16





Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
83	216632		
85	63.6	50.9	76.3
127	9.3	7.3	10.9



#48
 Methyl methacrylate
 Concen: 57.184 ug/l
 RT: 7.78 min Scan# 1087
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
41	226631		
69	80.9	70.2	105.4
39	51.8	42.7	64.1









#49
 1,4-Dioxane
 Concen: 1081.318 ug/l
 RT: 7.76 min Scan# 1083
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion	Resp	Lower	Upper
88	106468		
43	32.3	24.7	37.1
58	72.8	55.3	82.9



#50
 Toluene-d8
 Concen: 50.206 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
98	557533		
100	64.9	52.9	79.3









#51
 4-Methyl-2-Pentanone
 Concen: 277.110 ug/l
 RT: 8.65 min Scan# 1230
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Instrument : MSVOA_X
 ClientSampleID : ICVVX092618

Tgt Ion: 43 Resp: 1523520




Ion	Ratio	Lower	Upper
43	100		
58	38.8	33.1	49.7




#52
 Toluene
 Concen: 52.933 ug/l
 RT: 8.79 min Scan# 1252
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 92 Resp: 414999

Ion	Ratio	Lower	Upper
92	100		
91	175.5	136.4	204.6









#53
 t-1,3-Dichloropropene
 Concen: 54.101 ug/l
 RT: 9.04 min Scan# 1294
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampleId : ICVVX092618


Tgt Ion: 75 Resp: 251702
 Ion Ratio Lower Upper
 75 100
 77 31.3 24.6 37.0



#54
 cis-1,3-Dichloropropene
 Concen: 55.878 ug/l
 RT: 8.44 min Scan# 1195
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 75 Resp: 272299
 Ion Ratio Lower Upper
 75 100
 77 31.9 26.2 39.2
 39 46.2 36.4 54.6









#55
 1,1,2-Trichloroethane
 Concen: 49.730 ug/l
 RT: 9.22 min Scan# 1323
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
97	170783		
83	85.7	66.4	99.6
85	55.5	43.3	64.9
99	63.9	49.0	73.4



#56
 Ethyl methacrylate
 Concen: 48.908 ug/l
 RT: 9.18 min Scan# 1317
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
69	272184		
41	70.4	51.0	76.4
39	33.8	26.1	39.1








#57
 1,3-Dichloropropane
 Concen: 50.774 ug/l
 RT: 9.37 min Scan# 1348
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16





Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
76	290208		
78	31.8	25.5	38.3



#58
 2-Chloroethyl Vinyl ether
 Concen: 256.841 ug/l
 RT: 8.32 min Scan# 1175
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
63	761232		
106	27.0	23.9	35.9









#59
 2-Hexanone
 Concen: 267.588 ug/l
 RT: 9.50 min Scan# 1369
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Instrument :
 MSVOA_X
ClientSampled :
 ICVVX092618

Tgt Ion: 43 Resp: 1225954




Ion	Ratio	Lower	Upper
43	100		
58	53.3	29.0	87.0




#60
 Dibromochloromethane
 Concen: 51.644 ug/l
 RT: 9.59 min Scan# 1383
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 129 Resp: 177369

Ion	Ratio	Lower	Upper
129	100		
127	76.9	38.5	115.5









#61
 1,2-Dibromoethane
 Concen: 48.234 ug/l
 RT: 9.68 min Scan# 1398
 Delta R.T. 0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
107	177398		
109	94.5	76.0	114.0



#62
 4-Bromofluorobenzene
 Concen: 52.149 ug/l
 RT: 11.14 min Scan# 1638
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
95	208629		
174	90.2	0.0	185.2
176	87.2	0.0	178.6









#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.12 min Scan# 1470
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
117	363426		
82	54.9	47.8	71.6
119	32.2	29.3	43.9



#64
 Tetrachloroethene
 Concen: 48.331 ug/l
 RT: 9.34 min Scan# 1342
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
164	172874		
166	129.6	102.8	154.2
129	91.5	69.4	104.0
131	88.7	67.9	101.9









#65
 Chlorobenzene
 Concen: 49.902 ug/l
 RT: 10.14 min Scan# 1474
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
112	100		
114	32.2	27.8	41.8



#66
 1,1,1,2-Tetrachloroethane
 Concen: 50.535 ug/l
 RT: 10.23 min Scan# 1488
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
131	100		
133	95.4	48.1	144.4
119	65.3	32.9	98.6









#67
Ethyl Benzene
Concen: 53.633 ug/l
RT: 10.26 min Scan# 1493
Delta R.T. -0.00 min
Lab File: VX004727.D
Acq: 26 Sep 2018 14:16




Instrument :
MSVOA_X
ClientSampled :
ICVVX092618


Tgt Ion: 91 Resp: 793533
Ion Ratio Lower Upper
91 100
106 31.0 25.9 38.9



#68
m/p-Xylenes
Concen: 108.351 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.01 min
Lab File: VX004727.D
Acq: 26 Sep 2018 14:16

Tgt Ion: 106 Resp: 626451
Ion Ratio Lower Upper
106 100
91 203.5 157.1 235.7









#69
 o-Xylene
 Concen: 56.214 ug/l
 RT: 10.70 min Scan# 1566
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
106	298519		
91	214.1	105.1	315.1



#70
 Styrene
 Concen: 50.886 ug/l
 RT: 10.71 min Scan# 1568
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
104	505796		
78	49.8	37.4	56.0
103	55.8	43.8	65.6









#71
 Bromoform
 Concen: 51.373 ug/l
 RT: 10.86 min Scan# 1592
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
173	144095		
175	48.5	24.1	72.3
254	0.2	0.2	0.2



#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
152	223846		
150	176.1	0.0	351.0
115	80.6	39.0	117.0









#73
 Isopropylbenzene
 Concen: 56.237 ug/l
 RT: 11.02 min Scan# 1618
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
105	100		
120	26.8	13.5	40.4



#74
 N-amyl acetate
 Concen: 50.419 ug/l
 RT: 10.90 min Scan# 1599
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
43	100		
70	40.3	37.4	56.0
55	24.9	21.8	32.8
61	23.6	20.6	30.8









#75
 1,1,2,2-Tetrachloroethane
 Concen: 48.835 ug/l
 RT: 11.27 min Scan# 1659
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
83	100		
131	10.1	5.2	15.6
85	64.7	32.3	96.8



#76
 1,2,3-Trichloropropane
 Concen: 65.260 ug/l
 RT: 11.30 min Scan# 1664
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
75	100		
77	33.5	20.2	60.6







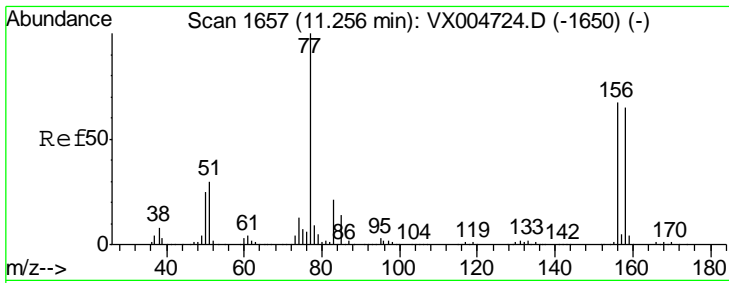

#77
 Bromobenzene
 Concen: 51.948 ug/l
 RT: 11.26 min Scan# 1657
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
156	212891		
77	147.1	71.5	214.3
158	98.1	48.9	146.8



#78
 n-propylbenzene
 Concen: 57.331 ug/l
 RT: 11.36 min Scan# 1674
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
91	928111		
120	23.7	11.9	35.9









#79
 2-Chlorotoluene
 Concen: 54.942 ug/l
 RT: 11.42 min Scan# 1684
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
91	100		
126	34.9	17.9	53.7



#80
 1,3,5-Trimethylbenzene
 Concen: 53.379 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
105	100		
120	48.9	25.6	76.8









#81
 trans-1,4-Dichloro-2-butene
 Concen: 47.121 ug/l
 RT: 11.08 min Scan# 1628
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
75	100		
53	97.5	80.1	120.1
89	46.3	37.2	55.8



#82
 4-Chlorotoluene
 Concen: 55.937 ug/l
 RT: 11.51 min Scan# 1699
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
91	100		
126	30.4	15.5	46.5









#83
 tert-Butylbenzene
 Concen: 57.236 ug/l
 RT: 11.77 min Scan# 1742
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument : MSVOA_X
 ClientSampled : ICVVX092618


Tgt Ion	Resp	Lower	Upper
119	664895		
91	100	27.0	81.0
134	100	11.7	35.1

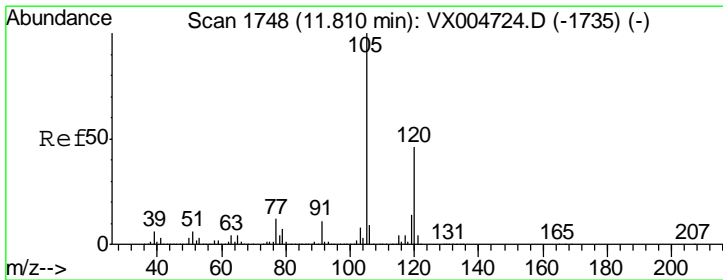

#84
 1,2,4-Trimethylbenzene
 Concen: 53.374 ug/l
 RT: 11.81 min Scan# 1748
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
105	711624		
120	100	23.2	69.6









#85
 sec-Butylbenzene
 Concen: 57.396 ug/l
 RT: 11.94 min Scan# 1770
 Delta R.T. -0.01 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
105	100		
134	20.2	10.5	31.5



#86
 p-Isopropyltoluene
 Concen: 57.507 ug/l
 RT: 12.07 min Scan# 1790
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
119	100		
134	26.5	13.4	40.2
91	23.2	10.9	32.7









#87
 1,3-Dichlorobenzene
 Concen: 52.202 ug/l
 RT: 12.03 min Scan# 1784
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
146	100		
111	38.2	18.7	56.1
148	64.5	32.1	96.5



#88
 1,4-Dichlorobenzene
 Concen: 51.737 ug/l
 RT: 12.10 min Scan# 1795
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
146	100		
111	37.1	18.1	54.1
148	64.2	32.0	96.0









#89
 n-Butylbenzene
 Concen: 58.244 ug/l
 RT: 12.39 min Scan# 1843
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampled :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
91	678112		
92	52.5	27.3	81.9
134	26.6	13.6	40.7



#90
 Hexachloroethane
 Concen: 52.287 ug/l
 RT: 12.60 min Scan# 1877
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
117	111602		
201	94.9	46.9	140.6









#91
 1,2-Dichlorobenzene
 Concen: 50.023 ug/l
 RT: 12.40 min Scan# 1844
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Instrument :
 MSVOA_X
 ClientSampleID :
 ICVVX092618

Tgt Ion: 146 Resp: 400041




Ion	Ratio	Lower	Upper
146	100		
111	39.6	19.4	58.1
148	64.0	32.8	98.3




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 50.203 ug/l
 RT: 13.00 min Scan# 1943
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion: 75 Resp: 63310

Ion	Ratio	Lower	Upper
75	100		
155	93.3	48.0	144.2
157	118.0	61.4	184.1









#93
 1,2,4-Trichlorobenzene
 Concen: 55.528 ug/l
 RT: 13.65 min Scan# 2049
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16




Instrument :
 MSVOA_X
 ClientSampleId :
 ICVVX092618


Tgt Ion	Resp	Lower	Upper
180	311506		
182	95.4	48.4	145.0
145	28.5	14.3	42.9



#94
 Hexachlorobutadiene
 Concen: 52.290 ug/l
 RT: 13.79 min Scan# 2072
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
225	152114		
223	63.3	30.1	90.5
227	64.9	30.8	92.4









#95
 Naphthalene
 Concen: 51.985 ug/l
 RT: 13.83 min Scan# 2080
 Delta R.T. 0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Instrument : MSVOA_X
 ClientSampled : ICVVX092618

Tgt Ion	Resp	Lower	Upper
128	968467		
127	13.0	10.2	15.2
129	10.9	8.6	12.8



#96
 1,2,3-Trichlorobenzene
 Concen: 54.120 ug/l
 RT: 14.02 min Scan# 2111
 Delta R.T. -0.00 min
 Lab File: VX004727.D
 Acq: 26 Sep 2018 14:16

Tgt Ion	Resp	Lower	Upper
180	313631		
182	95.8	48.5	145.6
145	29.6	14.9	44.9

