

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092618\
 Data File : VX004744.D
 Acq On : 27 Sep 2018 01:04
 Operator : JC/MD
 Sample : J5078-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 600-WILSON-AVE-NEWARK

Quant Time: Sep 27 05:21:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	281314	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	416385	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	396698	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	233866	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	215836	53.71	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.42%	
35) Dibromofluoromethane	5.50	113	185511	52.57	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.14%	
50) Toluene-d8	8.72	98	584328	49.81	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.62%	
62) 4-Bromofluorobenzene	11.14	95	219814	52.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.02%	

Target Compounds


					Qvalue	
3) Chloromethane	1.30	50	2668	0.573	ug/l #	42
6) Chloroethane	1.71	64	4355	Below Cal	#	52
11) Tert butyl alcohol	3.07	59	4751	4.228	ug/l #	72
13) Acrolein	2.30	56	208	0.260	ug/l #	16
14) Allyl chloride	2.62	41	7663	1.152	ug/l #	72
16) Acetone	2.45	43	37713	16.075	ug/l	93
17) Carbon Disulfide	2.57	76	2405	0.263	ug/l	98
19) Methyl tert-butyl Ether	3.21	73	66702	6.344	ug/l	94
20) Methylene Chloride	2.87	84	452	Below Cal	#	81
25) 2-Butanone	4.70	43	778	0.225	ug/l #	88
29) Tetrahydrofuran	5.19	42	524	0.244	ug/l #	46
31) Cyclohexane	5.58	56	1139	0.223	ug/l	89
36) 1,1-Dichloropropene	5.67	75	18424	3.827	ug/l #	50
38) Carbon Tetrachloride	5.66	117	24461	4.833	ug/l #	15
39) Methylcyclohexane	7.45	83	1122	0.228	ug/l	92
56) Ethyl methacrylate	9.21	69	44	2.869	ug/l #	1
58) 2-Chloroethyl Vinyl ether	8.32	63	80	14.266	ug/l #	45
68) m/p-Xylenes	10.36	106	1676	0.266	ug/l	96
70) Styrene	10.72	104	352	2.172	ug/l #	78
74) N-amyl acetate	10.91	43	155	1.766	ug/l #	1
76) 1,2,3-Trichloropropane	11.14	75	109158	20.825	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.51	105	852	Below Cal		94
81) trans-1,4-Dichloro-2-buten	11.14	75	109158	56.526	ug/l #	10
83) tert-Butylbenzene	11.77	119	4405	0.363	ug/l	76
84) 1,2,4-Trimethylbenzene	11.80	105	1586	Below Cal		91
85) sec-Butylbenzene	11.94	105	3257	0.220	ug/l #	1
86) p-Isopropyltoluene	12.23	119	6305	0.471	ug/l	91
90) Hexachloroethane	12.67	117	2391	1.072	ug/l #	3
95) Naphthalene	13.83	128	15010	1.480	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092618\
Data File : VX004744.D
Acq On : 27 Sep 2018 01:04
Operator : JC/MD
Sample : J5078-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK

Quant Time: Sep 27 05:21:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 26 14:17:02 2018
Response via : Initial Calibration

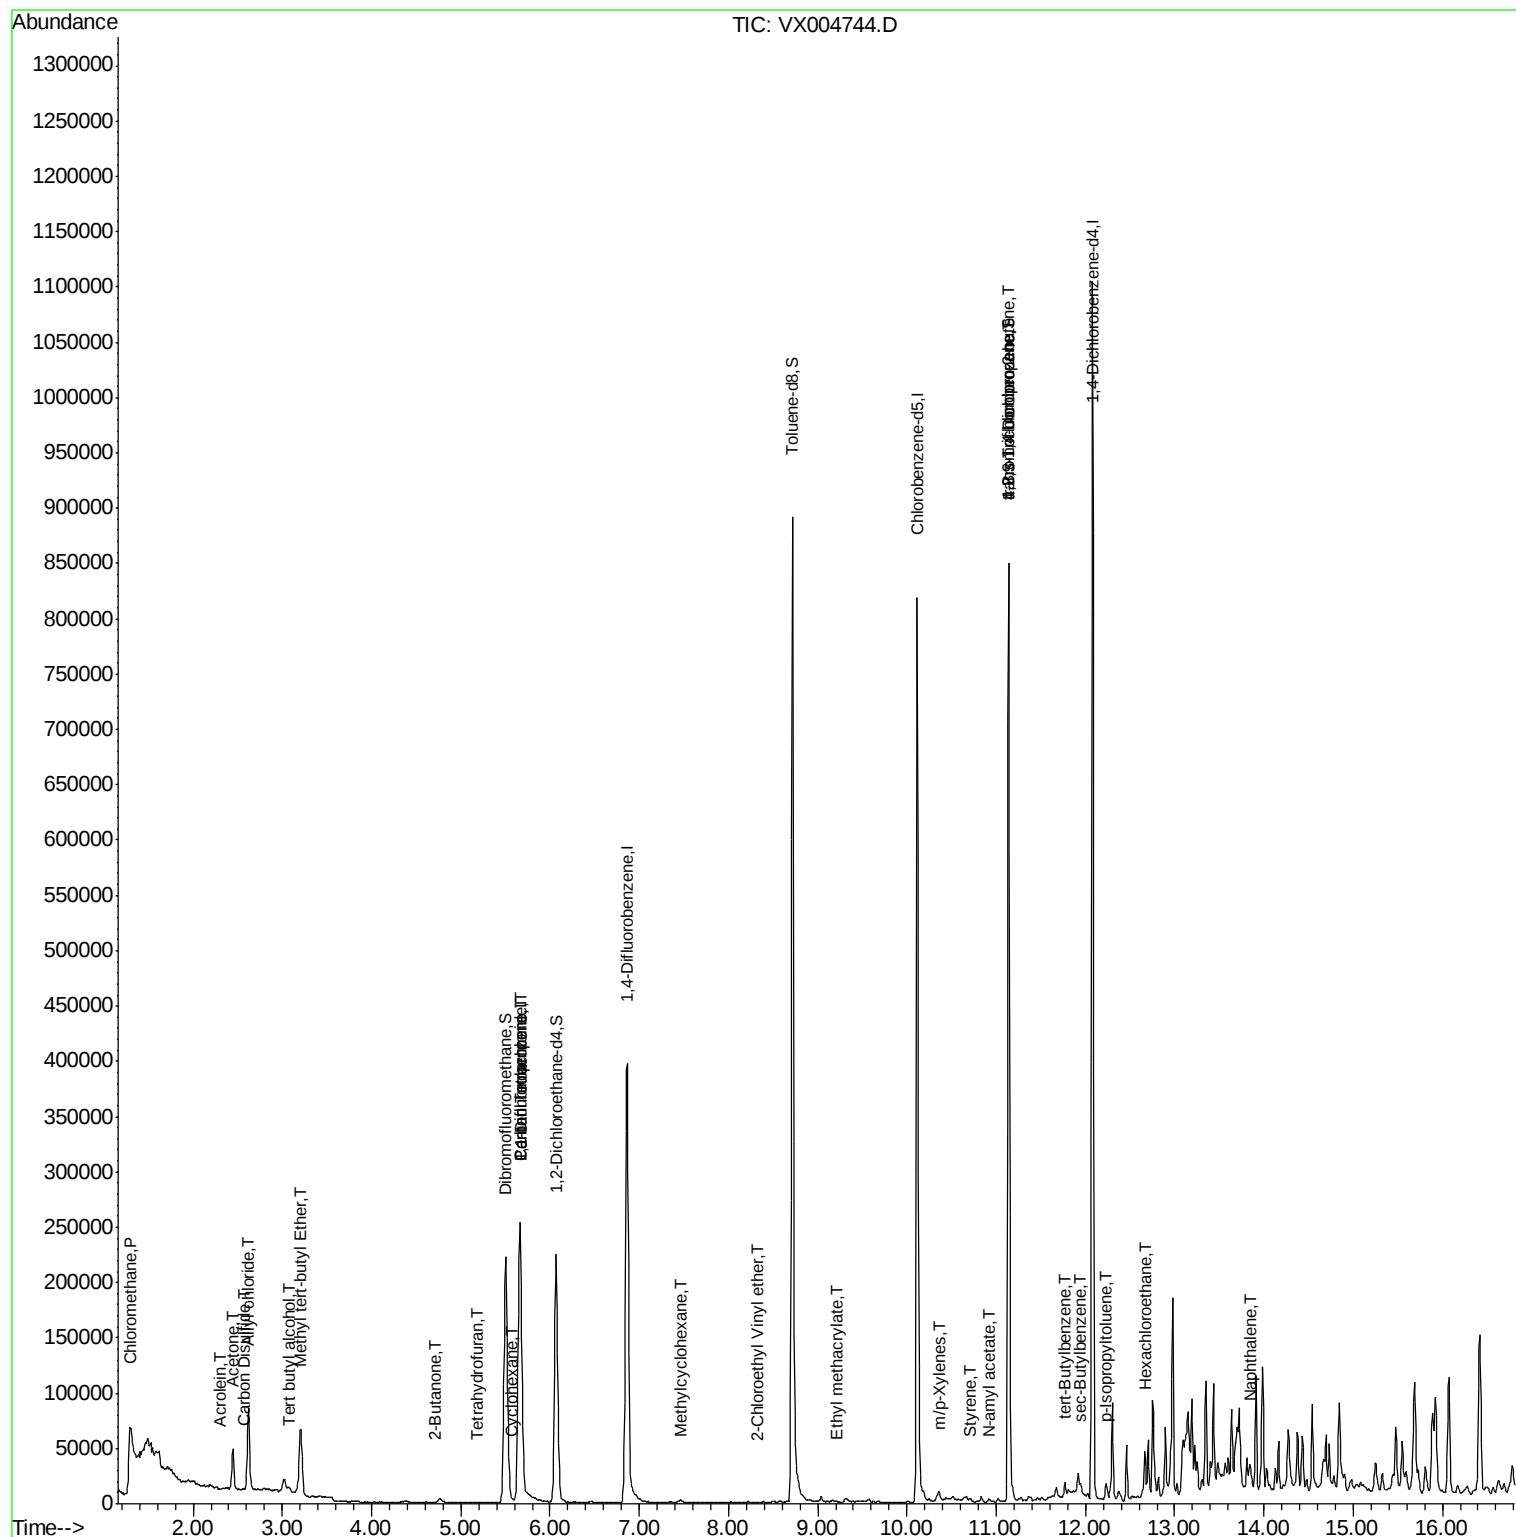



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :


600-WILSON-AVE-NEWARK

Tot Ion:168 Resp: 281314

Ion Ratio Lower Upper

168 100

99 48.0 39.9 59.9

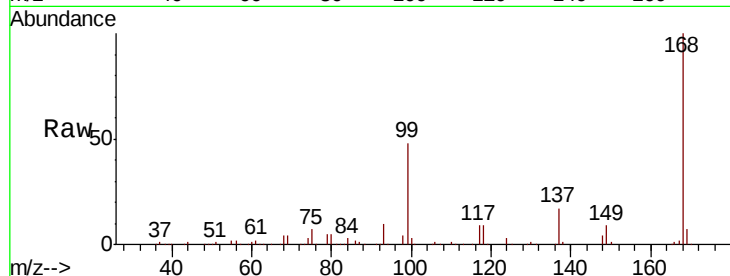

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000



60000

40000

20000

0

Time-->



#3

Chloromethane

Concen: 0.573 ug/l

RT: 1.30 min Scan# 24

Delta R.T. -0.02 min

Lab File: VX004744.D


Acq: 27 Sep 2018 01:04

Tgt Ion: 50 Resp: 2668

Ion Ratio Lower Upper

50 100

52 0.0 26.2 39.2#



Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

1.30

1200

1000

800


600


400

200

0

Time-->



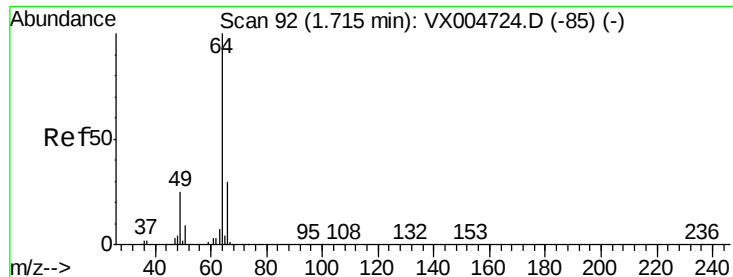

#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 92

Delta R.T. 0.00 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :





600-WILSON-AVE-NEWARK

Tot Ion: 64 Resp: 4355

Ion Ratio Lower Upper

64 100

66 4.2 24.6 36.8#

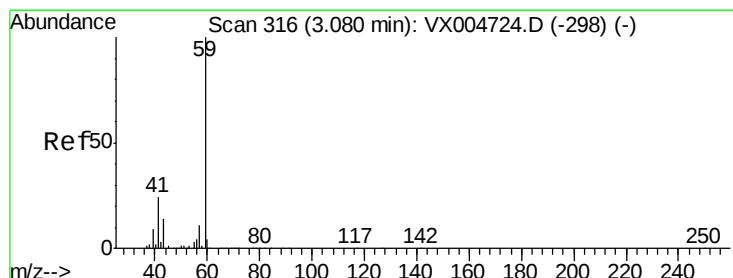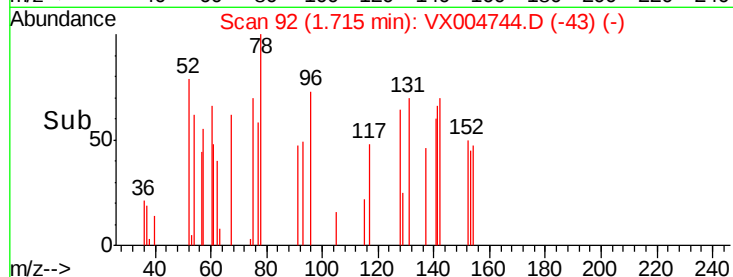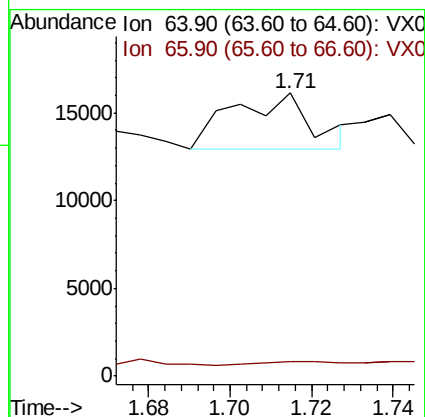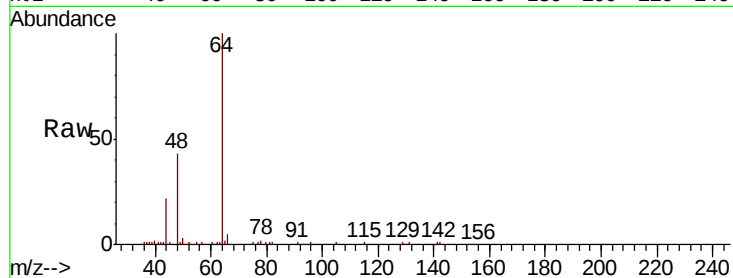

#11

Tert butyl alcohol

Concen: 4.228 ug/l

RT: 3.07 min Scan# 315

Delta R.T. -0.01 min

Lab File: VX004744.D




Acq: 27 Sep 2018 01:04


Tgt Ion: 59 Resp: 4751

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.4#

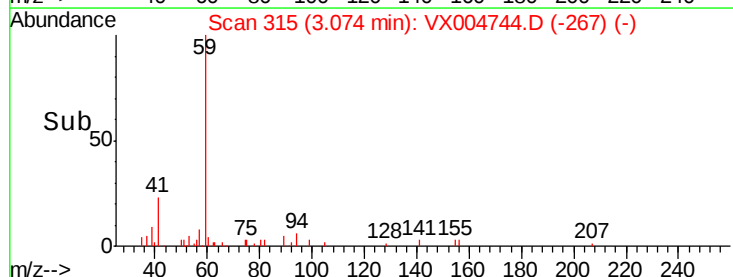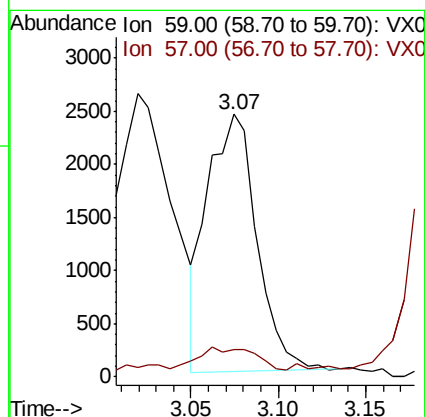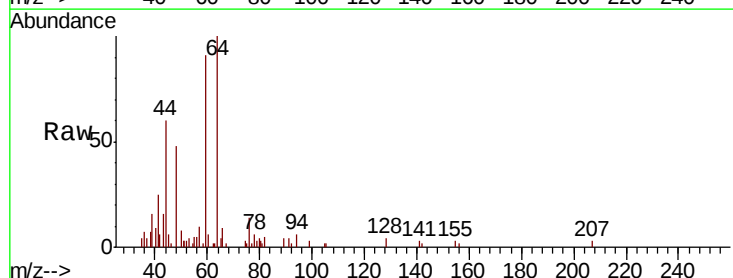



#13

Acrolein

Concen: 0.260 ug/l

RT: 2.30 min Scan# 188

Delta R.T. 0.01 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :


600-WILSON-AVE-NEWARK

Tot Ion: 56 Resp: 208




Ion Ratio Lower Upper

56 100

55 0.0 54.7 82.1#

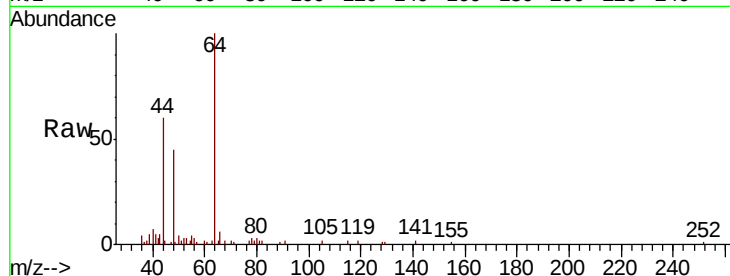

Abundance Ion 56.00 (55.70 to 56.70): VX0

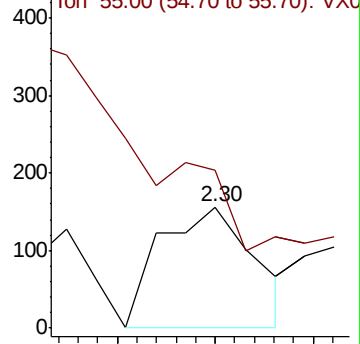

#14

Allyl chloride

Concen: 1.152 ug/l

RT: 2.62 min Scan# 240

Delta R.T. -0.10 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04


Tgt Ion: 41 Resp: 7663

Ion Ratio Lower Upper



41 100


39 71.4 48.9 73.3

76 2.5 26.7 40.1#



Abundance Ion 41.00 (40.70 to 41.70): VX0

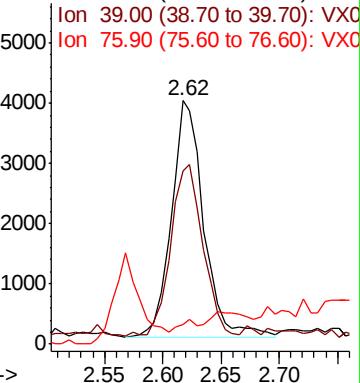



#16

Acetone

Concen: 16.075 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :


600-WILSON-AVE-NEWARK

Tot Ion: 43 Resp: 37713

Ion Ratio Lower Upper

43 100

58 29.1 26.2 39.4

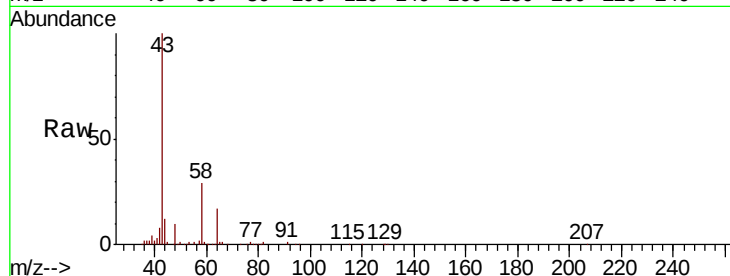

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2.45

25000

20000



15000

10000

5000

0

Time--> 2.35 2.40 2.45 2.50 2.55



#17

Carbon Disulfide

Concen: 0.263 ug/l

RT: 2.57 min Scan# 232

Delta R.T. 0.00 min

Lab File: VX004744.D


Acq: 27 Sep 2018 01:04

Tgt Ion: 76 Resp: 2405

Ion Ratio Lower Upper

76 100

78 9.4 7.0 10.6



Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

2.57


1500


1000

500

0

Time--> 2.55 2.60









#19

Methyl tert-butyl Ether
 Concen: 6.344 ug/l
 RT: 3.21 min Scan# 337
 Delta R.T. 0.01 min
 Lab File: VX004744.D
 Acq: 27 Sep 2018 01:04

Instrument :
 MSVOA_X
 ClientSampleId :
 600-WILSON-AVE-NEWARK




Tot Ion: 73 Resp: 66702
 Ion Ratio Lower Upper
 73 100
 57 24.2 17.1 25.7

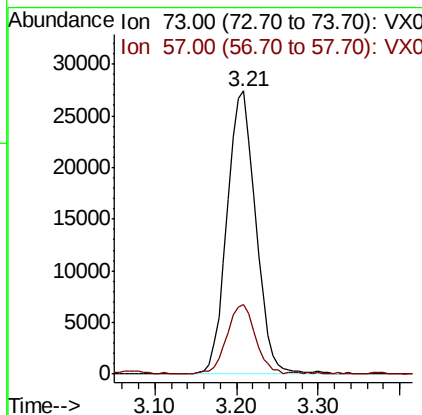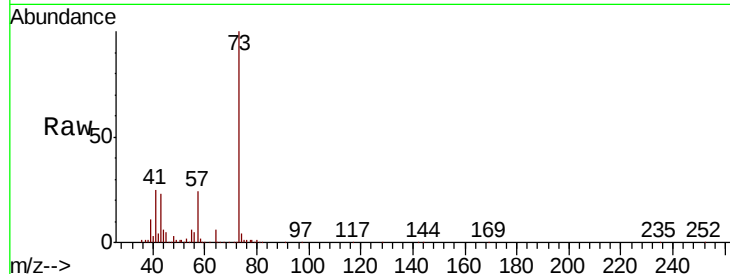


#20

Methylene Chloride
 Concen: Below Cal
 RT: 2.87 min Scan# 281
 Delta R.T. 0.01 min
 Lab File: VX004744.D
 Acq: 27 Sep 2018 01:04

Tgt Ion: 84 Resp: 452
 Ion Ratio Lower Upper
 84 100
 49 95.5 101.2 151.8#
 51 40.7 29.5 44.3
 86 56.3 52.3 78.5

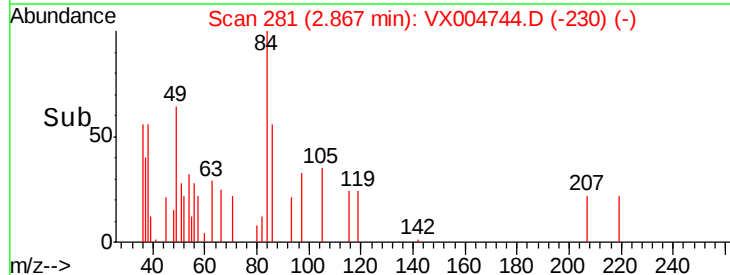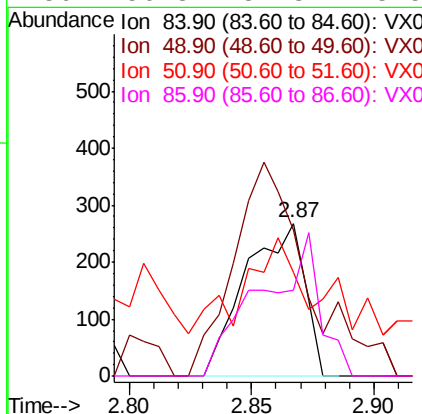

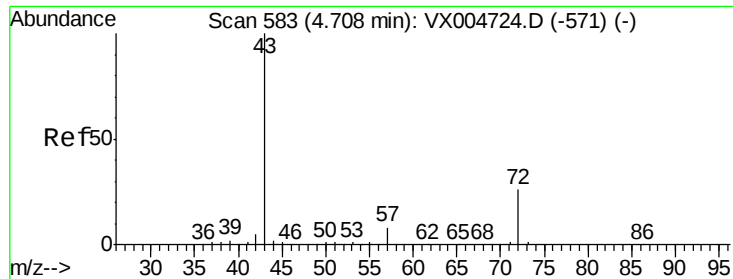

#25

2-Butanone

Concen: 0.225 ug/l

RT: 4.70 min Scan# 582

Delta R.T. -0.01 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :


600-WILSON-AVE-NEWARK

Tot Ion: 43 Resp: 778

Ion Ratio Lower Upper




43 100

72 21.2 22.0 33.0#

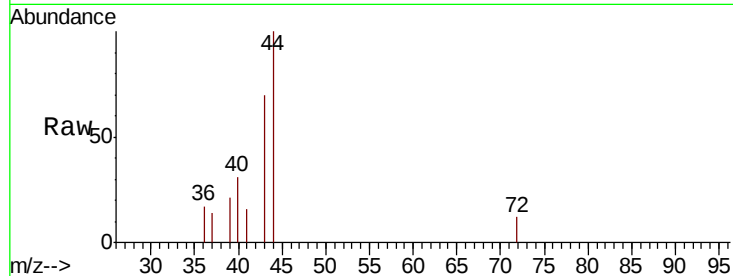

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

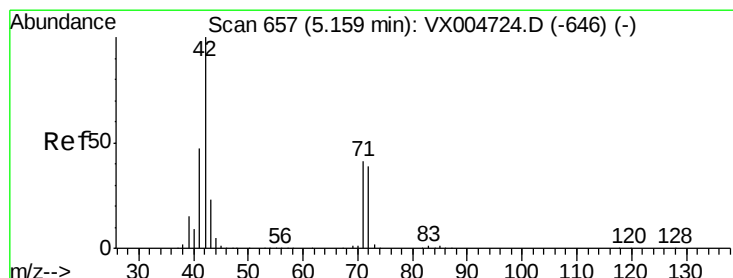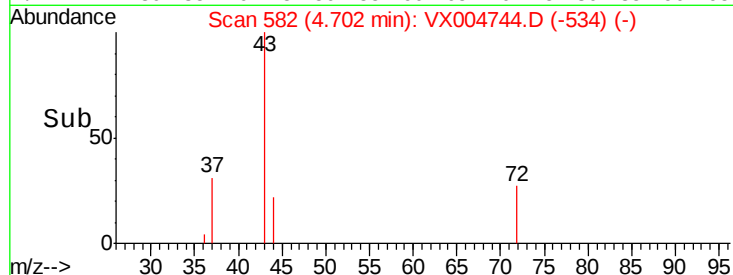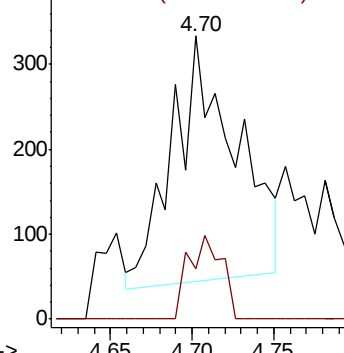

#29

Tetrahydrofuran

Concen: 0.244 ug/l

RT: 5.19 min Scan# 662

Delta R.T. 0.03 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04


Tgt Ion: 42 Resp: 524

Ion Ratio Lower Upper

42 100

72 0.0 37.4 56.0#



71 19.5 34.5 51.7#

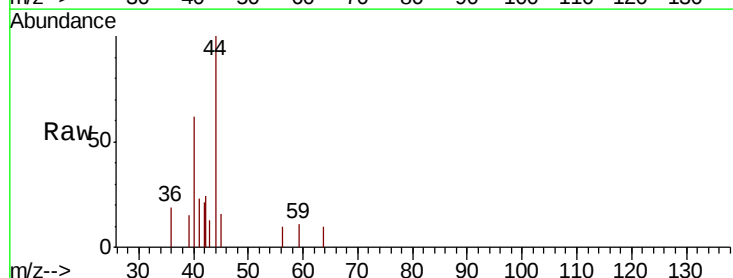


Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0



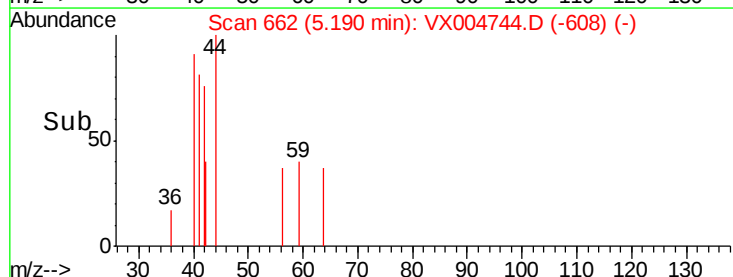
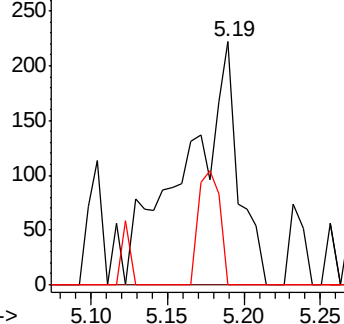




#31
Cyclohexane
Concen: 0.223 ug/l
RT: 5.58 min Scan# 726
Delta R.T. 0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04




Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK


Tot Ion: 56 Resp: 1139
Ion Ratio Lower Upper
56 100
69 33.5 25.4 38.2
84 75.7 71.4 107.2

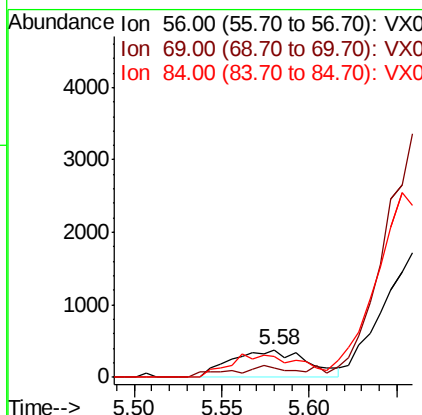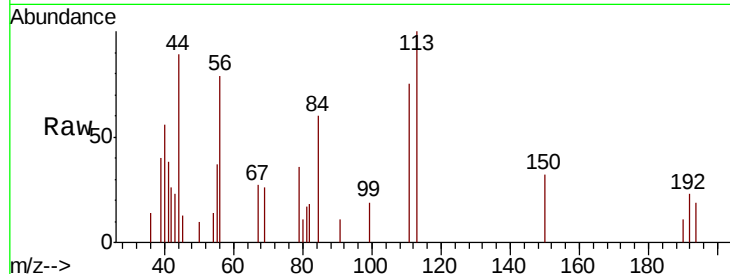

#33
1,2-Dichloroethane-d4
Concen: 53.710 ug/l
RT: 6.07 min Scan# 807
Delta R.T. 0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion: 65 Resp: 215836
Ion Ratio Lower Upper
65 100
67 50.6 0.0 106.8

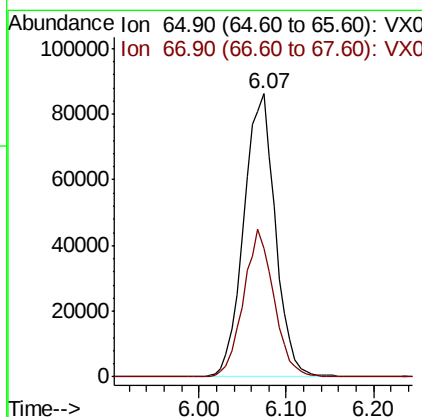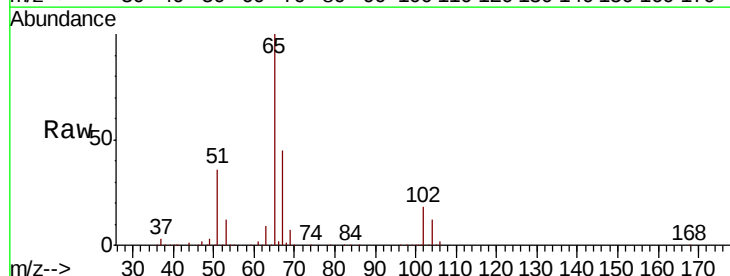


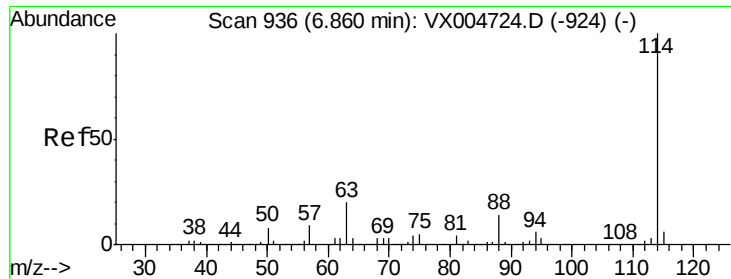




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.87 min Scan# 937
 Delta R.T. 0.01 min
 Lab File: VX004744.D
 Acq: 27 Sep 2018 01:04

Instrument :
 MSVOA_X
 ClientSampleId :
 600-WILSON-AVE-NEWARK

Tot Ion:114 Resp: 416385
 Ion Ratio Lower Upper
 114 100
 63 17.3 0.0 39.0
 88 13.9 0.0 30.4

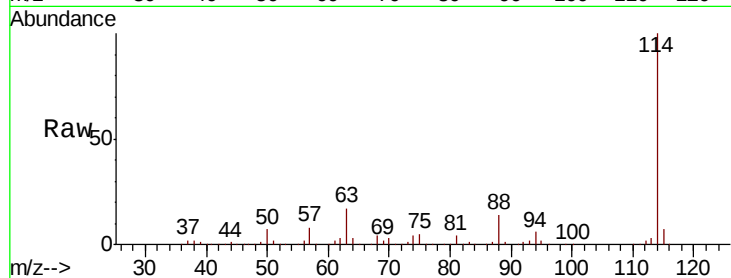


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VX0
 Ion 87.90 (87.60 to 88.60): VX0

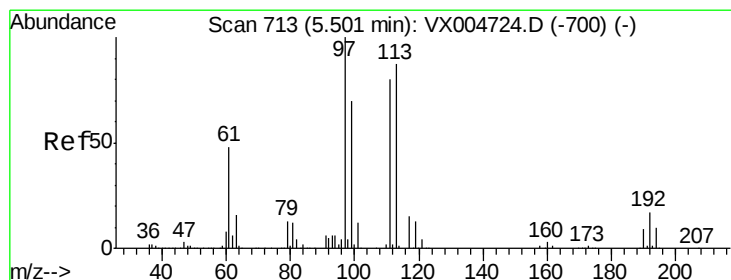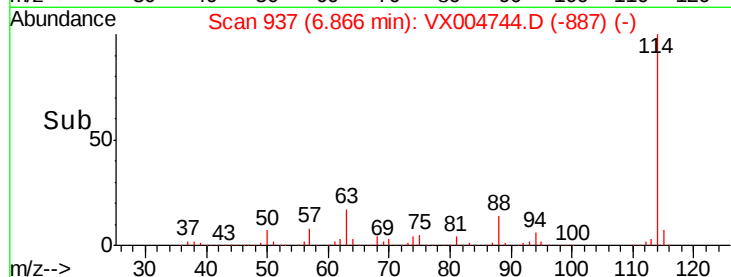
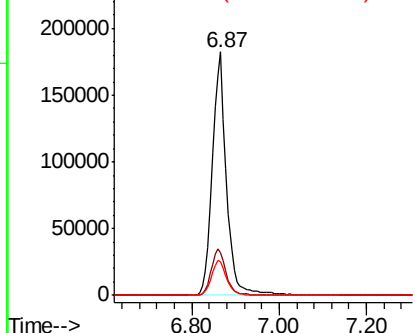



#35
 Dibromofluoromethane
 Concen: 52.569 ug/l
 RT: 5.50 min Scan# 713
 Delta R.T. 0.00 min
 Lab File: VX004744.D
 Acq: 27 Sep 2018 01:04

Tgt Ion:113 Resp: 185511
 Ion Ratio Lower Upper
 113 100
 111 100.0 82.4 123.6
 192 22.0 19.4 29.2

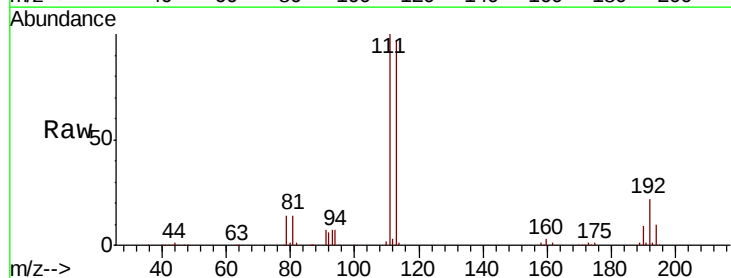

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

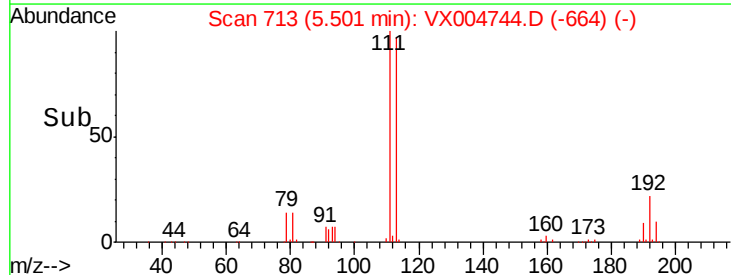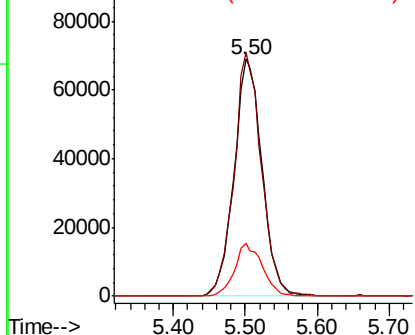

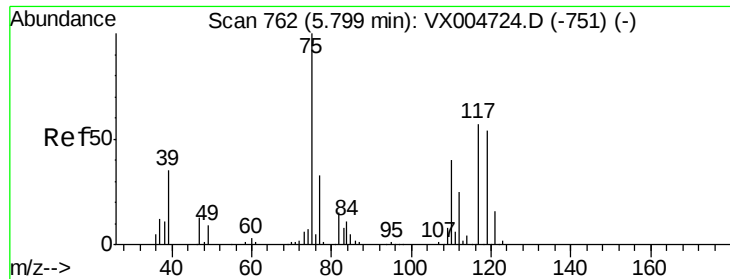

#36

1,1-Dichloropropene

Concen: 3.827 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :

600-WILSON-AVE-NEWARK


Tot Ion: 75 Resp: 18424

Ion Ratio Lower Upper

75 100

110 9.6 18.0 54.0#




77 0.0 24.6 36.8#

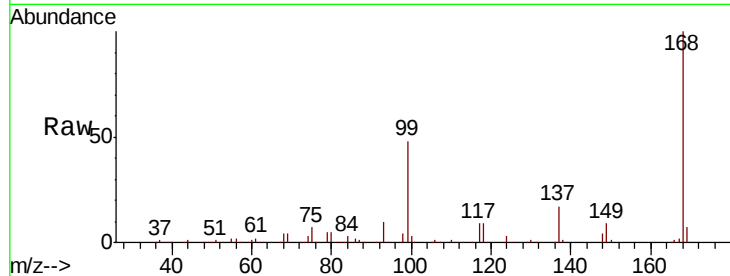

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VX0

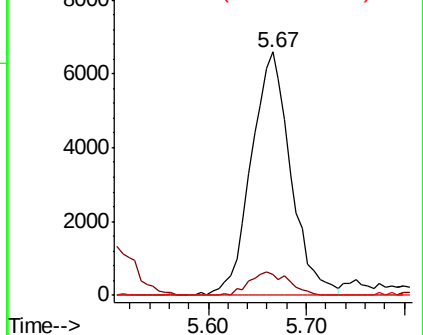

#38

Carbon Tetrachloride

Concen: 4.833 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.12 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04


Tgt Ion: 117 Resp: 24461

Ion Ratio Lower Upper

117 100

119 5.2 78.8 118.2#



121 0.0 24.9 37.3#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V




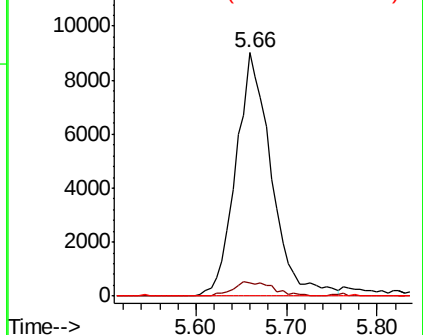


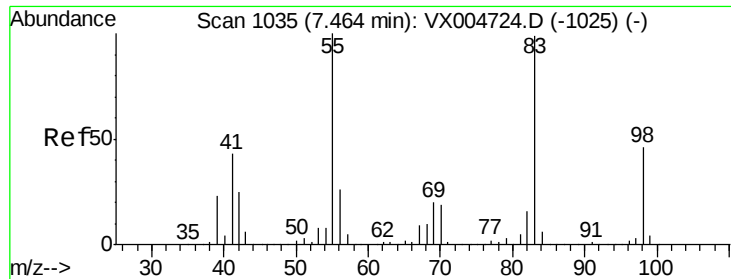

#39
Methylcyclohexane
Concen: 0.228 ug/l
RT: 7.45 min Scan# 1033
Delta R.T. -0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04




Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK


Tot Ion: 83 Resp: 1122
Ion Ratio Lower Upper
83 100
55 81.1 61.0 91.4
98 41.9 39.6 59.4

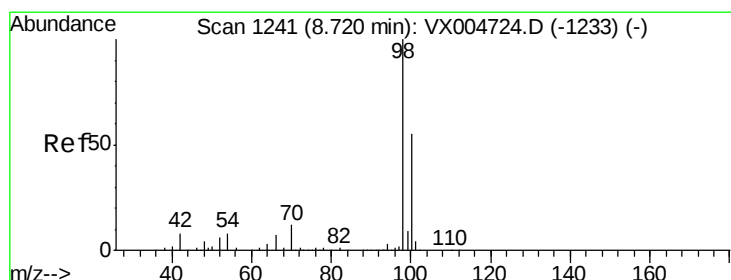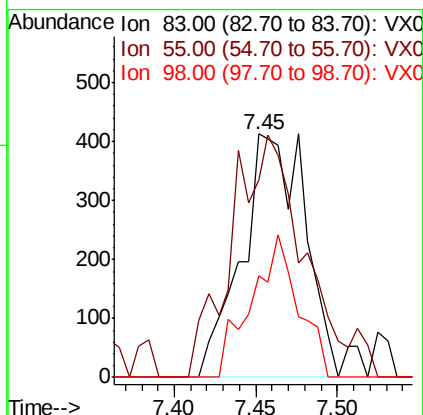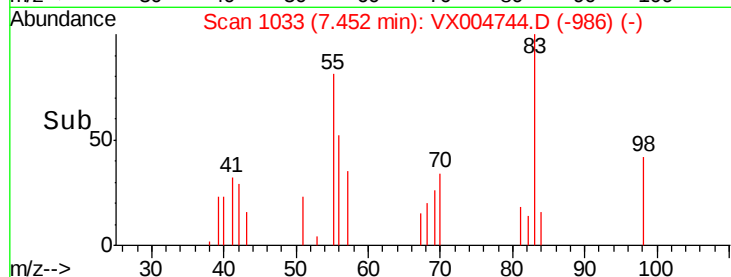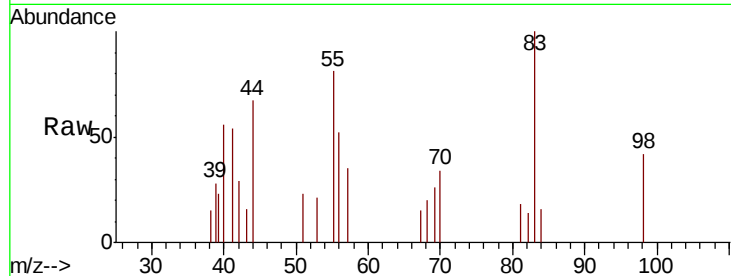

#50
Toluene-d8
Concen: 49.807 ug/l
RT: 8.72 min Scan# 1241
Delta R.T. 0.00 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion: 98 Resp: 584328
Ion Ratio Lower Upper
98 100
100 63.9 52.9 79.3

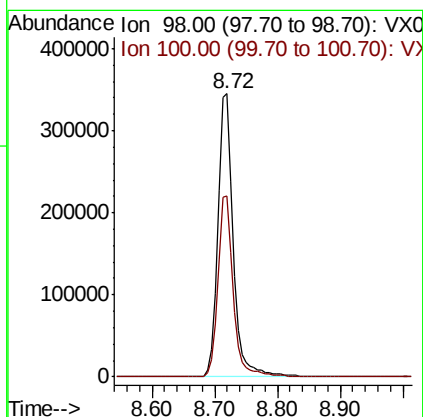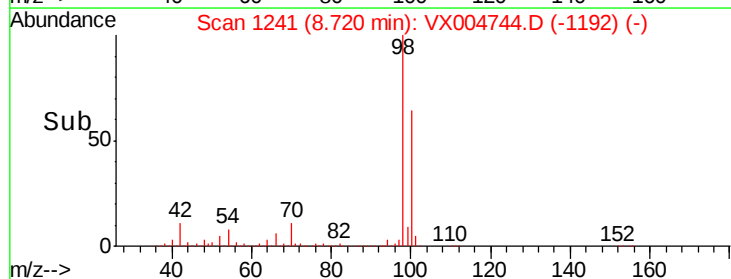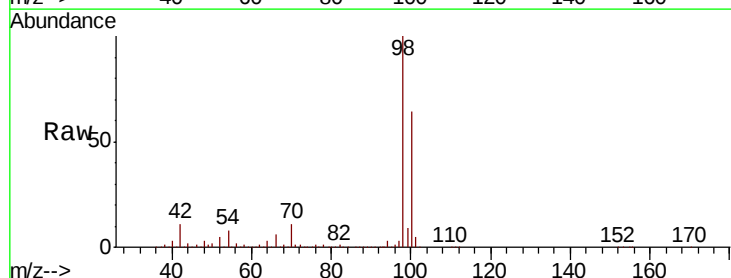

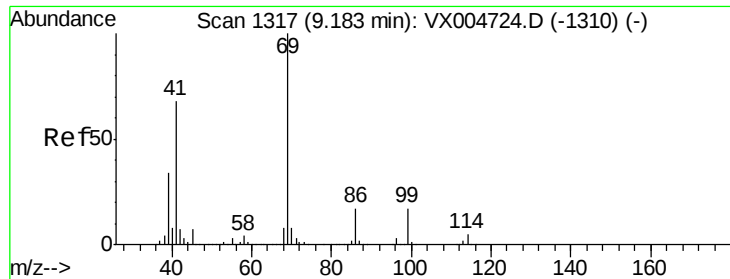

#56

Ethyl methacrylate

Concen: 2.869 ug/l

RT: 9.21 min Scan# 1322

Delta R.T. 0.03 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :

600-WILSON-AVE-NEWARK


Tot Ion: 69 Resp: 44

Ion Ratio Lower Upper

69 100

41 0.0 51.0 76.4#




39 384.1 26.1 39.1#

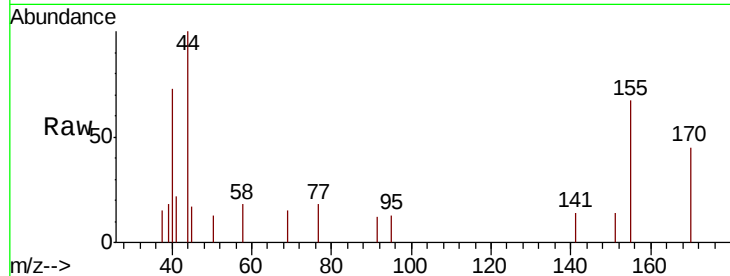

Abundance Ion 69.00 (68.70 to 69.70): VX0

Ion 41.00 (40.70 to 41.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

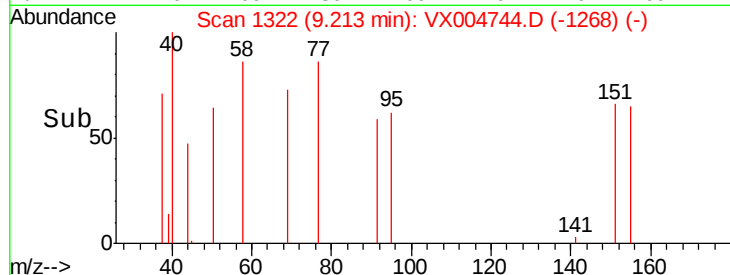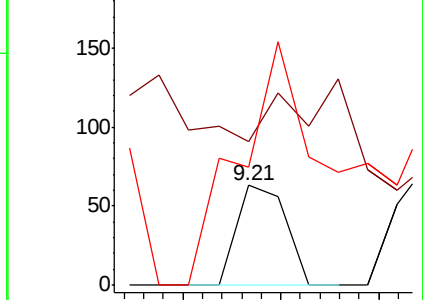

#58

2-Chloroethyl Vinyl ether

Concen: 14.266 ug/l

RT: 8.32 min Scan# 1176

Delta R.T. 0.01 min

Lab File: VX004744.D


Acq: 27 Sep 2018 01:04

Tgt Ion: 63 Resp: 80

Ion Ratio Lower Upper



63 100


106 0.0 23.9 35.9#



Abundance Ion 62.90 (62.60 to 63.60): VX0

Ion 105.90 (105.60 to 106.60): V



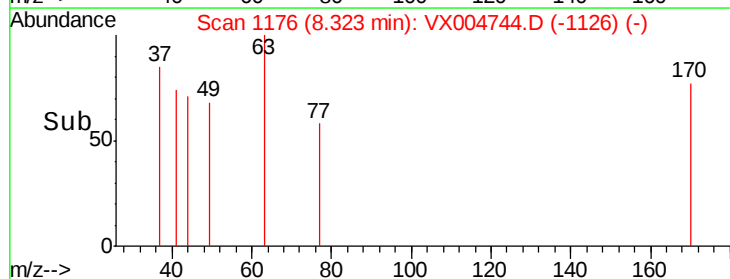
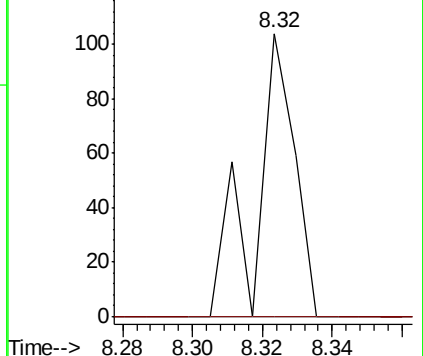




#62
4-Bromofluorobenzene
Concen: 52.009 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.00 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04




Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK


Tot Ion: 95 Resp: 219814
Ion Ratio Lower Upper
95 100
174 91.1 0.0 185.2
176 87.6 0.0 178.6

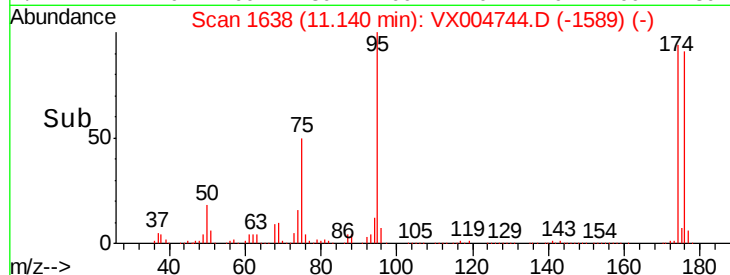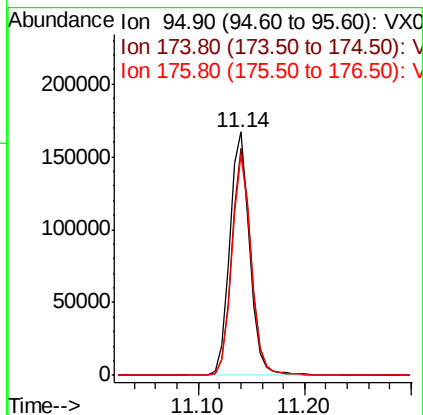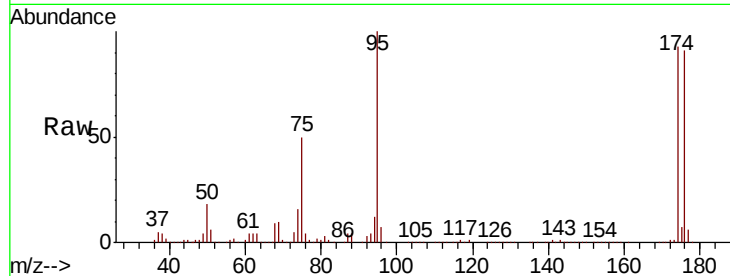

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion: 117 Resp: 396698
Ion Ratio Lower Upper
117 100
82 55.6 47.8 71.6
119 32.6 29.3 43.9



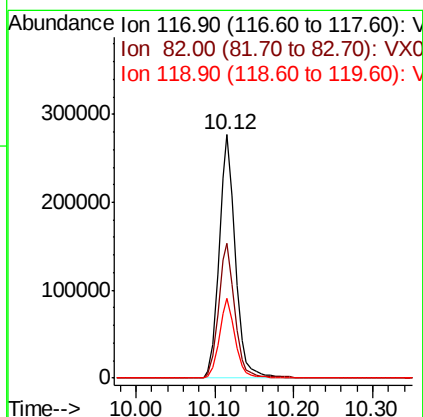
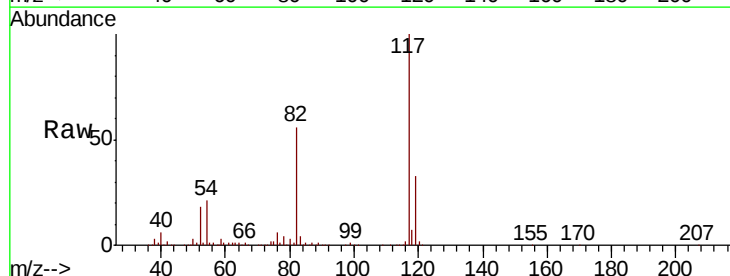


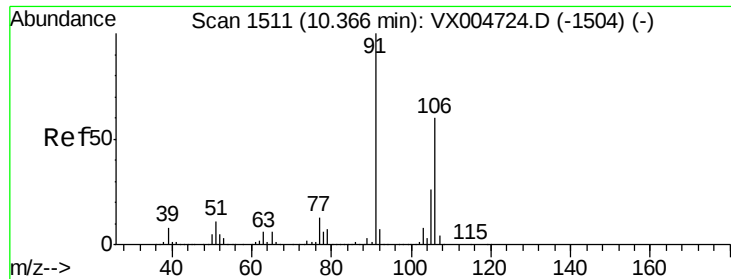

#68
m/p-Xvlenes
Concen: 0.266 ug/l
RT: 10.36 min Scan# 1510
Delta R.T. -0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04




Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK


Tot Ion:106 Resp: 1676
Ion Ratio Lower Upper
106 100
91 202.5 157.1 235.7

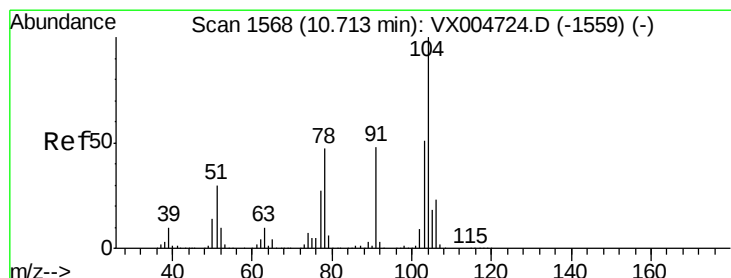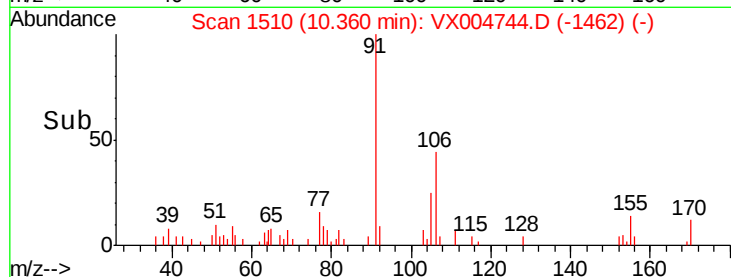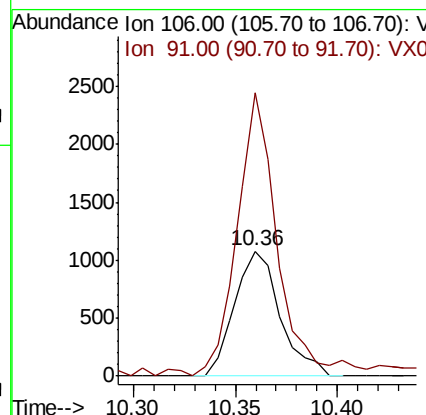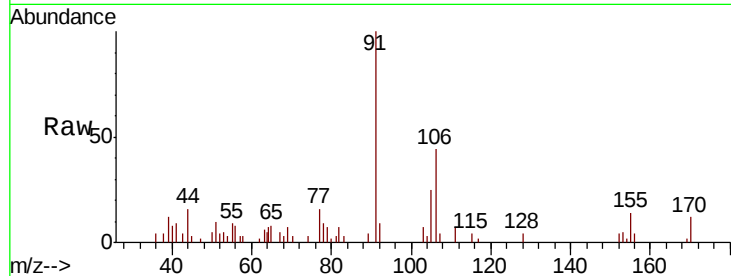

#70
Styrene
Concen: 2.172 ug/l
RT: 10.72 min Scan# 1569
Delta R.T. 0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion:104 Resp: 352
Ion Ratio Lower Upper
104 100
78 68.5 37.4 56.0#
103 45.7 43.8 65.6

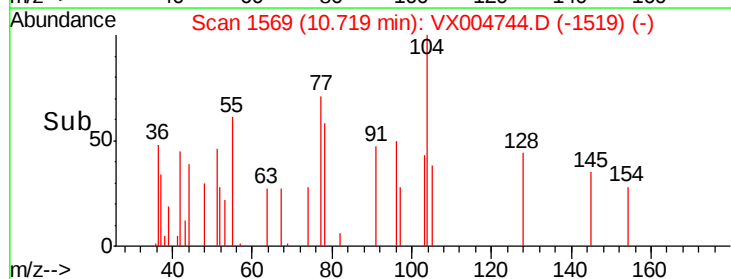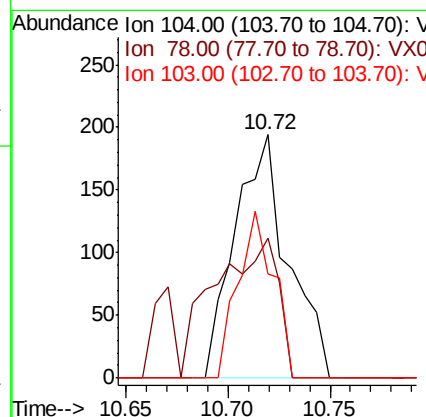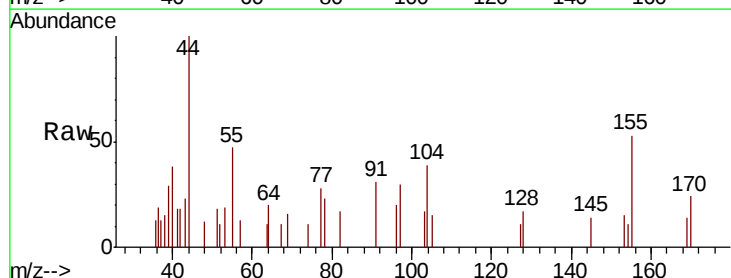

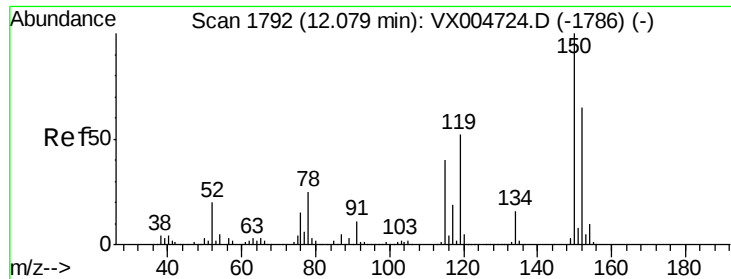

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :

600-WILSON-AVE-NEWARK


Tot Ion:152 Resp: 233866

Ion Ratio Lower Upper

152 100

115 55.2 39.0 117.0




150 155.8 0.0 351.0

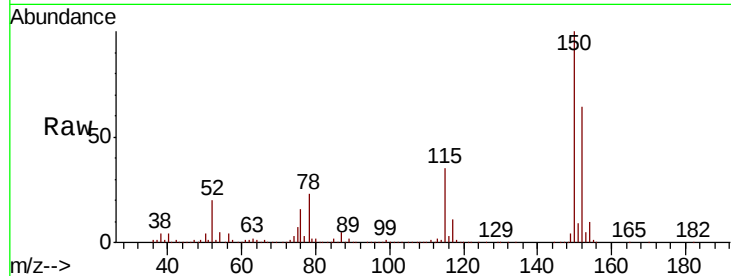

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

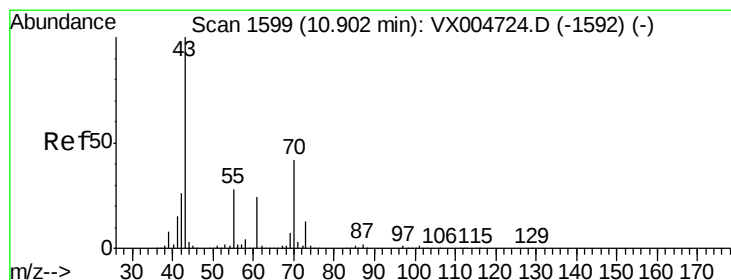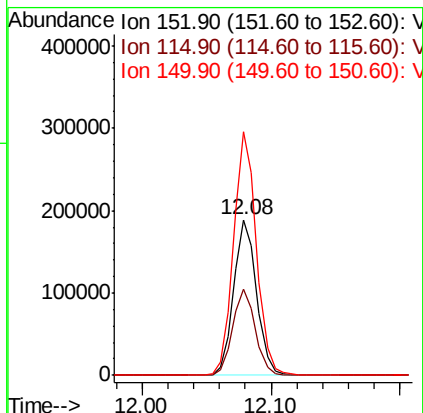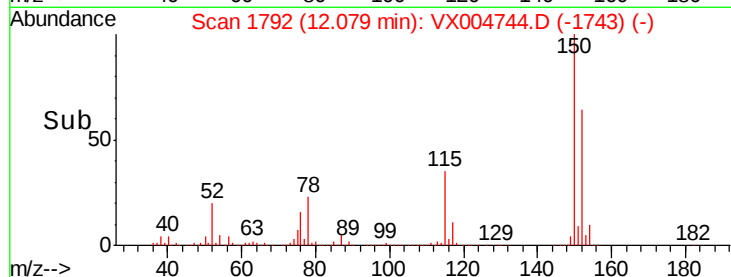

#74

N-ethyl acetate

Concen: 1.766 ug/l

RT: 10.91 min Scan# 1601

Delta R.T. 0.01 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Tgt Ion: 43 Resp: 155


Ion Ratio Lower Upper

43 100

70 58.1 37.4 56.0#

55 452.9 21.8 32.8#

61 0.0 20.6 30.8#


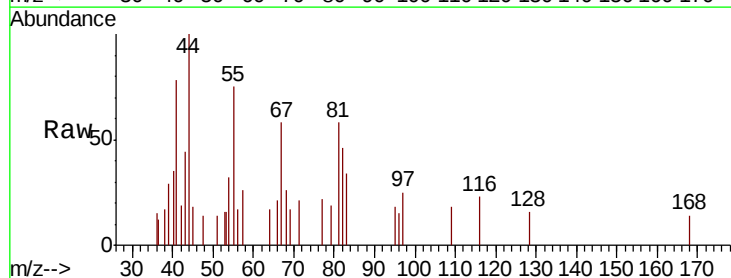



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 70.00 (69.70 to 70.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

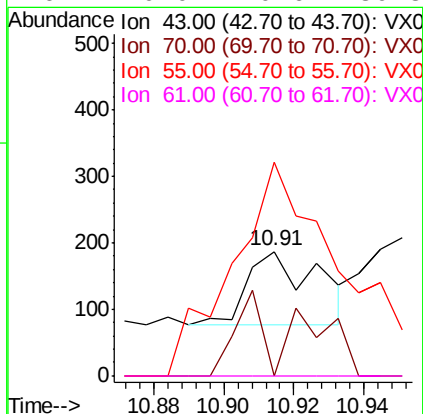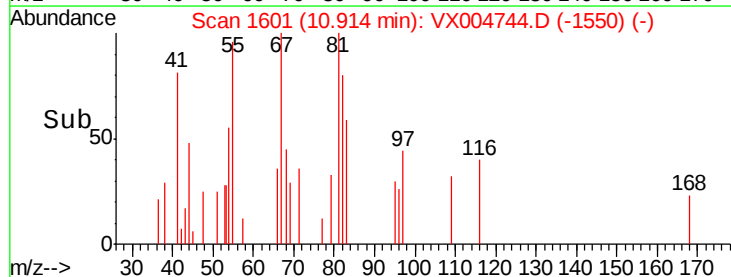

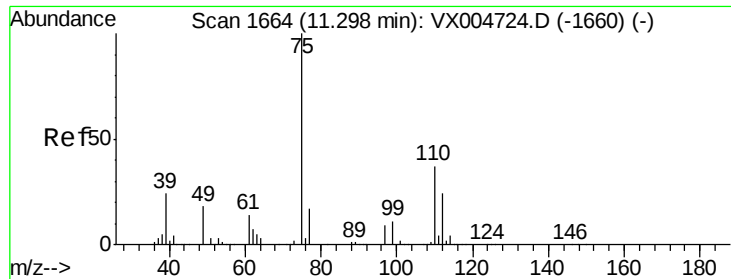

#76

1,2,3-Trichloropropane

Concen: 20.825 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. -0.16 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04

Instrument :

MSVOA_X

ClientSampleId :


600-WILSON-AVE-NEWARK

Tot Ion: 75 Resp: 109158

Ion Ratio Lower Upper




75 100

77 1.4 20.2 60.6#

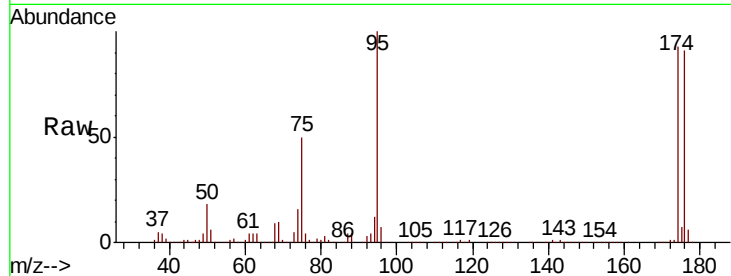

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

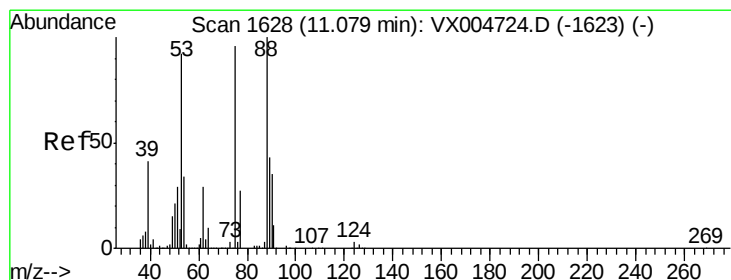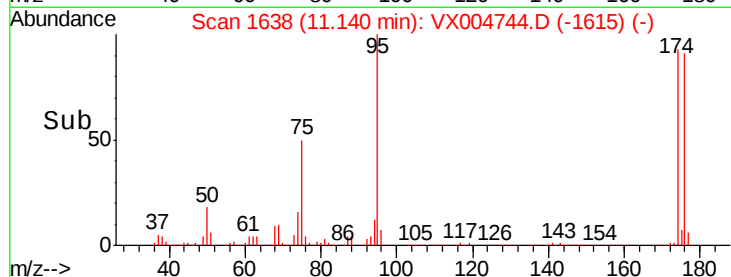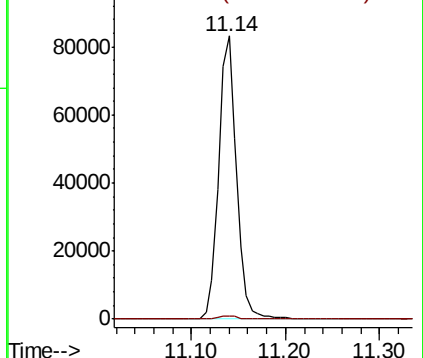

#81

trans-1,4-Dichloro-2-butene

Concen: 56.526 ug/l

RT: 11.14 min Scan# 1638

Delta R.T. 0.06 min

Lab File: VX004744.D

Acq: 27 Sep 2018 01:04


Tgt Ion: 75 Resp: 109158

Ion Ratio Lower Upper

75 100

53 0.2 80.1 120.1#



89 0.0 37.2 55.8#

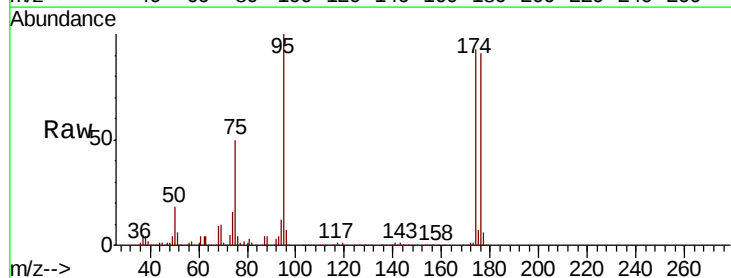


Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0



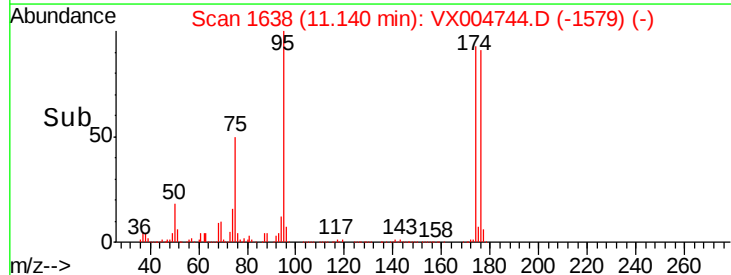
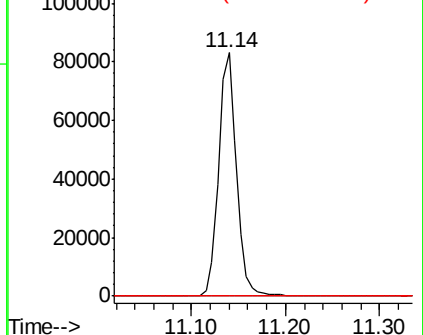




#83
tert-Butylbenzene
Concen: 0.363 ug/l
RT: 11.77 min Scan# 1741
Delta R.T. -0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04




Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK


Tot Ion:119 Resp: 4405
Ion Ratio Lower Upper
119 100
91 76.8 27.0 81.0
134 26.2 11.7 35.1

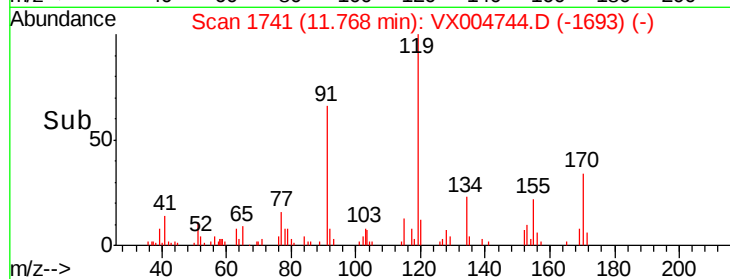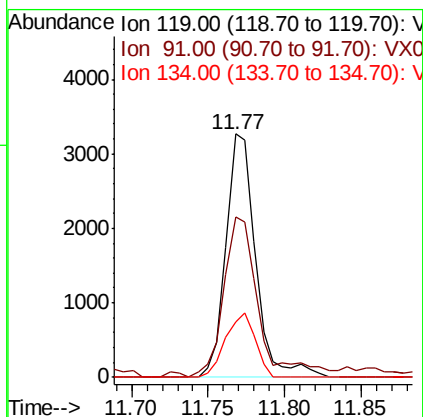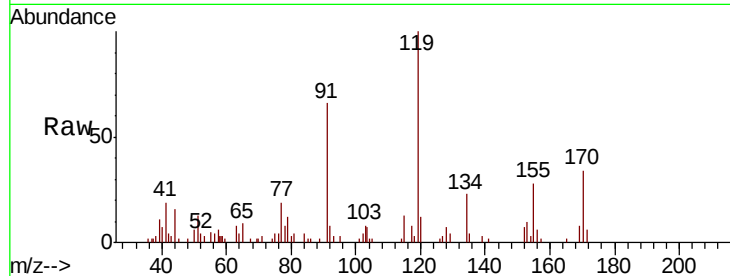

#85
sec-Butylbenzene
Concen: 0.220 ug/l
RT: 11.94 min Scan# 1770
Delta R.T. -0.01 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion:105 Resp: 3257
Ion Ratio Lower Upper
105 100
134 83.1 10.5 31.5#

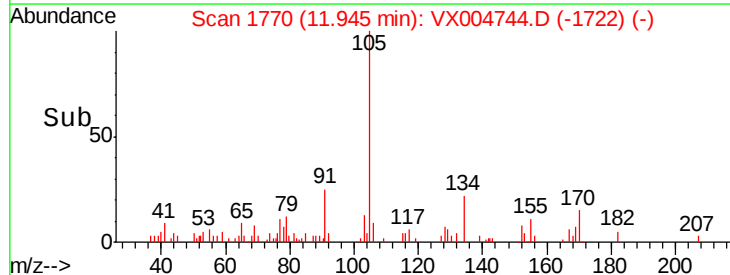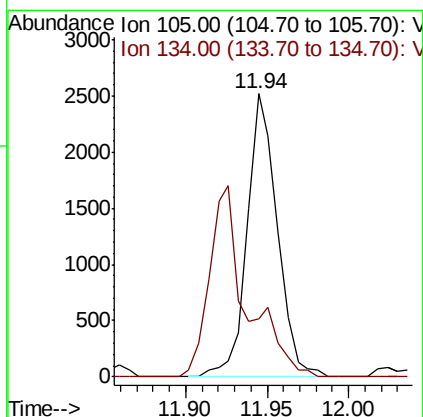


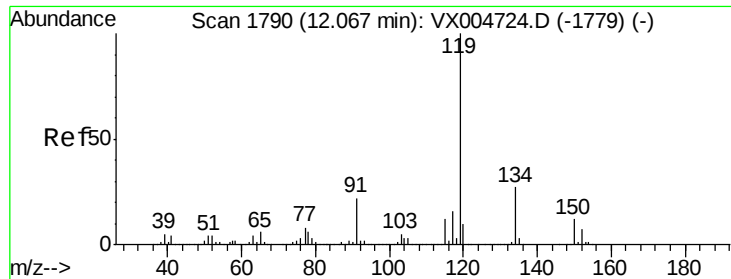




#86
p-Isopropyltoluene
Concen: 0.471 ug/l
RT: 12.23 min Scan# 1817
Delta R.T. 0.16 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK

Tot Ion:119 Resp: 6305
Ion Ratio Lower Upper
119 100
134 27.7 13.4 40.2
91 30.6 10.9 32.7

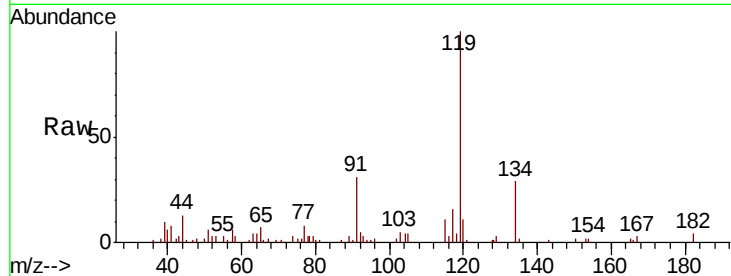


Abundance Ion 119.00 (118.70 to 119.70): V
Ion 134.00 (133.70 to 134.70): V
Ion 91.00 (90.70 to 91.70): V

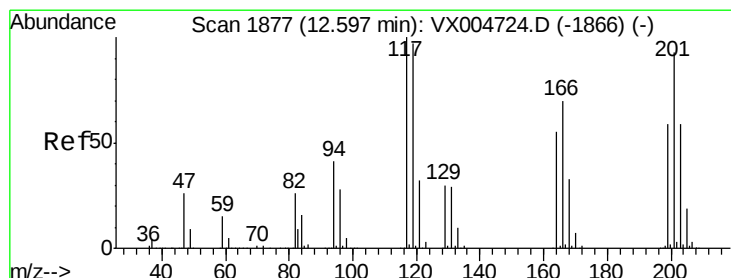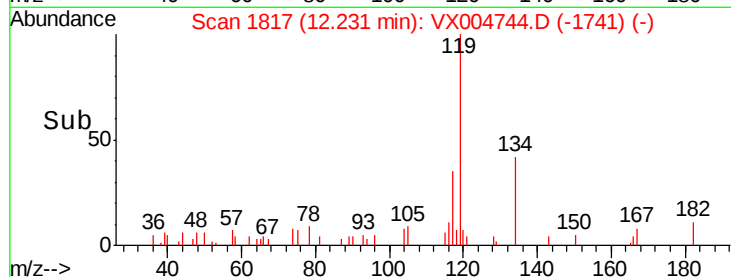
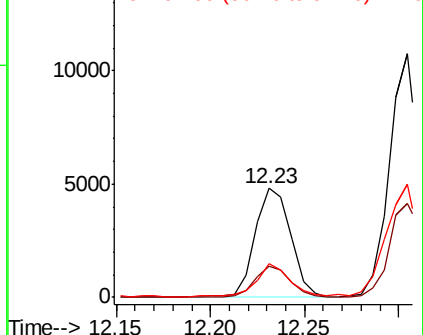



#90
Hexachloroethane
Concen: 1.072 ug/l
RT: 12.67 min Scan# 1889
Delta R.T. 0.07 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Tgt Ion:117 Resp: 2391
Ion Ratio Lower Upper
117 100
201 0.0 46.9 140.6#

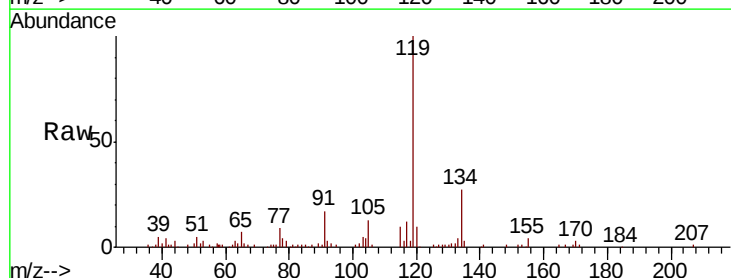

Abundance Ion 116.80 (116.50 to 117.50): V
Ion 200.70 (200.40 to 201.40): V

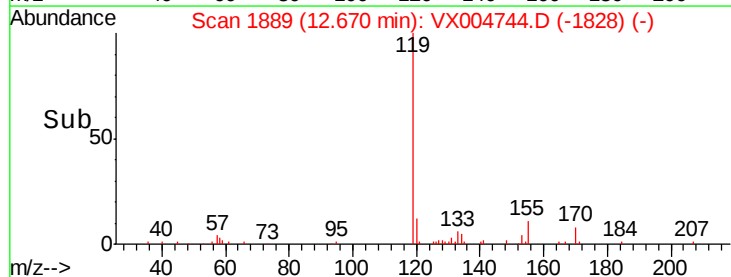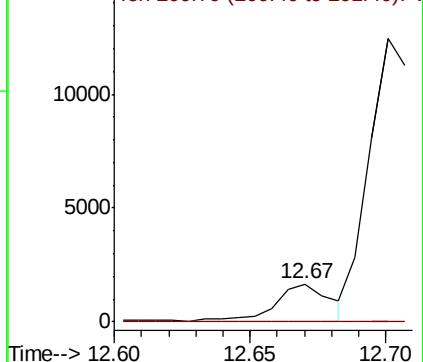

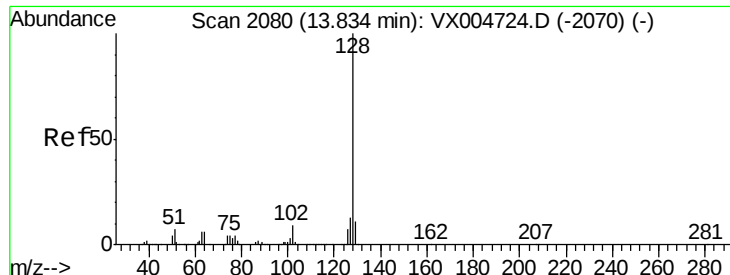

#95
Naphthalene
Concen: 1.480 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX004744.D
Acq: 27 Sep 2018 01:04

Instrument :
MSVOA_X
ClientSampleId :
600-WILSON-AVE-NEWARK

Tot Ion	Ratio	Lower	Upper
128	100		
127	16.5	10.2	15.2#
129	13.4	8.6	12.8#

