



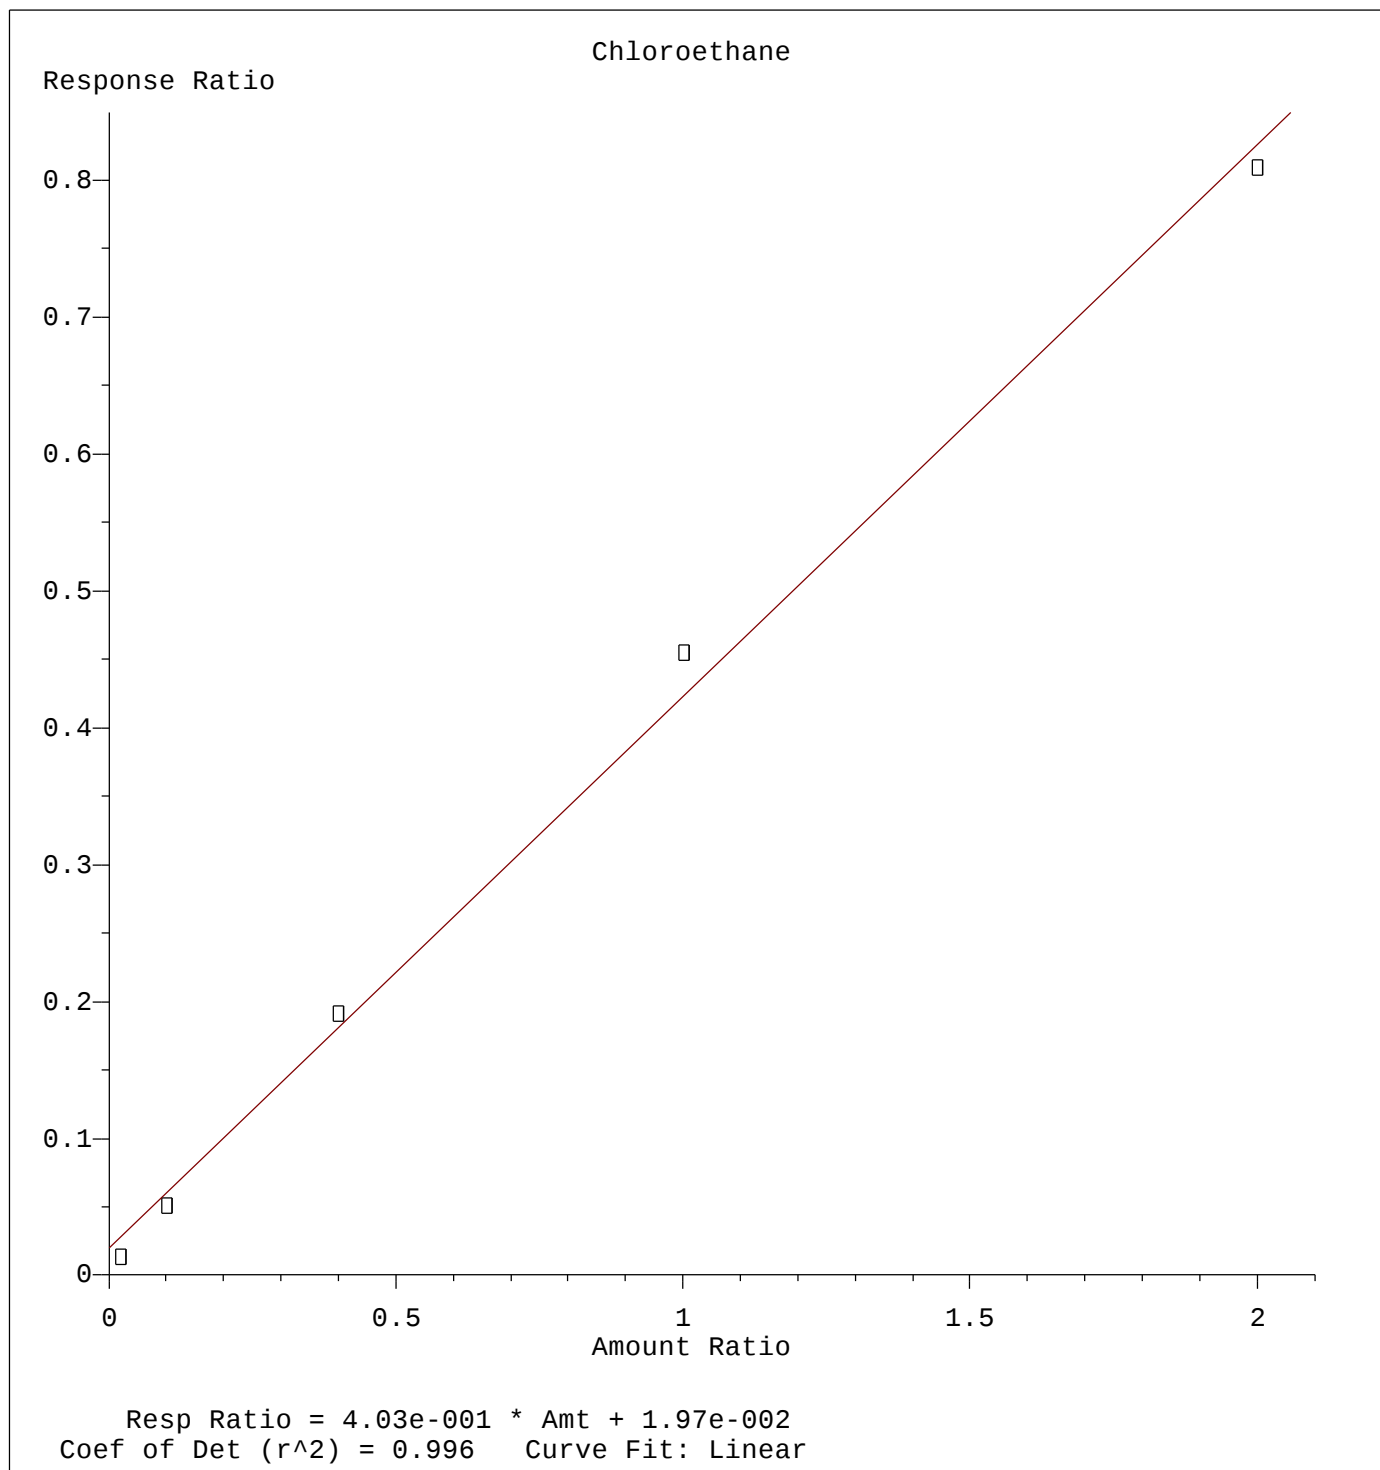


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

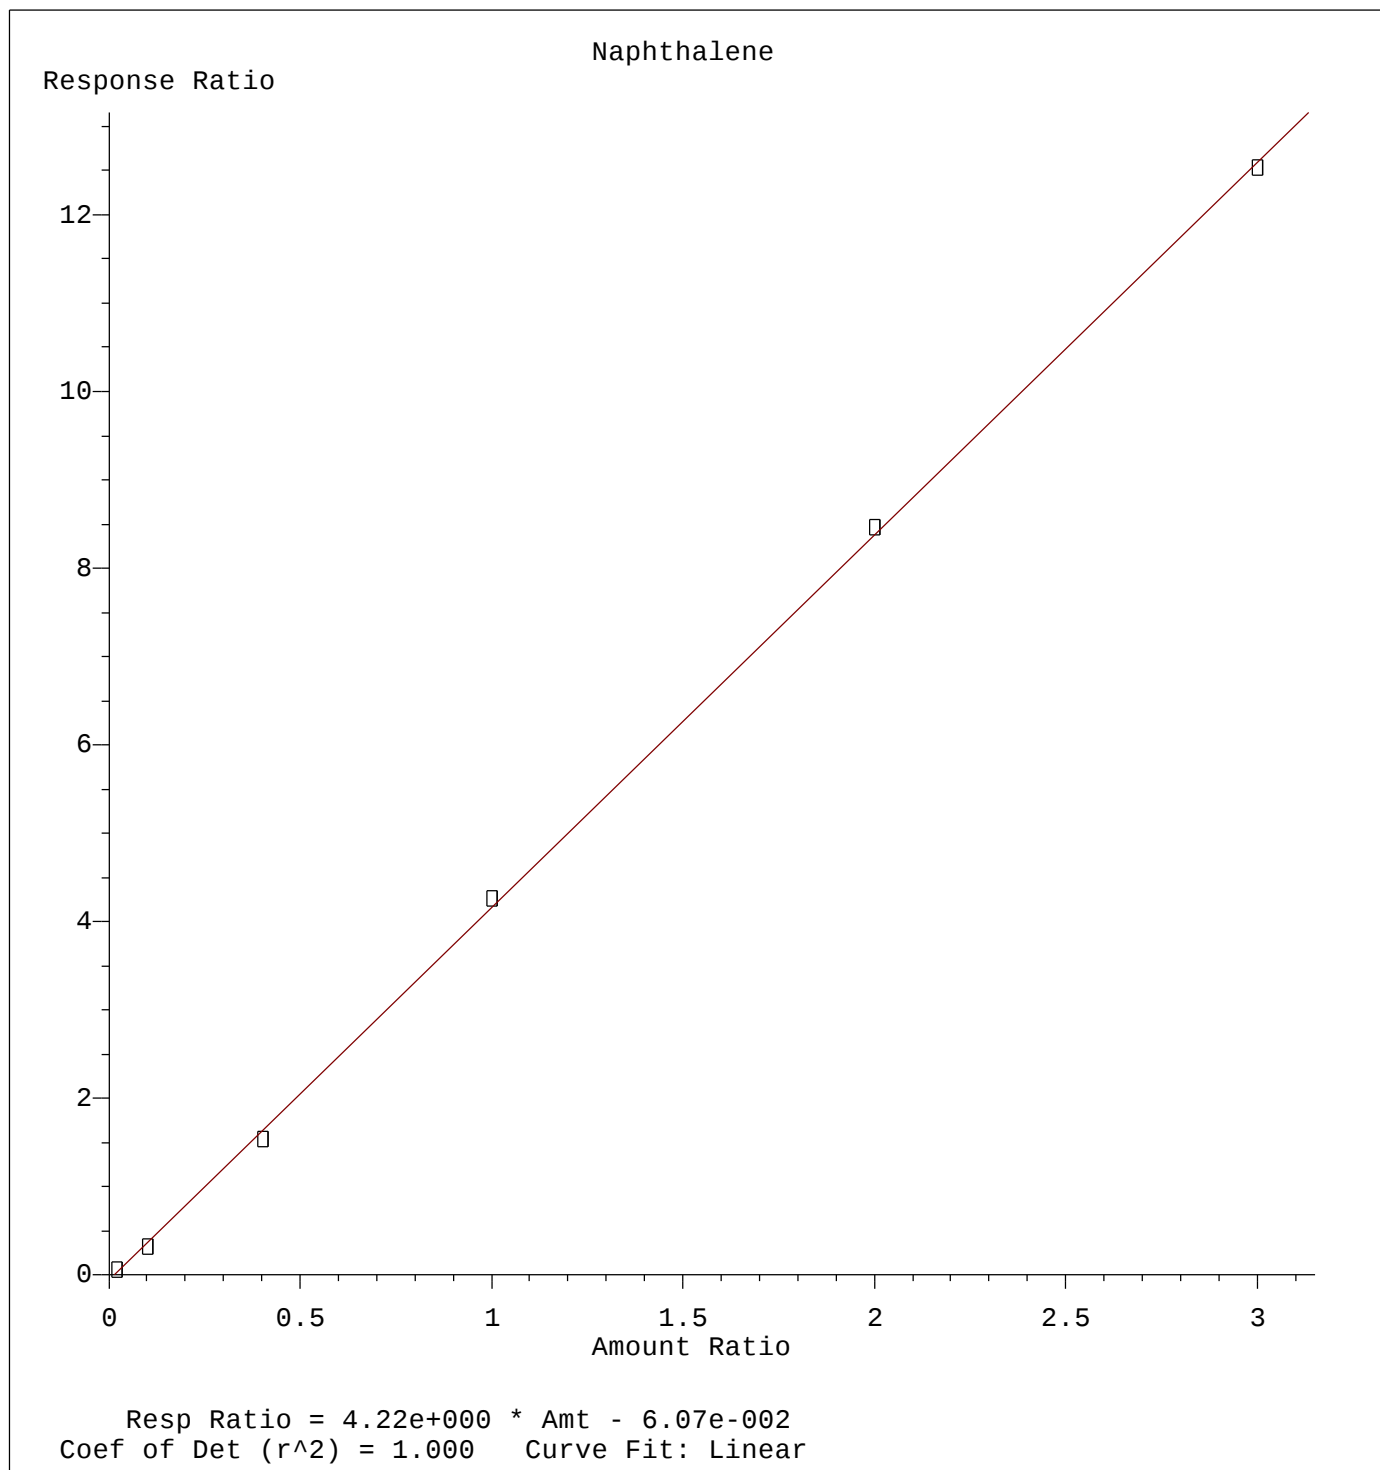

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

1,2,4-Trimethylbenzene

Response Ratio

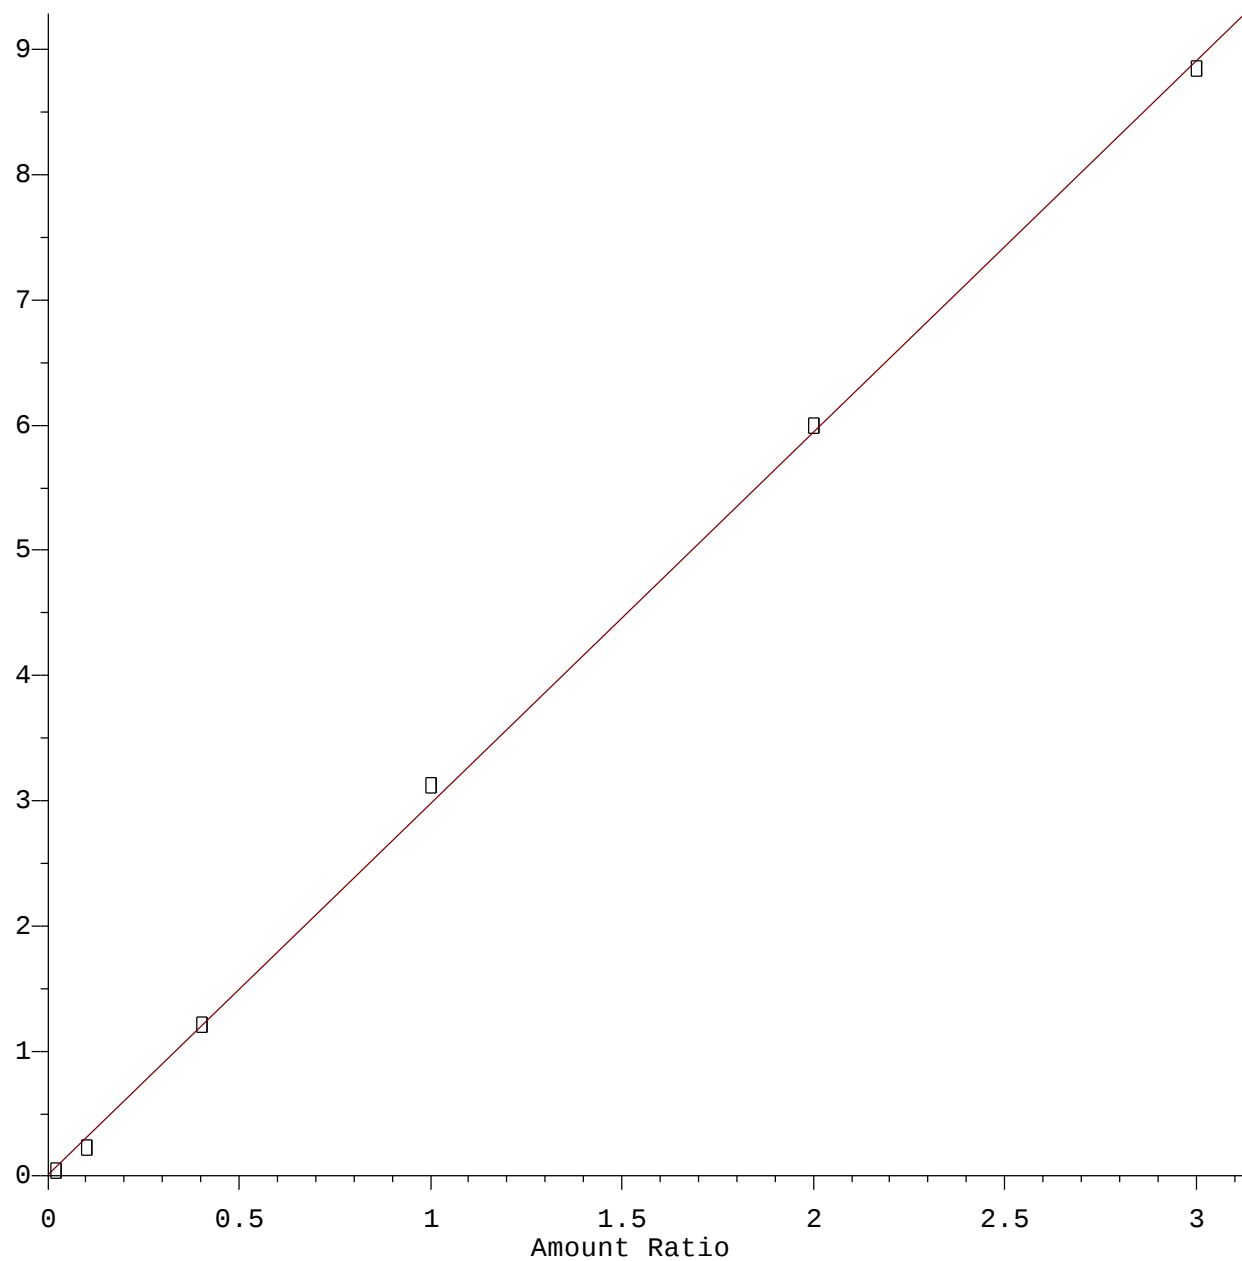


Resp Ratio = 2.97e+000 * Amt + 1.18e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

trans-1,4-Dichloro-2-butene

Response Ratio

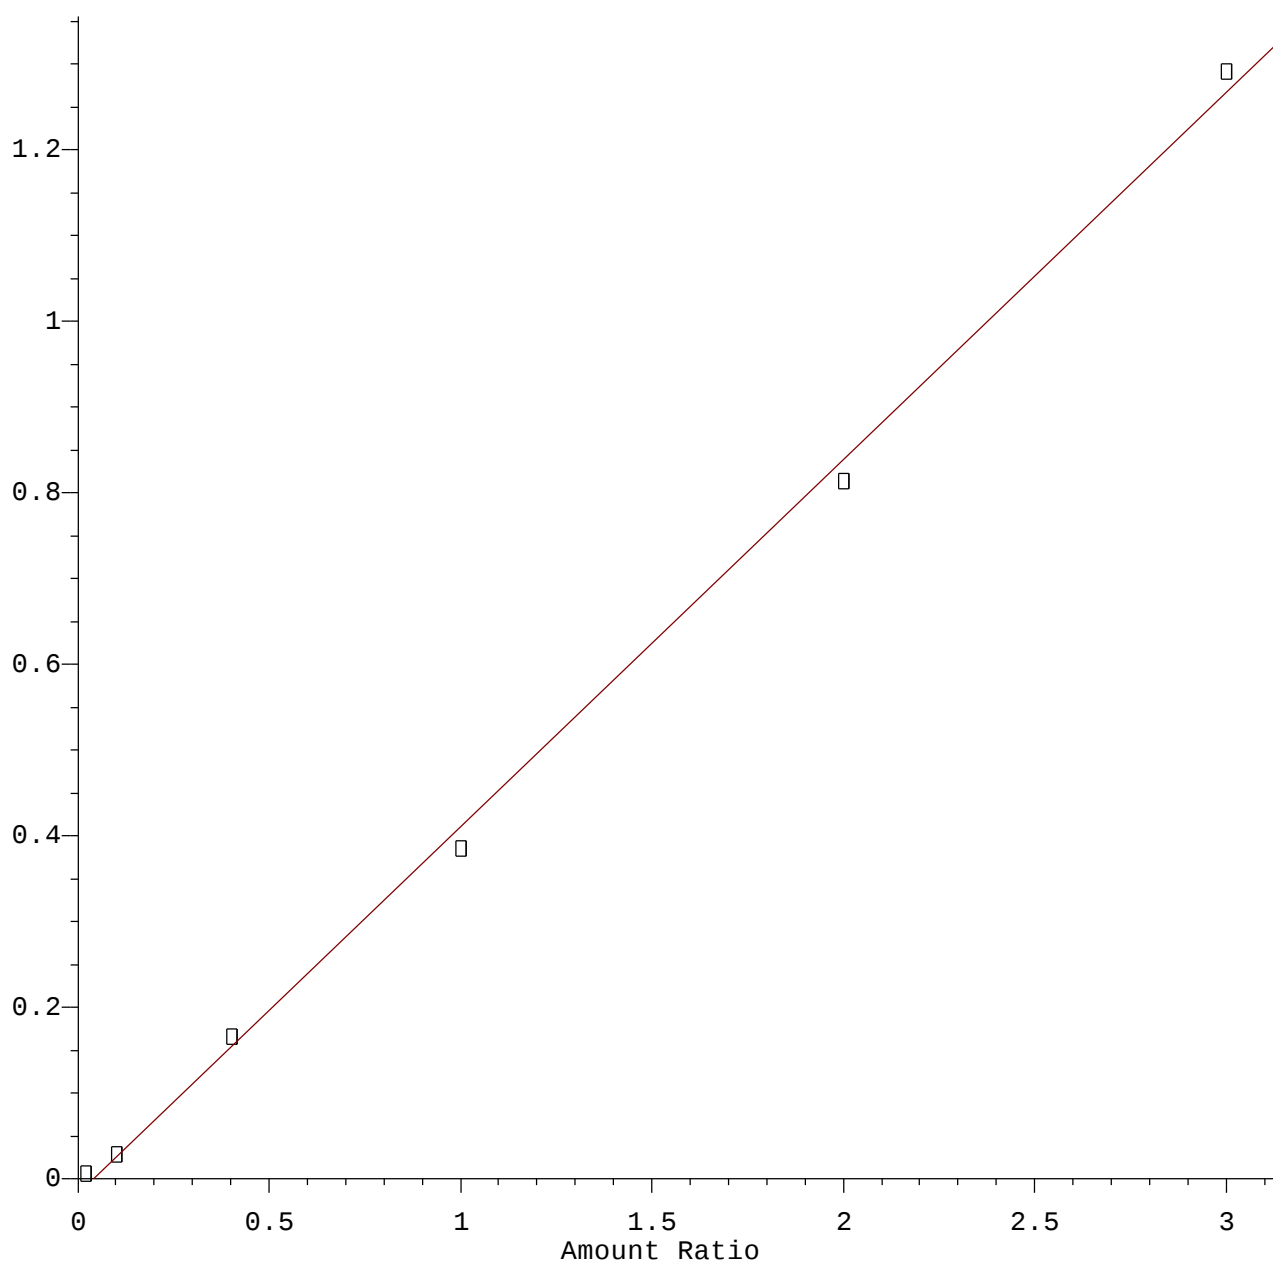


Resp Ratio = $4.28 \times 10^{-1} \times \text{Amt} - 1.70 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018


1,3,5-Trimethylbenzene

Response Ratio

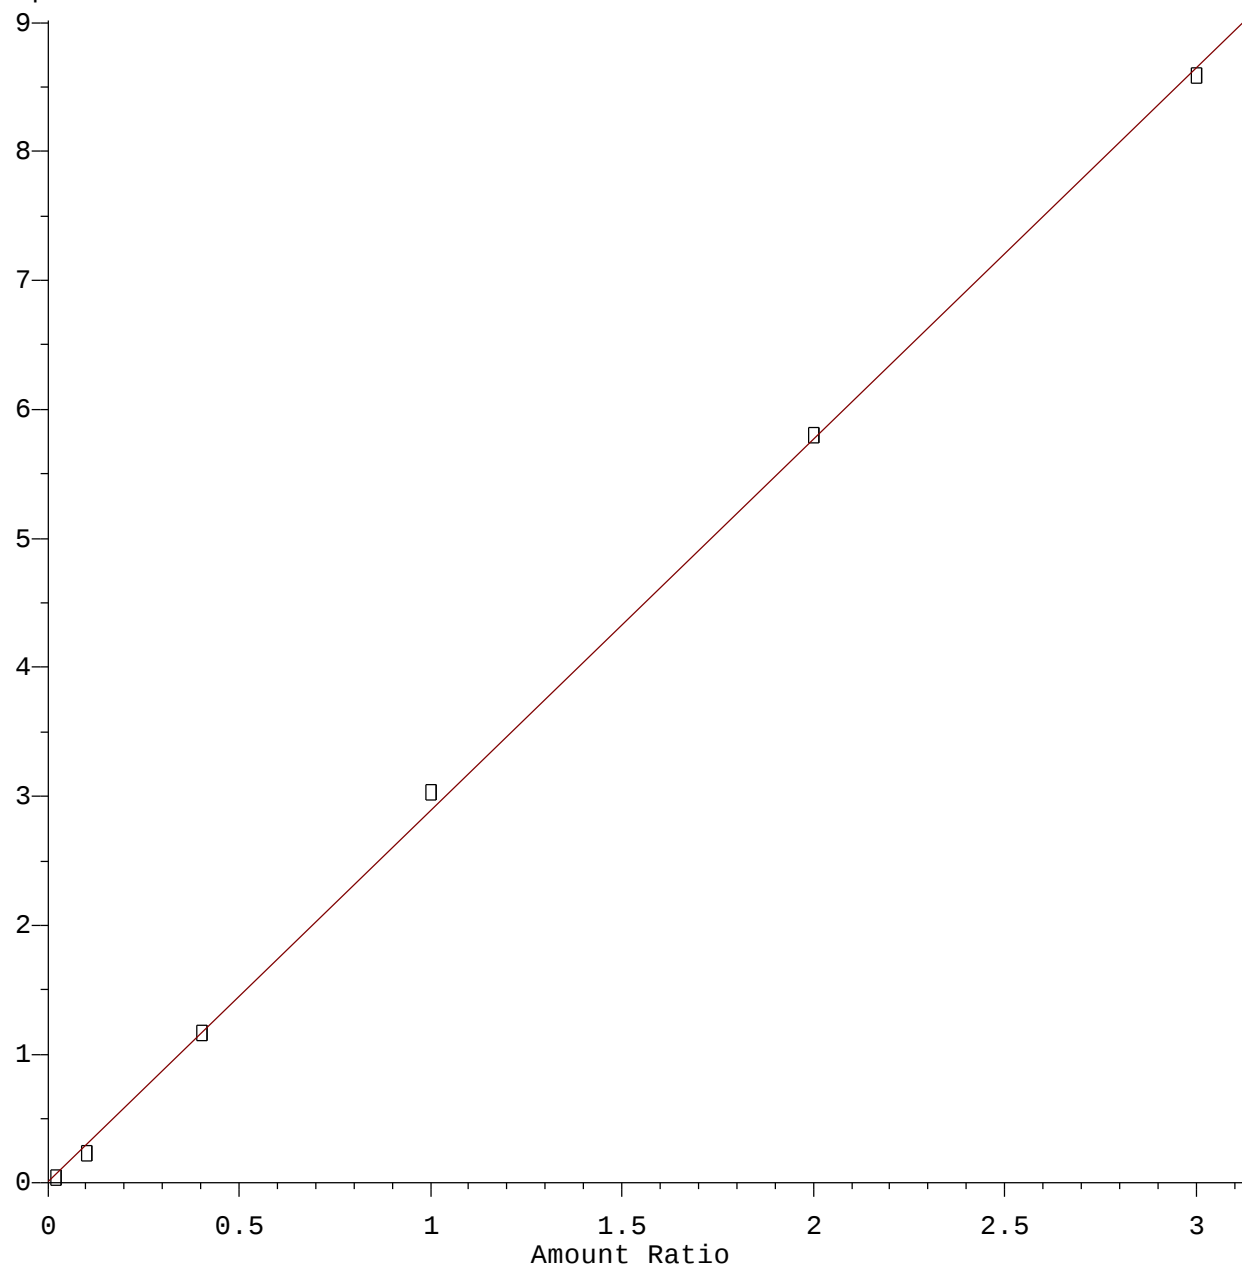


Resp Ratio = 2.88e+000 * Amt + 1.14e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

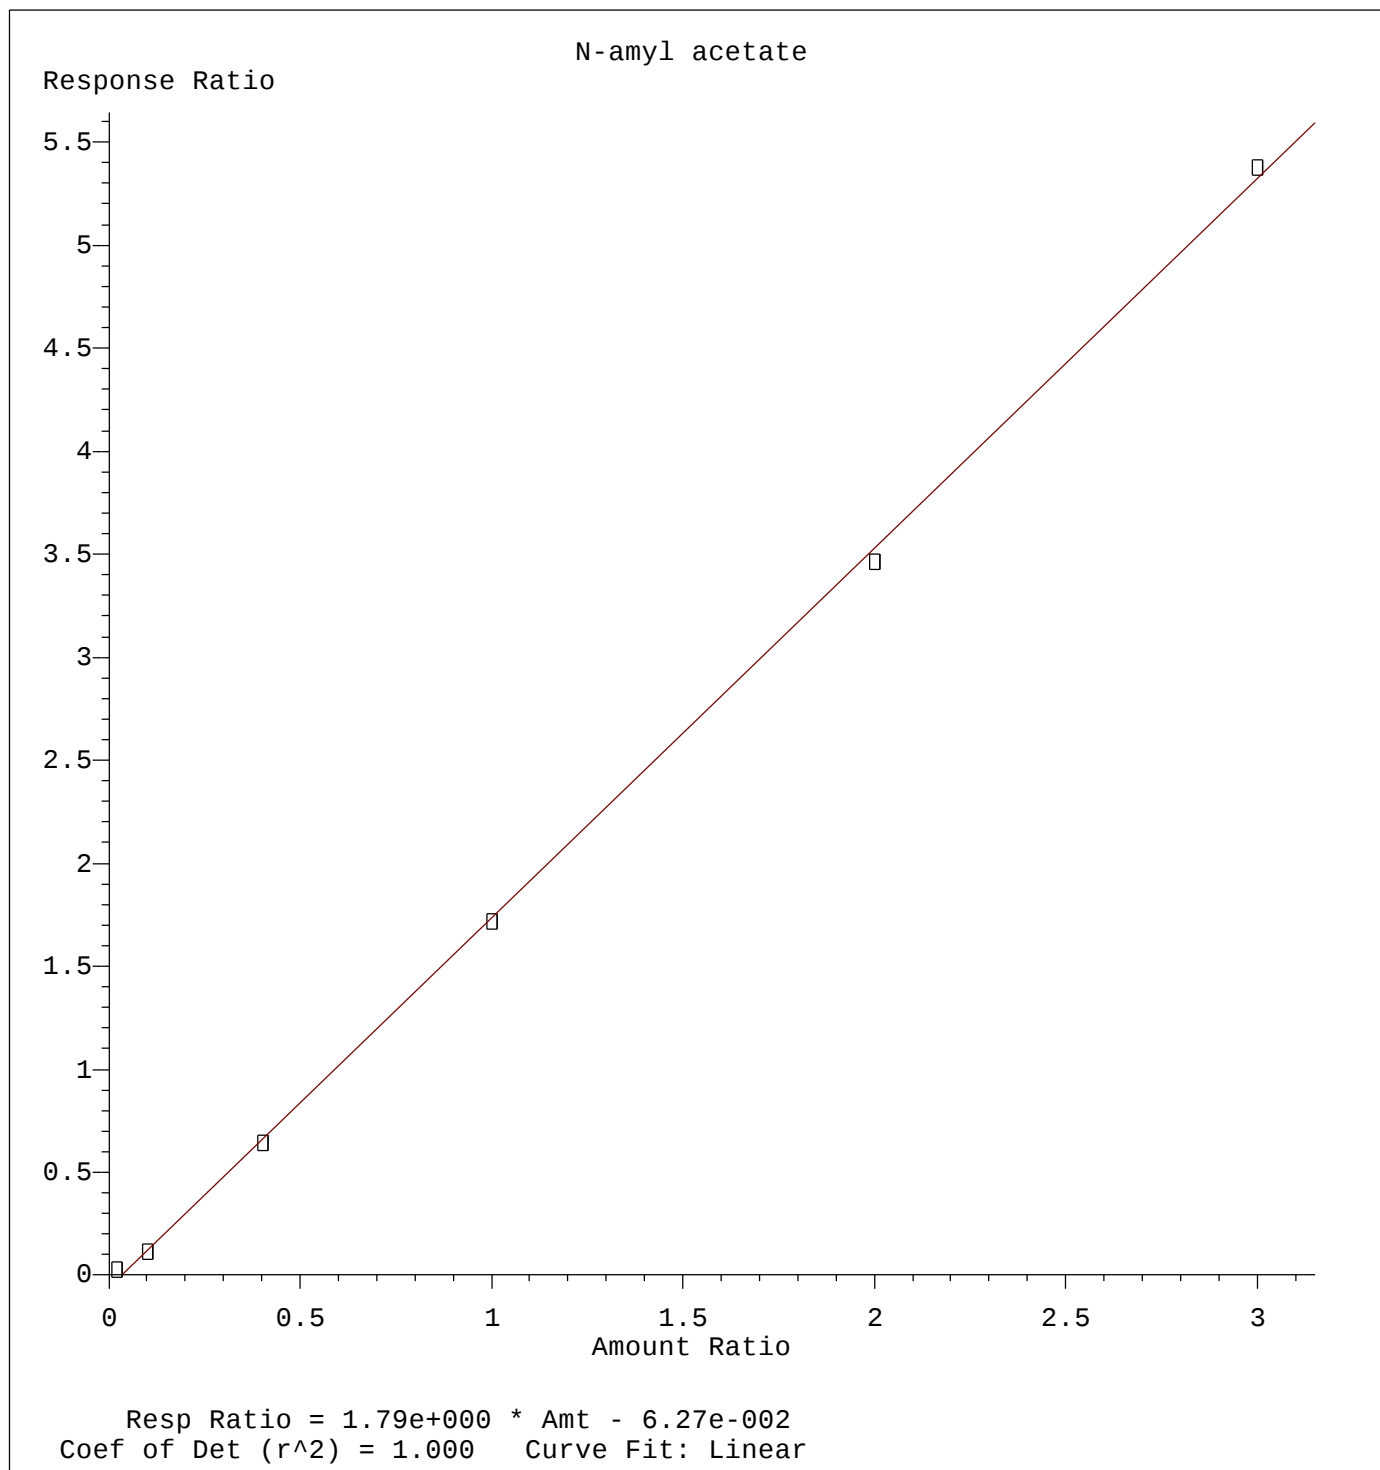


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

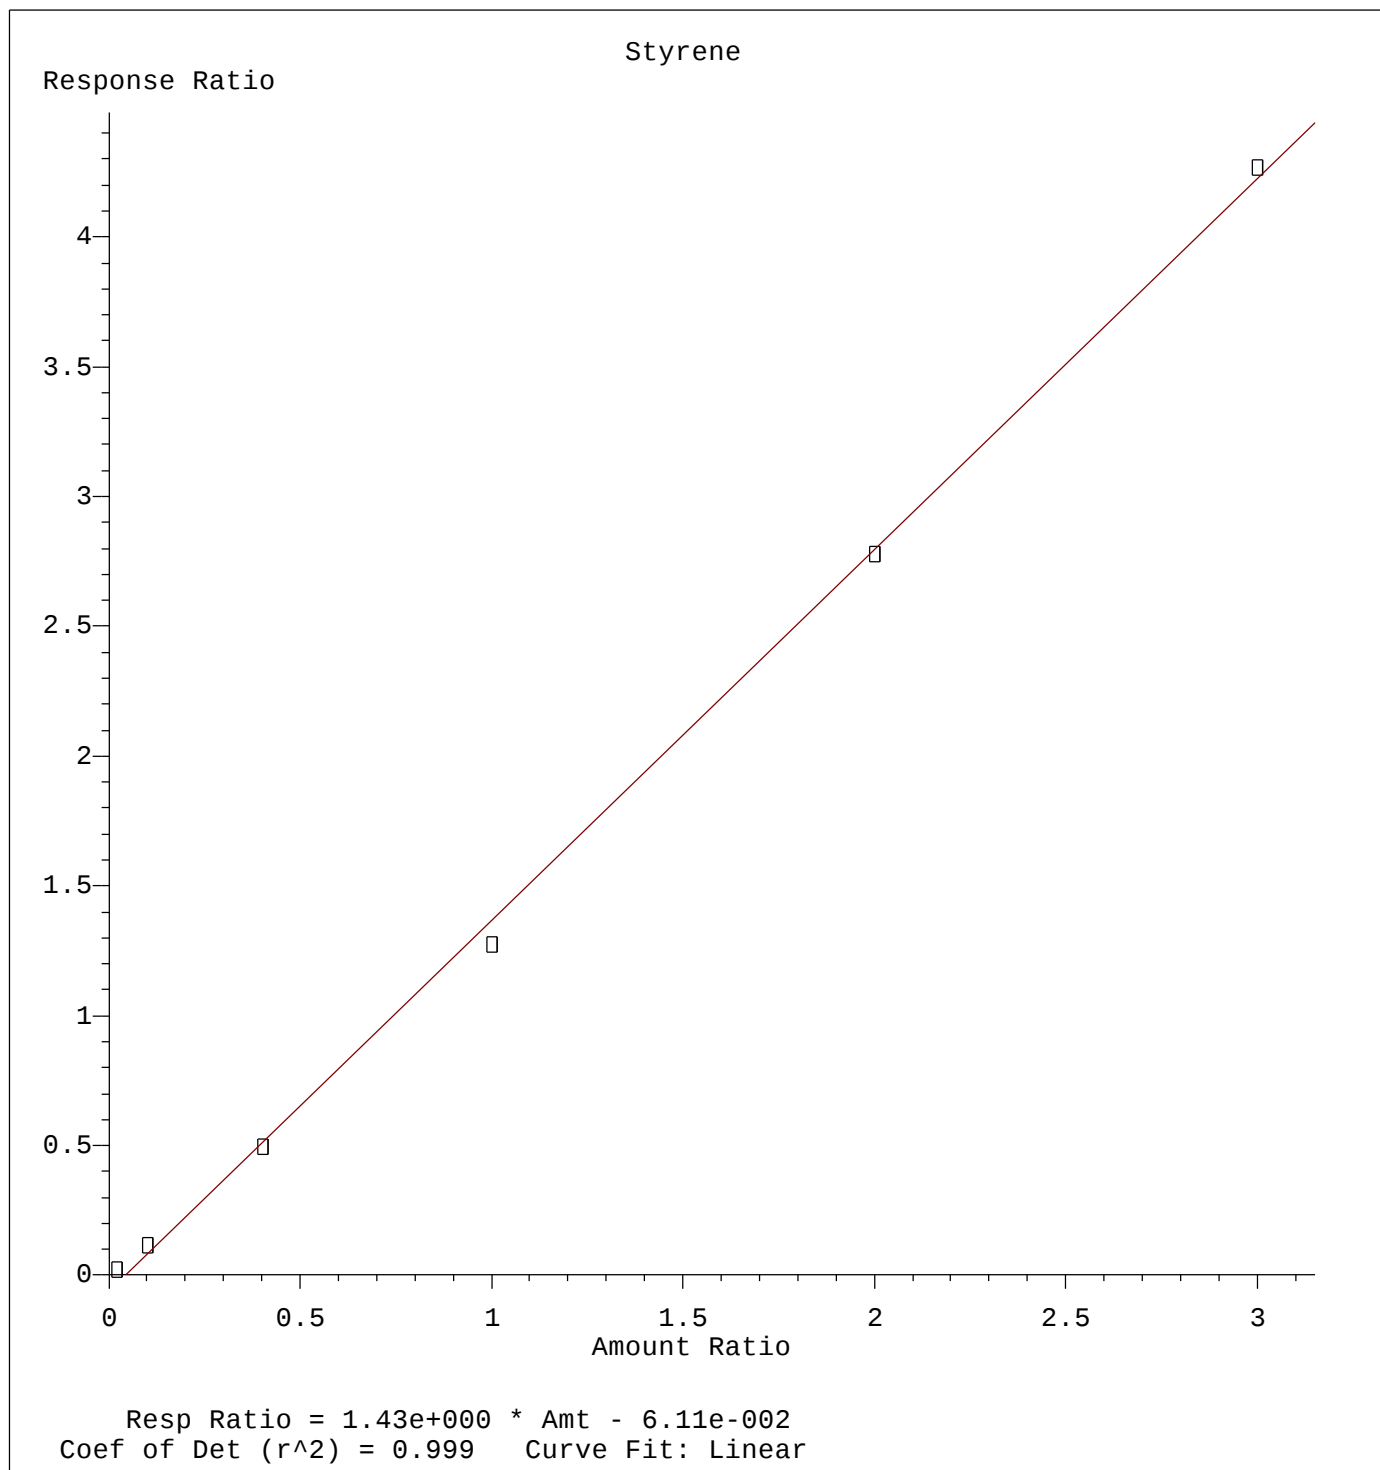

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018


2-Chloroethyl Vinyl ether

Response Ratio

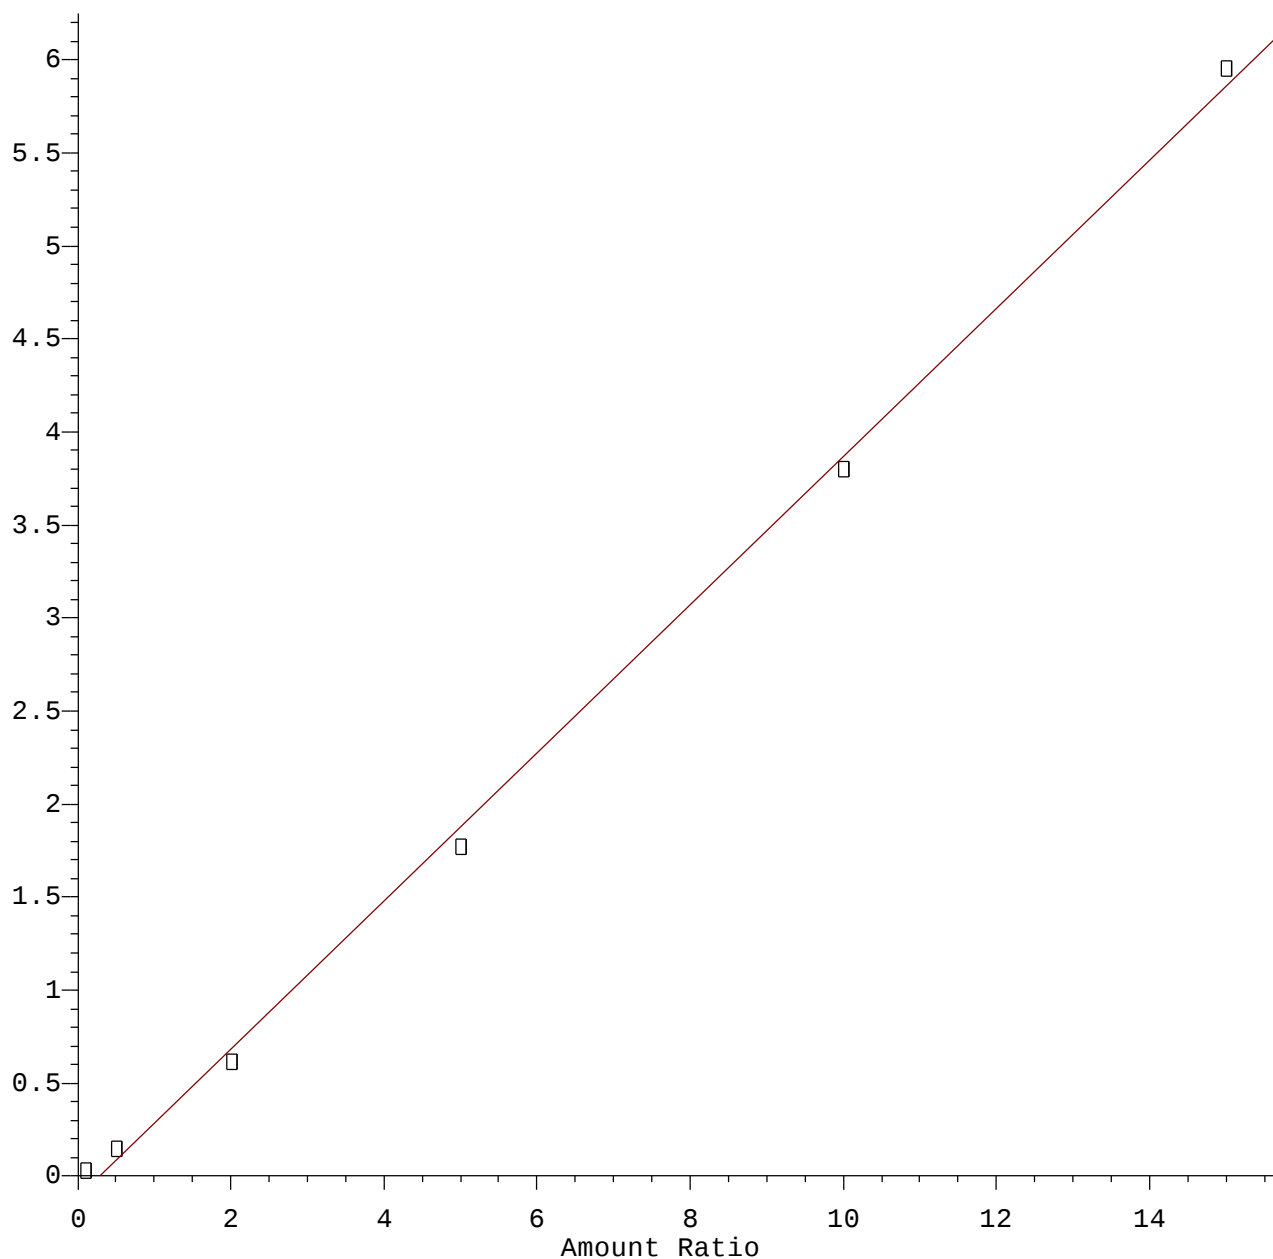

Resp Ratio = $3.98 \times 10^{-1} \times \text{Amt} - 1.13 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

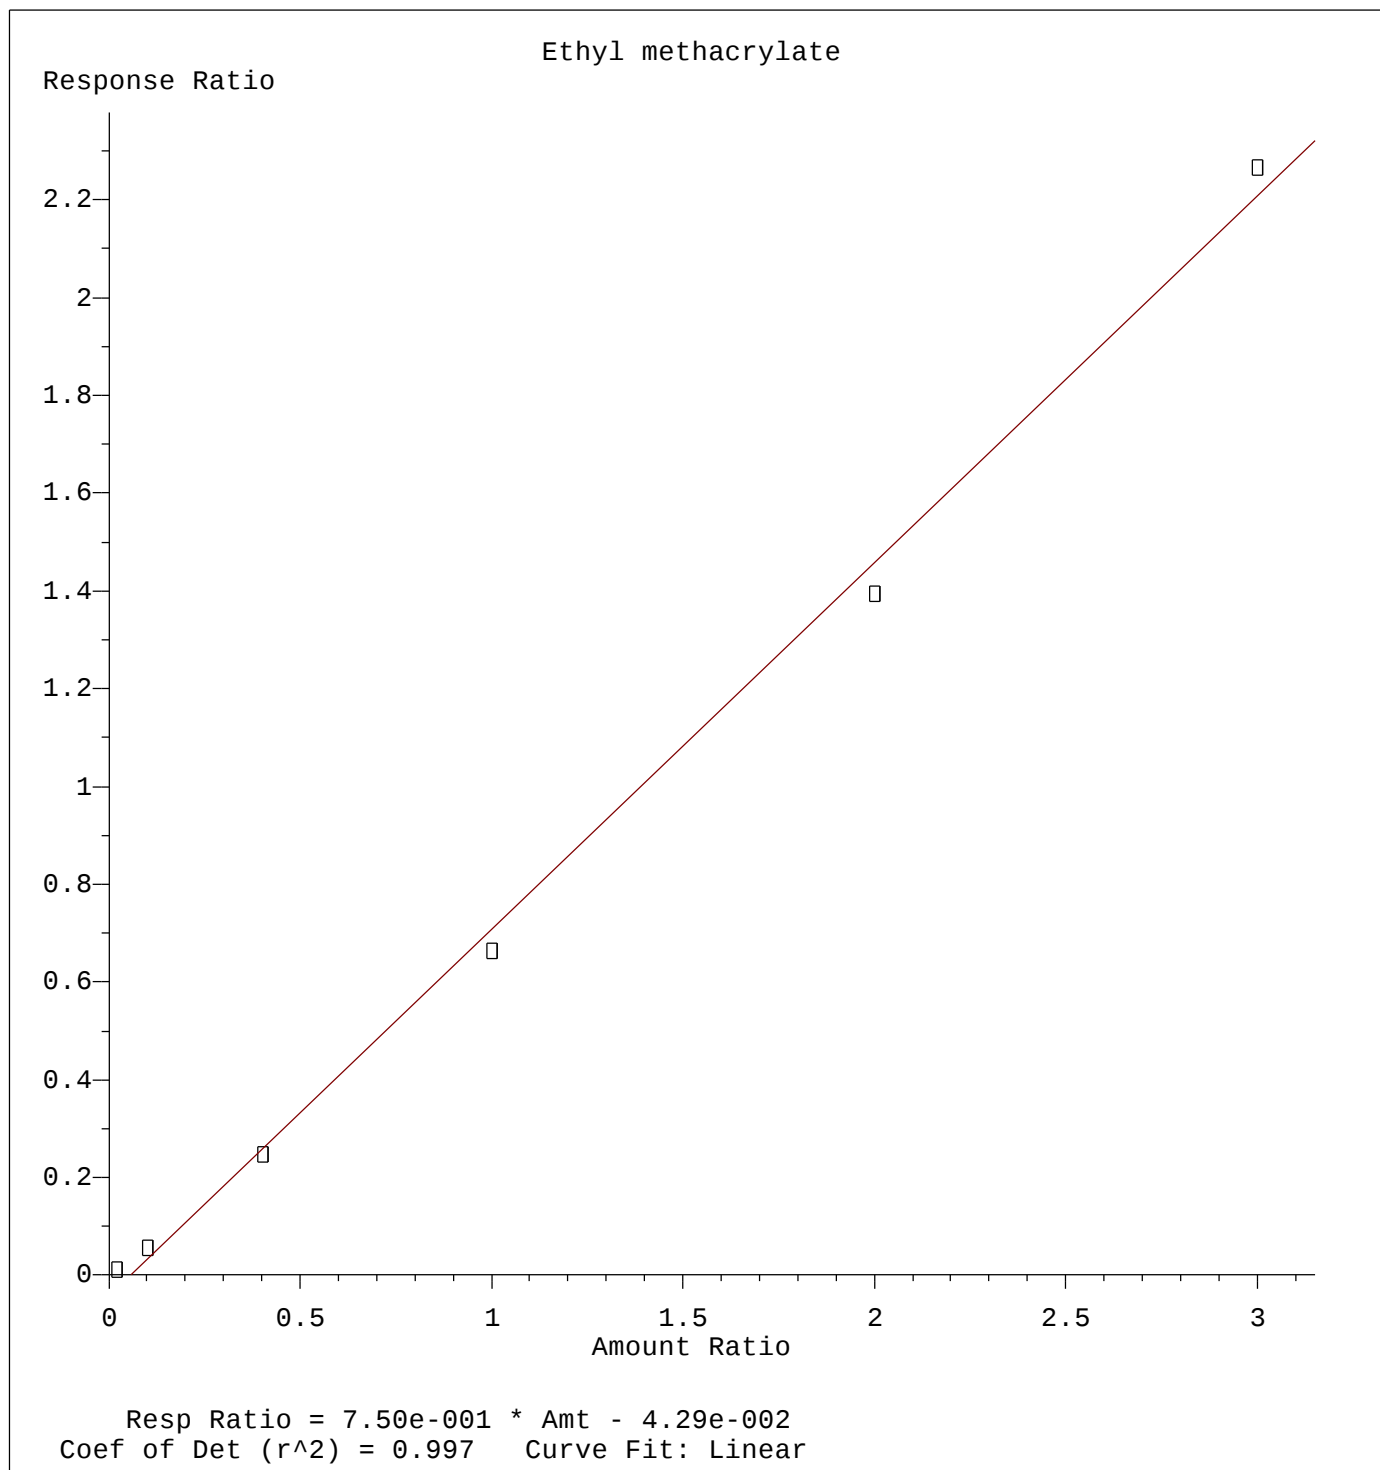

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018

Methylene Chloride

Response Ratio

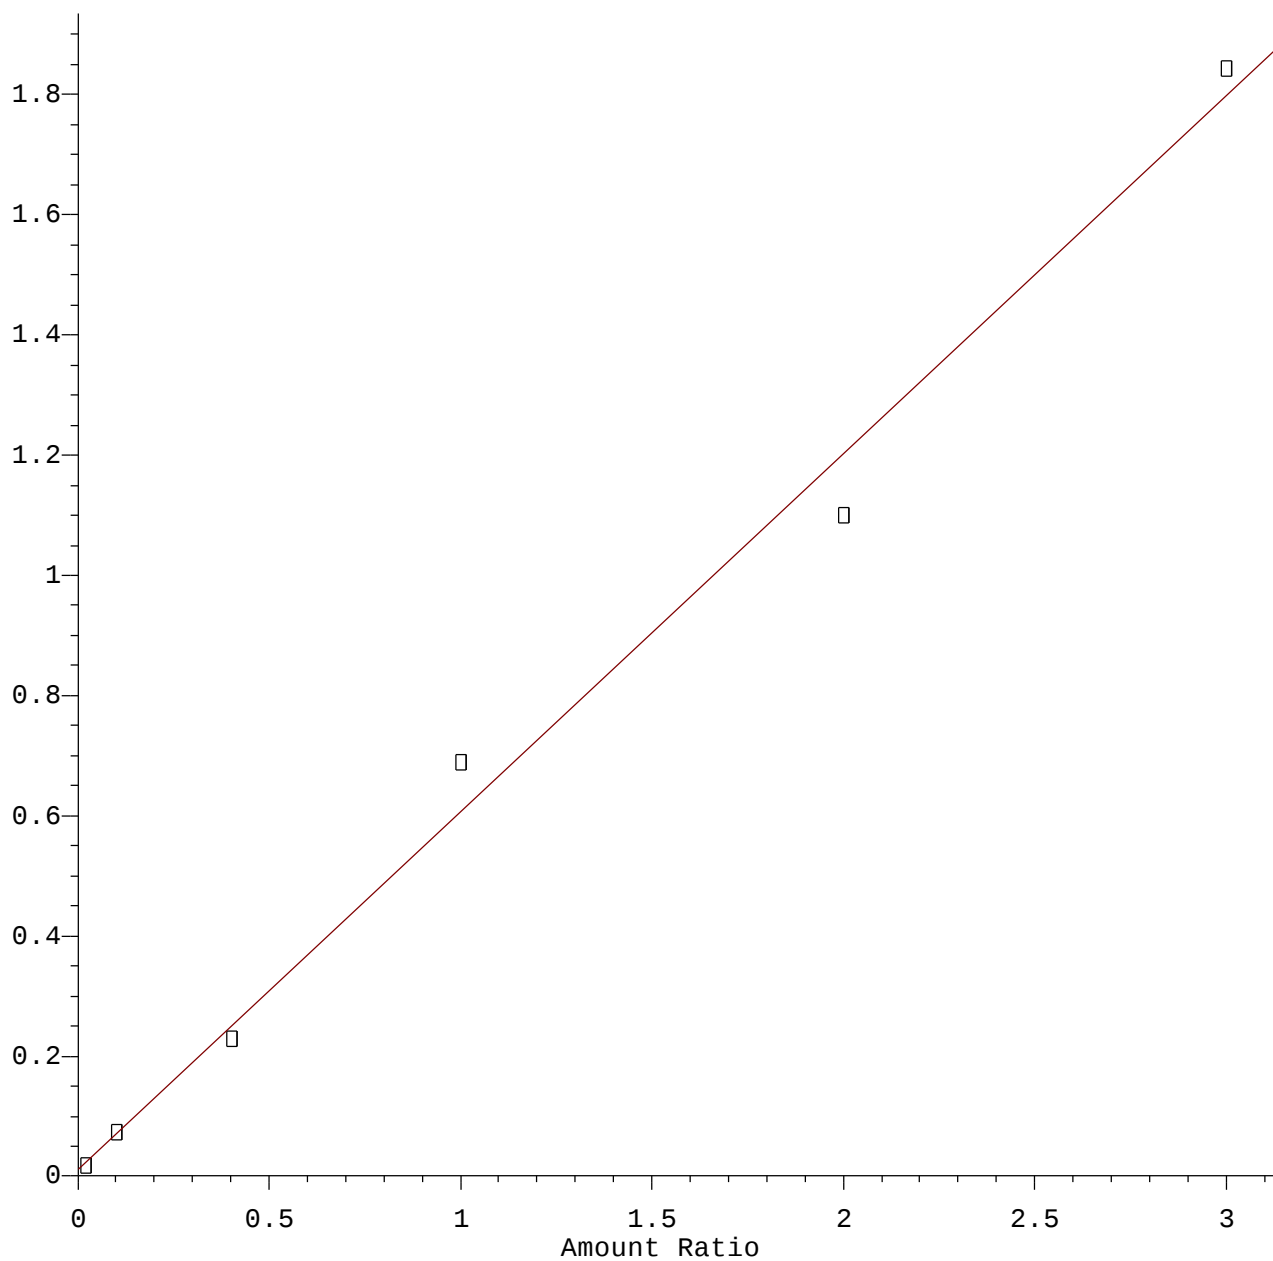

Resp Ratio = $5.96 \times 10^{-1} \times \text{Amt} + 1.02 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Calibration Table Last Updated: Wed Sep 26 14:17:02 2018