


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092618\
 Data File : VX004720.D
 Acq On : 26 Sep 2018 09:28
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM092818S.M
 Title : VOC Analysis
 Last Update : Mon Oct 01 05:52:45 2018

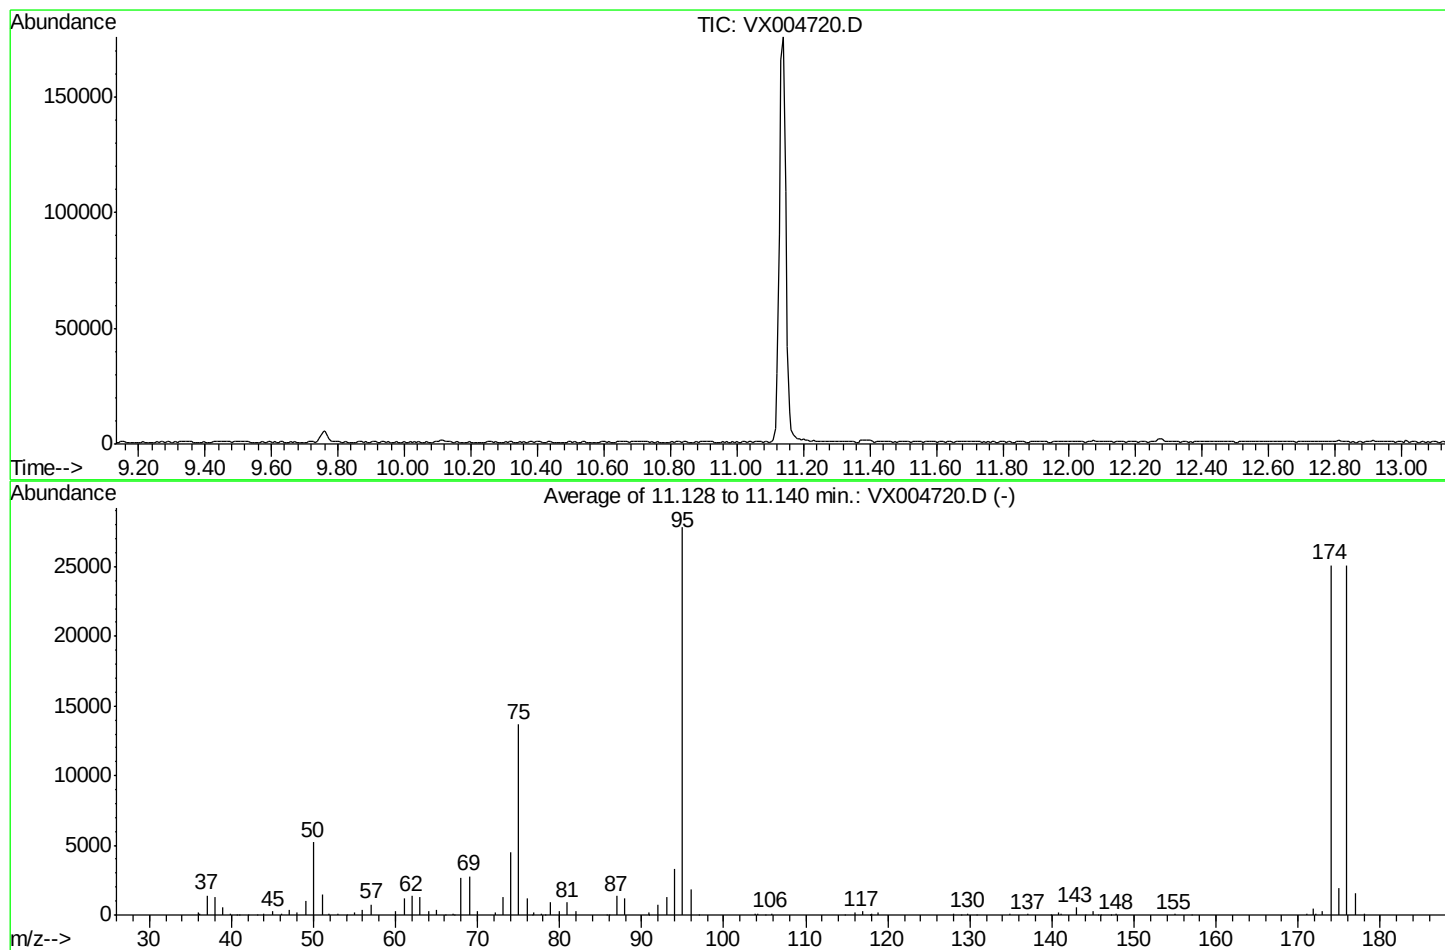

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	5226	PASS
75	95	30	80	49.2	13687	PASS
95	95	100	100	100.0	27829	PASS
96	95	5	9	6.7	1855	PASS
173	174	0.00	2	1.2	313	PASS
174	95	50	120	90.2	25089	PASS
175	174	5	9	7.6	1916	PASS
176	174	95	101	99.8	25049	PASS
177	176	5	9	6.3	1581	PASS