


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092619\
Data File : VX012663.D
Acq On : 26 Sep 2019 08:19
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260
Last Update : Mon Sep 23 12:27:01 2019

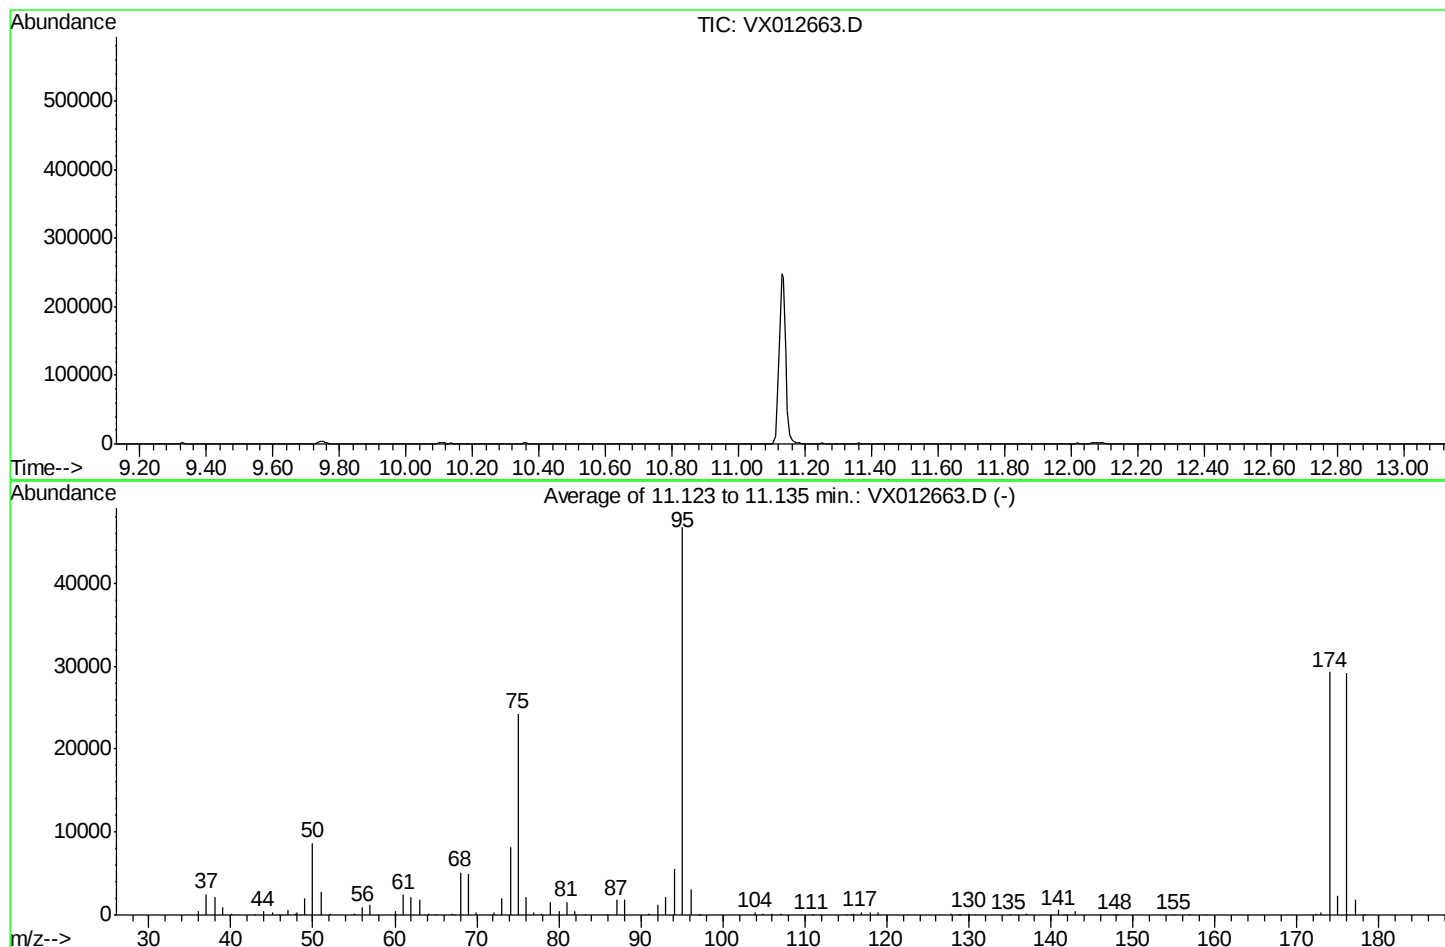

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1673

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	8665	PASS
75	95	30	60	51.9	24232	PASS
95	95	100	100	100.0	46725	PASS
96	95	5	9	6.8	3164	PASS
173	174	0.00	2	1.0	296	PASS
174	95	50	100	62.7	29280	PASS
175	174	5	9	7.7	2261	PASS
176	174	95	101	99.4	29114	PASS
177	176	5	9	6.4	1850	PASS