

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
 Data File : VX047852.D
 Acq On : 26 Sep 2025 13:01
 Operator : JC/MD
 Sample : Q3127-02DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D1-20250915DL

Quant Time: Sep 26 23:12:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	121604	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	248889	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	250346	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	121706	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	94625	48.886	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.780%		
35) Dibromofluoromethane	5.379	113	80258	48.082	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.160%		
50) Toluene-d8	8.635	98	279266	48.352	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	96.700%		
62) 4-Bromofluorobenzene	11.067	95	113991	52.003	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.000%		
Target Compounds						Qvalue
5) Bromomethane	1.624	94	442	0.430	ug/l	85
9) 1,1,2-Trichlorotrifluo...	2.337	101	787	0.560	ug/l #	74
10) Methyl Iodide	2.471	142	1810	0.825	ug/l #	83
11) Tert butyl alcohol	2.947	59	1736	8.053	ug/l #	72
13) Acrolein	2.239	56	81	0.408	ug/l #	1
15) Acrylonitrile	3.075	53	247	0.309	ug/l #	61
16) Acetone	2.386	43	935	1.111	ug/l #	66
17) Carbon Disulfide	2.514	76	1538	0.389	ug/l #	69
19) Methyl tert-butyl Ether	3.111	73	1273	0.241	ug/l	99
20) Methylene Chloride	2.788	84	1101	0.618	ug/l #	72
24) 1,1-Dichloroethane	3.611	63	814	0.265	ug/l #	81
27) cis-1,2-Dichloroethene	4.483	96	1364	0.716	ug/l	79
29) Tetrahydrofuran	5.019	42	223	0.353	ug/l #	42
30) Chloroform	5.074	83	781	0.252	ug/l	91
38) Carbon Tetrachloride	5.538	117	12619	4.762	ug/l #	19
39) Methylcyclohexane	7.360	83	661	0.239	ug/l #	84
44) Trichloroethene	7.110	130	74439	41.563	ug/l	95
49) 1,4-Dioxane	7.671	88	111	5.148	ug/l #	17
51) 4-Methyl-2-Pentanone	8.568	43	582	0.245	ug/l #	37
59) 2-Hexanone	9.433	43	365	0.214	ug/l #	46
60) Dibromochloromethane	9.256	129	4949	2.441	ug/l #	11
64) Tetrachloroethene	9.256	164	4832	2.961	ug/l	92
76) 1,2,3-Trichloropropane	11.061	75	59969	24.336	ug/l #	40
81) trans-1,4-Dichloro-2-b...	11.061	75	59969	62.061	ug/l #	8
85) sec-Butylbenzene	11.872	105	2374	0.257	ug/l	99
86) p-Isopropyltoluene	11.988	119	2211	0.283	ug/l #	78
87) 1,3-Dichlorobenzene	11.951	146	1005	0.237	ug/l	92
88) 1,4-Dichlorobenzene	11.951	146	1005	0.231	ug/l	93
89) n-Butylbenzene	12.317	91	3531	0.488	ug/l	99
93) 1,2,4-Trichlorobenzene	13.573	180	1625	0.620	ug/l	95
94) Hexachlorobutadiene	13.707	225	1618	1.817	ug/l	95
95) Naphthalene	13.756	128	3699	0.463	ug/l #	92
96) 1,2,3-Trichlorobenzene	13.939	180	1553	0.637	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
Data File : VX047852.D
Acq On : 26 Sep 2025 13:01
Operator : JC/MD
Sample : Q3127-02DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Quant Time: Sep 26 23:12:54 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration

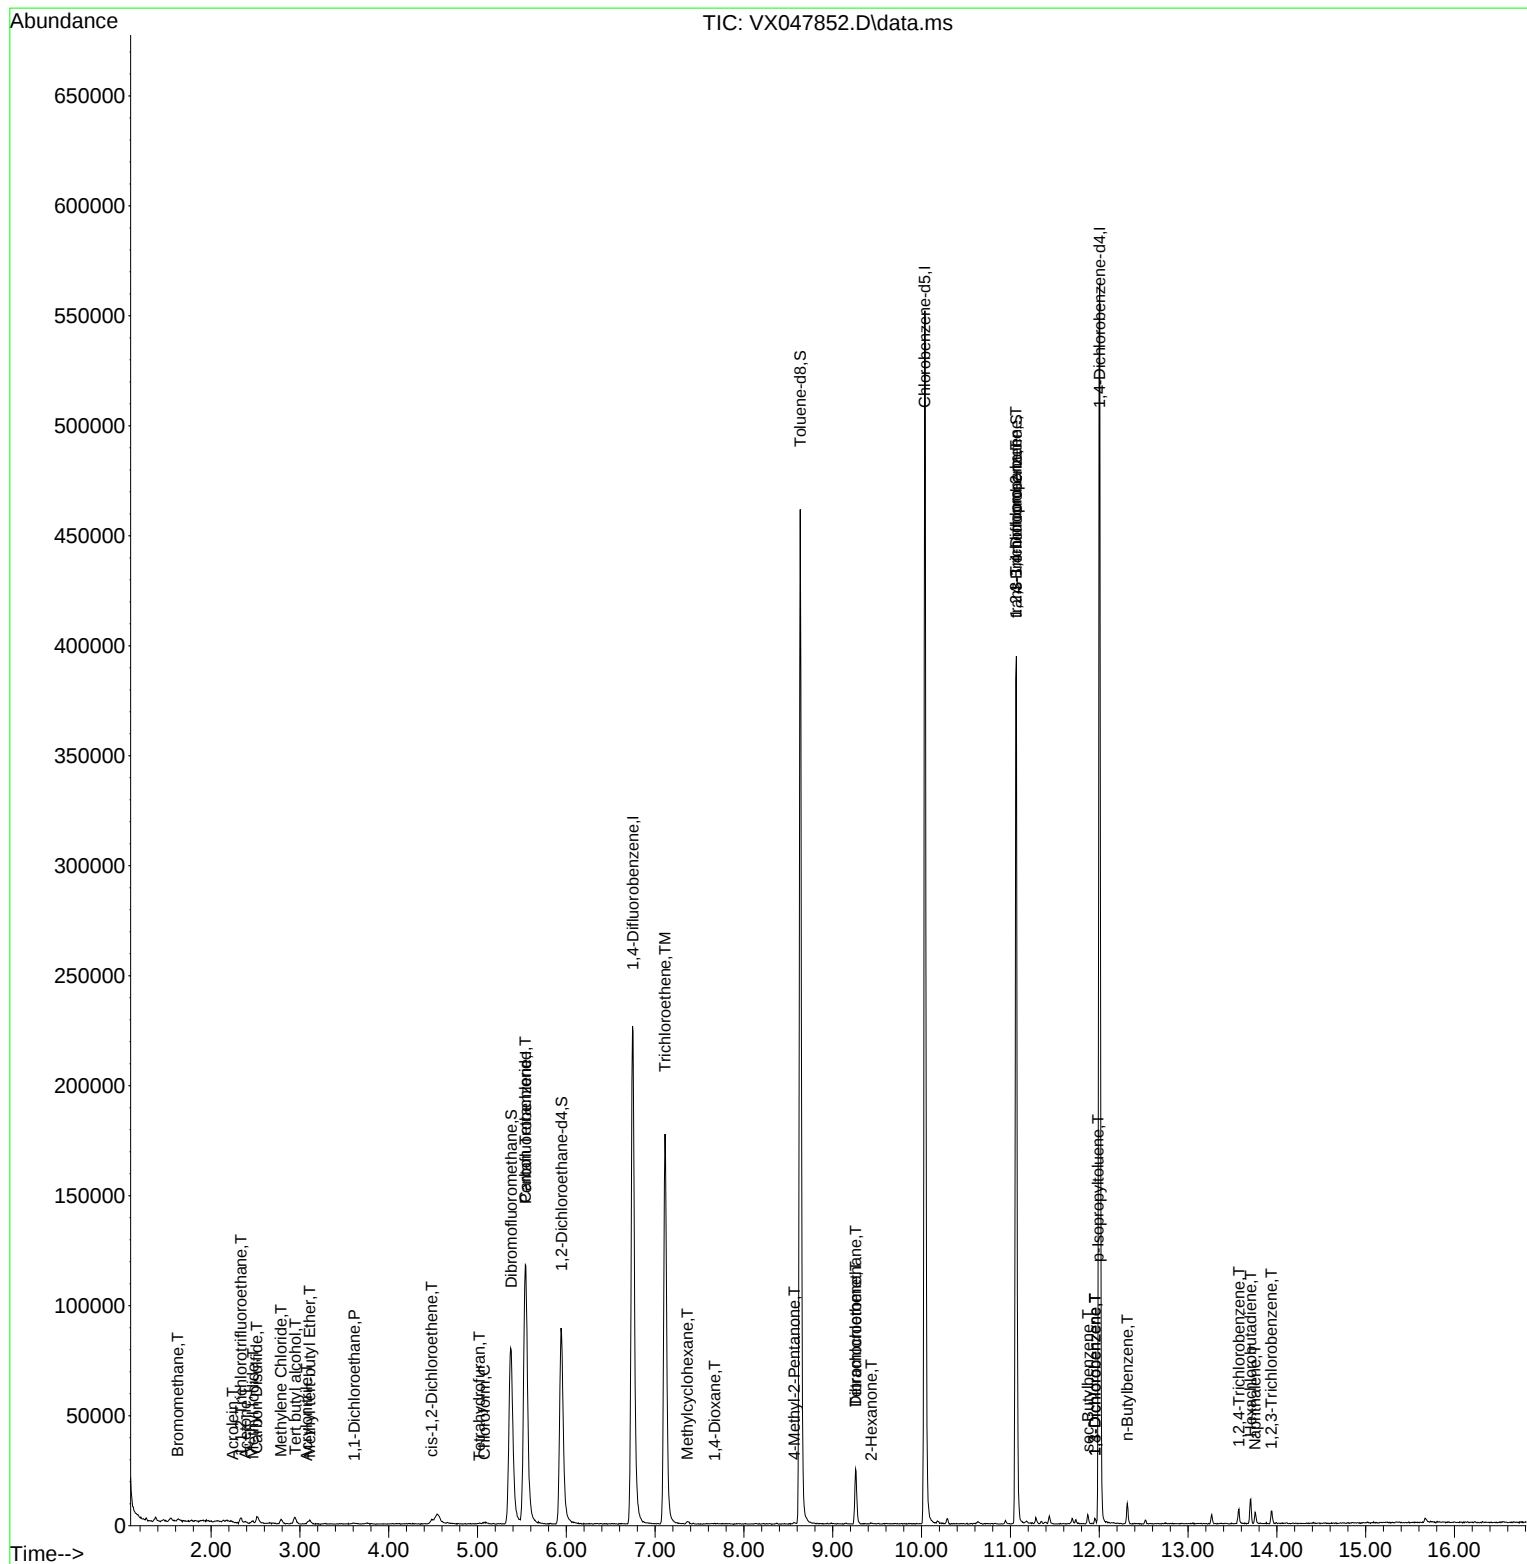






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL







Tgt Ion:168 Resp: 121604
Ion Ratio Lower Upper
168 100
99 61.5 48.8 73.2

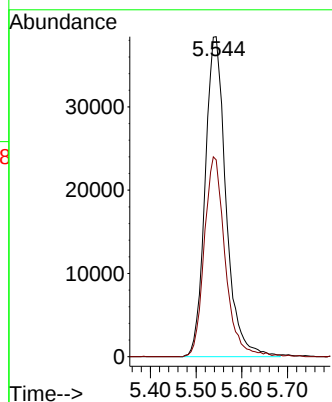

#5
Bromomethane
Concen: 0.430 ug/l
RT: 1.624 min Scan# 88
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 94 Resp: 442
Ion Ratio Lower Upper
94 100
96 80.9 76.6 115.0









#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.560 ug/l
RT: 2.337 min Scan# 205
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:101 Resp: 787
Ion Ratio Lower Upper
101 100
85 38.5 35.5 53.3
151 105.3 59.4 89.0#



#10
Methyl Iodide
Concen: 0.825 ug/l
RT: 2.471 min Scan# 227
Delta R.T. 0.012 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion:142 Resp: 1810
Ion Ratio Lower Upper
142 100
127 37.0 37.2 55.8#
141 4.5 11.4 17.0#



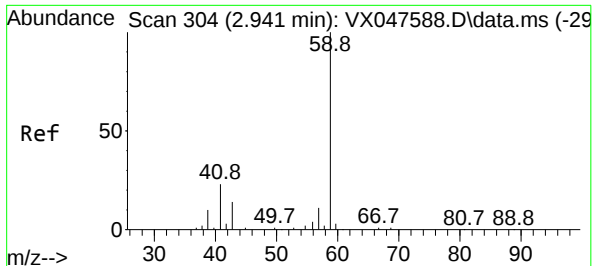

#11

Tert butyl alcohol

Concen: 8.053 ug/l

RT: 2.947 min Scan# 304

Delta R.T. 0.006 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01

Instrument :

MSVOA_X

ClientSampleId :





RE131D1-20250915DL

Tgt Ion: 59 Resp: 1736

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

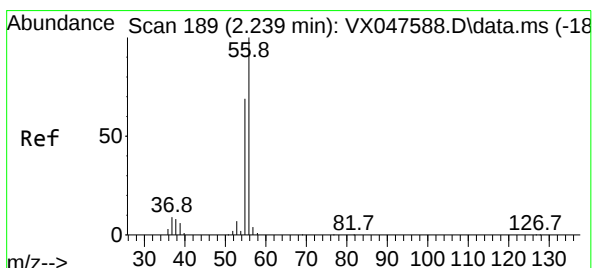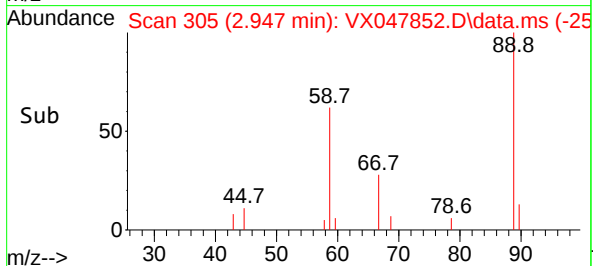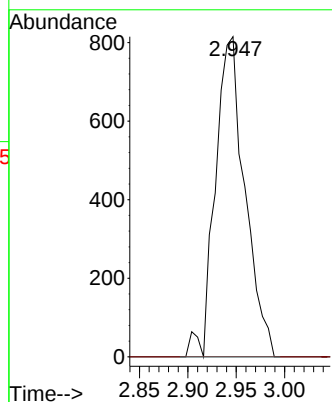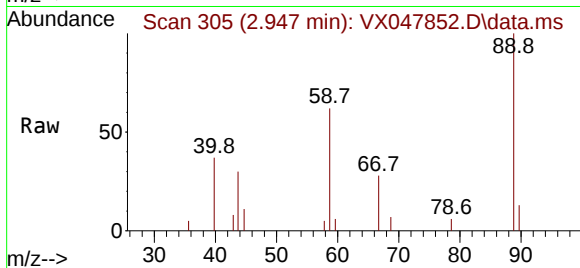

#13

Acrolein

Concen: 0.408 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min

Lab File: VX047852.D




Acq: 26 Sep 2025 13:01


Tgt Ion: 56 Resp: 81

Ion Ratio Lower Upper

56 100


55 161.7 57.2 85.8#

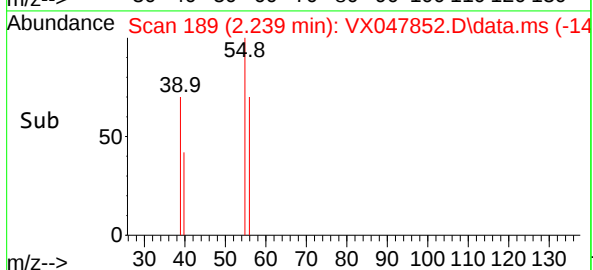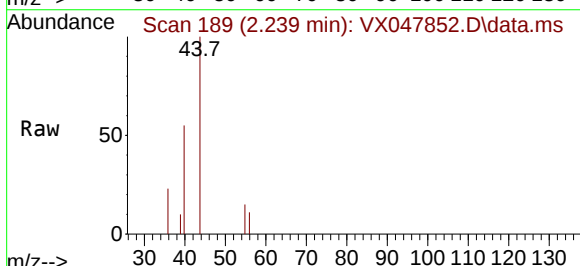






#15
Acrylonitrile
Concen: 0.309 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.012 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL







Tgt Ion: 53 Resp: 247
Ion Ratio Lower Upper
53 100
52 48.6 66.4 99.6#
51 61.5 29.5 44.3#

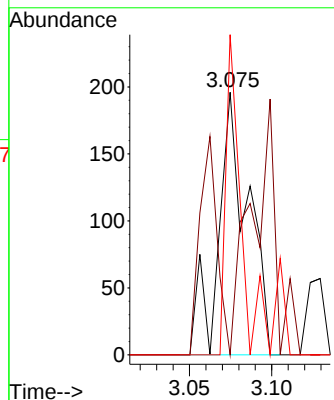

#16
Acetone
Concen: 1.111 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.012 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01


Tgt Ion: 43 Resp: 935
Ion Ratio Lower Upper
43 100
58 11.1 23.4 35.0#

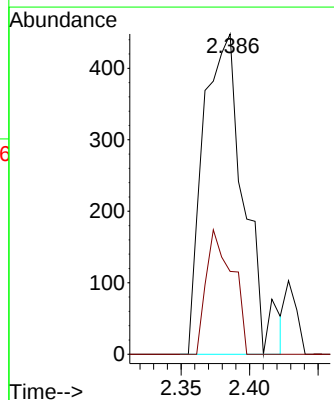






#17
Carbon Disulfide
Concen: 0.389 ug/l
RT: 2.514 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL



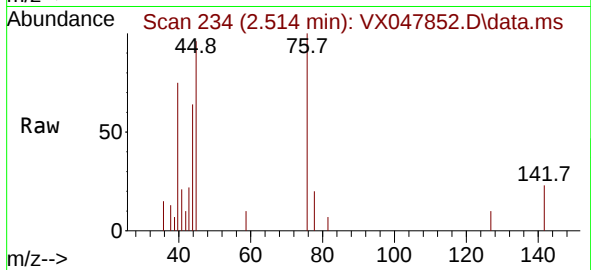



Tgt Ion: 76 Resp: 1538
Ion Ratio Lower Upper
76 100
78 19.5 6.8 10.2#

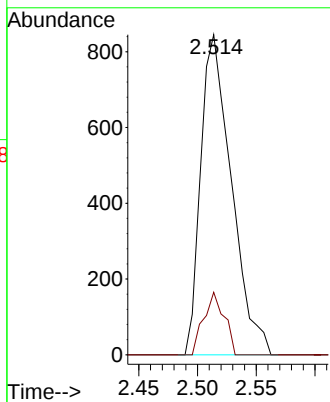

#19
Methyl tert-butyl Ether
Concen: 0.241 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01


Tgt Ion: 73 Resp: 1273
Ion Ratio Lower Upper
73 100
57 21.3 17.4 26.2

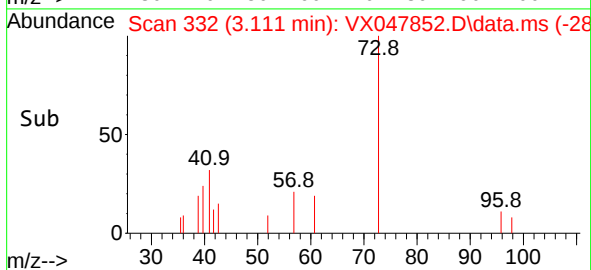






#20
Methylene Chloride
Concen: 0.618 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL







Tgt Ion:	84	Resp:	1101
Ion	Ratio	Lower	Upper
84	100		
49	96.5	108.6	162.8#
51	33.9	32.6	48.8
86	42.5	52.0	78.0#



#24
1,1-Dichloroethane
Concen: 0.265 ug/l
RT: 3.611 min Scan# 414
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion:	63	Resp:	814
Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.8	11.2#
100	0.0	2.3	6.9#









#27
cis-1,2-Dichloroethene
Concen: 0.716 ug/l
RT: 4.483 min Scan# 51
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:	96	Resp:	1364
Ion	Ratio	Lower	Upper
96	100		
61	160.1	0.0	303.2
98	20.3	0.0	127.8



#29
Tetrahydrofuran
Concen: 0.353 ug/l
RT: 5.019 min Scan# 645
Delta R.T. 0.030 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion:	42	Resp:	223
Ion	Ratio	Lower	Upper
42	100		
72	9.9	34.2	51.2#
71	0.0	31.9	47.9#

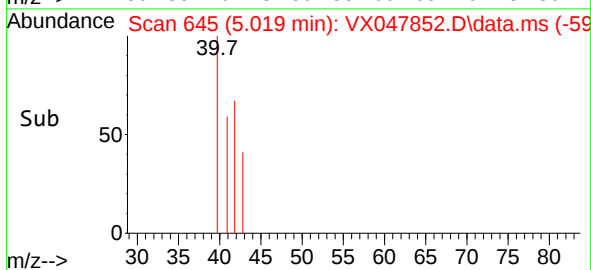



#30

Chloroform

Concen: 0.252 ug/l

RT: 5.074 min Scan# 61

Delta R.T. -0.006 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01

Instrument :

MSVOA_X

ClientSampleId :





RE131D1-20250915DL

Tgt Ion: 83 Resp: 781

Ion Ratio Lower Upper

83 100

85 57.6 51.8 77.6

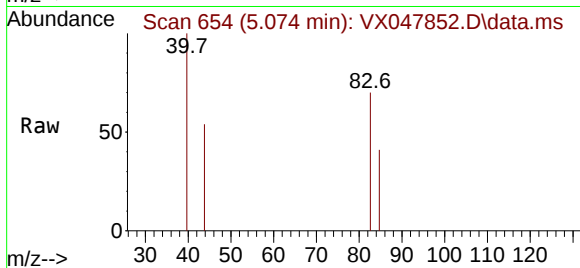

#33

1,2-Dichloroethane-d4

Concen: 48.886 ug/l

RT: 5.946 min Scan# 797

Delta R.T. 0.006 min

Lab File: VX047852.D




Acq: 26 Sep 2025 13:01


Tgt Ion: 65 Resp: 94625

Ion Ratio Lower Upper

65 100

67 52.2 0.0 103.0




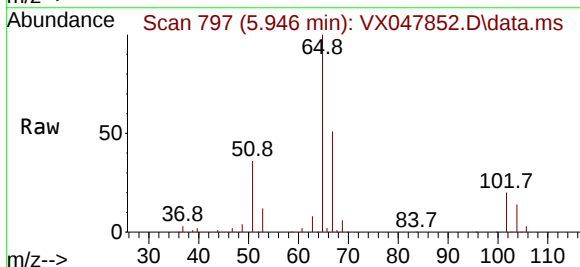




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:114 Resp: 248889
Ion Ratio Lower Upper
114 100
63 20.9 0.0 44.0
88 15.9 0.0 34.2

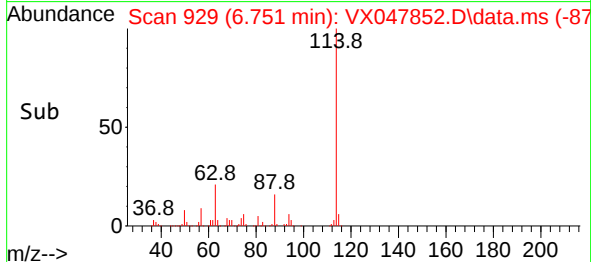

#35
Dibromofluoromethane
Concen: 48.082 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01


Tgt Ion:113 Resp: 80258
Ion Ratio Lower Upper
113 100
111 101.5 80.9 121.3
192 17.6 14.2 21.4








#38
Carbon Tetrachloride
Concen: 4.762 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.134 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL







Tgt Ion:117 Resp: 12619
Ion Ratio Lower Upper
117 100
119 6.3 73.4 110.2#
121 0.0 23.8 35.6#

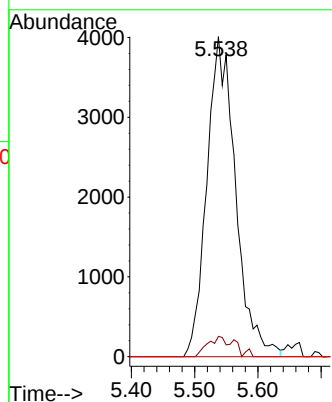

#39
Methylcyclohexane
Concen: 0.239 ug/l
RT: 7.360 min Scan# 1029
Delta R.T. -0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 83 Resp: 661
Ion Ratio Lower Upper
83 100
55 61.8 66.4 99.6#
98 45.4 38.1 57.1









#44
Trichloroethene
Concen: 41.563 ug/l
RT: 7.110 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:130 Resp: 74439
Ion Ratio Lower Upper
130 100
95 100.7 0.0 210.8



#49
1,4-Dioxane
Concen: 5.148 ug/l
RT: 7.671 min Scan# 1080
Delta R.T. 0.024 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 88 Resp: 111
Ion Ratio Lower Upper
88 100
43 81.1 30.2 45.2#
58 0.0 59.5 89.3#


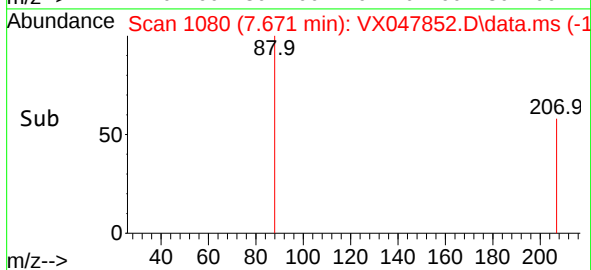






#50
Toluene-d8
Concen: 48.352 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion: 98 Resp: 279266
Ion Ratio Lower Upper
98 100
100 66.4 53.0 79.4

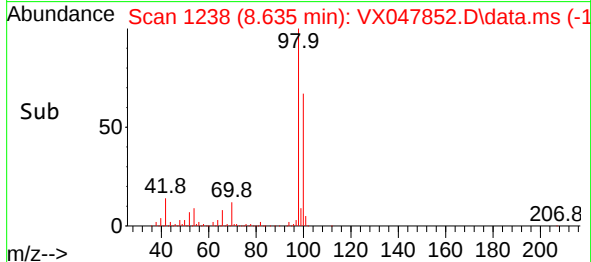

#51
4-Methyl-2-Pentanone
Concen: 0.245 ug/l
RT: 8.568 min Scan# 1227
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 43 Resp: 582
Ion Ratio Lower Upper
43 100
58 0.0 30.3 45.5#







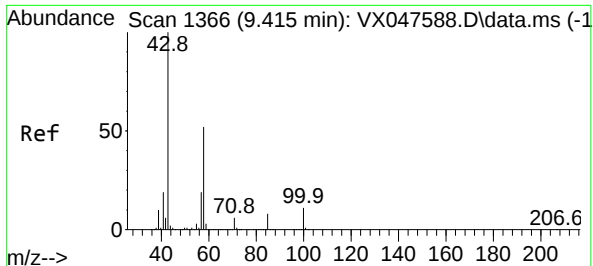

#59
2-Hexanone
Concen: 0.214 ug/l
RT: 9.433 min Scan# 11
Delta R.T. 0.018 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion: 43 Resp: 365
Ion Ratio Lower Upper
43 100
58 14.0 26.1 78.2#

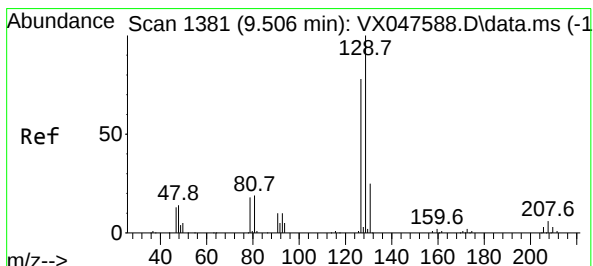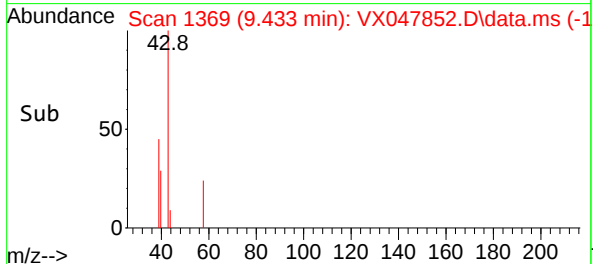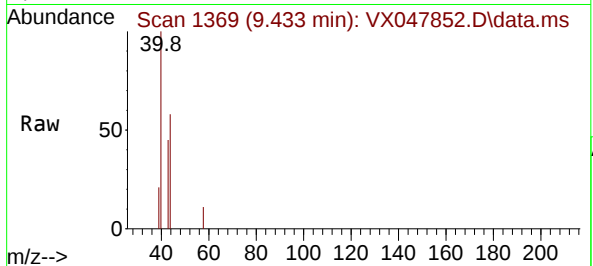

#60
Dibromochloromethane
Concen: 2.441 ug/l
RT: 9.256 min Scan# 1340
Delta R.T. -0.250 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 129 Resp: 4949
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#


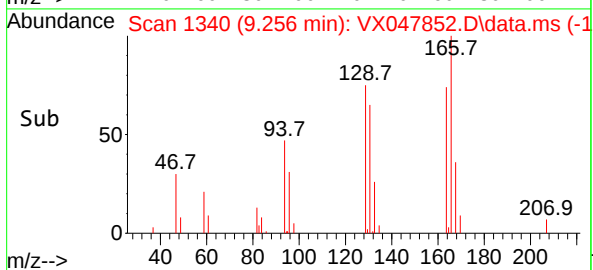

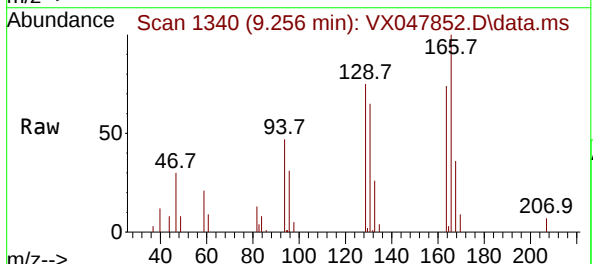




#62
4-Bromofluorobenzene
Concen: 52.003 ug/l
RT: 11.067 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion: 95 Resp: 113991
Ion Ratio Lower Upper
95 100
174 74.7 0.0 141.6
176 71.3 0.0 138.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion: 117 Resp: 250346
Ion Ratio Lower Upper
117 100
82 58.9 47.8 71.6
119 32.2 25.2 37.8


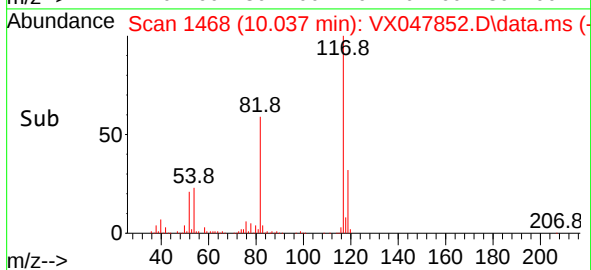






#64
Tetrachloroethene
Concen: 2.961 ug/l
RT: 9.256 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt	Ion:164	Resp:	4832
Ion	Ratio	Lower	Upper
164	100		
166	135.9	100.2	150.2
129	104.9	81.8	122.6
131	87.8	78.6	118.0

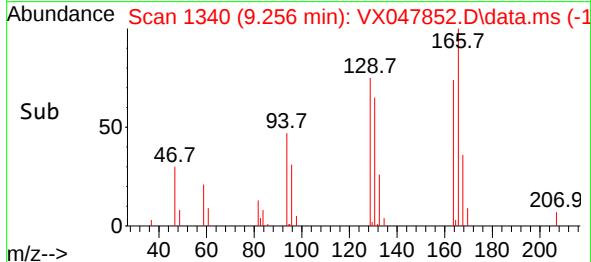

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion:152	Resp:	121706	
Ion	Ratio	Lower	Upper
152	100		
115	62.0	44.9	134.5
150	158.4	0.0	352.0



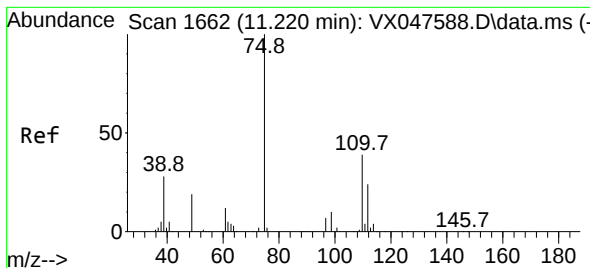

#76

1,2,3-Trichloropropane

Concen: 24.336 ug/l

RT: 11.061 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01

Instrument :

MSVOA_X

ClientSampleId :





RE131D1-20250915DL

Tgt Ion: 75 Resp: 59969

Ion Ratio Lower Upper

75 100

77 1.4 18.8 56.4#

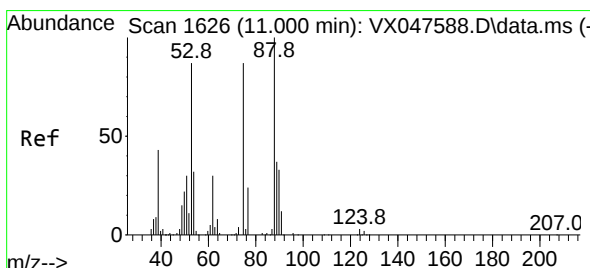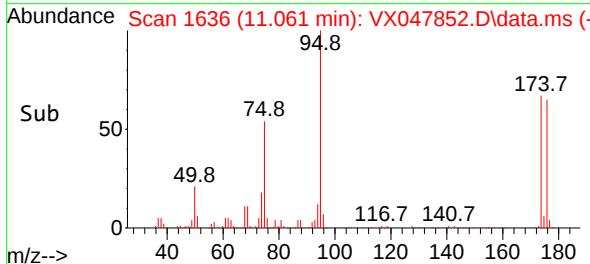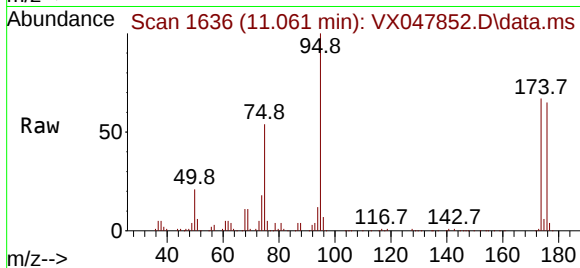

#81

trans-1,4-Dichloro-2-butene

Concen: 62.061 ug/l

RT: 11.061 min Scan# 1636

Delta R.T. 0.061 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01




Tgt Ion: 75 Resp: 59969


Ion Ratio Lower Upper

75 100

53 0.0 83.4 125.2#

89 0.0 36.3 54.5#

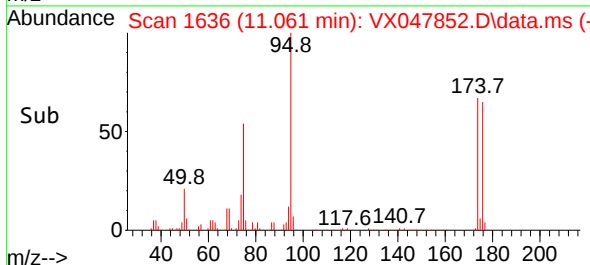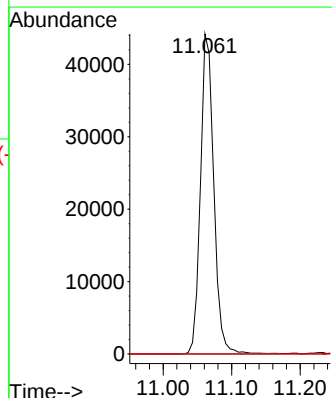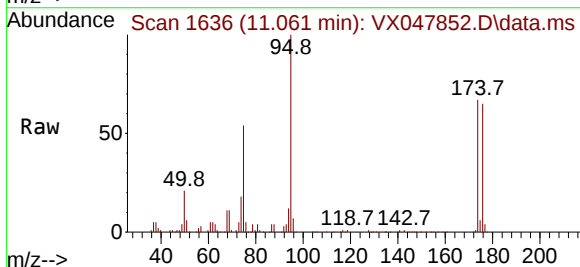



#85

sec-Butylbenzene

Concen: 0.257 ug/l

RT: 11.872 min Scan# 1769

Delta R.T. -0.000 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01

Instrument :

MSVOA_X

ClientSampleId :





RE131D1-20250915DL

Tgt Ion:105 Resp: 2374

Ion Ratio Lower Upper

105 100

134 19.1 9.8 29.5

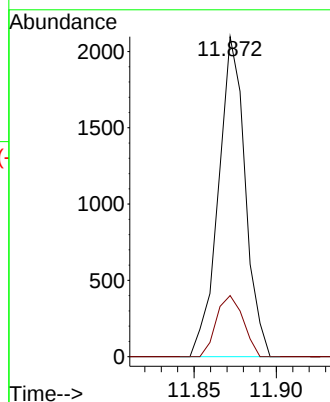

#86

p-Isopropyltoluene

Concen: 0.283 ug/l

RT: 11.988 min Scan# 1788

Delta R.T. -0.006 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01




Tgt Ion:119 Resp: 2211


Ion Ratio Lower Upper

119 100

134 28.3 12.6 37.8

91 44.0 12.6 37.6#









#87
1,3-Dichlorobenzene
Concen: 0.237 ug/l
RT: 11.951 min Scan# 1782
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:146	Resp:	1005
Ion Ratio	Lower	Upper
146	100	
111	38.4	21.5 64.5
148	57.4	32.0 96.0

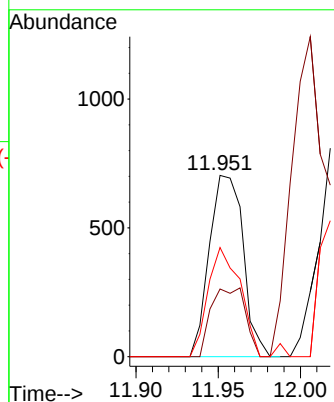

#88
1,4-Dichlorobenzene
Concen: 0.231 ug/l
RT: 11.951 min Scan# 1782
Delta R.T. -0.073 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01

Tgt Ion:146	Resp:	1005
Ion Ratio	Lower	Upper
146	100	
111	38.4	20.8 62.4
148	57.4	31.7 95.1

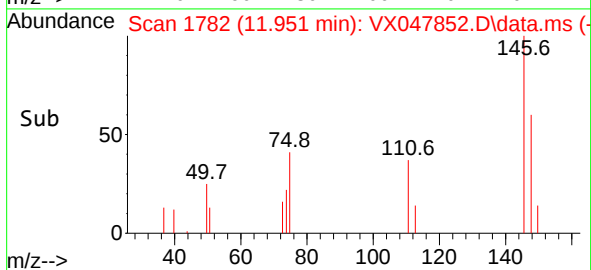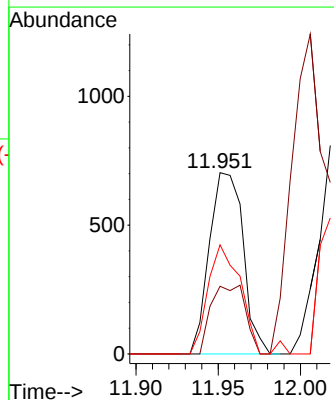



#89

n-Butylbenzene

Concen: 0.488 ug/l

RT: 12.317 min Scan# 1841

Delta R.T. 0.006 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01

Instrument :

MSVOA_X

ClientSampleId :

RE131D1-20250915DL





Tgt Ion: 91 Resp: 3531

Ion Ratio Lower Upper

91 100

92 56.5 27.6 82.7

134 25.4 12.6 37.8

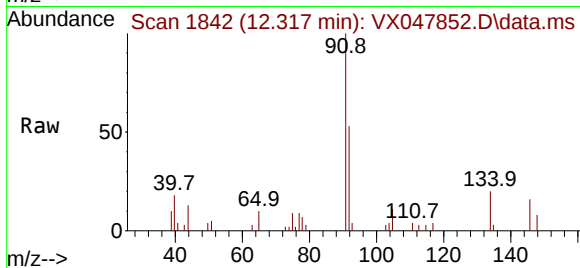

#93

1,2,4-Trichlorobenzene

Concen: 0.620 ug/l

RT: 13.573 min Scan# 2048

Delta R.T. 0.006 min

Lab File: VX047852.D

Acq: 26 Sep 2025 13:01




Tgt Ion:180 Resp: 1625


Ion Ratio Lower Upper

180 100

182 99.9 46.6 139.8

145 32.6 16.4 49.1




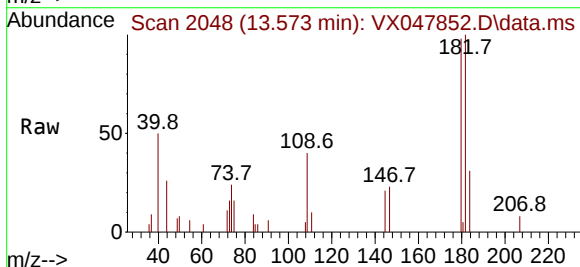




#94
Hexachlorobutadiene
Concen: 1.817 ug/l
RT: 13.707 min Scan# 2070
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01




Instrument :
MSVOA_X
ClientSampleId :
RE131D1-20250915DL


Tgt Ion:	225	Resp:	1618
Ion	Ratio	Lower	Upper
225	100		
223	69.4	31.7	95.1
227	65.9	32.0	96.0

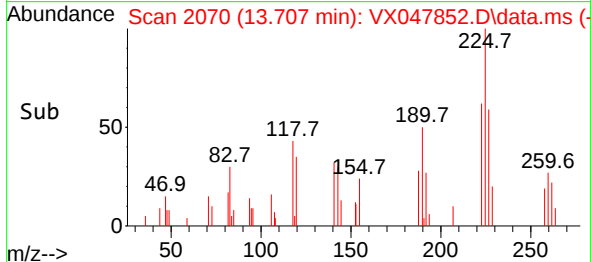

#95
Naphthalene
Concen: 0.463 ug/l
RT: 13.756 min Scan# 2078
Delta R.T. -0.000 min
Lab File: VX047852.D
Acq: 26 Sep 2025 13:01


Tgt Ion:	128	Resp:	3699
Ion	Ratio	Lower	Upper
128	100		
127	9.0	10.2	15.2#
129	8.6	8.8	13.2#



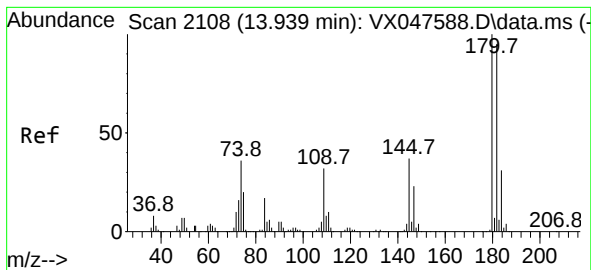

#96
 1,2,3-Trichlorobenzene
 Concen: 0.637 ug/l
 RT: 13.939 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX047852.D
 Acq: 26 Sep 2025 13:01

Instrument :
 MSVOA_X
 ClientSampleId :
 RE131D1-20250915DL

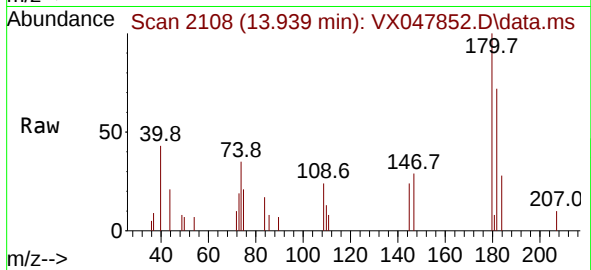

Tgt Ion:	180	Resp:	1553
Ion	Ratio	Lower	Upper
180	100		
182	103.2	47.6	142.8
145	36.9	17.9	53.7

