

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
 Data File : VX047854.D
 Acq On : 26 Sep 2025 13:43
 Operator : JC/MD
 Sample : Q3156-04DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT190D1-20250918DL

Quant Time: Sep 26 23:14:29 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	129371	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	270470	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	274305	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	134213	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	109732	53.287	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 106.580%	
35) Dibromofluoromethane	5.373	113	90161	49.705	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 99.420%	
50) Toluene-d8	8.635	98	303928	48.423	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 96.840%	
62) 4-Bromofluorobenzene	11.061	95	128407	53.906	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 107.820%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.630	94	499	0.457	ug/l #	78
9) 1,1,2-Trichlorotrifluo...	2.349	101	1018	0.680	ug/l #	89
10) Methyl Iodide	2.465	142	1514	0.649	ug/l #	91
11) Tert butyl alcohol	2.953	59	1249	5.446	ug/l #	72
12) 1,1-Dichloroethene	2.331	96	764	0.497	ug/l #	76
13) Acrolein	2.239	56	60	0.284	ug/l #	14
15) Acrylonitrile	3.087	53	210	0.247	ug/l #	81
16) Acetone	2.380	43	1048	1.170	ug/l	93
17) Carbon Disulfide	2.520	76	1507	0.358	ug/l #	76
18) Methyl Acetate	2.709	43	477	0.239	ug/l #	54
20) Methylene Chloride	2.788	84	1157	0.610	ug/l #	75
25) 2-Butanone	4.550	43	391	0.350	ug/l #	50
27) cis-1,2-Dichloroethene	4.489	96	1380	0.681	ug/l	79
30) Chloroform	5.086	83	1215	0.368	ug/l #	80
31) Cyclohexane	5.544	56	3145	1.156	ug/l #	1
36) 1,1-Dichloropropene	5.538	75	10991	4.147	ug/l #	47
38) Carbon Tetrachloride	5.666	117	1142	0.397	ug/l #	68
44) Trichloroethene	7.110	130	123155	63.276	ug/l	98
55) 1,1,2-Trichloroethane	9.141	97	876	0.458	ug/l #	87
58) 2-Chloroethyl Vinyl ether	8.177	63	19	7.906	ug/l #	47
76) 1,2,3-Trichloropropane	11.061	75	67094	24.691	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.061	75	67094	62.964	ug/l #	8
85) sec-Butylbenzene	11.872	105	2080	0.204	ug/l	98
86) p-Isopropyltoluene	11.994	119	1853	0.215	ug/l #	72
89) n-Butylbenzene	12.317	91	2841	0.356	ug/l	98
93) 1,2,4-Trichlorobenzene	13.573	180	1530	0.529	ug/l	99
94) Hexachlorobutadiene	13.707	225	1266	1.290	ug/l	96
95) Naphthalene	13.756	128	2972	0.338	ug/l	98
96) 1,2,3-Trichlorobenzene	13.938	180	1342	0.499	ug/l	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
Data File : VX047854.D
Acq On : 26 Sep 2025 13:43
Operator : JC/MD
Sample : Q3156-04DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Quant Time: Sep 26 23:14:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration

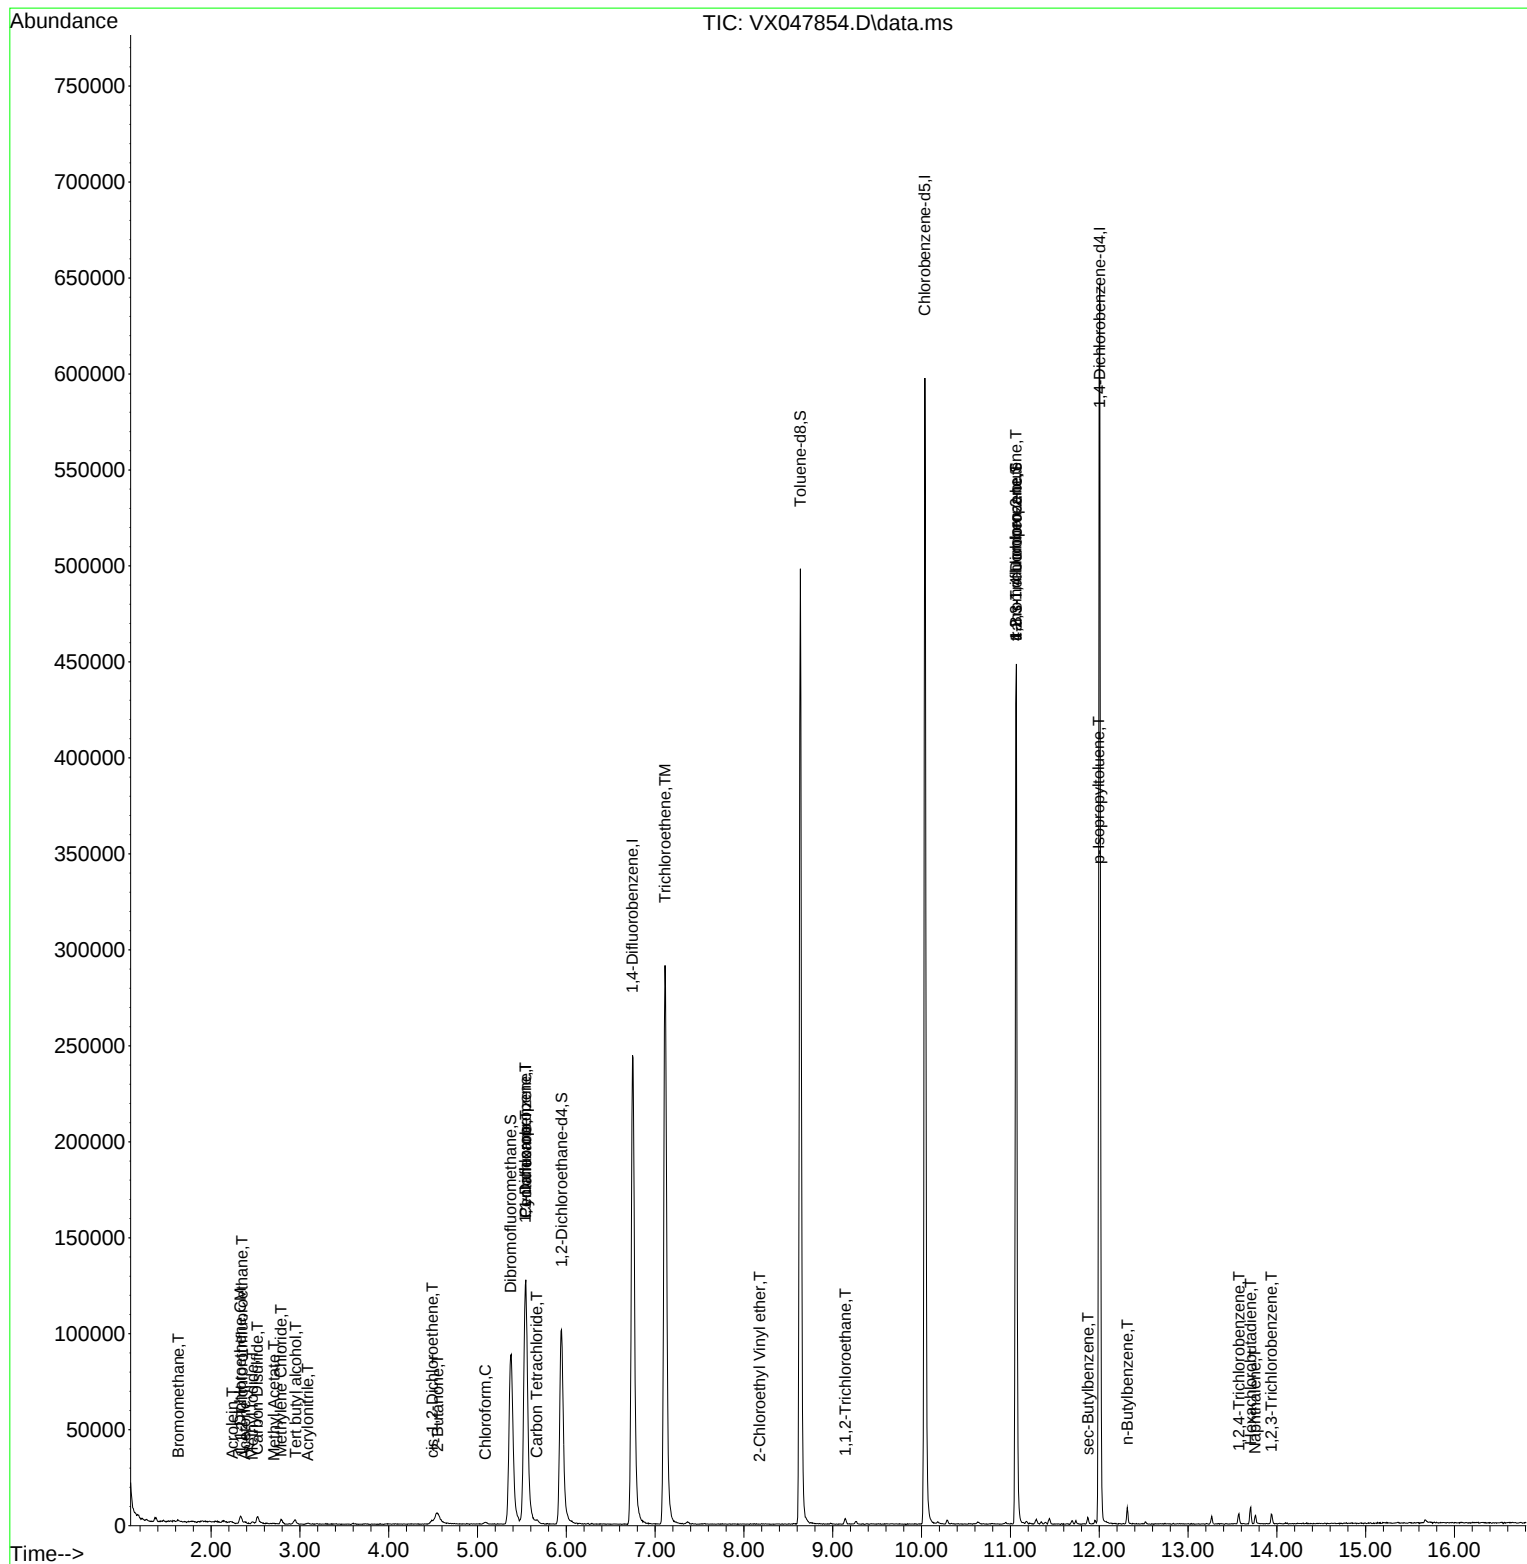






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL







Tgt Ion:168 Resp: 129371
Ion Ratio Lower Upper
168 100
99 59.7 48.8 73.2



#5
Bromomethane
Concen: 0.457 ug/l
RT: 1.630 min Scan# 89
Delta R.T. 0.012 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 94 Resp: 499
Ion Ratio Lower Upper
94 100
96 74.0 76.6 115.0#


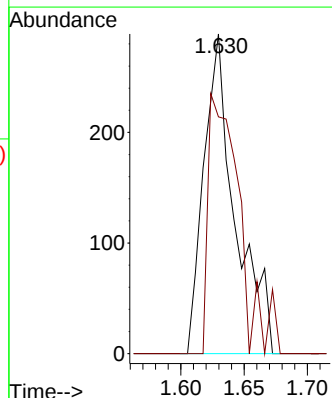






#9
1,1,2-Trichlorotrifluoroethane
Concen: 0.680 ug/l
RT: 2.349 min Scan# 205
Delta R.T. 0.012 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion:101 Resp: 1018
Ion Ratio Lower Upper
101 100
85 55.6 35.5 53.3#
151 80.1 59.4 89.0



#10
Methyl Iodide
Concen: 0.649 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion:142 Resp: 1514
Ion Ratio Lower Upper
142 100
127 41.7 37.2 55.8
141 8.7 11.4 17.0#

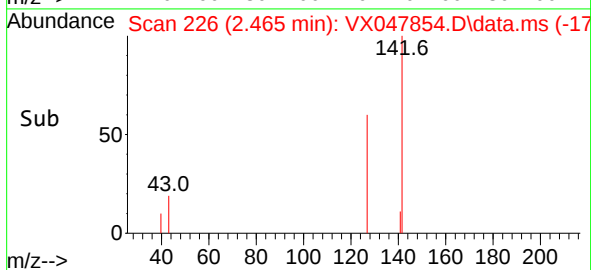

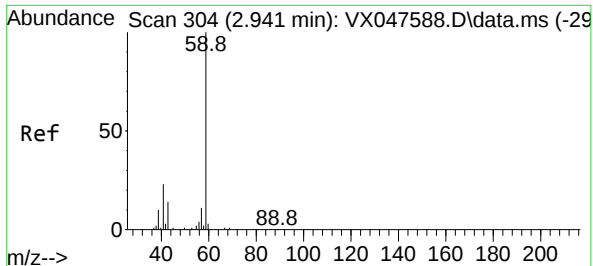

#11

Tert butyl alcohol

Concen: 5.446 ug/l

RT: 2.953 min Scan# 304

Delta R.T. 0.012 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43

Instrument :

MSVOA_X

ClientSampleId :





TT190D1-20250918DL

Tgt Ion: 59 Resp: 1249

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

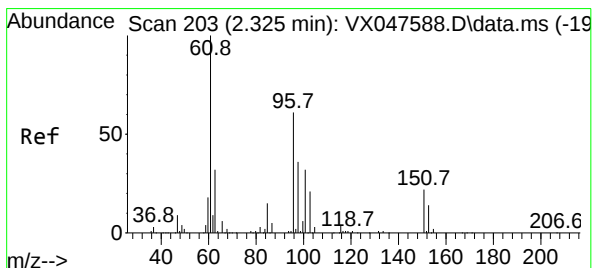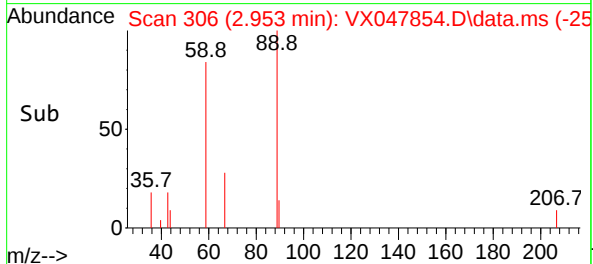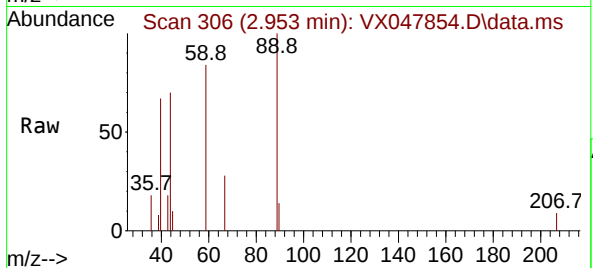

#12

1,1-Dichloroethene

Concen: 0.497 ug/l

RT: 2.331 min Scan# 204

Delta R.T. 0.006 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43




Tgt Ion: 96 Resp: 764


Ion Ratio Lower Upper

96 100

61 132.0 131.0 196.6

98 78.2 47.7 71.5#


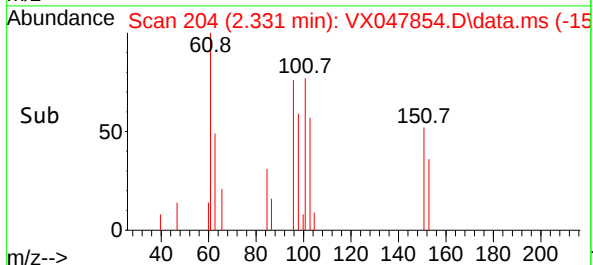
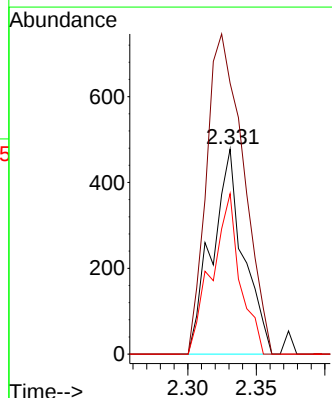
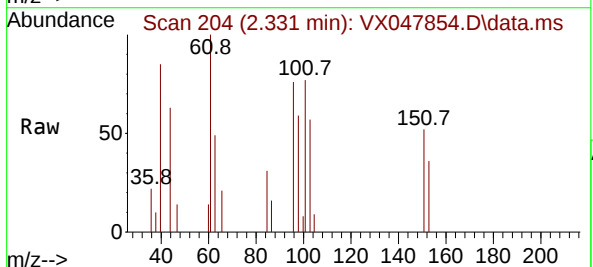




#13
Acrolein
Concen: 0.284 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 56 Resp: 60
Ion Ratio Lower Upper
56 100
55 0.0 57.2 85.8#



#15
Acrylonitrile
Concen: 0.247 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.024 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 53 Resp: 210
Ion Ratio Lower Upper
53 100
52 83.3 66.4 99.6
51 0.0 29.5 44.3#


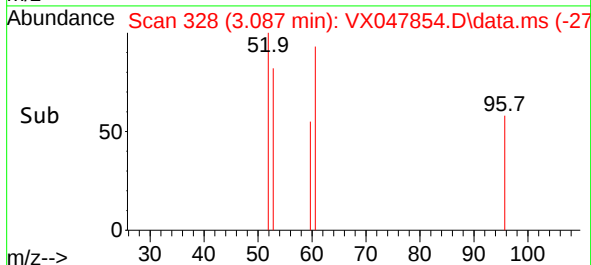
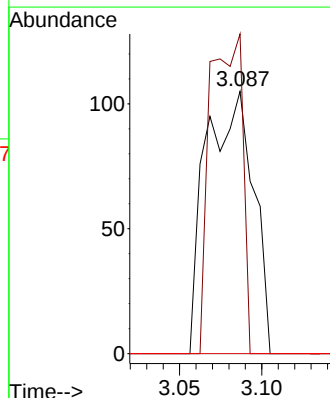





#16
Acetone
Concen: 1.170 ug/l
RT: 2.380 min Scan# 211
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 43 Resp: 1048
Ion Ratio Lower Upper
43 100
58 33.0 23.4 35.0



#17
Carbon Disulfide
Concen: 0.358 ug/l
RT: 2.520 min Scan# 235
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 76 Resp: 1507
Ion Ratio Lower Upper
76 100
78 0.0 6.8 10.2#









#18
Methyl Acetate
Concen: 0.239 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 43 Resp: 477
Ion Ratio Lower Upper
43 100
74 0.0 17.4 26.2#

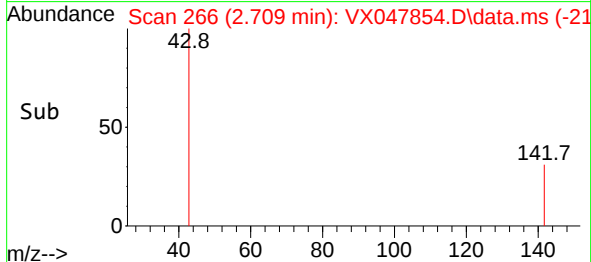

#20
Methylene Chloride
Concen: 0.610 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 84 Resp: 1157
Ion Ratio Lower Upper
84 100
49 105.1 108.6 162.8#
51 23.7 32.6 48.8#
86 47.1 52.0 78.0#


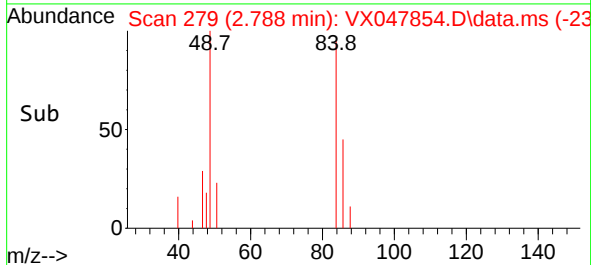






#25
2-Butanone
Concen: 0.350 ug/l
RT: 4.550 min Scan# 50
Delta R.T. 0.012 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 43 Resp: 391
Ion Ratio Lower Upper
43 100
72 0.0 20.1 30.1#

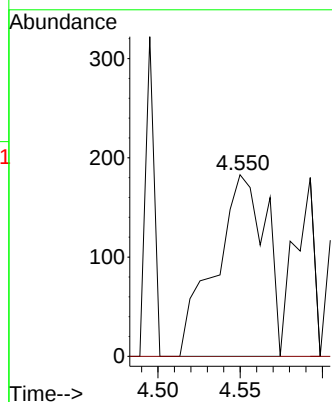

#27
cis-1,2-Dichloroethene
Concen: 0.681 ug/l
RT: 4.489 min Scan# 558
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43


Tgt Ion: 96 Resp: 1380
Ion Ratio Lower Upper
96 100
61 169.9 0.0 303.2
98 34.6 0.0 127.8

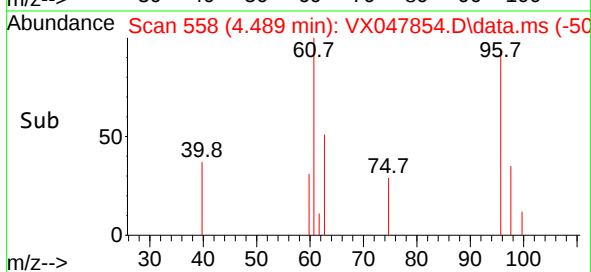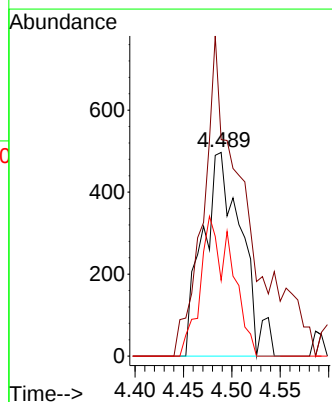






#30
Chloroform
Concen: 0.368 ug/l
RT: 5.086 min Scan# 611
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43


Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL





Tgt Ion: 83 Resp: 1215
Ion Ratio Lower Upper
83 100
85 49.0 51.8 77.6#




#31
Cyclohexane
Concen: 1.156 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.085 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43



Tgt Ion: 56 Resp: 3145
Ion Ratio Lower Upper
56 100
69 152.7 23.8 35.8#
84 142.7 64.6 97.0#

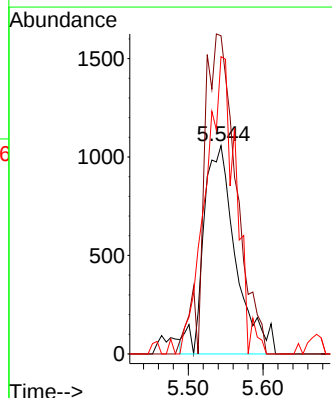



#33

1,2-Dichloroethane-d4

Concen: 53.287 ug/l

RT: 5.946 min Scan# 796

Delta R.T. 0.006 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43

Instrument :

MSVOA_X

ClientSampleId :





TT190D1-20250918DL

Tgt Ion: 65 Resp: 109732

Ion Ratio Lower Upper

65 100

67 52.5 0.0 103.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.745 min Scan# 928

Delta R.T. -0.000 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43




Tgt Ion: 114 Resp: 270470


Ion Ratio Lower Upper

114 100

63 22.5 0.0 44.0

88 16.1 0.0 34.2









#35
Dibromofluoromethane
Concen: 49.705 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion:113 Resp: 90161
Ion Ratio Lower Upper
113 100
111 101.0 80.9 121.3
192 17.7 14.2 21.4

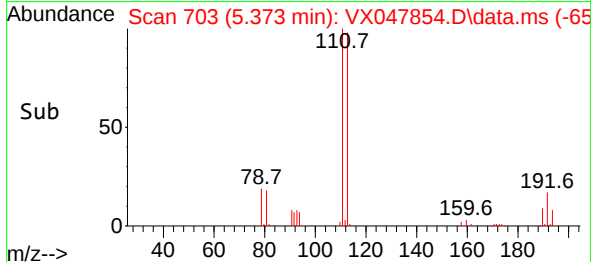

#36
1,1-Dichloropropene
Concen: 4.147 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.146 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 75 Resp: 10991
Ion Ratio Lower Upper
75 100
110 4.3 16.7 50.1#
77 0.0 24.3 36.5#




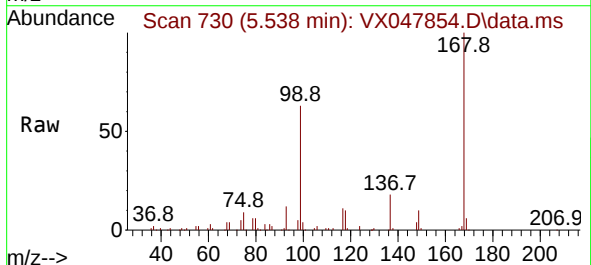




#38
Carbon Tetrachloride
Concen: 0.397 ug/l
RT: 5.666 min Scan# 751
Delta R.T. -0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion:117 Resp: 1142
Ion Ratio Lower Upper
117 100
119 58.3 73.4 110.2#
121 16.9 23.8 35.6#



#44
Trichloroethene
Concen: 63.276 ug/l
RT: 7.110 min Scan# 988
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion:130 Resp: 123155
Ion Ratio Lower Upper
130 100
95 103.3 0.0 210.8



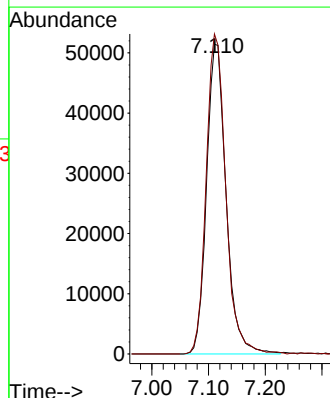





#50
Toluene-d8
Concen: 48.423 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 98 Resp: 303928
Ion Ratio Lower Upper
98 100
100 66.9 53.0 79.4

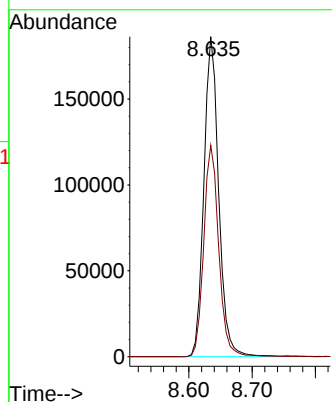

#55
1,1,2-Trichloroethane
Concen: 0.458 ug/l
RT: 9.141 min Scan# 1321
Delta R.T. 0.006 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 97 Resp: 876
Ion Ratio Lower Upper
97 100
83 67.6 69.6 104.4#
85 45.8 45.0 67.6
99 60.4 49.6 74.4


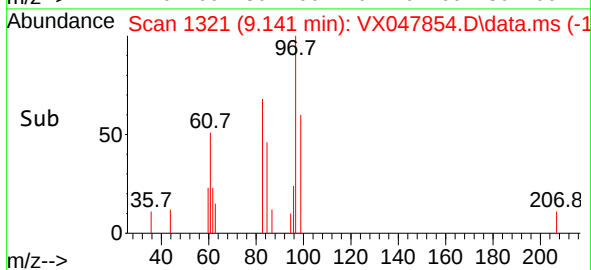

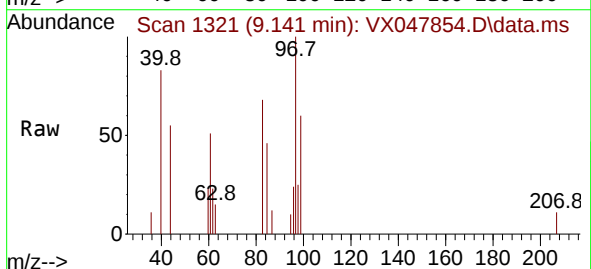




#58
2-Chloroethyl Vinyl ether
Concen: 7.906 ug/l
RT: 8.177 min Scan# 1171
Delta R.T. -0.049 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 63 Resp: 19
Ion Ratio Lower Upper
63 100
106 0.0 21.9 32.9#

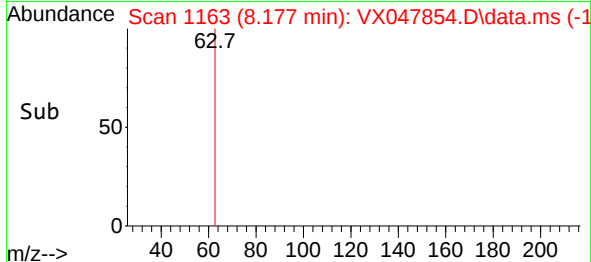

#62
4-Bromofluorobenzene
Concen: 53.906 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 95 Resp: 128407
Ion Ratio Lower Upper
95 100
174 72.9 0.0 141.6
176 71.2 0.0 138.4

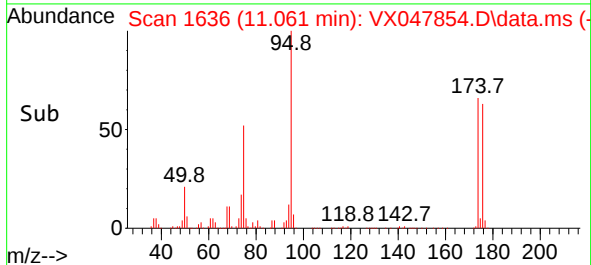



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VX047854.D


Acq: 26 Sep 2025 13:43

Instrument :

MSVOA_X

ClientSampleId :

TT190D1-20250918DL

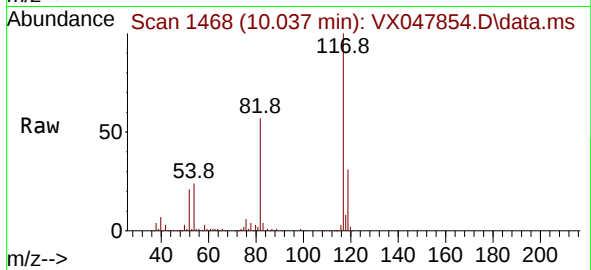




Tgt Ion:117 Resp: 274305

Ion Ratio Lower Upper

117 100

82 56.8 47.8 71.6

119 31.2 25.2 37.8

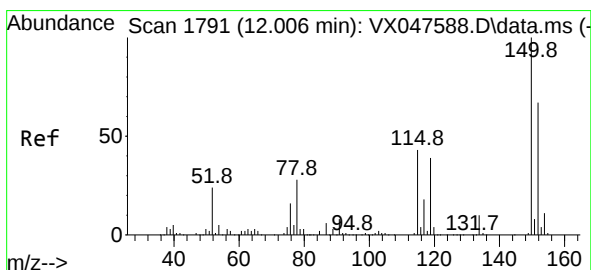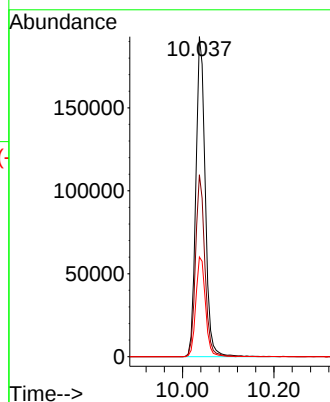

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.006 min Scan# 1791

Delta R.T. -0.000 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43




Tgt Ion:152 Resp: 134213


Ion Ratio Lower Upper

152 100

115 63.6 44.9 134.5

150 160.3 0.0 352.0







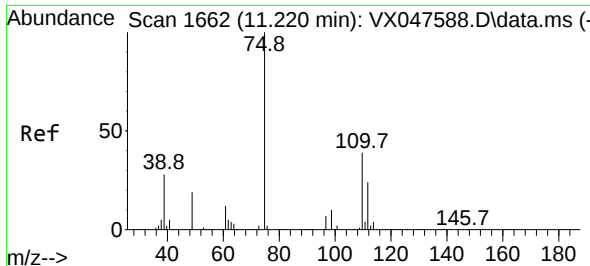

#76
1,2,3-Trichloropropane
Concen: 24.691 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion: 75 Resp: 67094
Ion Ratio Lower Upper
75 100
77 0.6 18.8 56.4#

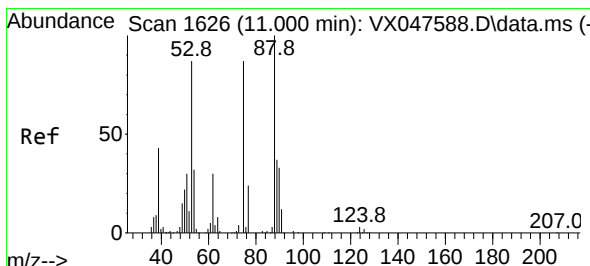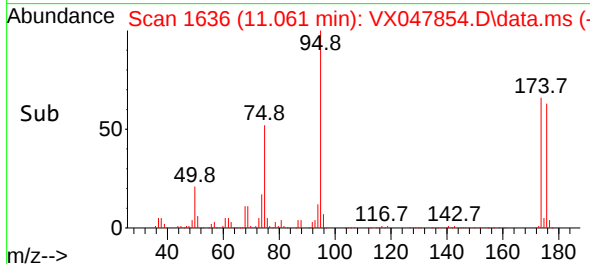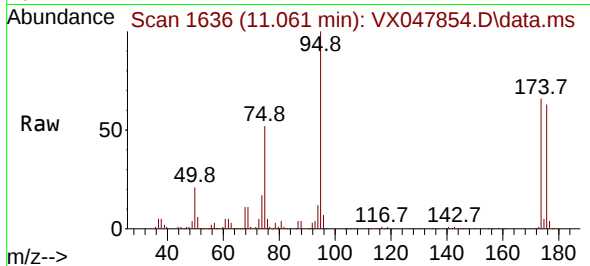

#81
trans-1,4-Dichloro-2-butene
Concen: 62.964 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.061 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43

Tgt Ion: 75 Resp: 67094
Ion Ratio Lower Upper
75 100
53 0.1 83.4 125.2#
89 0.0 36.3 54.5#

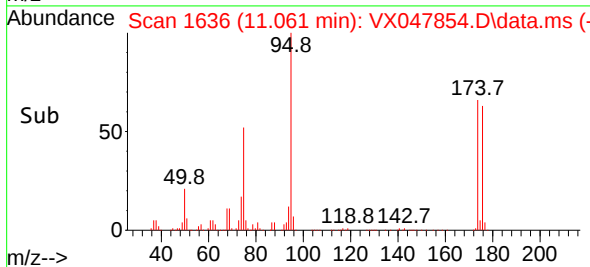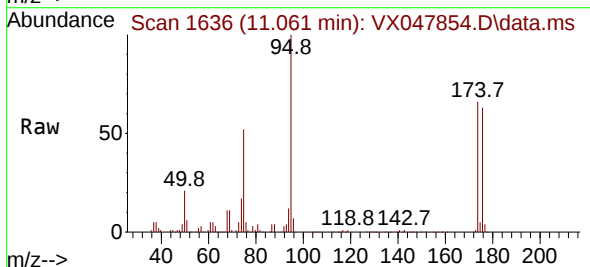



#85

sec-Butylbenzene

Concen: 0.204 ug/l

RT: 11.872 min Scan# 1769

Delta R.T. -0.000 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43

Instrument :

MSVOA_X

ClientSampleId :





TT190D1-20250918DL

Tgt Ion:105 Resp: 2080

Ion Ratio Lower Upper

105 100

134 20.6 9.8 29.5

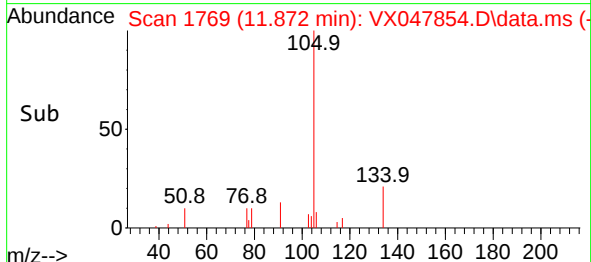

#86

p-Isopropyltoluene

Concen: 0.215 ug/l

RT: 11.994 min Scan# 1789

Delta R.T. -0.000 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43




Tgt Ion:119 Resp: 1853


Ion Ratio Lower Upper

119 100

134 31.1 12.6 37.8

91 47.5 12.6 37.6#





#89

n-Butylbenzene

Concen: 0.356 ug/l

RT: 12.317 min Scan# 1841

Delta R.T. 0.006 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43





Instrument :

MSVOA_X

ClientSampleId :

TT190D1-20250918DL

Tgt Ion: 91	Resp: 2841
Ion Ratio	Lower Upper
91	100
92	55.9 27.6 82.7
134	26.6 12.6 37.8

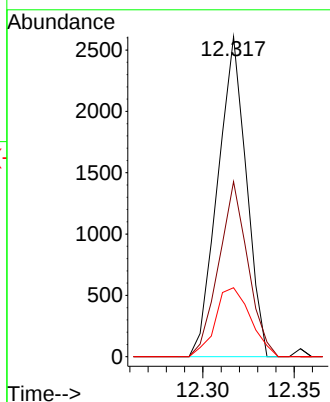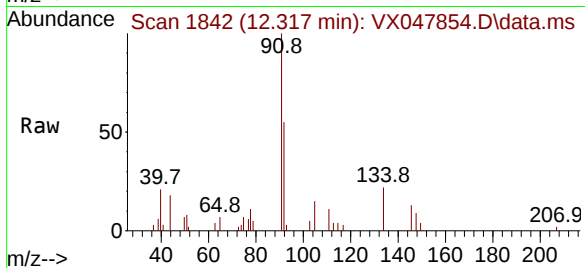

#93

1,2,4-Trichlorobenzene

Concen: 0.529 ug/l




RT: 13.573 min Scan# 2048


Delta R.T. 0.006 min

Lab File: VX047854.D

Acq: 26 Sep 2025 13:43

Tgt Ion: 180	Resp: 1530
Ion Ratio	Lower Upper
180	100
182	92.3 46.6 139.8
145	32.7 16.4 49.1




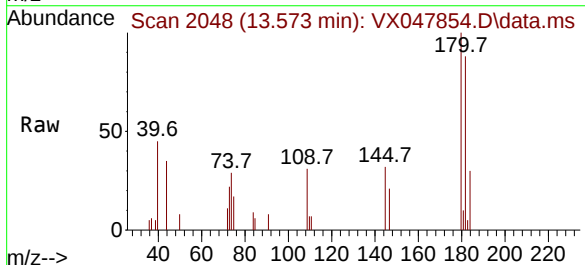




#94
Hexachlorobutadiene
Concen: 1.290 ug/l
RT: 13.707 min Scan# 2070
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43




Instrument :
MSVOA_X
ClientSampleId :
TT190D1-20250918DL


Tgt Ion:	225	Resp:	1266
Ion Ratio	Lower	Upper	
225	100		
223	63.2	31.7	95.1
227	58.1	32.0	96.0

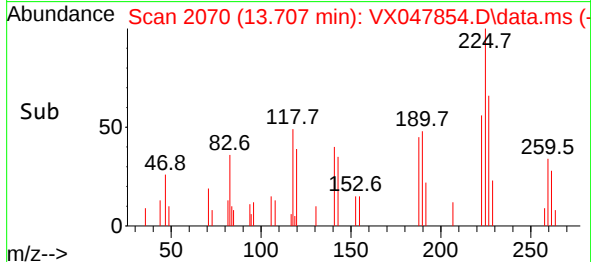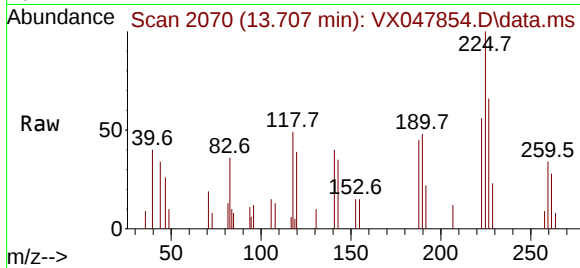

#95
Naphthalene
Concen: 0.338 ug/l
RT: 13.756 min Scan# 2078
Delta R.T. -0.000 min
Lab File: VX047854.D
Acq: 26 Sep 2025 13:43


Tgt Ion:	128	Resp:	2972
Ion Ratio	Lower	Upper	
128	100		
127	11.4	10.2	15.2
129	10.4	8.8	13.2

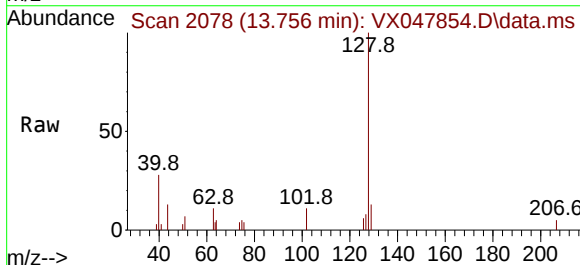



#96
 1,2,3-Trichlorobenzene
 Concen: 0.499 ug/l
 RT: 13.938 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX047854.D
 Acq: 26 Sep 2025 13:43

Instrument :
 MSVOA_X
 ClientSampleId :
 TT190D1-20250918DL

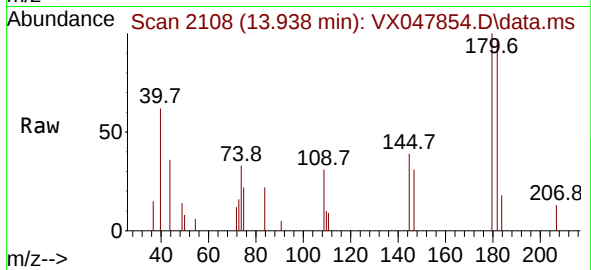

Tgt Ion:	180	Resp:	1342
Ion Ratio	Lower	Upper	
180	100		
182	103.0	47.6	142.8
145	37.7	17.9	53.7

