

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
 Data File : VX047849.D
 Acq On : 26 Sep 2025 11:22
 Operator : JC/MD
 Sample : VX0926MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0926MBL01

Quant Time: Sep 26 23:10:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	119168	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	243600	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	244792	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	120069	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	89830	47.357	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	94.720%
35) Dibromofluoromethane	5.367	113	75685	46.327	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.660%
50) Toluene-d8	8.635	98	264760	46.835	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	93.680%
62) 4-Bromofluorobenzene	11.061	95	109449	51.015	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.040%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
Data File : VX047849.D
Acq On : 26 Sep 2025 11:22
Operator : JC/MD
Sample : VX0926MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0926MBL01

Quant Time: Sep 26 23:10:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




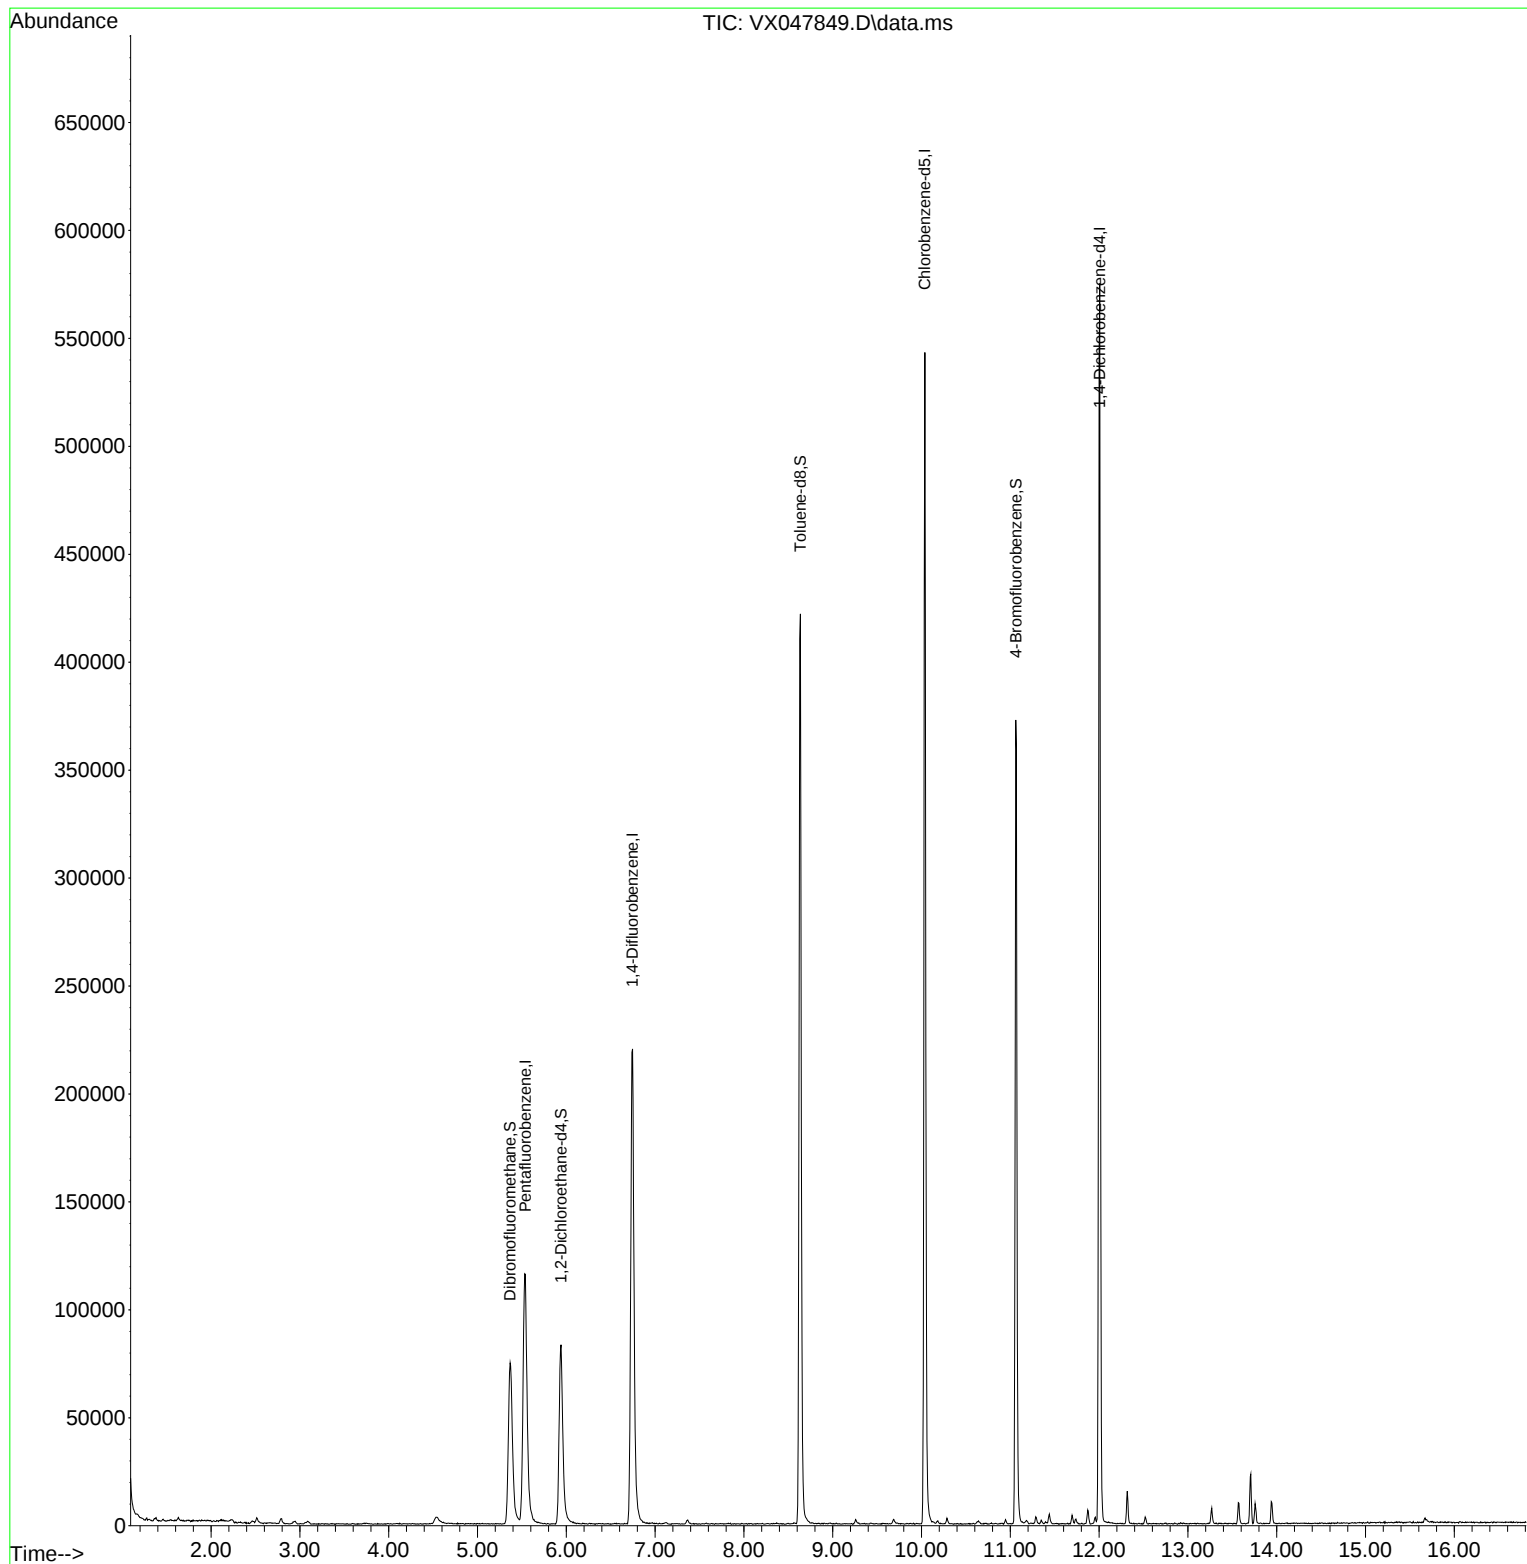


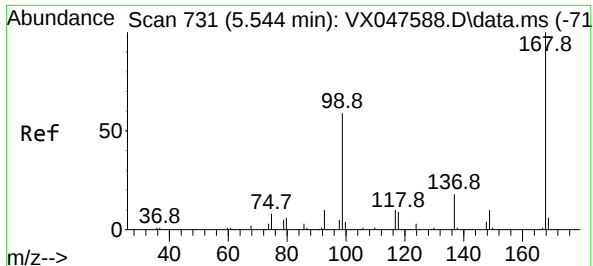

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22




Instrument :
MSVOA_X
ClientSampleId :
VX0926MBL01


Tgt Ion:168 Resp: 119168
Ion Ratio Lower Upper
168 100
99 59.2 48.8 73.2

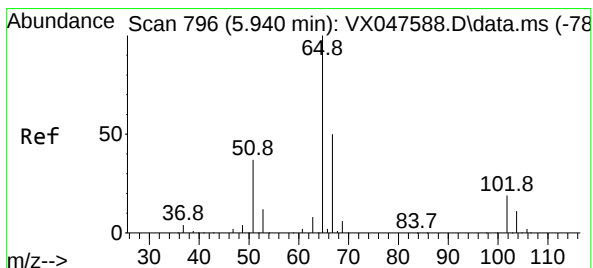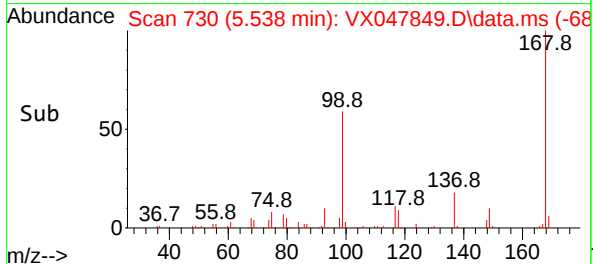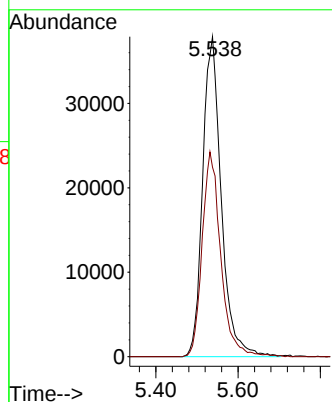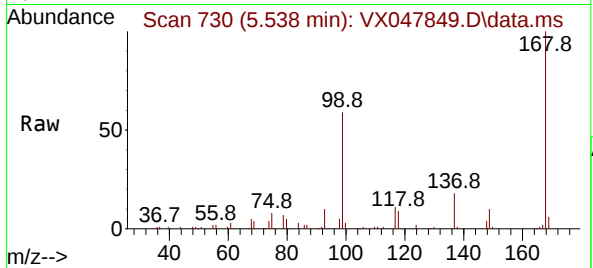

#33
1,2-Dichloroethane-d4
Concen: 47.357 ug/l
RT: 5.940 min Scan# 796
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22

Tgt Ion: 65 Resp: 89830
Ion Ratio Lower Upper
65 100
67 52.7 0.0 103.0


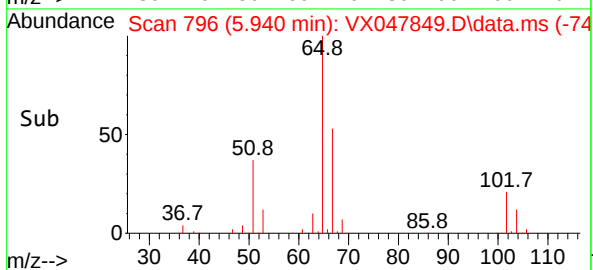
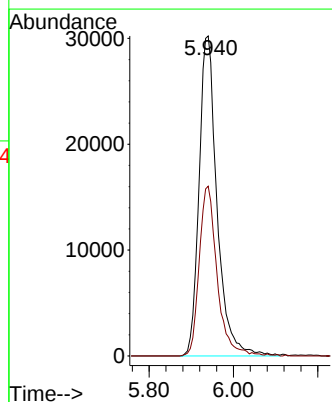
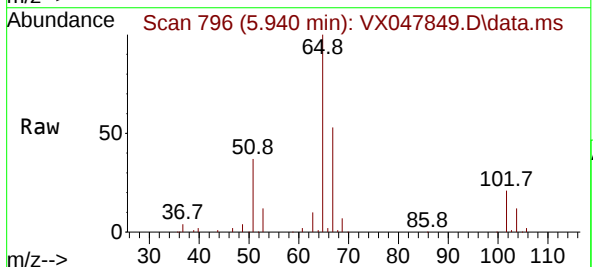


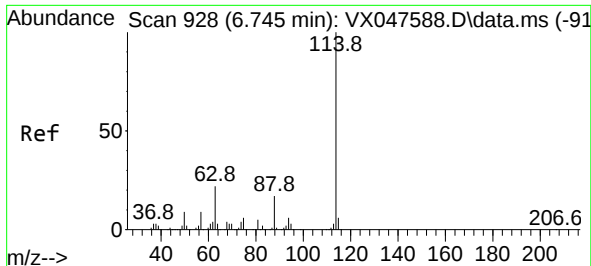

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.745 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22




Instrument :
MSVOA_X
ClientSampleId :
VX0926MBL01


Tgt Ion:114 Resp: 243600
Ion Ratio Lower Upper
114 100
63 21.6 0.0 44.0
88 16.4 0.0 34.2

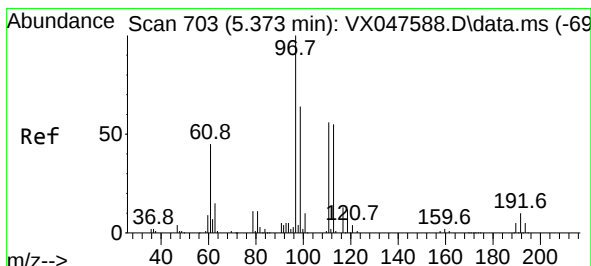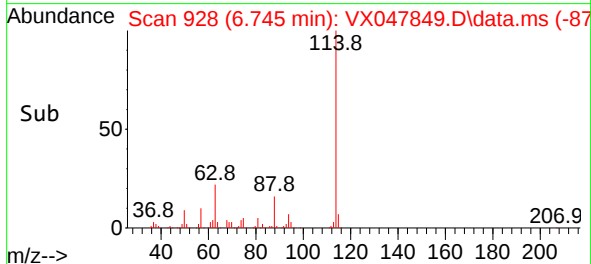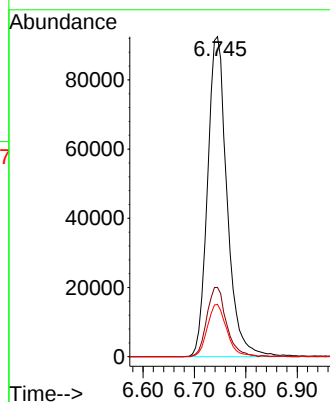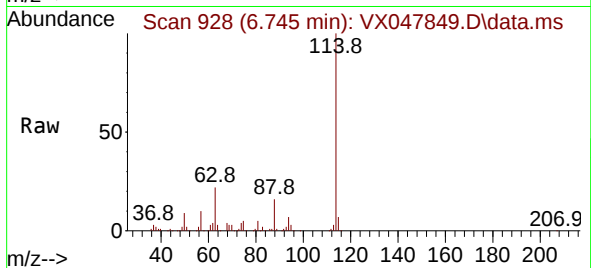

#35
Dibromofluoromethane
Concen: 46.327 ug/l
RT: 5.367 min Scan# 702
Delta R.T. -0.006 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22

Tgt Ion:113 Resp: 75685
Ion Ratio Lower Upper
113 100
111 101.9 80.9 121.3
192 17.7 14.2 21.4


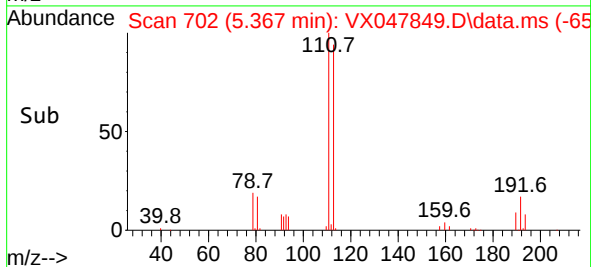
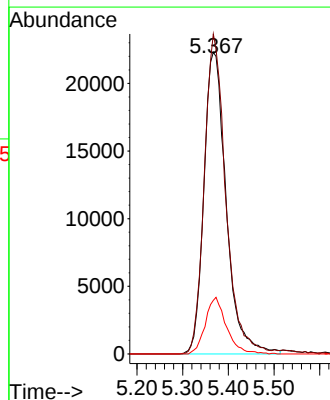
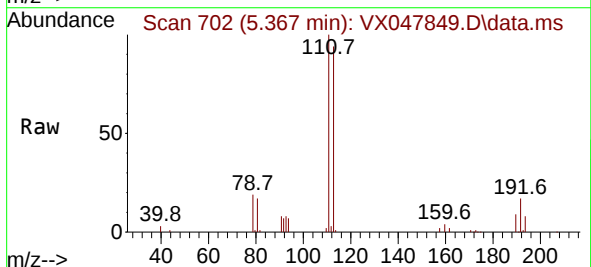


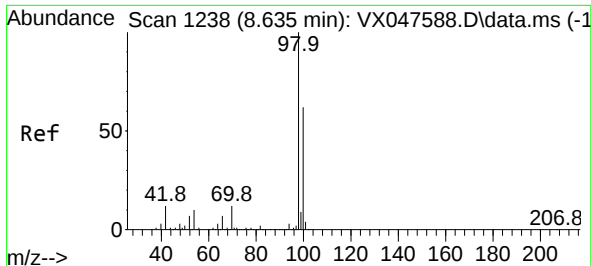

#50
Toluene-d8
Concen: 46.835 ug/l
RT: 8.635 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22




Instrument :
MSVOA_X
ClientSampleId :
VX0926MBL01


Tgt Ion: 98 Resp: 264760
Ion Ratio Lower Upper
98 100
100 66.6 53.0 79.4

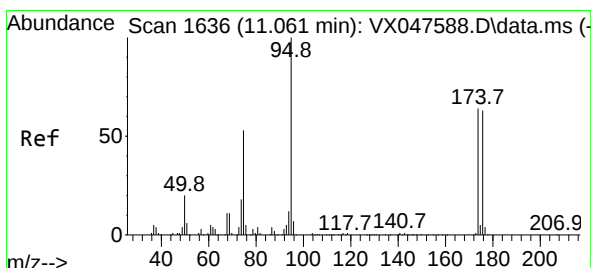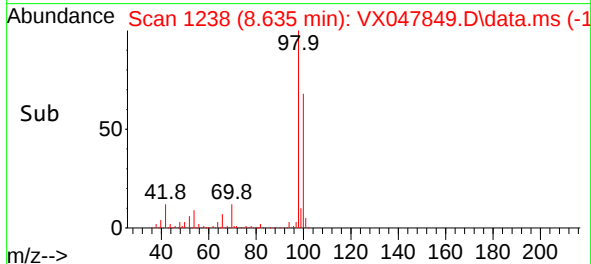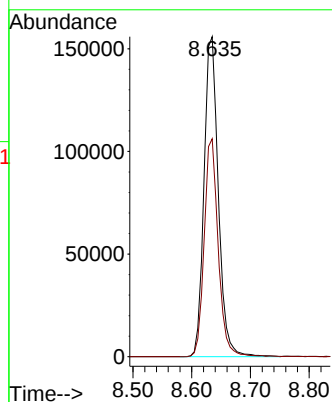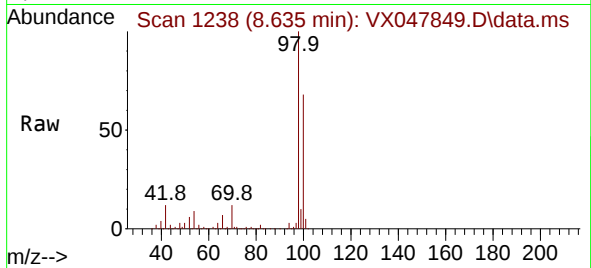

#62
4-Bromofluorobenzene
Concen: 51.015 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22

Tgt Ion: 95 Resp: 109449
Ion Ratio Lower Upper
95 100
174 72.8 0.0 141.6
176 70.9 0.0 138.4


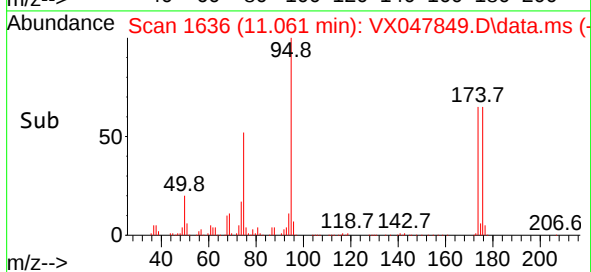
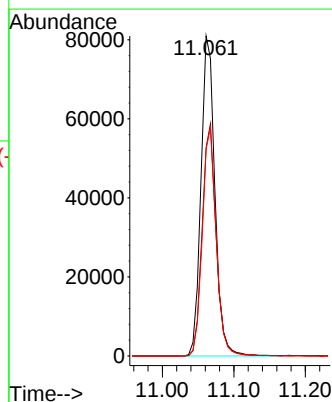
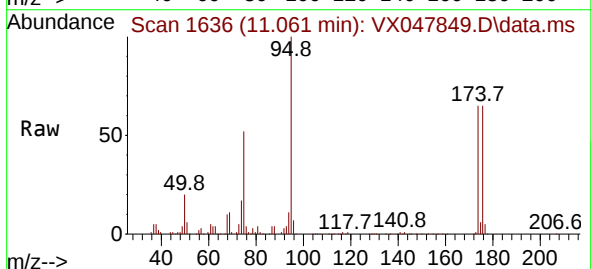


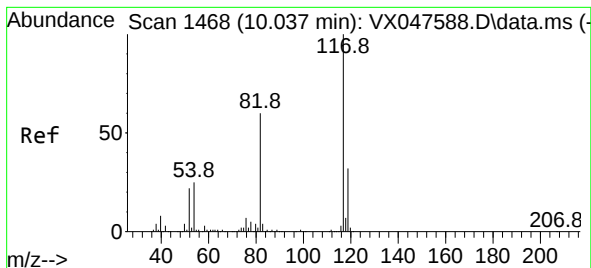

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22

Instrument :
MSVOA_X
ClientSampleId :
VX0926MBL01

Tgt Ion:117 Resp: 244792
Ion Ratio Lower Upper
117 100
82 57.1 47.8 71.6
119 31.8 25.2 37.8

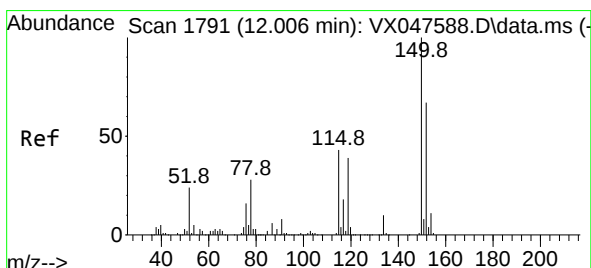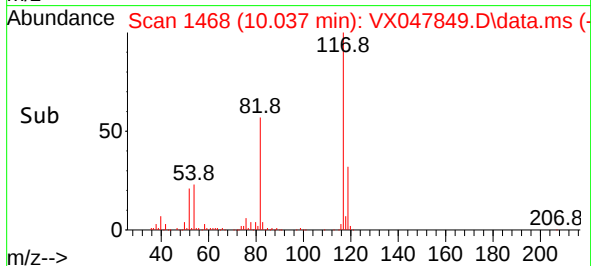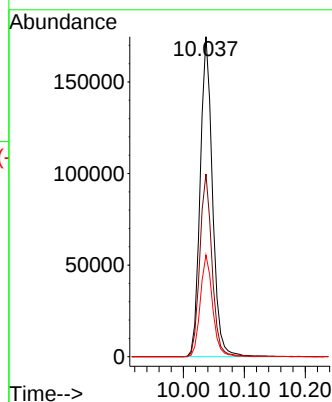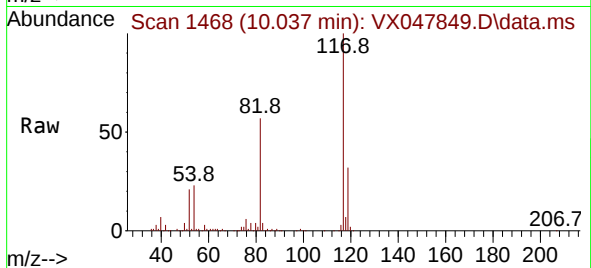

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. 0.000 min
Lab File: VX047849.D
Acq: 26 Sep 2025 11:22

Tgt Ion:152 Resp: 120069
Ion Ratio Lower Upper
152 100
115 64.1 44.9 134.5
150 157.8 0.0 352.0

