

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
 Data File : VX047858.D
 Acq On : 26 Sep 2025 15:07
 Operator : JC/MD
 Sample : Q3143-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Sep 26 23:16:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 17 06:39:58 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	114866	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	240217	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	244825	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	120344	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	94540	51.707	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.420%
35) Dibromofluoromethane	5.373	113	78590	48.783	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.560%
50) Toluene-d8	8.635	98	274065	49.164	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	98.320%
62) 4-Bromofluorobenzene	11.067	95	111462	52.685	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	105.380%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX092625\
Data File : VX047858.D
Acq On : 26 Sep 2025 15:07
Operator : JC/MD
Sample : Q3143-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Sep 26 23:16:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X091625W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 17 06:39:58 2025
Response via : Initial Calibration




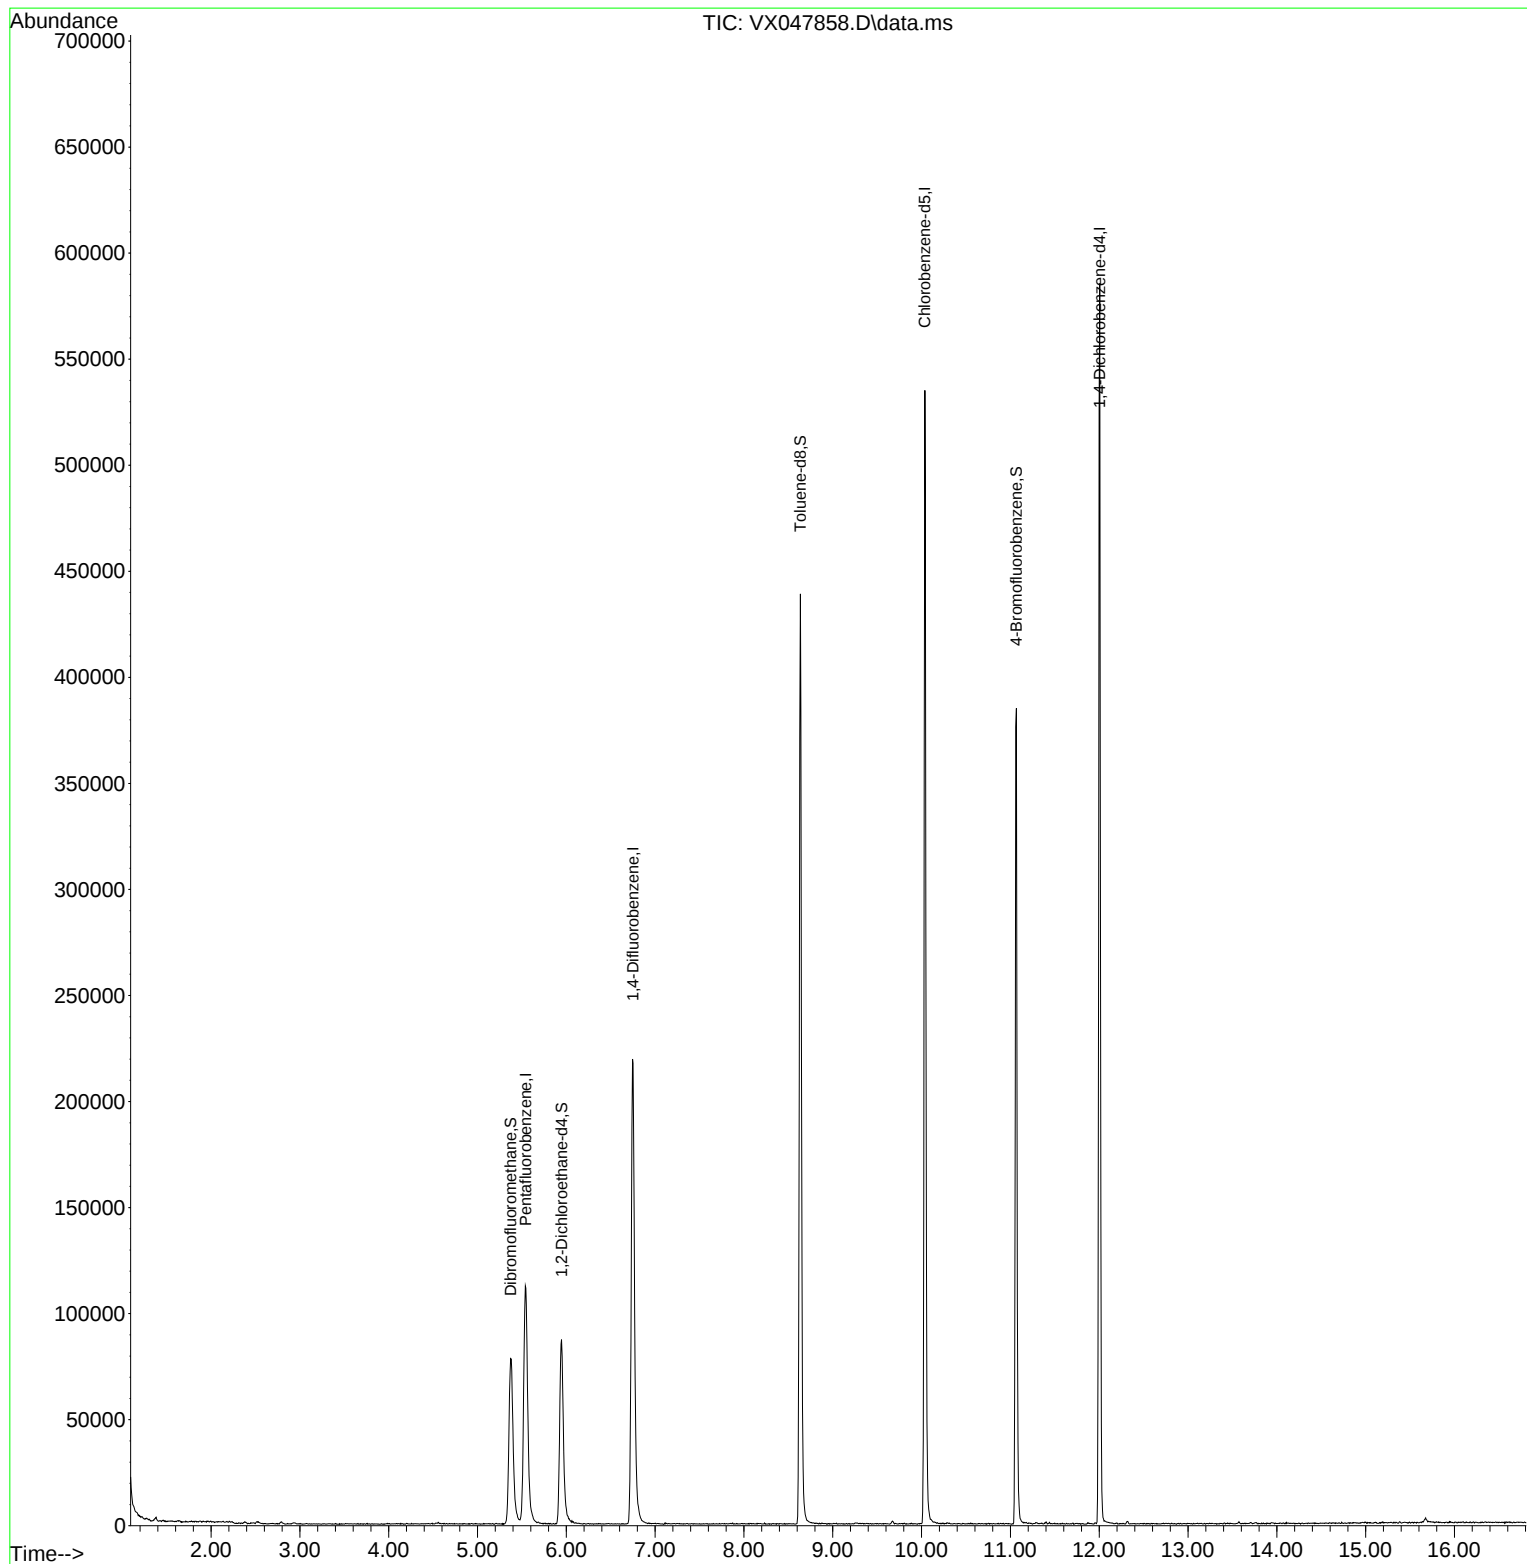


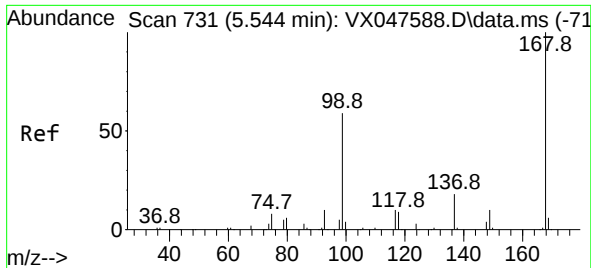

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:168 Resp: 114866
Ion Ratio Lower Upper
168 100
99 63.3 48.8 73.2

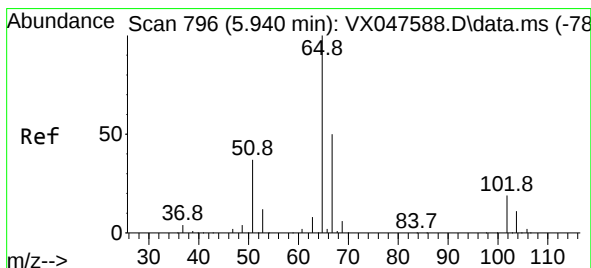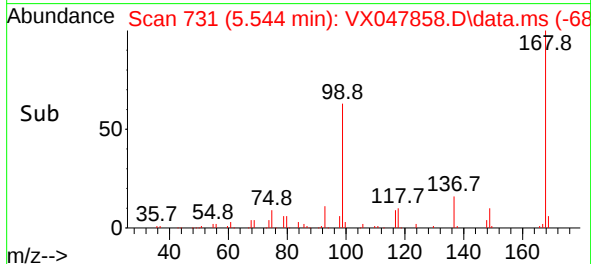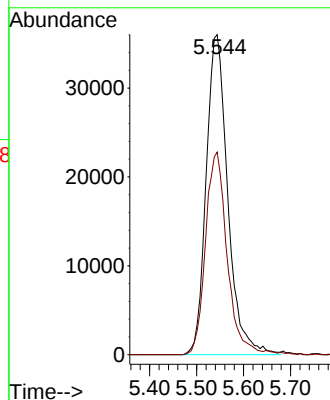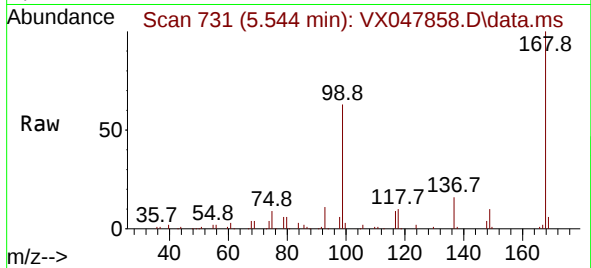

#33
1,2-Dichloroethane-d4
Concen: 51.707 ug/l
RT: 5.946 min Scan# 797
Delta R.T. 0.006 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07

Tgt Ion: 65 Resp: 94540
Ion Ratio Lower Upper
65 100
67 51.2 0.0 103.0


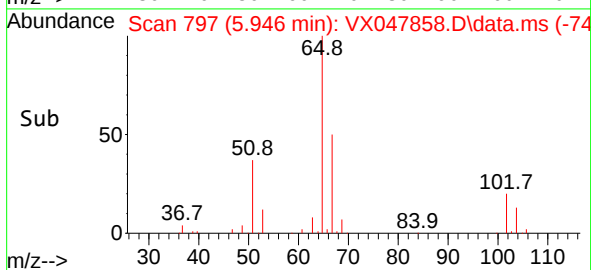
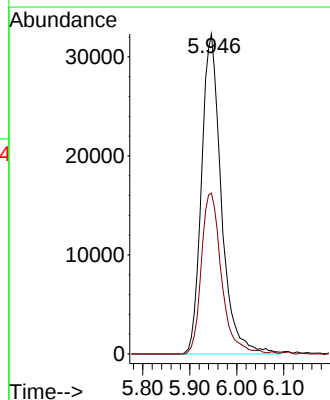
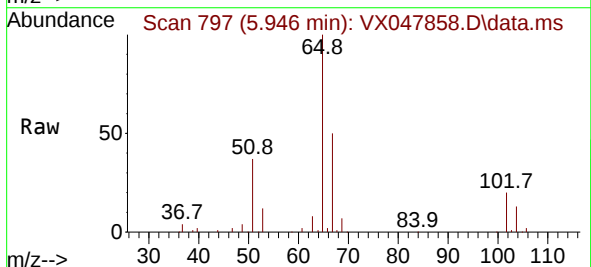


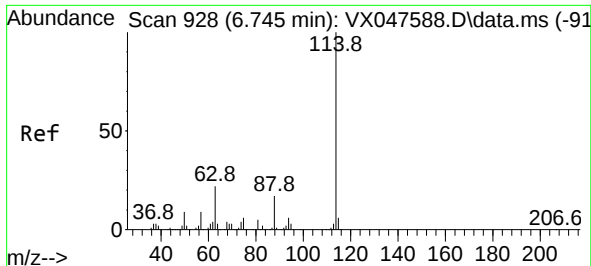

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion:114 Resp: 240217
Ion Ratio Lower Upper
114 100
63 22.2 0.0 44.0
88 15.9 0.0 34.2

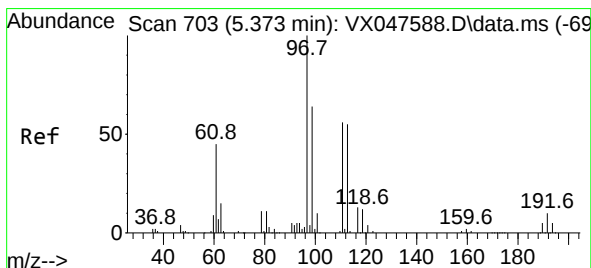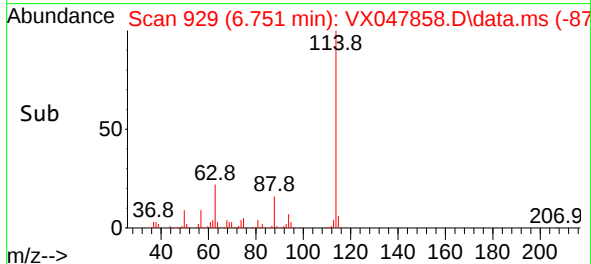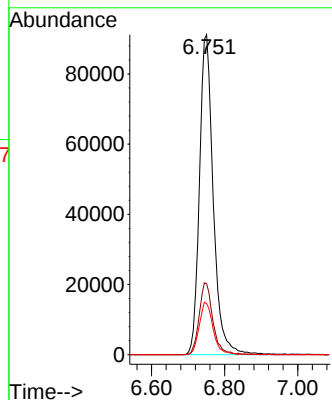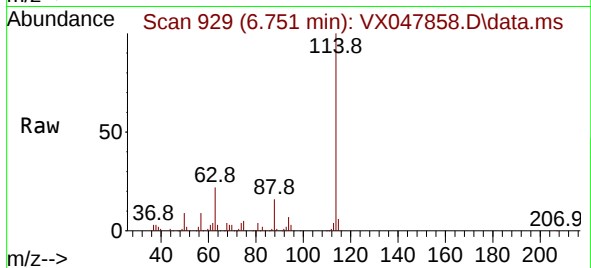

#35
Dibromofluoromethane
Concen: 48.783 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07

Tgt Ion:113 Resp: 78590
Ion Ratio Lower Upper
113 100
111 102.0 80.9 121.3
192 18.5 14.2 21.4


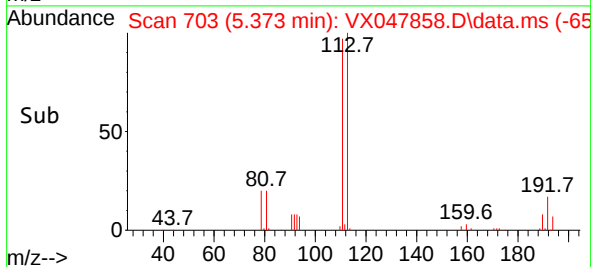
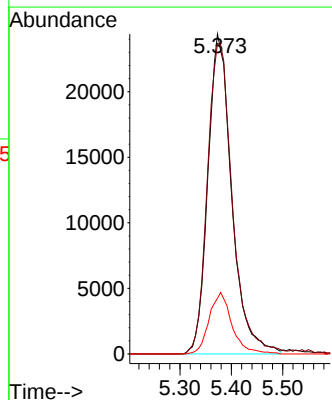
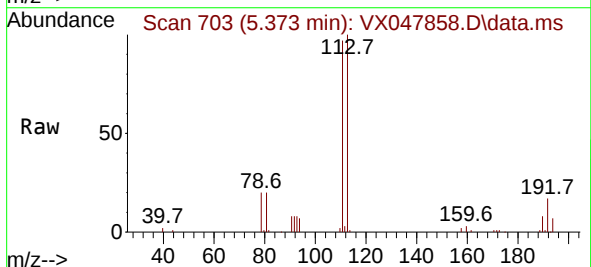


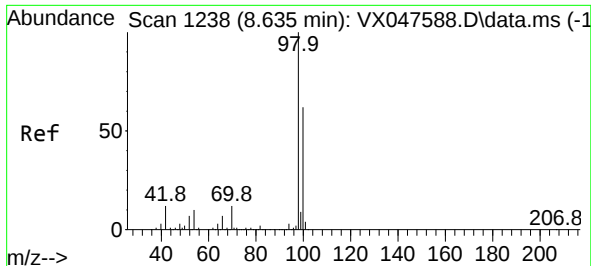

#50
Toluene-d8
Concen: 49.164 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6


Tgt Ion: 98 Resp: 274065
Ion Ratio Lower Upper
98 100
100 66.2 53.0 79.4

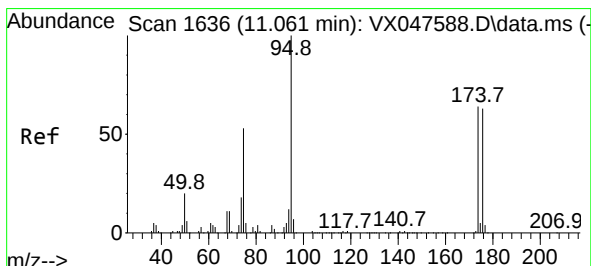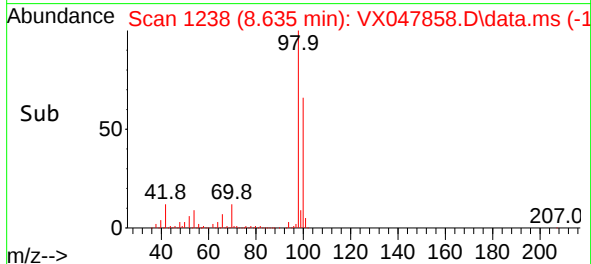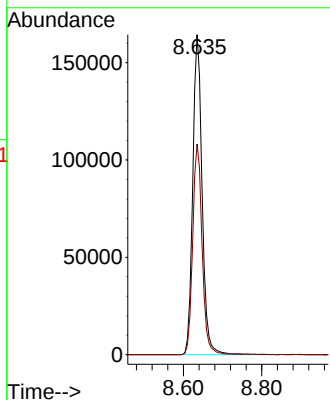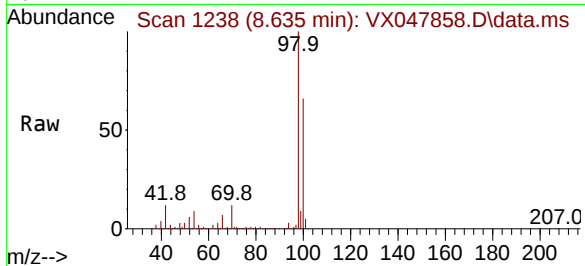

#62
4-Bromofluorobenzene
Concen: 52.685 ug/l
RT: 11.067 min Scan# 1637
Delta R.T. 0.006 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07

Tgt Ion: 95 Resp: 111462
Ion Ratio Lower Upper
95 100
174 73.0 0.0 141.6
176 71.2 0.0 138.4


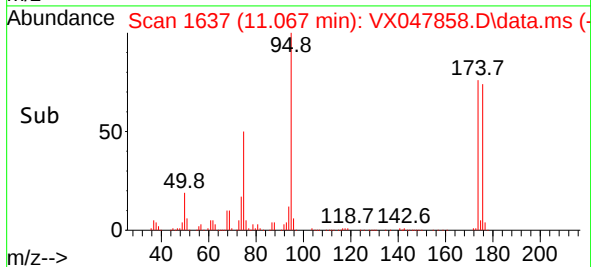
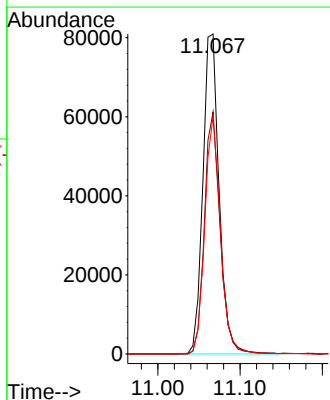
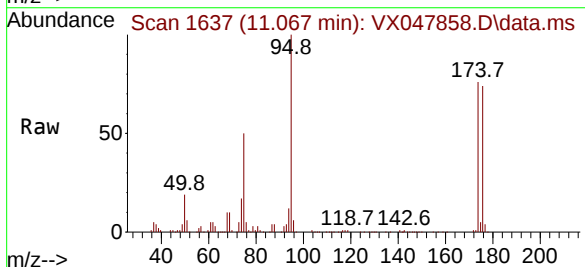


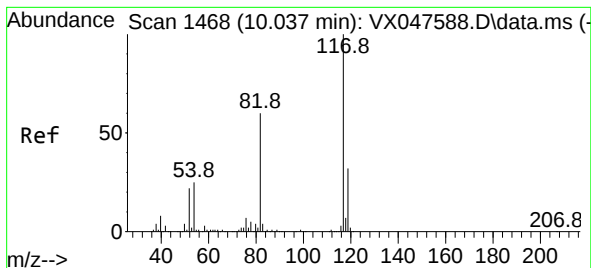

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tgt Ion:117 Resp: 244825
Ion Ratio Lower Upper
117 100
82 58.5 47.8 71.6
119 32.7 25.2 37.8

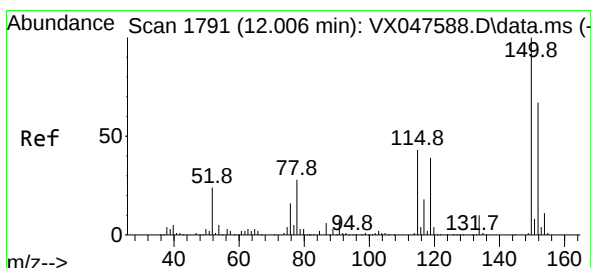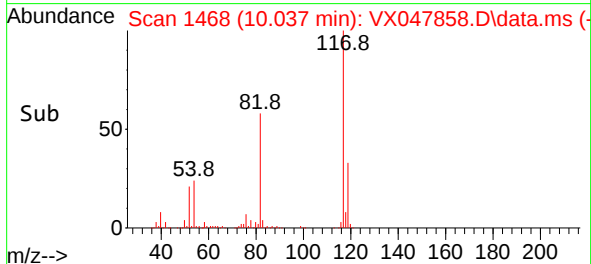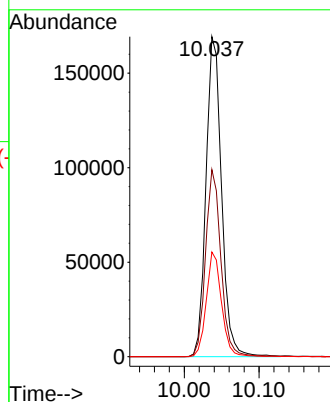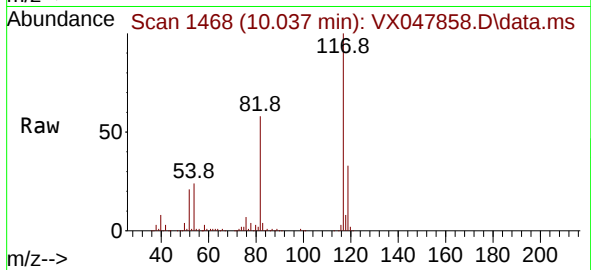

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX047858.D
Acq: 26 Sep 2025 15:07

Tgt Ion:152 Resp: 120344
Ion Ratio Lower Upper
152 100
115 62.3 44.9 134.5
150 159.2 0.0 352.0

