

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX092718\
 Data File : VX004766.D
 Acq On : 27 Sep 2018 11:43
 Operator : JC/MD
 Sample : J5048-19
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-2-SEP18

Quant Time: Sep 28 12:44:55 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
 Quant Title : SW846 8260
 QLast Update : Wed Sep 26 14:17:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	278556	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	443408	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	421154	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	234483	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	197603	49.66	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.32%	
35) Dibromofluoromethane	5.50	113	169426	45.08	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.16%	
50) Toluene-d8	8.71	98	633269	50.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.38%	
62) 4-Bromofluorobenzene	11.14	95	229186	50.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.84%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX092718\
Data File : VX004766.D
Acq On : 27 Sep 2018 11:43
Operator : JC/MD
Sample : J5048-19
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2-SEP18

Quant Time: Sep 28 12:44:55 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X092618W.M
Quant Title : SW846 8260
QLast Update : Wed Sep 26 14:17:02 2018
Response via : Initial Calibration

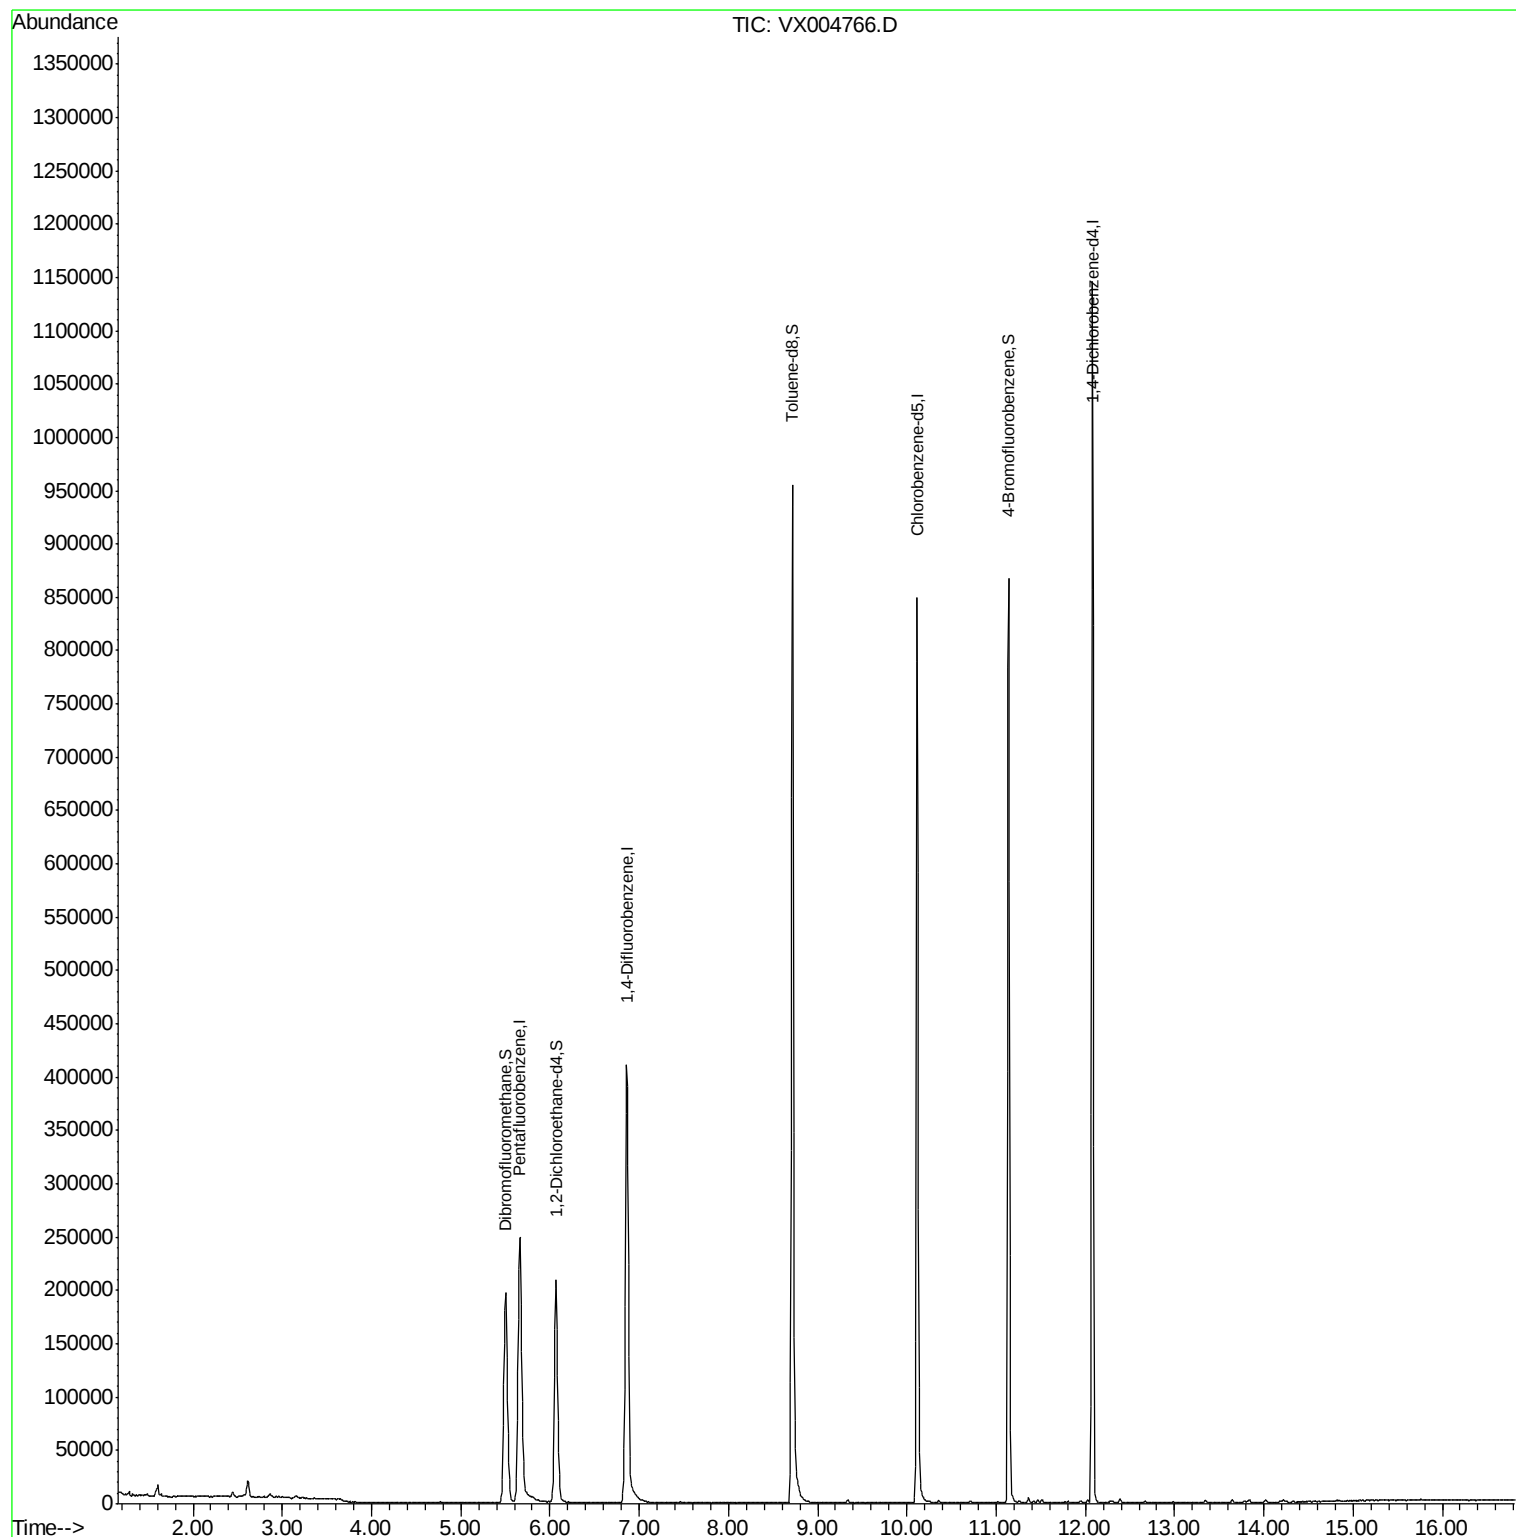

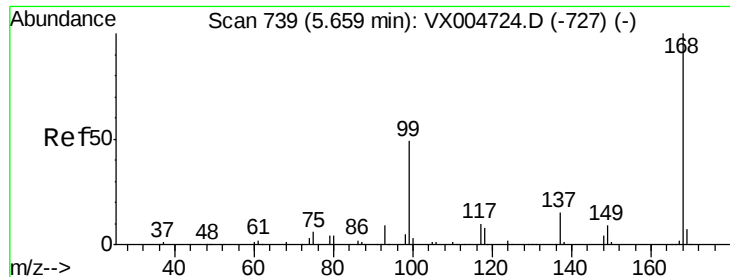

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX004766.D

Acq: 27 Sep 2018 11:43

Instrument :

MSVOA_X

ClientSampleId :


TB-2-SEP18

Tot Ion:168 Resp: 278556

Ion Ratio Lower Upper

168 100

99 47.8 39.9 59.9

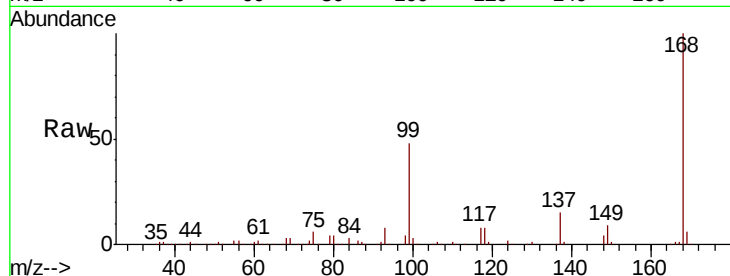

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

100000

80000



60000

40000

20000

0

Time-->

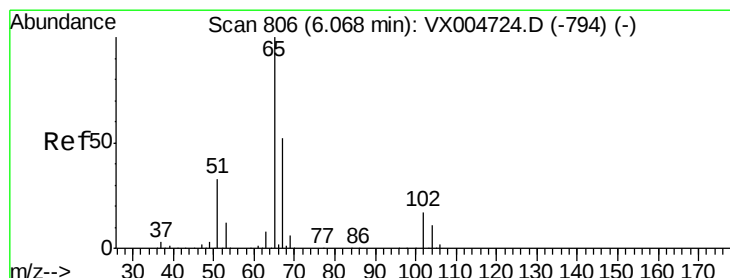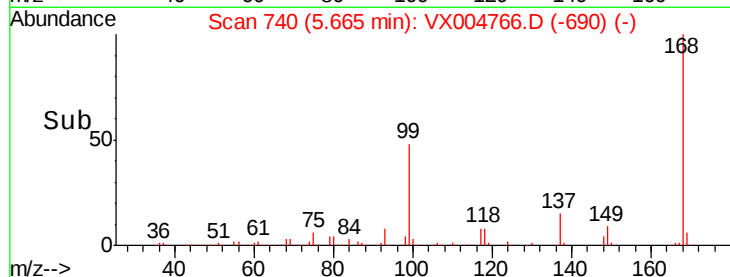

#33

1,2-Dichloroethane-d4

Concen: 49.659 ug/l

RT: 6.07 min Scan# 806

Delta R.T. 0.00 min

Lab File: VX004766.D


Acq: 27 Sep 2018 11:43

Tgt Ion: 65 Resp: 197603

Ion Ratio Lower Upper

65 100

67 53.8 0.0 106.8

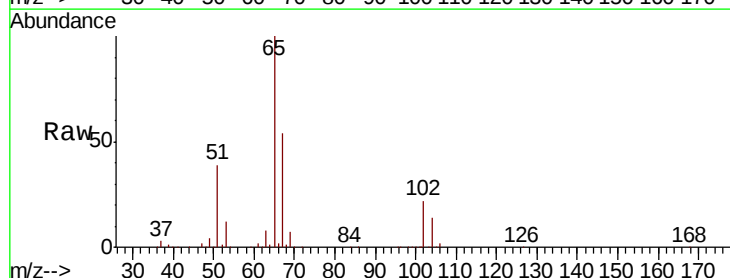

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.07

80000


60000


40000

20000

0

Time-->

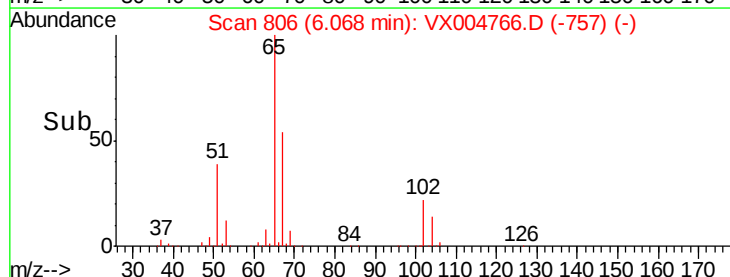


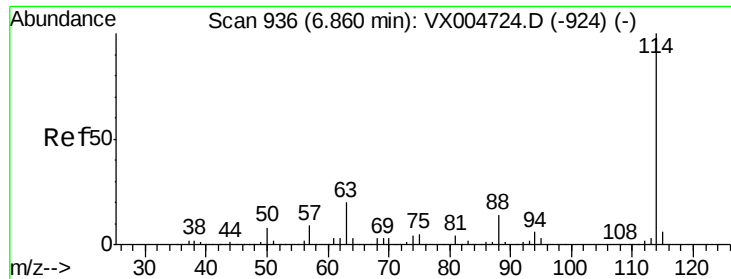




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.86 min Scan# 936
Delta R.T. 0.00 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43

Instrument :
MSVOA_X
ClientSampleId :
TB-2-SEP18

Tot Ion:114 Resp: 443408
Ion Ratio Lower Upper
114 100
63 21.0 0.0 39.0
88 16.0 0.0 30.4

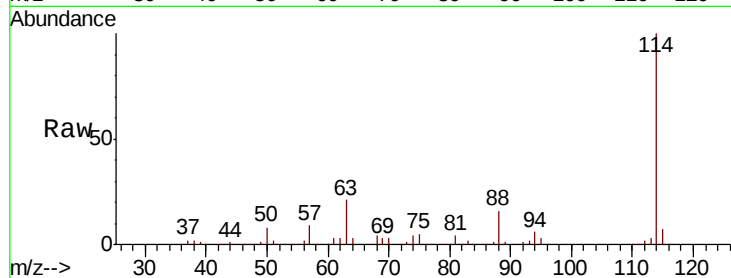


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

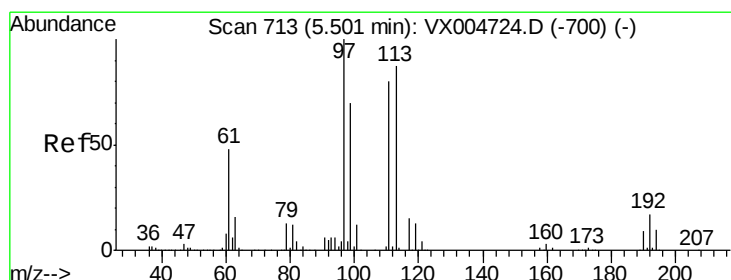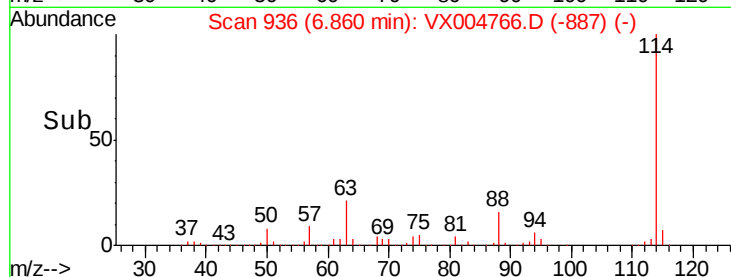
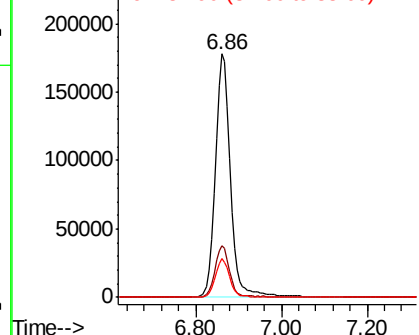



#35
Dibromofluoromethane
Concen: 45.085 ug/l
RT: 5.50 min Scan# 713
Delta R.T. 0.00 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43

Tgt Ion:113 Resp: 169426
Ion Ratio Lower Upper
113 100
111 103.1 82.4 123.6
192 23.4 19.4 29.2

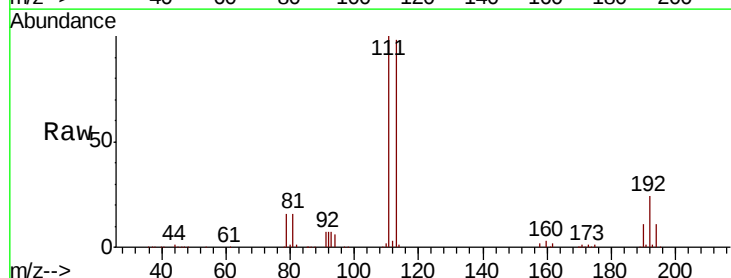

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V



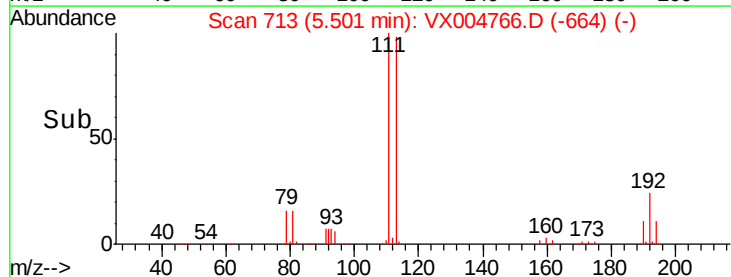
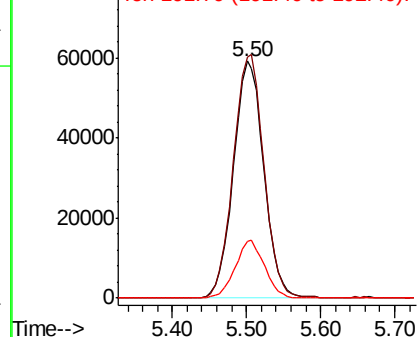


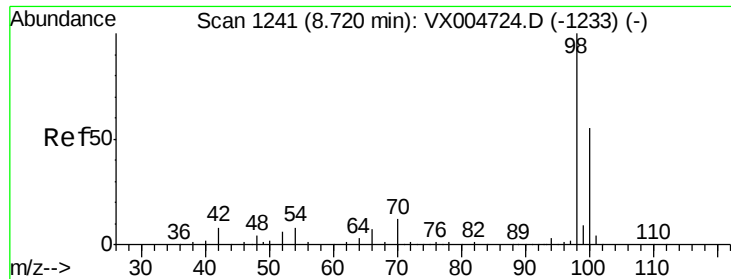

#50
Toluene-d8
Concen: 50.689 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.01 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43




Instrument :
MSVOA_X
ClientSampleId :
TB-2-SEP18


Tot Ion: 98 Resp: 633269
Ion Ratio Lower Upper
98 100
100 63.9 52.9 79.3

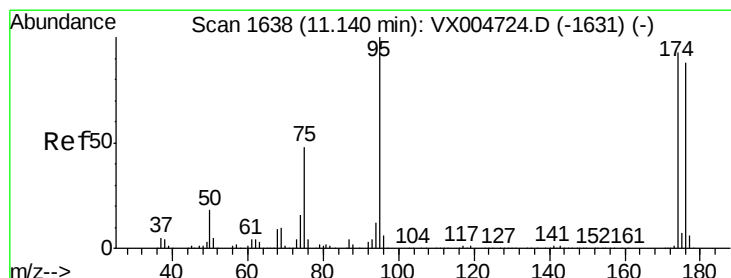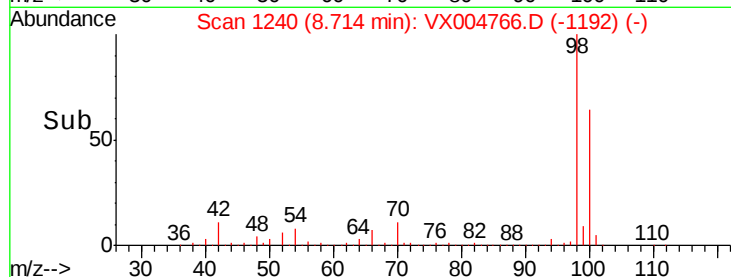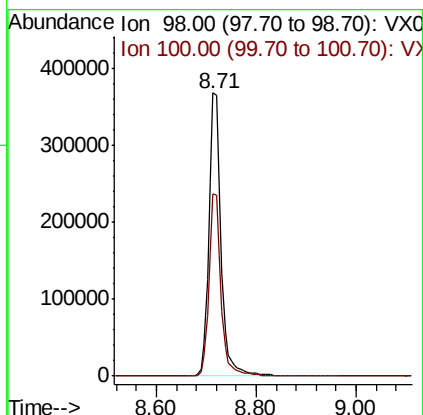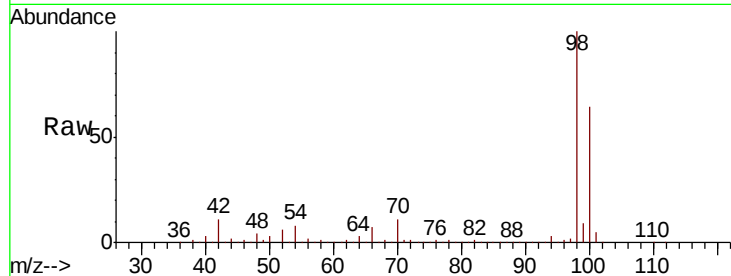

#62
4-Bromofluorobenzene
Concen: 50.922 ug/l
RT: 11.14 min Scan# 1638
Delta R.T. 0.00 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43

Tgt Ion: 95 Resp: 229186
Ion Ratio Lower Upper
95 100
174 91.8 0.0 185.2
176 89.5 0.0 178.6

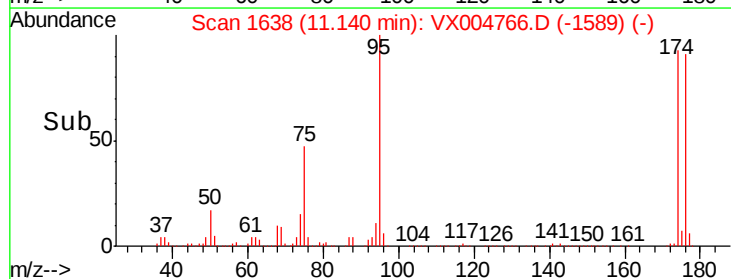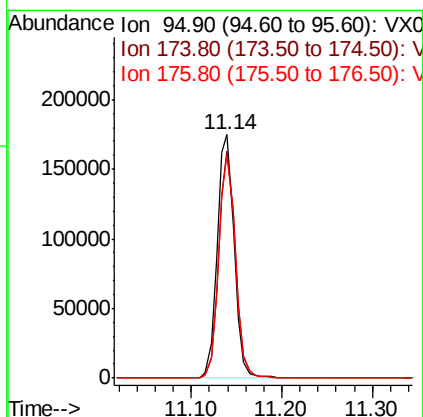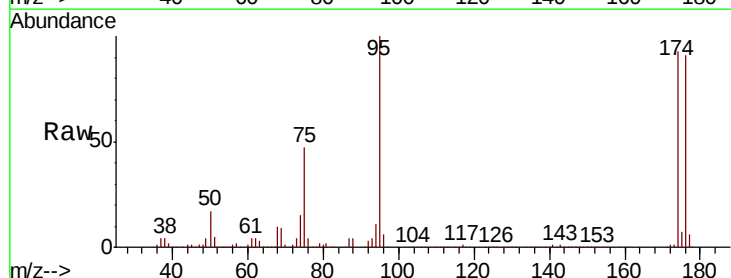


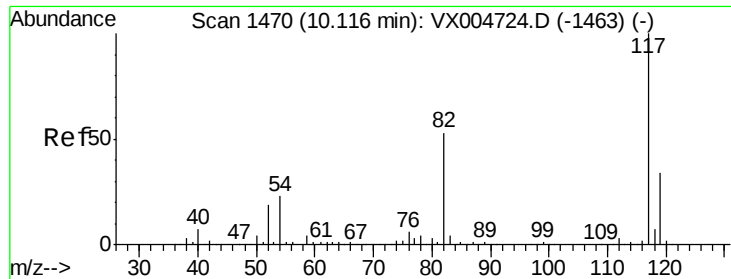




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.12 min Scan# 1470
Delta R.T. 0.00 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43

Instrument :
MSVOA_X
ClientSampleId :
TB-2-SEP18

Tot Ion:117 Resp: 421154
Ion Ratio Lower Upper
117 100
82 54.0 47.8 71.6
119 32.3 29.3 43.9

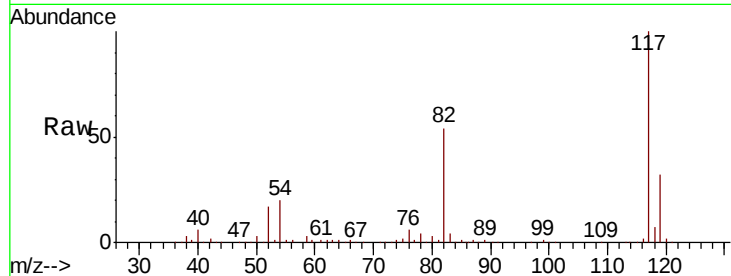


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

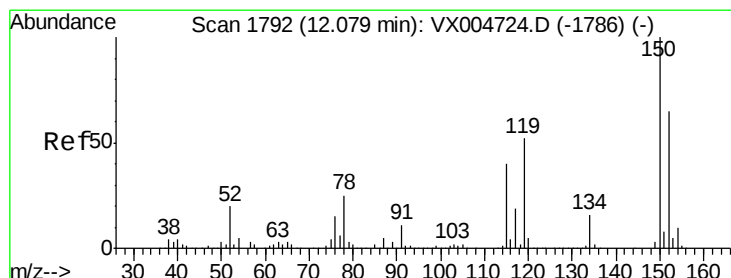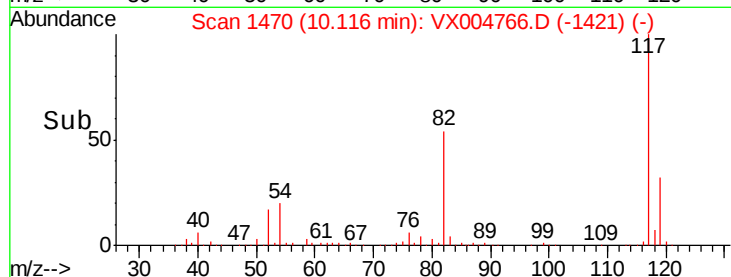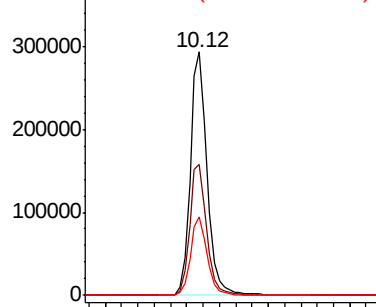

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. 0.00 min
Lab File: VX004766.D
Acq: 27 Sep 2018 11:43

Tgt Ion:152 Resp: 234483
Ion Ratio Lower Upper
152 100
115 55.5 39.0 117.0
150 156.3 0.0 351.0

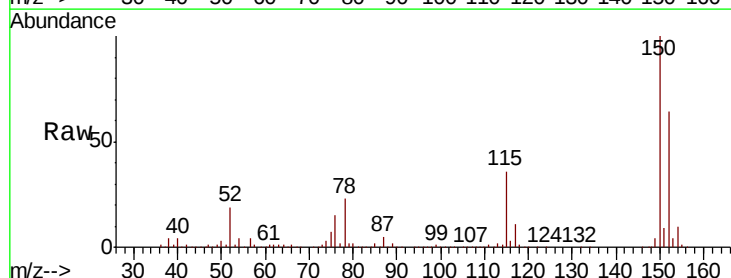

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

