


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092718\
Data File : VX004787.D
Acq On : 27 Sep 2018 21:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W092118S.M
Title : SW846 8260
Last Update : Fri Sep 21 09:05:42 2018

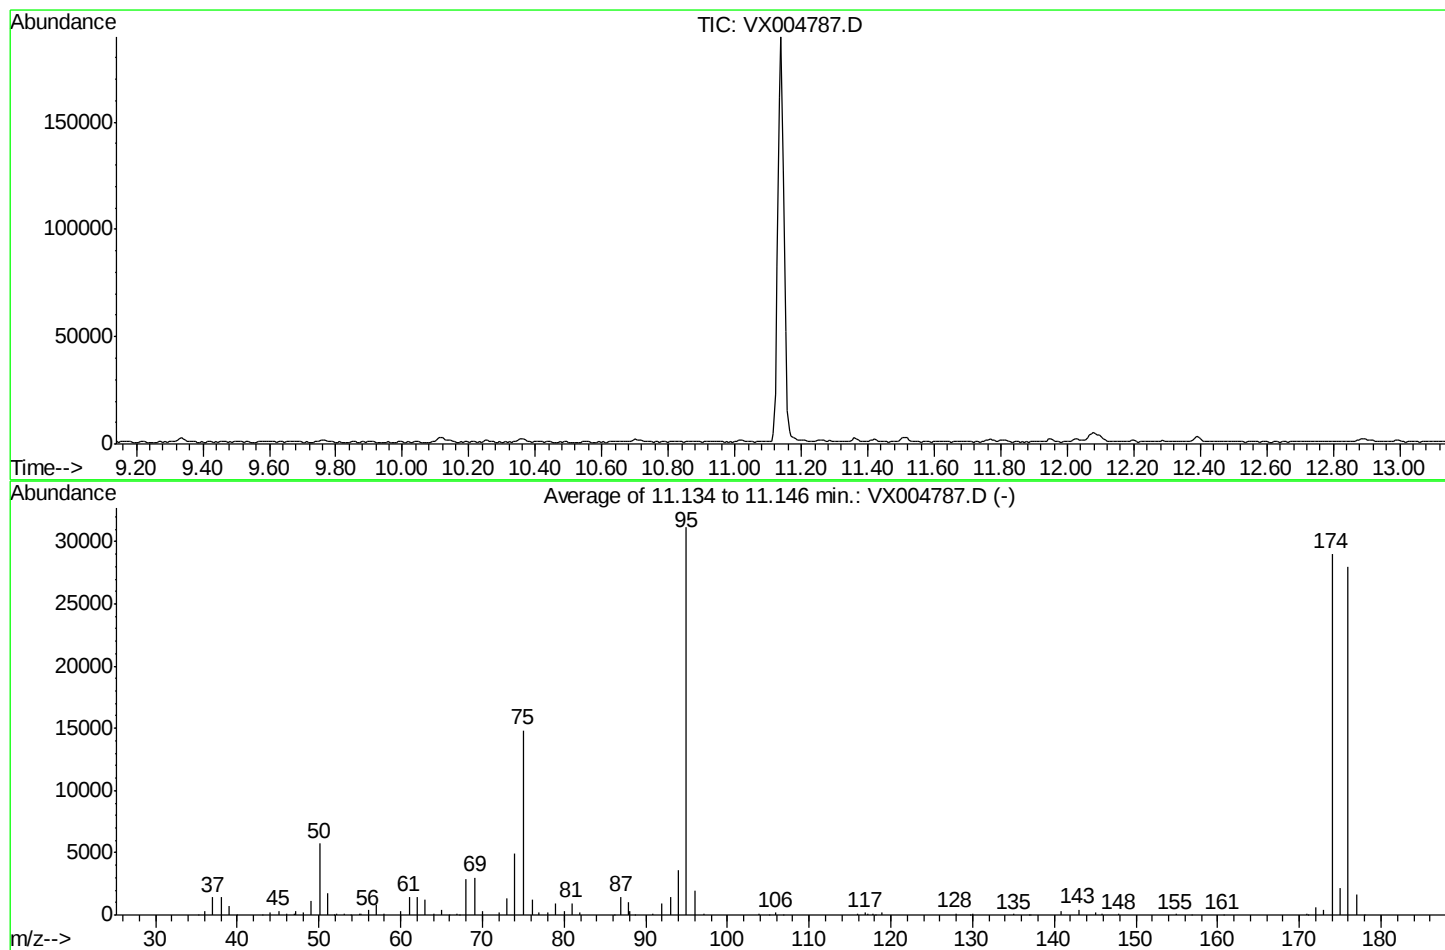

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	5727	PASS
75	95	30	60	47.7	14864	PASS
95	95	100	100	100.0	31152	PASS
96	95	5	9	6.3	1965	PASS
173	174	0.00	2	1.4	393	PASS
174	95	50	100	93.1	29013	PASS
175	174	5	9	7.3	2116	PASS
176	174	95	101	96.3	27949	PASS
177	176	5	9	6.0	1689	PASS