


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX092719\
Data File : VX012687.D
Acq On : 27 Sep 2019 09:04
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X092319W.M
Title : SW846 8260
Last Update : Mon Sep 23 12:27:01 2019

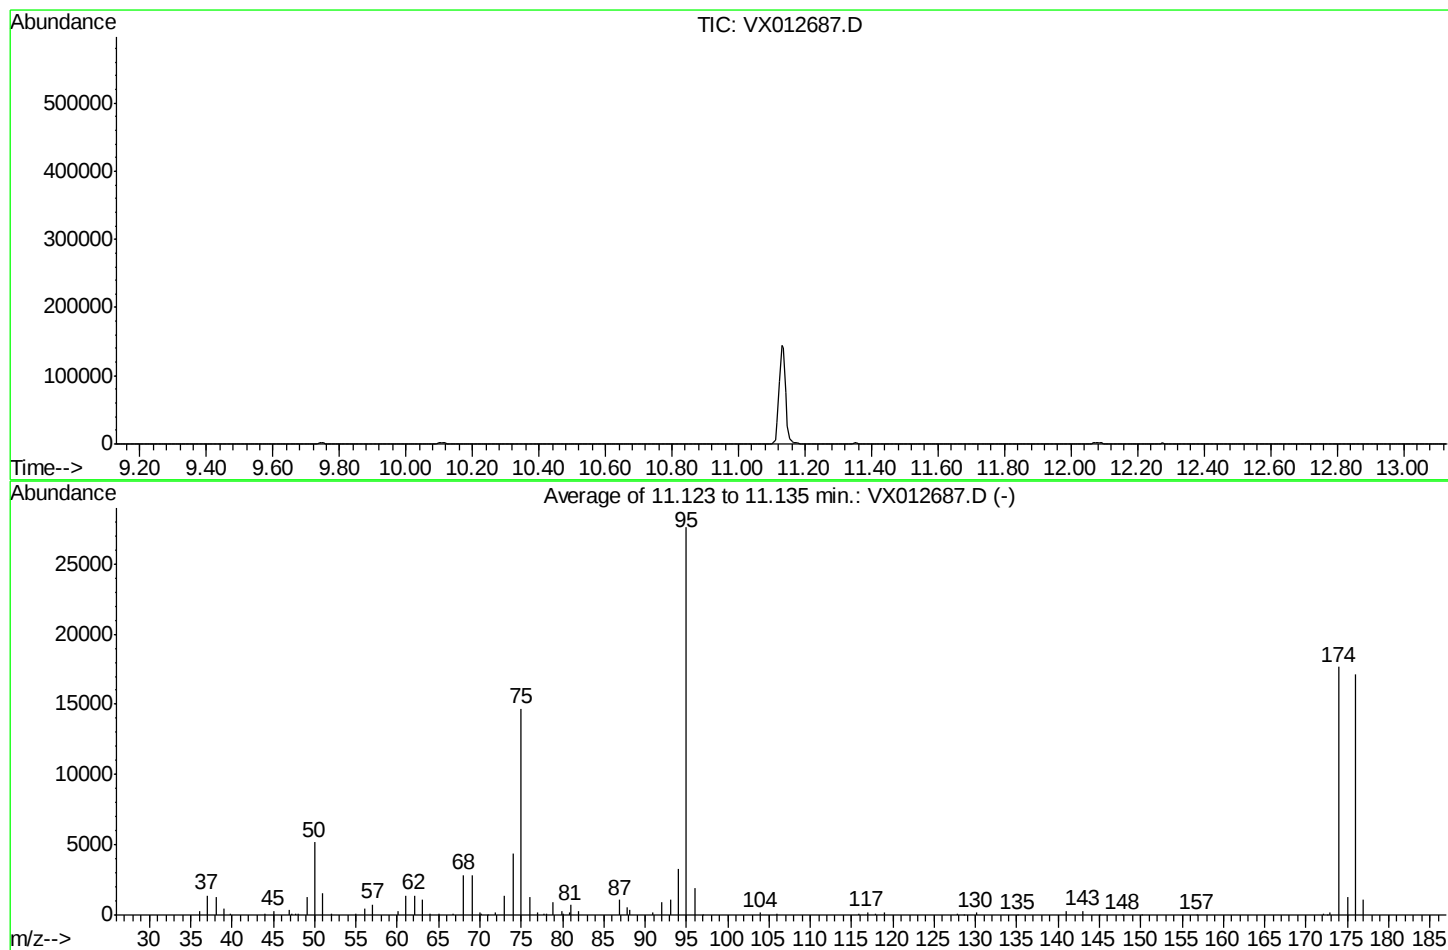

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	5170	PASS
75	95	30	60	53.3	14713	PASS
95	95	100	100	100.0	27602	PASS
96	95	5	9	6.8	1883	PASS
173	174	0.00	2	1.0	171	PASS
174	95	50	100	64.0	17676	PASS
175	174	5	9	7.3	1286	PASS
176	174	95	101	96.7	17092	PASS
177	176	5	9	6.6	1126	PASS